

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012722\
 Data File : PS018158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2022 21:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:35:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.044	6.647	647.2E6	289.4E6	447.735	498.833
Target Compounds							
5) T	DICAMBA	7.231	0.000	6736463	0	1.079	N.D. #
7) T	MCPA	7.489f	0.000	8368416	0	1.254	N.D. #
9) T	2,4-D	8.157	0.000	2923096	0	1.605	N.D. #
10) T	Pentachlo...	8.443	8.117	15535557	6483233	<MDL	<MDL #
11) T	2,4,5-TP ...	8.993	8.437f	16434508	26505580	1.942	7.436 #
12) T	2,4,5-T	9.278	8.923f	25864410	17237783	2.918	5.270 #
13) T	2,4-DB	9.825	0.000	28746590	0	17.390	N.D. #
14) T	DINOSEB	10.966	0.000	13339610	0	2.031	N.D. #
15) T	Picloram	10.805	10.675	260.7E6	132.8E6	21.842	28.404 #
16) T	DCPA	11.232	0.000	21973187	0	2.034	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012722\
Data File : PS018158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2022 21:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:35:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

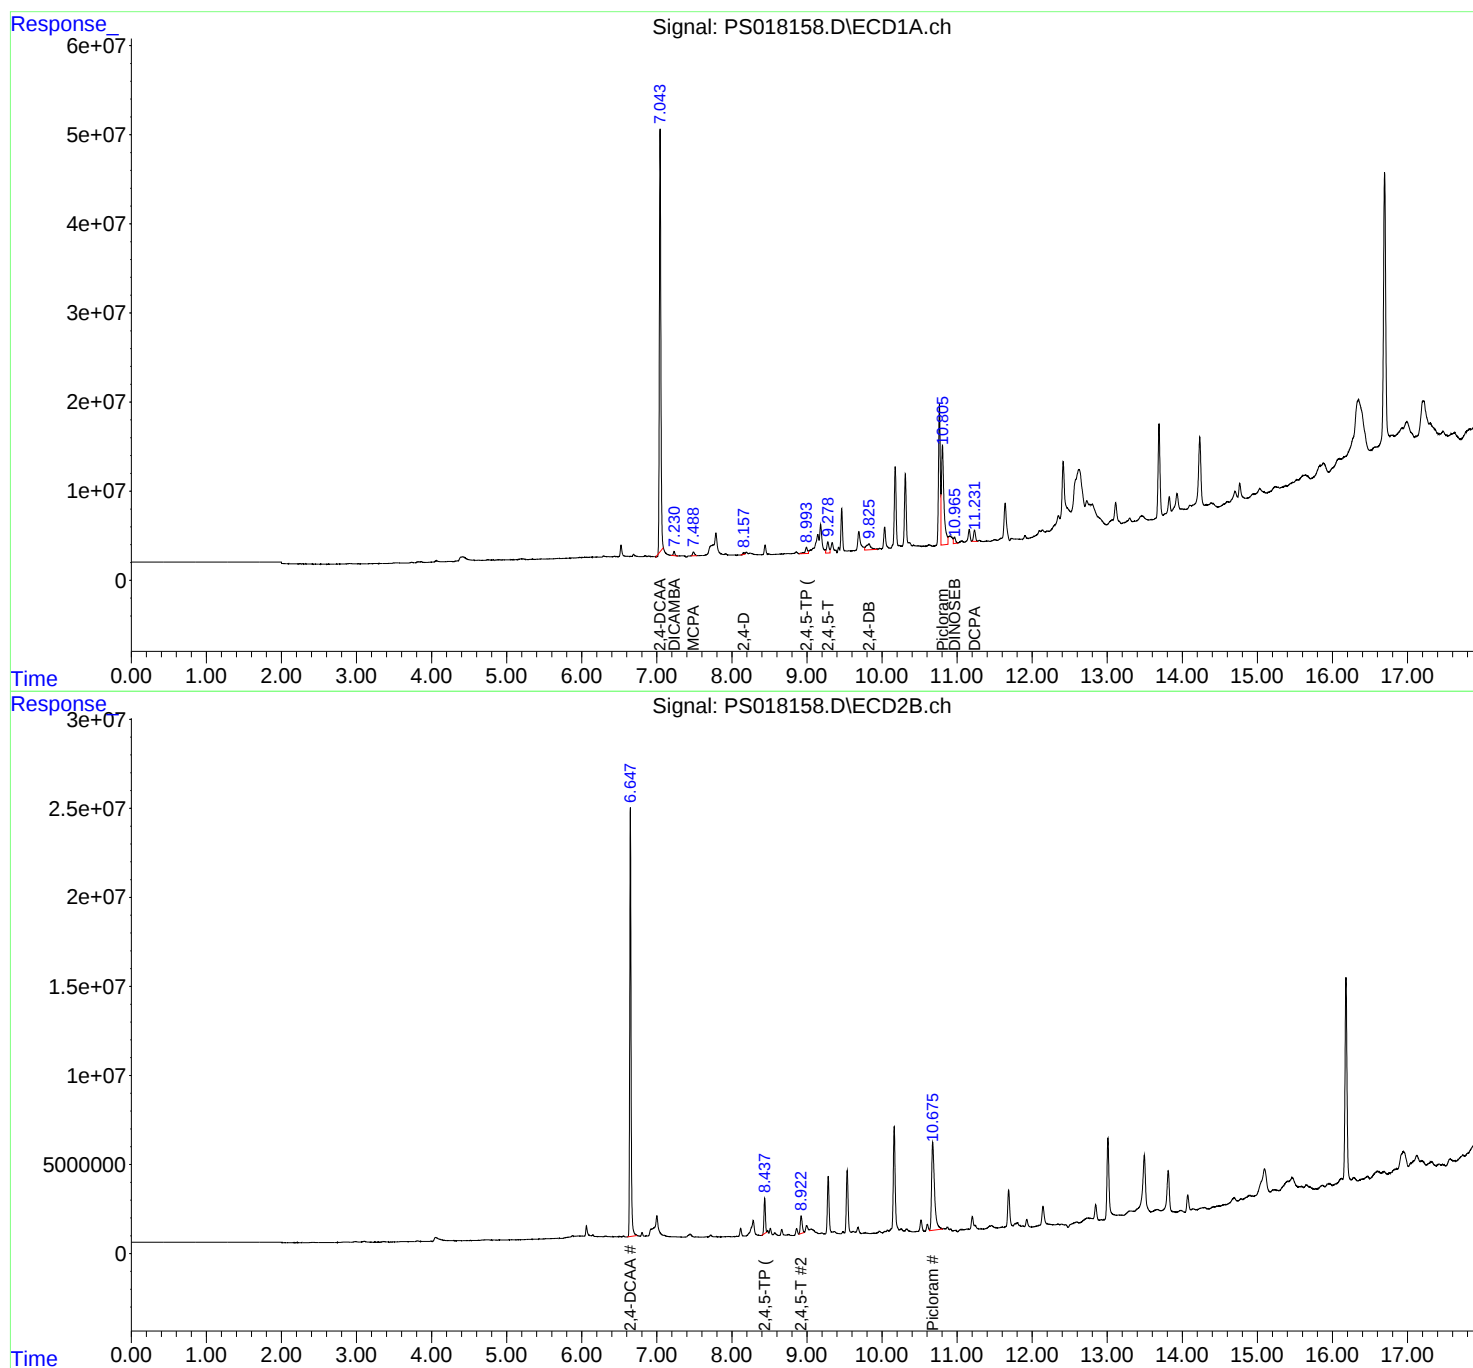


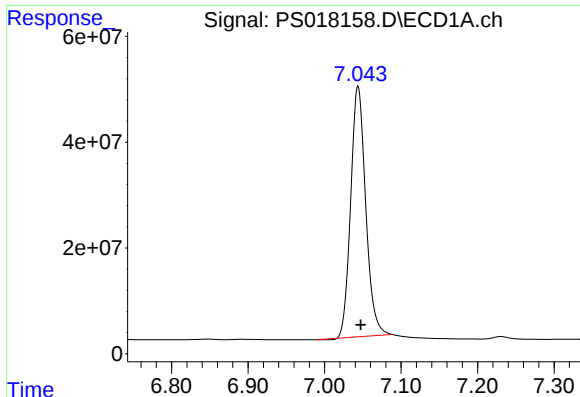

#4 2,4-DCAA


R.T.: 7.044 min
Delta R.T.: -0.004 min
Response: 647195628
Conc: 447.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

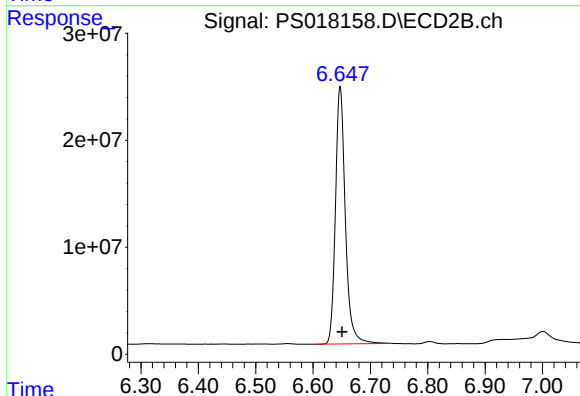


#4 2,4-DCAA

R.T.: 6.647 min
Delta R.T.: -0.003 min
Response: 289447154
Conc: 498.83 ng/ml

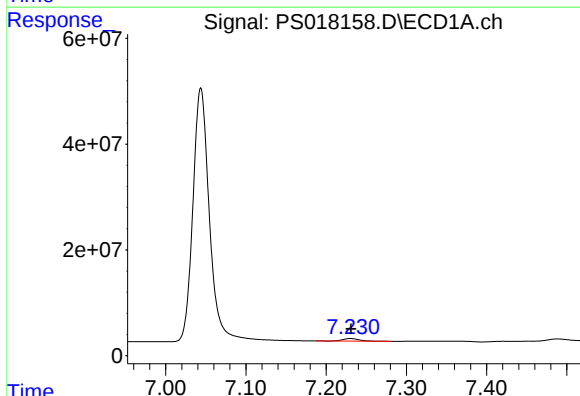


#5 DICAMBA

R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 6736463
Conc: 1.08 ng/ml

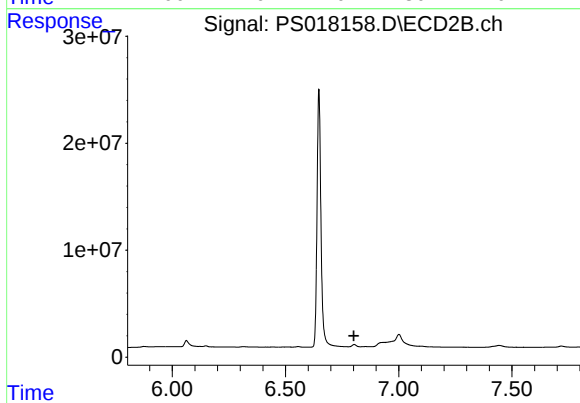

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

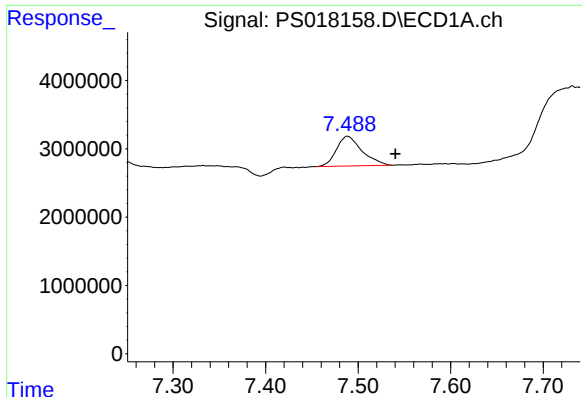

#7 MCPA


R.T.: 7.489 min
Delta R.T.: -0.052 min
Response: 8368416
Conc: 1.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

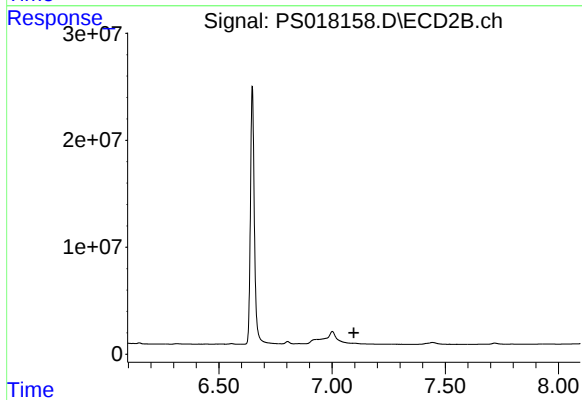


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

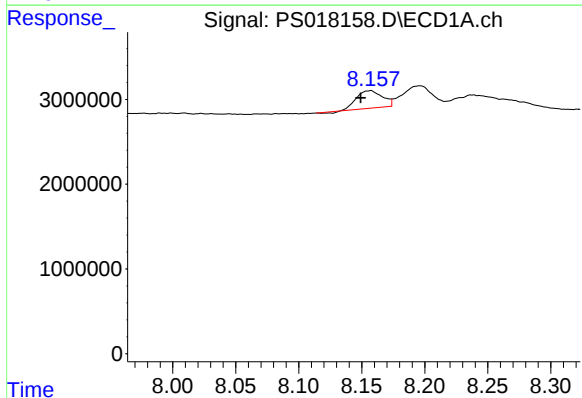


#9 2,4-D

R.T.: 8.157 min
Delta R.T.: 0.007 min
Response: 2923096
Conc: 1.61 ng/ml

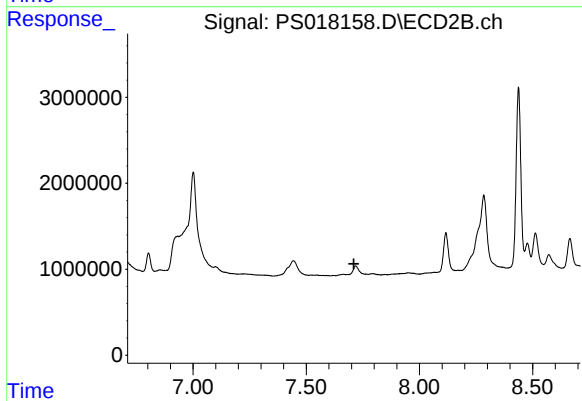

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

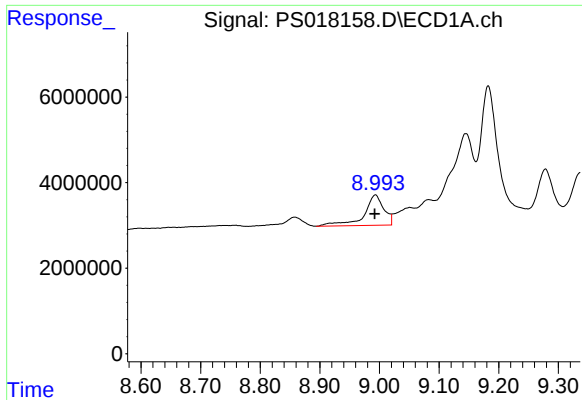

#11 2,4,5-TP (SILVEX)


R.T.: 8.993 min
Delta R.T.: 0.001 min
Response: 16434508
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

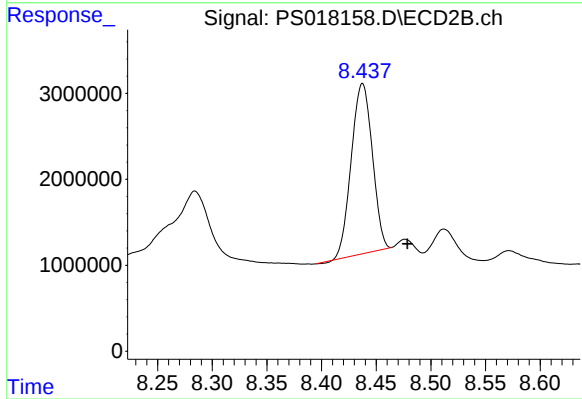


#11 2,4,5-TP (SILVEX)

R.T.: 8.437 min
Delta R.T.: -0.041 min
Response: 26505580
Conc: 7.44 ng/ml

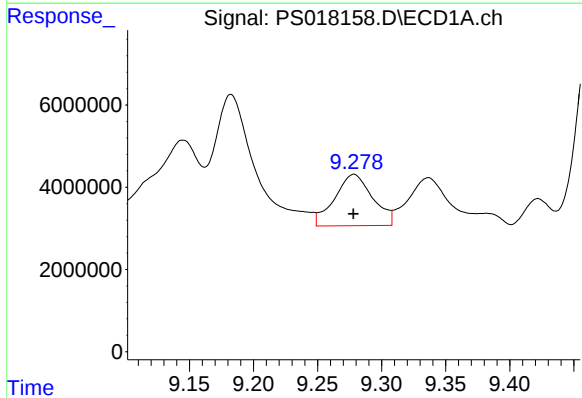


#12 2,4,5-T

R.T.: 9.278 min
Delta R.T.: 0.000 min
Response: 25864410
Conc: 2.92 ng/ml

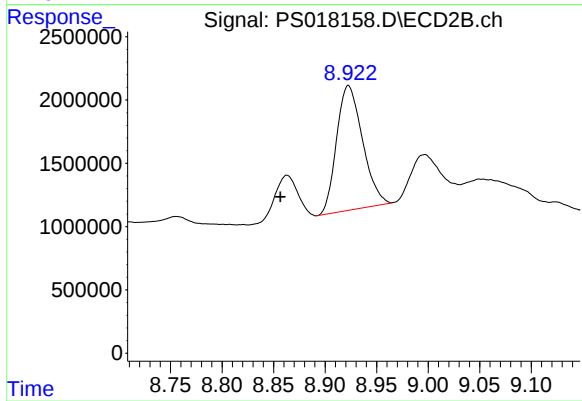

#12 2,4,5-T


R.T.: 8.923 min
Delta R.T.: 0.066 min
Response: 17237783
Conc: 5.27 ng/ml

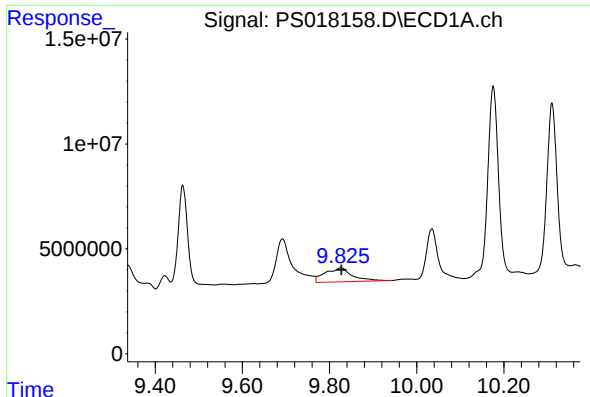

#13 2,4-DB


R.T.: 9.825 min
Delta R.T.: -0.002 min
Response: 28746590
Conc: 17.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

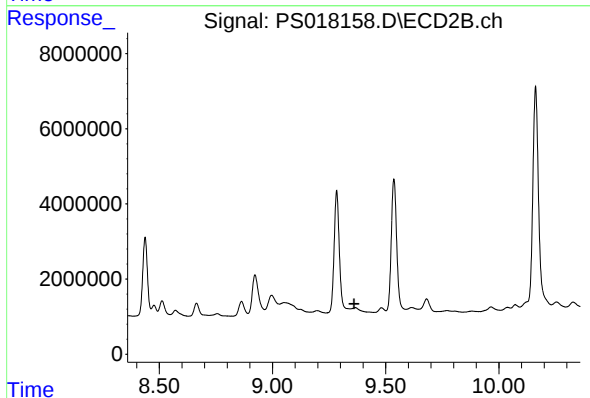


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

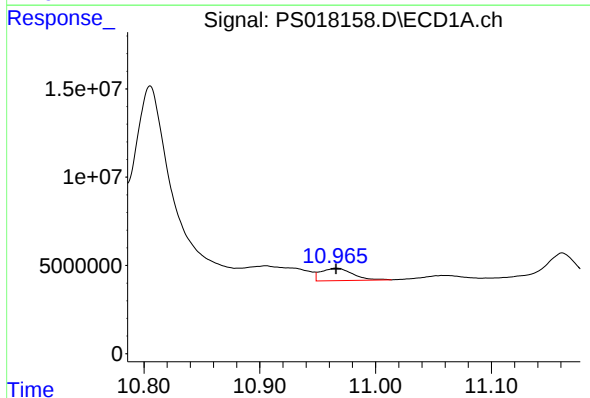


#14 DINOSEB

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 13339610
Conc: 2.03 ng/ml

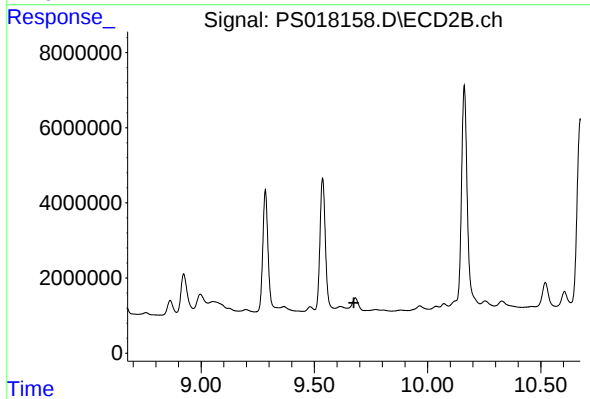

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

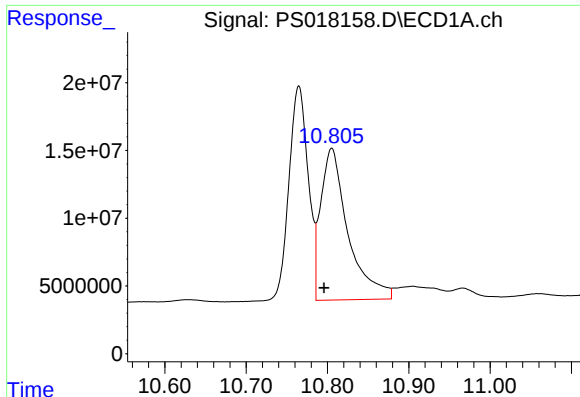

#15 Picloram


R.T.: 10.805 min
Delta R.T.: 0.009 min
Response: 260701405
Conc: 21.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

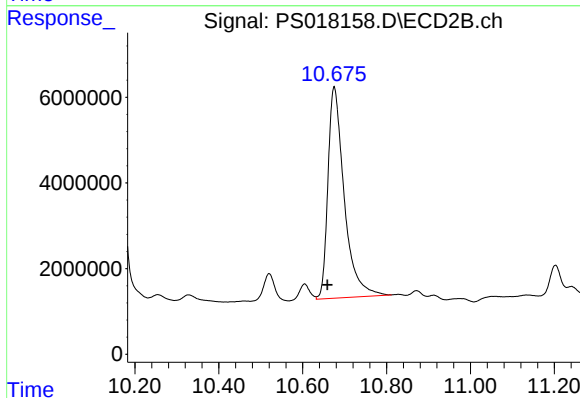


#15 Picloram

R.T.: 10.675 min
Delta R.T.: 0.016 min
Response: 132821960
Conc: 28.40 ng/ml

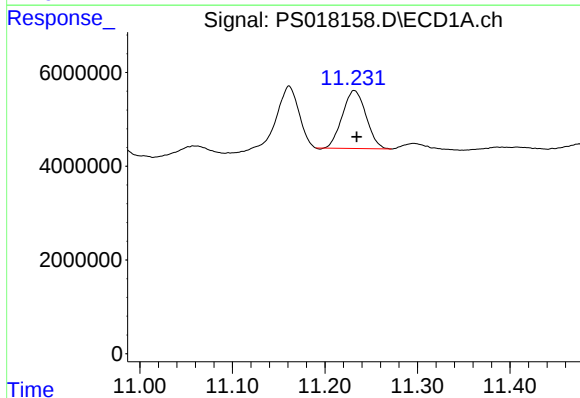

#16 DCPA

R.T.: 11.232 min
Delta R.T.: -0.003 min
Response: 21973187
Conc: 2.03 ng/ml

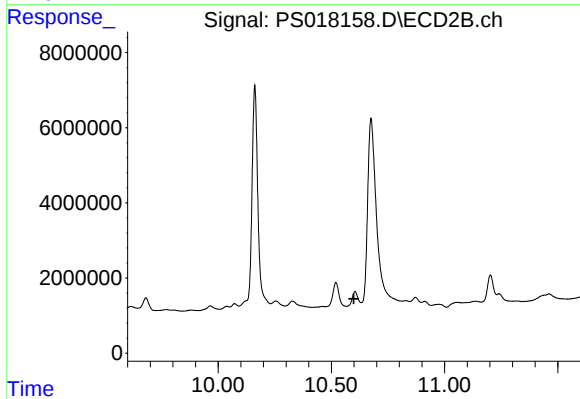

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.