

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
 Data File : PS002952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2019 21:06
 Operator : EI\SJ
 Sample : PB116656BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116656BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 06:14:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.785	0	255.3E6	N.D.	597.055 #
Target Compounds							
1) T	Dalapon	0.000	2.289	0	128.0E6	N.D.	238.860 #
2) T	3,5-DICHL...	0.000	8.955	0	2281180	N.D.	4.048 #
6) T	MCPD	11.955	0.000	20374433	0	17.005	N.D. #
7) T	MCPA	12.251	11.755	552539	2834337	0.312	1.802 #
10) T	Pentachlo...	0.000	13.282	0	2039218	N.D.	0.330 #
14) T	DINOSEB	0.000	15.516	0	7253646	N.D.	4.138 #
15) T	Picloram	16.759	16.707	6174411	38786604	1.952	12.901 #
16) T	DCPA	0.000	16.707	0	38786604	N.D.	12.522 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
Data File : PS002952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2019 21:06
Operator : EI\SJ
Sample : PB116656BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116656BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 06:14:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

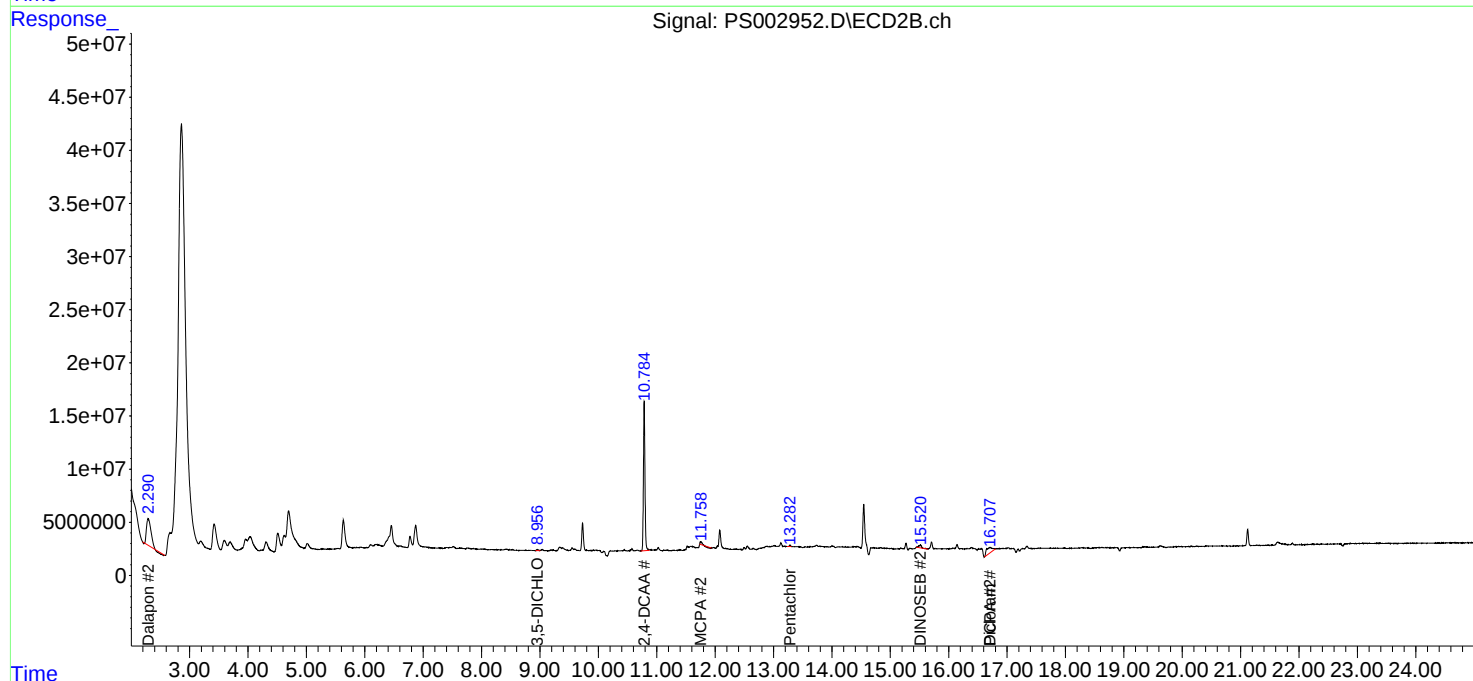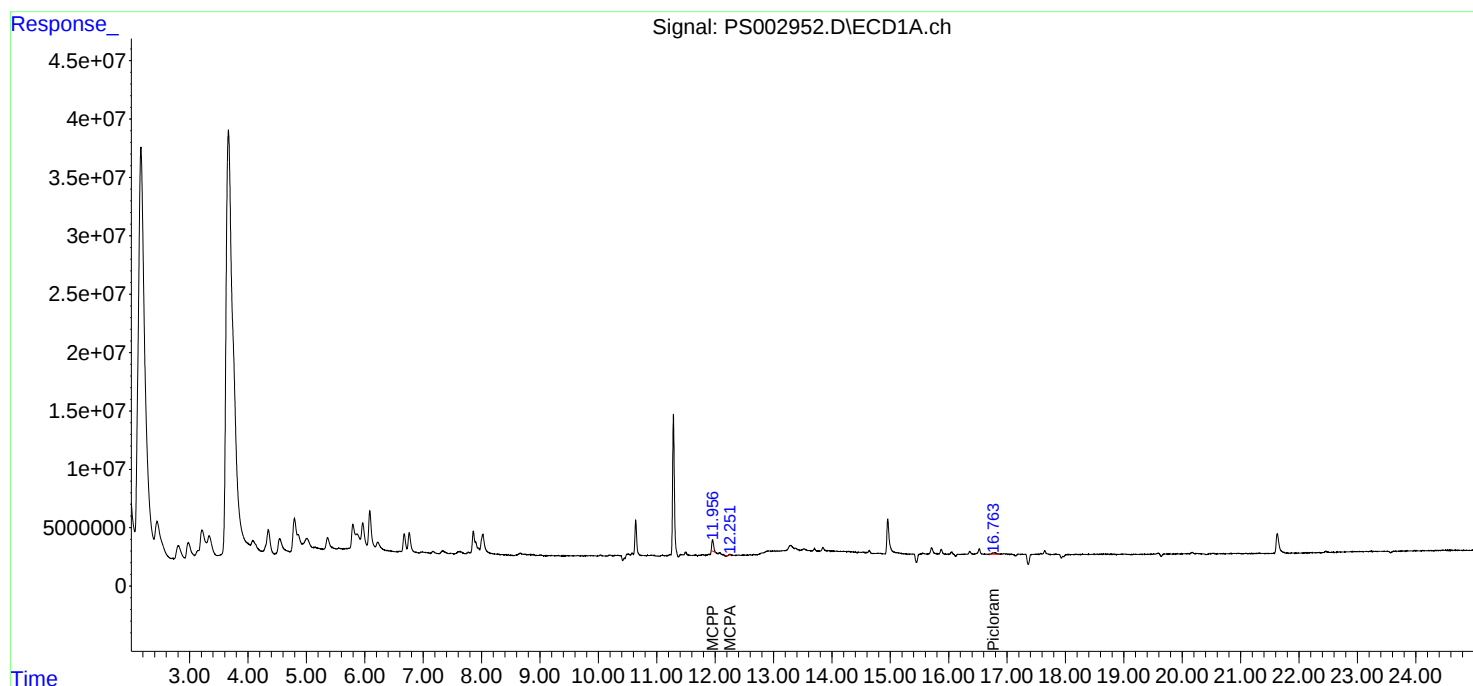


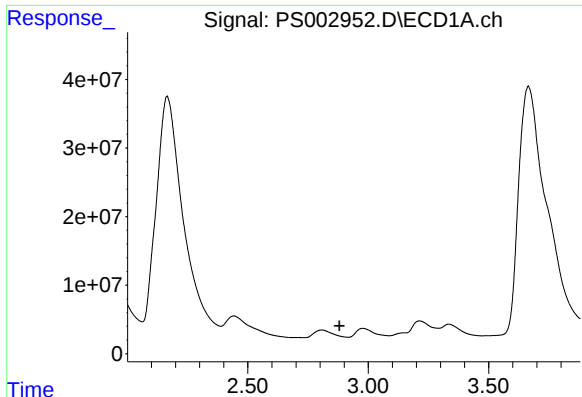

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656BL

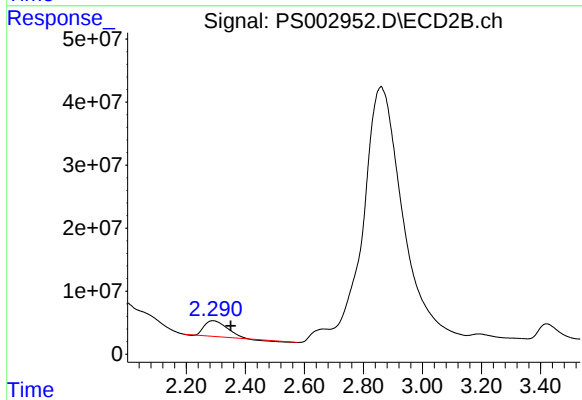


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.061 min
Response: 128010188
Conc: 238.86 ng/ml

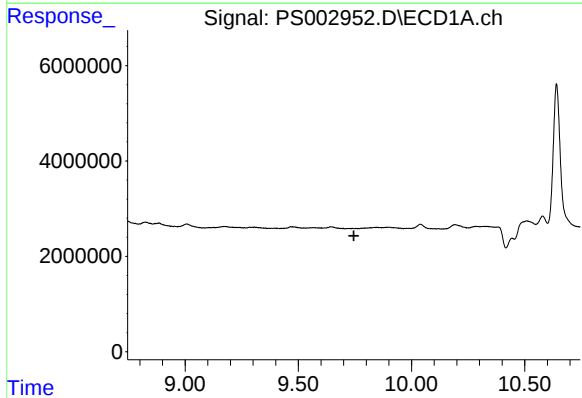


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

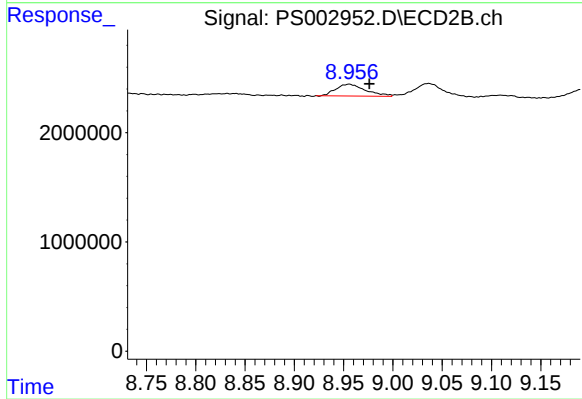

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.955 min
Delta R.T.: -0.021 min
Response: 2281180
Conc: 4.05 ng/ml

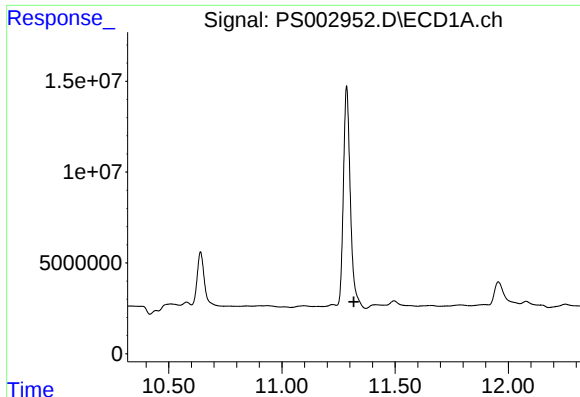

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656BL

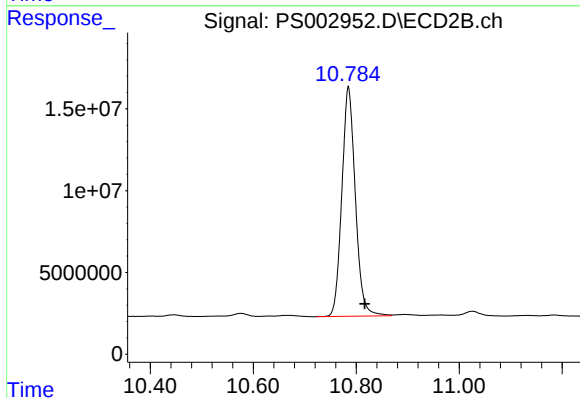


#4 2,4-DCAA

R.T.: 10.785 min
Delta R.T.: -0.032 min
Response: 255268214
Conc: 597.05 ng/ml

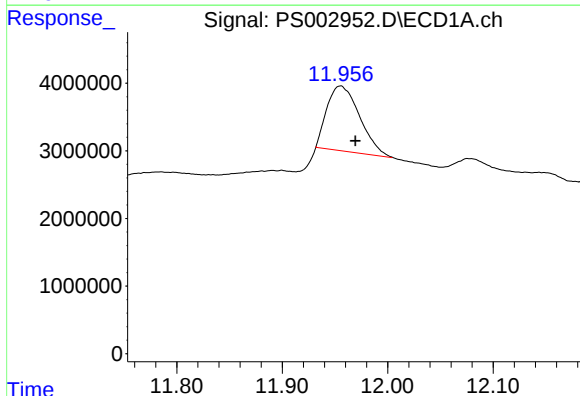


#6 MCP

R.T.: 11.955 min
Delta R.T.: -0.014 min
Response: 20374433
Conc: 17.01 ug/ml

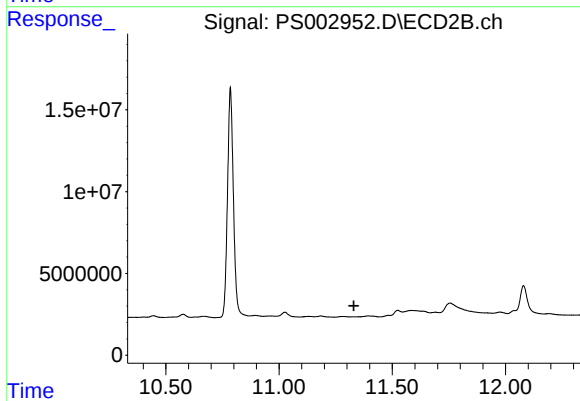

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

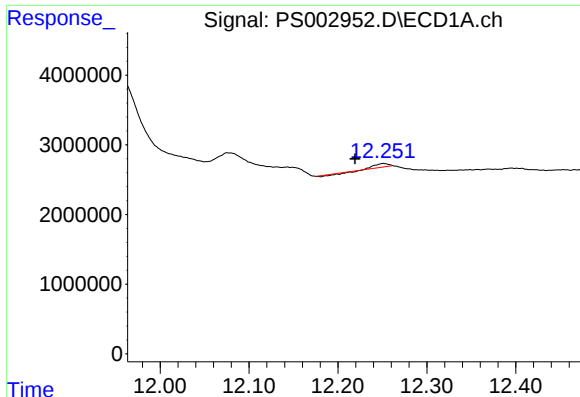

#7 MCPA


R.T.: 12.251 min
Delta R.T.: 0.032 min
Response: 552539
Conc: 0.31 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB116656BL

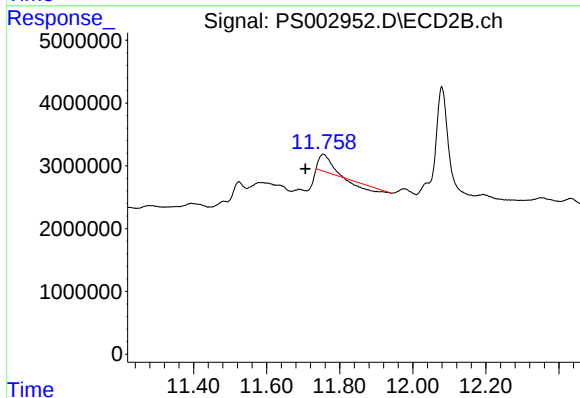


#7 MCPA

R.T.: 11.755 min
Delta R.T.: 0.049 min
Response: 2834337
Conc: 1.80 ug/ml

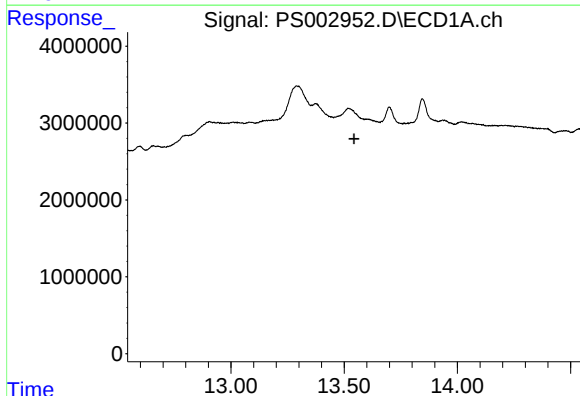


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.543 min
Response: 0
Conc: N.D.

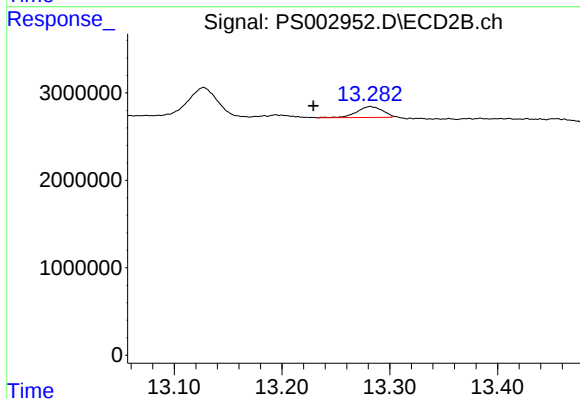

#10 Pentachlorophenol


R.T.: 13.282 min
Delta R.T.: 0.053 min
Response: 2039218
Conc: 0.33 ng/ml

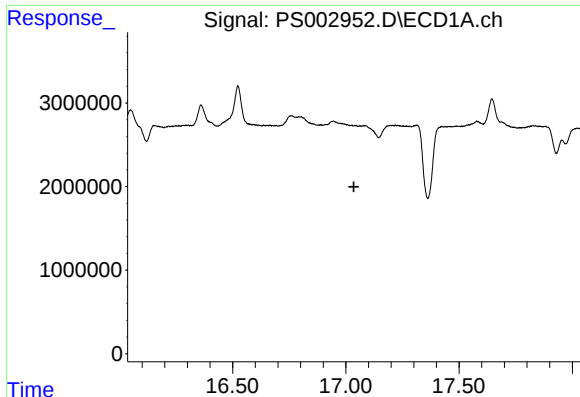

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656BL

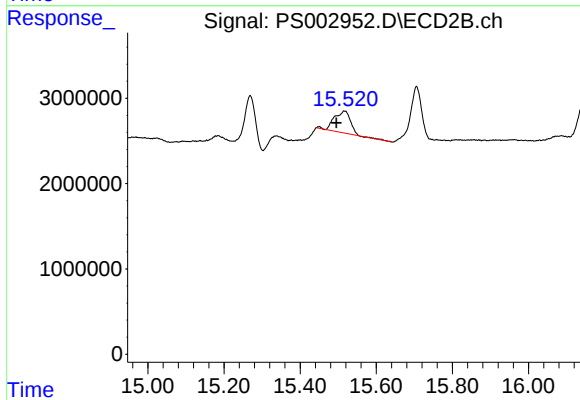


#14 DINOSEB

R.T.: 15.516 min
Delta R.T.: 0.021 min
Response: 7253646
Conc: 4.14 ng/ml

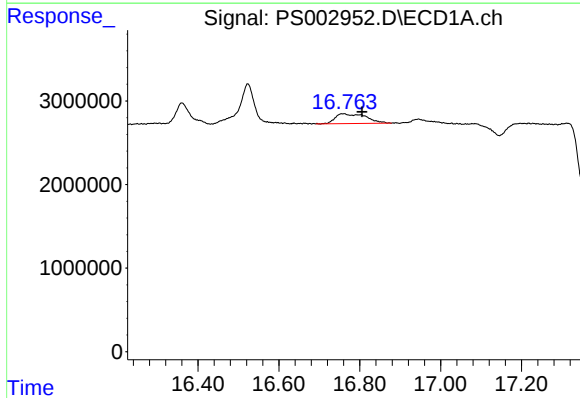


#15 Picloram

R.T.: 16.759 min
Delta R.T.: -0.046 min
Response: 6174411
Conc: 1.95 ng/ml

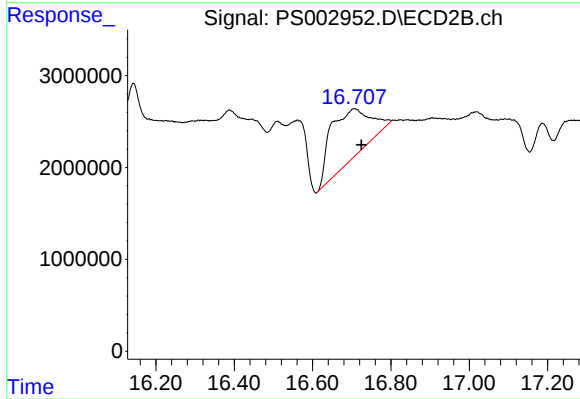

#15 Picloram


R.T.: 16.707 min
Delta R.T.: -0.017 min
Response: 38786604
Conc: 12.90 ng/ml

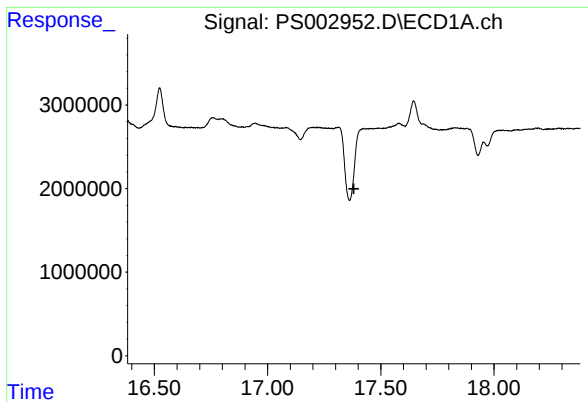

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656BL

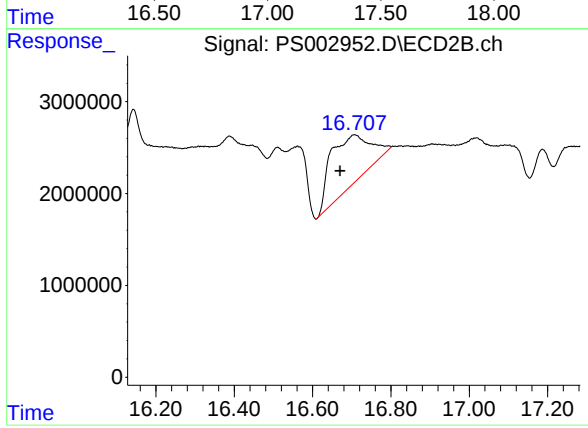

#16 DCPA

R.T.: 16.707 min
Delta R.T.: 0.038 min
Response: 38786604
Conc: 12.52 ng/ml