

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
 Data File : PS002954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2019 22:08
 Operator : EI\SJ
 Sample : PB116656TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116656TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 06:15:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.780	0	78513990	N.D.	183.639 #
Target Compounds							
1) T	Dalapon	0.000	2.285	0	66434447	N.D.	123.963 #
2) T	3,5-DICHL...	0.000	8.946	0	9088048	N.D.	16.126 #
7) T	MCPA	0.000	11.724	0	26477132	N.D.	16.832 #
8) T	DICHLORPROP	12.832	0.000	1225965	0	3.197	N.D. #
9) T	2,4-D	0.000	12.743	0	3529554	N.D.	7.040 #
12) T	2,4,5-T	0.000	14.388	0	3204761	N.D.	1.675 #
14) T	DINOSEB	0.000	15.484	0	4091556	N.D.	2.334 #
15) T	Picloram	0.000	16.697	0	31353629	N.D.	10.429 #
16) T	DCPA	0.000	16.697	0	31353629	N.D.	10.122 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
Data File : PS002954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2019 22:08
Operator : EI\SJ
Sample : PB116656TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116656TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 06:15:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

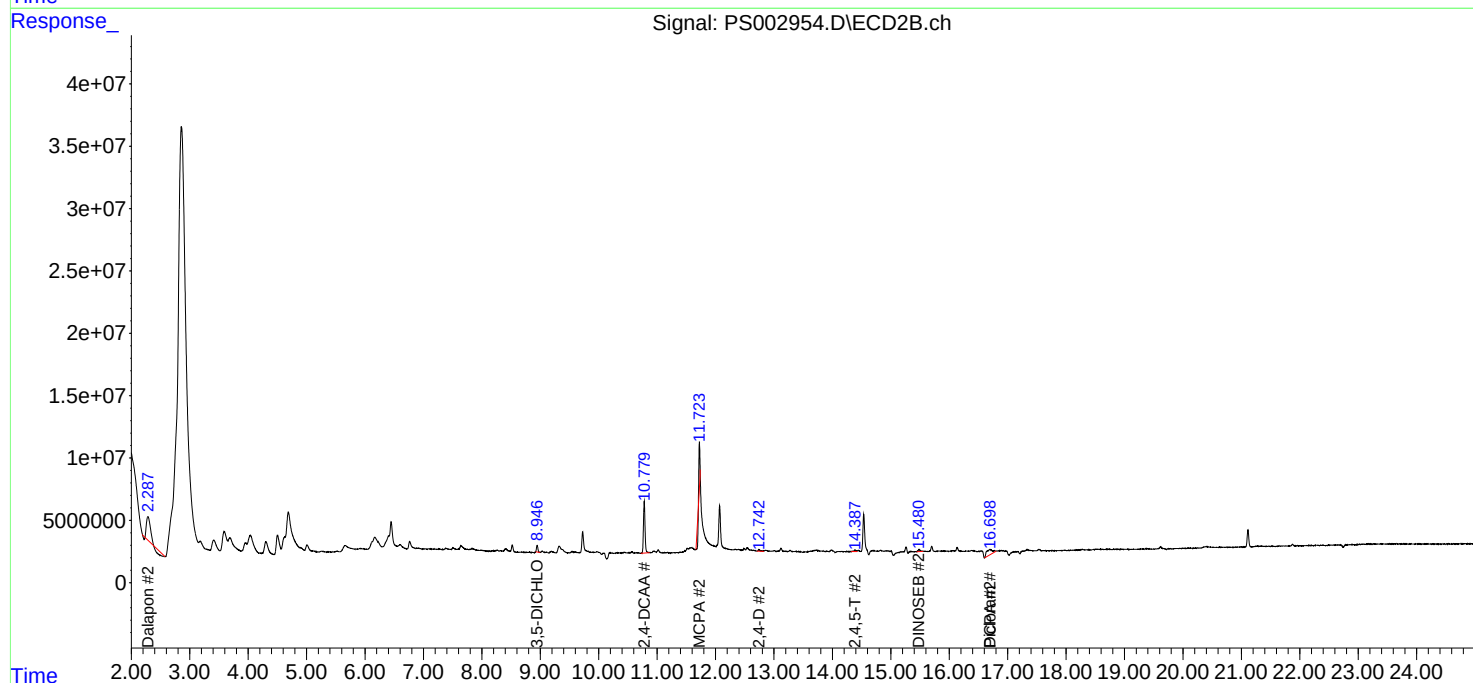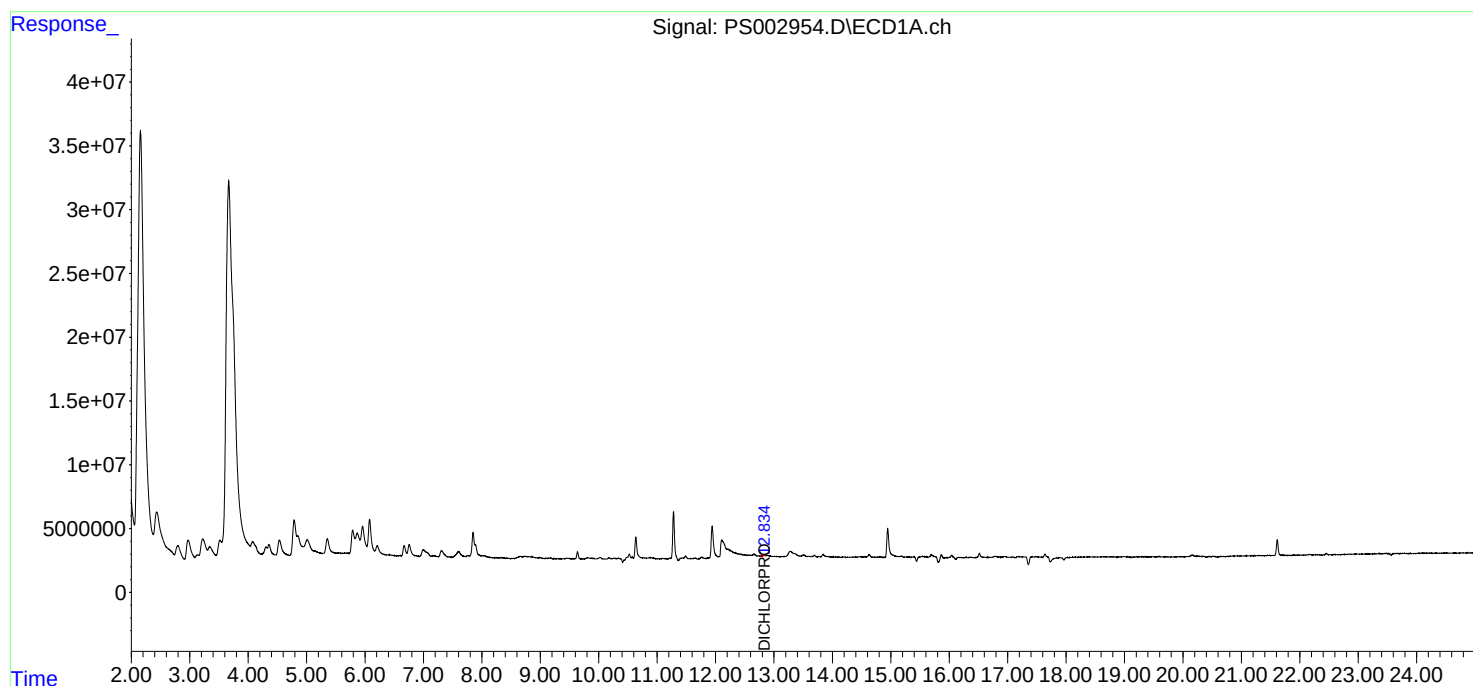


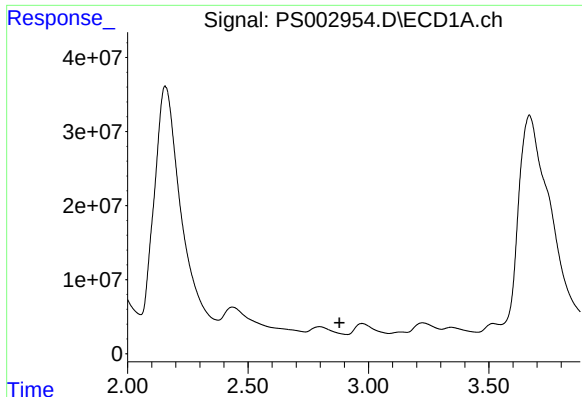

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

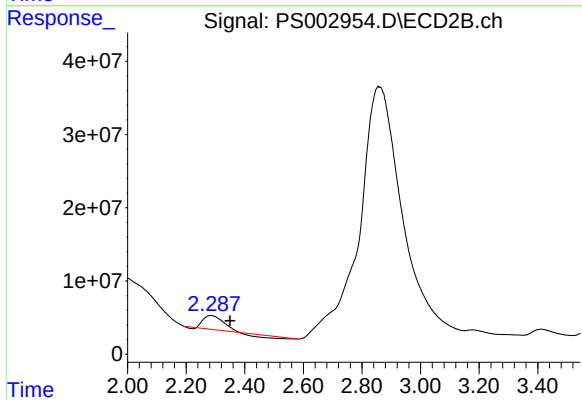


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.066 min
Response: 66434447
Conc: 123.96 ng/ml

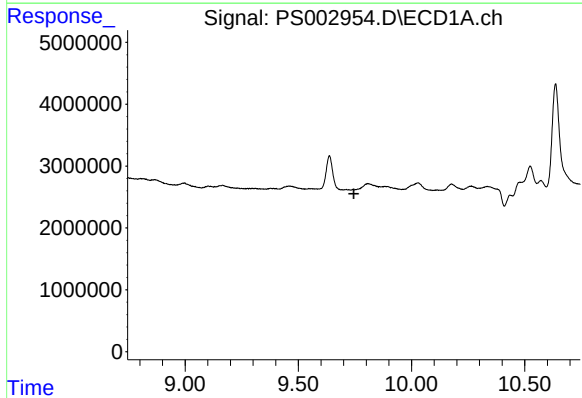


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

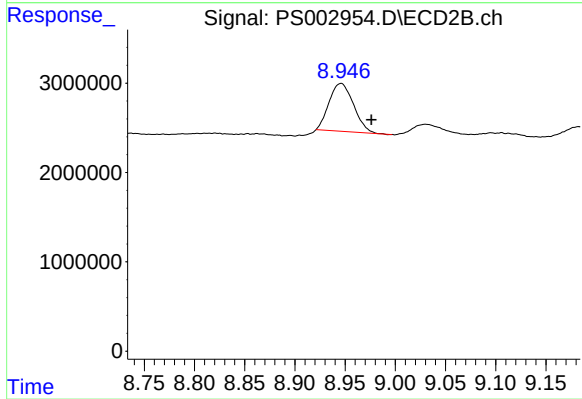

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.946 min
Delta R.T.: -0.031 min
Response: 9088048
Conc: 16.13 ng/ml

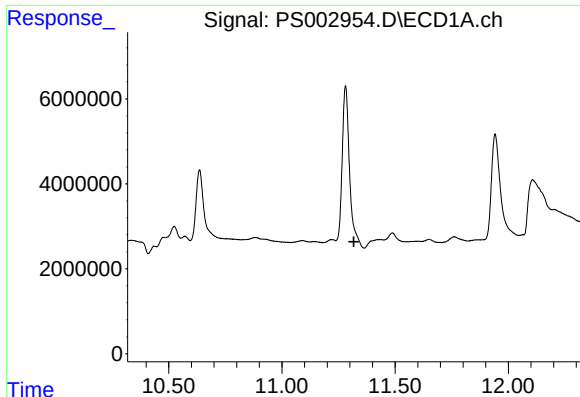

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

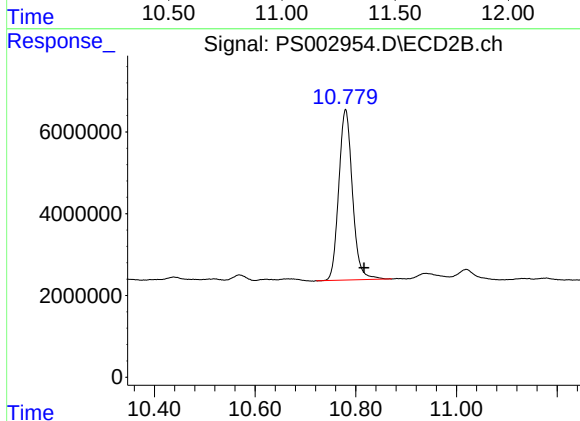


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 78513990
Conc: 183.64 ng/ml

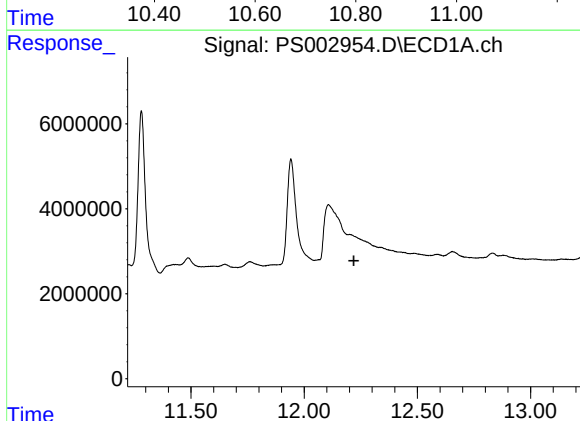


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

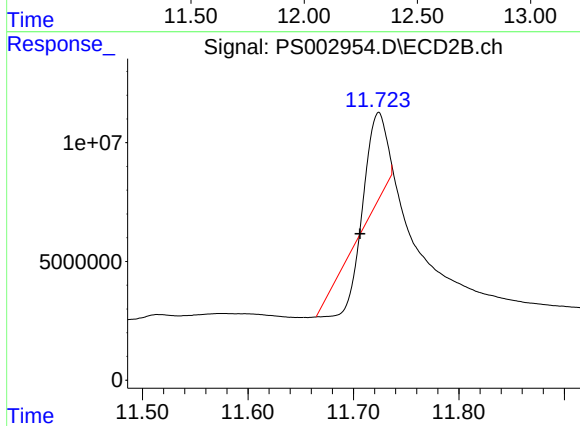

#7 MCPA


R.T.: 11.724 min
Delta R.T.: 0.018 min
Response: 26477132
Conc: 16.83 ug/ml

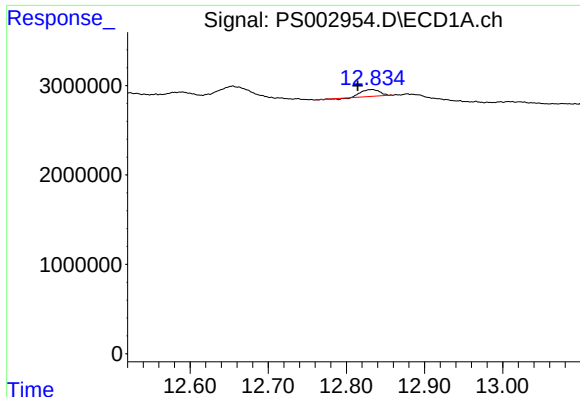

#8 DICHLORPROP


R.T.: 12.832 min
Delta R.T.: 0.017 min
Response: 1225965
Conc: 3.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116656TB

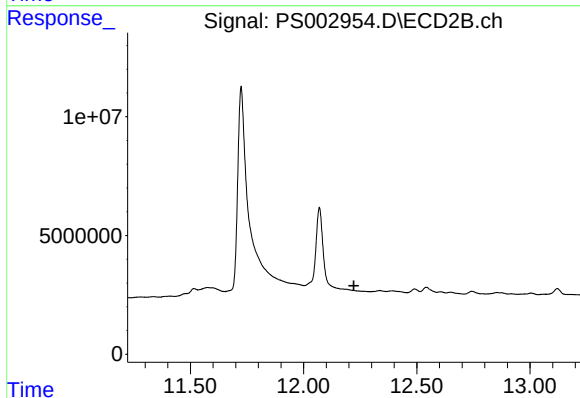


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.222 min
Response: 0
Conc: N.D.

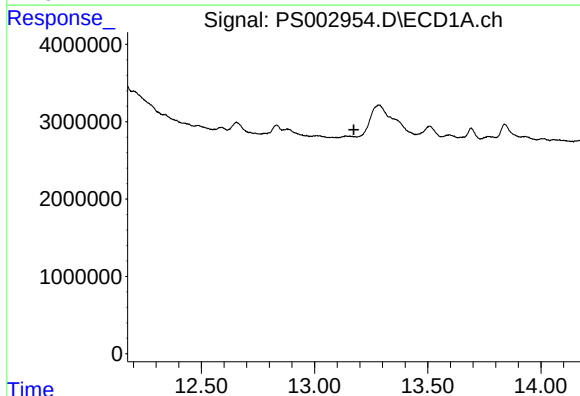


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.173 min
Response: 0
Conc: N.D.

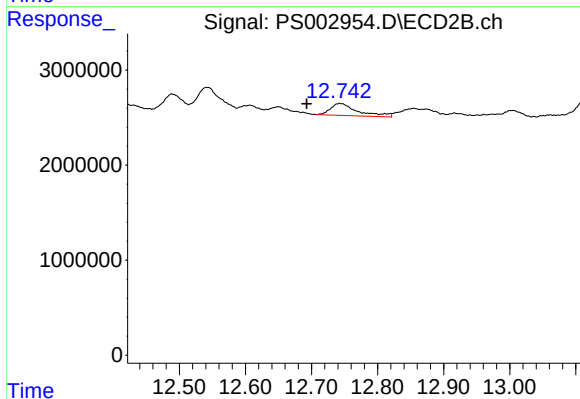

#9 2,4-D


R.T.: 12.743 min
Delta R.T.: 0.050 min
Response: 3529554
Conc: 7.04 ng/ml

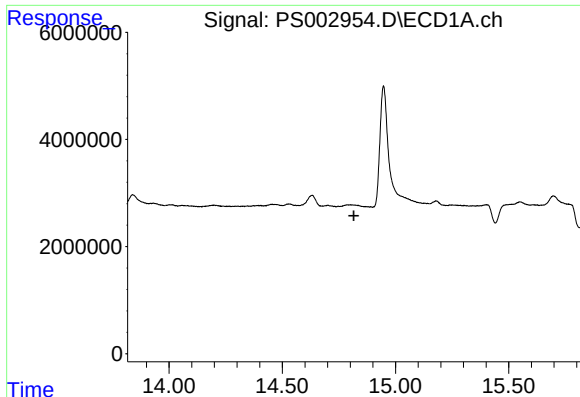

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

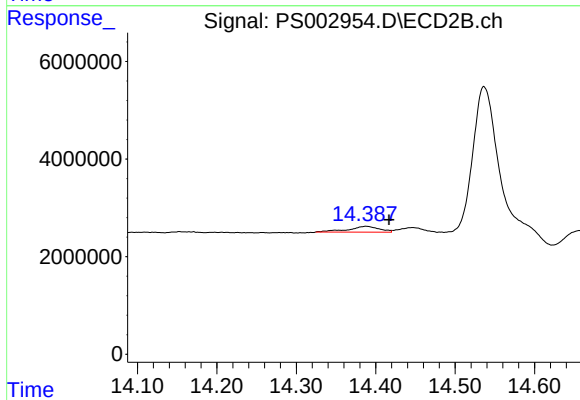


#12 2,4,5-T

R.T.: 14.388 min
Delta R.T.: -0.029 min
Response: 3204761
Conc: 1.67 ng/ml

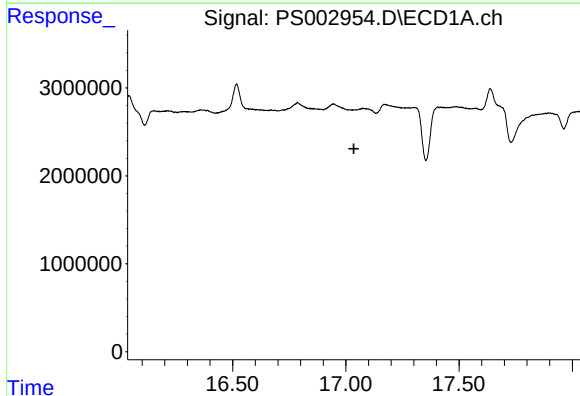


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

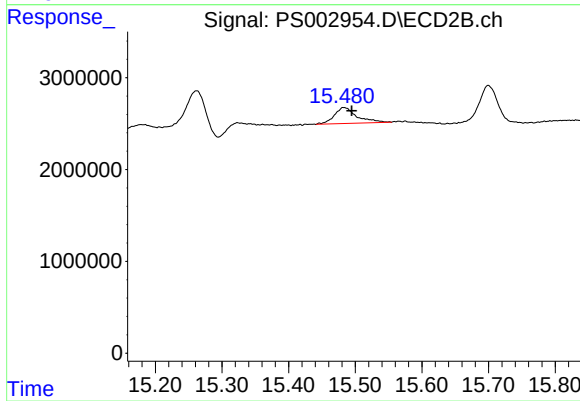

#14 DINOSEB


R.T.: 15.484 min
Delta R.T.: -0.011 min
Response: 4091556
Conc: 2.33 ng/ml

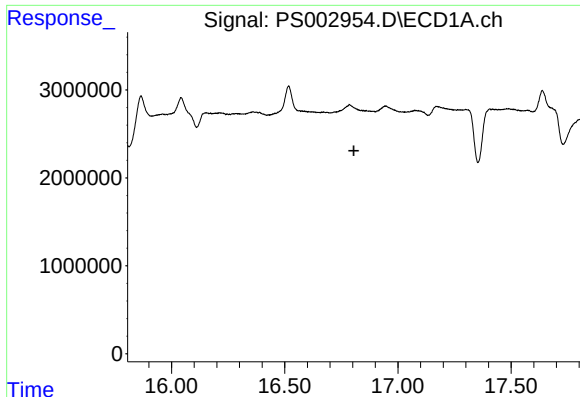

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

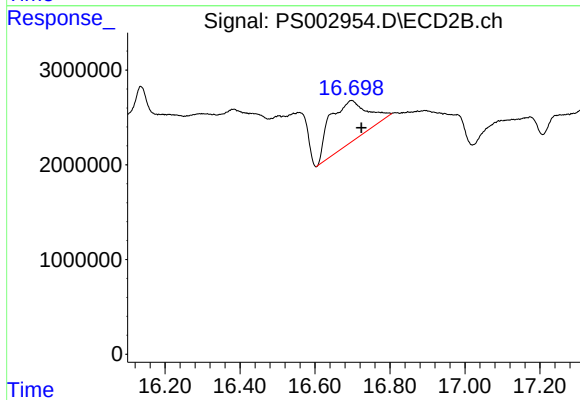


#15 Picloram

R.T.: 16.697 min
Delta R.T.: -0.027 min
Response: 31353629
Conc: 10.43 ng/ml

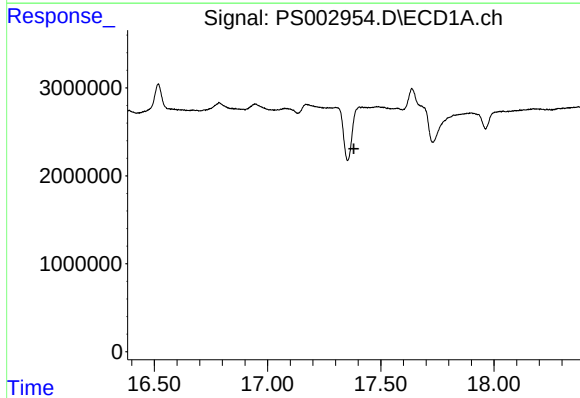

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

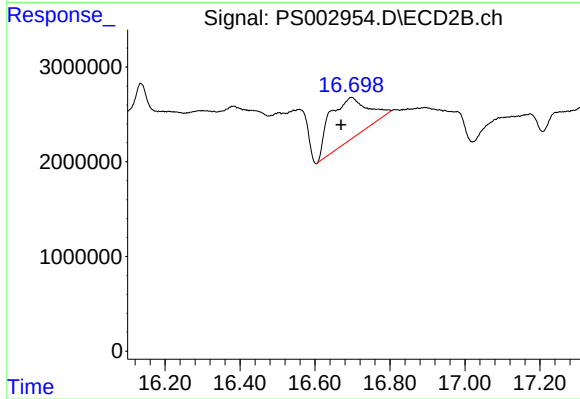

#16 DCPA

R.T.: 16.697 min
Delta R.T.: 0.028 min
Response: 31353629
Conc: 10.12 ng/ml