

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
 Data File : PS002961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 01:46
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 06:17:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.784	0	318.8E6	N.D.	745.672 #
Target Compounds							
1) T	Dalapon	2.848	2.316	190.9E6	354.5E6	346.125	661.423 #
2) T	3,5-DICHL...	0.000	8.943	0	224.4E6	N.D.	398.194 #
3) T	4-Nitroph...	0.000	9.932	0	148.2E6	N.D.	709.022 #
5) T	DICAMBA	11.592	11.064	632.2E6	710.1E6	394.423	447.573
8) T	DICHLORPROP	0.000	12.190	0	272.7E6	N.D.	713.244 #
9) T	2,4-D	0.000	12.661	0	313.8E6	N.D.	625.922 #
10) T	Pentachlo...	13.511	13.197	3067.4E6	1050.6E6	478.318	169.982 #
11) T	2,4,5-TP ...	14.386	13.822	1847.6E6	1769.5E6	733.665	713.397
12) T	2,4,5-T	14.784	14.384	1798.6E6	1030.5E6	737.310	538.526 #
14) T	DINOSEB	17.002	15.462	1350.0E6	168.1E6	717.567	95.893 #
15) T	Picloram	16.772	16.691	2385.9E6	2283.6E6	754.179	759.569
16) T	DCPA	17.349	16.691	1532.5E6	2283.6E6	509.591	737.209 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
Data File : PS002961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 01:46
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 06:17:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

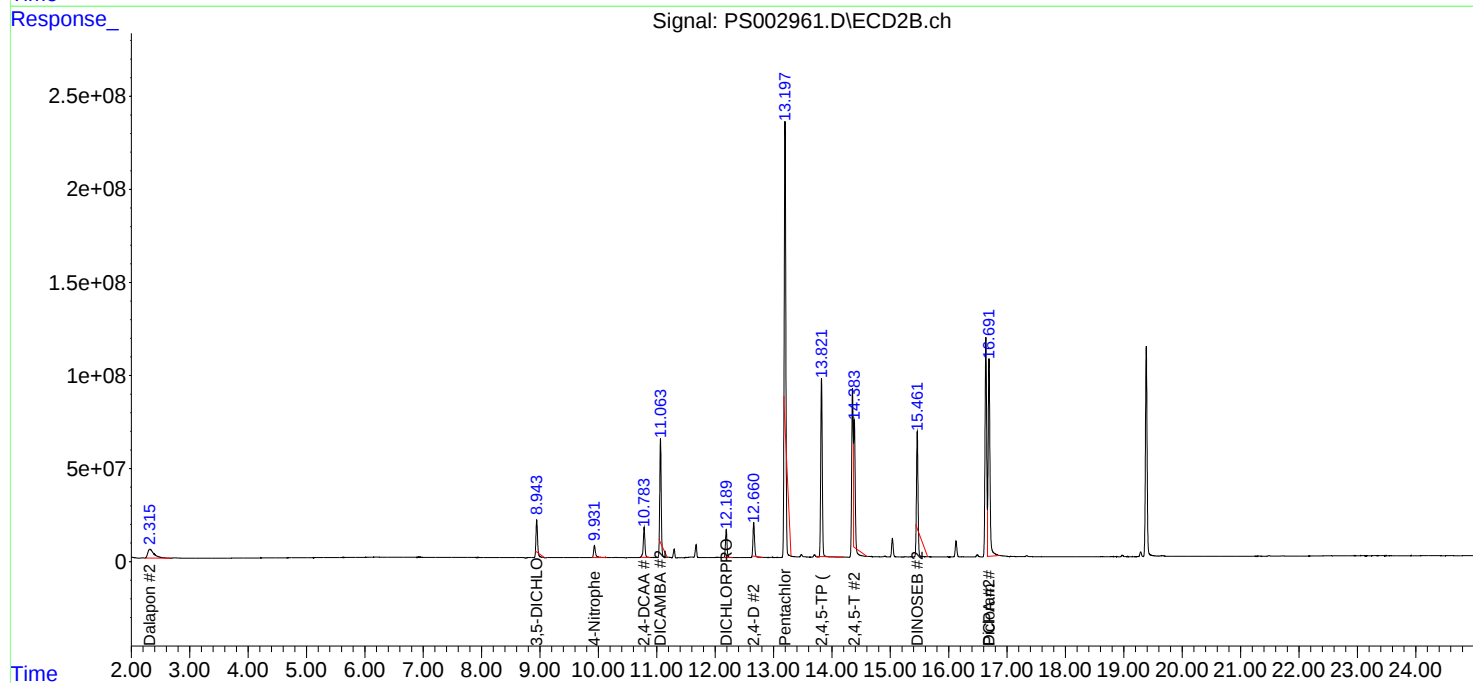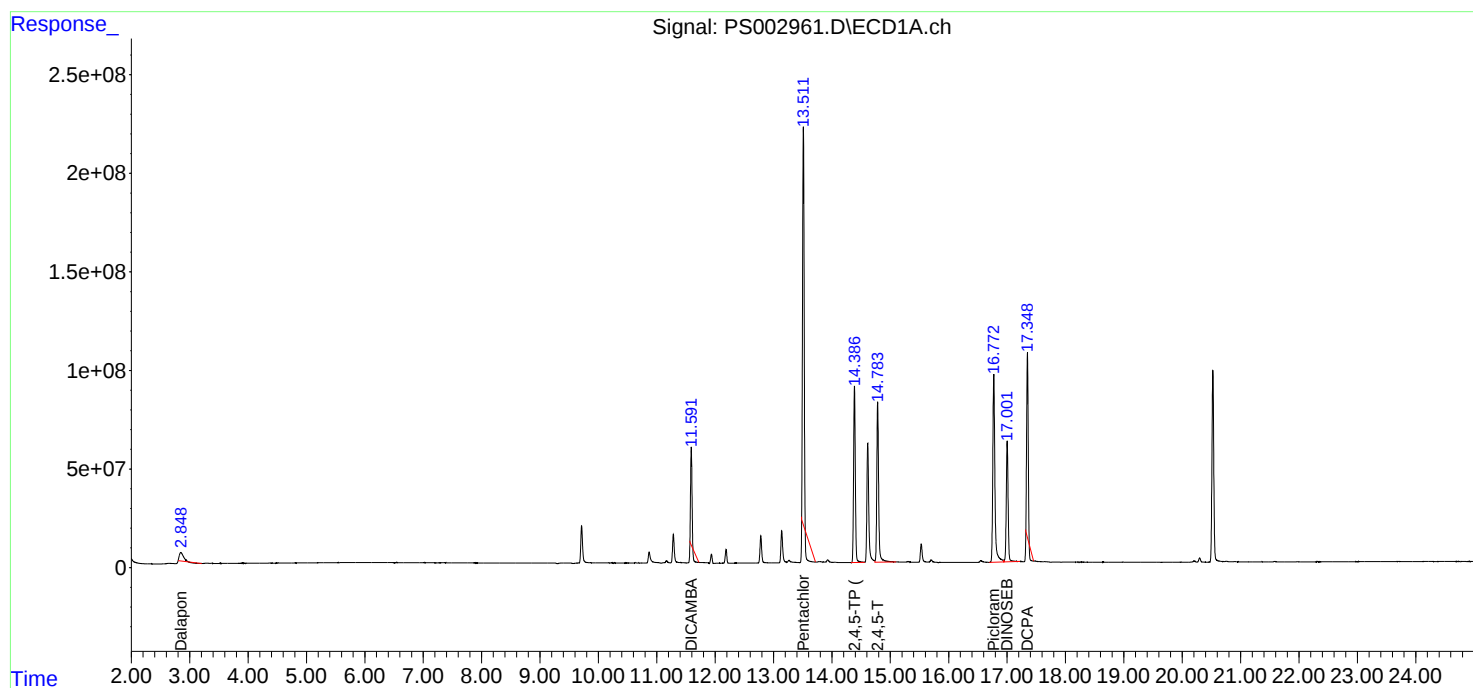


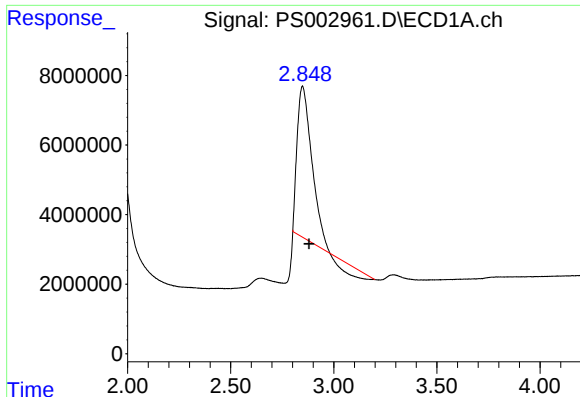

#1 Dalapon


R.T.: 2.848 min
Delta R.T.: -0.032 min
Response: 190938837
Conc: 346.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

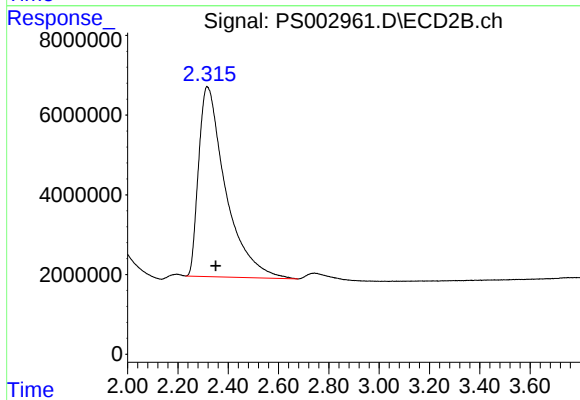


#1 Dalapon

R.T.: 2.316 min
Delta R.T.: -0.034 min
Response: 354470687
Conc: 661.42 ng/ml

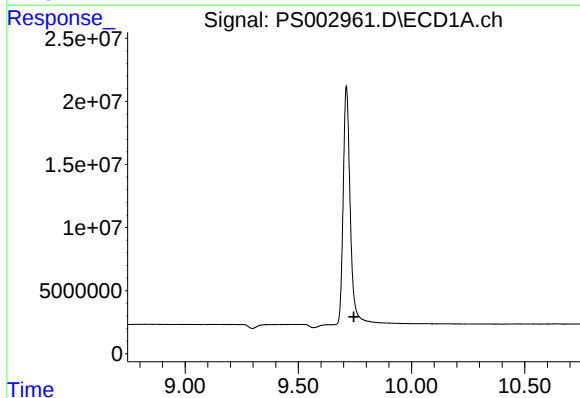


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

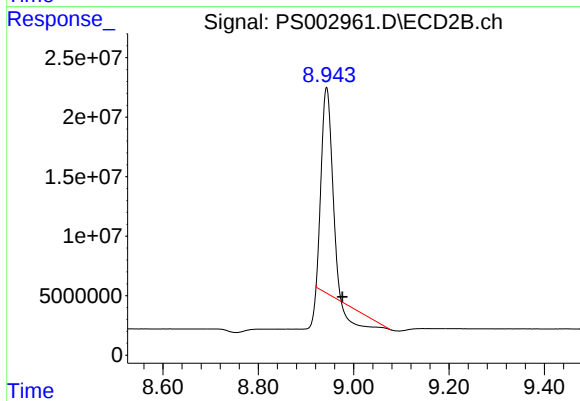

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: -0.033 min
Response: 224409165
Conc: 398.19 ng/ml

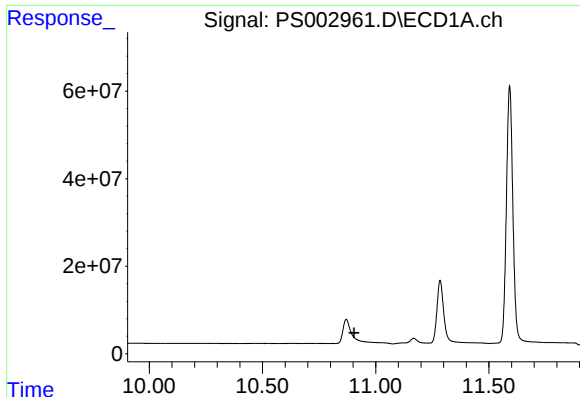

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

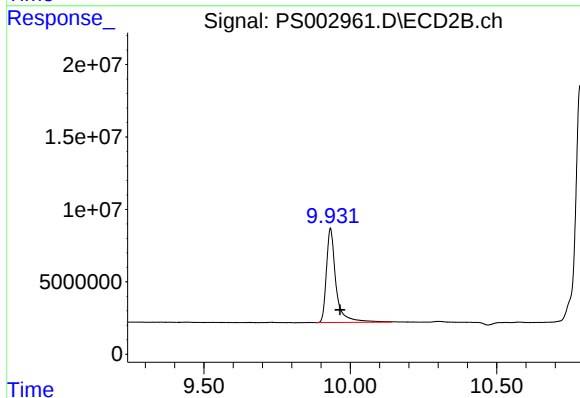


#3 4-Nitrophenol

R.T.: 9.932 min
Delta R.T.: -0.033 min
Response: 148201592
Conc: 709.02 ng/ml

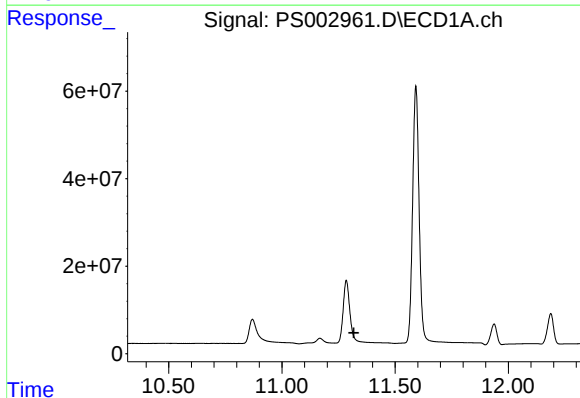


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

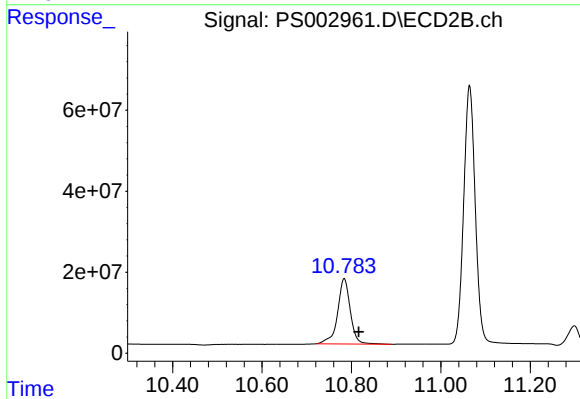

#4 2,4-DCAA


R.T.: 10.784 min
Delta R.T.: -0.033 min
Response: 318808778
Conc: 745.67 ng/ml

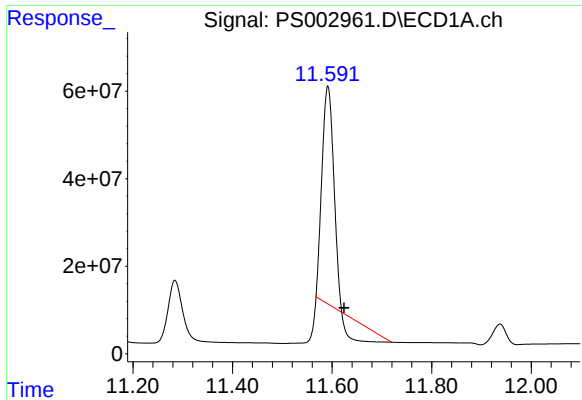

#5 DICAMBA


R.T.: 11.592 min
Delta R.T.: -0.033 min
Response: 632215731
Conc: 394.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

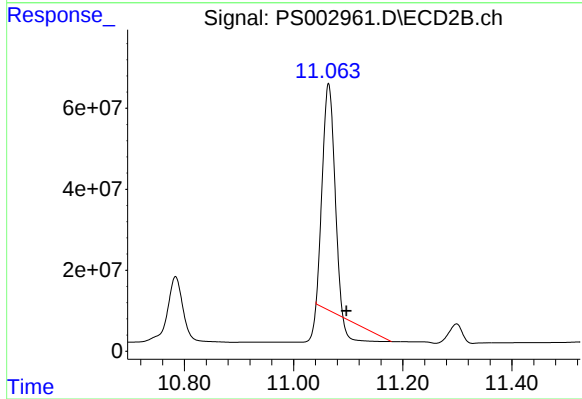


#5 DICAMBA

R.T.: 11.064 min
Delta R.T.: -0.033 min
Response: 710148957
Conc: 447.57 ng/ml

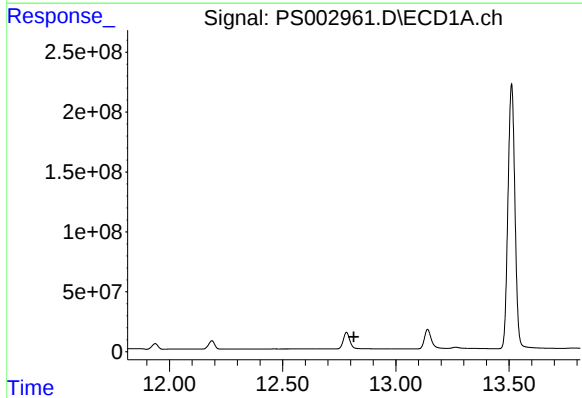


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

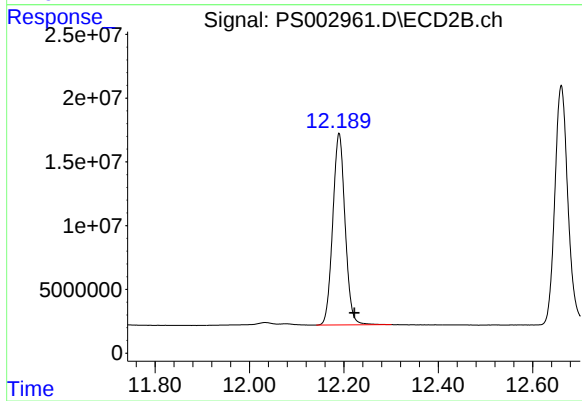

#8 DICHLORPROP


R.T.: 12.190 min
Delta R.T.: -0.032 min
Response: 272702526
Conc: 713.24 ng/ml

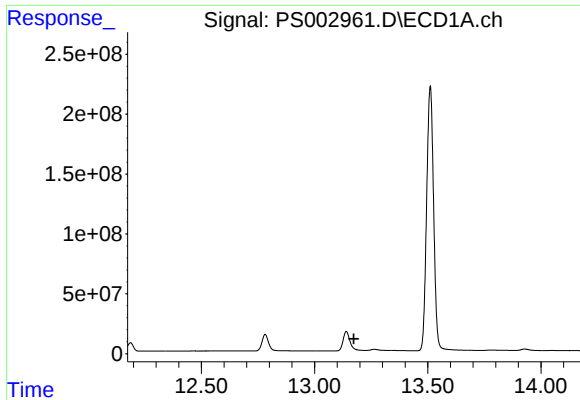

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

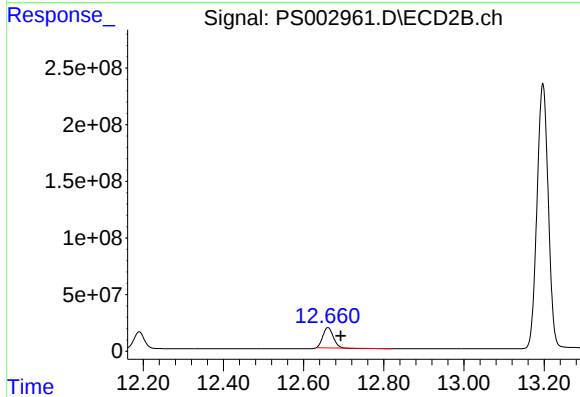


#9 2,4-D

R.T.: 12.661 min
Delta R.T.: -0.032 min
Response: 313828545
Conc: 625.92 ng/ml

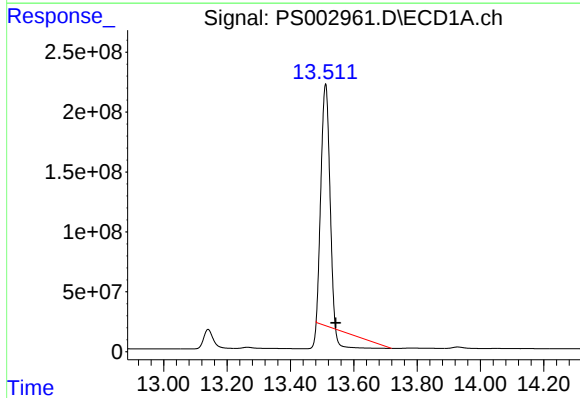


#10 Pentachlorophenol

R.T.: 13.511 min
Delta R.T.: -0.033 min
Response: 3067448870
Conc: 478.32 ng/ml

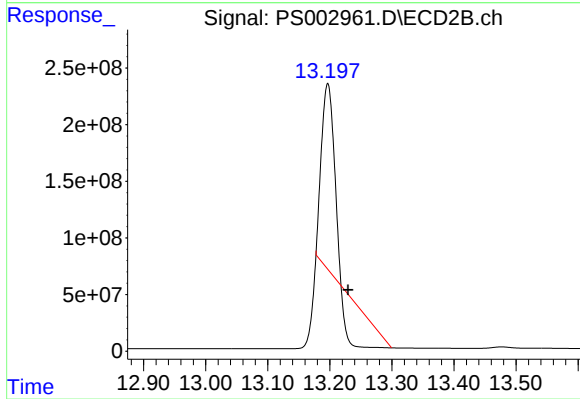

#10 Pentachlorophenol


R.T.: 13.197 min
Delta R.T.: -0.033 min
Response: 1050592747
Conc: 169.98 ng/ml

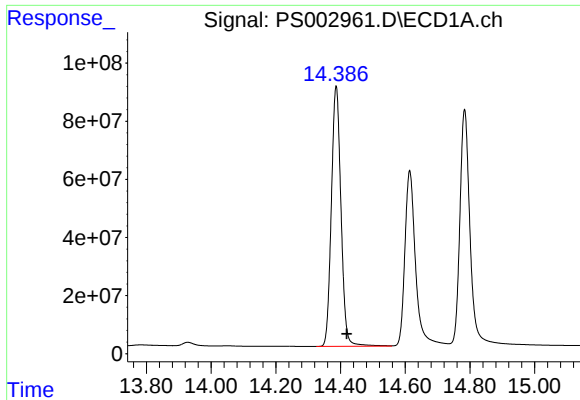

#11 2,4,5-TP (SILVEX)


R.T.: 14.386 min
Delta R.T.: -0.033 min
Response: 1847642102
Conc: 733.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

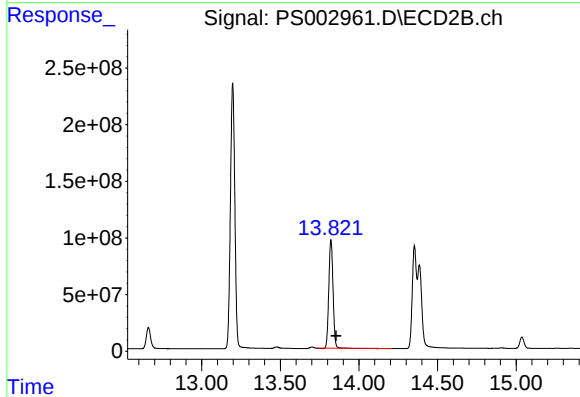


#11 2,4,5-TP (SILVEX)

R.T.: 13.822 min
Delta R.T.: -0.033 min
Response: 1769478414
Conc: 713.40 ng/ml

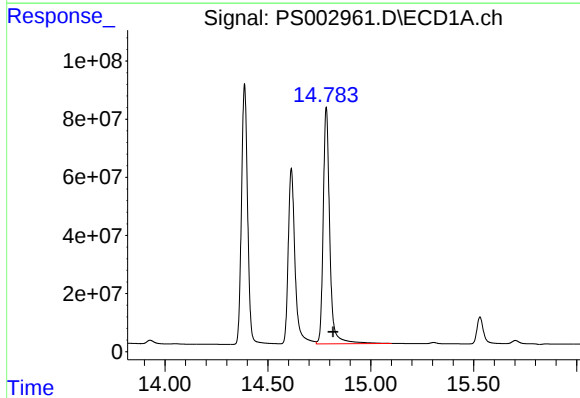


#12 2,4,5-T

R.T.: 14.784 min
Delta R.T.: -0.033 min
Response: 1798598467
Conc: 737.31 ng/ml

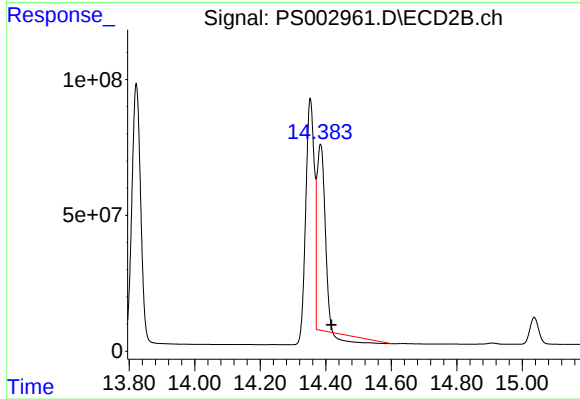

#12 2,4,5-T


R.T.: 14.384 min
Delta R.T.: -0.033 min
Response: 1030464135
Conc: 538.53 ng/ml

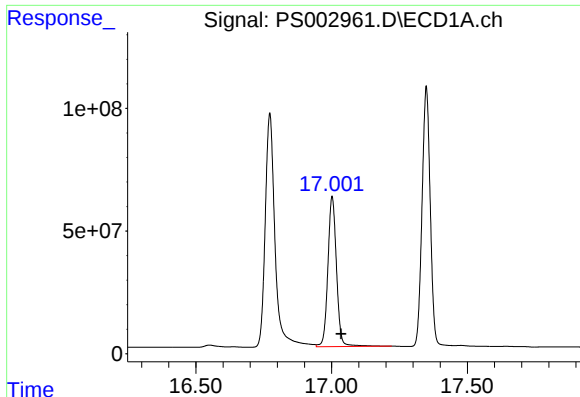

#14 DINOSEB


R.T.: 17.002 min
Delta R.T.: -0.033 min
Response: 1349978060
Conc: 717.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

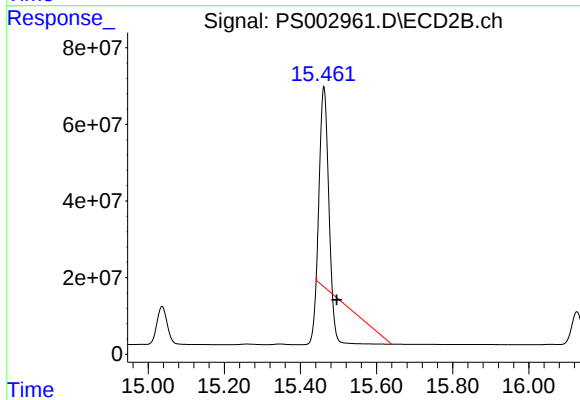


#14 DINOSEB

R.T.: 15.462 min
Delta R.T.: -0.033 min
Response: 168100618
Conc: 95.89 ng/ml

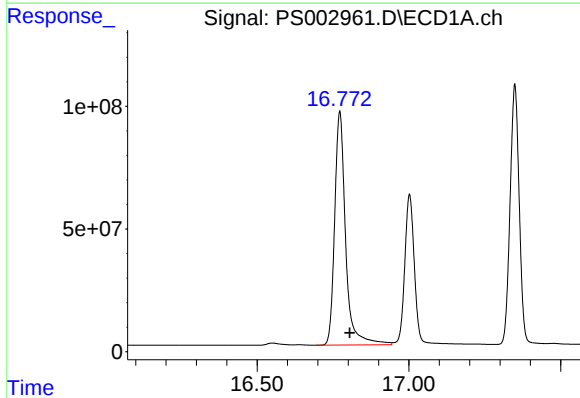


#15 Picloram

R.T.: 16.772 min
Delta R.T.: -0.034 min
Response: 2385943825
Conc: 754.18 ng/ml

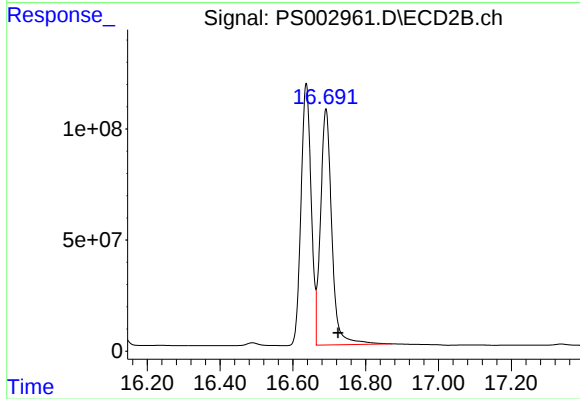

#15 Picloram


R.T.: 16.691 min
Delta R.T.: -0.034 min
Response: 2283570842
Conc: 759.57 ng/ml

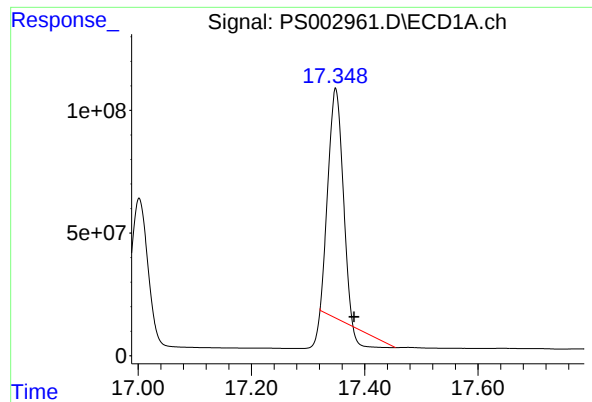

#16 DCPA

R.T.: 17.349 min
Delta R.T.: -0.033 min
Response: 1532491586
Conc: 509.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

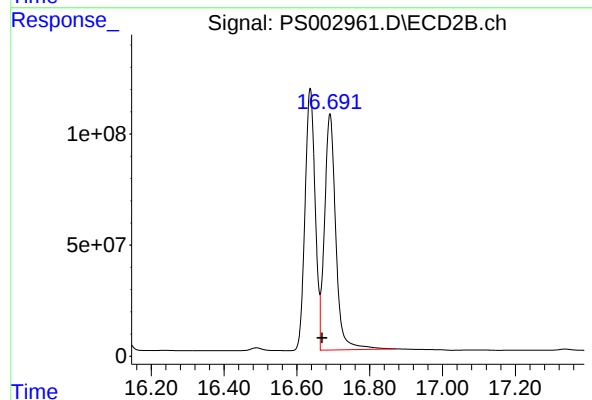

#16 DCPA

R.T.: 16.691 min
Delta R.T.: 0.021 min
Response: 2283570842
Conc: 737.21 ng/ml