

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
 Data File : PS002963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 02:48
 Operator : EI\SJ
 Sample : K1250-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DRUM-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 06:17:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.781	0	125.6E6	N.D.	293.876 #
Target Compounds							
1) T	Dalapon	0.000	2.285	0	57223967	N.D.	106.777 #
2) T	3,5-DICHL...	0.000	8.949	0	8066175	N.D.	14.313 #
3) T	4-Nitroph...	0.000	9.904	0	41447473	N.D.	198.292 #
8) T	DICHLORPROP	12.838	0.000	3089648	0	8.056	N.D. #
14) T	DINOSEB	0.000	15.486	0	5138613	N.D.	2.931 #
15) T	Picloram	0.000	16.700	0	24460999	N.D.	8.136 #
16) T	DCPA	0.000	16.700	0	24460999	N.D.	7.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012819\
Data File : PS002963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 02:48
Operator : EI\SJ
Sample : K1250-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DRUM-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 06:17:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

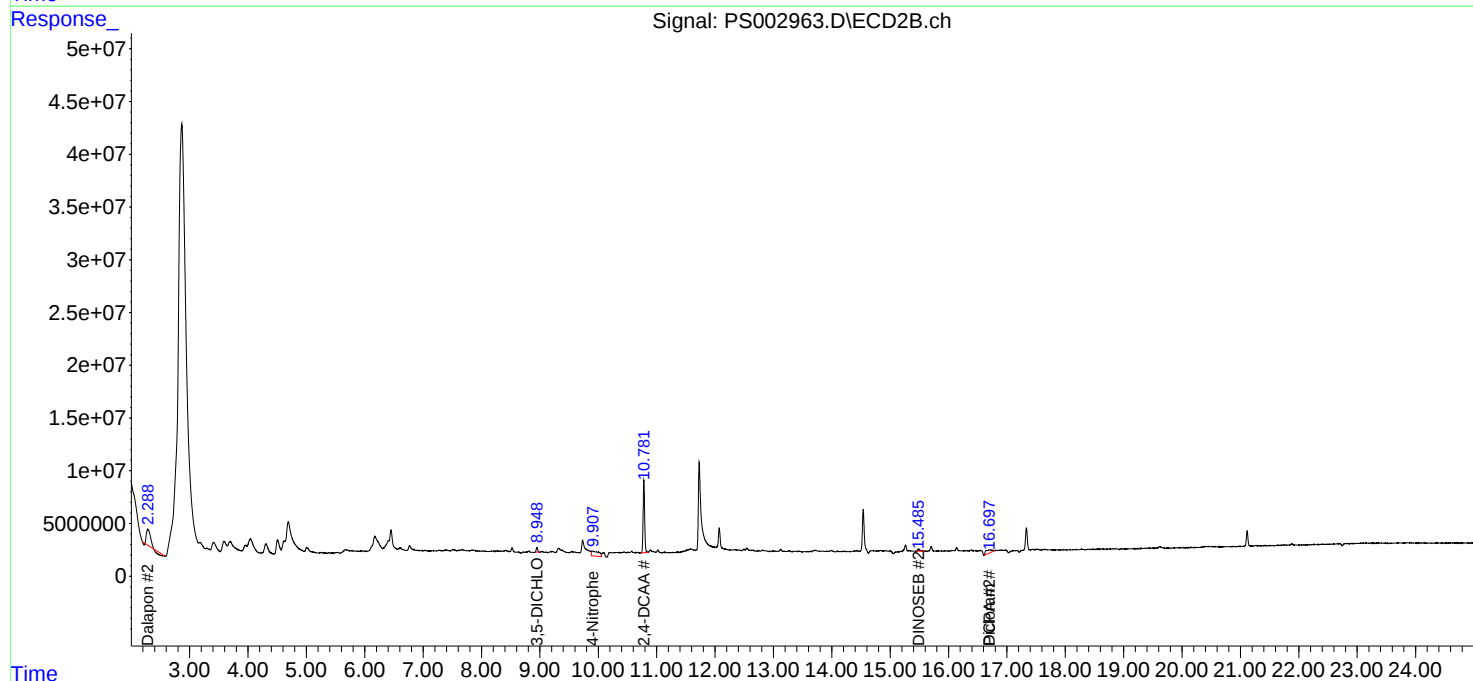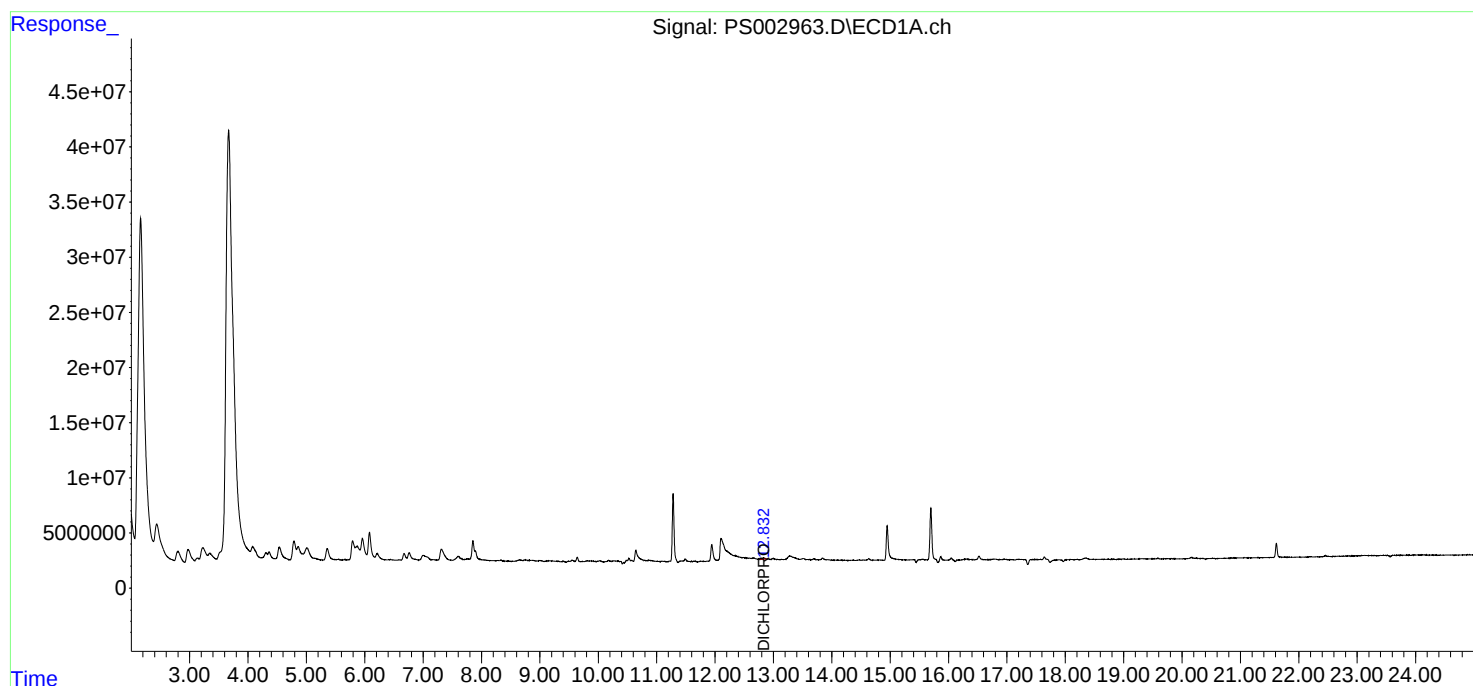


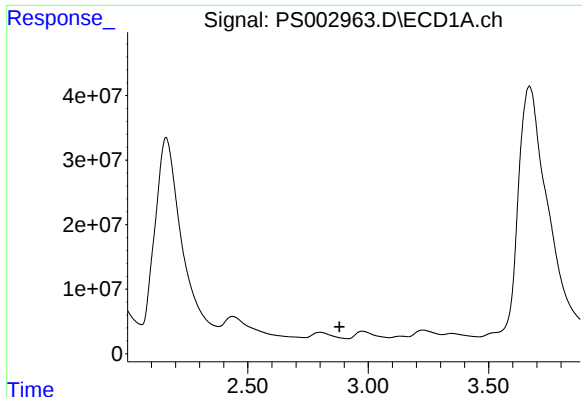

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DRUM-6

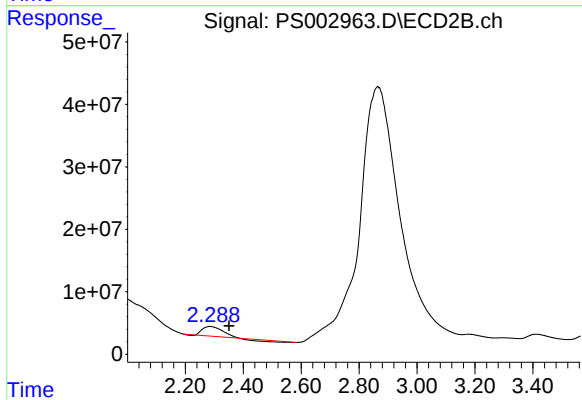


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.066 min
Response: 57223967
Conc: 106.78 ng/ml

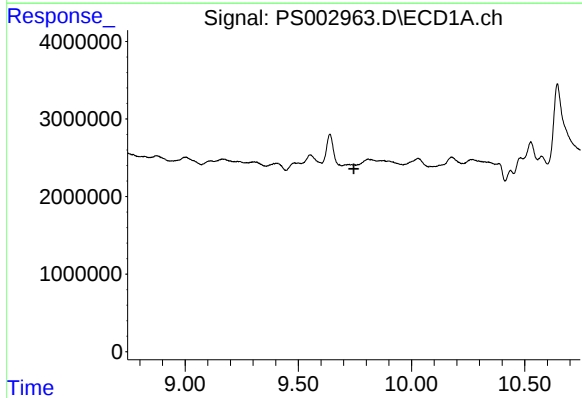


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

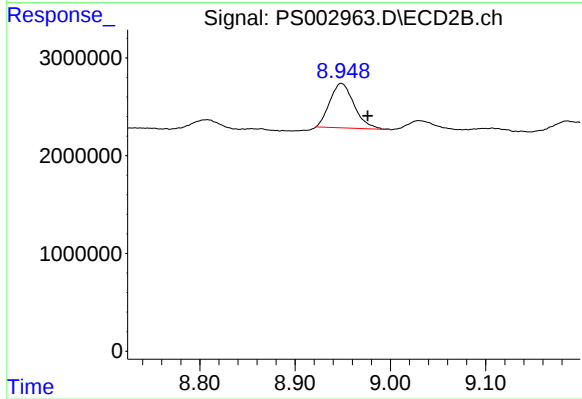

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: -0.028 min
Response: 8066175
Conc: 14.31 ng/ml

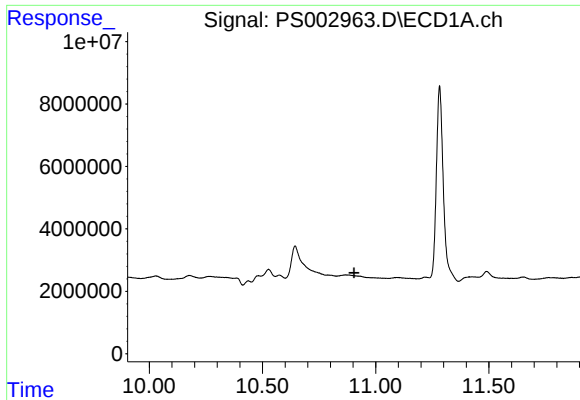

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DRUM-6

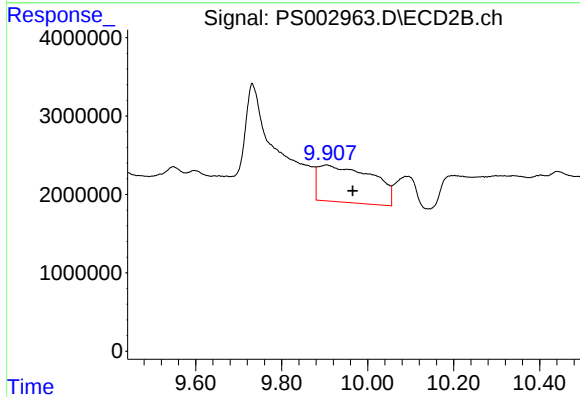


#3 4-Nitrophenol

R.T.: 9.904 min
Delta R.T.: -0.061 min
Response: 41447473
Conc: 198.29 ng/ml

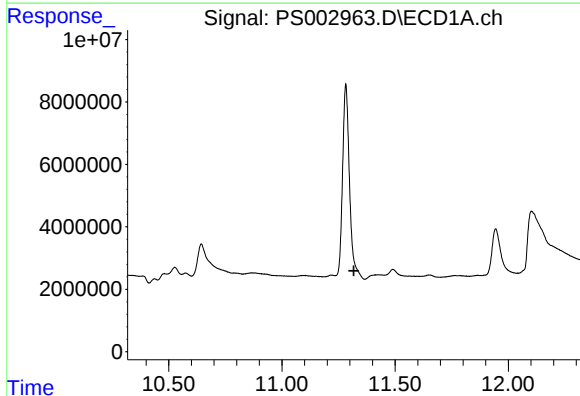


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

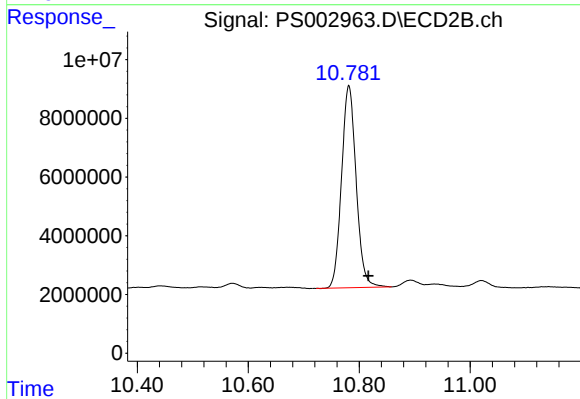

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: -0.035 min
Response: 125645385
Conc: 293.88 ng/ml

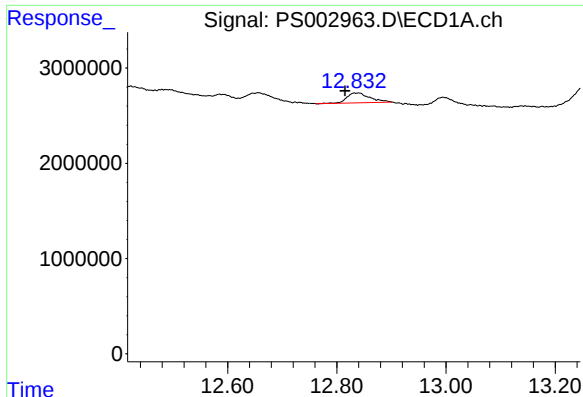

#8 DICHLORPROP


R.T.: 12.838 min
Delta R.T.: 0.023 min
Response: 3089648
Conc: 8.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
DRUM-6

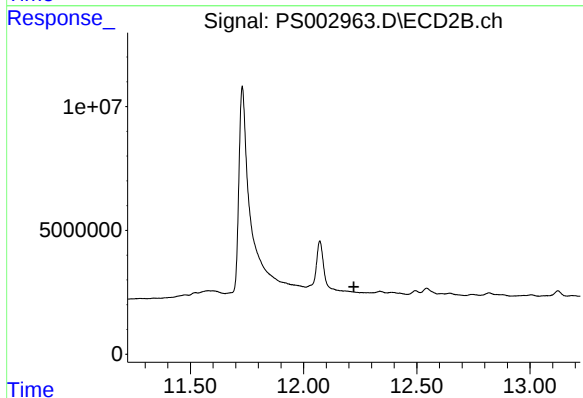


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.222 min
Response: 0
Conc: N.D.

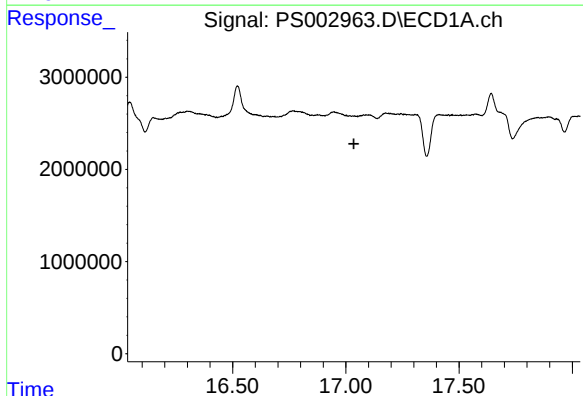


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

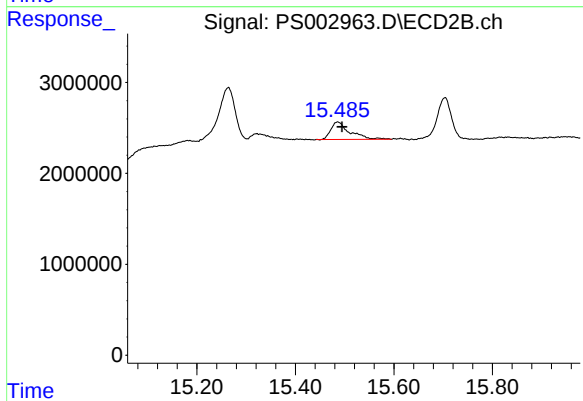

#14 DINOSEB


R.T.: 15.486 min
Delta R.T.: -0.009 min
Response: 5138613
Conc: 2.93 ng/ml

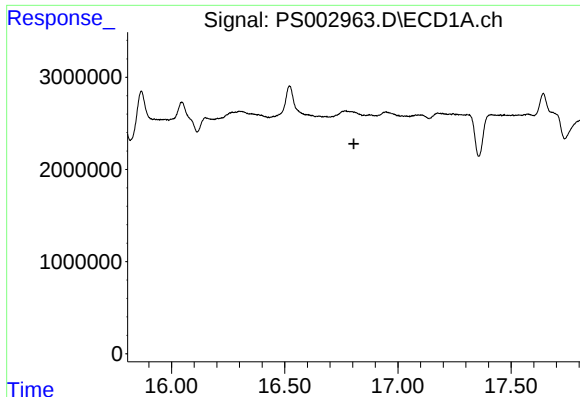

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DRUM-6

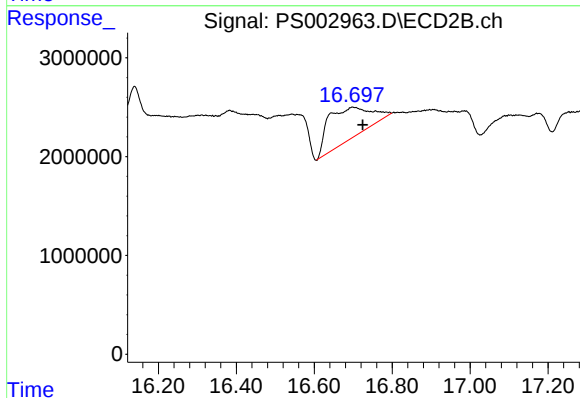


#15 Picloram

R.T.: 16.700 min
Delta R.T.: -0.024 min
Response: 24460999
Conc: 8.14 ng/ml

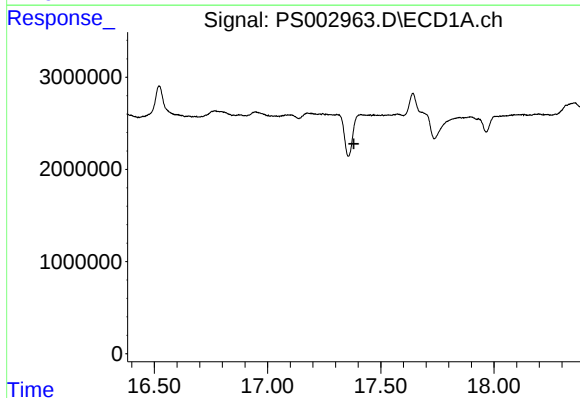

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

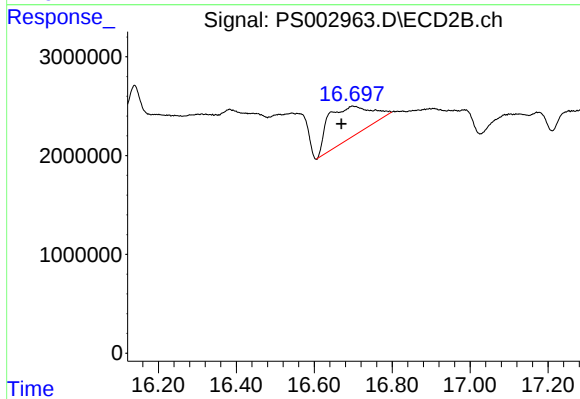

#16 DCPA

R.T.: 16.700 min
Delta R.T.: 0.031 min
Response: 24460999
Conc: 7.90 ng/ml