

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
 Data File : PS008581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2020 13:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 03:54:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.275	5.965	951.5E6	500.9E6	538.901	528.655
Target Compounds							
5) T	DICAMBA	0.000	6.210	0 29917875	N.D.	7.481	
6) T	MCP	0.000	6.210	0 29917875	N.D.	9.839	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
Data File : PS008581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2020 13:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 03:54:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

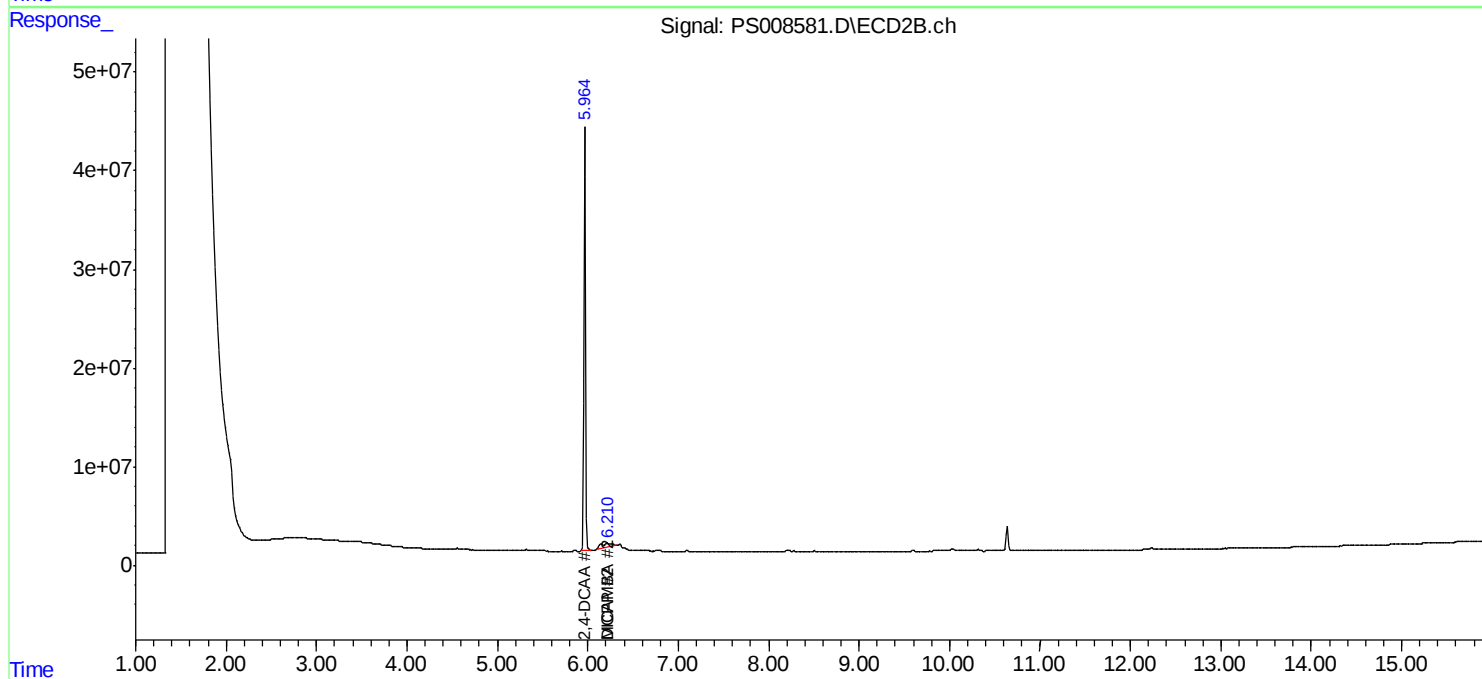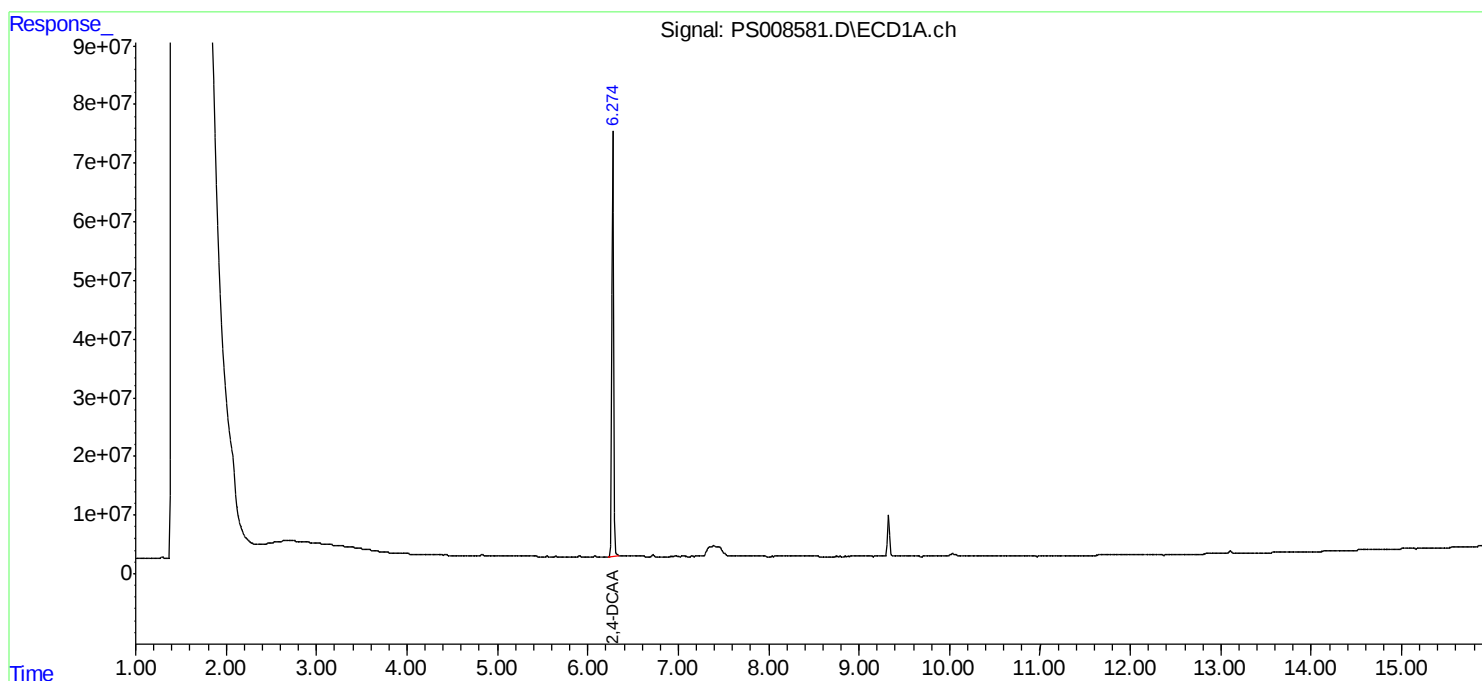


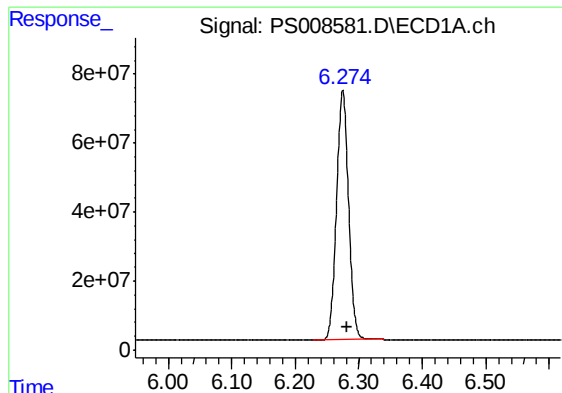

#4 2,4-DCAA


R.T.: 6.275 min
Delta R.T.: -0.008 min
Response: 951540025
Conc: 538.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

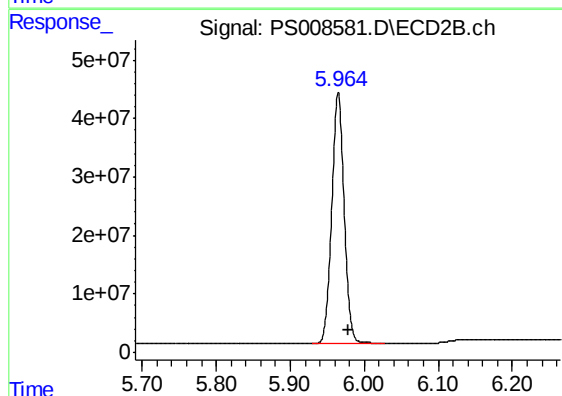


#4 2,4-DCAA

R.T.: 5.965 min
Delta R.T.: -0.014 min
Response: 500881305
Conc: 528.66 ng/ml

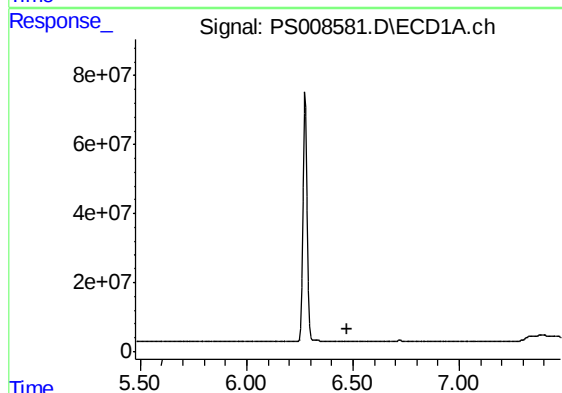


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

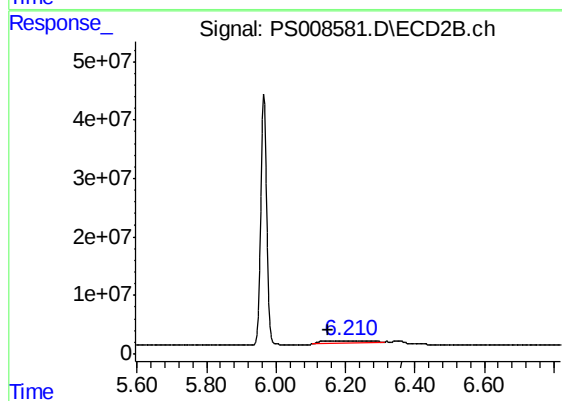

#5 DICAMBA


R.T.: 6.210 min
Delta R.T.: 0.061 min
Response: 29917875
Conc: 7.48 ng/ml

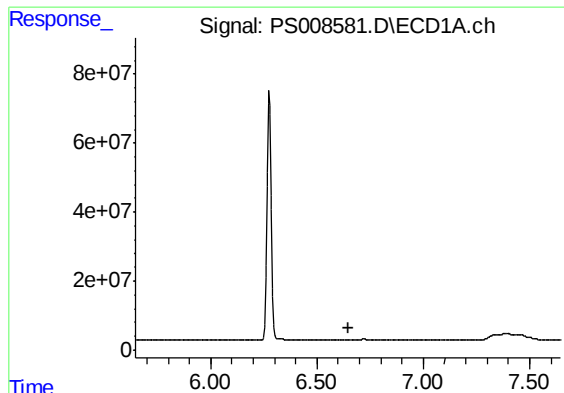

#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

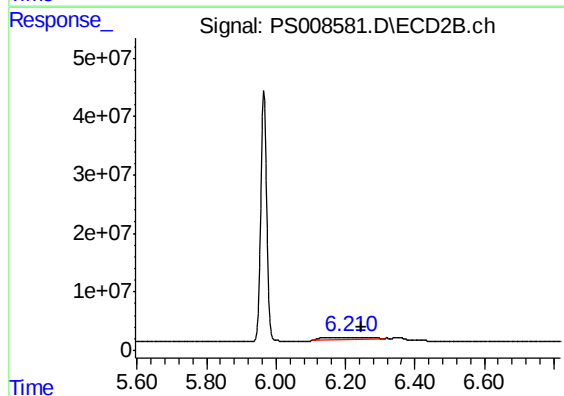

#6 MCPP

R.T.: 6.210 min
Delta R.T.: -0.036 min
Response: 29917875
Conc: 9.84 ug/ml