

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
 Data File : PS008595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2020 22:18
 Operator : DD\AJ
 Sample : L1269-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-25-24-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:27:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.270	5.959	624.2E6	312.0E6	353.535	329.311
Target Compounds							
1) T	Dalapon	2.505	2.182	41354184	22281986	16.130	17.576
2) T	3,5-DICHL...	0.000	5.146	0	130.2E6	N.D.	93.196
5) T	DICAMBA	6.535	6.093	27774438	10854341	4.041	2.714 #
6) T	MCP	6.712	0.000	204.8E6	0	40.184	N.D. #
7) T	MCPA	0.000	6.486	0	13742396	N.D.	3.218
8) T	DICHLORPROP	0.000	6.778	0	33568403	N.D.	34.745
10) T	Pentachlo...	7.755	0.000	28039616	0	1.153	N.D. #
12) T	2,4,5-T	8.475	8.285	103.6E6	23994563	11.229	4.537 #
13) T	2,4-DB	9.034	0.000	29695351	0	21.421	N.D. #
14) T	DINOSEB	0.000	9.114	0	40779153	N.D.	10.795
15) T	Picloram	10.056	10.044	57066080	37572323	4.572	5.057
16) T	DCPA	0.000	10.044	0	37572323	N.D.	5.766



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
Data File : PS008595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2020 22:18
Operator : DD\AJ
Sample : L1269-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-25-24-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:27:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

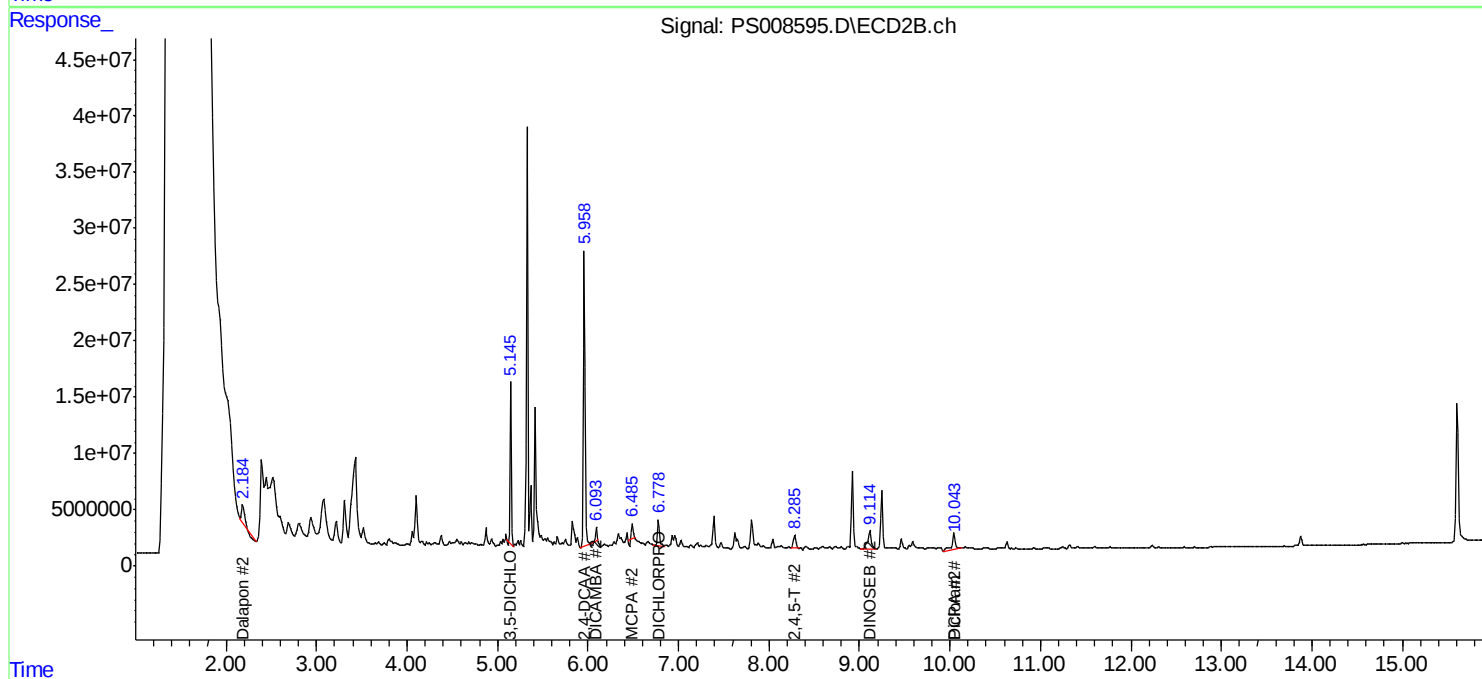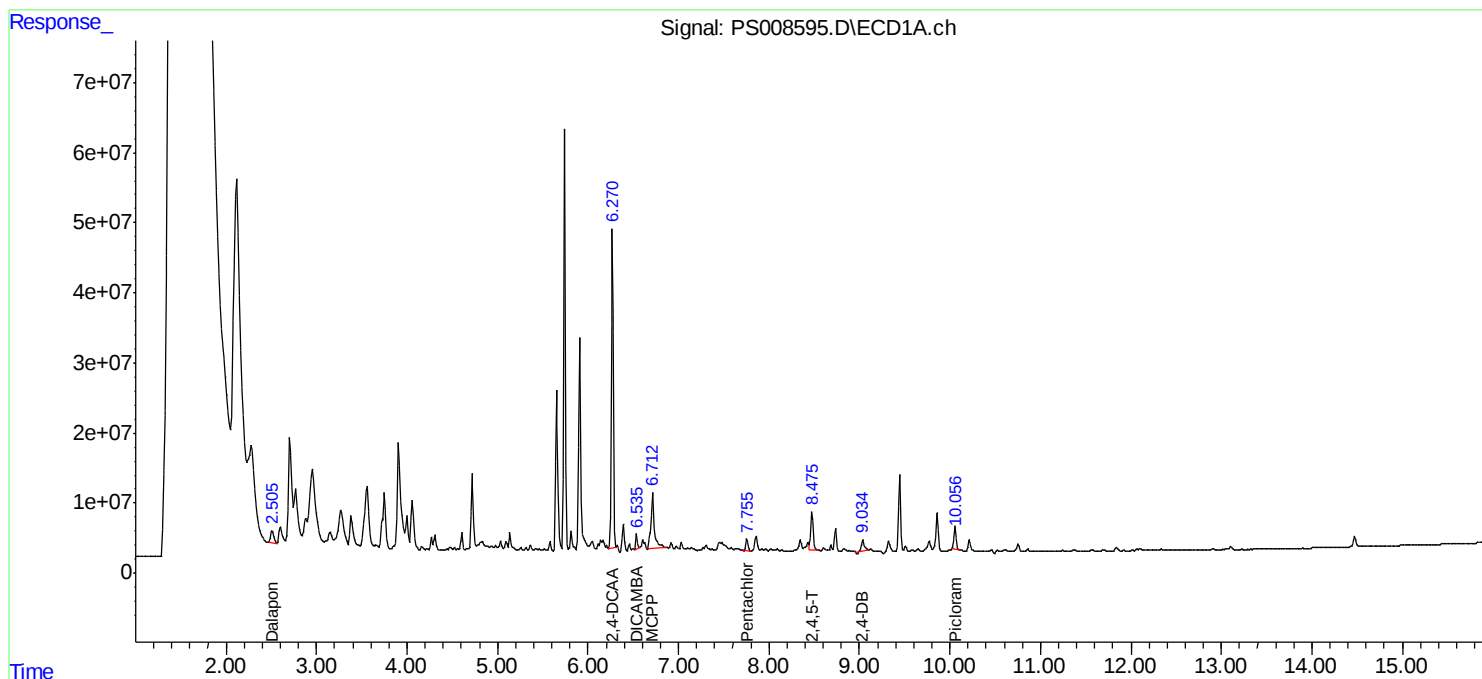


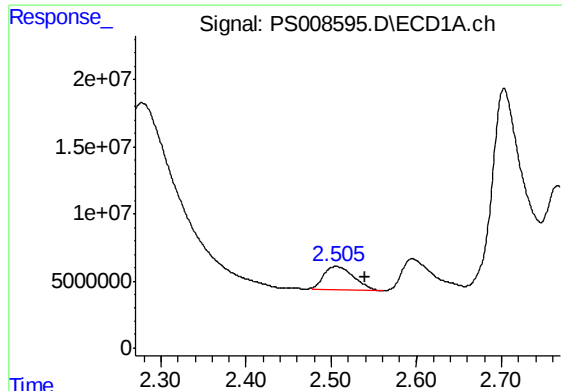

#1 Dalapon


R.T.: 2.505 min
Delta R.T.: -0.035 min
Response: 41354184
Conc: 16.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

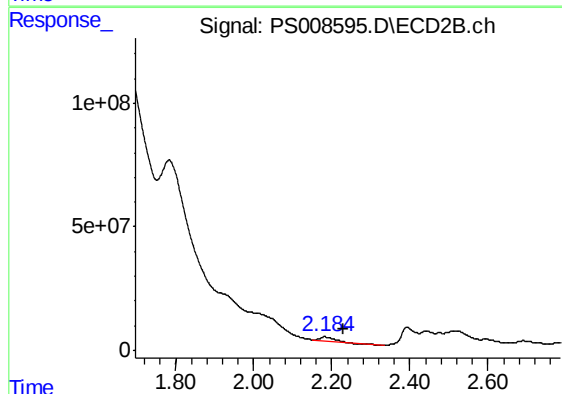


#1 Dalapon

R.T.: 2.182 min
Delta R.T.: -0.049 min
Response: 22281986
Conc: 17.58 ng/ml

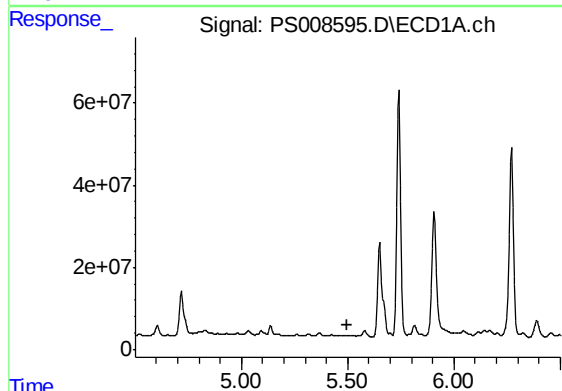


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

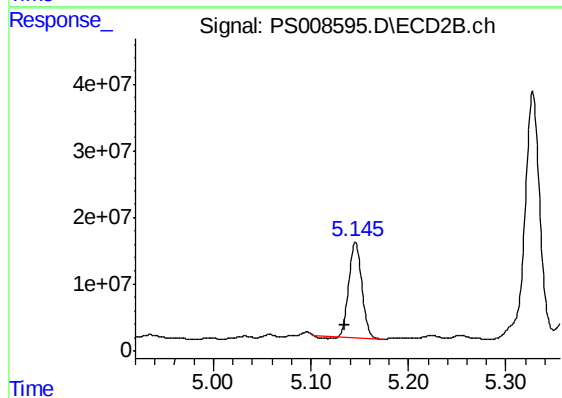

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 130211473
Conc: 93.20 ng/ml

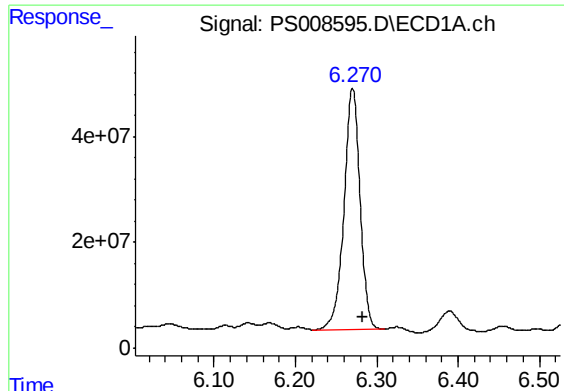

#4 2,4-DCAA


R.T.: 6.270 min
Delta R.T.: -0.012 min
Response: 624237637
Conc: 353.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

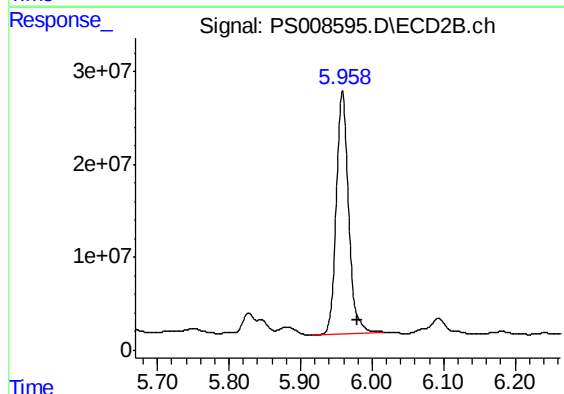


#4 2,4-DCAA

R.T.: 5.959 min
Delta R.T.: -0.021 min
Response: 312009581
Conc: 329.31 ng/ml

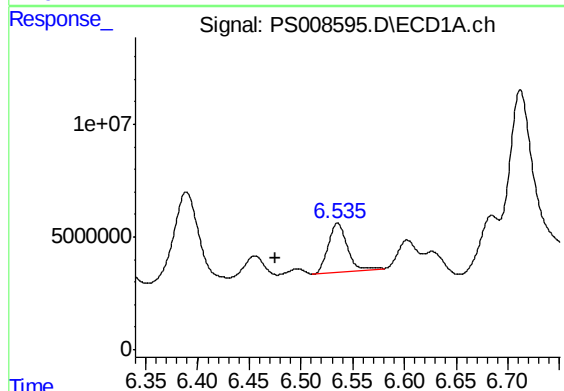


#5 DICAMBA

R.T.: 6.535 min
Delta R.T.: 0.060 min
Response: 27774438
Conc: 4.04 ng/ml

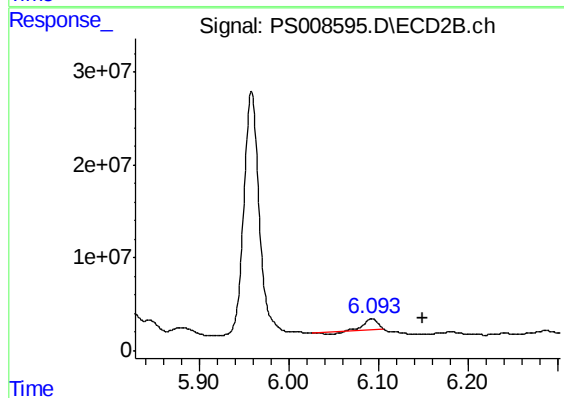

#5 DICAMBA


R.T.: 6.093 min
Delta R.T.: -0.057 min
Response: 10854341
Conc: 2.71 ng/ml

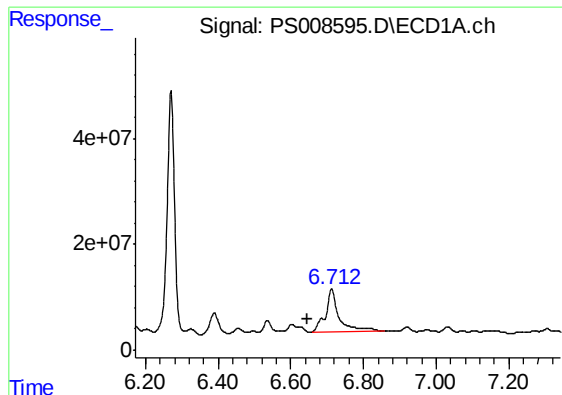

#6 MCPP


R.T.: 6.712 min
Delta R.T.: 0.067 min
Response: 204812261
Conc: 40.18 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

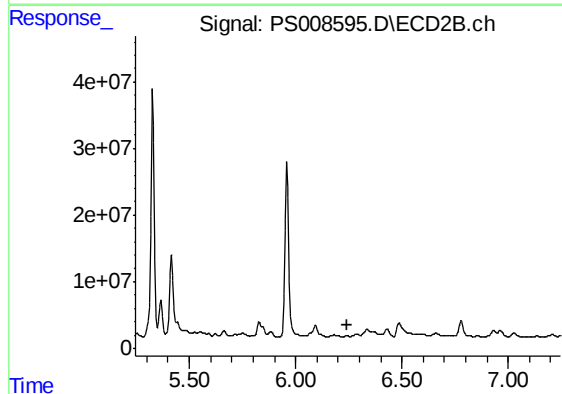


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

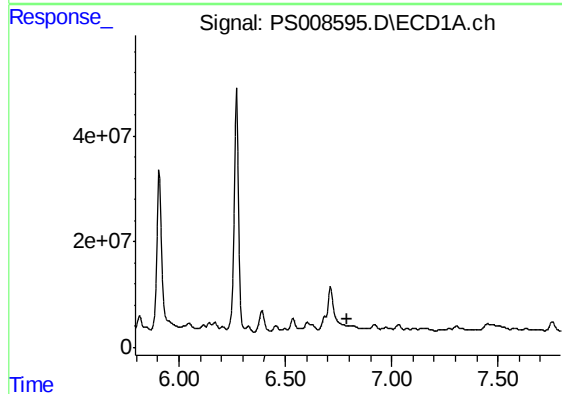


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

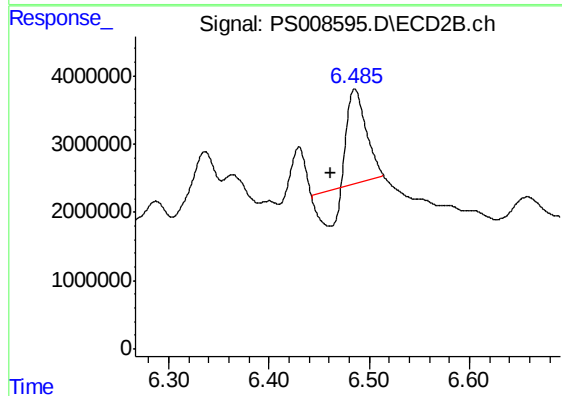

#7 MCPA


R.T.: 6.486 min
Delta R.T.: 0.024 min
Response: 13742396
Conc: 3.22 ug/ml

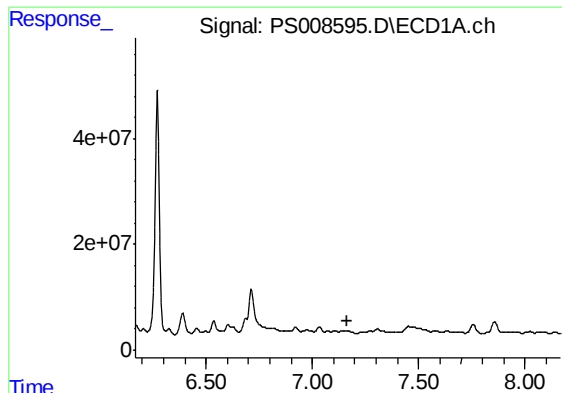

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

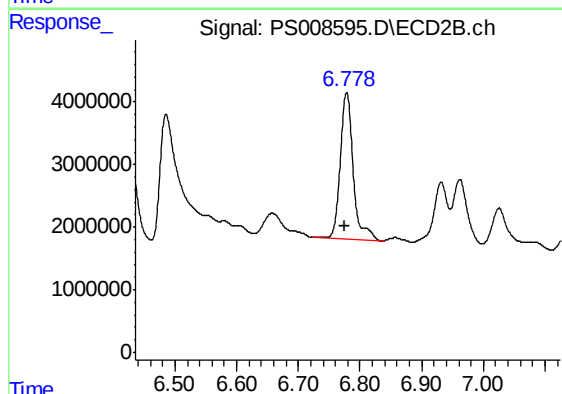


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.004 min
Response: 33568403
Conc: 34.74 ng/ml

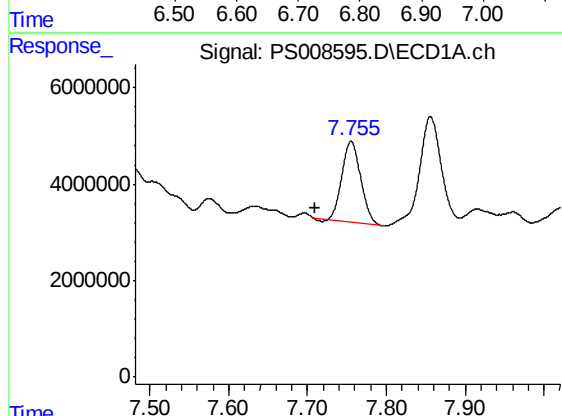


#10 Pentachlorophenol

R.T.: 7.755 min
Delta R.T.: 0.045 min
Response: 28039616
Conc: 1.15 ng/ml

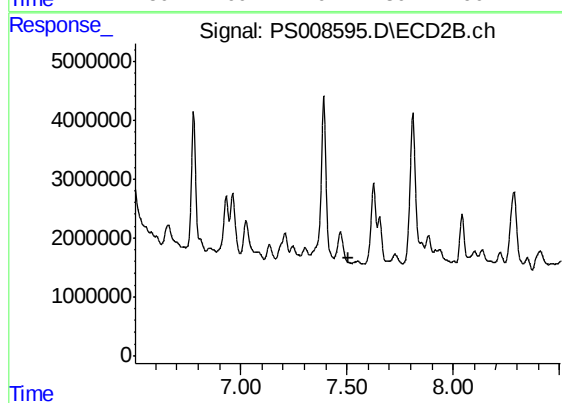

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

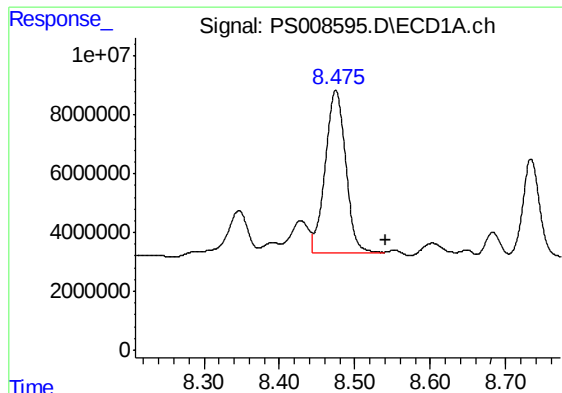

#12 2,4,5-T


R.T.: 8.475 min
Delta R.T.: -0.067 min
Response: 103607841
Conc: 11.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

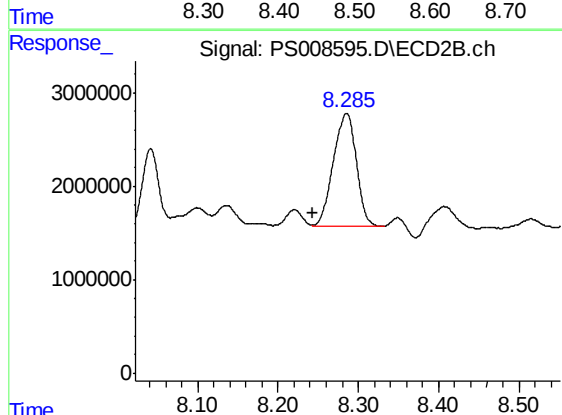


#12 2,4,5-T

R.T.: 8.285 min
Delta R.T.: 0.042 min
Response: 23994563
Conc: 4.54 ng/ml

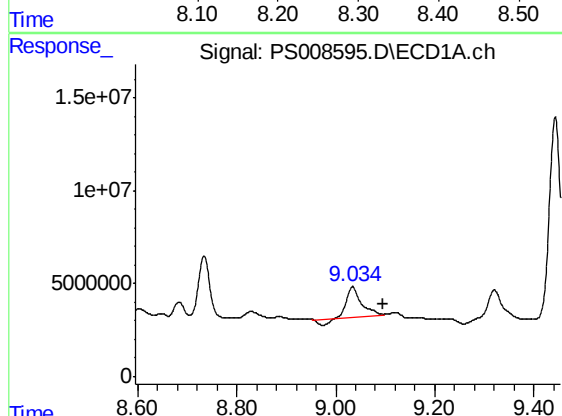


#13 2,4-DB

R.T.: 9.034 min
Delta R.T.: -0.061 min
Response: 29695351
Conc: 21.42 ng/ml

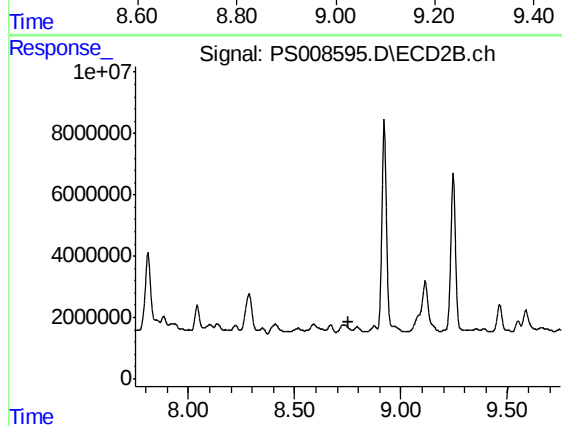

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

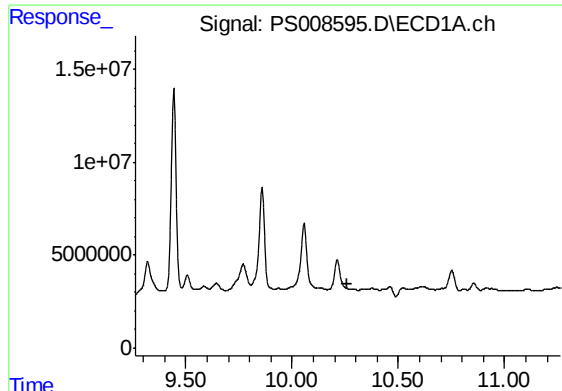

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 10.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

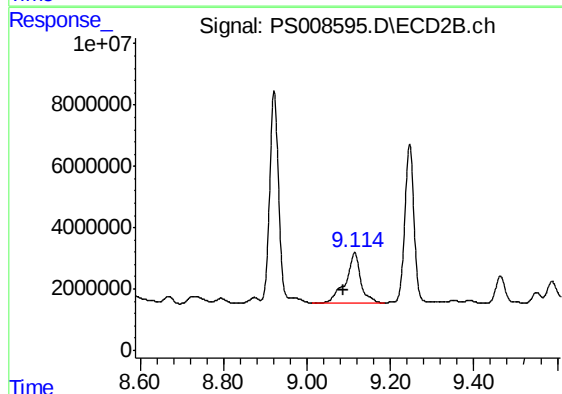


#14 DINOSEB

R.T.: 9.114 min
Delta R.T.: 0.027 min
Response: 40779153
Conc: 10.79 ng/ml

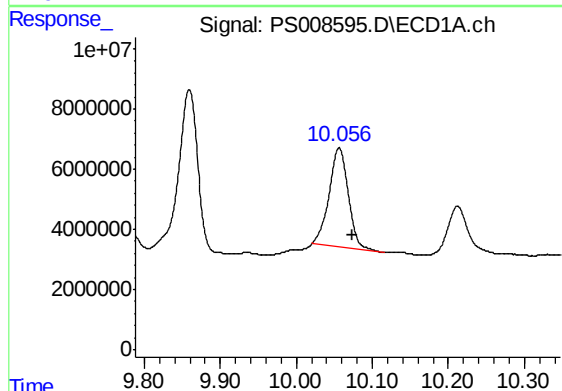


#15 Picloram

R.T.: 10.056 min
Delta R.T.: -0.017 min
Response: 57066080
Conc: 4.57 ng/ml

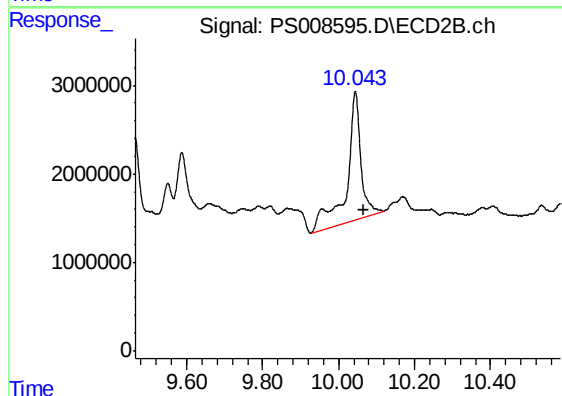

#15 Picloram


R.T.: 10.044 min
Delta R.T.: -0.024 min
Response: 37572323
Conc: 5.06 ng/ml

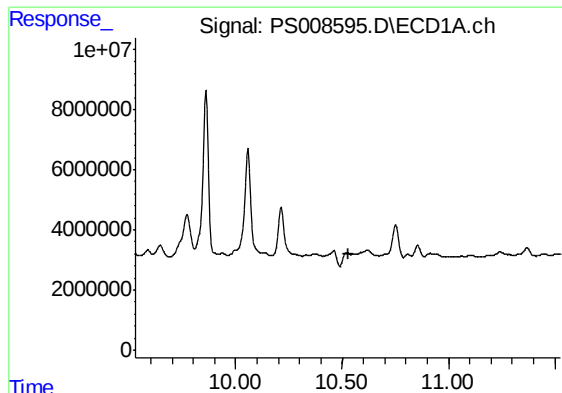

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-25-24-COMP

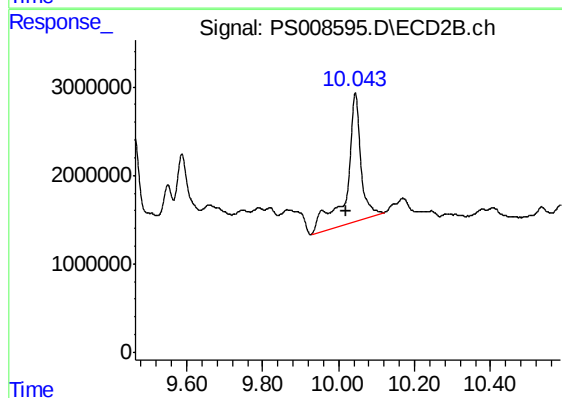

#16 DCPA

R.T.: 10.044 min
Delta R.T.: 0.025 min
Response: 37572323
Conc: 5.77 ng/ml