

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
 Data File : PS008602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 00:51
 Operator : DD\AJ
 Sample : L1274-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BORING-B2-SAMPLE-S1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:21:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.267	5.961	99242105	36970946	56.205	39.021 #
Target Compounds							
1) T	Dalapon	2.501	0.000	236.9E6	0	92.393	N.D. #
2) T	3,5-DICHL...	0.000	5.149	0	60555948	N.D.	43.342
6) T	MCP	6.706	0.000	38433928	0	7.541	N.D. #
7) T	MCPA	6.816	0.000	91174859	0	12.477	N.D. #
8) T	DICHLORPROP	0.000	6.781	0	28158034	N.D.	29.145
9) T	2,4-D	7.390	7.028	273.8E6	16246364	150.488	13.859 #
10) T	Pentachlo...	7.754	7.516	86549811	22684293	3.560	1.680 #
12) T	2,4,5-T	8.555	0.000	8844437	0	<MDL	N.D. #
13) T	2,4-DB	9.122	8.753	64548825	14304772	46.564	20.207 #
14) T	DINOSEB	0.000	9.091	0	23076733	N.D.	6.109
15) T	Picloram	0.000	10.077	0	41572676	N.D.	5.596
16) T	DCPA	10.532	10.077	27649199	41572676	2.330	6.379 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012820\
Data File : PS008602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 00:51
Operator : DD\AJ
Sample : L1274-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:21:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

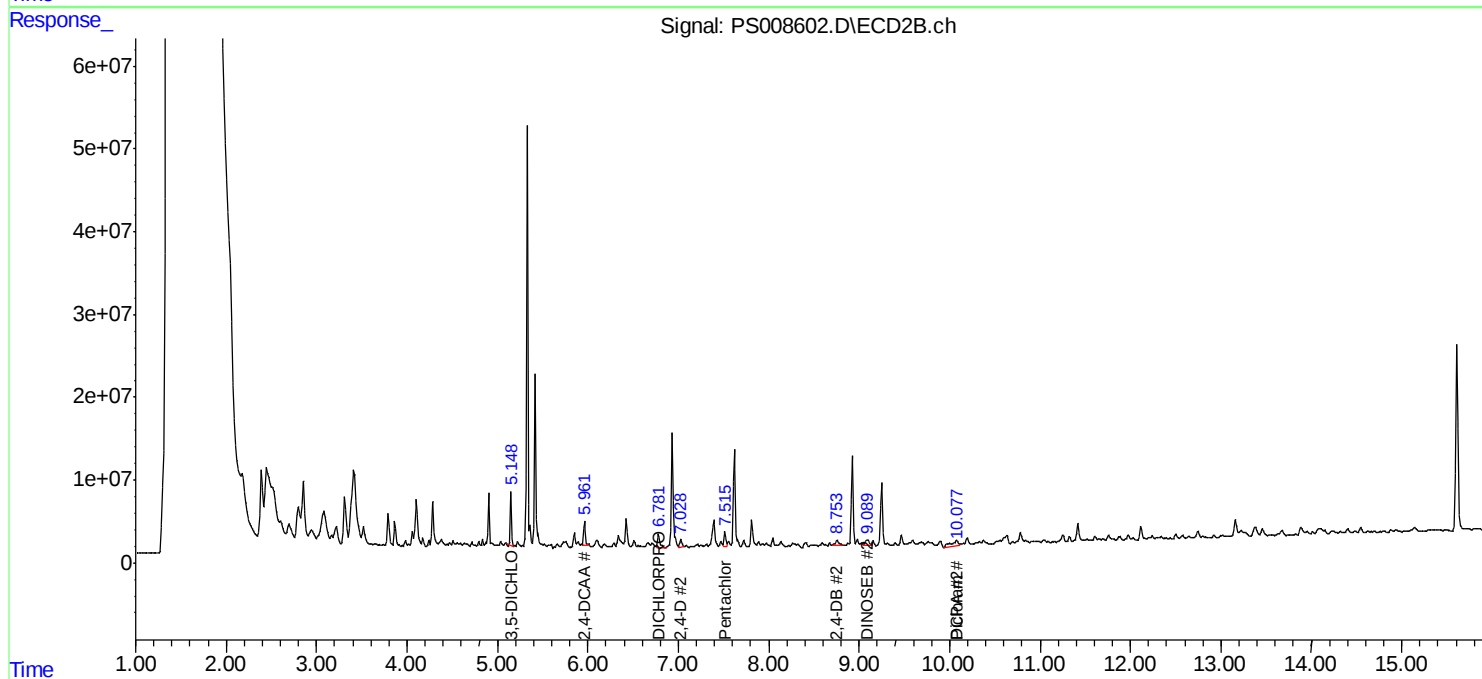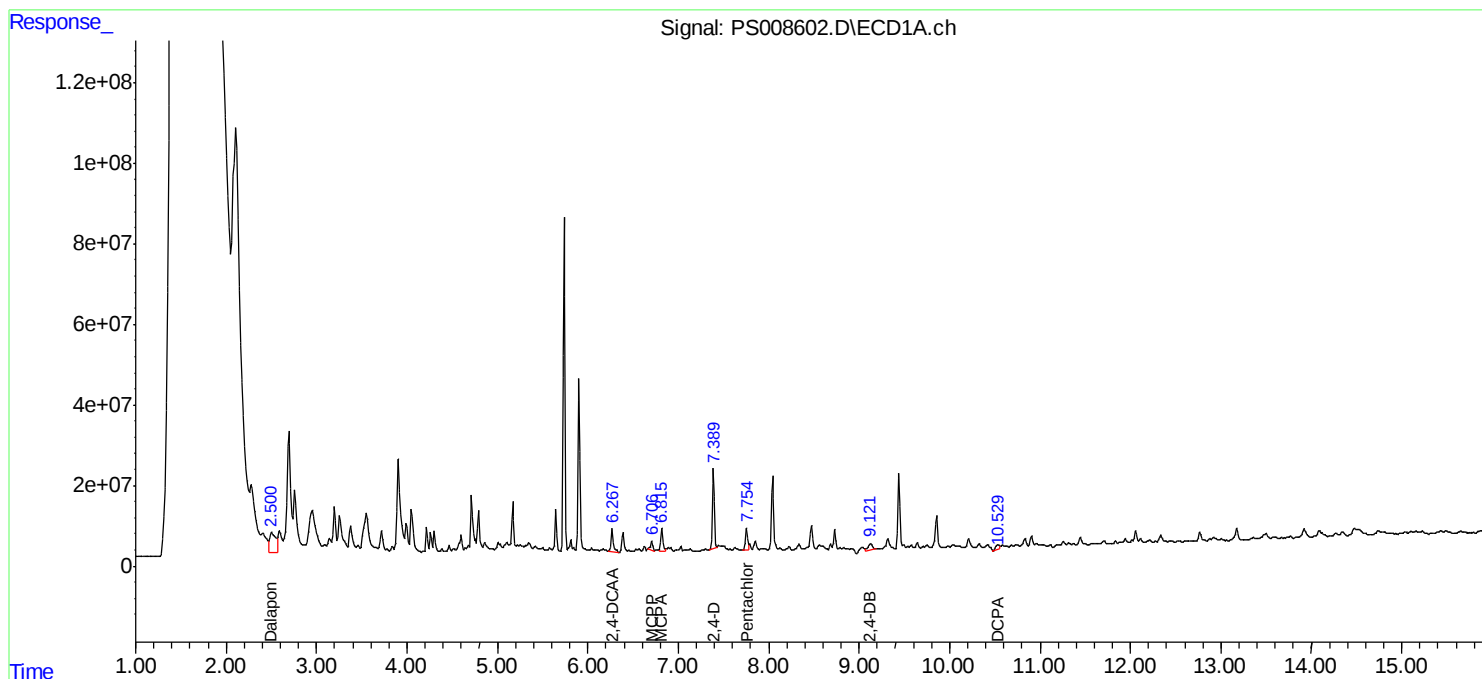


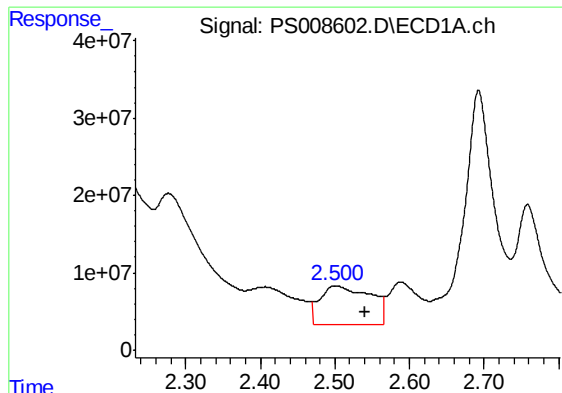

#1 Dalapon


R.T.: 2.501 min
Delta R.T.: -0.039 min
Response: 236882079
Conc: 92.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

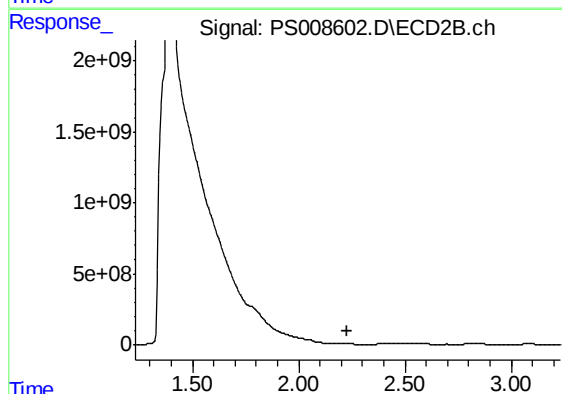


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.231 min
Response: 0
Conc: N.D.

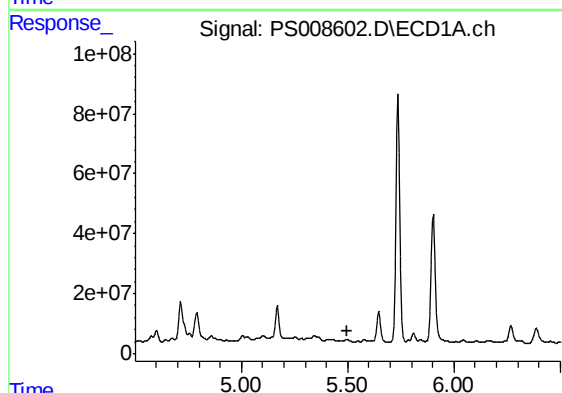


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

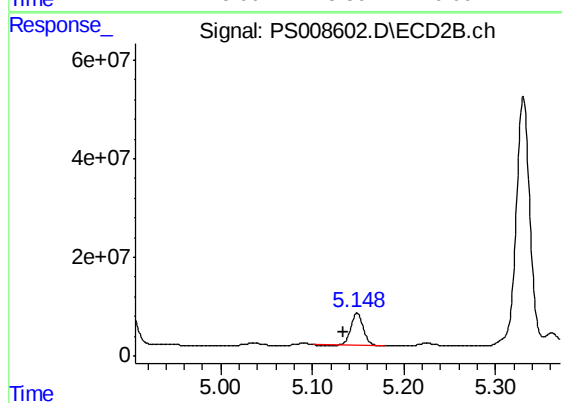

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.149 min
Delta R.T.: 0.014 min
Response: 60555948
Conc: 43.34 ng/ml

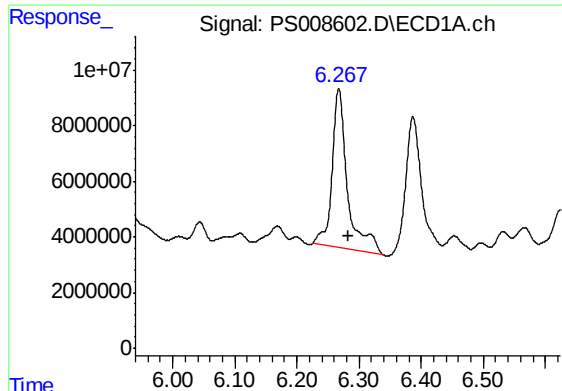

#4 2,4-DCAA


R.T.: 6.267 min
Delta R.T.: -0.015 min
Response: 99242105
Conc: 56.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

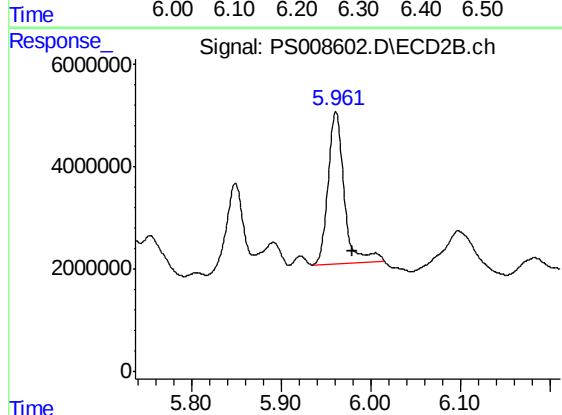


#4 2,4-DCAA

R.T.: 5.961 min
Delta R.T.: -0.018 min
Response: 36970946
Conc: 39.02 ng/ml

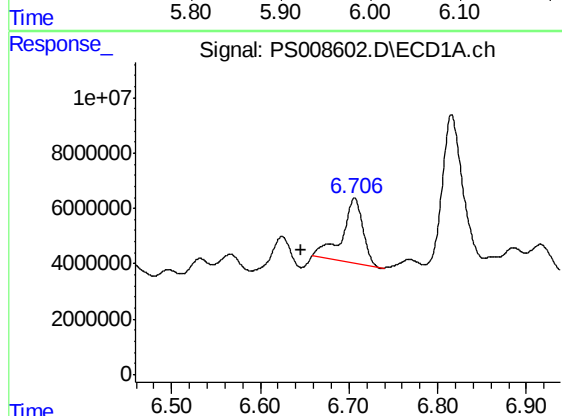


#6 MCP

R.T.: 6.706 min
Delta R.T.: 0.061 min
Response: 38433928
Conc: 7.54 ug/ml

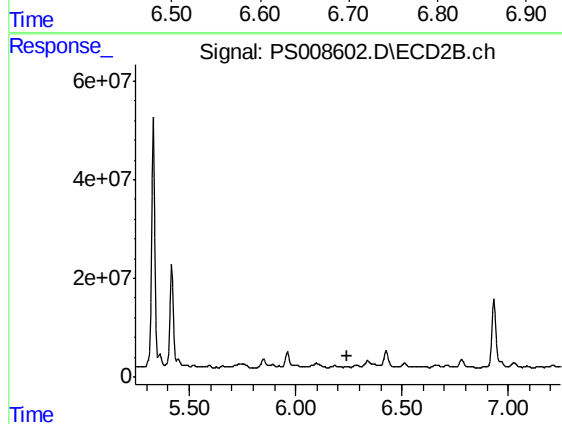

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

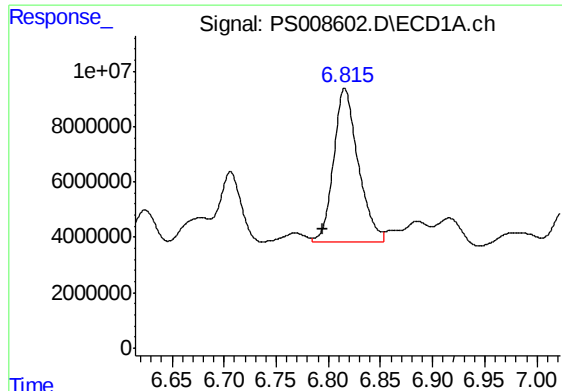

#7 MCPA


R.T.: 6.816 min
Delta R.T.: 0.021 min
Response: 91174859
Conc: 12.48 ug/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

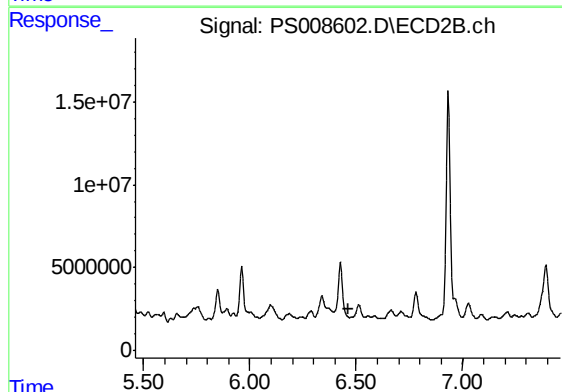


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

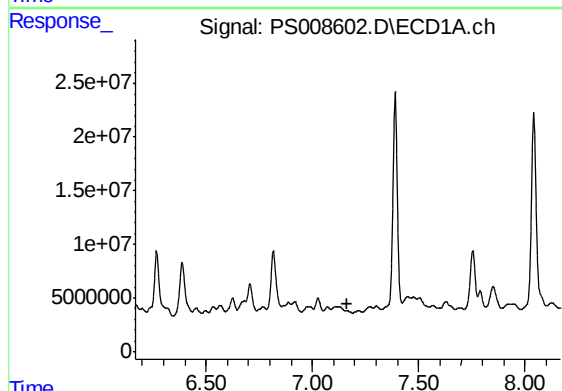


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

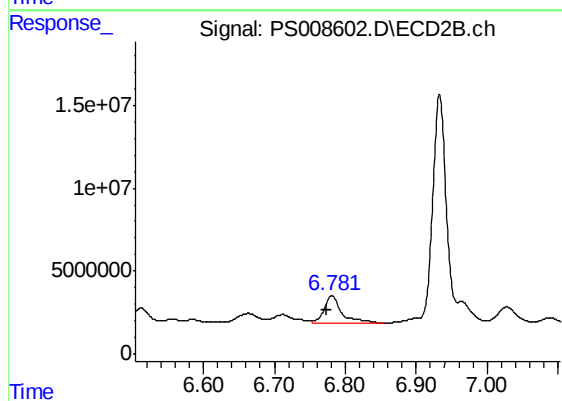

#8 DICHLORPROP


R.T.: 6.781 min
Delta R.T.: 0.006 min
Response: 28158034
Conc: 29.14 ng/ml

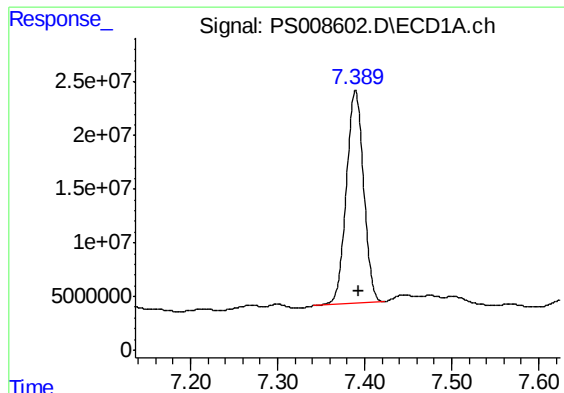

#9 2,4-D


R.T.: 7.390 min
Delta R.T.: -0.004 min
Response: 273752848
Conc: 150.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

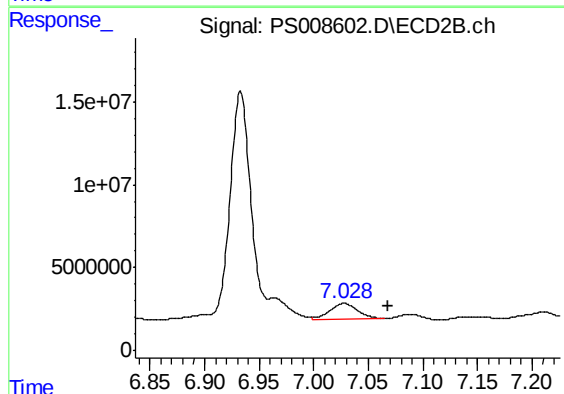


#9 2,4-D

R.T.: 7.028 min
Delta R.T.: -0.041 min
Response: 16246364
Conc: 13.86 ng/ml

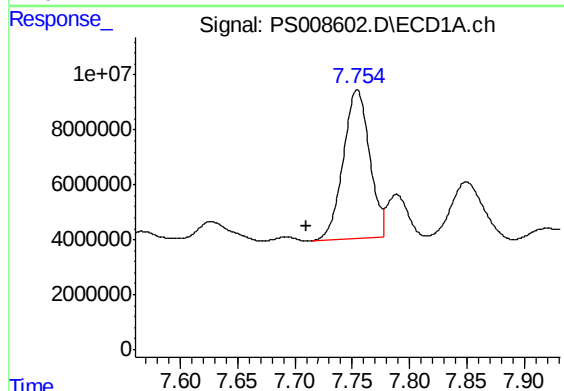


#10 Pentachlorophenol

R.T.: 7.754 min
Delta R.T.: 0.044 min
Response: 86549811
Conc: 3.56 ng/ml

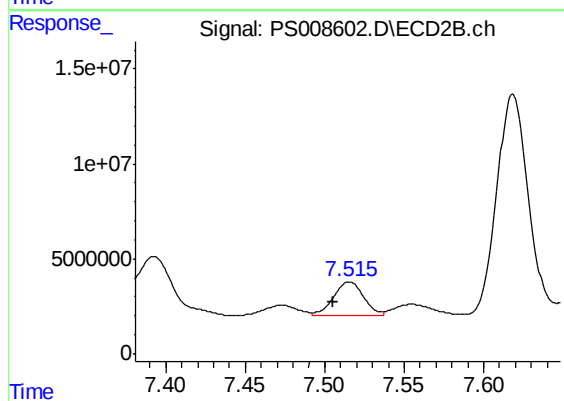

#10 Pentachlorophenol


R.T.: 7.516 min
Delta R.T.: 0.011 min
Response: 22684293
Conc: 1.68 ng/ml

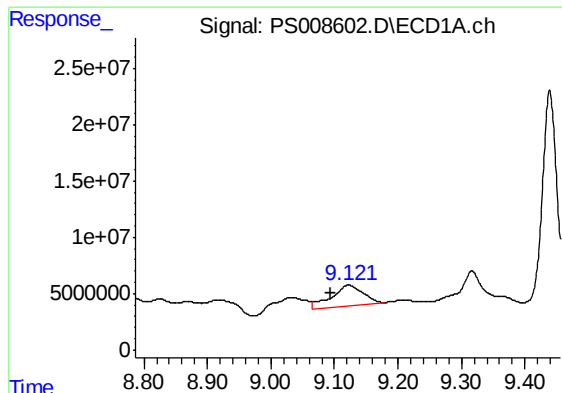

#13 2,4-DB


R.T.: 9.122 min
Delta R.T.: 0.028 min
Response: 64548825
Conc: 46.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

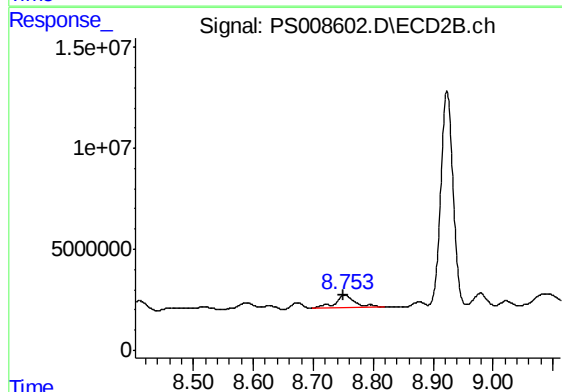


#13 2,4-DB

R.T.: 8.753 min
Delta R.T.: 0.002 min
Response: 14304772
Conc: 20.21 ng/ml

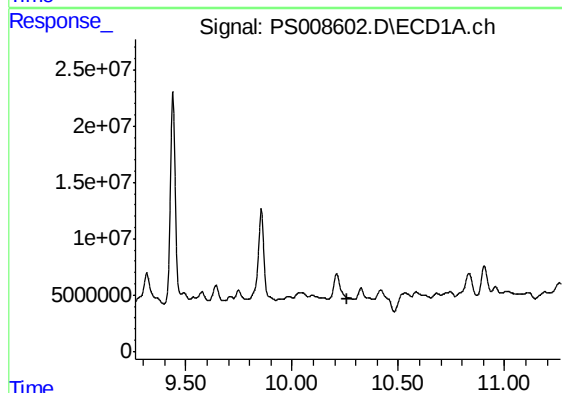


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

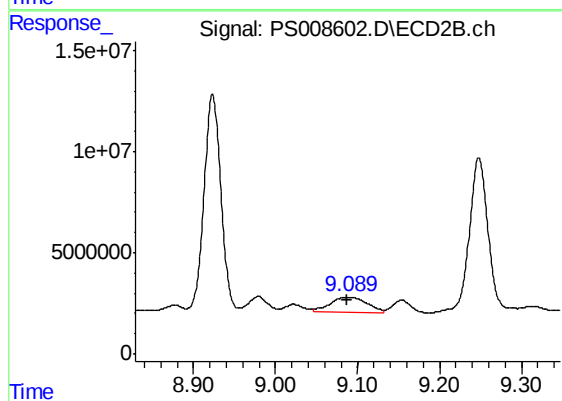

#14 DINOSEB


R.T.: 9.091 min
Delta R.T.: 0.003 min
Response: 23076733
Conc: 6.11 ng/ml

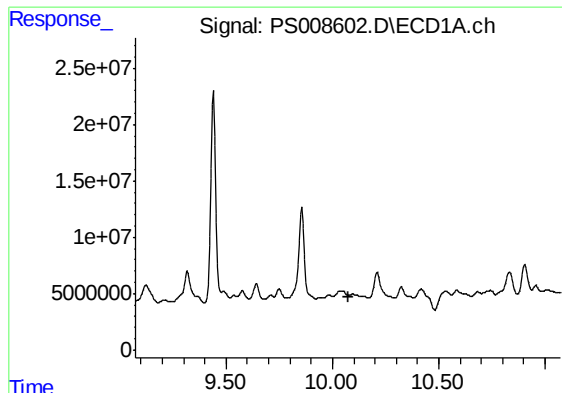

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

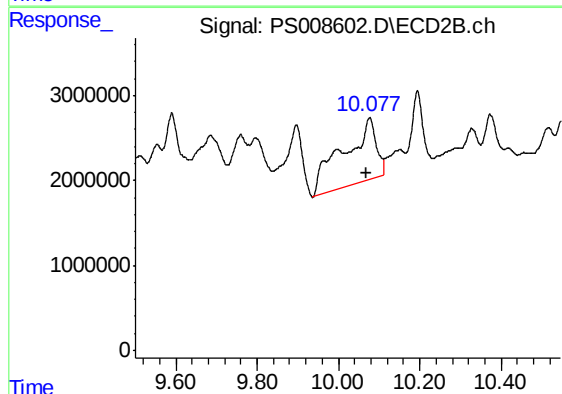


#15 Picloram

R.T.: 10.077 min
Delta R.T.: 0.009 min
Response: 41572676
Conc: 5.60 ng/ml

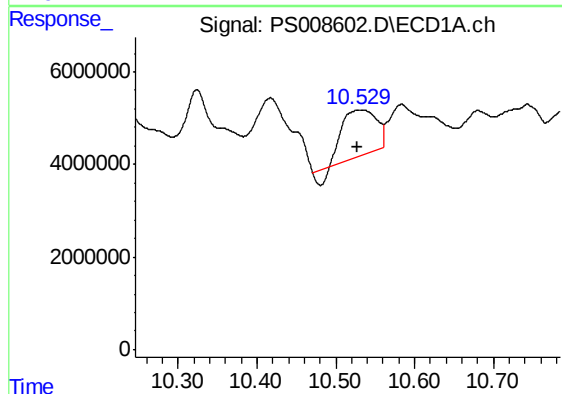

#16 DCPA

R.T.: 10.532 min
Delta R.T.: 0.005 min
Response: 27649199
Conc: 2.33 ng/ml

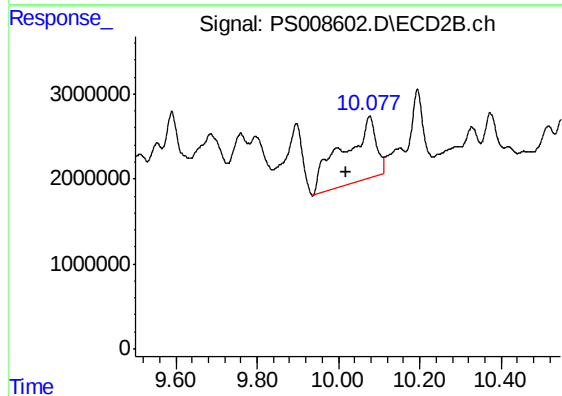

#16 DCPA

R.T.: 10.077 min
Delta R.T.: 0.058 min
Response: 41572676
Conc: 6.38 ng/ml