

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012821\
 Data File : PS013896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 00:23
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:01:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	6.906	815.2E6	293.3E6	757.686	760.299
Target Compounds							
1) T	Dalapon	3.027	2.621	812.4E6	336.0E6	650.898	653.560
2) T	3,5-DICHL...	6.421	6.062	1039.8E6	430.3E6	699.714	708.686
3) T	4-Nitroph...	7.038	6.521	363.7E6	170.1E6	669.406	676.606
5) T	DICAMBA	7.392	7.073	3112.5E6	1199.3E6	723.883	727.733
6) T	MCPD	7.560	7.167	233.8E6	98001738	74.104	72.967
7) T	MCPA	7.709	7.382	329.8E6	138.6E6	72.867	71.511
8) T	DICHLORPROP	8.084	7.697	774.1E6	306.2E6	712.189	719.695
9) T	2,4-D	8.315	7.996	888.7E6	378.2E6	723.791	709.541
10) T	Pentachlo...	8.621	8.419	11406.1E6	4034.9E6	720.248	724.308
11) T	2,4,5-TP ...	9.171	8.780	4528.7E6	1672.8E6	721.259	728.706
12) T	2,4,5-T	9.458	9.161	4595.5E6	1620.3E6	713.463	727.646
13) T	2,4-DB	10.011	9.668	768.9E6	217.5E6	696.591	727.215
14) T	DINOSEB	11.162	9.995	3437.2E6	1129.6E6	678.209	691.434
15) T	Picloram	10.997	10.990	5671.3E6	2223.4E6	667.903	651.521
16) T	DCPA	11.428	10.922	5809.3E6	2181.6E6	718.629	728.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012821\
Data File : PS013896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 00:23
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:01:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

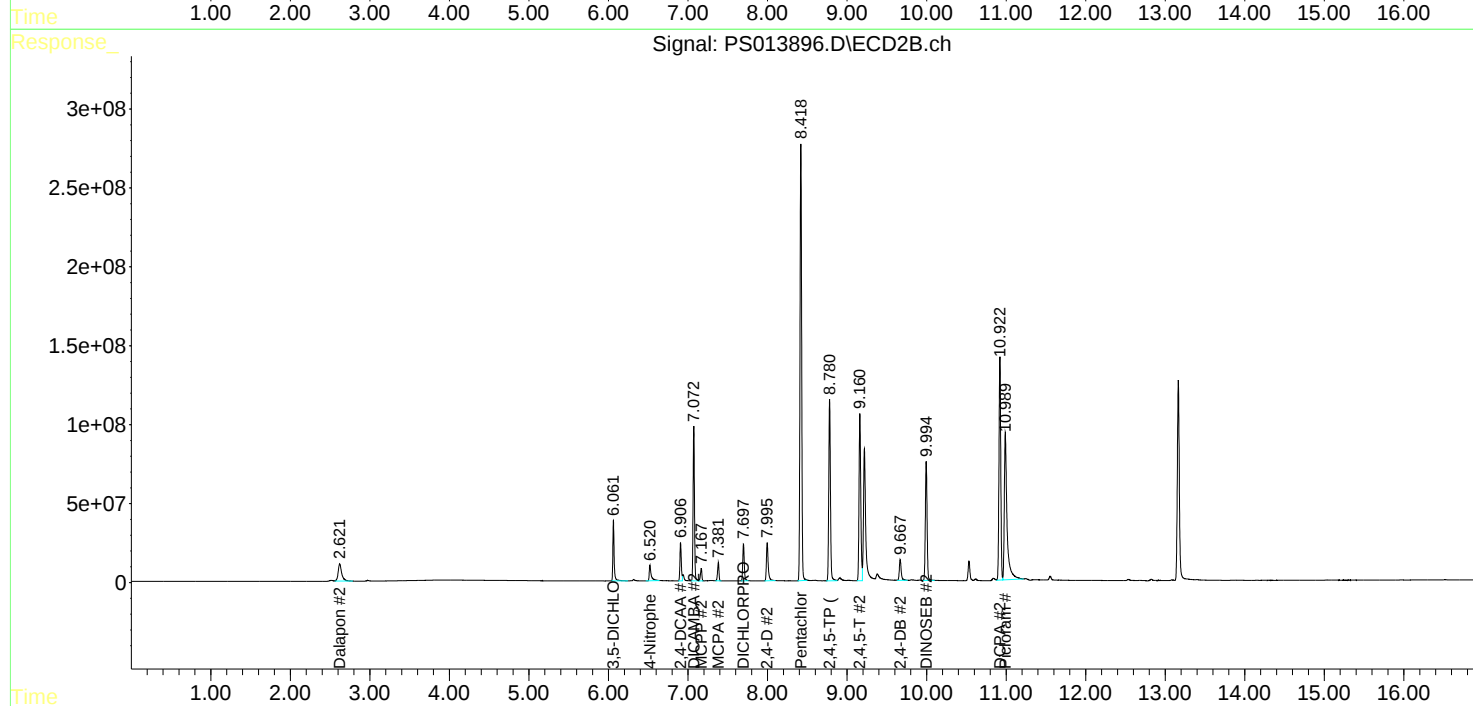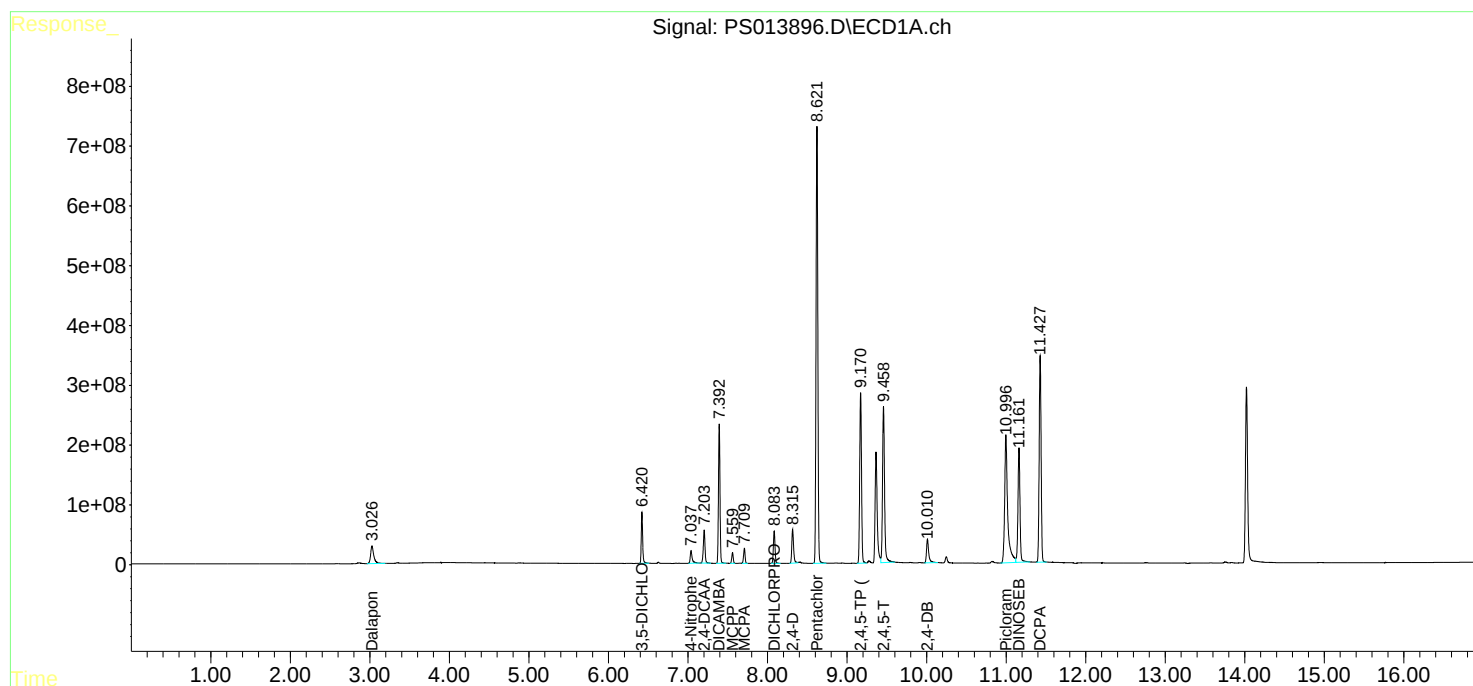


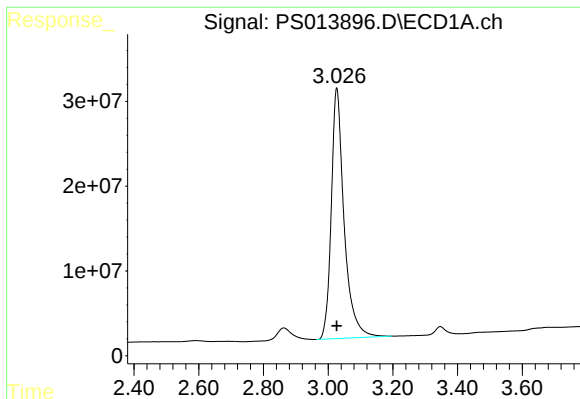

#1 Dalapon


R.T.: 3.027 min
Delta R.T.: 0.000 min
Response: 812370294
Conc: 650.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

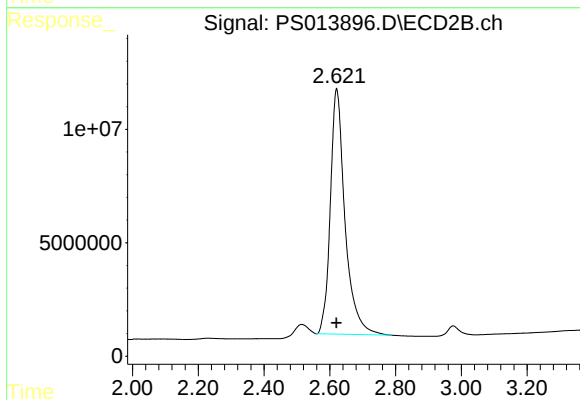


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 336034955
Conc: 653.56 ng/ml

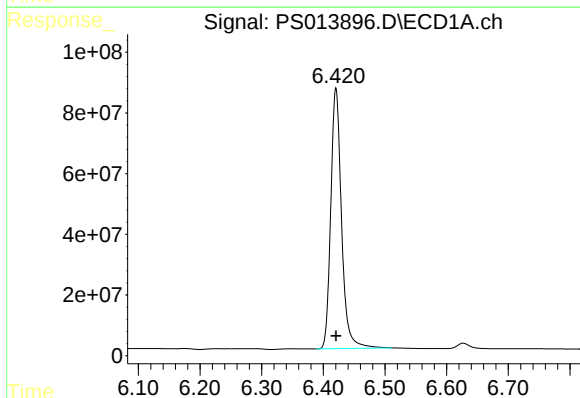


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 1039800169
Conc: 699.71 ng/ml

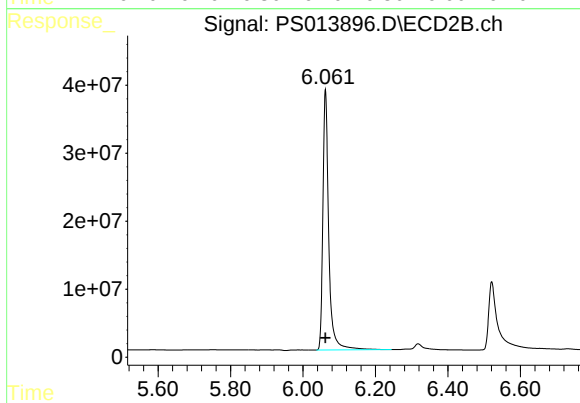

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 430275716
Conc: 708.69 ng/ml

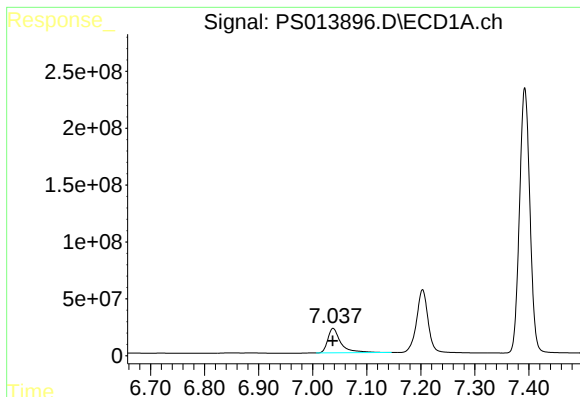

#3 4-Nitrophenol


R.T.: 7.038 min
Delta R.T.: 0.001 min
Response: 363743693
Conc: 669.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

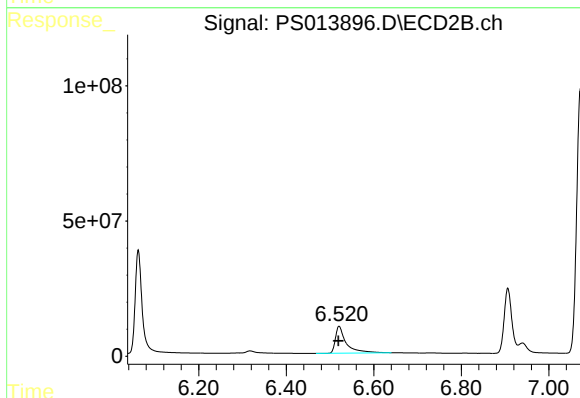


#3 4-Nitrophenol

R.T.: 6.521 min
Delta R.T.: 0.001 min
Response: 170149114
Conc: 676.61 ng/ml

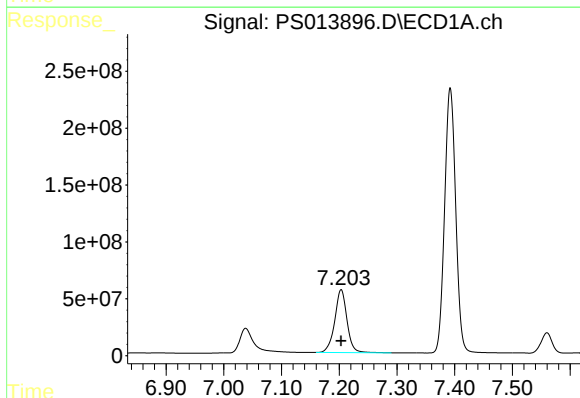


#4 2,4-DCAA

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 815160352
Conc: 757.69 ng/ml

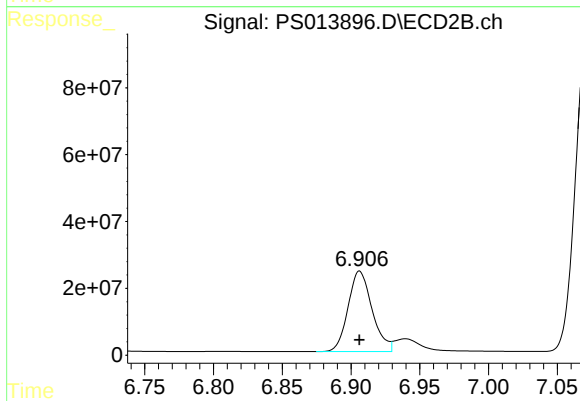

#4 2,4-DCAA


R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 293287831
Conc: 760.30 ng/ml

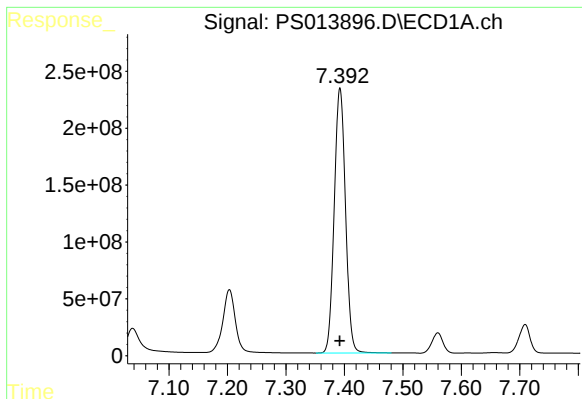

#5 DICAMBA


R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 3112526659
Conc: 723.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

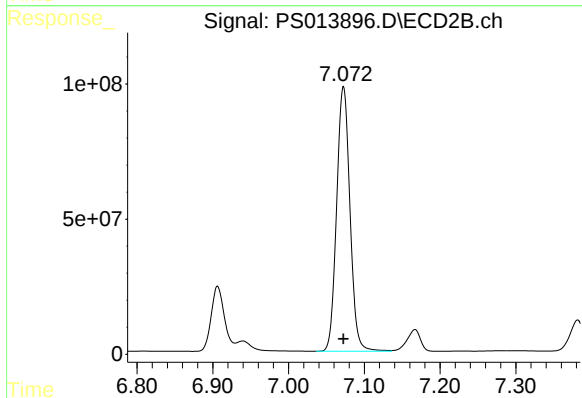


#5 DICAMBA

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 1199269097
Conc: 727.73 ng/ml

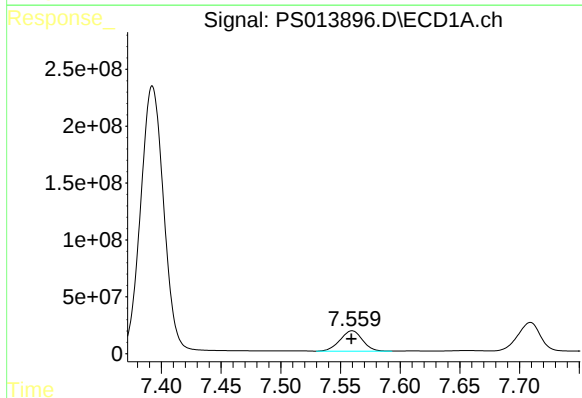


#6 MCP

R.T.: 7.560 min
Delta R.T.: 0.000 min
Response: 233846146
Conc: 74.10 ug/ml

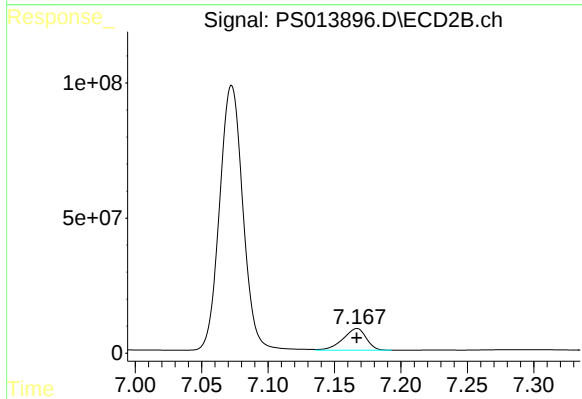

#6 MCP


R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 98001738
Conc: 72.97 ug/ml

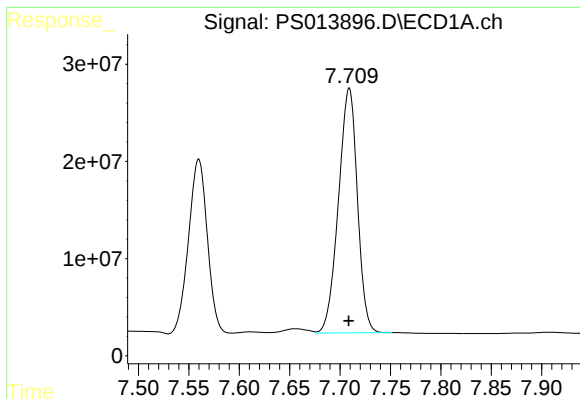

#7 MCPA


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 329780990
Conc: 72.87 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

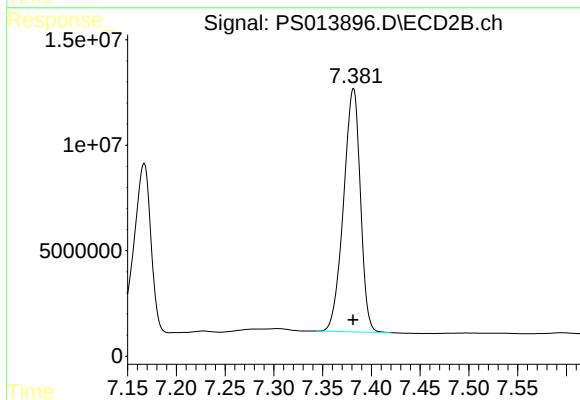


#7 MCPA

R.T.: 7.382 min
Delta R.T.: 0.000 min
Response: 138627582
Conc: 71.51 ug/ml

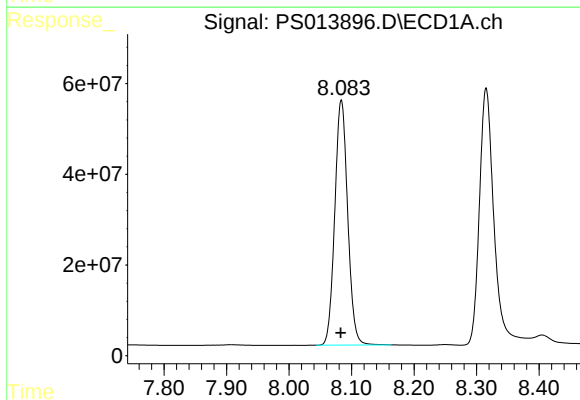


#8 DICHLORPROP

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 774095225
Conc: 712.19 ng/ml

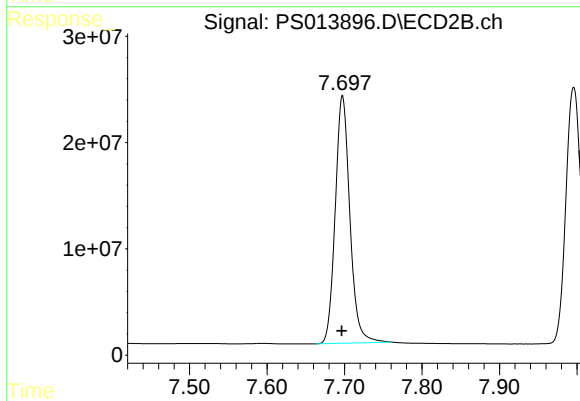

#8 DICHLORPROP


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 306214487
Conc: 719.70 ng/ml

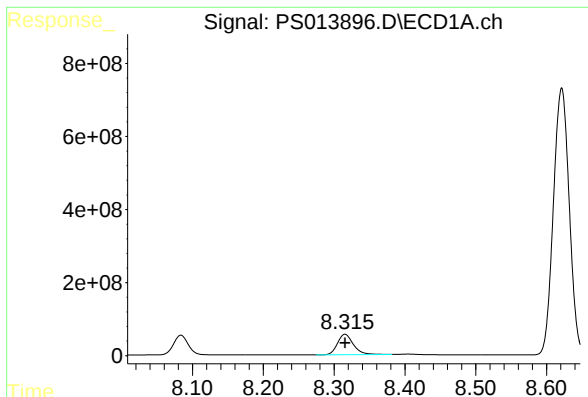

#9 2,4-D


R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 888731617
Conc: 723.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

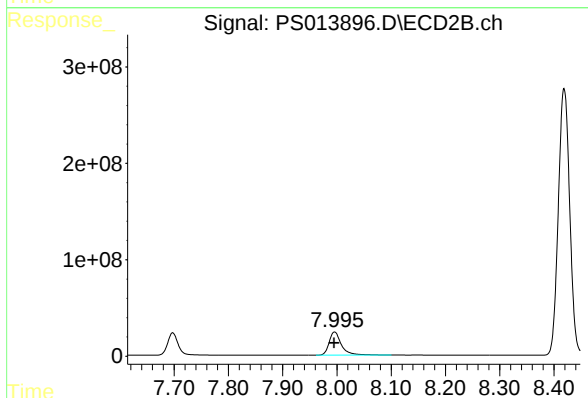


#9 2,4-D

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 378219480
Conc: 709.54 ng/ml

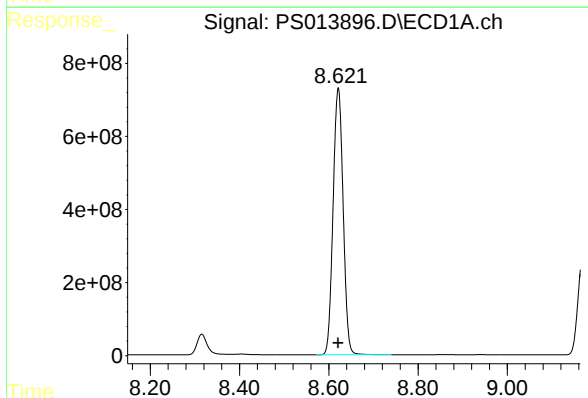


#10 Pentachlorophenol

R.T.: 8.621 min
Delta R.T.: 0.000 min
Response: 11406119087
Conc: 720.25 ng/ml

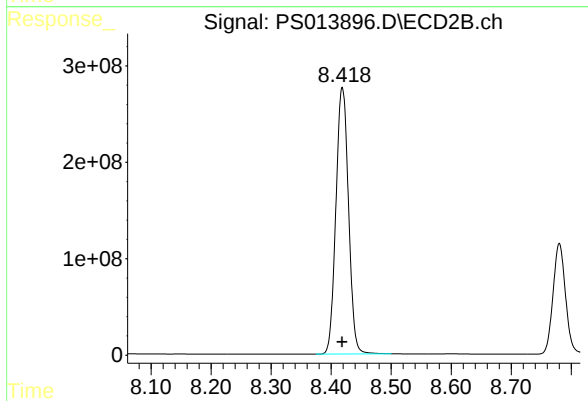

#10 Pentachlorophenol


R.T.: 8.419 min
Delta R.T.: 0.000 min
Response: 4034895258
Conc: 724.31 ng/ml

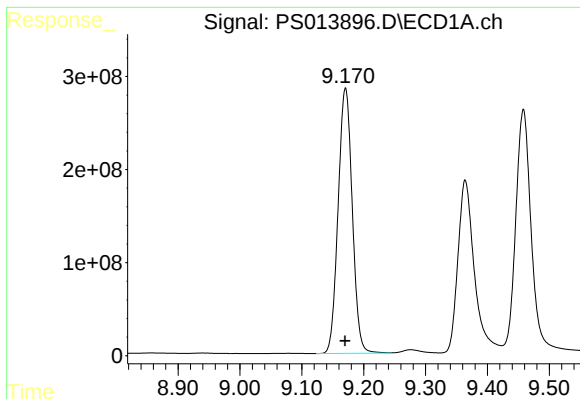

#11 2,4,5-TP (SILVEX)


R.T.: 9.171 min
Delta R.T.: 0.001 min
Response: 4528711437
Conc: 721.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

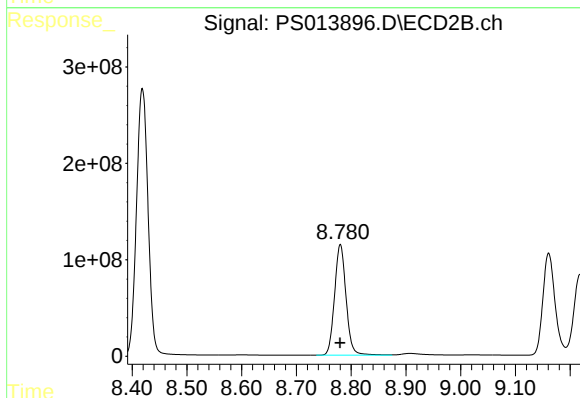


#11 2,4,5-TP (SILVEX)

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 1672758081
Conc: 728.71 ng/ml

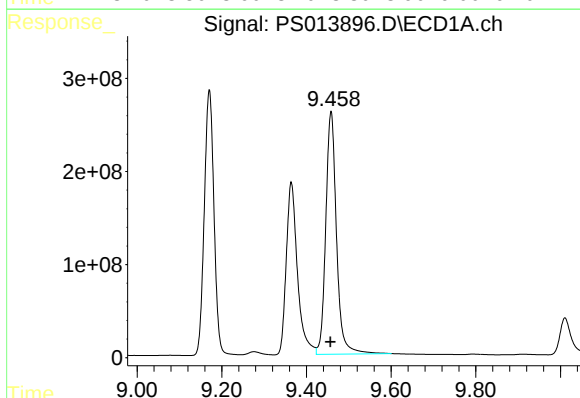


#12 2,4,5-T

R.T.: 9.458 min
Delta R.T.: 0.001 min
Response: 4595501527
Conc: 713.46 ng/ml

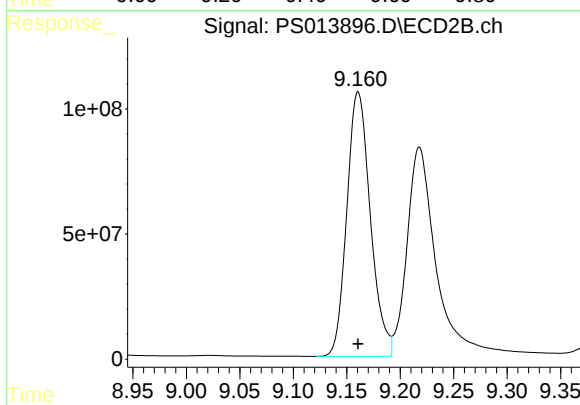

#12 2,4,5-T


R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 1620283002
Conc: 727.65 ng/ml

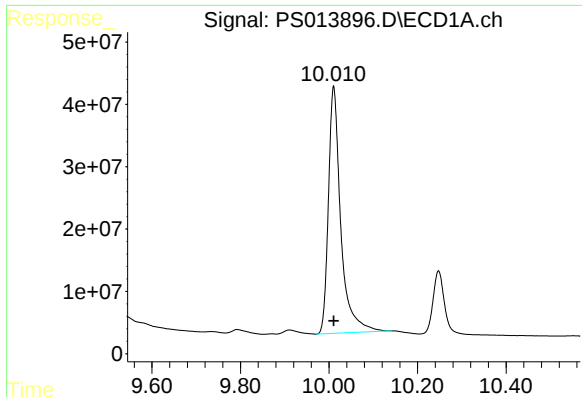

#13 2,4-DB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 768936176
Conc: 696.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

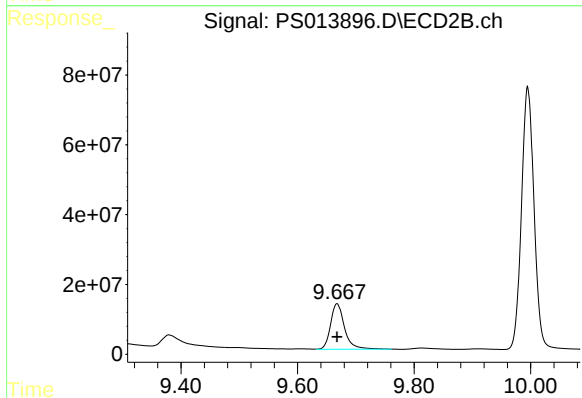


#13 2,4-DB

R.T.: 9.668 min
Delta R.T.: 0.000 min
Response: 217450169
Conc: 727.21 ng/ml

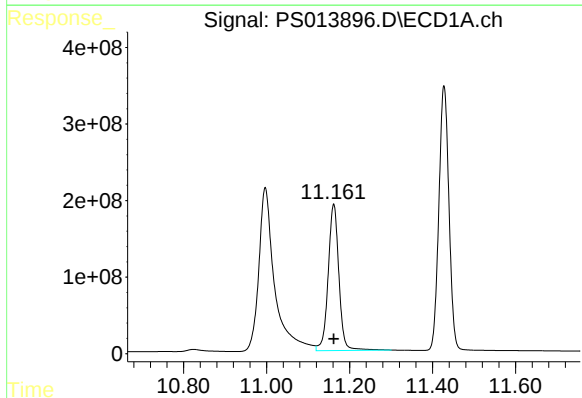


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: 0.000 min
Response: 3437166727
Conc: 678.21 ng/ml

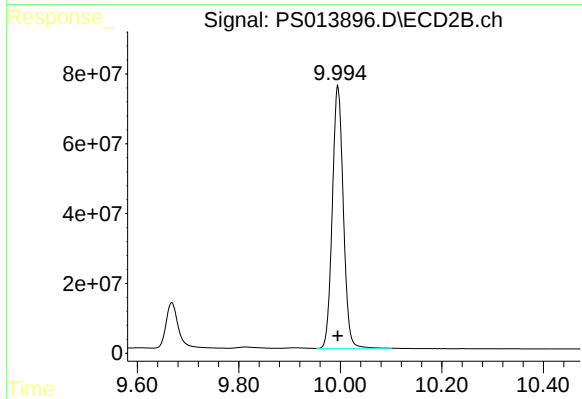

#14 DINOSEB


R.T.: 9.995 min
Delta R.T.: 0.000 min
Response: 1129602670
Conc: 691.43 ng/ml

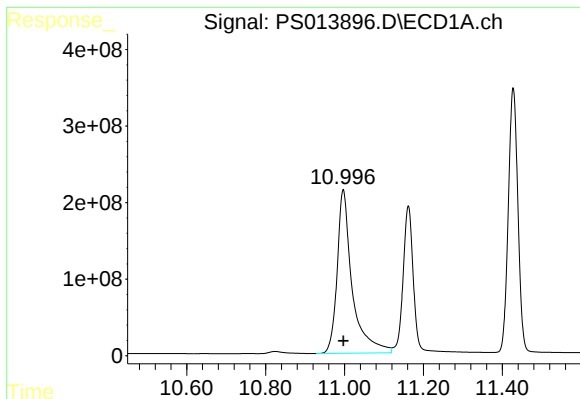

#15 Picloram


R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 5671256105
Conc: 667.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

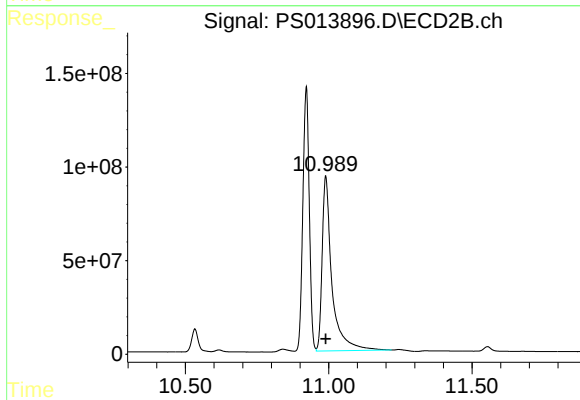


#15 Picloram

R.T.: 10.990 min
Delta R.T.: 0.000 min
Response: 2223410298
Conc: 651.52 ng/ml

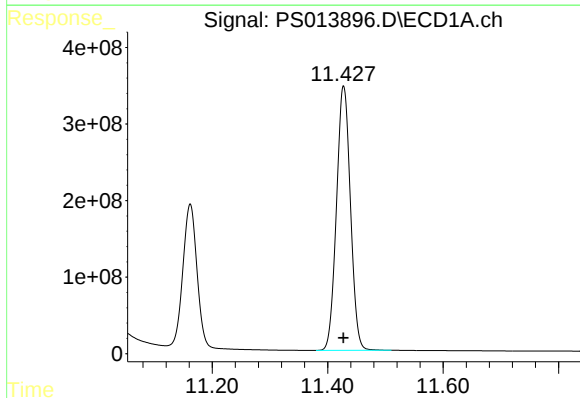

#16 DCPA

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 5809300623
Conc: 718.63 ng/ml

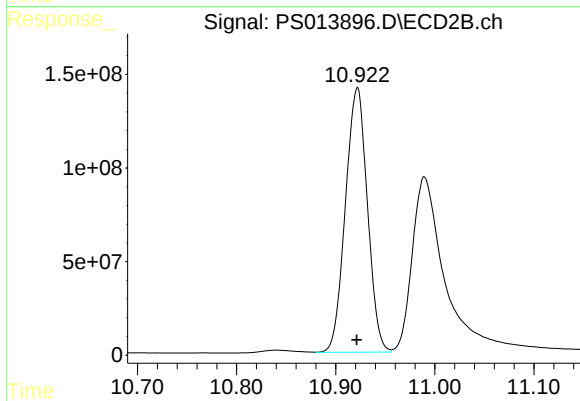

#16 DCPA

R.T.: 10.922 min
Delta R.T.: 0.000 min
Response: 2181635022
Conc: 728.21 ng/ml