

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 12:01
 Operator : EI\SJ
 Sample : PB116656TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116656TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 14:44:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.298	10.791	206.3E6	255.2E6	543.334	596.902
Target Compounds							
1) T	Dalapon	0.000	2.290	0	116.1E6	N.D.	216.564 #
2) T	3,5-DICHL...	0.000	8.958	0	3090946	N.D.	5.485 #
5) T	DICAMBA	0.000	11.032	0	2307352	N.D.	1.454 #
6) T	MCP	11.964	0.000	32537937	0	27.157	N.D. #
12) T	2,4,5-T	0.000	14.447	0	4623965	N.D.	2.417 #
14) T	DINOSEB	0.000	15.527	0	12380195	N.D.	7.062 #
15) T	Picloram	0.000	16.719	0	45756343	N.D.	15.220 #
16) T	DCPA	0.000	16.719	0	45756343	N.D.	14.772 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 12:01
Operator : EI\SJ
Sample : PB116656TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116656TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 14:44:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

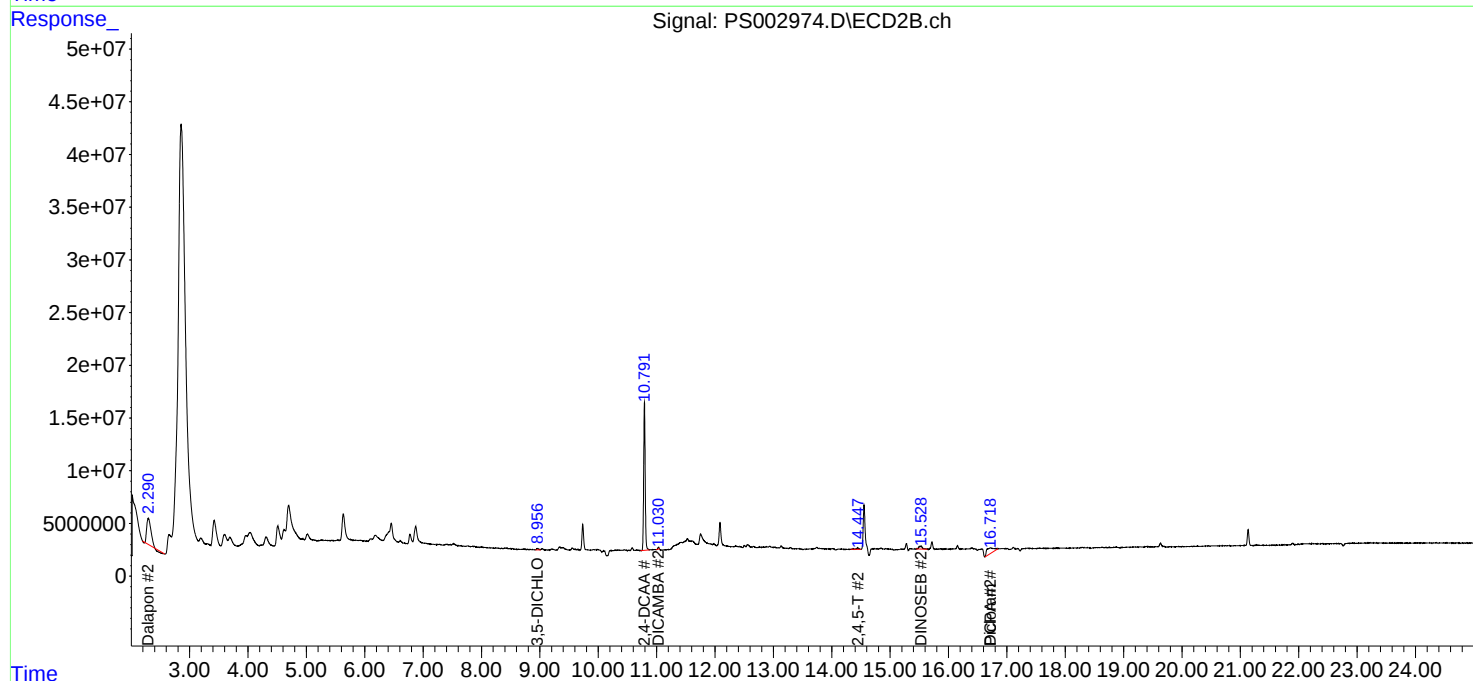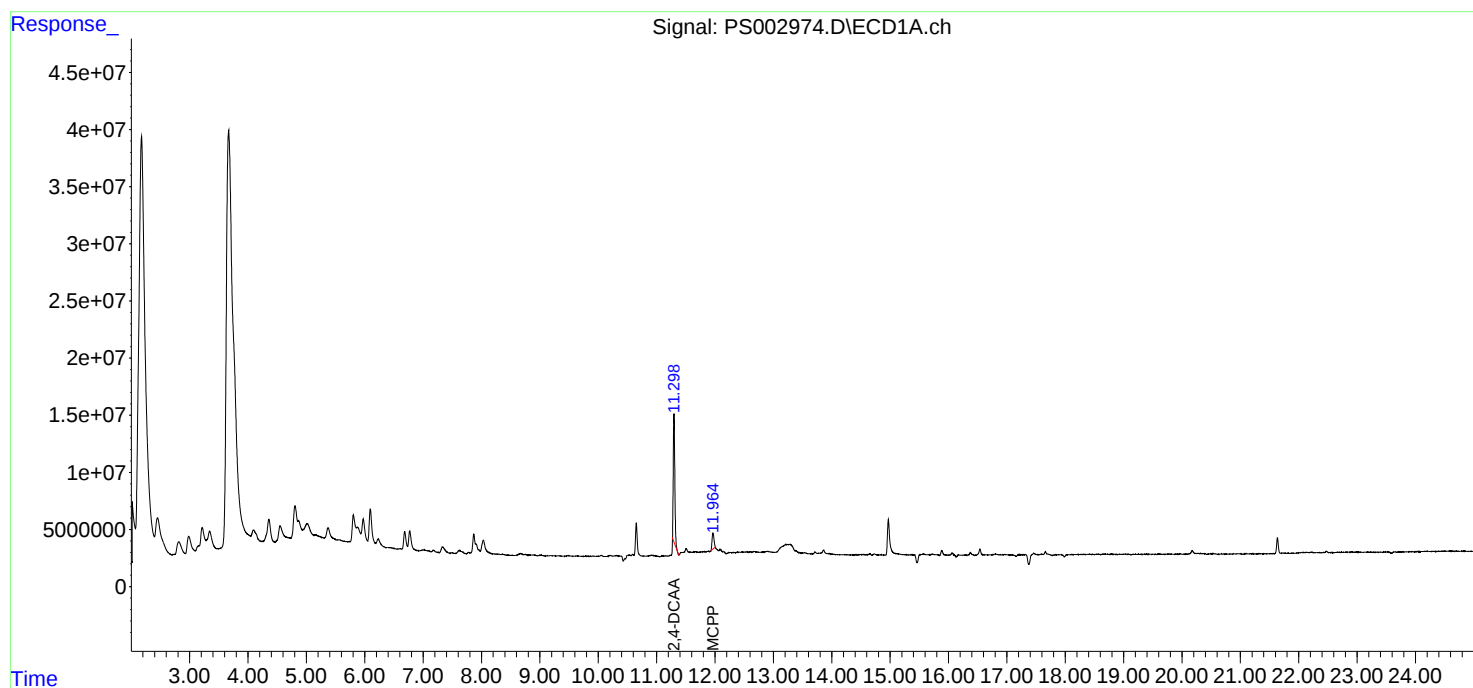


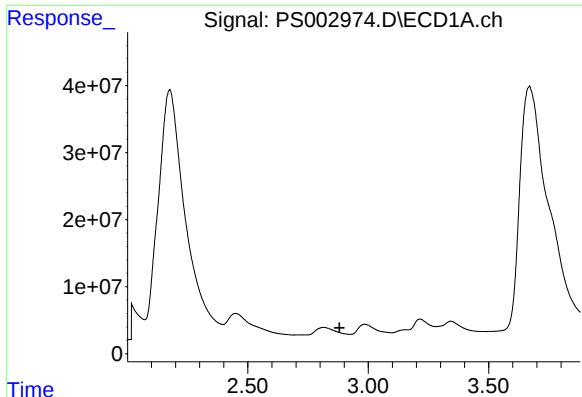

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

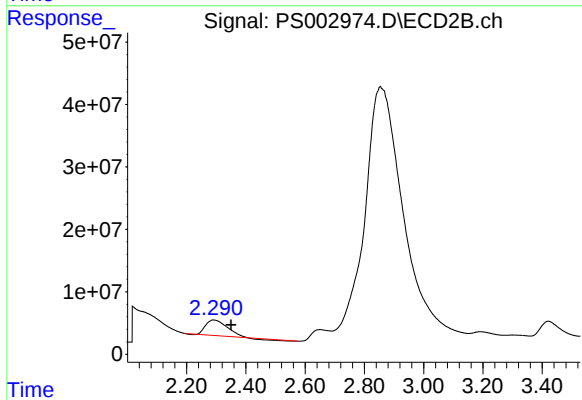


#1 Dalapon

R.T.: 2.290 min
Delta R.T.: -0.060 min
Response: 116061207
Conc: 216.56 ng/ml

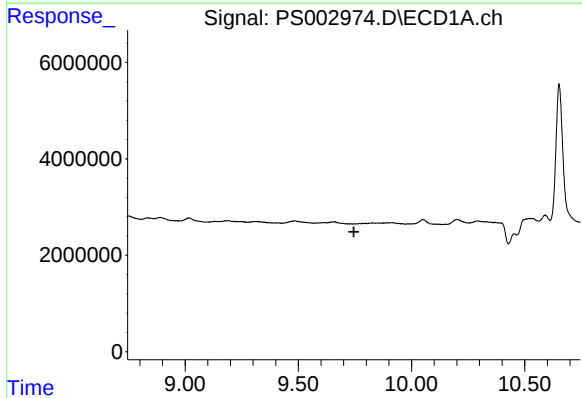


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

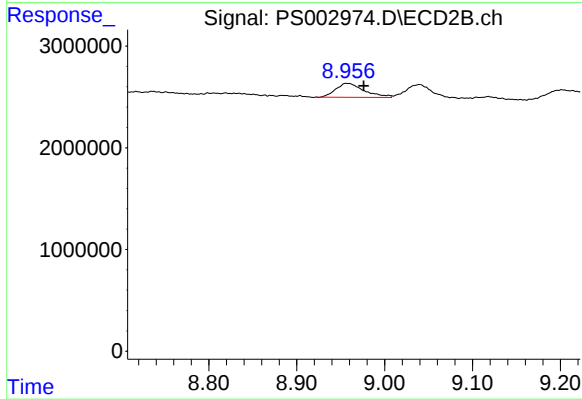

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.958 min
Delta R.T.: -0.018 min
Response: 3090946
Conc: 5.48 ng/ml

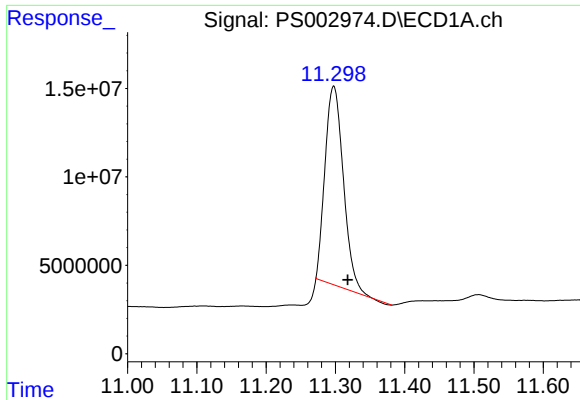

#4 2,4-DCAA


R.T.: 11.298 min
Delta R.T.: -0.020 min
Response: 206271802
Conc: 543.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116656TB

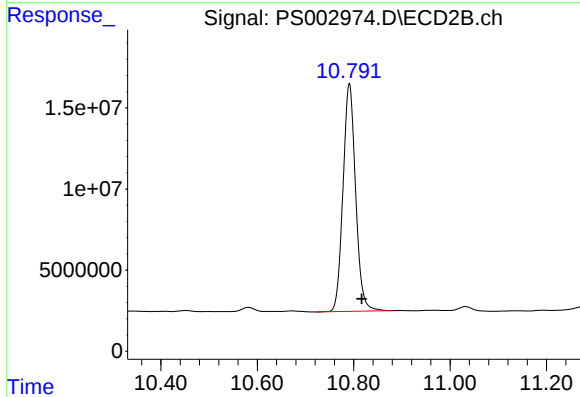


#4 2,4-DCAA

R.T.: 10.791 min
Delta R.T.: -0.026 min
Response: 255202937
Conc: 596.90 ng/ml

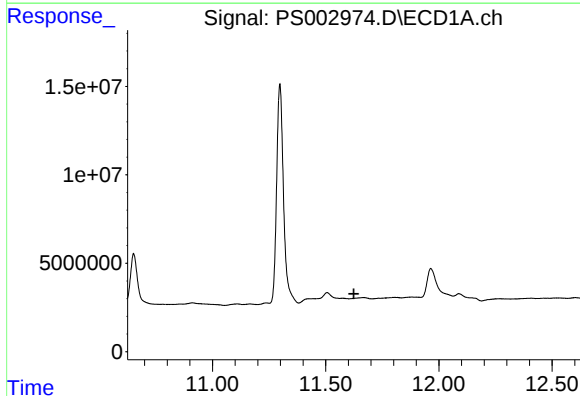


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.624 min
Response: 0
Conc: N.D.

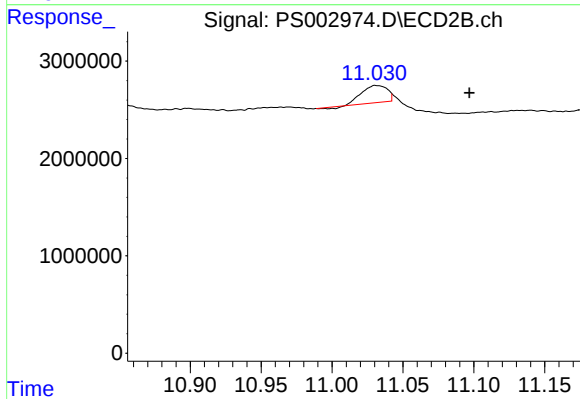

#5 DICAMBA


R.T.: 11.032 min
Delta R.T.: -0.065 min
Response: 2307352
Conc: 1.45 ng/ml

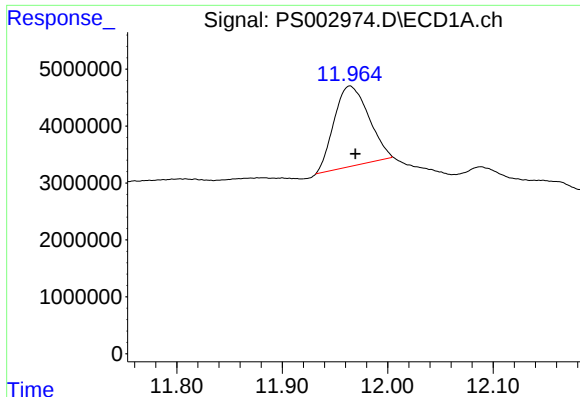

#6 MCP


R.T.: 11.964 min
Delta R.T.: -0.005 min
Response: 32537937
Conc: 27.16 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB116656TB

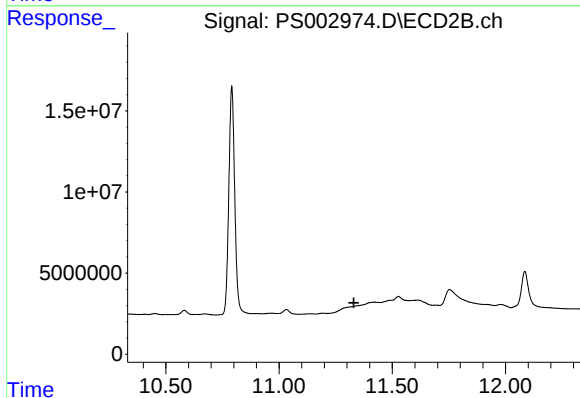


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

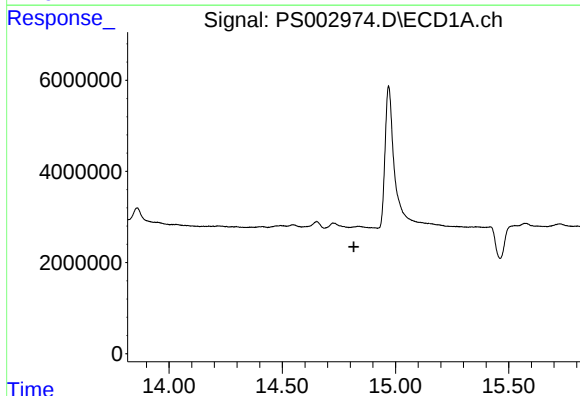


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

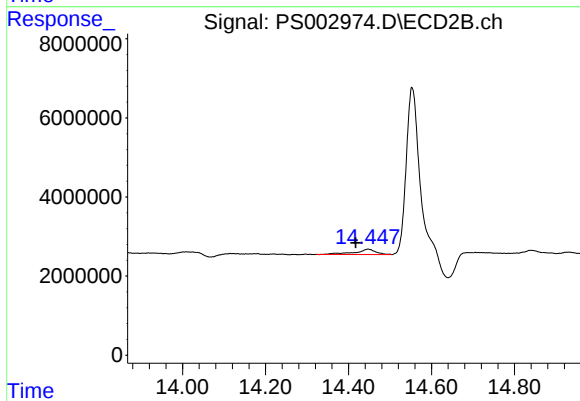

#12 2,4,5-T


R.T.: 14.447 min
Delta R.T.: 0.030 min
Response: 4623965
Conc: 2.42 ng/ml

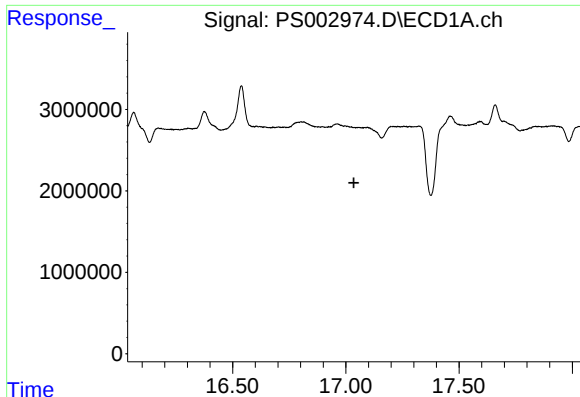

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

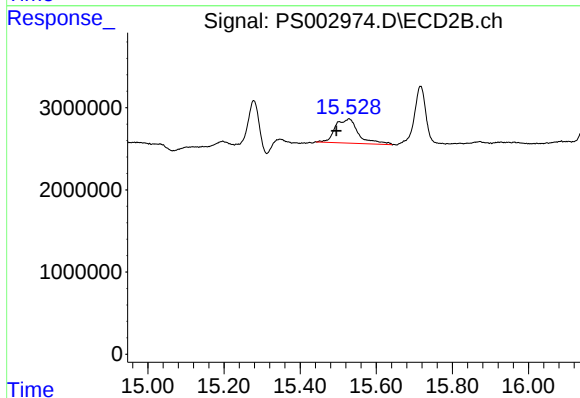


#14 DINOSEB

R.T.: 15.527 min
Delta R.T.: 0.032 min
Response: 12380195
Conc: 7.06 ng/ml

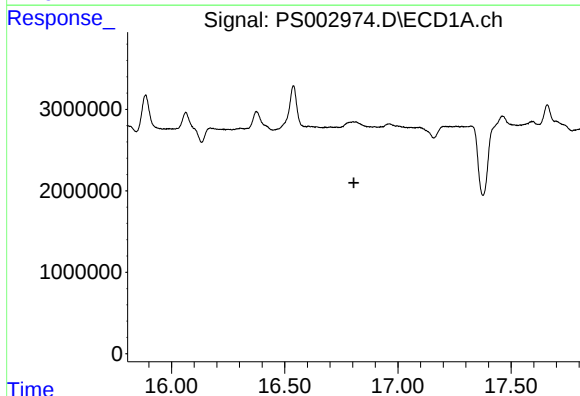


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

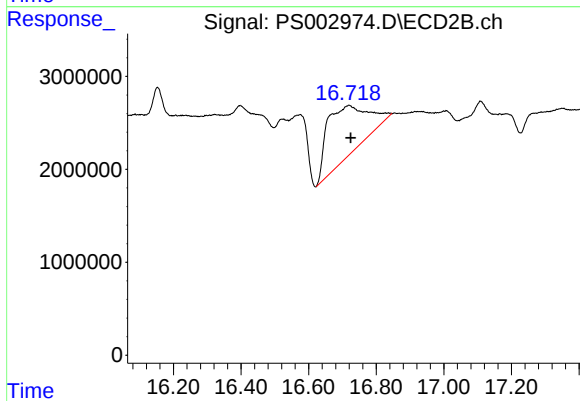

#15 Picloram


R.T.: 16.719 min
Delta R.T.: -0.005 min
Response: 45756343
Conc: 15.22 ng/ml

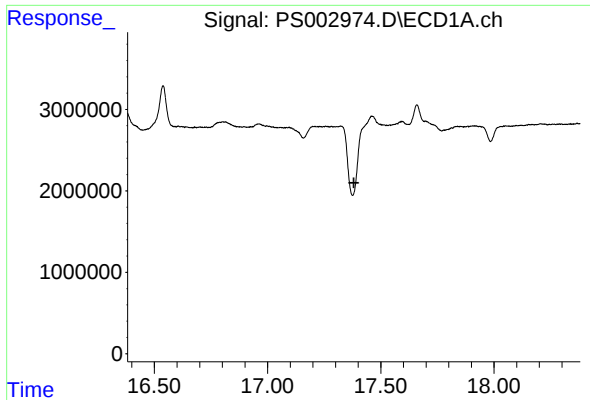

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116656TB

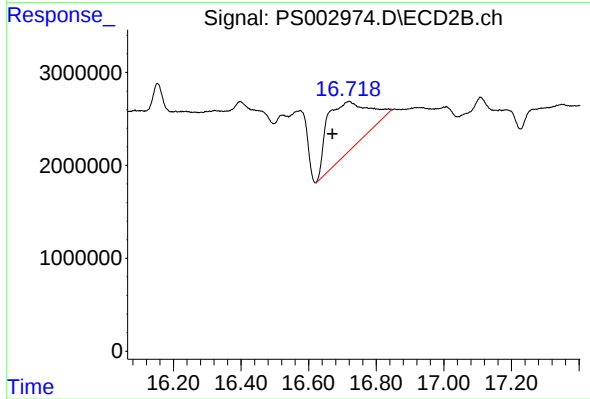

#16 DCPA

R.T.: 16.719 min
Delta R.T.: 0.049 min
Response: 45756343
Conc: 14.77 ng/ml