

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 13:03
 Operator : EI\SJ
 Sample : K1011-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-01-012519-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 14:45:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.301	10.800	143.6E6	158.0E6	378.165	369.636
Target Compounds							
1) T	Dalapon	0.000	2.297	0	16161216	N.D.	30.156 #
2) T	3,5-DICHL...	0.000	8.967	0	6610350	N.D.	11.729 #
6) T	MCP	11.969	0.000	22579710	0	18.846	N.D. #
11) T	2,4,5-TP ...	14.426	0.000	3470206	0	1.378	N.D. #
14) T	DINOSEB	0.000	15.507	0	3659761	N.D.	2.088 #
15) T	Picloram	0.000	16.724	0	23550673	N.D.	7.834 #
16) T	DCPA	0.000	16.724	0	23550673	N.D.	7.603 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 13:03
Operator : EI\SJ
Sample : K1011-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-01-012519-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 14:45:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

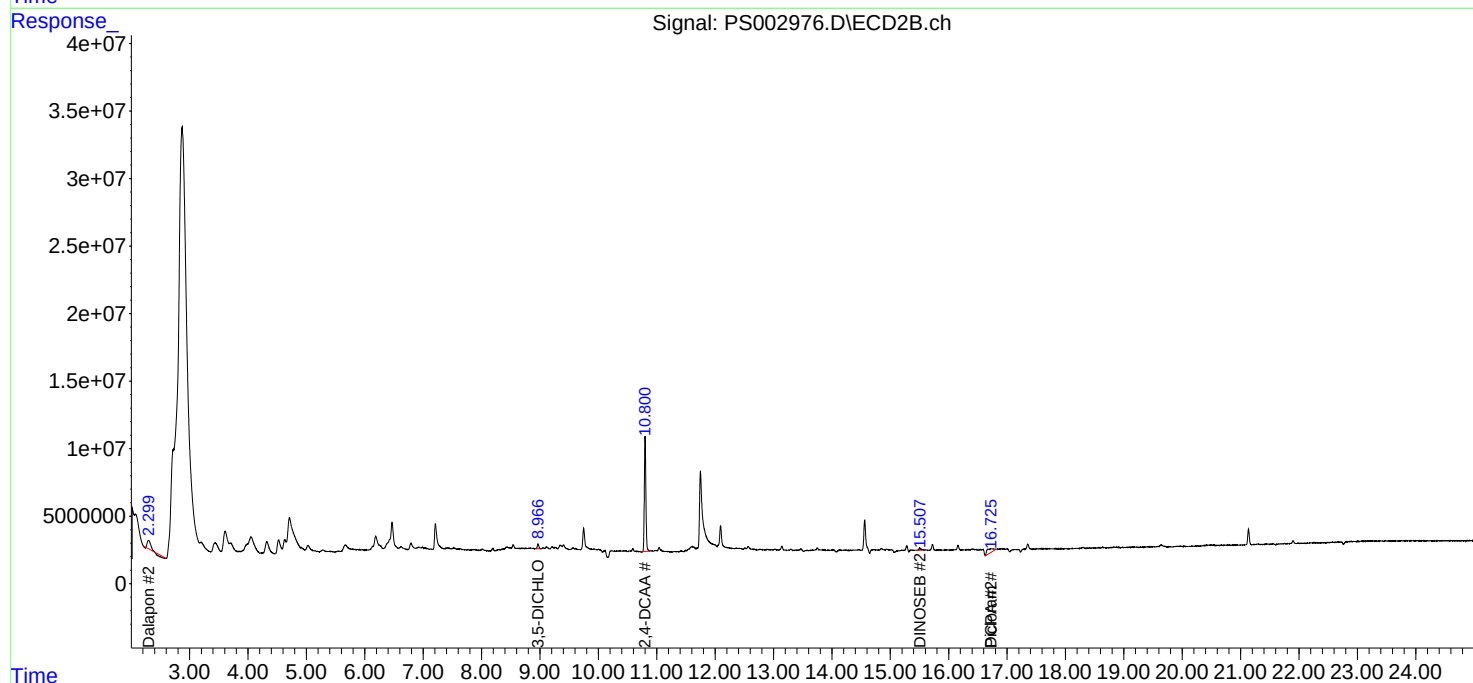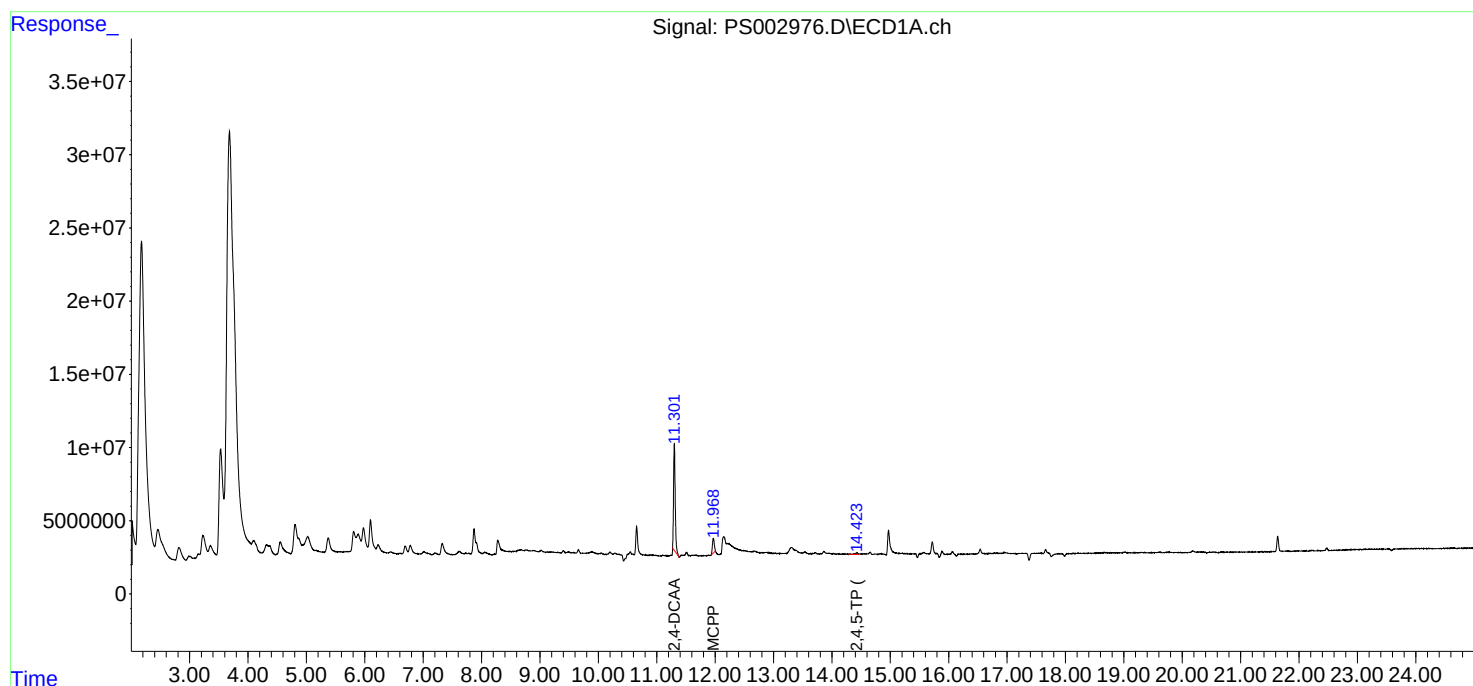


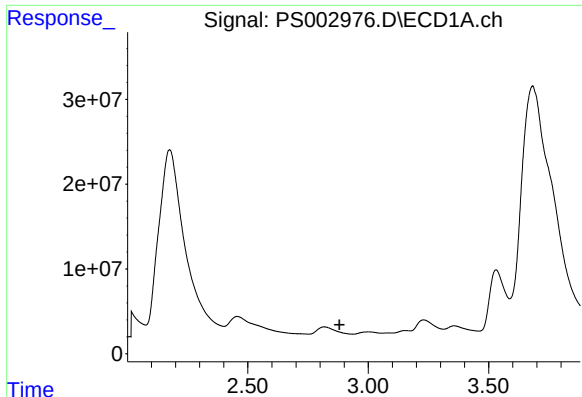

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-012519-A

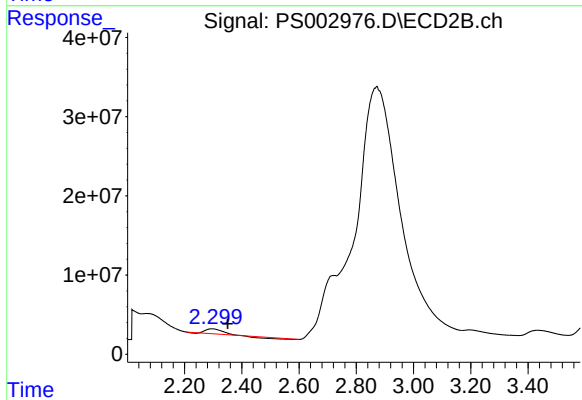


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.054 min
Response: 16161216
Conc: 30.16 ng/ml

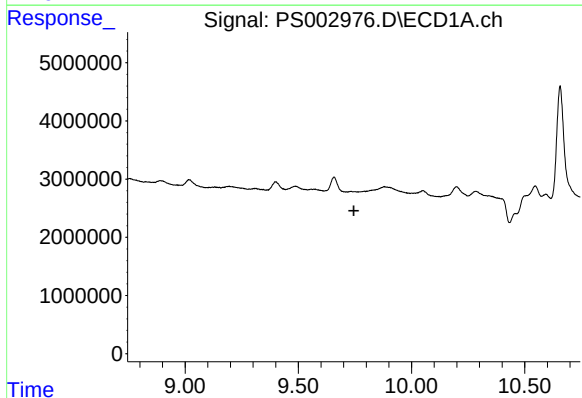


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

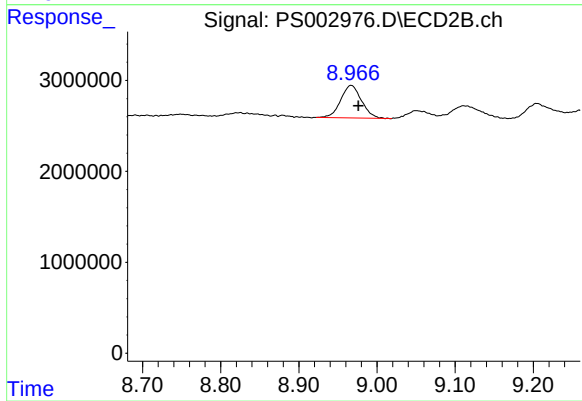

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.967 min
Delta R.T.: -0.009 min
Response: 6610350
Conc: 11.73 ng/ml

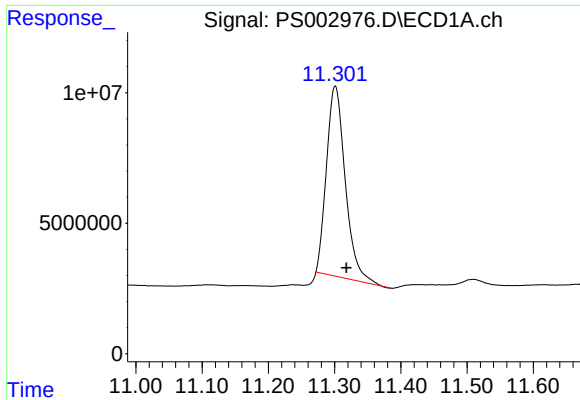

#4 2,4-DCAA


R.T.: 11.301 min
Delta R.T.: -0.017 min
Response: 143566928
Conc: 378.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-01-012519-A

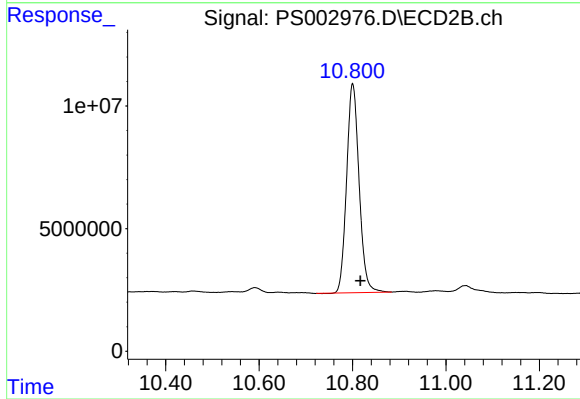


#4 2,4-DCAA

R.T.: 10.800 min
Delta R.T.: -0.016 min
Response: 158036185
Conc: 369.64 ng/ml

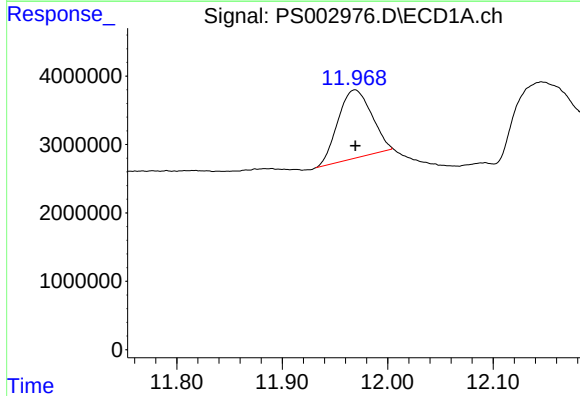


#6 MCP

R.T.: 11.969 min
Delta R.T.: 0.000 min
Response: 22579710
Conc: 18.85 ug/ml

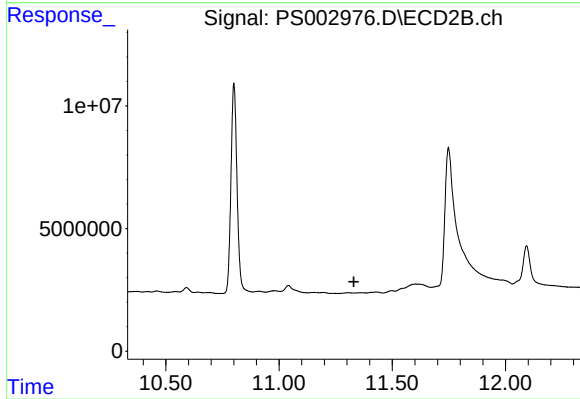

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

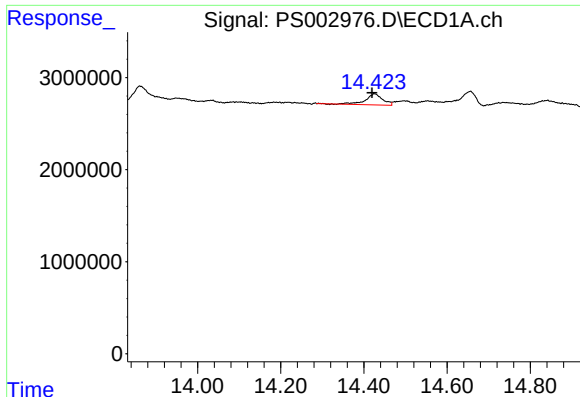

#11 2,4,5-TP (SILVEX)


R.T.: 14.426 min
Delta R.T.: 0.006 min
Response: 3470206
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-01-012519-A

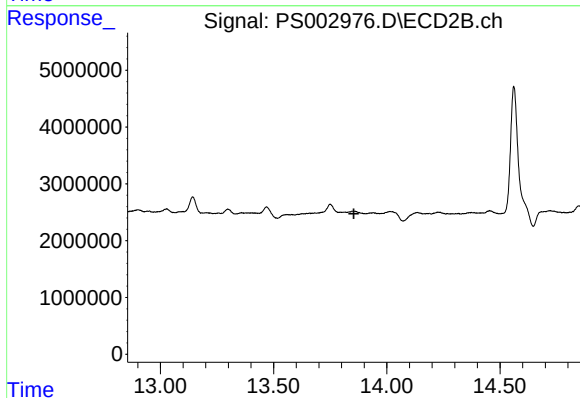


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

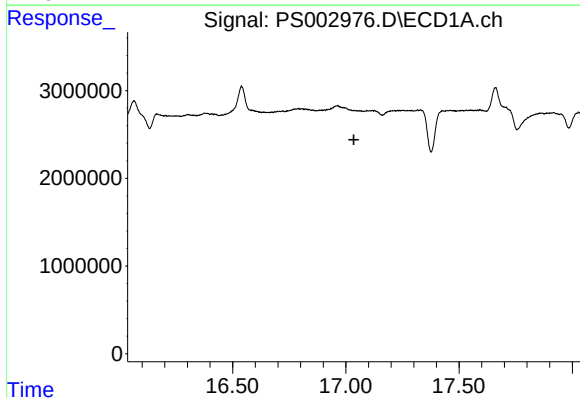


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

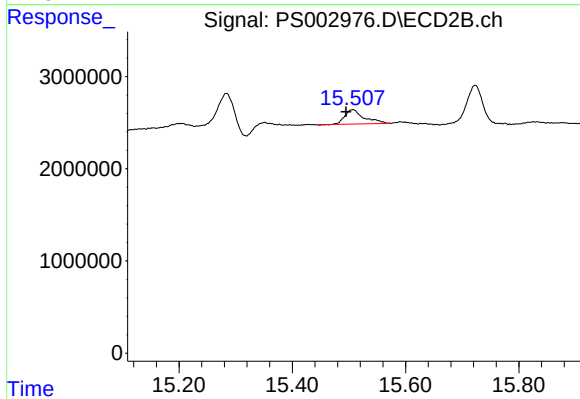

#14 DINOSEB


R.T.: 15.507 min
Delta R.T.: 0.012 min
Response: 3659761
Conc: 2.09 ng/ml

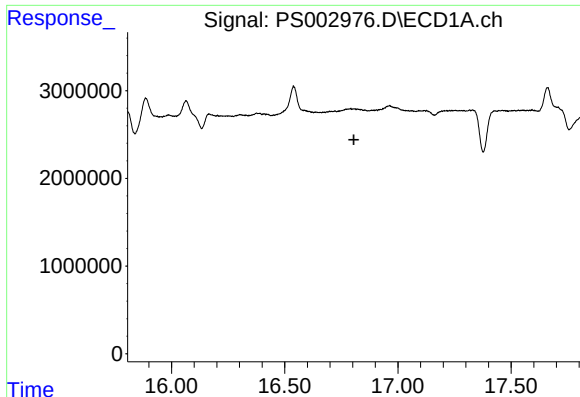

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-01-012519-A

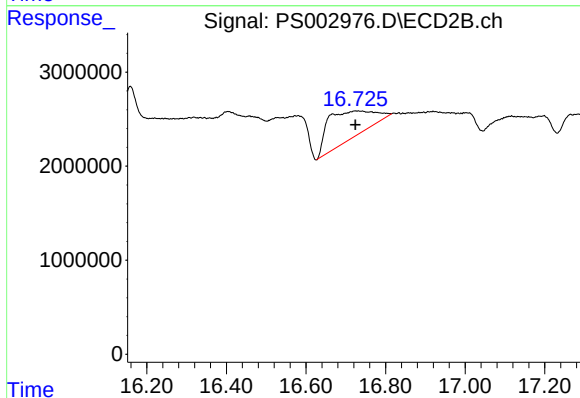


#15 Picloram

R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 23550673
Conc: 7.83 ng/ml

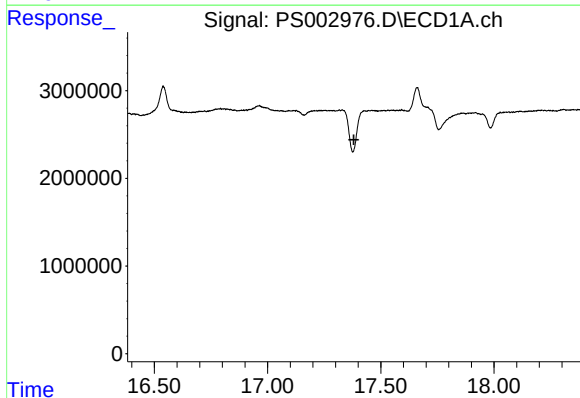

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

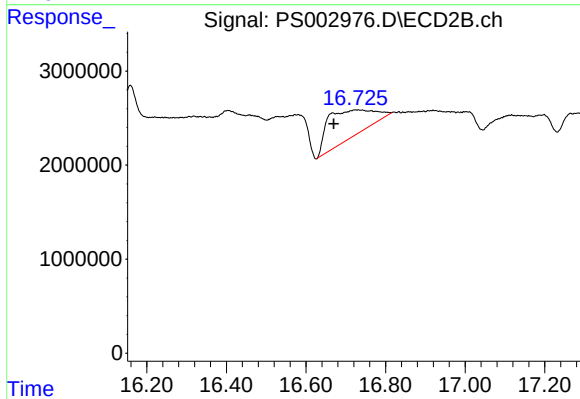

#16 DCPA

R.T.: 16.724 min
Delta R.T.: 0.055 min
Response: 23550673
Conc: 7.60 ng/ml