

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 13:35
 Operator : EI\SJ
 Sample : K1261-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 14:45:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.794	164.6E6	241.3E6	433.625	564.302 #
Target Compounds							
1) T	Dalapon	0.000	2.289	0	9363879	N.D.	17.472 #
2) T	3,5-DICHL...	0.000	8.962	0	7739855	N.D.	13.734 #
6) T	MCP	11.962	0.000	22402127	0	18.698	N.D. #
11) T	2,4,5-TP ...	14.420	0.000	21042389	0	8.356	N.D. #
13) T	2,4-DB	15.566	0.000	2438109	0	9.326	N.D. #
14) T	DINOSEB	0.000	15.499	0	2194209	N.D.	1.252 #
15) T	Picloram	0.000	16.761	0	25549417	N.D.	8.498 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 13:35
Operator : EI\SJ
Sample : K1261-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 14:45:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

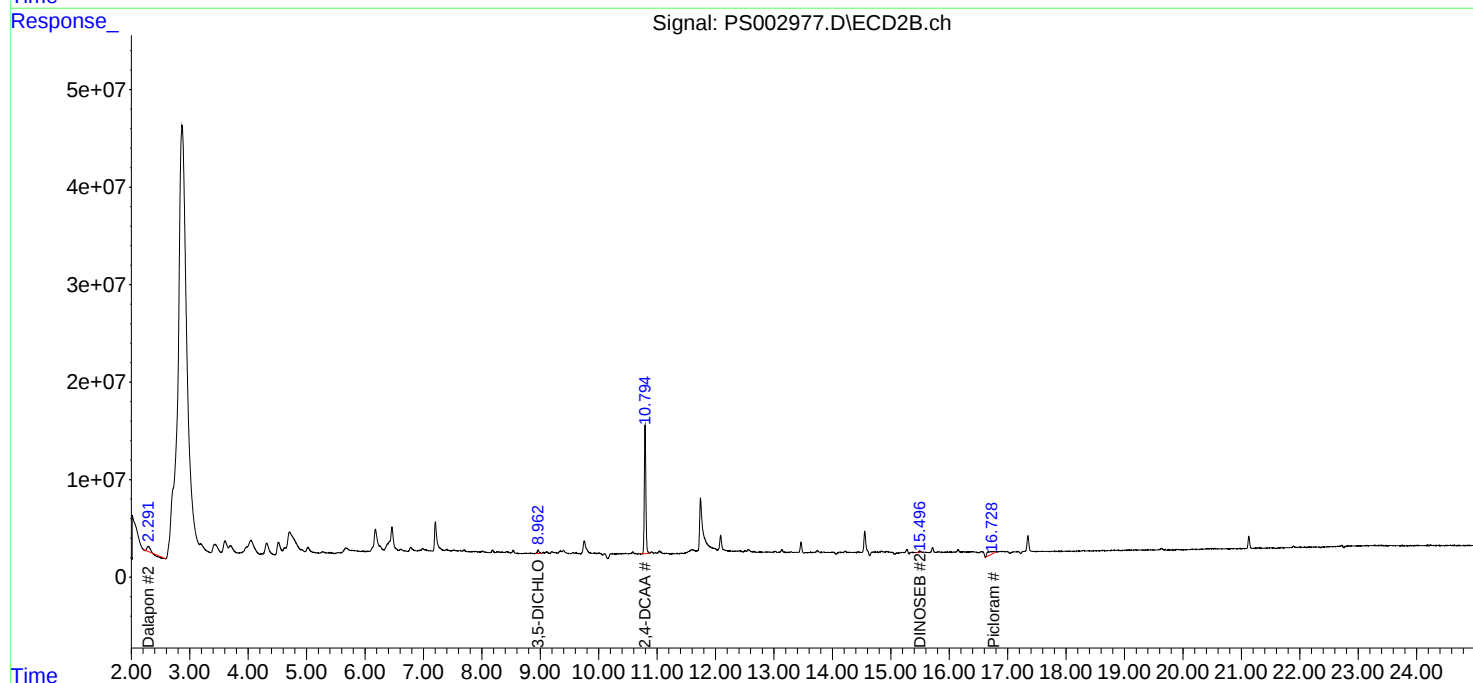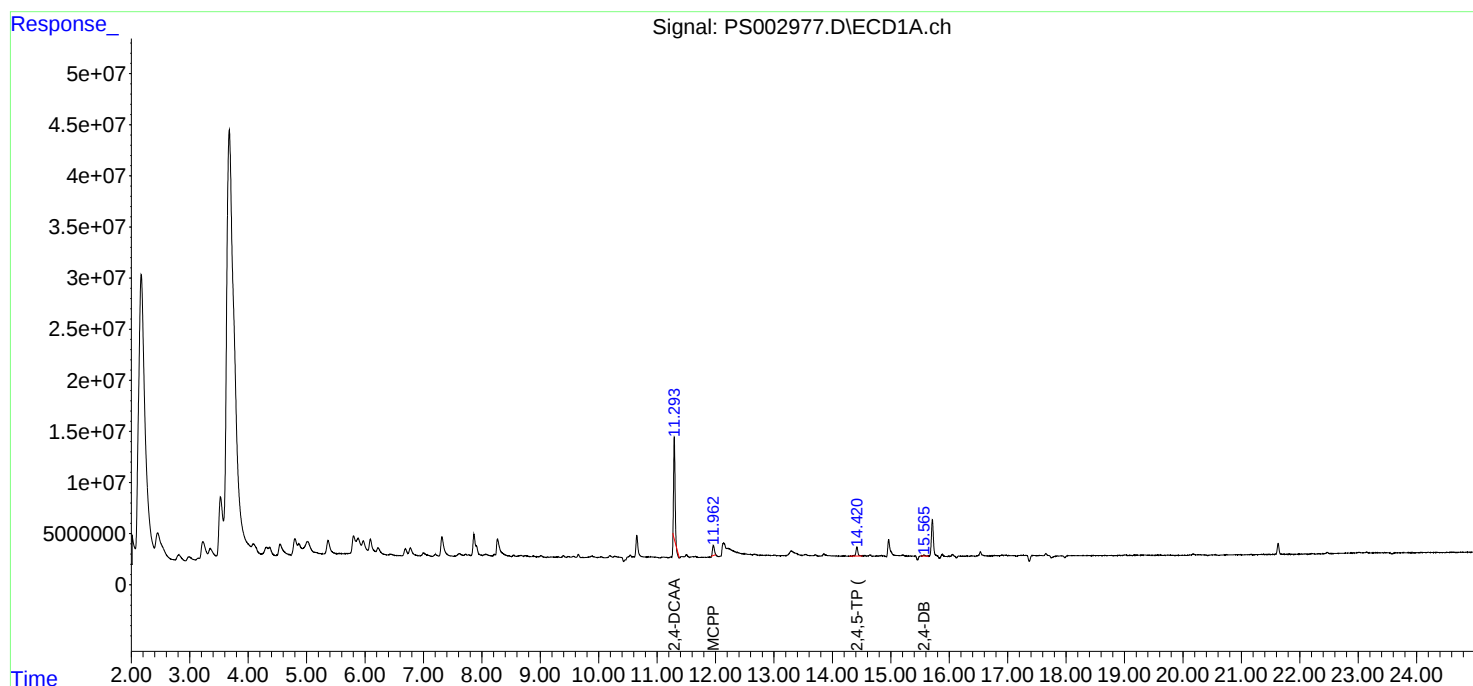


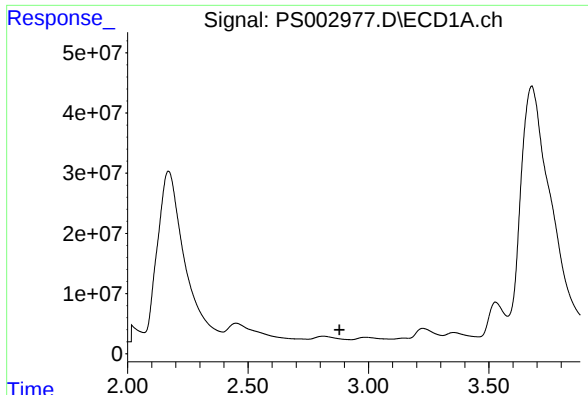

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

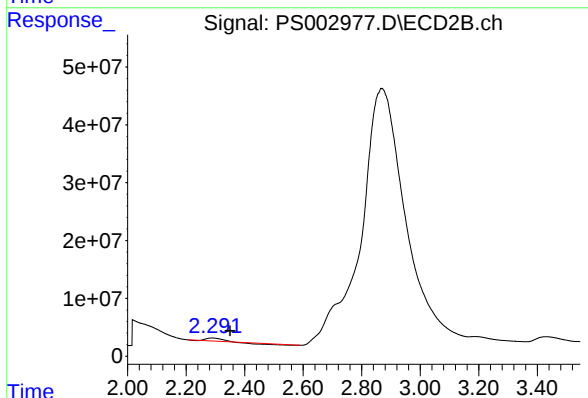


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.061 min
Response: 9363879
Conc: 17.47 ng/ml

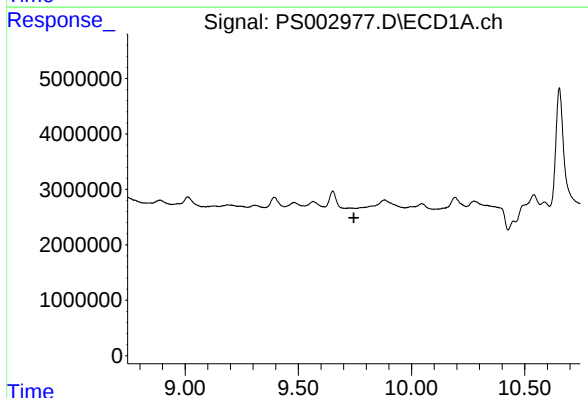


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

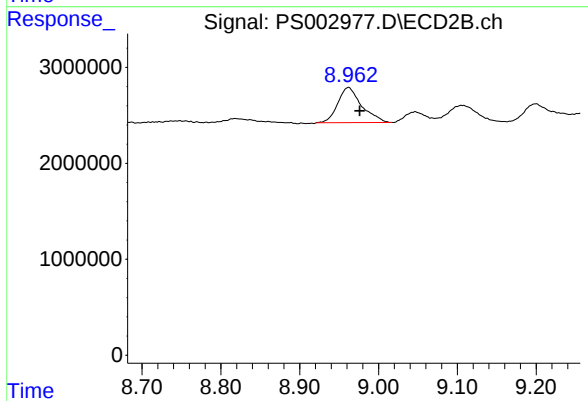

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: -0.015 min
Response: 7739855
Conc: 13.73 ng/ml

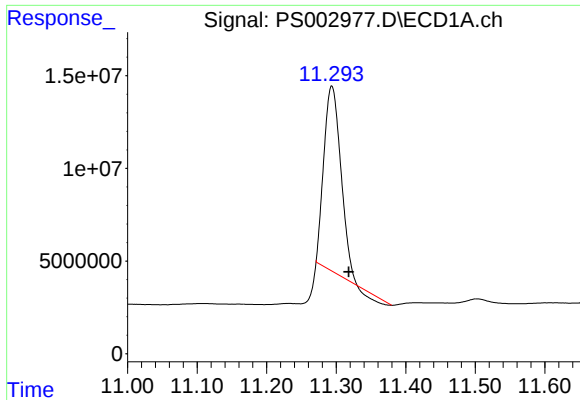

#4 2,4-DCAA


R.T.: 11.294 min
Delta R.T.: -0.024 min
Response: 164621750
Conc: 433.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

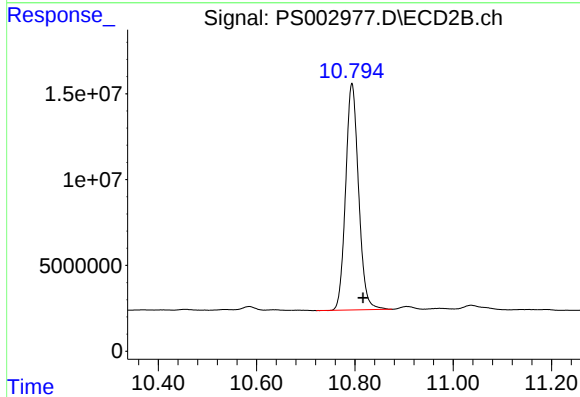


#4 2,4-DCAA

R.T.: 10.794 min
Delta R.T.: -0.023 min
Response: 241264710
Conc: 564.30 ng/ml

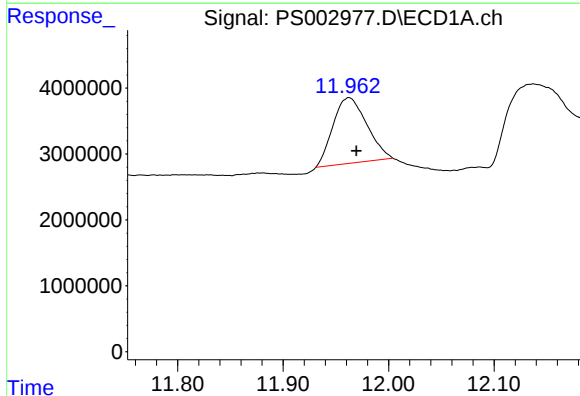


#6 MCP

R.T.: 11.962 min
Delta R.T.: -0.007 min
Response: 22402127
Conc: 18.70 ug/ml

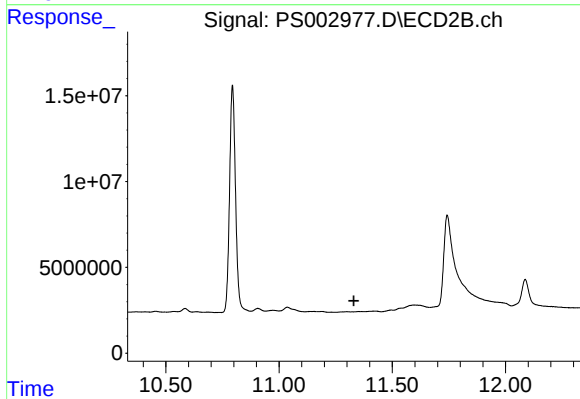

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

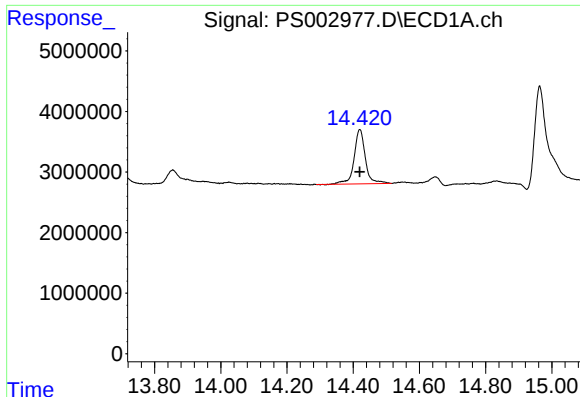

#11 2,4,5-TP (SILVEX)


R.T.: 14.420 min
Delta R.T.: 0.000 min
Response: 21042389
Conc: 8.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

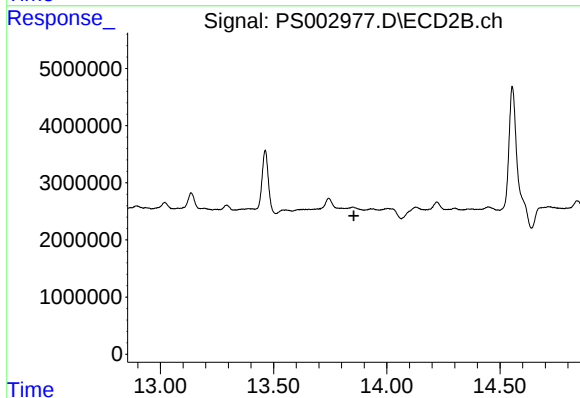


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

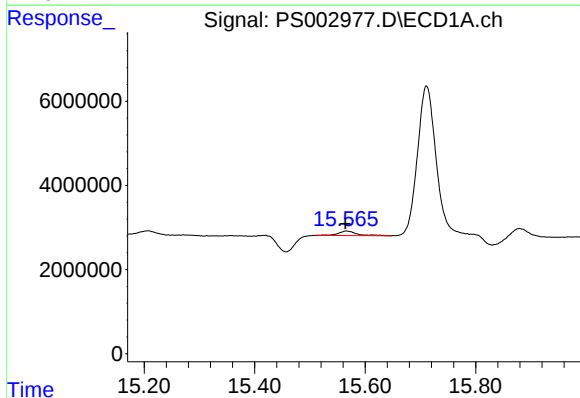


#13 2,4-DB

R.T.: 15.566 min
Delta R.T.: 0.001 min
Response: 2438109
Conc: 9.33 ng/ml

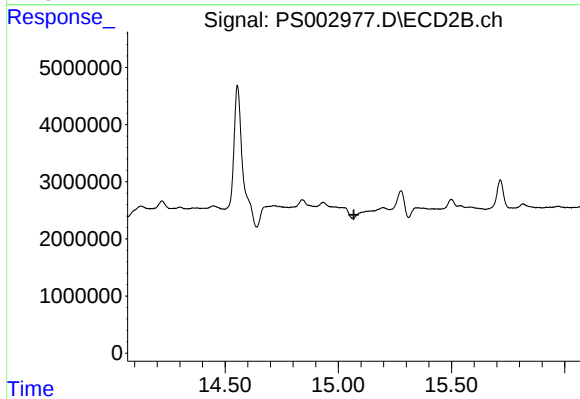

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.069 min
Response: 0
Conc: N.D.

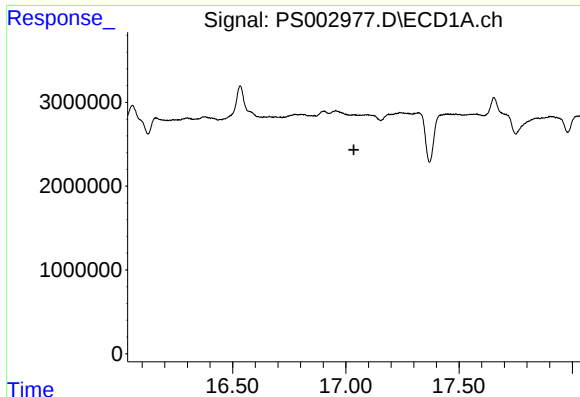

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

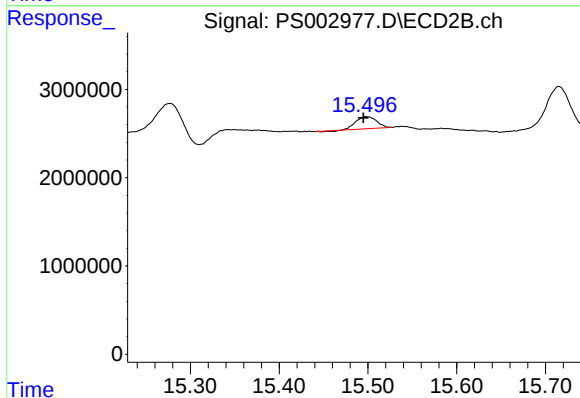


#14 DINOSEB

R.T.: 15.499 min
Delta R.T.: 0.004 min
Response: 2194209
Conc: 1.25 ng/ml

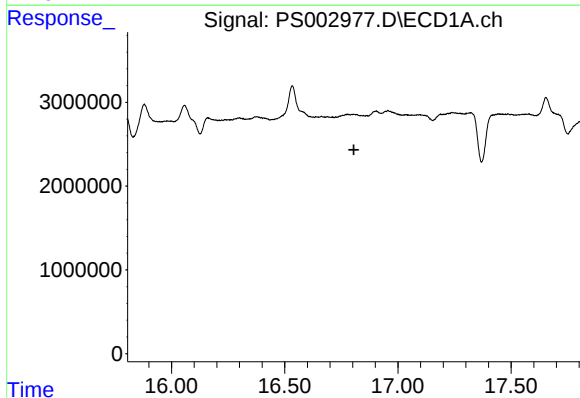

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

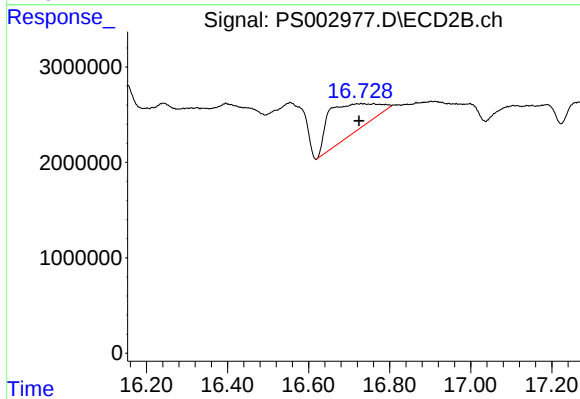

#15 Picloram

R.T.: 16.761 min
Delta R.T.: 0.036 min
Response: 25549417
Conc: 8.50 ng/ml