

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 21:21
 Operator : EI\SJ
 Sample : K1010-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-012819-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 02:45:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.317	10.817	97888804	94424421	257.846	220.852
Target Compounds							
1) T	Dalapon	2.833	2.325	16532887	109.0E6	29.970	203.422 #
2) T	3,5-DICHL...	0.000	8.984	0	3831660	N.D.	6.799 #
6) T	MCPD	11.983	0.000	14881357	0	12.421	N.D. #
7) T	MCPA	0.000	11.759	0	274.3E6	N.D.	174.353 #
10) T	Pentachlo...	13.541	0.000	12026854	0	1.875	N.D. #
12) T	2,4,5-T	0.000	14.426	0	2561765	N.D.	1.339 #
14) T	DINOSEB	0.000	15.521	0	3850563	N.D.	2.197 #
15) T	Picloram	16.819	16.732	5384483	22959757	1.702	7.637 #
16) T	DCPA	0.000	16.732	0	22959757	N.D.	7.412 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 21:21
Operator : EI\SJ
Sample : K1010-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 02:45:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

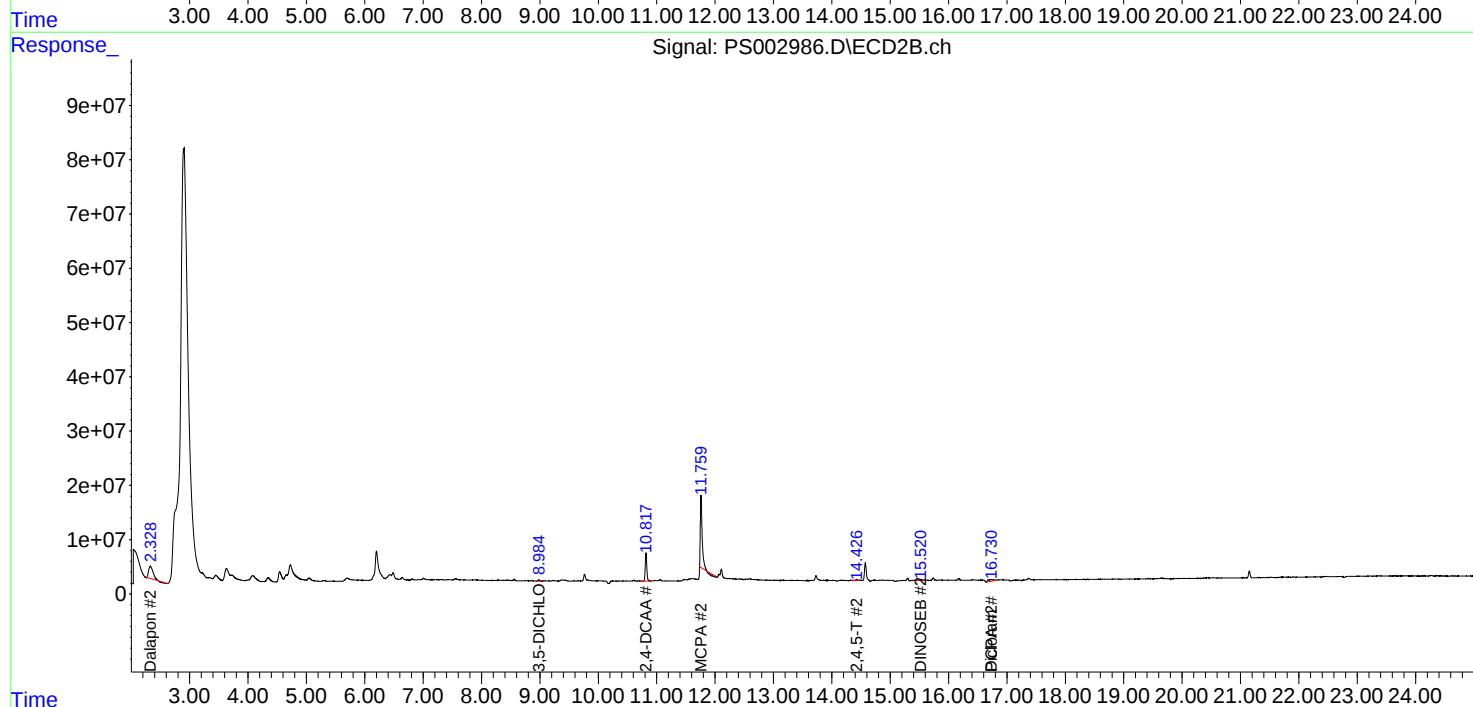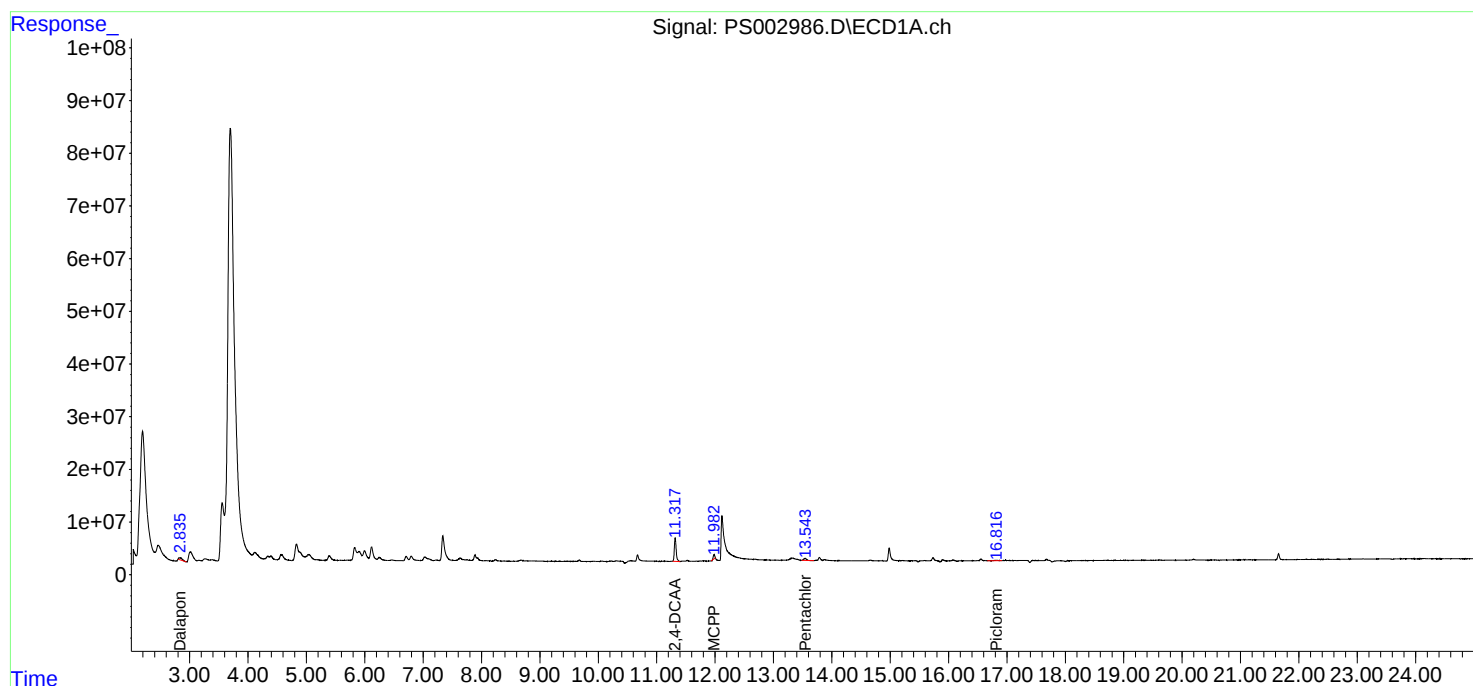


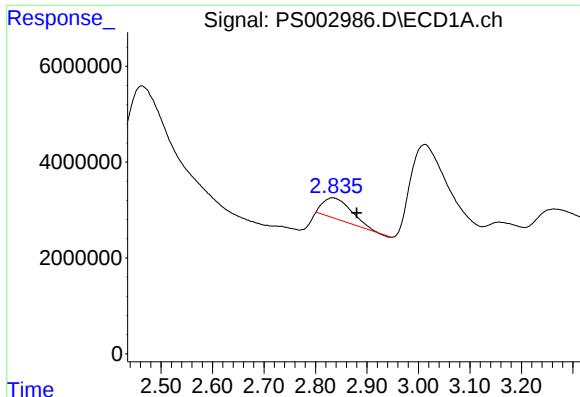

#1 Dalapon


R.T.: 2.833 min
Delta R.T.: -0.047 min
Response: 16532887
Conc: 29.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

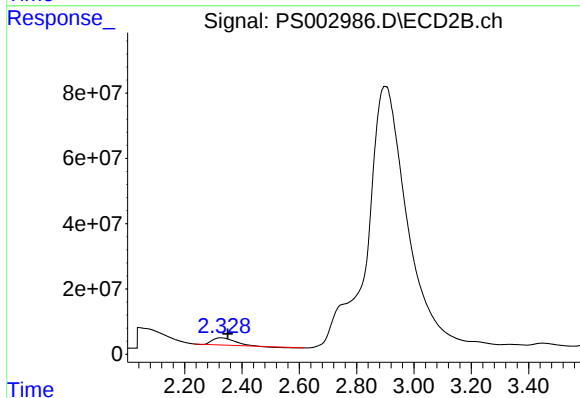


#1 Dalapon

R.T.: 2.325 min
Delta R.T.: -0.025 min
Response: 109018146
Conc: 203.42 ng/ml

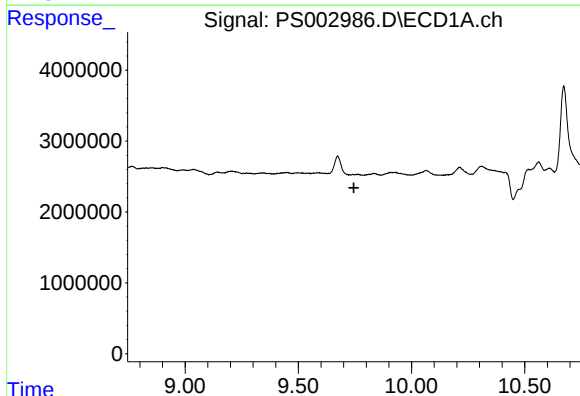


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

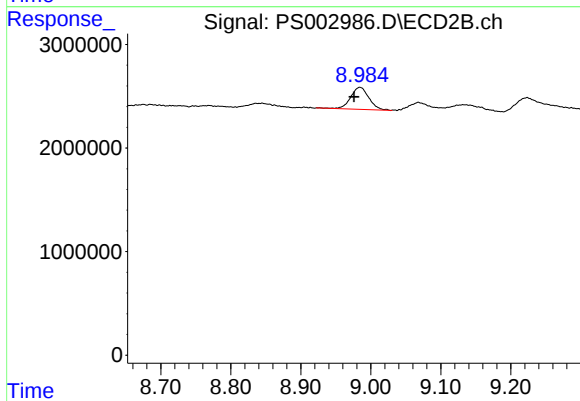

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.984 min
Delta R.T.: 0.008 min
Response: 3831660
Conc: 6.80 ng/ml

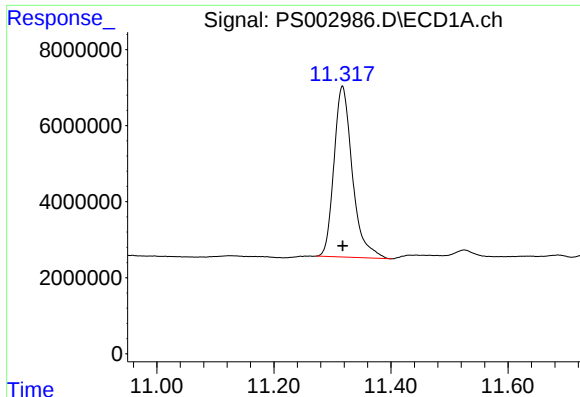

#4 2,4-DCAA


R.T.: 11.317 min
Delta R.T.: 0.000 min
Response: 97888804
Conc: 257.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

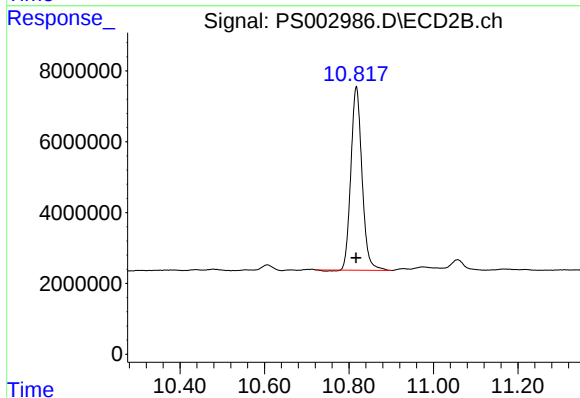


#4 2,4-DCAA

R.T.: 10.817 min
Delta R.T.: 0.000 min
Response: 94424421
Conc: 220.85 ng/ml

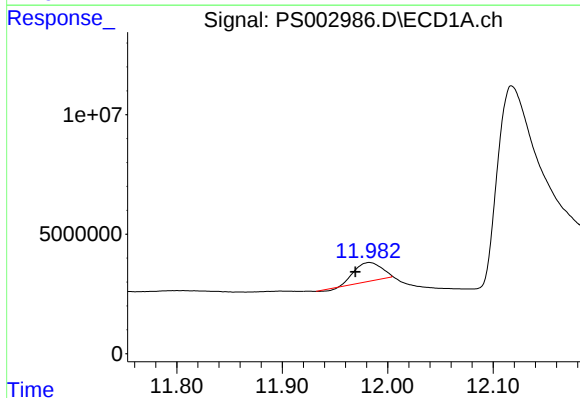


#6 MCP

R.T.: 11.983 min
Delta R.T.: 0.013 min
Response: 14881357
Conc: 12.42 ug/ml

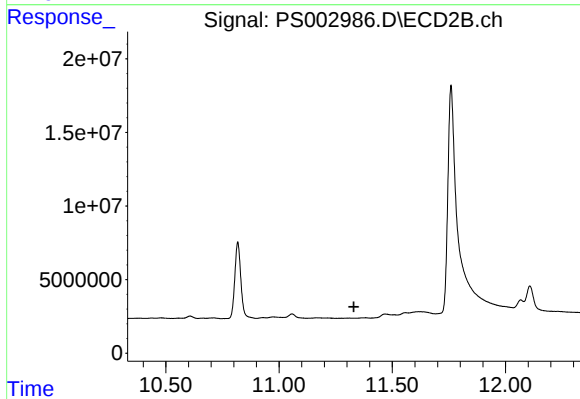

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

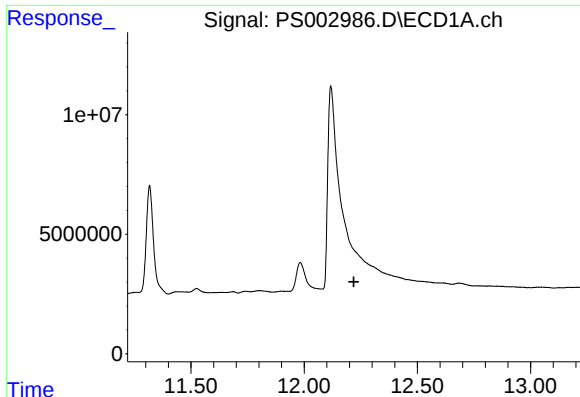

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

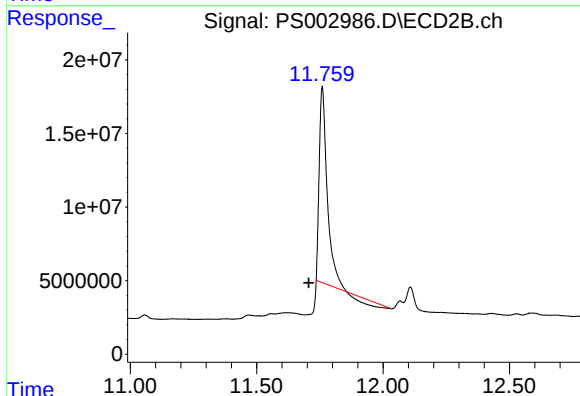


#7 MCPA

R.T.: 11.759 min
Delta R.T.: 0.053 min
Response: 274268195
Conc: 174.35 ug/ml

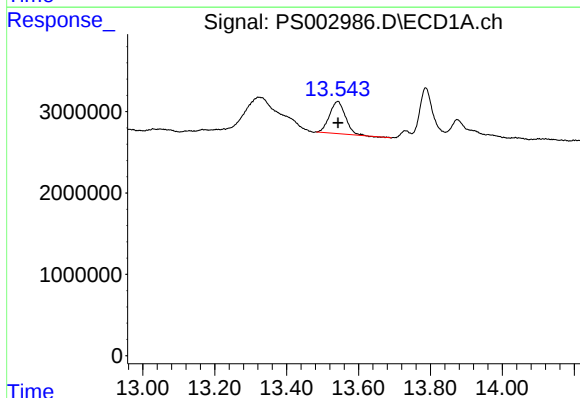


#10 Pentachlorophenol

R.T.: 13.541 min
Delta R.T.: -0.002 min
Response: 12026854
Conc: 1.88 ng/ml

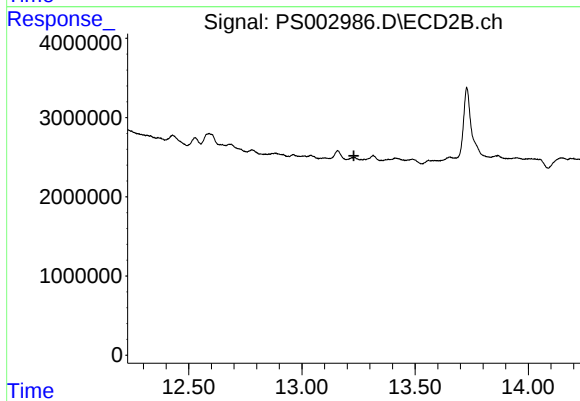

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.229 min
Response: 0
Conc: N.D.

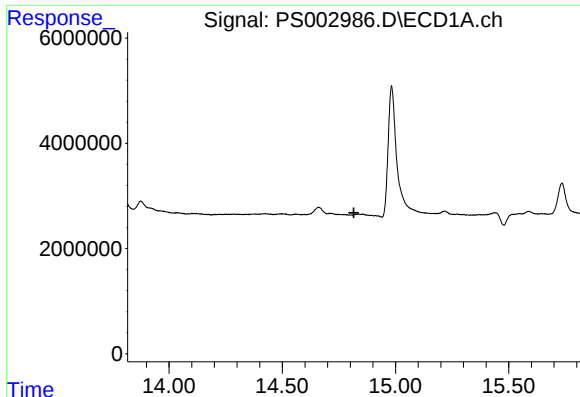

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

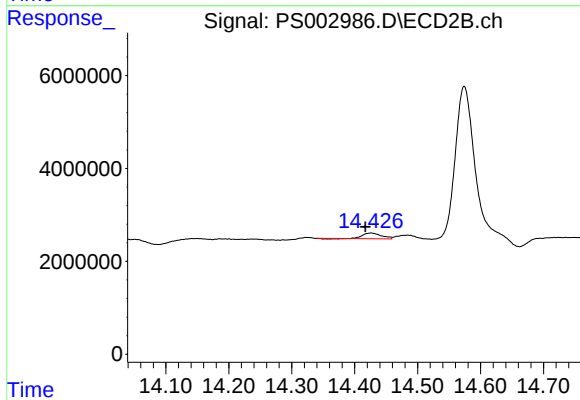


#12 2,4,5-T

R.T.: 14.426 min
Delta R.T.: 0.009 min
Response: 2561765
Conc: 1.34 ng/ml

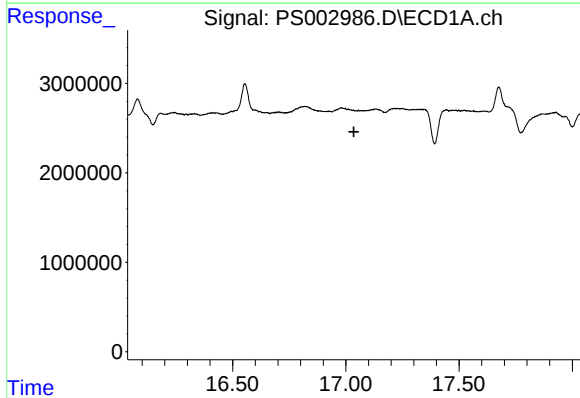


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

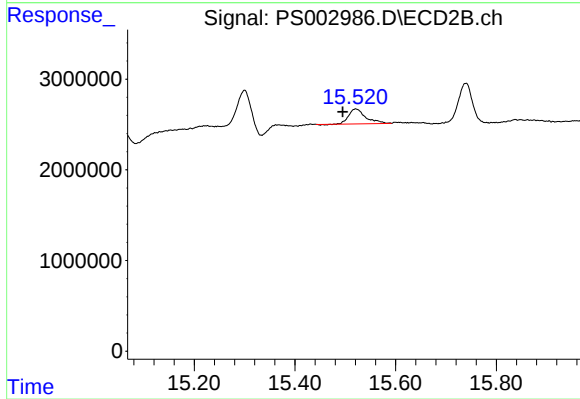

#14 DINOSEB


R.T.: 15.521 min
Delta R.T.: 0.026 min
Response: 3850563
Conc: 2.20 ng/ml

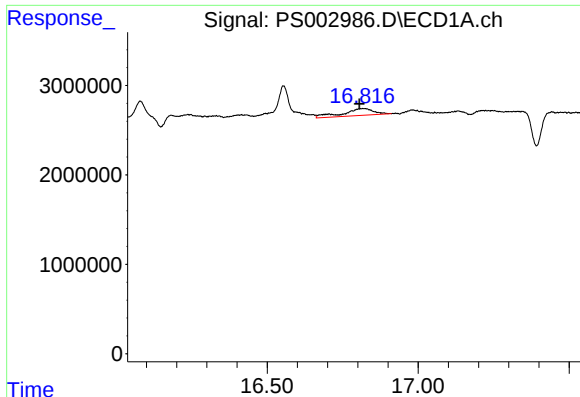

#15 Picloram


R.T.: 16.819 min
Delta R.T.: 0.013 min
Response: 5384483
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-A

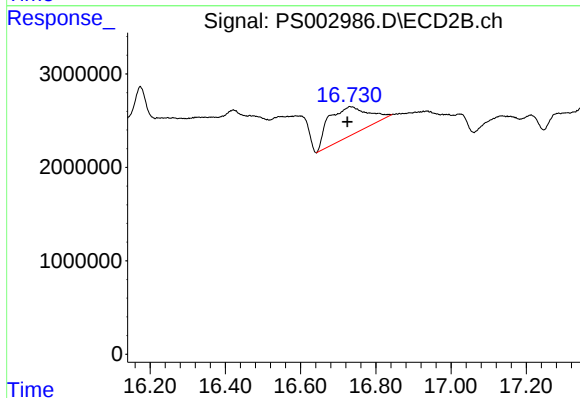


#15 Picloram

R.T.: 16.732 min
Delta R.T.: 0.008 min
Response: 22959757
Conc: 7.64 ng/ml

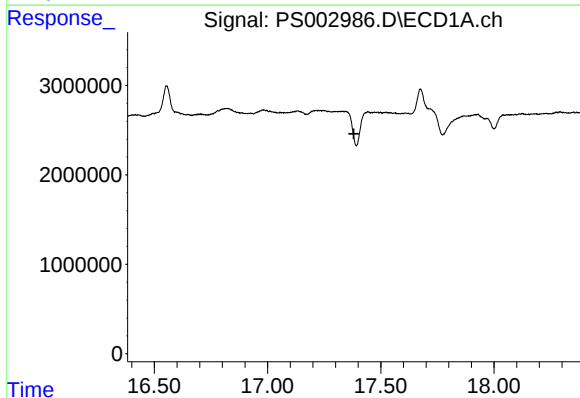

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

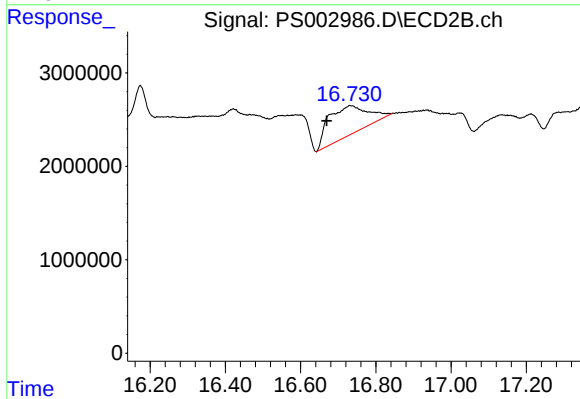

#16 DCPA

R.T.: 16.732 min
Delta R.T.: 0.063 min
Response: 22959757
Conc: 7.41 ng/ml