

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 21:52
 Operator : EI\SJ
 Sample : K1010-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-012819-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 02:45:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.795	71480538	99202360	188.285	232.027
Target Compounds							
1) T	Dalapon	0.000	2.300	0	115.6E6	N.D.	215.689 #
2) T	3,5-DICHL...	0.000	8.962	0	4276475	N.D.	7.588 #
6) T	MCP	11.958	0.000	29974367	0	25.018	N.D. #
8) T	DICHLORPROP	0.000	12.273	0	8713912	N.D.	22.791 #
12) T	2,4,5-T	0.000	14.403	0	2385234	N.D.	1.247 #
14) T	DINOSEB	0.000	15.499	0	3945324	N.D.	2.251 #
15) T	Picloram	16.785	16.710	4219689	24000781	1.334	7.983 #
16) T	DCPA	17.438	16.710	-8141829	24000781	N.D.	7.748



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 21:52
Operator : EI\SJ
Sample : K1010-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 02:45:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

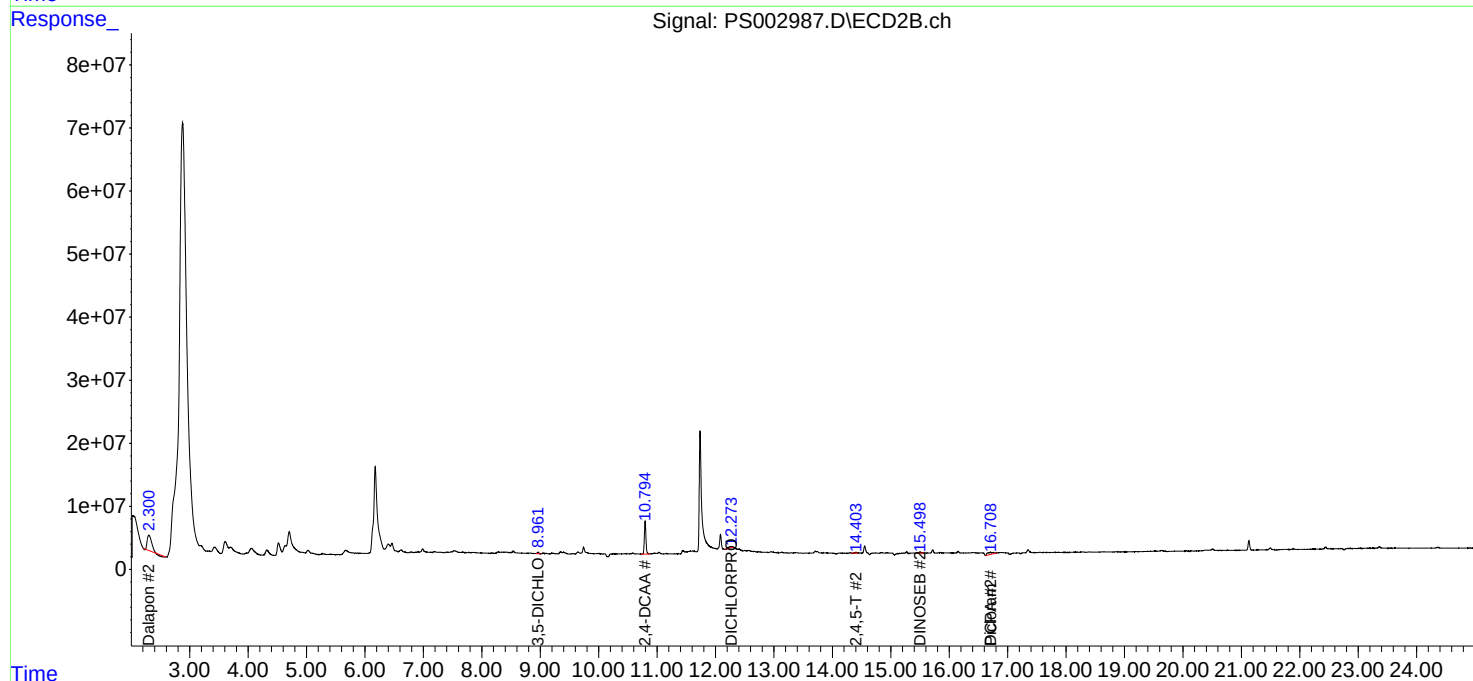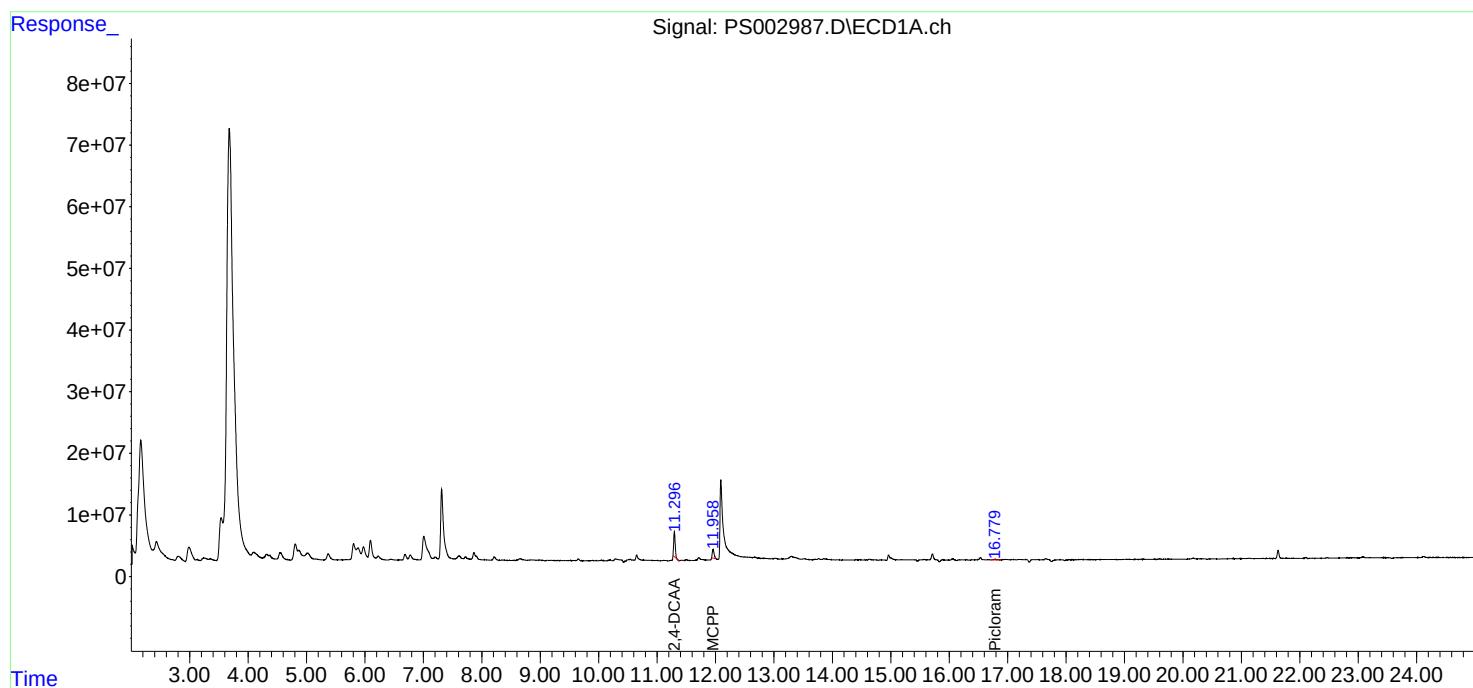


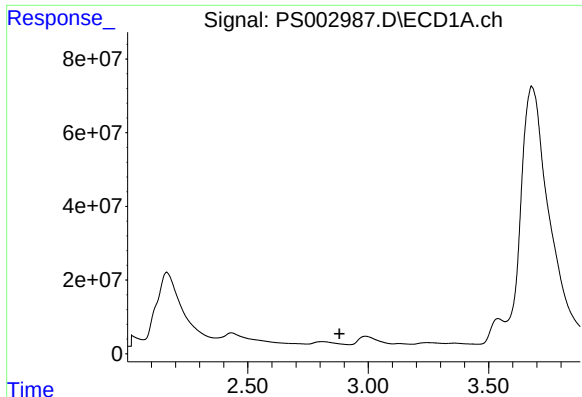

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

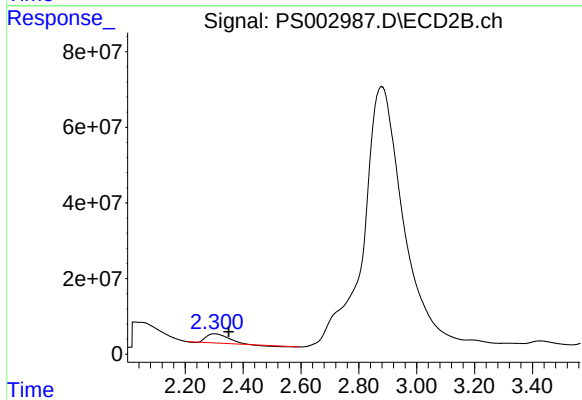


#1 Dalapon

R.T.: 2.300 min
Delta R.T.: -0.051 min
Response: 115592289
Conc: 215.69 ng/ml

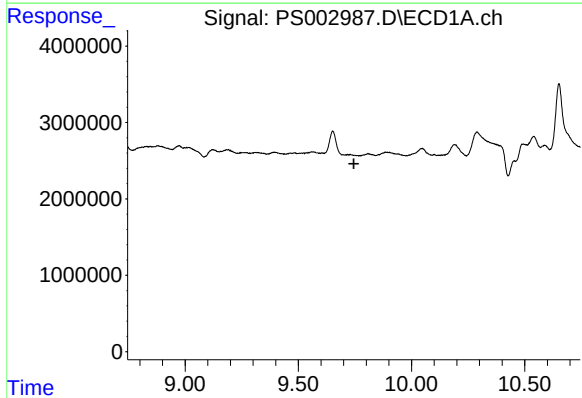


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

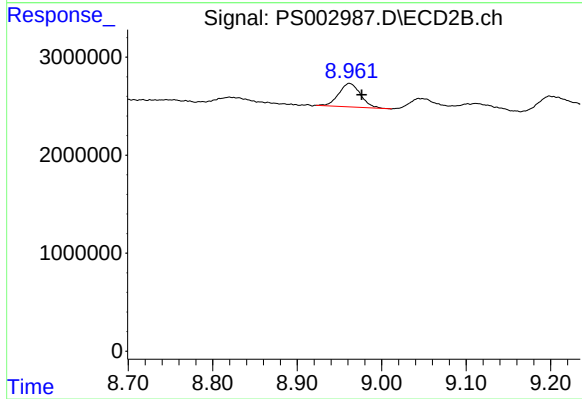

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: -0.014 min
Response: 4276475
Conc: 7.59 ng/ml

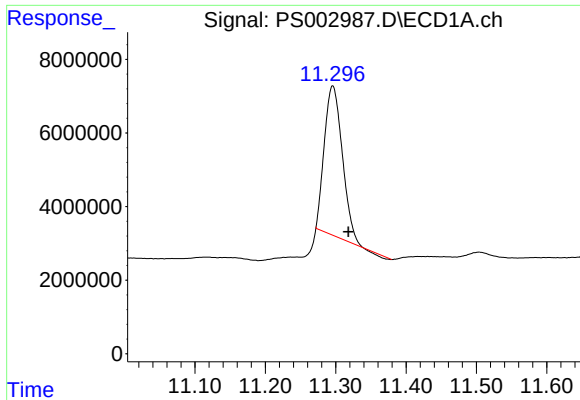

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 71480538
Conc: 188.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

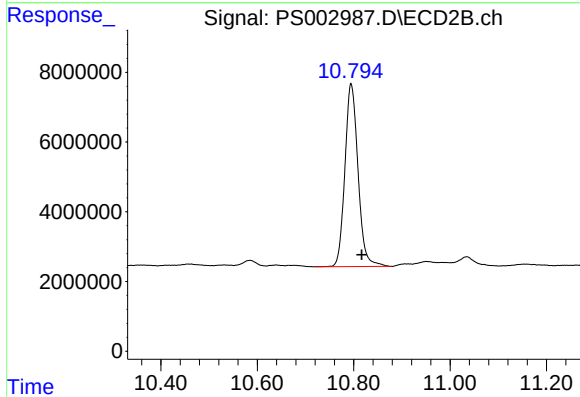


#4 2,4-DCAA

R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 99202360
Conc: 232.03 ng/ml

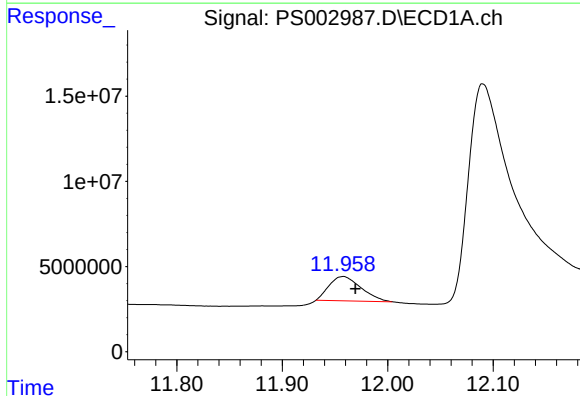


#6 MCP

R.T.: 11.958 min
Delta R.T.: -0.011 min
Response: 29974367
Conc: 25.02 ug/ml

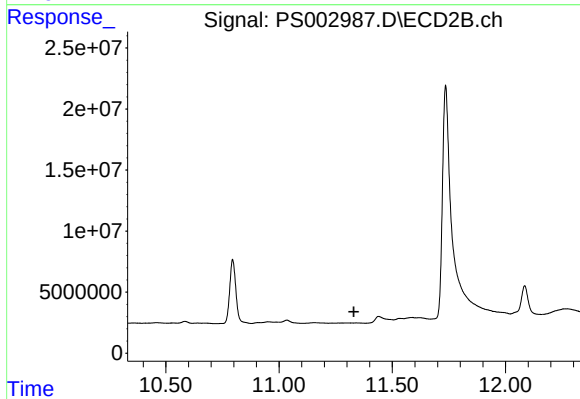

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

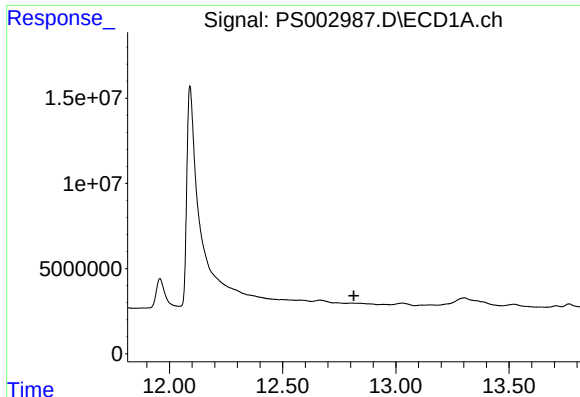

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

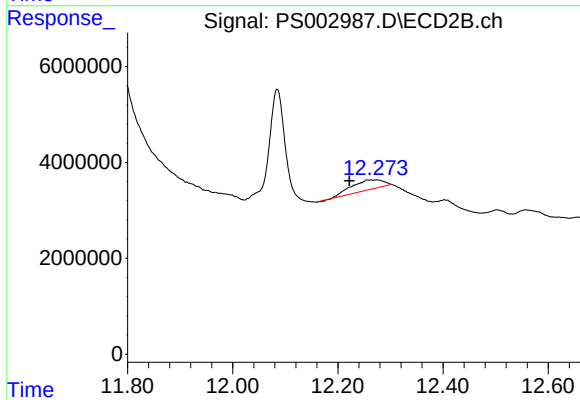


#8 DICHLORPROP

R.T.: 12.273 min
Delta R.T.: 0.051 min
Response: 8713912
Conc: 22.79 ng/ml

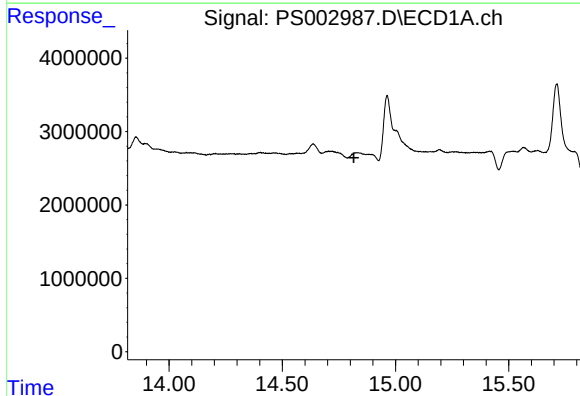


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

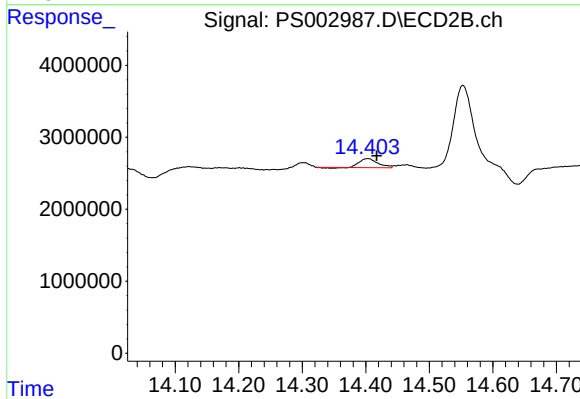

#12 2,4,5-T


R.T.: 14.403 min
Delta R.T.: -0.014 min
Response: 2385234
Conc: 1.25 ng/ml

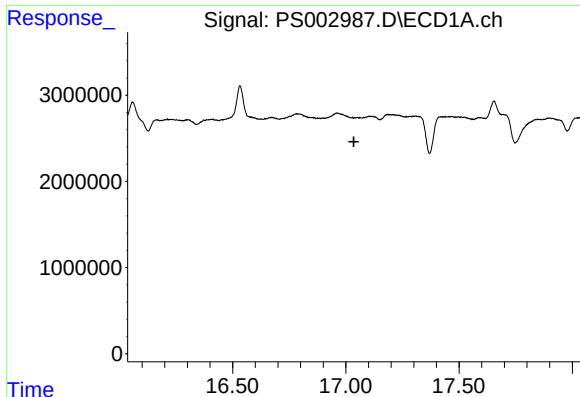

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

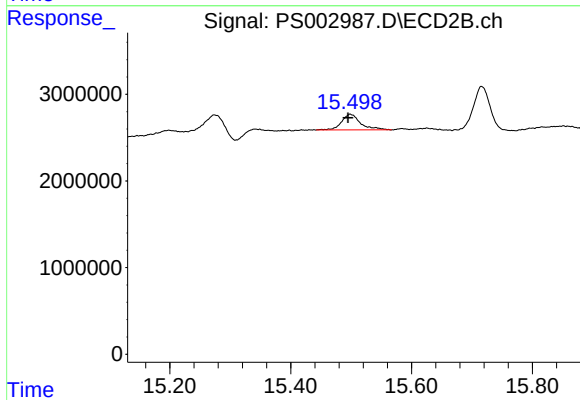


#14 DINOSEB

R.T.: 15.499 min
Delta R.T.: 0.004 min
Response: 3945324
Conc: 2.25 ng/ml

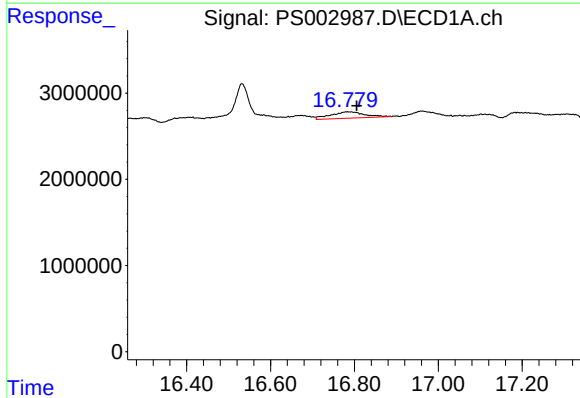


#15 Picloram

R.T.: 16.785 min
Delta R.T.: -0.020 min
Response: 4219689
Conc: 1.33 ng/ml

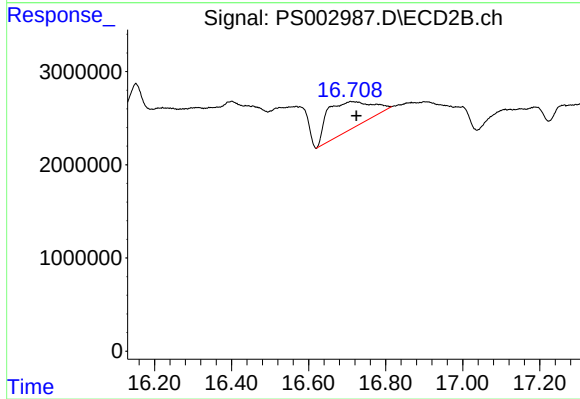

#15 Picloram


R.T.: 16.710 min
Delta R.T.: -0.014 min
Response: 24000781
Conc: 7.98 ng/ml

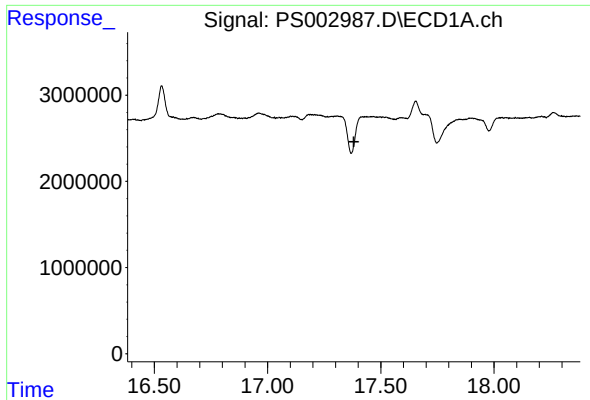

#16 DCPA

R.T.: 17.438 min
Delta R.T.: 0.056 min
Response: -8141829
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-012819-B

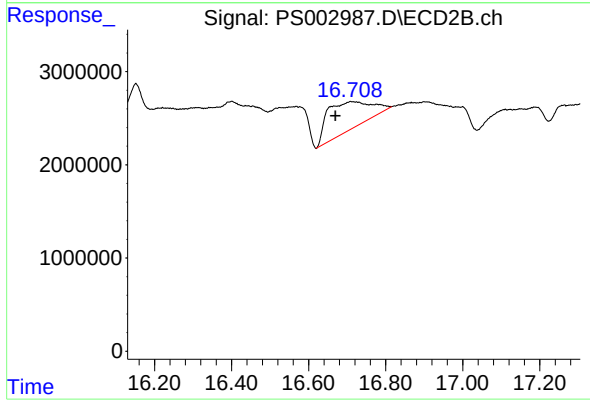

#16 DCPA

R.T.: 16.710 min
Delta R.T.: 0.041 min
Response: 24000781
Conc: 7.75 ng/ml