

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 22:54
 Operator : EI\SJ
 Sample : K1265-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OWS-3(OUTSIDE)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 02:46:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.782	0	108.7E6	N.D.	254.272 #
Target Compounds							
1) T	Dalapon	0.000	2.292	0	126.8E6	N.D.	236.694 #
2) T	3,5-DICHL...	0.000	8.949	0	2079743	N.D.	3.690 #
5) T	DICAMBA	0.000	11.123	0	3792161	N.D.	2.390 #
6) T	MCP	0.000	11.341	0	2248306	N.D.	2.038 #
7) T	MCPA	0.000	11.723	0	77645414	N.D.	49.359 #
8) T	DICHLORPROP	0.000	12.202	0	3556735	N.D.	9.303 #
10) T	Pentachlo...	13.509	0.000	3864915	0	0.603	N.D. #
11) T	2,4,5-TP ...	14.484	13.861	27707753	14645379	11.002	5.905 #
14) T	DINOSEB	0.000	15.487	0	3059749	N.D.	1.745 #
15) T	Picloram	0.000	16.701	0	20084414	N.D.	6.681 #
16) T	DCPA	17.437	16.701	-6022190	20084414	N.D.	6.484



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 22:54
Operator : EI\SJ
Sample : K1265-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
OWS-3(OUTSIDE)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 02:46:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

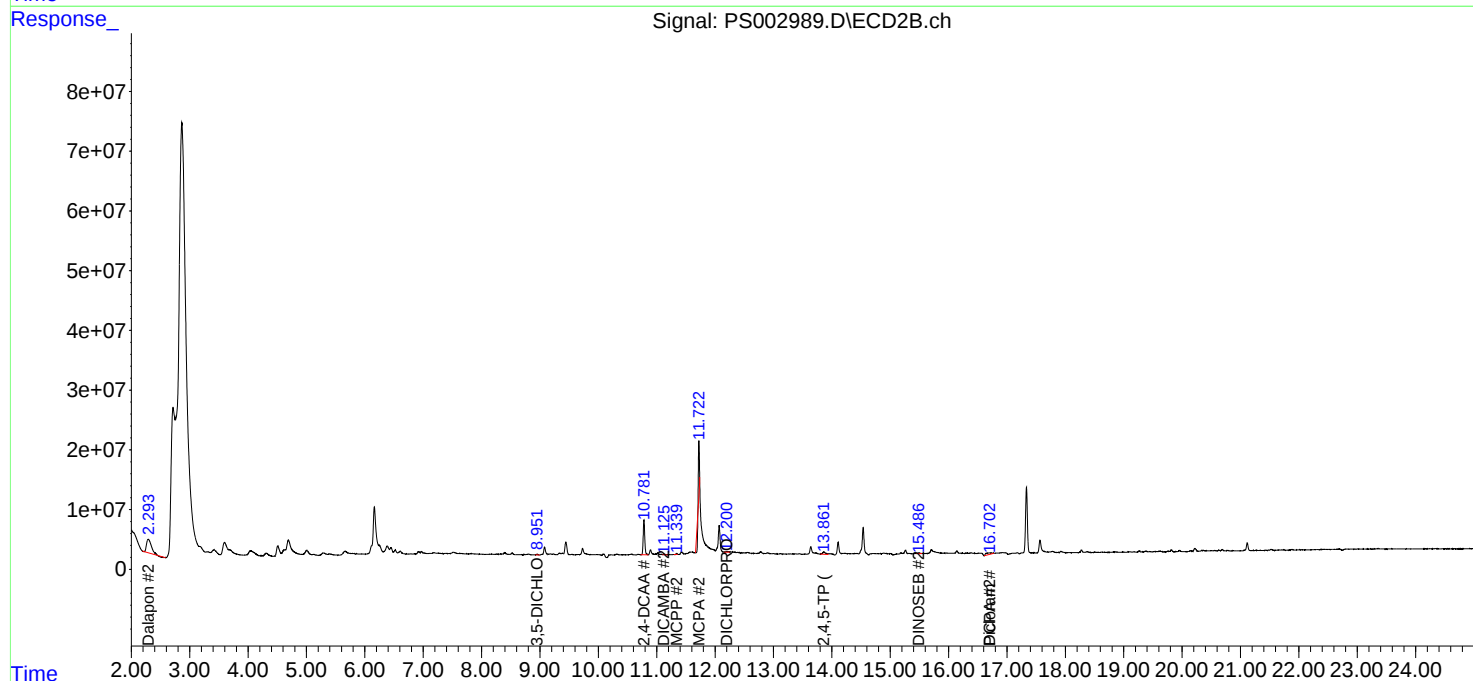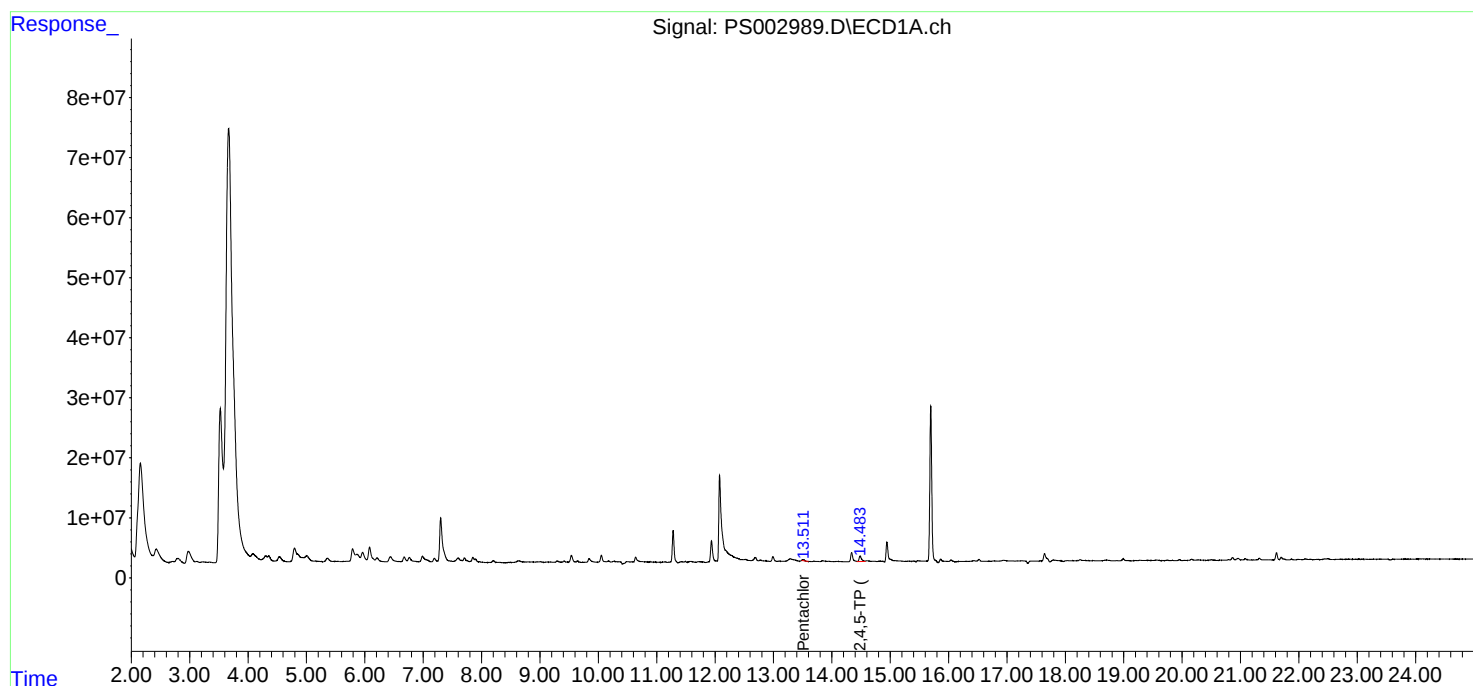


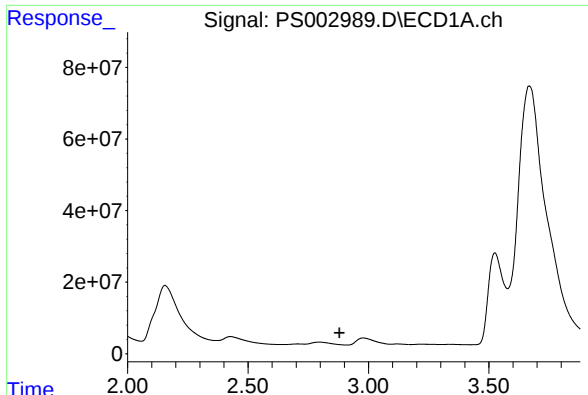

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

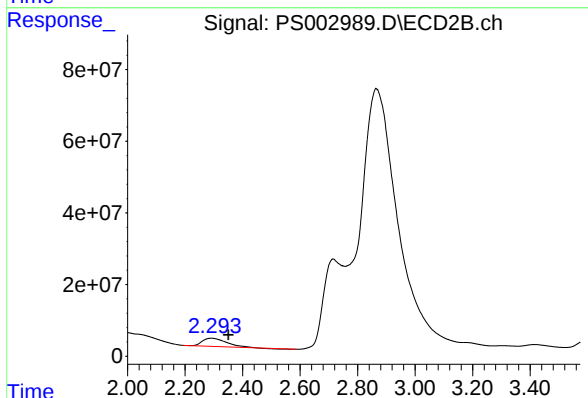


#1 Dalapon

R.T.: 2.292 min
Delta R.T.: -0.059 min
Response: 126849528
Conc: 236.69 ng/ml

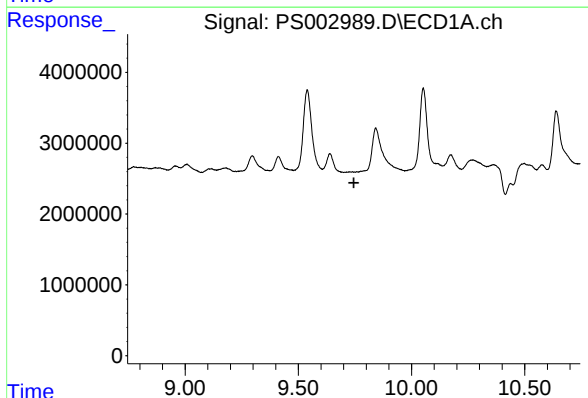


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

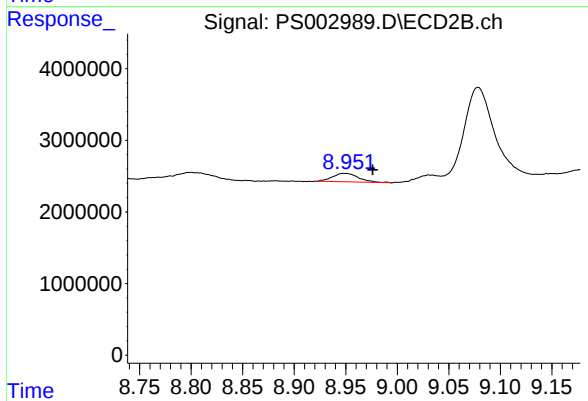

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: -0.027 min
Response: 2079743
Conc: 3.69 ng/ml

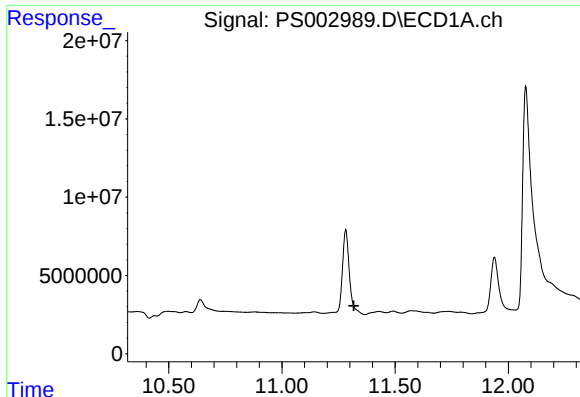

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

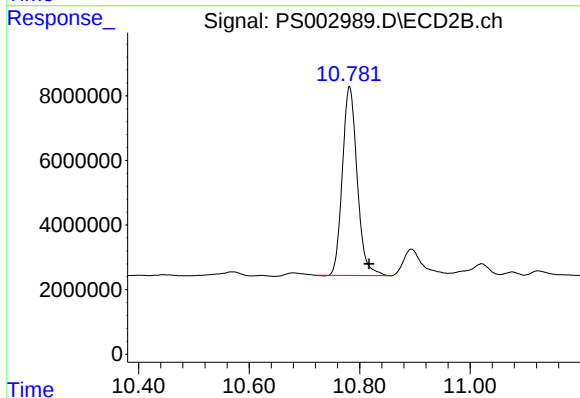


#4 2,4-DCAA

R.T.: 10.782 min
Delta R.T.: -0.035 min
Response: 108712992
Conc: 254.27 ng/ml

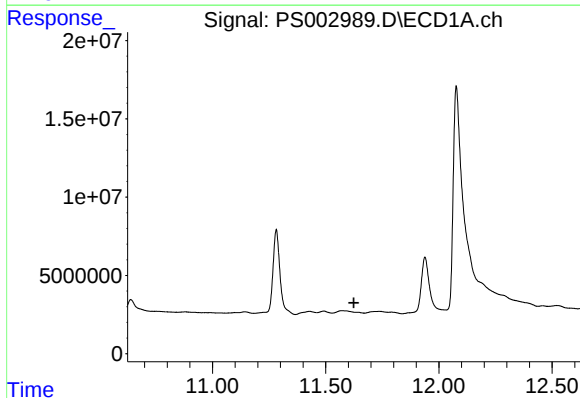


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

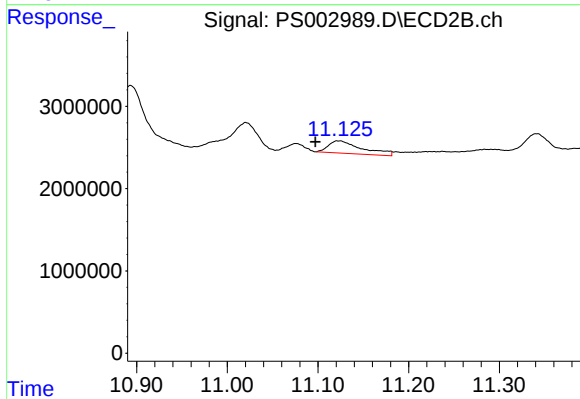

#5 DICAMBA


R.T.: 11.123 min
Delta R.T.: 0.026 min
Response: 3792161
Conc: 2.39 ng/ml

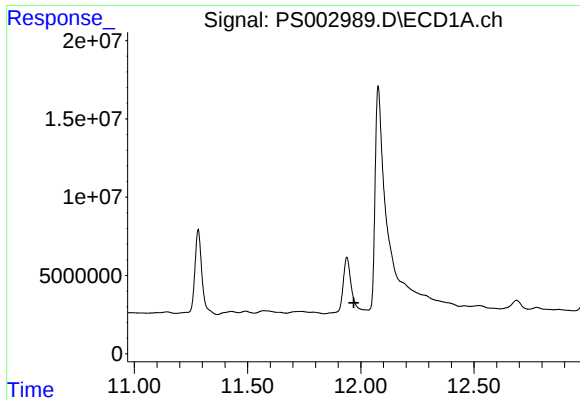

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

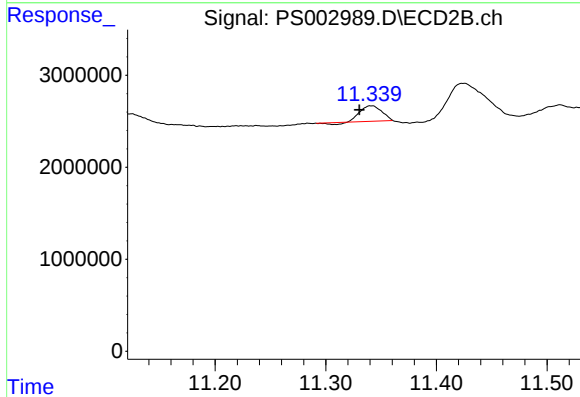


#6 MCPP

R.T.: 11.341 min
Delta R.T.: 0.011 min
Response: 2248306
Conc: 2.04 ug/ml

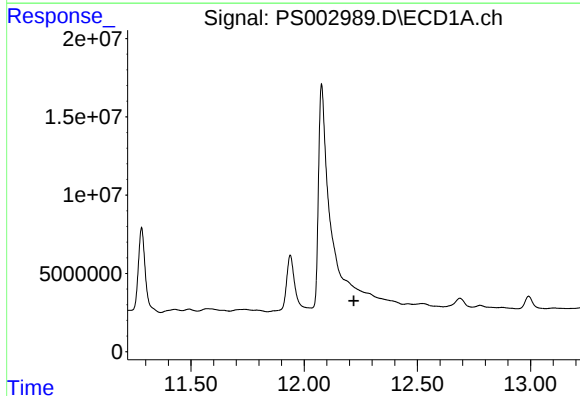


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

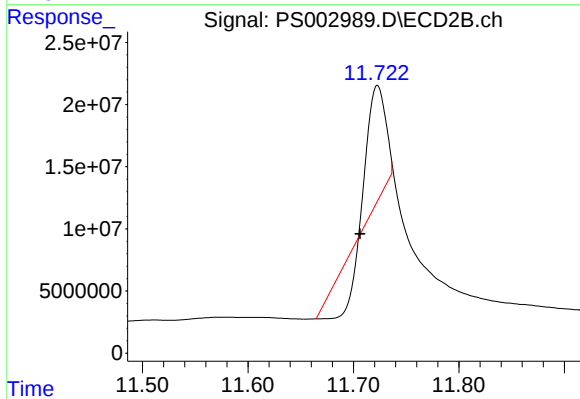

#7 MCPA


R.T.: 11.723 min
Delta R.T.: 0.017 min
Response: 77645414
Conc: 49.36 ug/ml

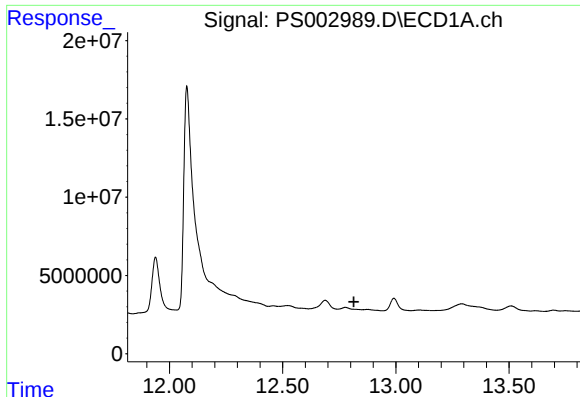

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

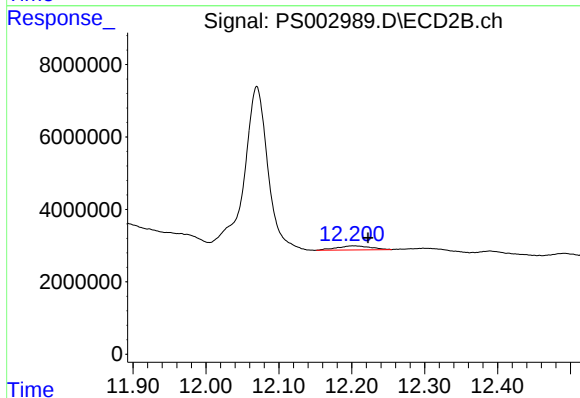


#8 DICHLORPROP

R.T.: 12.202 min
Delta R.T.: -0.020 min
Response: 3556735
Conc: 9.30 ng/ml

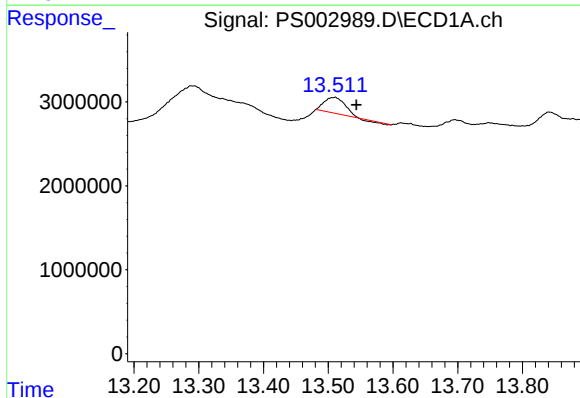


#10 Pentachlorophenol

R.T.: 13.509 min
Delta R.T.: -0.034 min
Response: 3864915
Conc: 0.60 ng/ml

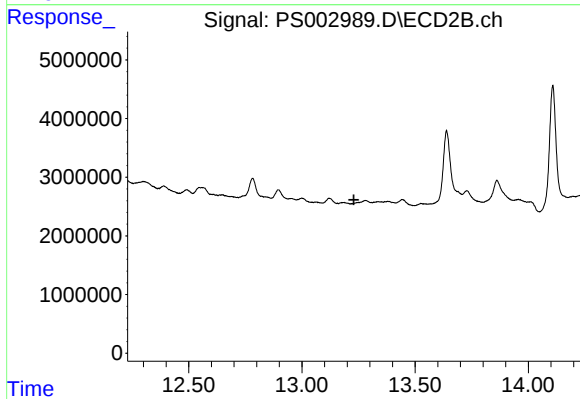

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.229 min
Response: 0
Conc: N.D.

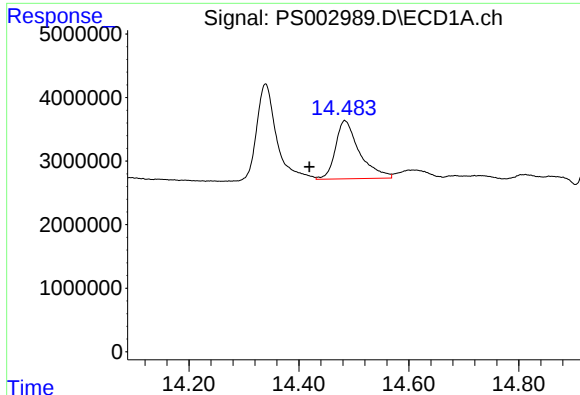

#11 2,4,5-TP (SILVEX)


R.T.: 14.484 min
Delta R.T.: 0.064 min
Response: 27707753
Conc: 11.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

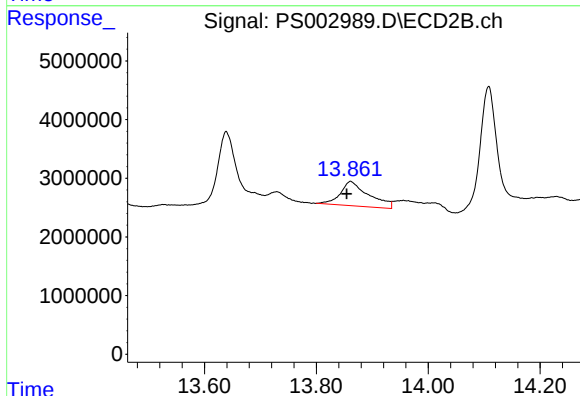


#11 2,4,5-TP (SILVEX)

R.T.: 13.861 min
Delta R.T.: 0.007 min
Response: 14645379
Conc: 5.90 ng/ml

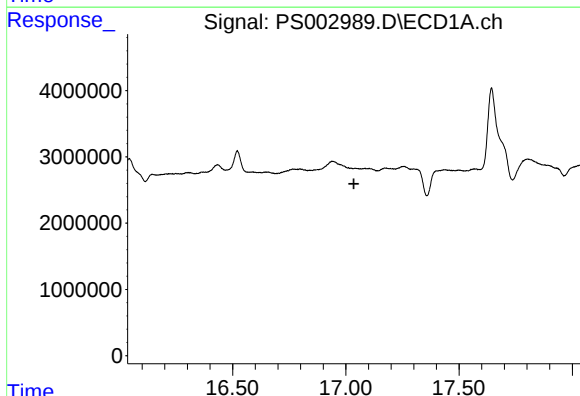


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

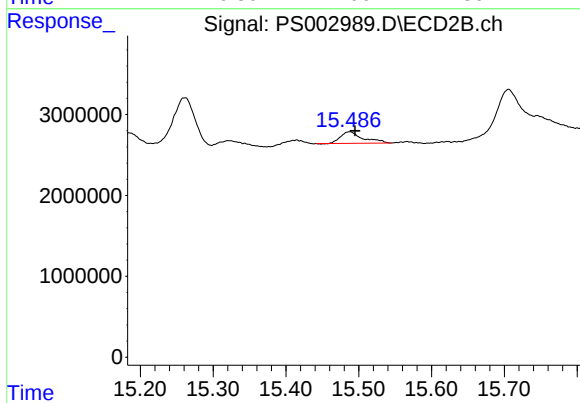

#14 DINOSEB


R.T.: 15.487 min
Delta R.T.: -0.008 min
Response: 3059749
Conc: 1.75 ng/ml

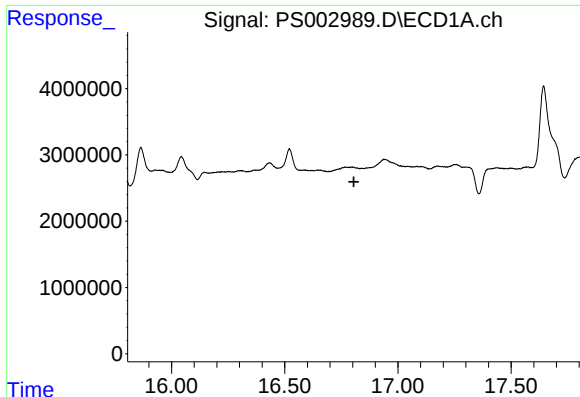

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OWS-3(OUTSIDE)

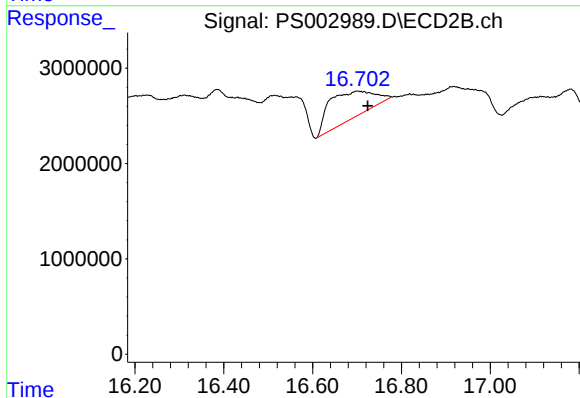


#15 Picloram

R.T.: 16.701 min
Delta R.T.: -0.023 min
Response: 20084414
Conc: 6.68 ng/ml

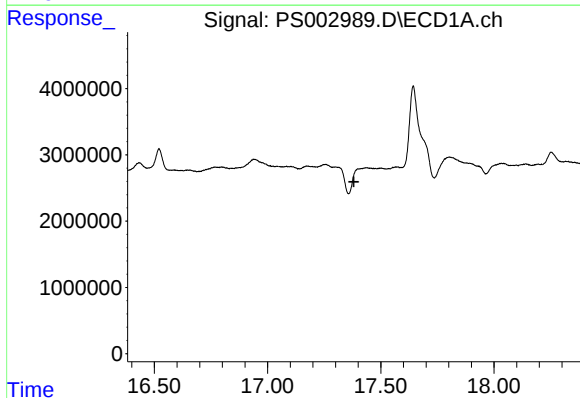

#16 DCPA

R.T.: 17.437 min
Delta R.T.: 0.055 min
Response: -6022190
Conc: N.D.

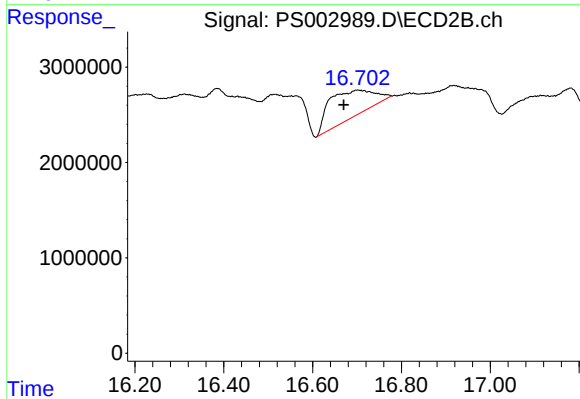

#16 DCPA

R.T.: 16.701 min
Delta R.T.: 0.032 min
Response: 20084414
Conc: 6.48 ng/ml