

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
 Data File : PS002991.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2019 23:57
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:52:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.780	0	317.8E6	N.D.	743.274 #
Target Compounds							
1) T	Dalapon	2.845	2.314	121.1E6	358.0E6	219.446	668.082 #
3) T	4-Nitroph...	0.000	9.928	0	151.2E6	N.D.	723.345 #
5) T	DICAMBA	11.586	11.060	77208055	339.0E6	48.168	213.654 #
8) T	DICHLORPROP	0.000	12.186	0	275.2E6	N.D.	719.743 #
9) T	2,4-D	0.000	12.656	0	251.4E6	N.D.	501.432 #
10) T	Pentachlo...	13.505	0.000	1011.3E6	0	157.702	N.D. #
11) T	2,4,5-TP ...	14.381	13.818	1867.6E6	1766.3E6	741.602	712.130
12) T	2,4,5-T	14.778	14.380	1827.4E6	616.2E6	749.130	322.028 #
14) T	DINOSEB	16.997	0.000	1374.5E6	0	730.614	N.D. #
15) T	Picloram	16.767	16.687	2401.9E6	2287.7E6	759.232	760.935
16) T	DCPA	17.343	16.687	907.8E6	2287.7E6	301.877	738.535 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012919\
Data File : PS002991.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2019 23:57
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:52:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

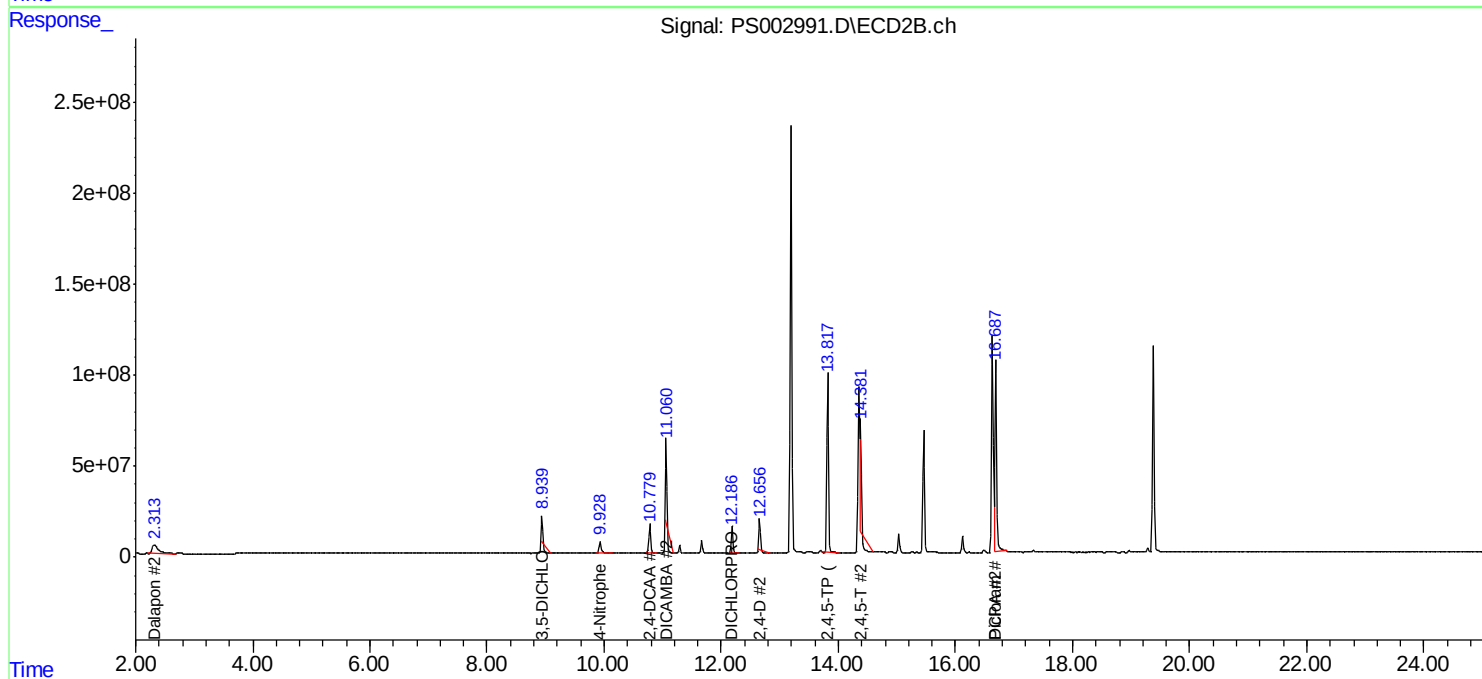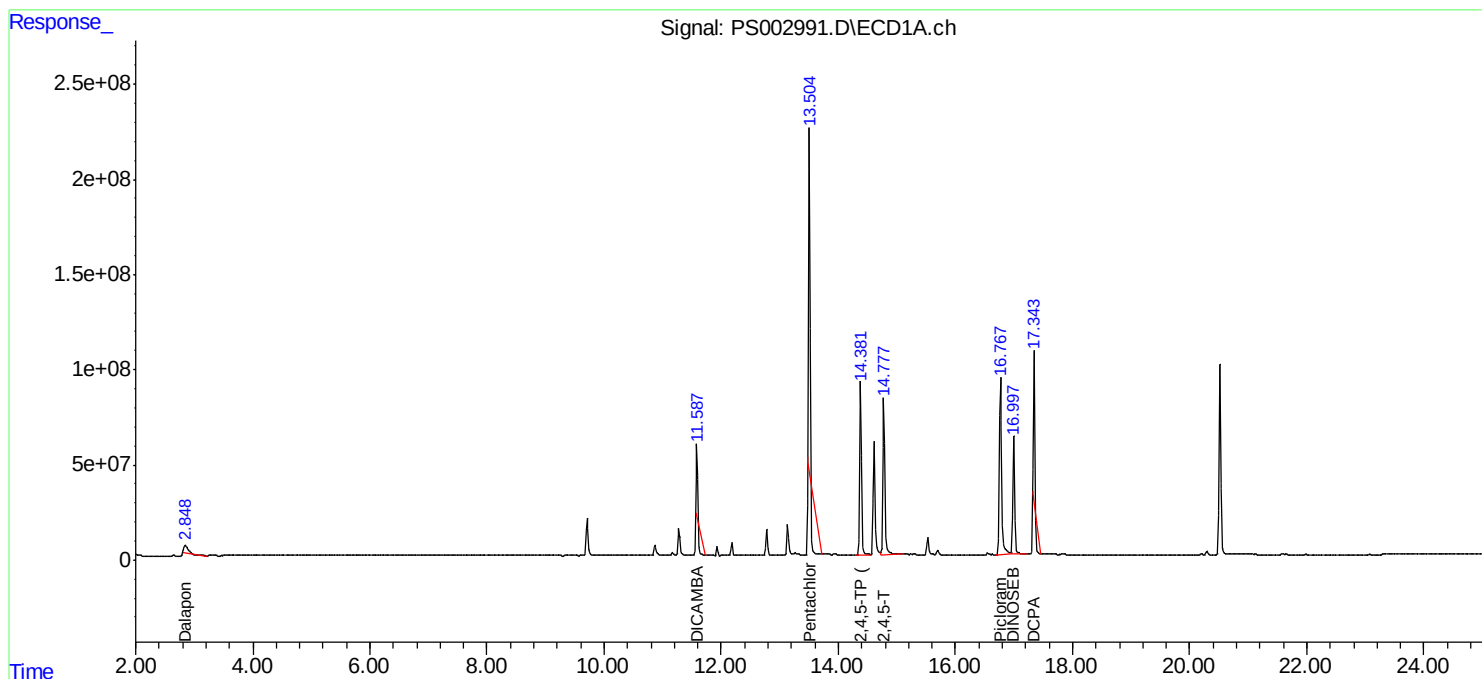


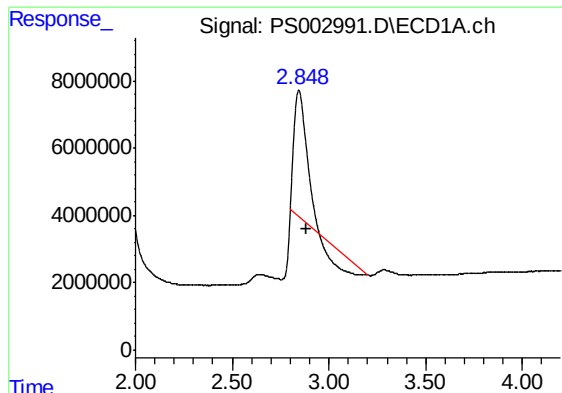

#1 Dalapon


R.T.: 2.845 min
Delta R.T.: -0.035 min
Response: 121056980
Conc: 219.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

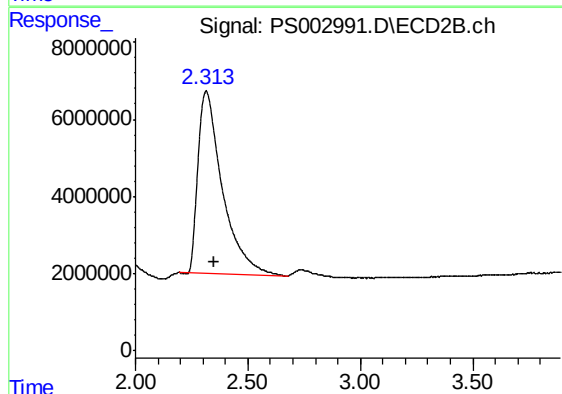


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.037 min
Response: 358039670
Conc: 668.08 ng/ml

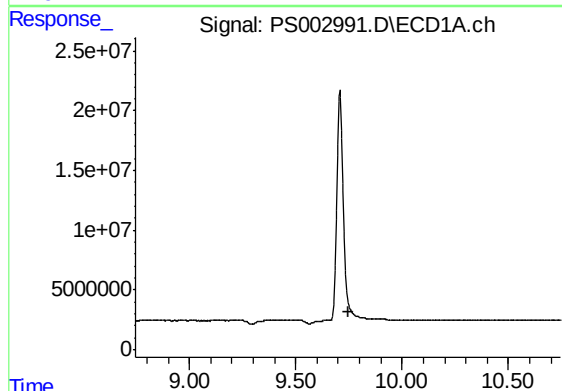


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.707 min
Delta R.T.: -0.038 min
Response: -217534208
Conc: N.D.

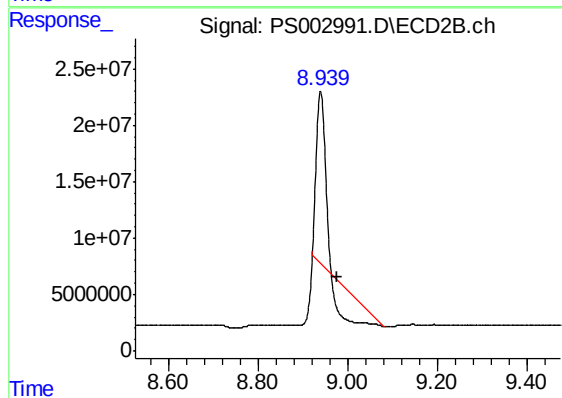

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: -0.037 min
Response: 83685058
Conc: 148.49 ng/ml

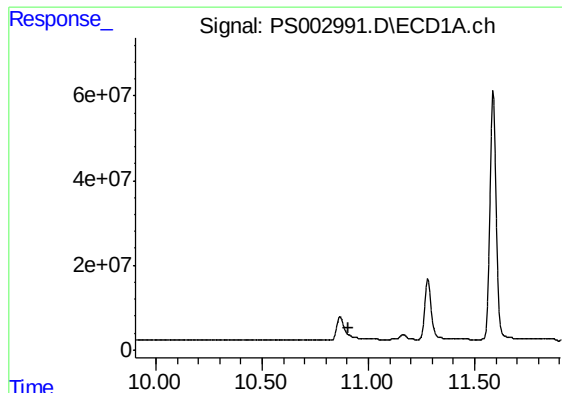

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

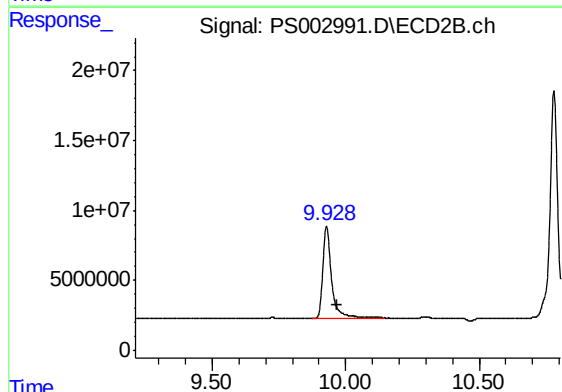


#3 4-Nitrophenol

R.T.: 9.928 min
Delta R.T.: -0.037 min
Response: 151195340
Conc: 723.34 ng/ml

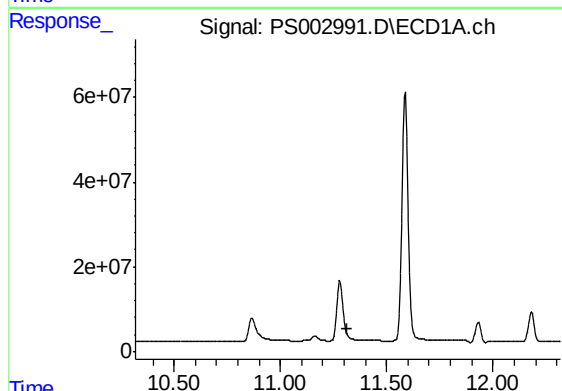


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

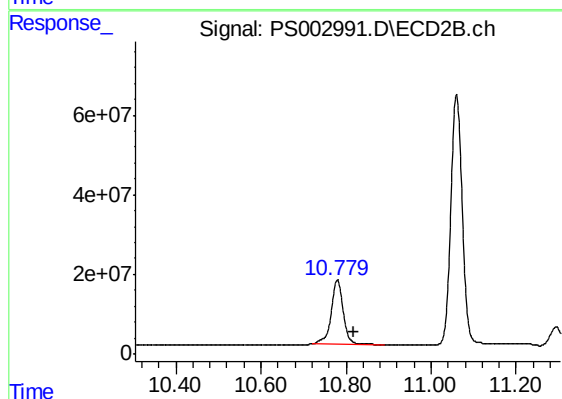

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 317783550
Conc: 743.27 ng/ml

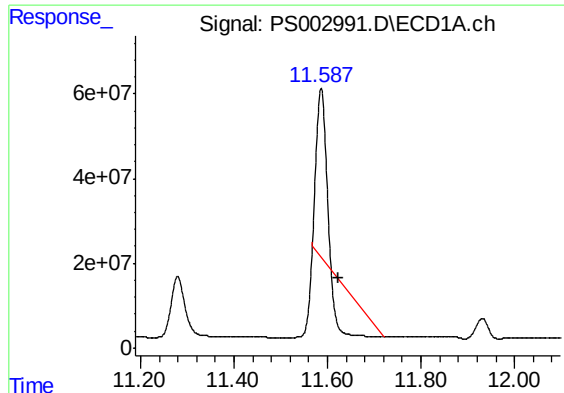

#5 DICAMBA


R.T.: 11.586 min
Delta R.T.: -0.038 min
Response: 77208055
Conc: 48.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

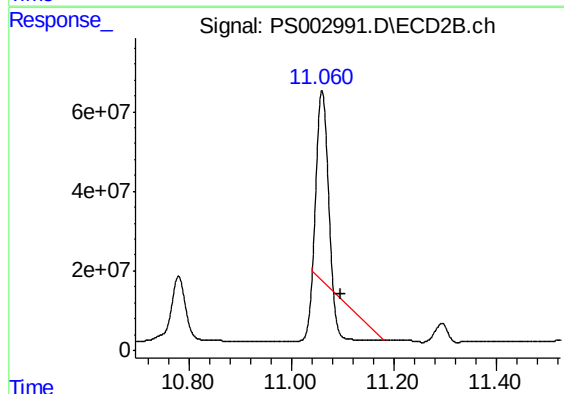


#5 DICAMBA

R.T.: 11.060 min
Delta R.T.: -0.037 min
Response: 338996856
Conc: 213.65 ng/ml

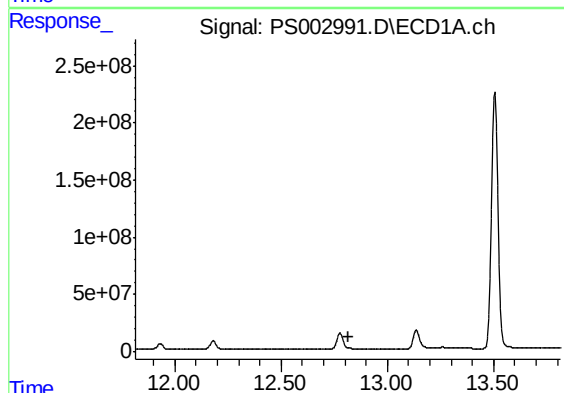


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.815 min
Response: 0
Conc: N.D.

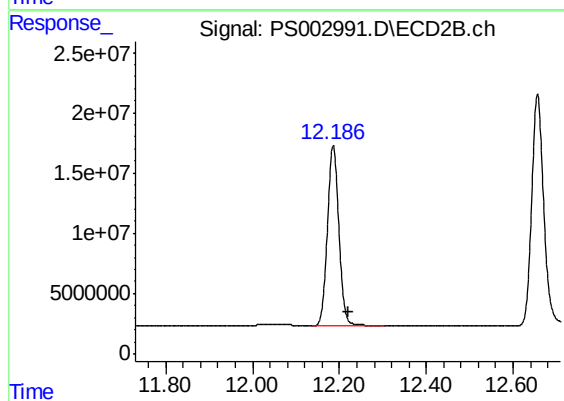

#8 DICHLORPROP


R.T.: 12.186 min
Delta R.T.: -0.037 min
Response: 275187486
Conc: 719.74 ng/ml

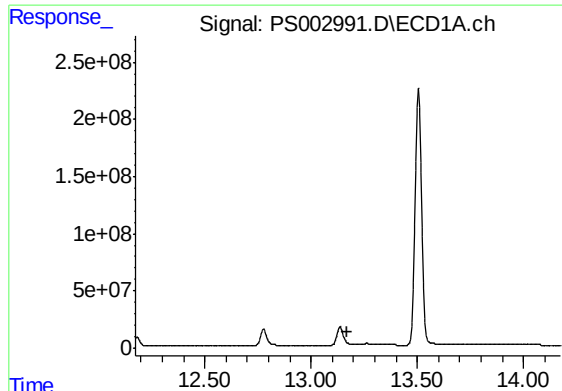

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

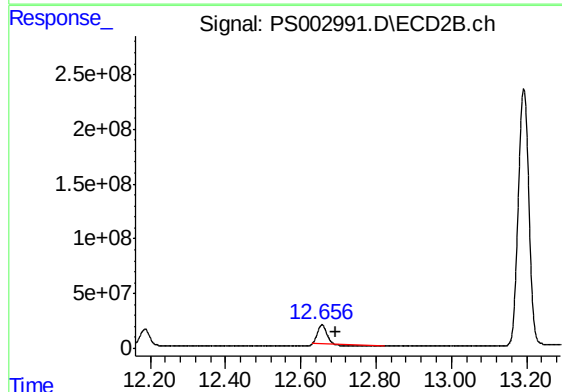


#9 2,4-D

R.T.: 12.656 min
Delta R.T.: -0.037 min
Response: 251411026
Conc: 501.43 ng/ml

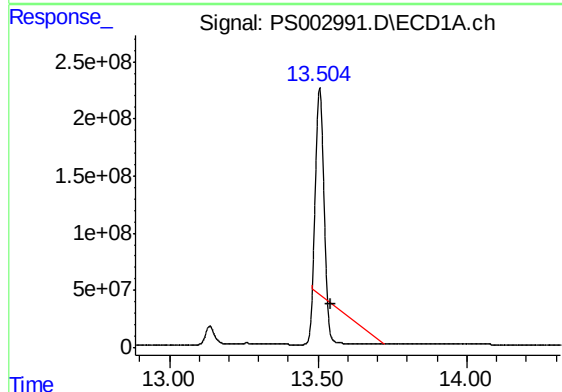


#10 Pentachlorophenol

R.T.: 13.505 min
Delta R.T.: -0.038 min
Response: 1011340923
Conc: 157.70 ng/ml

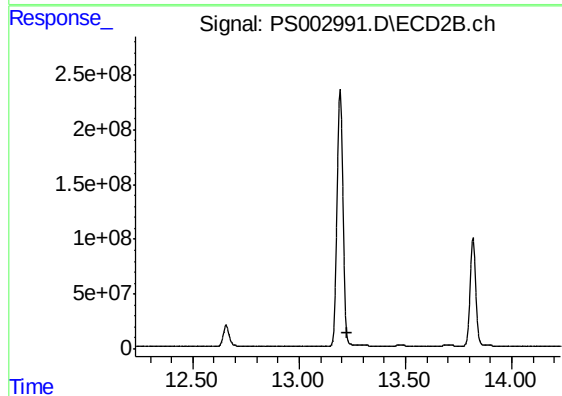

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.229 min
Response: 0
Conc: N.D.

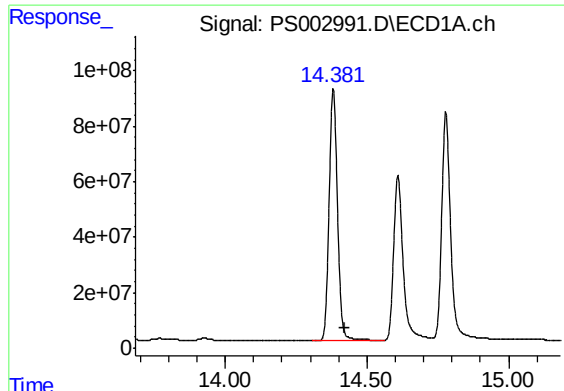

#11 2,4,5-TP (SILVEX)


R.T.: 14.381 min
Delta R.T.: -0.038 min
Response: 1867631627
Conc: 741.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

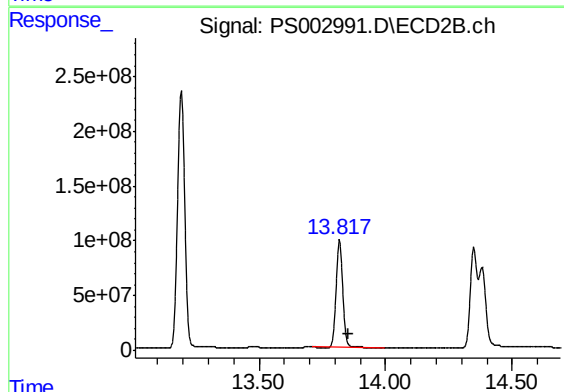


#11 2,4,5-TP (SILVEX)

R.T.: 13.818 min
Delta R.T.: -0.037 min
Response: 1766335019
Conc: 712.13 ng/ml

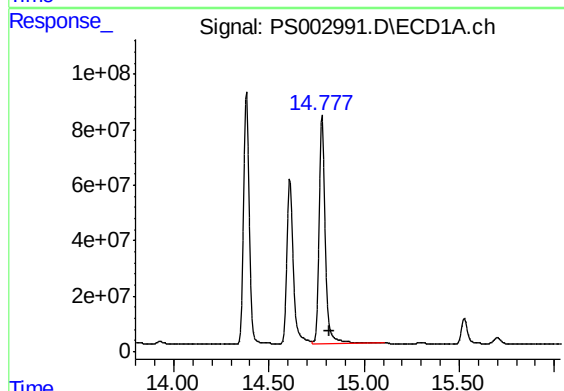


#12 2,4,5-T

R.T.: 14.778 min
Delta R.T.: -0.038 min
Response: 1827432291
Conc: 749.13 ng/ml

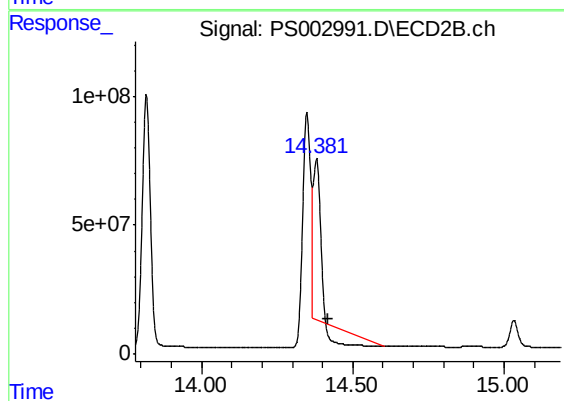

#12 2,4,5-T


R.T.: 14.380 min
Delta R.T.: -0.037 min
Response: 616197132
Conc: 322.03 ng/ml

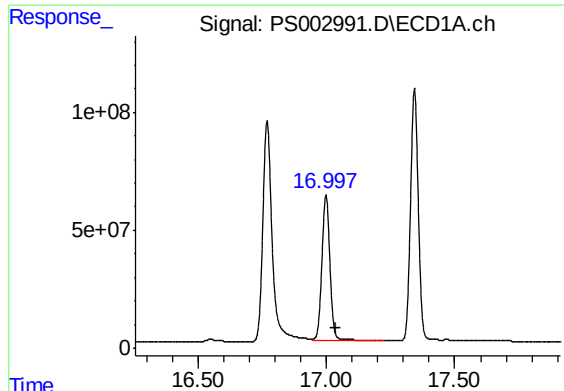

#14 DINOSEB


R.T.: 16.997 min
Delta R.T.: -0.038 min
Response: 1374525080
Conc: 730.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

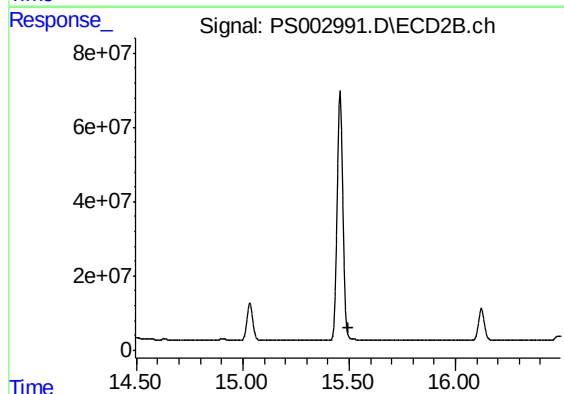


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

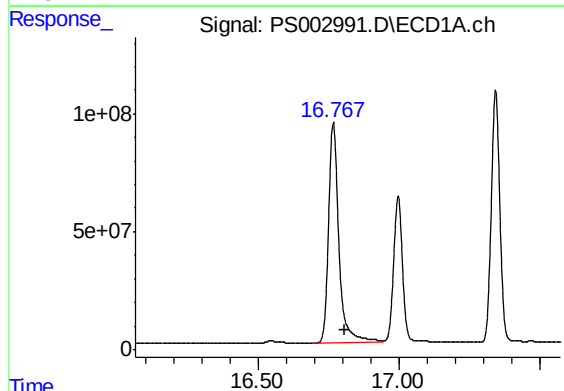


#15 Picloram

R.T.: 16.767 min
Delta R.T.: -0.039 min
Response: 2401930704
Conc: 759.23 ng/ml

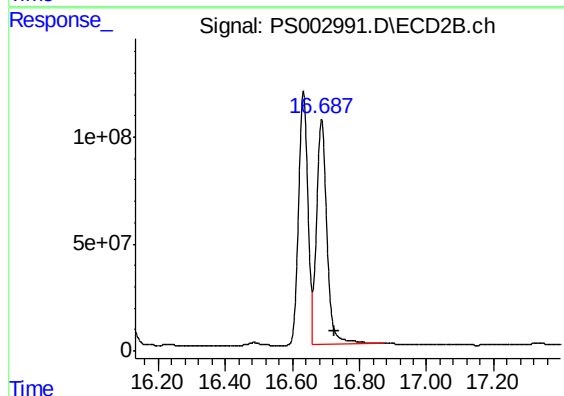

#15 Picloram


R.T.: 16.687 min
Delta R.T.: -0.037 min
Response: 2287676241
Conc: 760.93 ng/ml

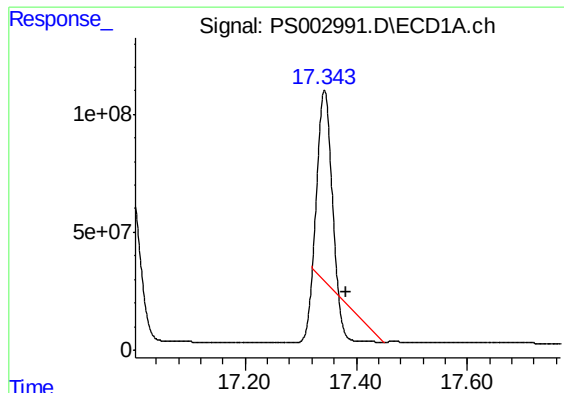

#16 DCPA

R.T.: 17.343 min
Delta R.T.: -0.039 min
Response: 907832481
Conc: 301.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

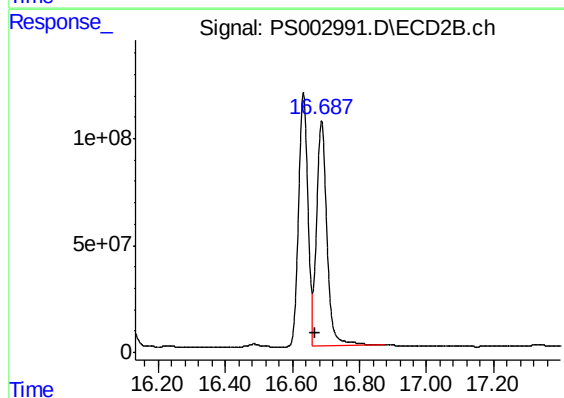

#16 DCPA

R.T.: 16.687 min
Delta R.T.: 0.017 min
Response: 2287676241
Conc: 738.53 ng/ml