

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS012920\  
 Data File : PS008615.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 Jan 2020 18:04  
 Operator : DD\AJ  
 Sample : PB126435BL  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB126435BL

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 30 00:47:02 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010820.M  
 Quant Title : 8080.M  
 QLast Update : Wed Jan 08 11:00:59 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|----------|----------|---------|---------|
| -----                       |              |        |        |          |          |         |         |
| System Monitoring Compounds |              |        |        |          |          |         |         |
| 4) S                        | 2,4-DCAA     | 6.284  | 5.979  | 982.3E6  | 523.4E6  | 556.321 | 552.430 |
| Target Compounds            |              |        |        |          |          |         |         |
| 1) T                        | Dalapon      | 2.517  | 2.201  | 121.1E6  | 60374982 | 47.217  | 47.624  |
| 2) T                        | 3,5-DICHL... | 0.000  | 5.166  | 0        | 62639632 | N.D.    | 44.833  |
| 7) T                        | MCPA         | 6.832  | 6.443  | 73842896 | 43106627 | 10.105  | 10.096  |
| 8) T                        | DICHLORPROP  | 0.000  | 6.799  | 0        | 40752351 | N.D.    | 42.180  |
| 9) T                        | 2,4-D        | 0.000  | 7.046  | 0        | 15499979 | N.D.    | 13.222  |
| 10) T                       | Pentachlo... | 7.767  | 0.000  | 50211045 | 0        | 2.065   | N.D. #  |
| 11) T                       | 2,4,5-TP ... | 0.000  | 7.830  | 0        | 51886669 | N.D.    | 9.927   |
| 12) T                       | 2,4,5-T      | 8.490  | 0.000  | 69830168 | 0        | 7.568   | N.D. #  |
| 14) T                       | DINOSEB      | 10.225 | 9.095  | 40089333 | 9332621  | 5.587   | 2.470 # |
| 15) T                       | Picloram     | 0.000  | 10.063 | 0        | 28828815 | N.D.    | 3.880   |
| 16) T                       | DCPA         | 0.000  | 10.063 | 0        | 28828815 | N.D.    | 4.424   |
| -----                       |              |        |        |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS012920\  
Data File : PS008615.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Jan 2020 18:04  
Operator : DD\AJ  
Sample : PB126435BL  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 30 00:47:02 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010820.M  
Quant Title : 8080.M  
QLast Update : Wed Jan 08 11:00:59 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

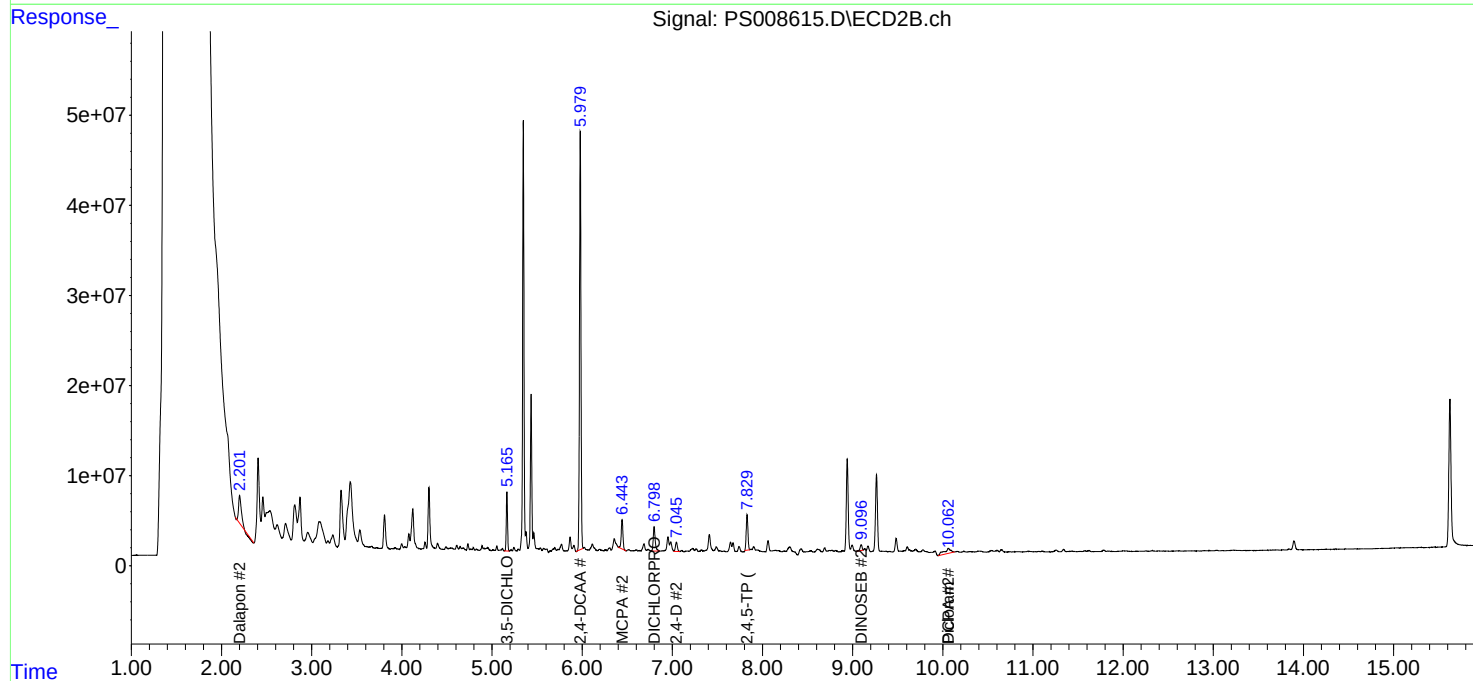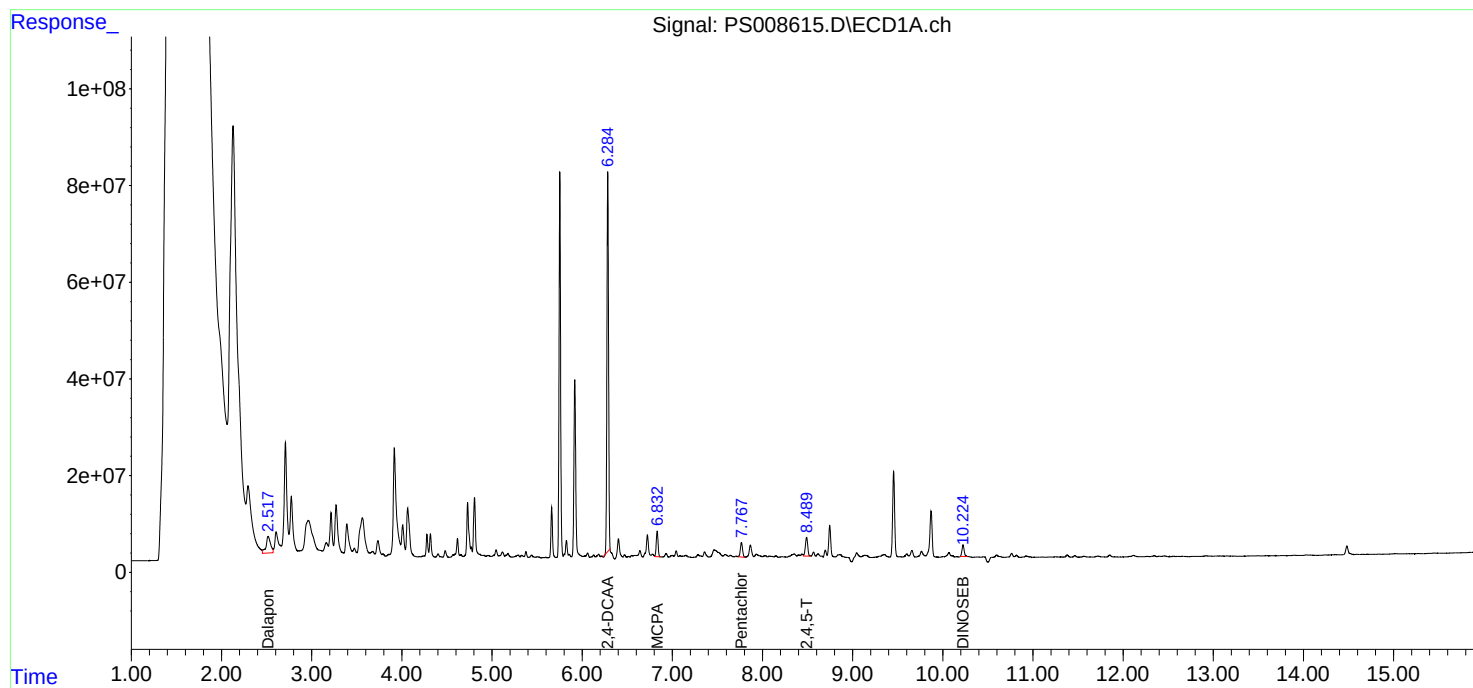


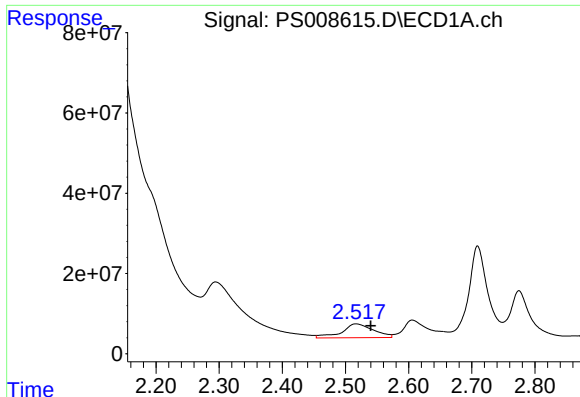

#1 Dalapon


R.T.: 2.517 min  
Delta R.T.: -0.023 min  
Response: 121058118  
Conc: 47.22 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

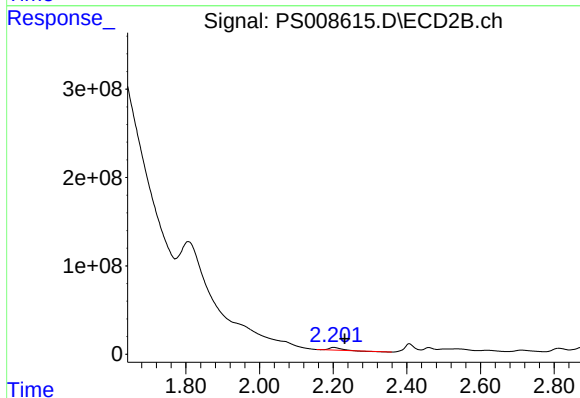


#1 Dalapon

R.T.: 2.201 min  
Delta R.T.: -0.030 min  
Response: 60374982  
Conc: 47.62 ng/ml

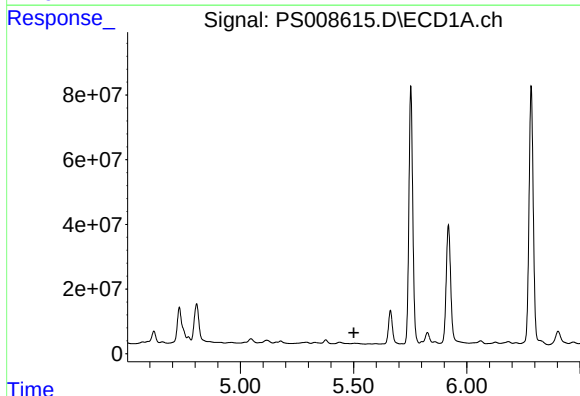


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 5.501 min  
Response: 0  
Conc: N.D.

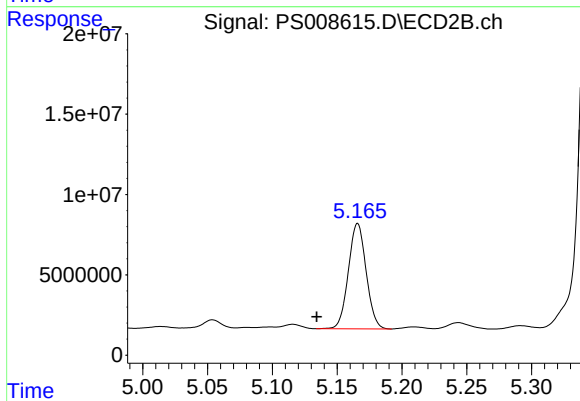

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.166 min  
Delta R.T.: 0.032 min  
Response: 62639632  
Conc: 44.83 ng/ml

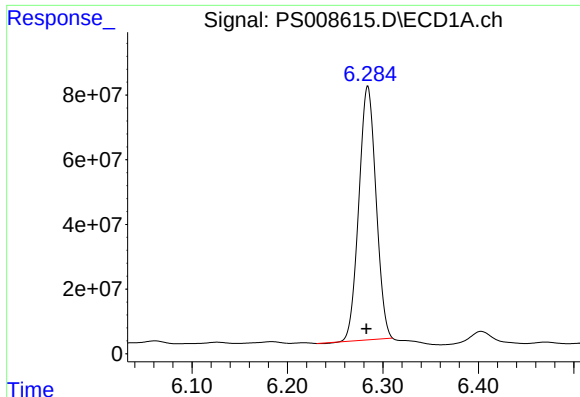

#4 2,4-DCAA


R.T.: 6.284 min  
Delta R.T.: 0.002 min  
Response: 982297843  
Conc: 556.32 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

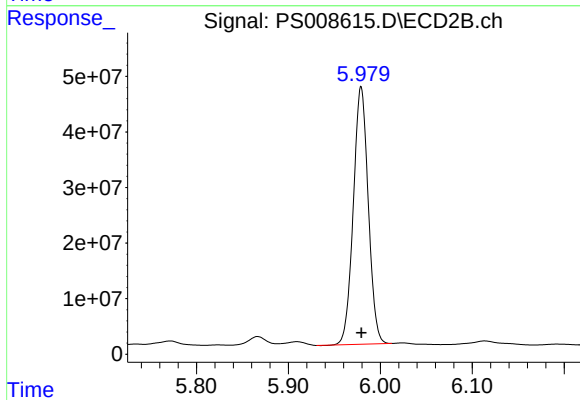


#4 2,4-DCAA

R.T.: 5.979 min  
Delta R.T.: 0.000 min  
Response: 523406758  
Conc: 552.43 ng/ml

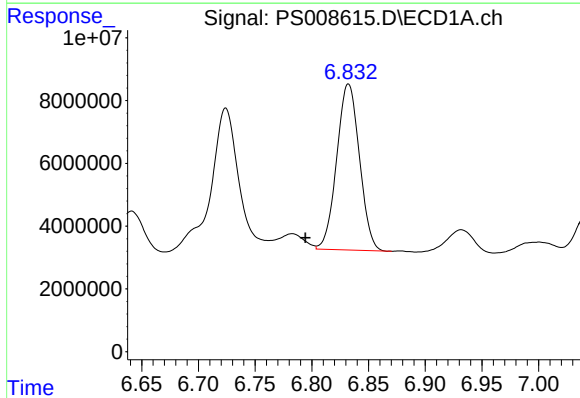


#7 MCPA

R.T.: 6.832 min  
Delta R.T.: 0.038 min  
Response: 73842896  
Conc: 10.11 ug/ml

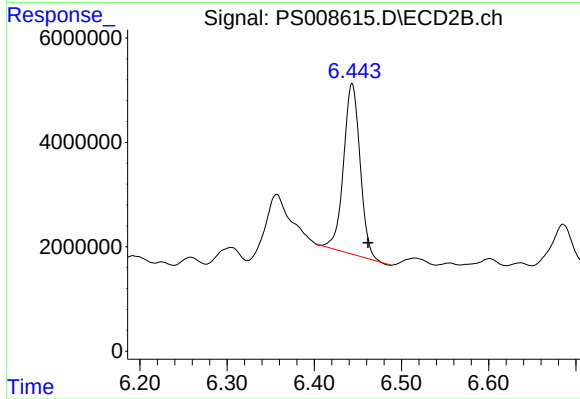

#7 MCPA


R.T.: 6.443 min  
Delta R.T.: -0.018 min  
Response: 43106627  
Conc: 10.10 ug/ml

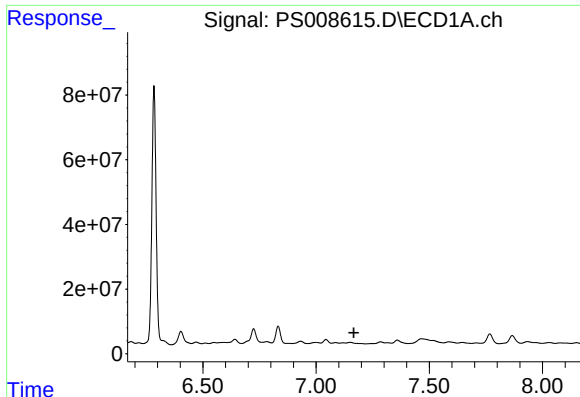

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T.: 7.167 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

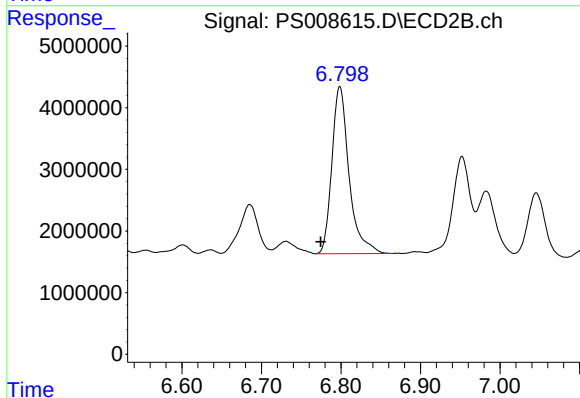


#8 DICHLORPROP

R.T.: 6.799 min  
Delta R.T.: 0.024 min  
Response: 40752351  
Conc: 42.18 ng/ml

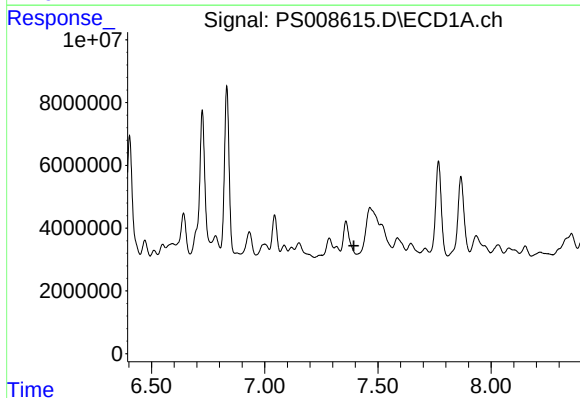


#9 2,4-D

R.T.: 0.000 min  
Exp R.T.: 7.394 min  
Response: 0  
Conc: N.D.

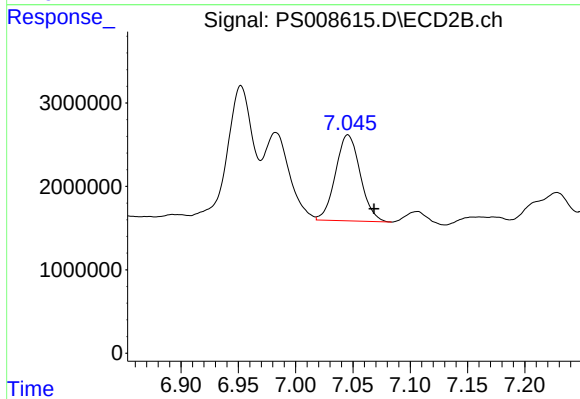

#9 2,4-D


R.T.: 7.046 min  
Delta R.T.: -0.023 min  
Response: 15499979  
Conc: 13.22 ng/ml

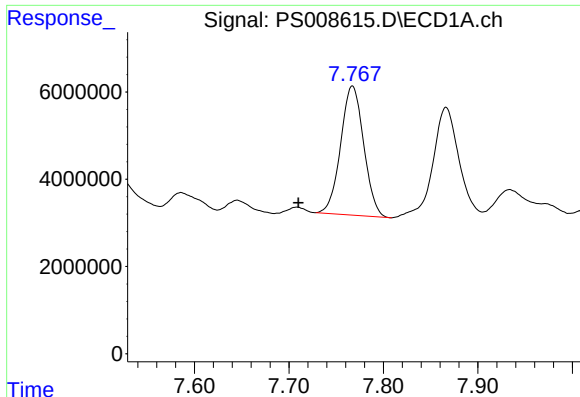

#10 Pentachlorophenol


R.T.: 7.767 min  
Delta R.T.: 0.057 min  
Response: 50211045  
Conc: 2.07 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

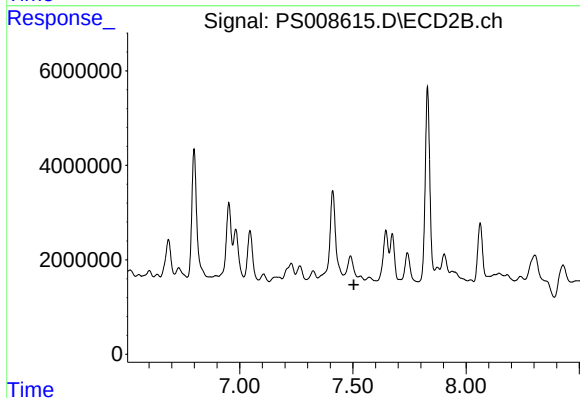


#10 Pentachlorophenol

R.T.: 0.000 min  
Exp R.T. : 7.505 min  
Response: 0  
Conc: N.D.

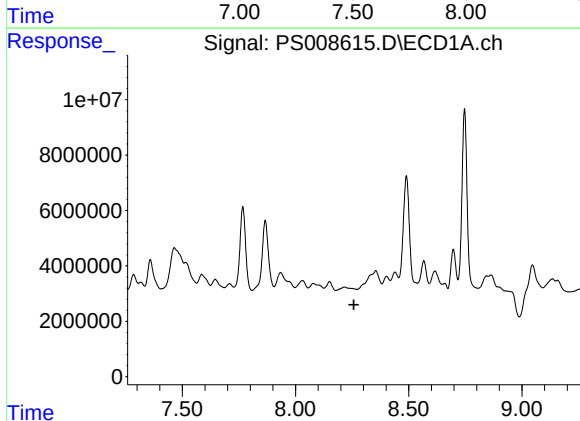


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T. : 8.258 min  
Response: 0  
Conc: N.D.

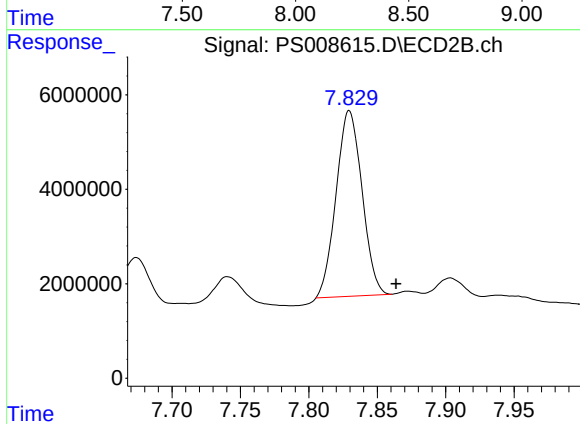

#11 2,4,5-TP (SILVEX)


R.T.: 7.830 min  
Delta R.T.: -0.034 min  
Response: 51886669  
Conc: 9.93 ng/ml

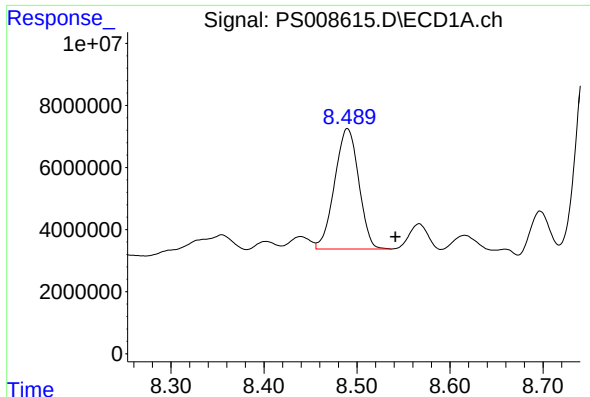

#12 2,4,5-T


R.T.: 8.490 min  
Delta R.T.: -0.052 min  
Response: 69830168  
Conc: 7.57 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

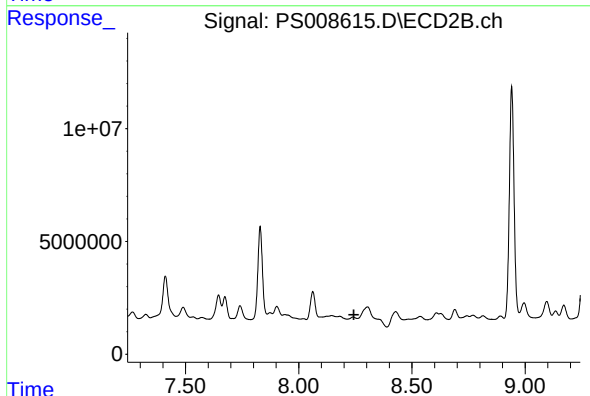


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 8.243 min  
Response: 0  
Conc: N.D.

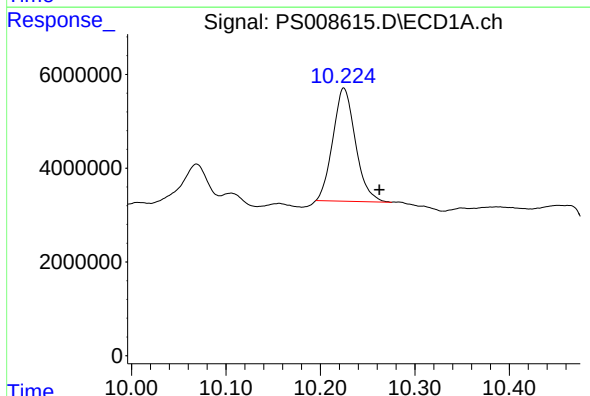


#14 DINOSEB

R.T.: 10.225 min  
Delta R.T.: -0.038 min  
Response: 40089333  
Conc: 5.59 ng/ml

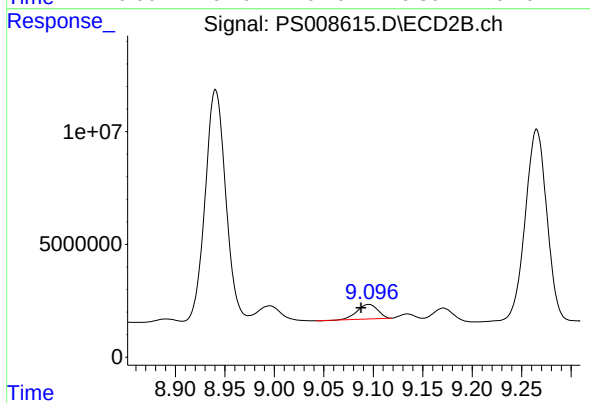

#14 DINOSEB


R.T.: 9.095 min  
Delta R.T.: 0.008 min  
Response: 9332621  
Conc: 2.47 ng/ml

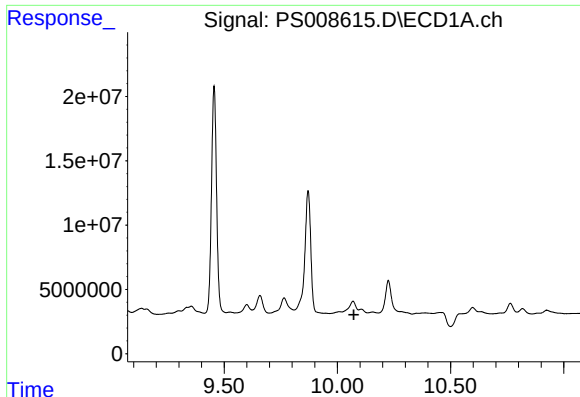

#15 Picloram


R.T.: 0.000 min  
Exp R.T.: 10.073 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
PB126435BL

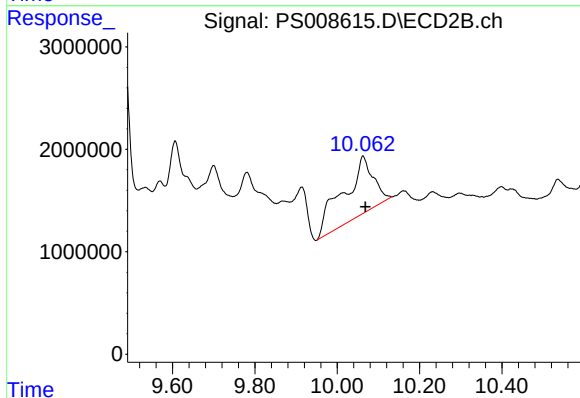


#15 Picloram

R.T.: 10.063 min  
Delta R.T.: -0.005 min  
Response: 28828815  
Conc: 3.88 ng/ml

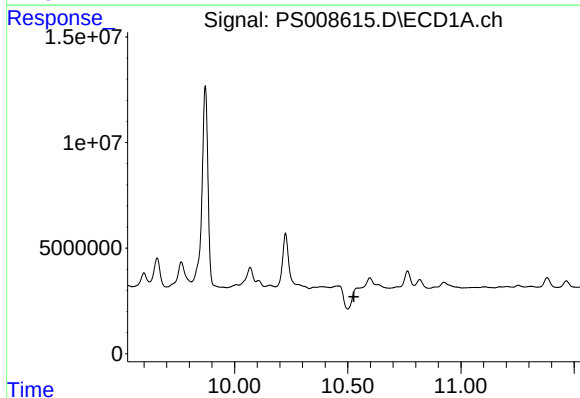

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 10.527 min  
Response: 0  
Conc: N.D.

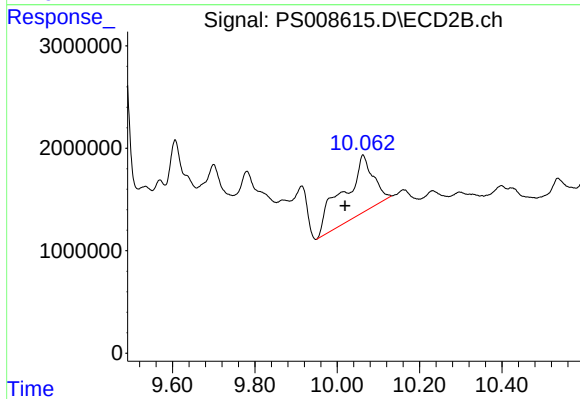

#16 DCPA

R.T.: 10.063 min  
Delta R.T.: 0.044 min  
Response: 28828815  
Conc: 4.42 ng/ml