

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
 Data File : PS008629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 23:11
 Operator : DD\AJ
 Sample : L1289-38
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:51:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.266	5.961	1724.0E6	940.0E6	976.395	992.094
Target Compounds							
1) T	Dalapon	2.499	2.187	204.2E6	118.3E6	79.659	93.294
2) T	3,5-DICHL...	0.000	5.148	0	173.2E6	N.D.	123.948
5) T	DICAMBA	6.450	6.095	13528793	8759799	1.968	2.190
6) T	MCP	6.706	0.000	177.0E6	0	34.721	N.D. #
7) T	MCPA	0.000	6.485	0	29844983	N.D.	6.990
8) T	DICHLORPROP	0.000	6.780	0	44059503	N.D.	45.603
9) T	2,4-D	0.000	7.027	0	12139585	N.D.	10.356
10) T	Pentachlo...	7.749	0.000	37536944	0	1.544	N.D. #
12) T	2,4,5-T	0.000	8.290	0	14579794	N.D.	2.757
14) T	DINOSEB	0.000	9.112	0	110.4E6	N.D.	29.237
15) T	Picloram	10.035	0.000	71085102	0	5.695	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
Data File : PS008629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 23:11
Operator : DD\AJ
Sample : L1289-38
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:51:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

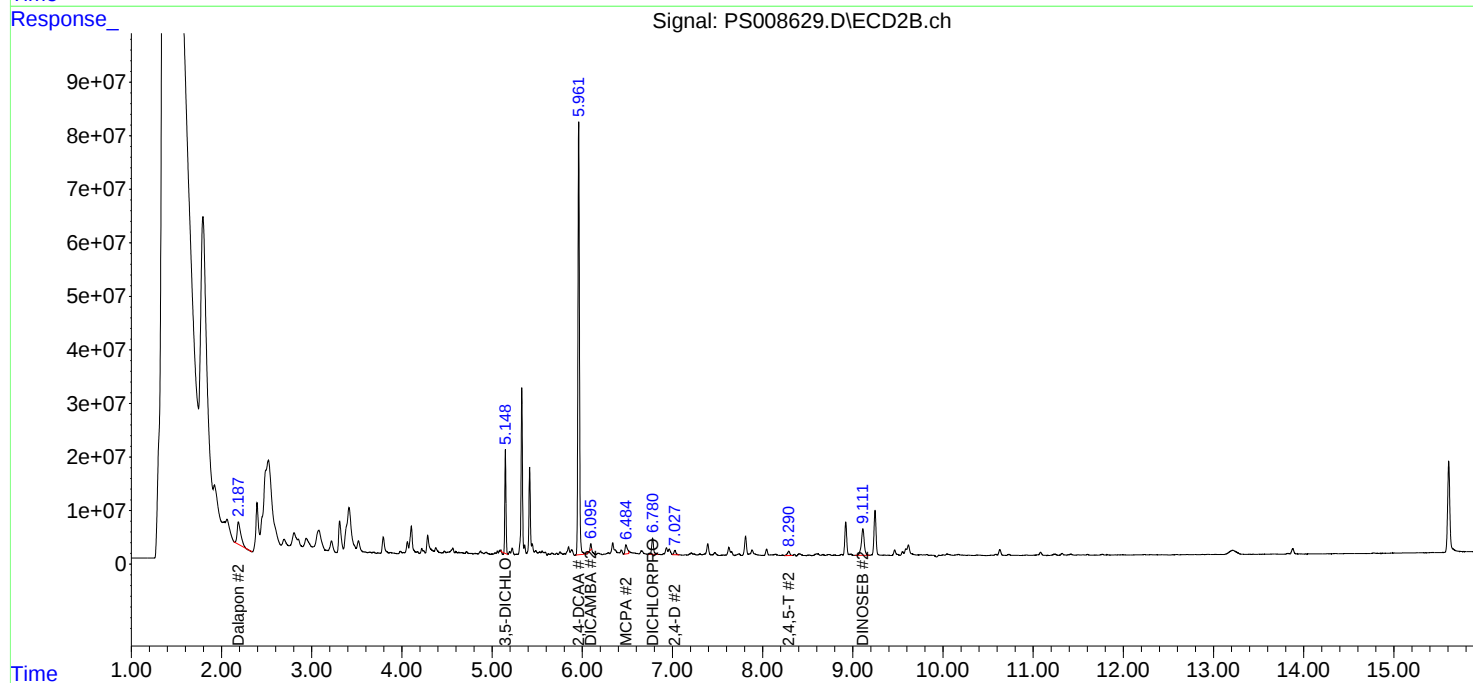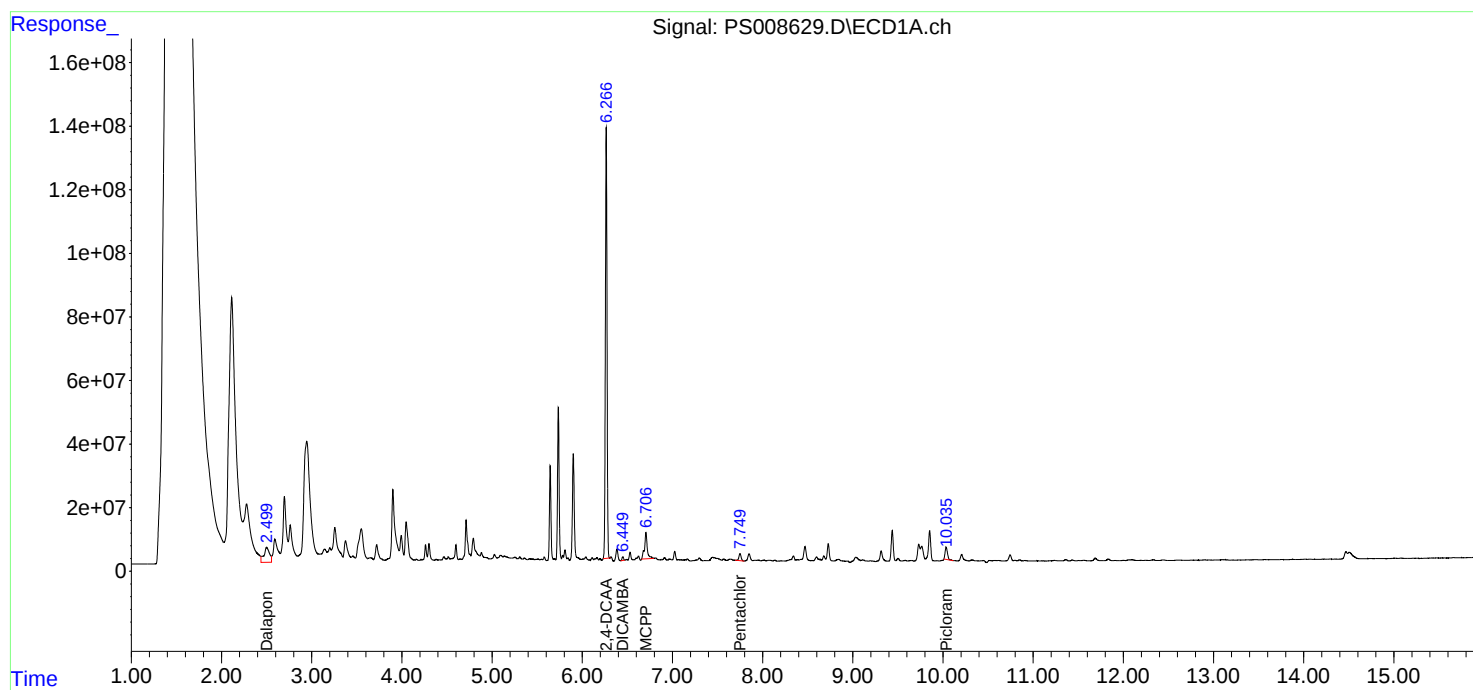


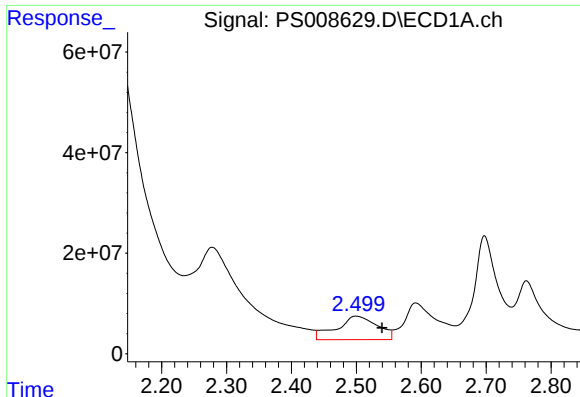

#1 Dalapon


R.T.: 2.499 min
Delta R.T.: -0.041 min
Response: 204233864
Conc: 79.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

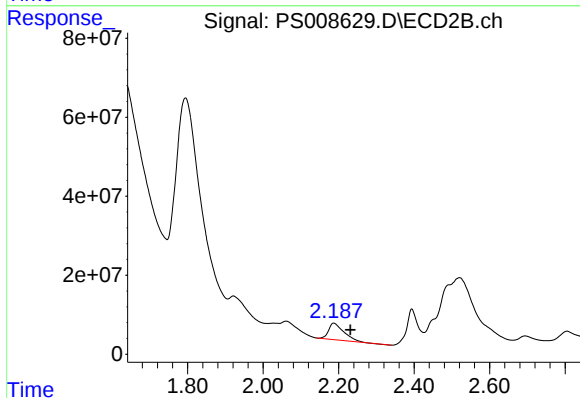


#1 Dalapon

R.T.: 2.187 min
Delta R.T.: -0.044 min
Response: 118272727
Conc: 93.29 ng/ml

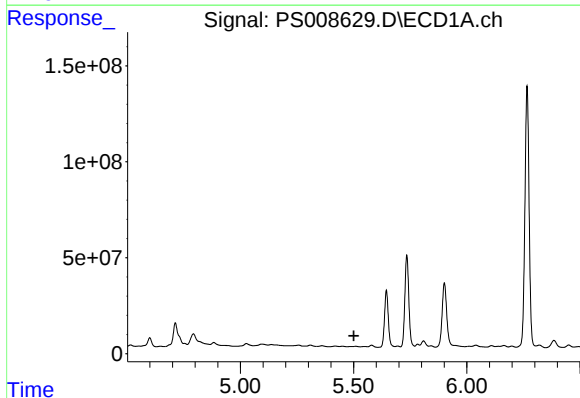


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

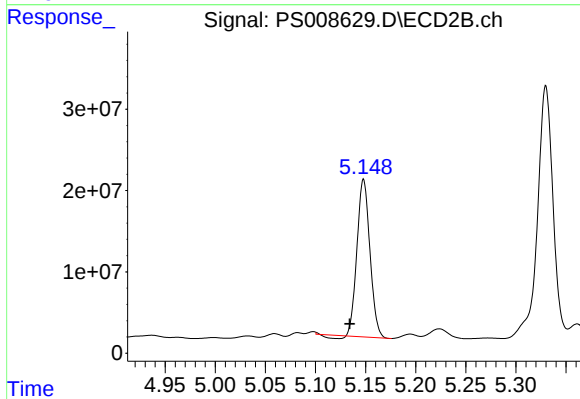

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.148 min
Delta R.T.: 0.014 min
Response: 173176983
Conc: 123.95 ng/ml

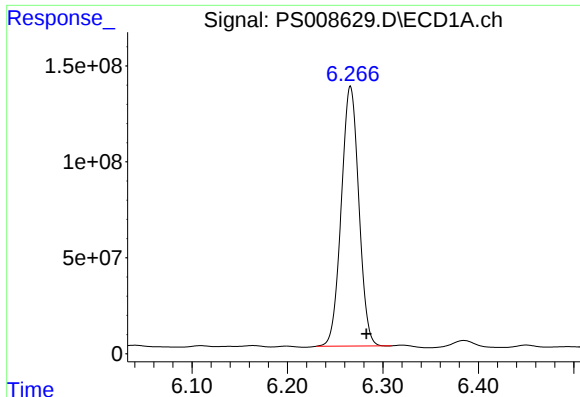

#4 2,4-DCAA


R.T.: 6.266 min
Delta R.T.: -0.017 min
Response: 1724024740
Conc: 976.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

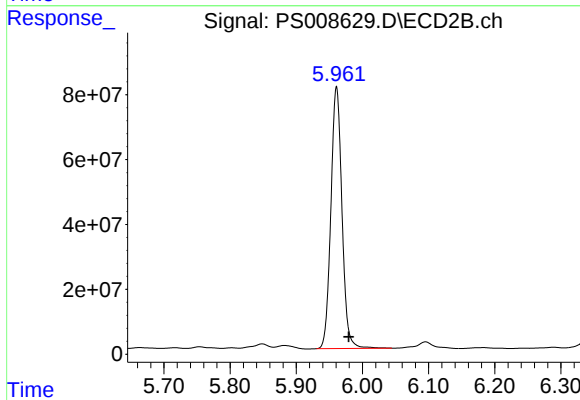


#4 2,4-DCAA

R.T.: 5.961 min
Delta R.T.: -0.018 min
Response: 939972595
Conc: 992.09 ng/ml

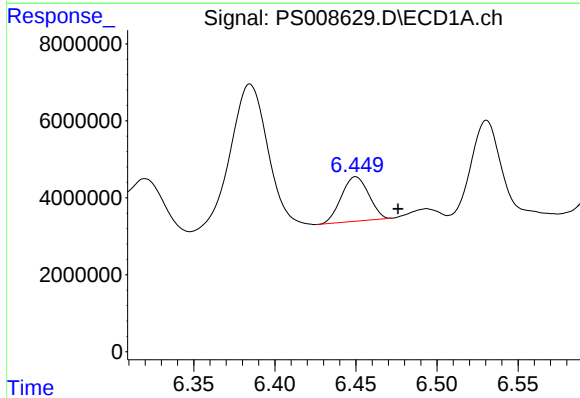


#5 DICAMBA

R.T.: 6.450 min
Delta R.T.: -0.026 min
Response: 13528793
Conc: 1.97 ng/ml

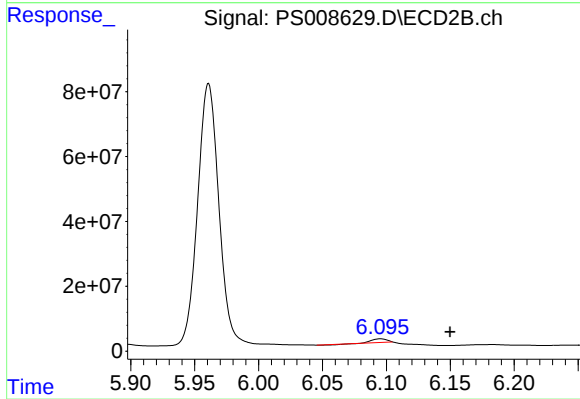

#5 DICAMBA


R.T.: 6.095 min
Delta R.T.: -0.055 min
Response: 8759799
Conc: 2.19 ng/ml

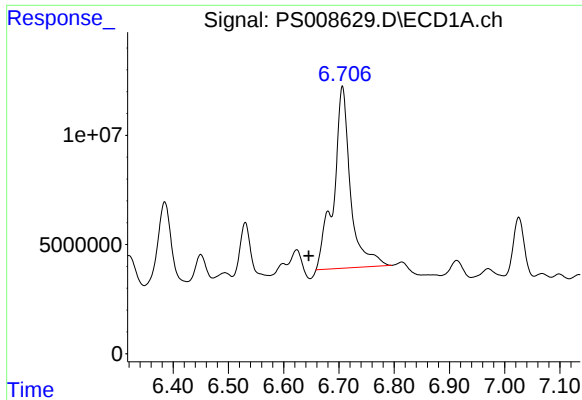

#6 MCPP


R.T.: 6.706 min
Delta R.T.: 0.061 min
Response: 176967094
Conc: 34.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

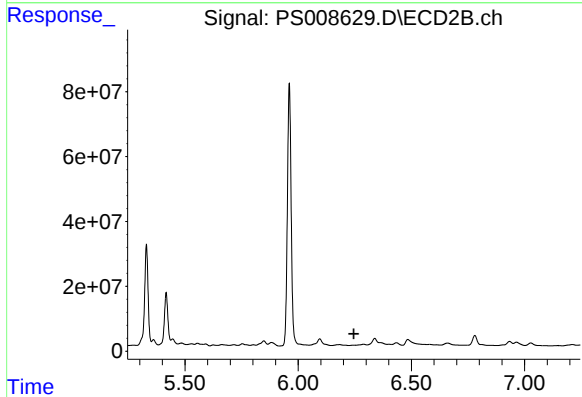


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

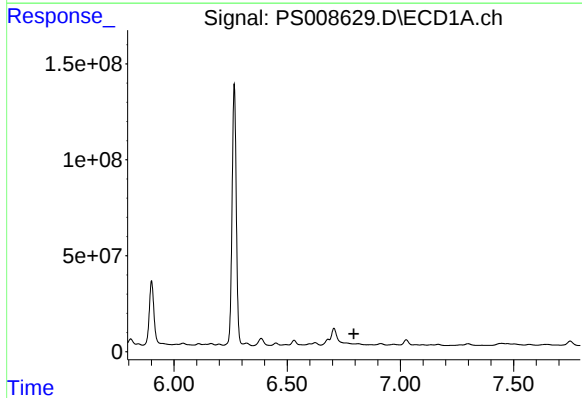


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

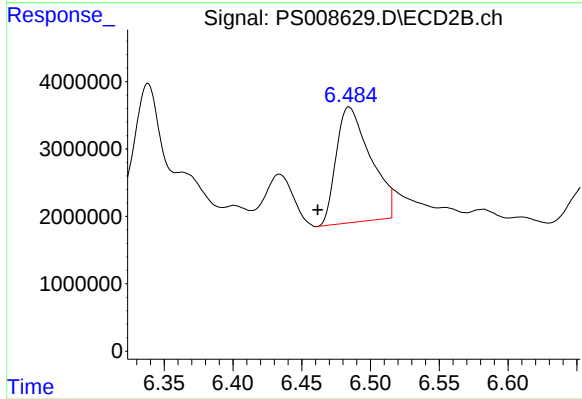

#7 MCPA


R.T.: 6.485 min
Delta R.T.: 0.023 min
Response: 29844983
Conc: 6.99 ug/ml

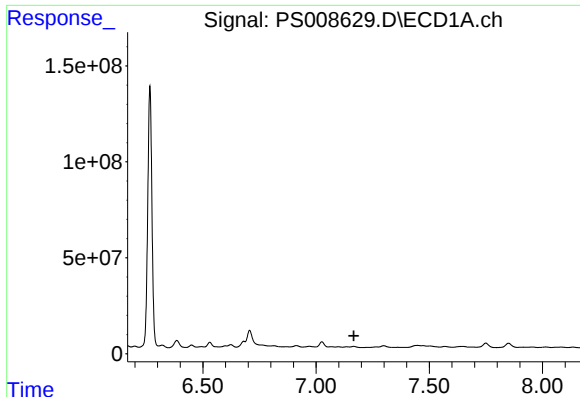

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

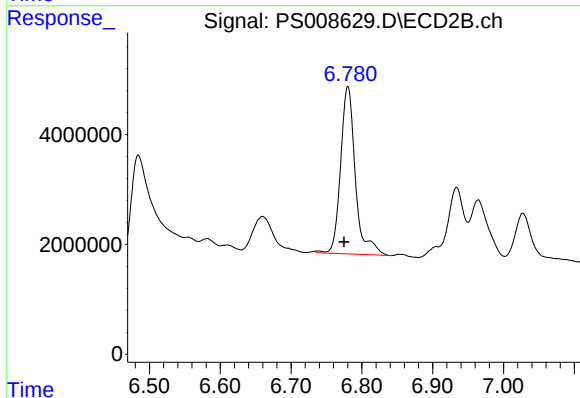


#8 DICHLORPROP

R.T.: 6.780 min
Delta R.T.: 0.006 min
Response: 44059503
Conc: 45.60 ng/ml

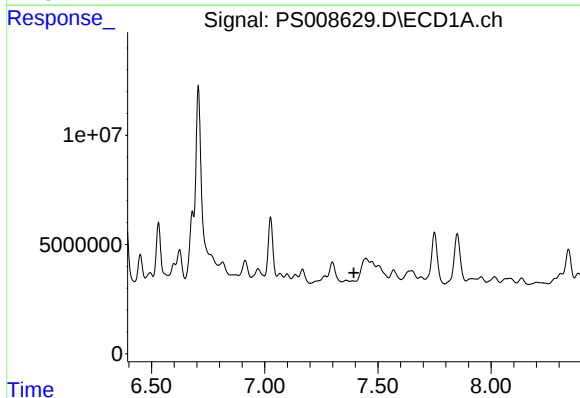


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

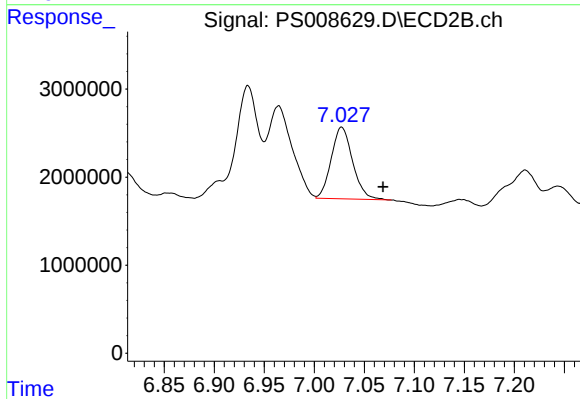

#9 2,4-D


R.T.: 7.027 min
Delta R.T.: -0.041 min
Response: 12139585
Conc: 10.36 ng/ml

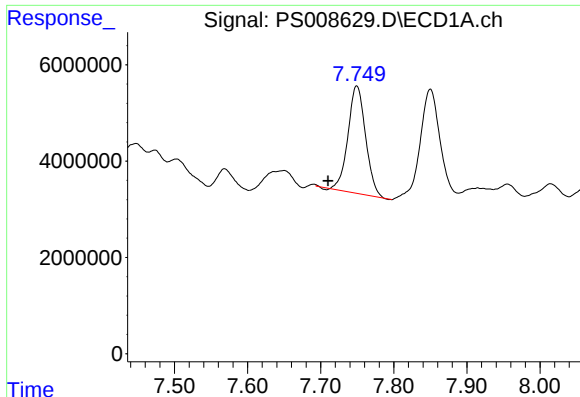

#10 Pentachlorophenol


R.T.: 7.749 min
Delta R.T.: 0.039 min
Response: 37536944
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

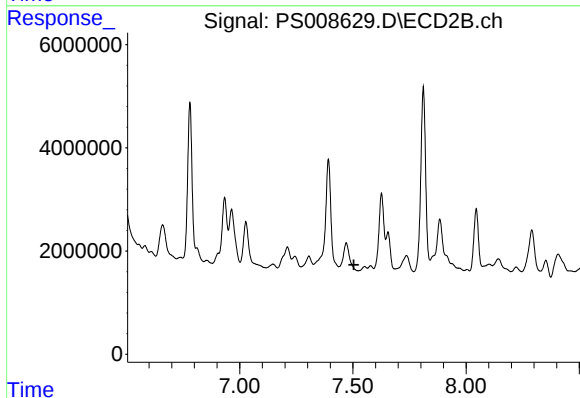


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

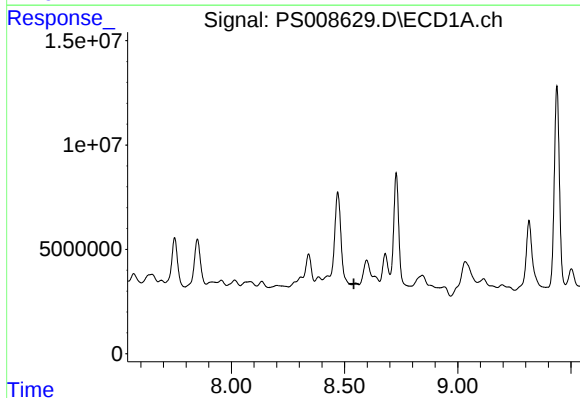


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

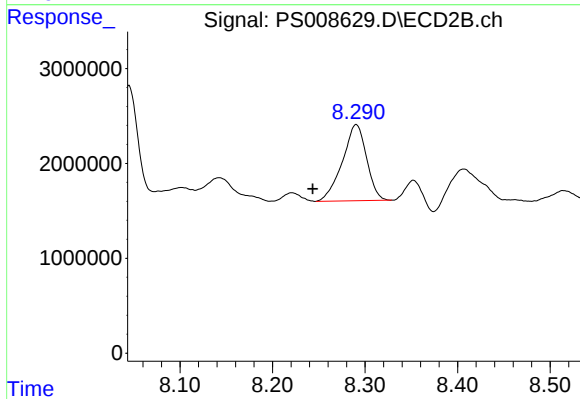

#12 2,4,5-T


R.T.: 8.290 min
Delta R.T.: 0.047 min
Response: 14579794
Conc: 2.76 ng/ml

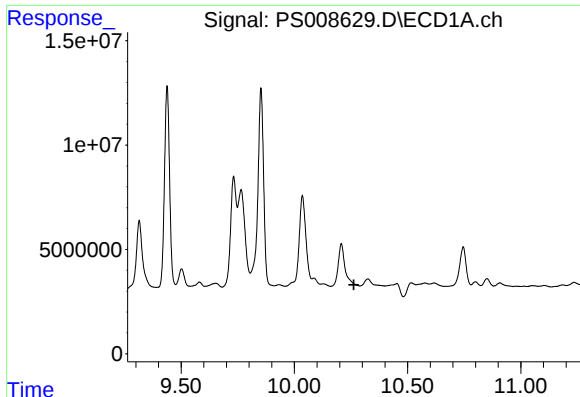

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 10.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

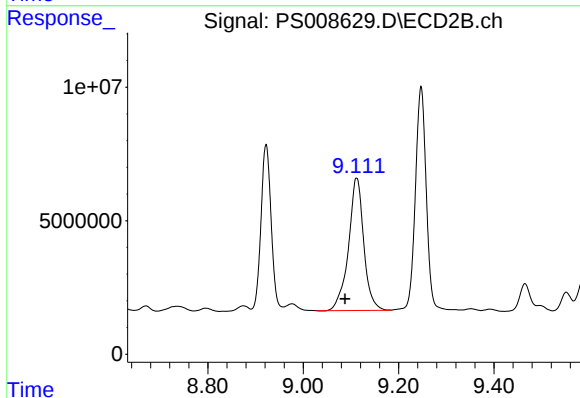


#14 DINOSEB

R.T.: 9.112 min
Delta R.T.: 0.024 min
Response: 110448514
Conc: 29.24 ng/ml

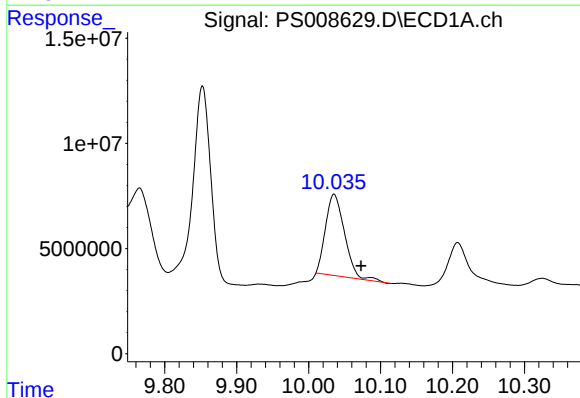

#15 Picloram

R.T.: 10.035 min
Delta R.T.: -0.038 min
Response: 71085102
Conc: 5.70 ng/ml

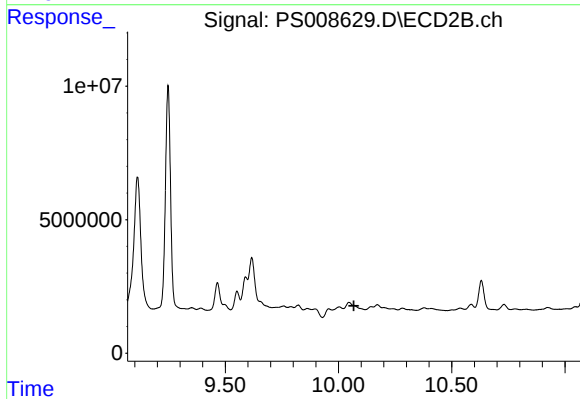

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.068 min
Response: 0
Conc: N.D.