

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
 Data File : PS008630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 23:33
 Operator : DD\AJ
 Sample : L1274-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BORING-B1-SAMPLE-S1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:51:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.264	5.959	871.3E6	430.7E6	493.473	454.564
Target Compounds							
2) T	3,5-DICHL...	0.000	5.147	0	29236380	N.D.	20.925
6) T	MCP	6.703	0.000	29798630	0	5.846	N.D. #
7) T	MCPA	6.813	6.423	81374950	34051574	11.136	7.975 #
8) T	DICHLORPROP	0.000	6.777	0	18821634	N.D.	19.481
9) T	2,4-D	0.000	7.026	0	25042335	N.D.	21.363
10) T	Pentachlo...	7.749	0.000	62578111	0	2.574	N.D. #
13) T	2,4-DB	9.026	0.000	13483023	0	9.726	N.D. #
14) T	DINOSEB	0.000	9.019	0	34664451	N.D.	9.176
16) T	DCPA	10.523	0.000	8114946	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
Data File : PS008630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 23:33
Operator : DD\AJ
Sample : L1274-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:51:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

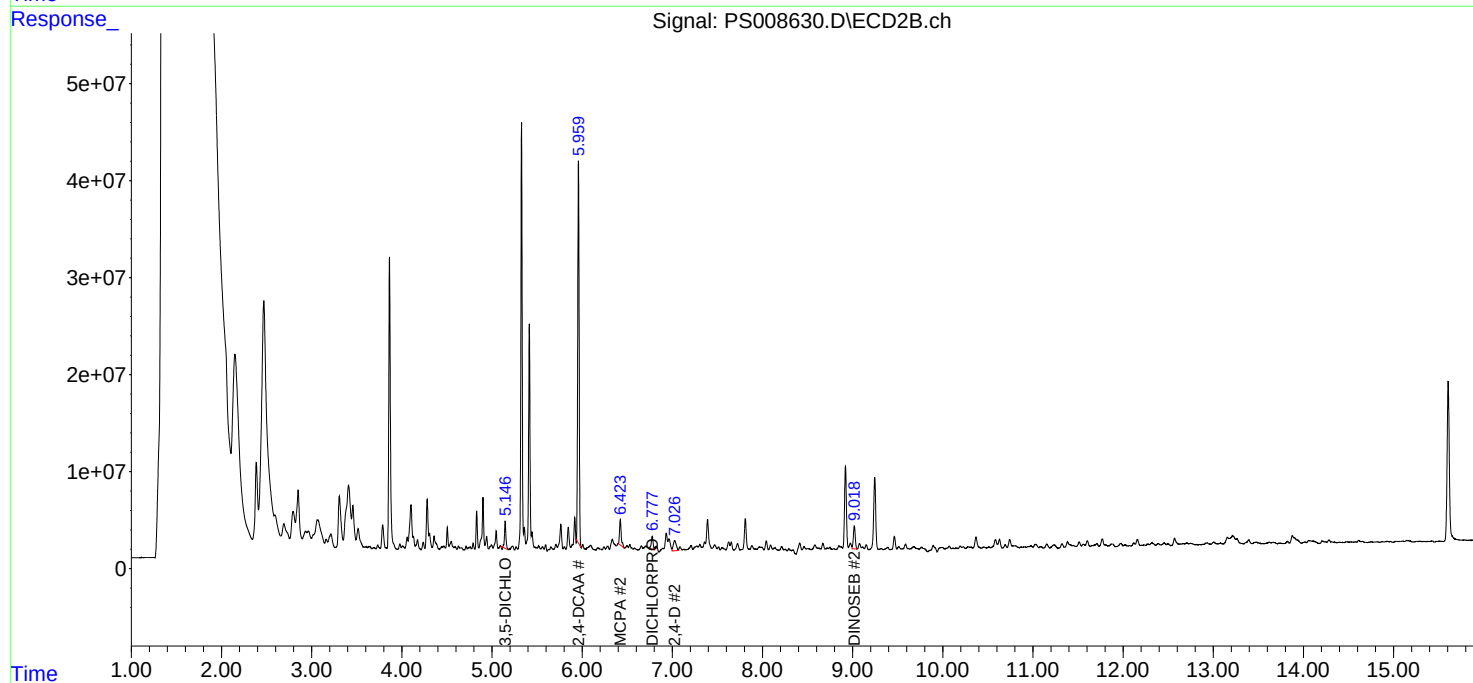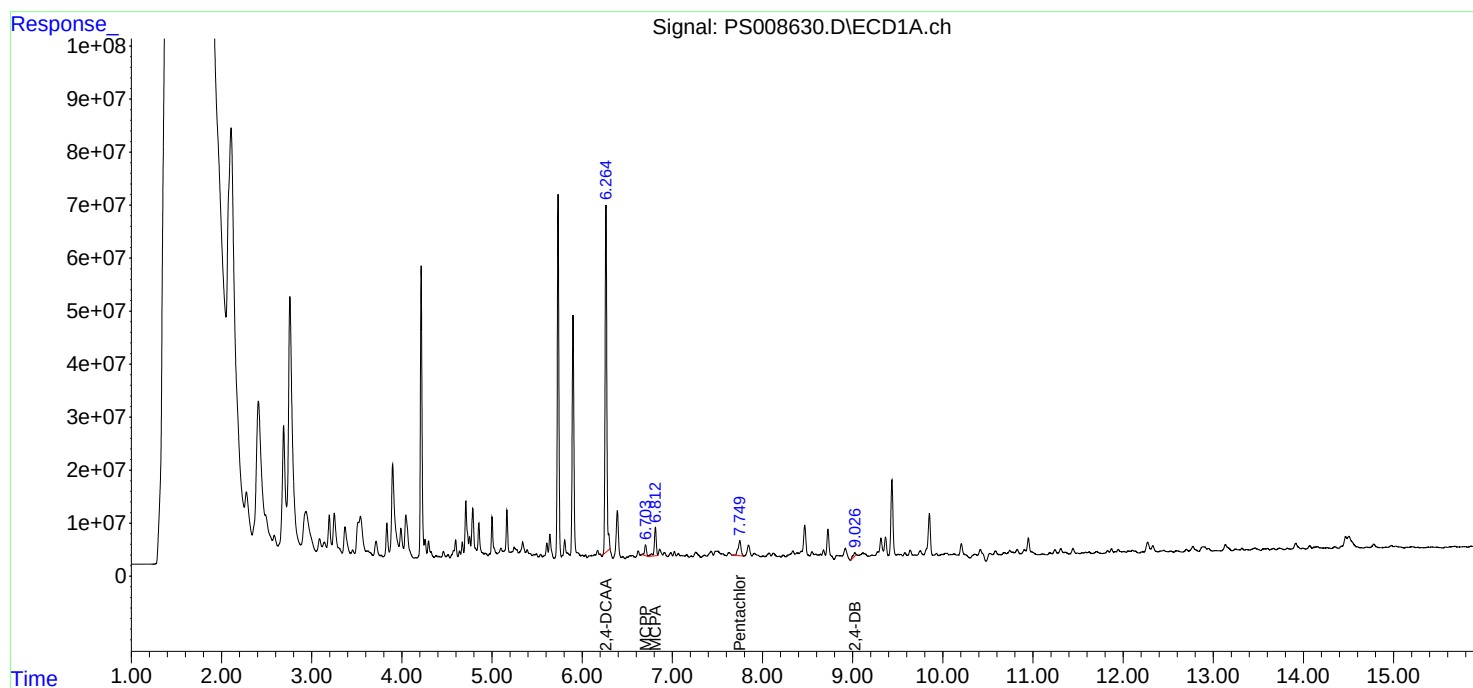


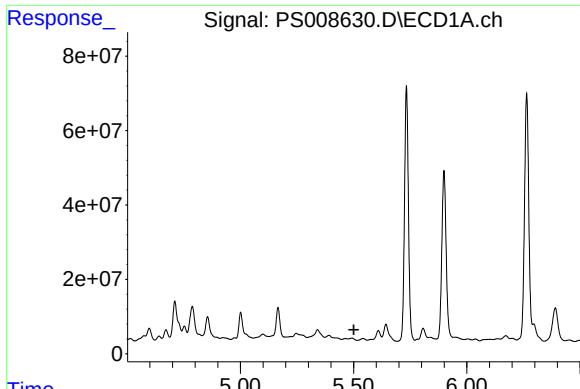

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

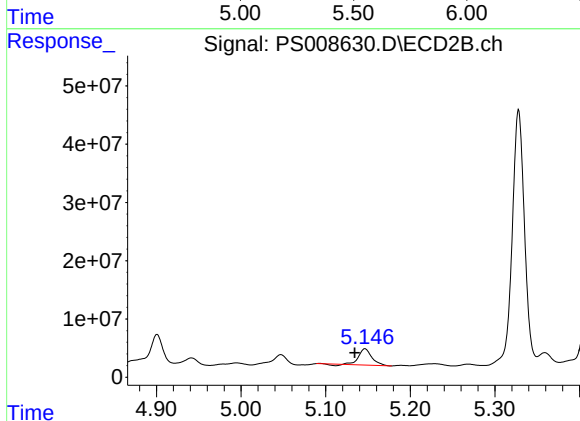


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.147 min
Delta R.T.: 0.012 min
Response: 29236380
Conc: 20.93 ng/ml

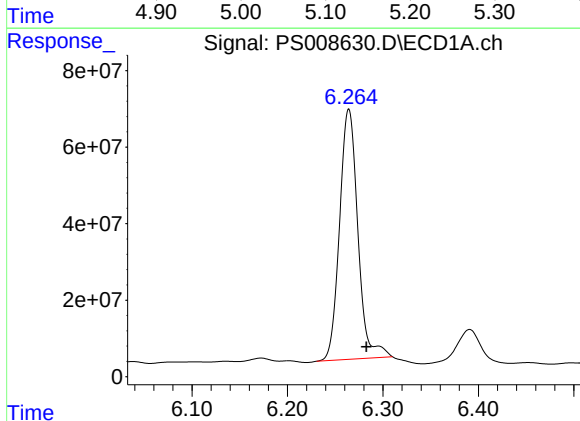


#4 2,4-DCAA

R.T.: 6.264 min
Delta R.T.: -0.018 min
Response: 871327220
Conc: 493.47 ng/ml

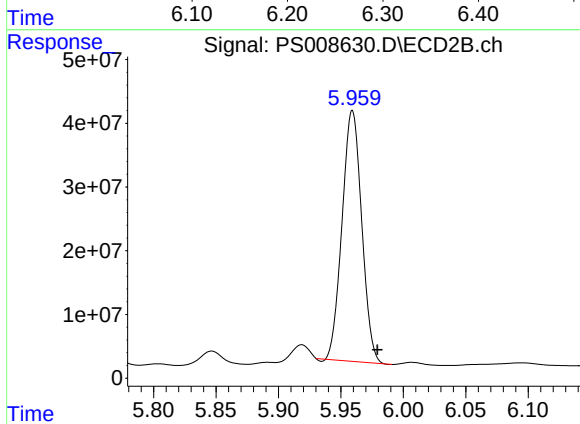

#4 2,4-DCAA


R.T.: 5.959 min
Delta R.T.: -0.020 min
Response: 430682082
Conc: 454.56 ng/ml

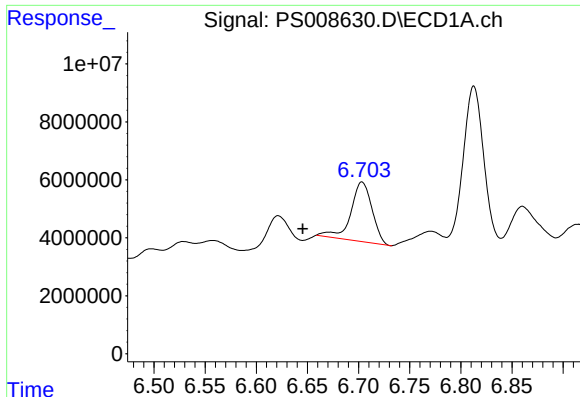

#6 MCPP


R.T.: 6.703 min
Delta R.T.: 0.058 min
Response: 29798630
Conc: 5.85 ug/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

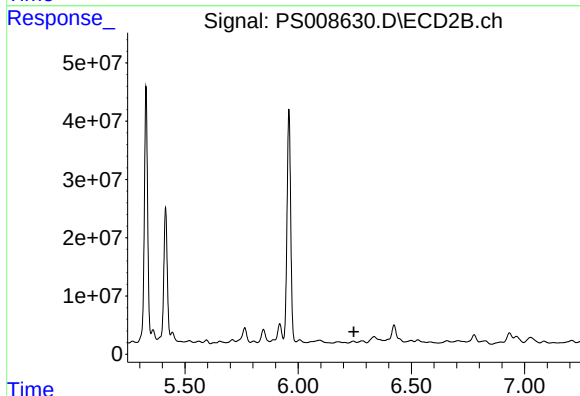


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

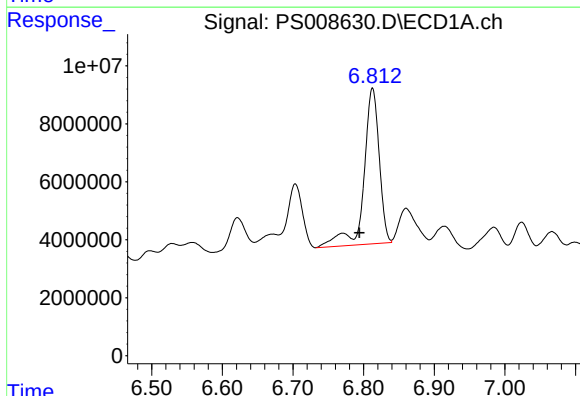


#7 MCPA

R.T.: 6.813 min
Delta R.T.: 0.018 min
Response: 81374950
Conc: 11.14 ug/ml

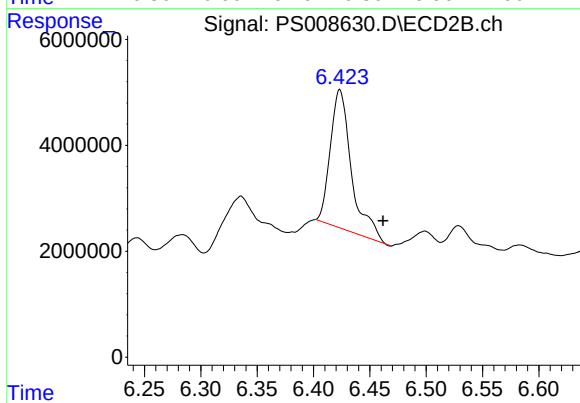

#7 MCPA


R.T.: 6.423 min
Delta R.T.: -0.038 min
Response: 34051574
Conc: 7.97 ug/ml

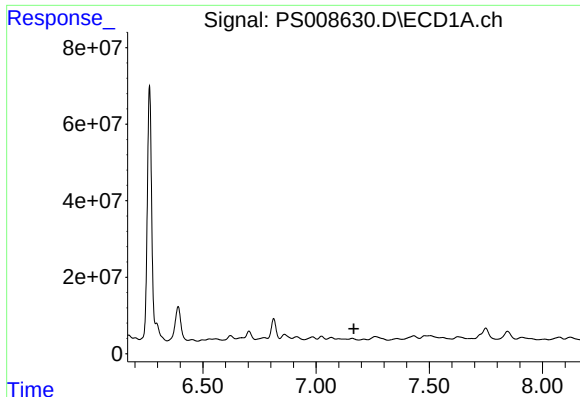

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

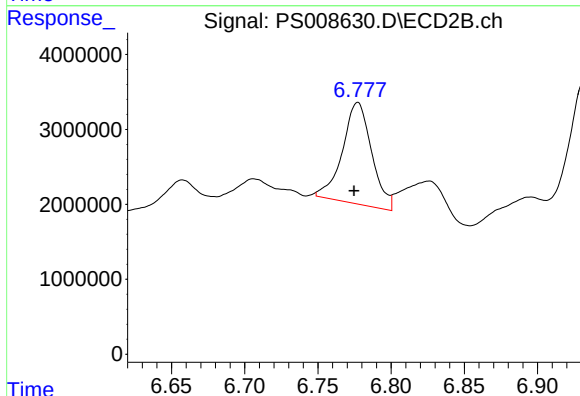


#8 DICHLORPROP

R.T.: 6.777 min
Delta R.T.: 0.002 min
Response: 18821634
Conc: 19.48 ng/ml

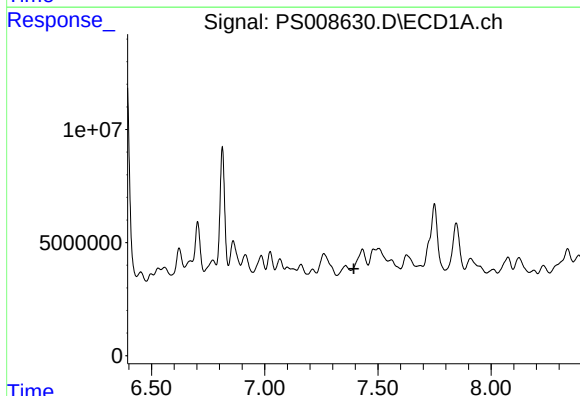


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

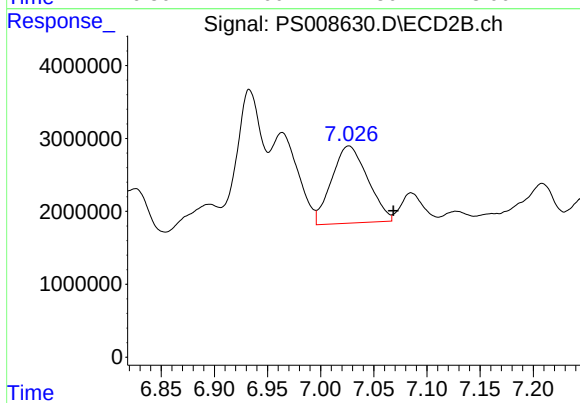

#9 2,4-D


R.T.: 7.026 min
Delta R.T.: -0.042 min
Response: 25042335
Conc: 21.36 ng/ml

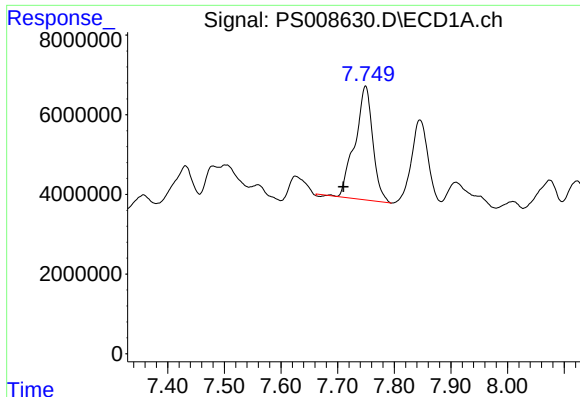

#10 Pentachlorophenol


R.T.: 7.749 min
Delta R.T.: 0.039 min
Response: 62578111
Conc: 2.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

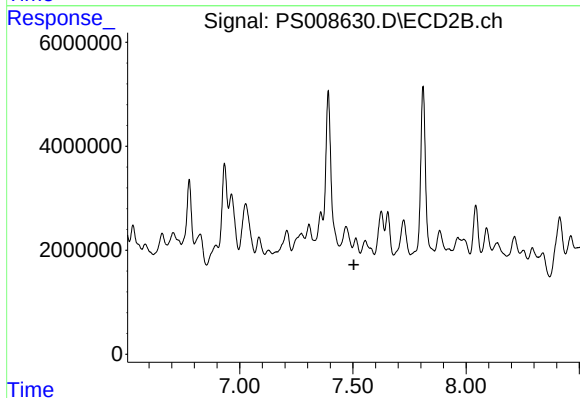


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

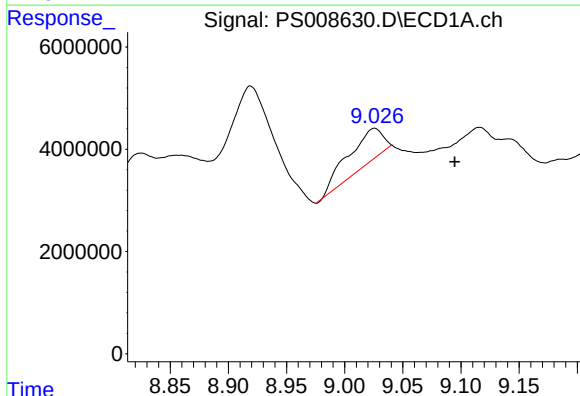


#13 2,4-DB

R.T.: 9.026 min
Delta R.T.: -0.069 min
Response: 13483023
Conc: 9.73 ng/ml

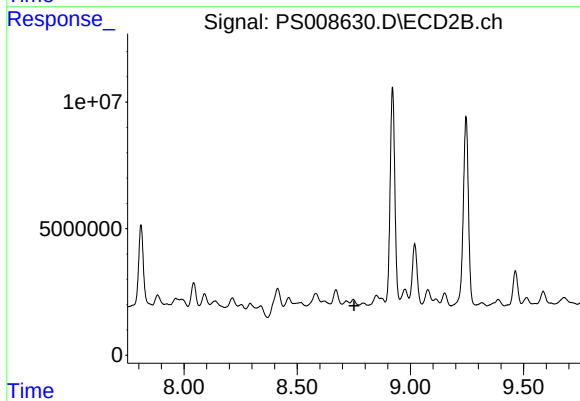

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

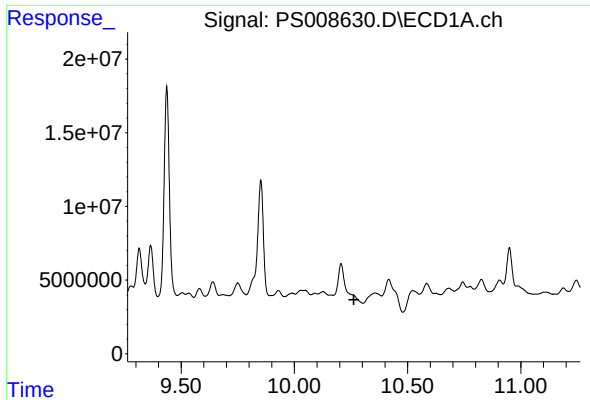

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 10.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BORING-B1-SAMPLE-S1

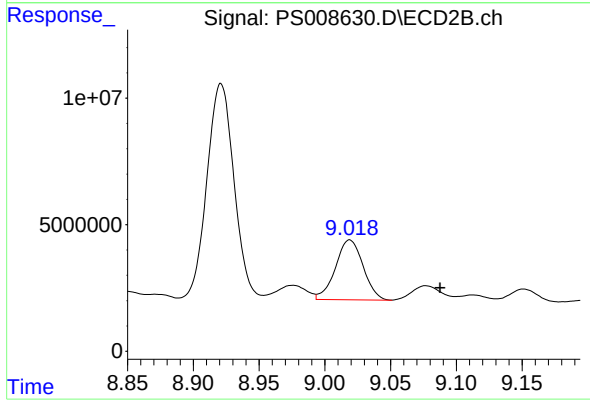

#14 DINOSEB

R.T.: 9.019 min
Delta R.T.: -0.069 min
Response: 34664451
Conc: 9.18 ng/ml