

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
 Data File : PS008631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 23:55
 Operator : DD\AJ
 Sample : L1274-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BORING-B2-SAMPLE-S1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:52:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.268	5.963	874.1E6	454.6E6	495.024	479.798
Target Compounds							
1) T	Dalapon	2.501	0.000	26806308	0	10.455	N.D. #
2) T	3,5-DICHL...	0.000	5.150	0	54871282	N.D.	39.273
5) T	DICAMBA	0.000	6.100	0	244361	N.D.	<MDL
6) T	MCP	6.625	0.000	15863298	0	3.112	N.D. #
7) T	MCPA	6.816	6.427	95016894	38188526	13.003	8.944 #
8) T	DICHLORPROP	0.000	6.782	0	14330566	N.D.	14.833
9) T	2,4-D	7.390	7.029	262.4E6	16075996	144.233	13.714 #
10) T	Pentachlo...	7.754	7.517	41935979	17162680	1.725	1.271 #
13) T	2,4-DB	0.000	8.754	0	10110643	N.D.	14.283
16) T	DCPA	10.520	0.000	9721458	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
Data File : PS008631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 23:55
Operator : DD\AJ
Sample : L1274-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:52:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

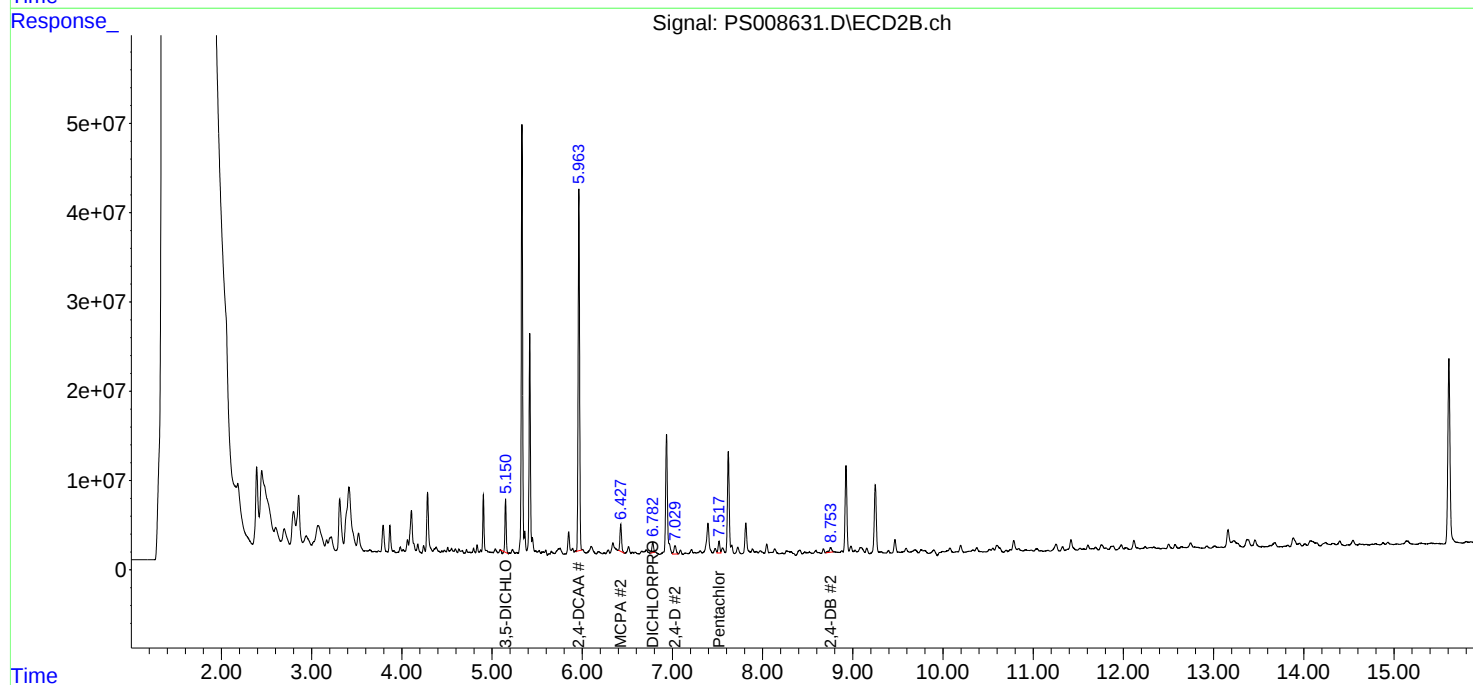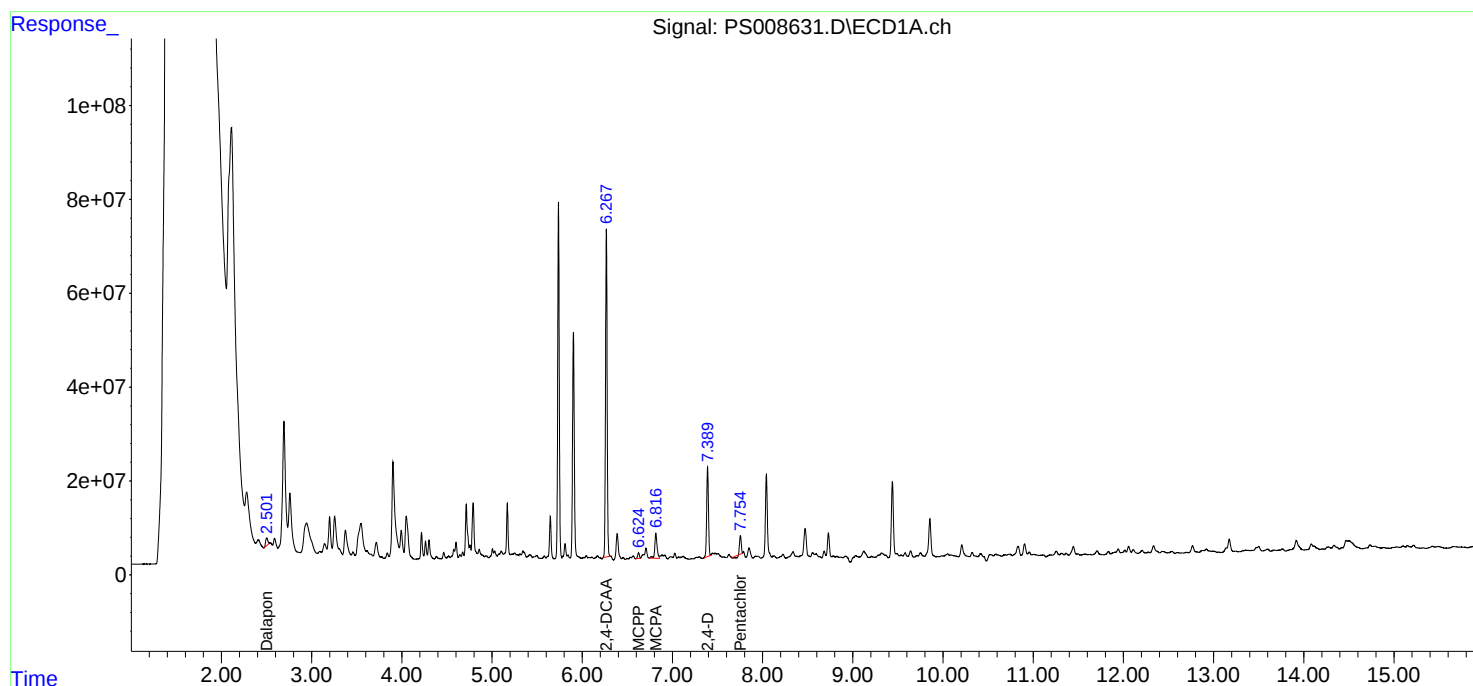


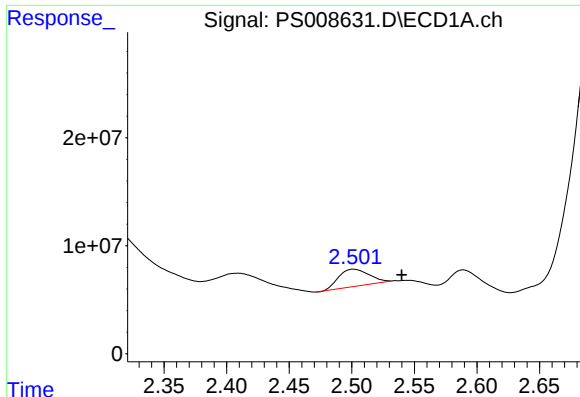

#1 Dalapon


R.T.: 2.501 min
Delta R.T.: -0.039 min
Response: 26806308
Conc: 10.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

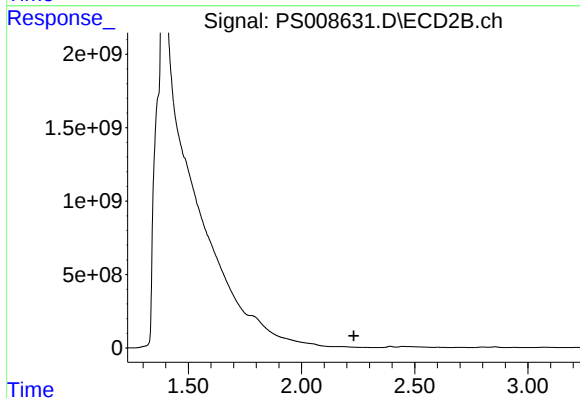


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.231 min
Response: 0
Conc: N.D.

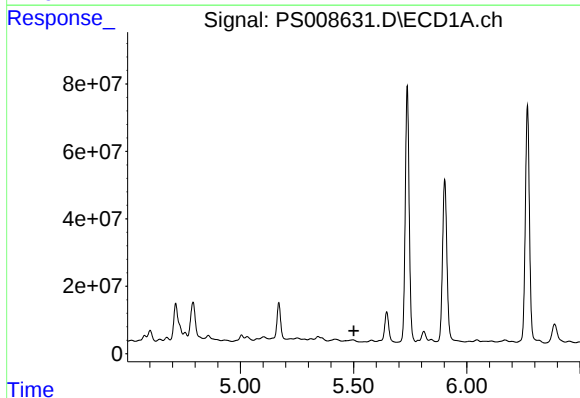


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

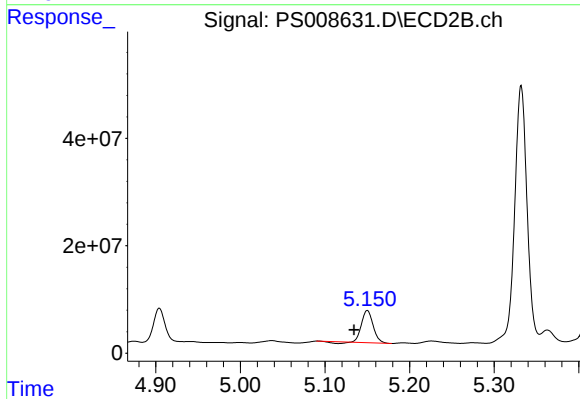

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.150 min
Delta R.T.: 0.016 min
Response: 54871282
Conc: 39.27 ng/ml

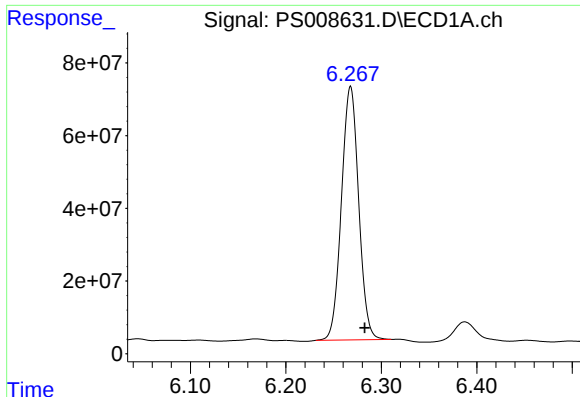

#4 2,4-DCAA


R.T.: 6.268 min
Delta R.T.: -0.015 min
Response: 874066322
Conc: 495.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

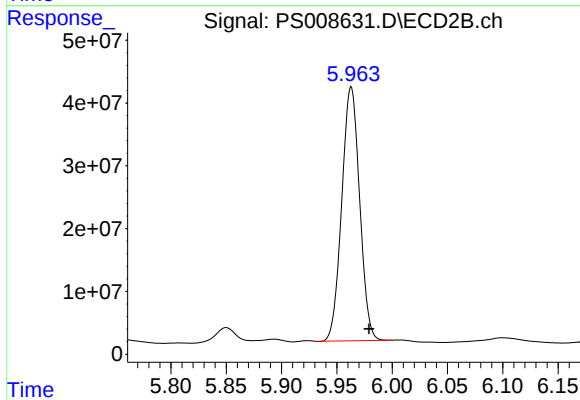


#4 2,4-DCAA

R.T.: 5.963 min
Delta R.T.: -0.016 min
Response: 454590993
Conc: 479.80 ng/ml

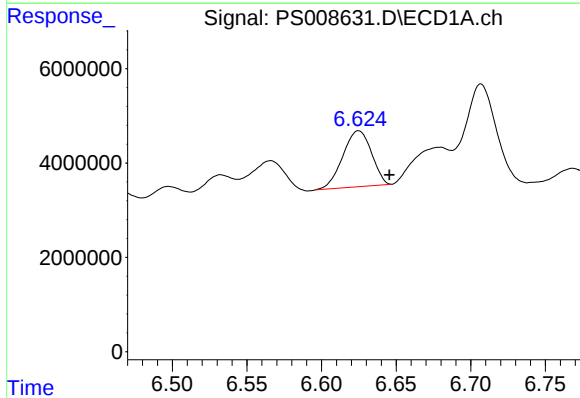


#6 MCP

R.T.: 6.625 min
Delta R.T.: -0.021 min
Response: 15863298
Conc: 3.11 ug/ml

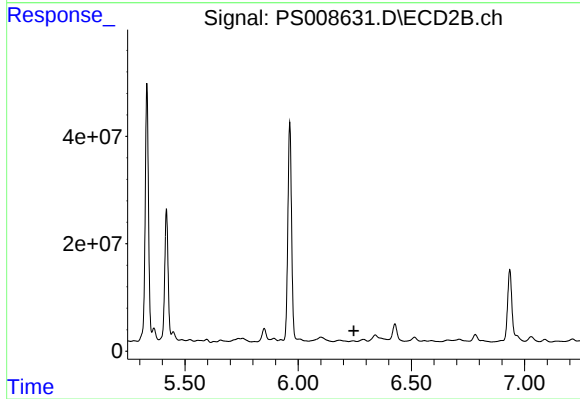

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

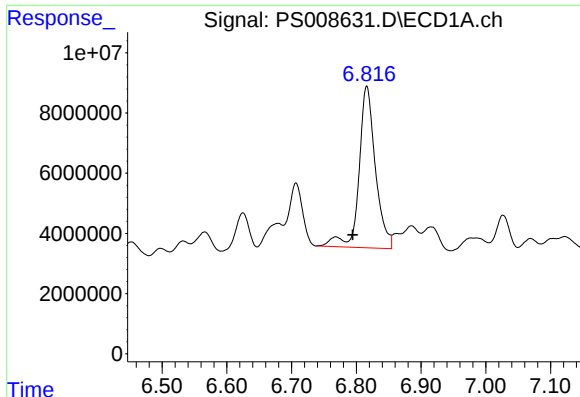

#7 MCPA


R.T.: 6.816 min
Delta R.T.: 0.022 min
Response: 95016894
Conc: 13.00 ug/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

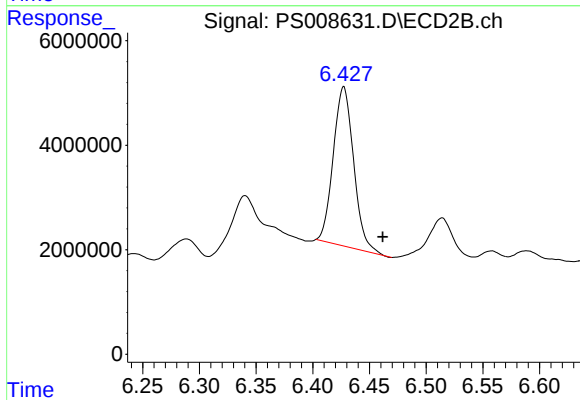


#7 MCPA

R.T.: 6.427 min
Delta R.T.: -0.034 min
Response: 38188526
Conc: 8.94 ug/ml

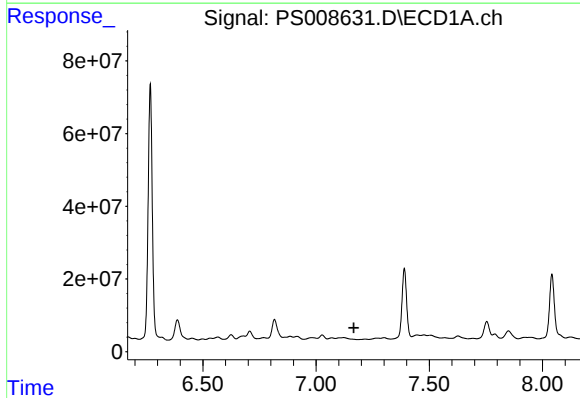


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

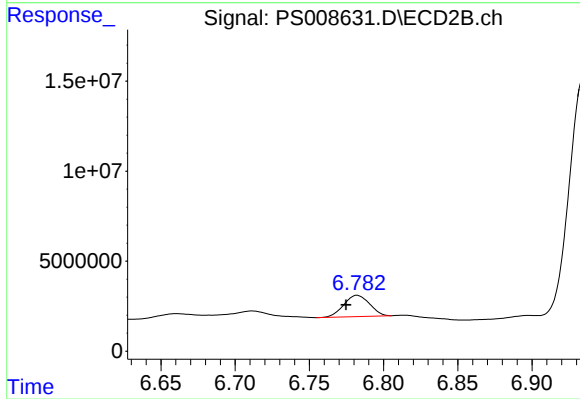

#8 DICHLORPROP


R.T.: 6.782 min
Delta R.T.: 0.007 min
Response: 14330566
Conc: 14.83 ng/ml

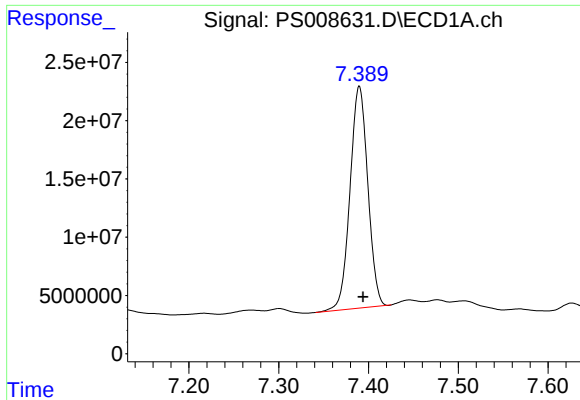

#9 2,4-D


R.T.: 7.390 min
Delta R.T.: -0.004 min
Response: 262374159
Conc: 144.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

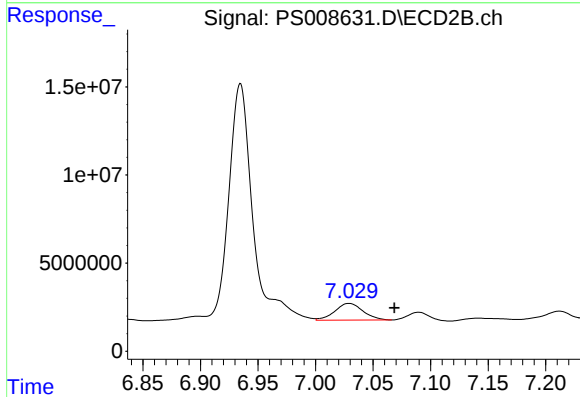


#9 2,4-D

R.T.: 7.029 min
Delta R.T.: -0.040 min
Response: 16075996
Conc: 13.71 ng/ml

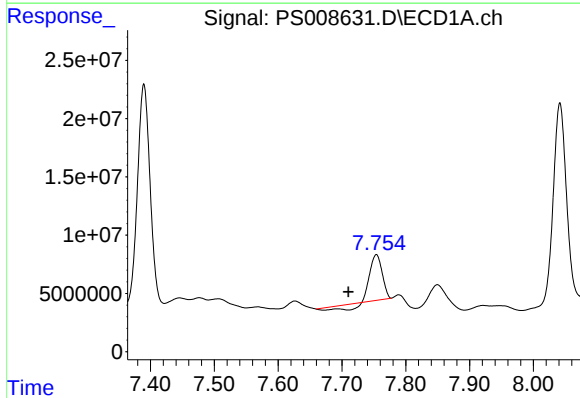


#10 Pentachlorophenol

R.T.: 7.754 min
Delta R.T.: 0.044 min
Response: 41935979
Conc: 1.72 ng/ml

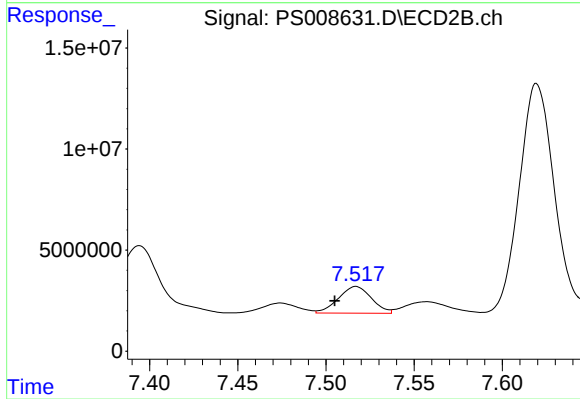

#10 Pentachlorophenol


R.T.: 7.517 min
Delta R.T.: 0.012 min
Response: 17162680
Conc: 1.27 ng/ml

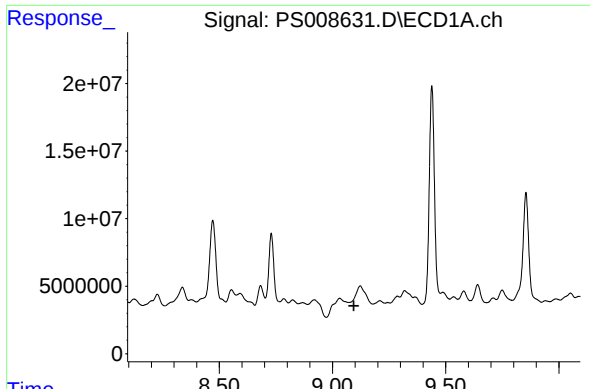

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BORING-B2-SAMPLE-S1

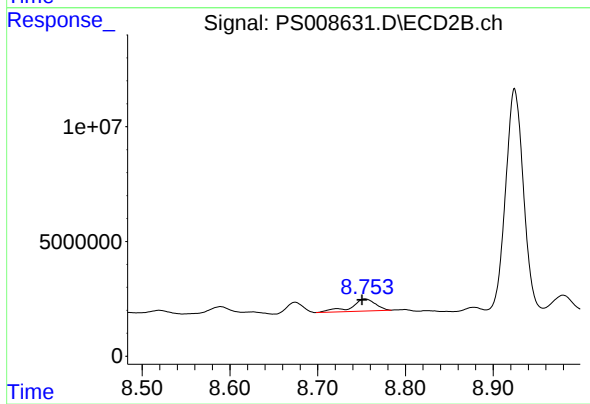

#13 2,4-DB

R.T.: 8.754 min
Delta R.T.: 0.003 min
Response: 10110643
Conc: 14.28 ng/ml