

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
 Data File : PS008633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 01:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 05:42:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.266	5.961	906.9E6	485.9E6	513.617	512.826
Target Compounds							
12) T	2,4,5-T	0.000	8.222	0	10735022	N.D.	2.030
15) T	Picloram	10.054	10.046	65399202	41002501	5.240	5.519
16) T	DCPA	10.505	9.996	31250603	19115792	2.633	2.933



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012920\
Data File : PS008633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 01:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 05:42:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

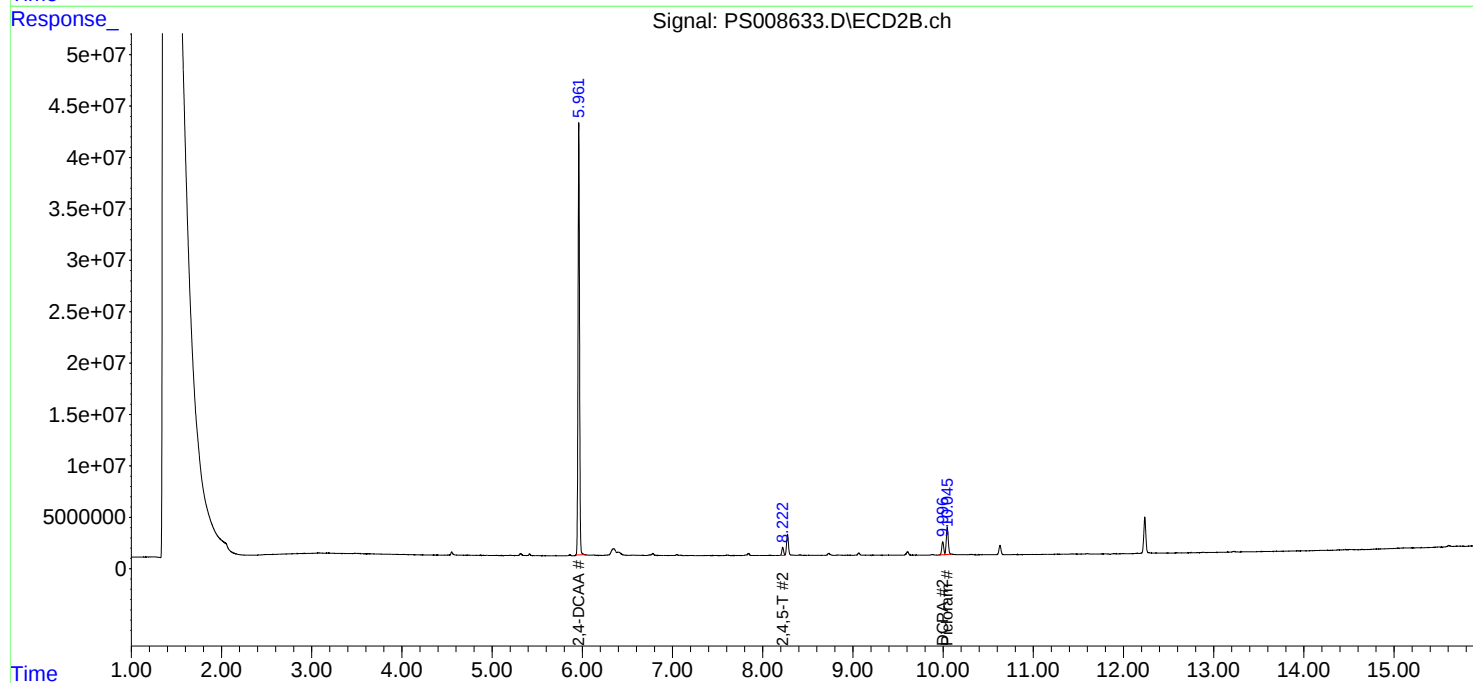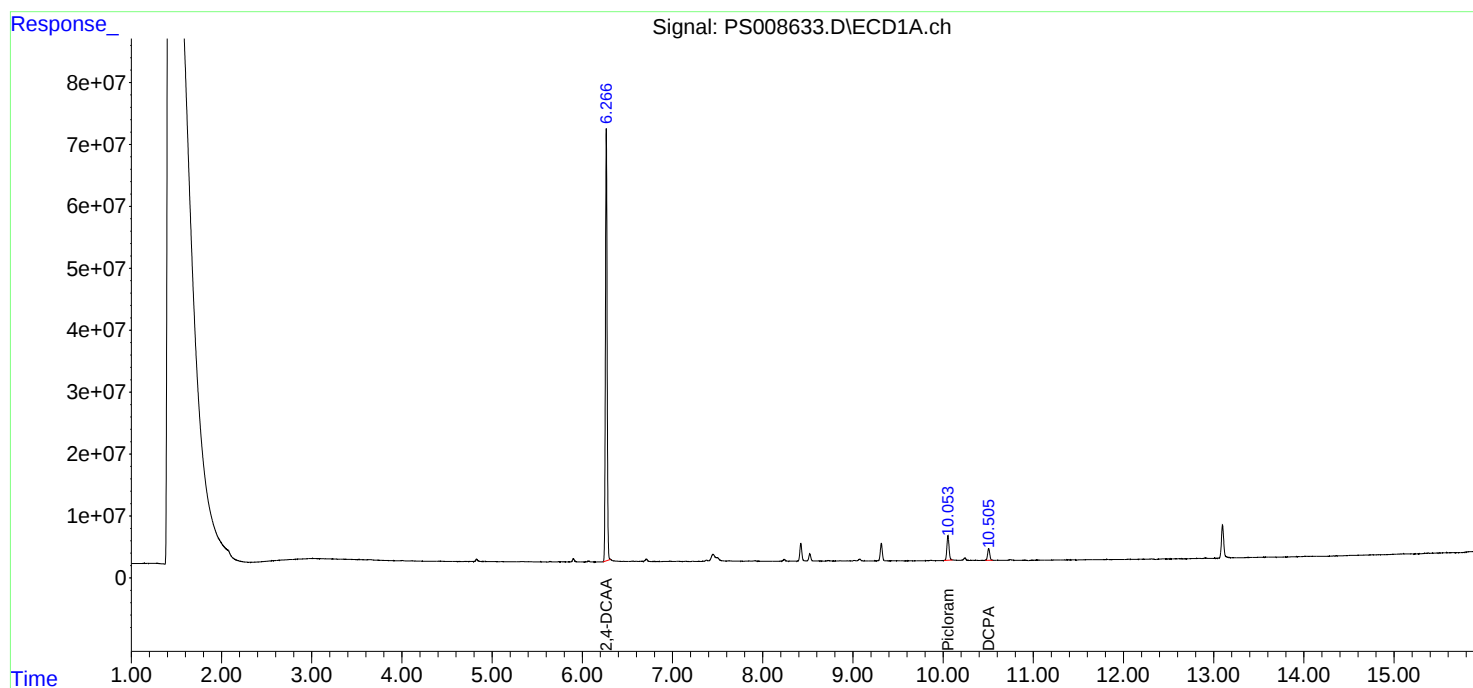


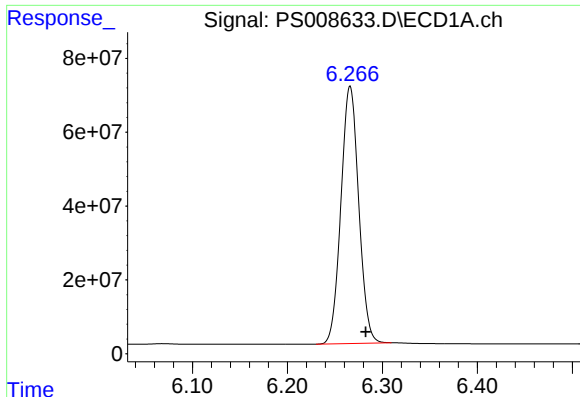

#4 2,4-DCAA


R.T.: 6.266 min
Delta R.T.: -0.017 min
Response: 906895396
Conc: 513.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

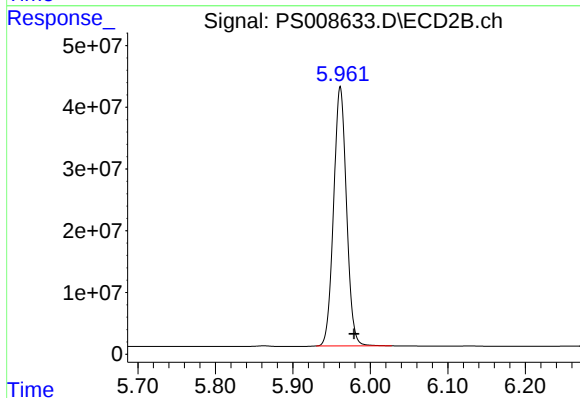


#4 2,4-DCAA

R.T.: 5.961 min
Delta R.T.: -0.018 min
Response: 485884062
Conc: 512.83 ng/ml

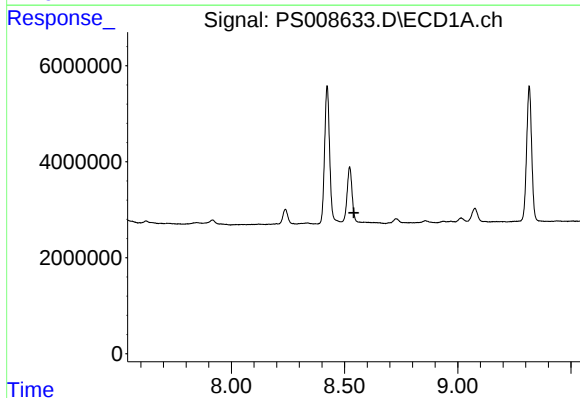


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

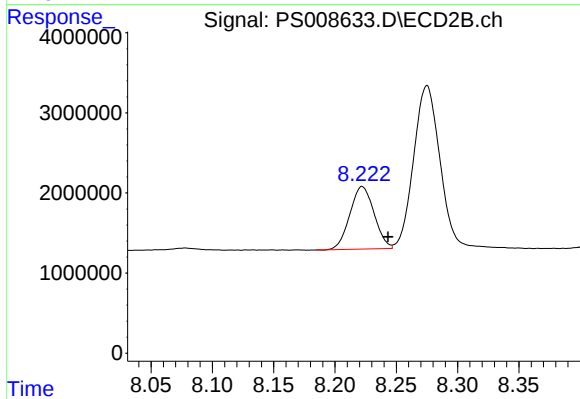

#12 2,4,5-T


R.T.: 8.222 min
Delta R.T.: -0.021 min
Response: 10735022
Conc: 2.03 ng/ml

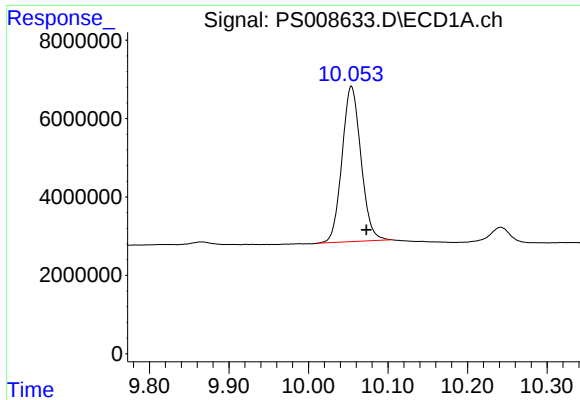

#15 Picloram


R.T.: 10.054 min
Delta R.T.: -0.019 min
Response: 65399202
Conc: 5.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

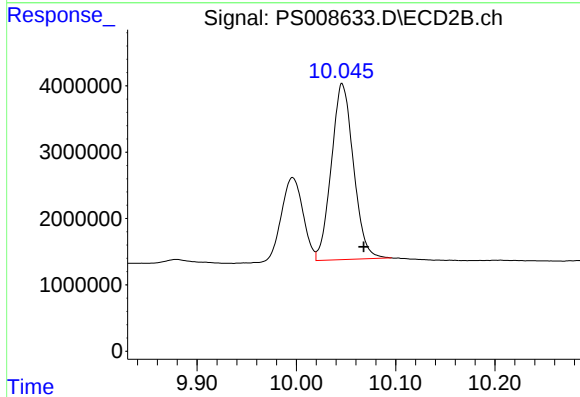


#15 Picloram

R.T.: 10.046 min
Delta R.T.: -0.022 min
Response: 41002501
Conc: 5.52 ng/ml

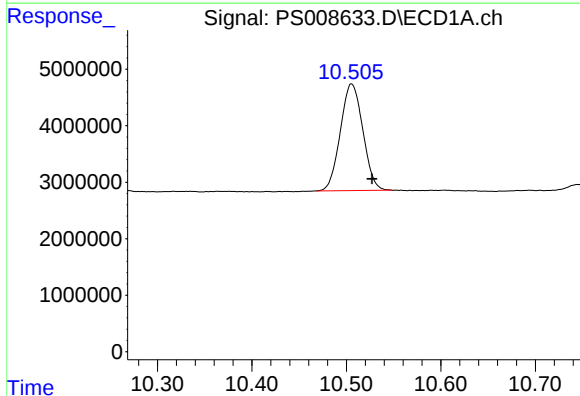

#16 DCPA

R.T.: 10.505 min
Delta R.T.: -0.022 min
Response: 31250603
Conc: 2.63 ng/ml

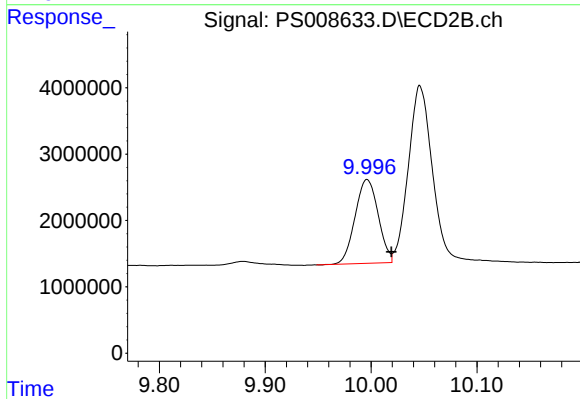

#16 DCPA

R.T.: 9.996 min
Delta R.T.: -0.023 min
Response: 19115792
Conc: 2.93 ng/ml