

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
 Data File : PS013898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 08:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:00:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.209	6.911	437.5E6	203.5E6	406.654	527.516	#
Target Compounds								
15) T	Picloram	10.987	0.000	8782318	0	1.034	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
Data File : PS013898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 08:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:00:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

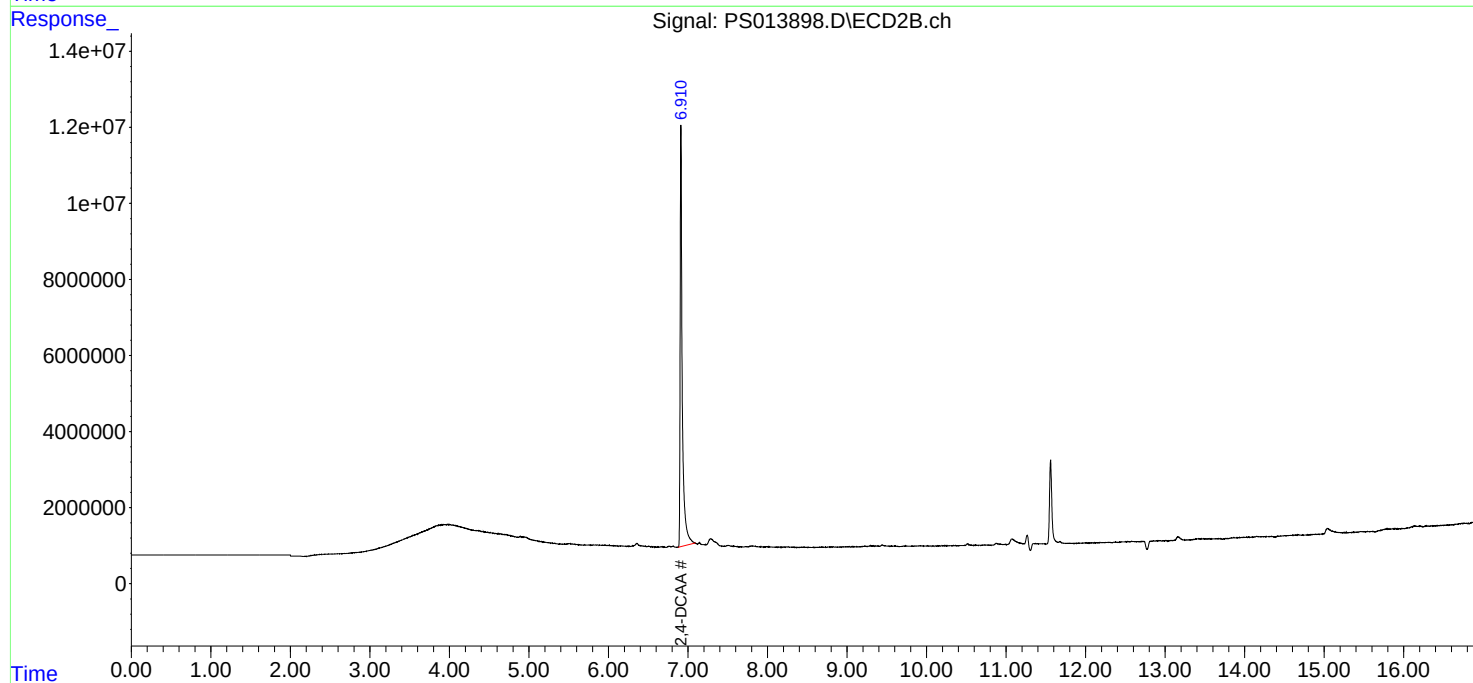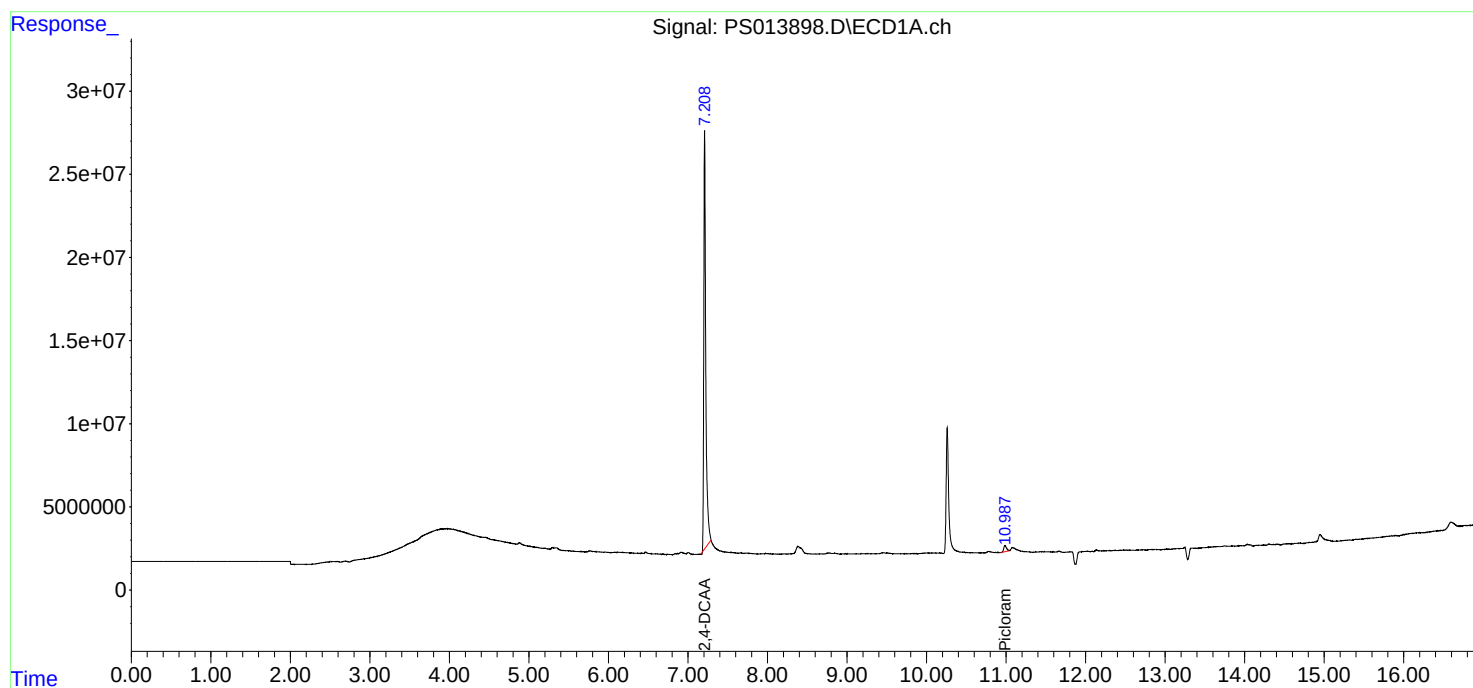


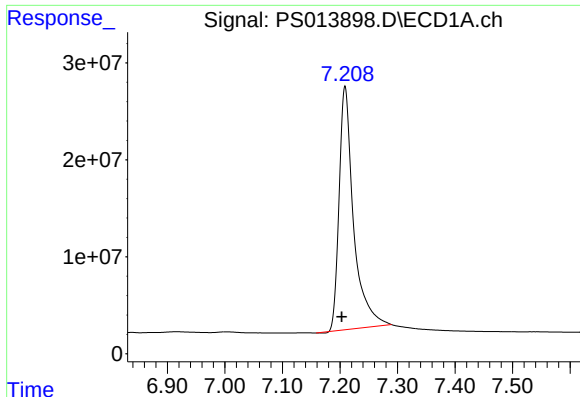

#4 2,4-DCAA


R.T.: 7.209 min
Delta R.T.: 0.006 min
Response: 437501019
Conc: 406.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

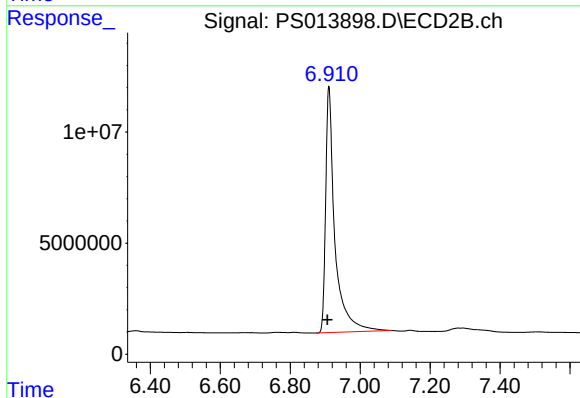


#4 2,4-DCAA

R.T.: 6.911 min
Delta R.T.: 0.005 min
Response: 203491070
Conc: 527.52 ng/ml

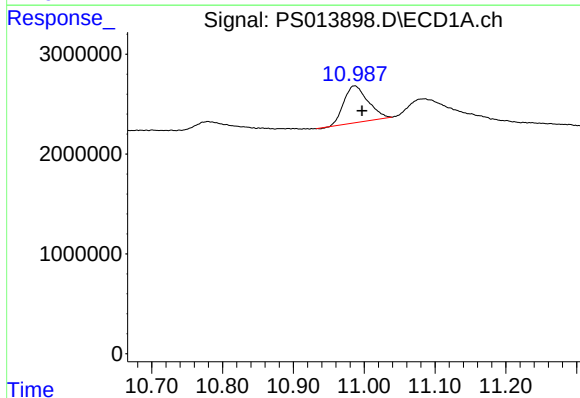

#15 Picloram

R.T.: 10.987 min
Delta R.T.: -0.010 min
Response: 8782318
Conc: 1.03 ng/ml

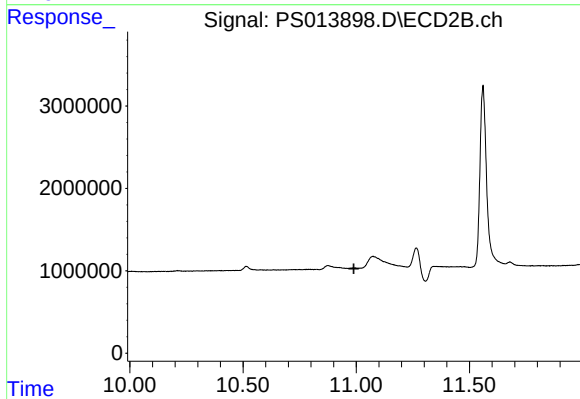

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.990 min
Response: 0
Conc: N.D.