

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
 Data File : PS013899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 09:17
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:00:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	6.906	828.6E6	296.9E6	770.158	769.669
Target Compounds							
1) T	Dalapon	3.027	2.621	833.5E6	350.1E6	667.808	680.988
2) T	3,5-DICHL...	6.421	6.062	1058.3E6	436.9E6	712.142	719.619
3) T	4-Nitroph...	7.038	6.521	372.9E6	172.3E6	686.330	685.176
5) T	DICAMBA	7.392	7.072	3173.7E6	1218.8E6	738.117	739.564
6) T	MCP	7.560	7.166	239.4E6	100.4E6	75.876	74.778
7) T	MCPA	7.709	7.381	335.4E6	141.3E6	74.098	72.882
8) T	DICHLORPROP	8.083	7.697	791.7E6	311.7E6	728.401	732.675
9) T	2,4-D	8.316	7.995	908.1E6	386.8E6	739.568	725.600
10) T	Pentachlo...	8.621	8.418	11569.1E6	4089.9E6	730.540	734.174
11) T	2,4,5-TP ...	9.170	8.780	4633.3E6	1703.9E6	737.920	742.288
12) T	2,4,5-T	9.457	9.161	4710.2E6	1653.3E6	731.272	742.490
13) T	2,4-DB	10.011	9.667	787.7E6	222.5E6	713.550	744.067
14) T	DINOSEB	11.162	9.995	3574.2E6	1178.7E6	705.253	721.460
15) T	Picloram	10.997	10.989	6065.1E6	2373.8E6	714.287	695.575
16) T	DCPA	11.428	10.921	5920.8E6	2216.9E6	732.426	739.968



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
Data File : PS013899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 09:17
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:00:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

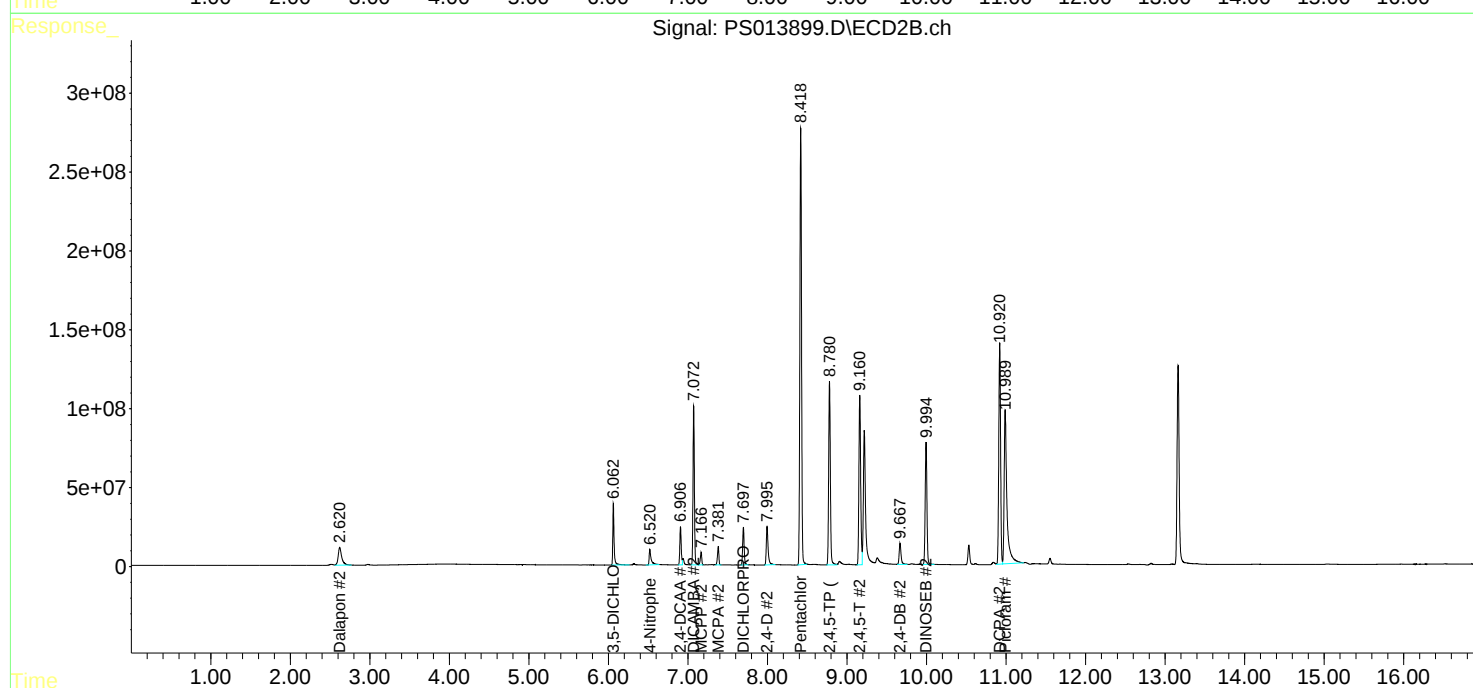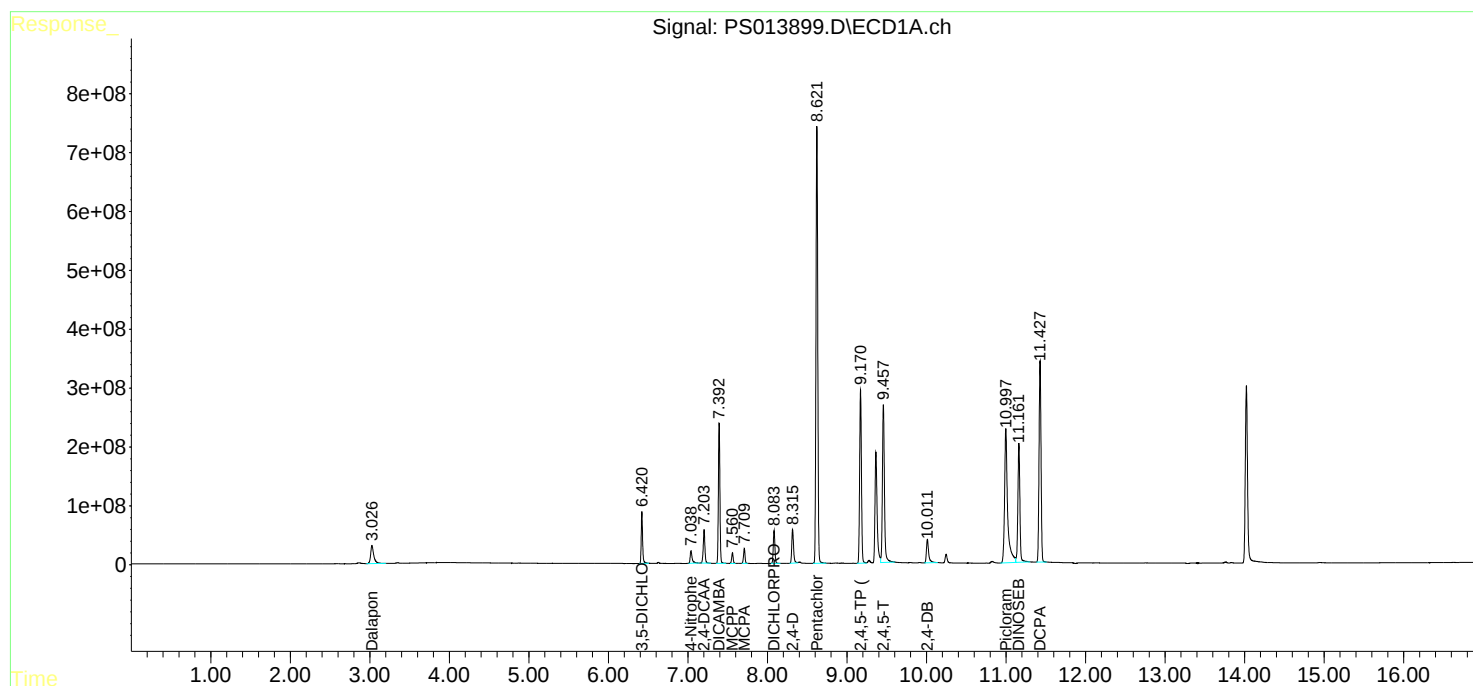


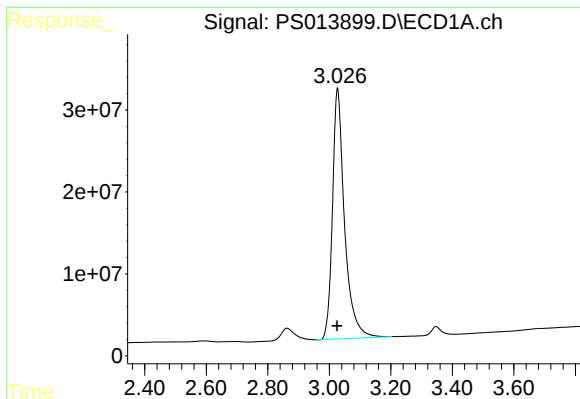

#1 Dalapon


R.T.: 3.027 min
Delta R.T.: 0.000 min
Response: 833475310
Conc: 667.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

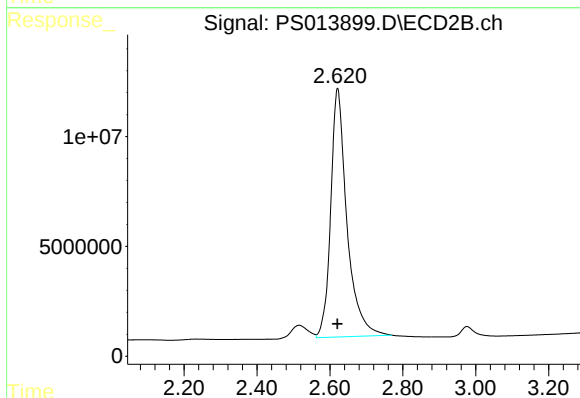


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 350137875
Conc: 680.99 ng/ml

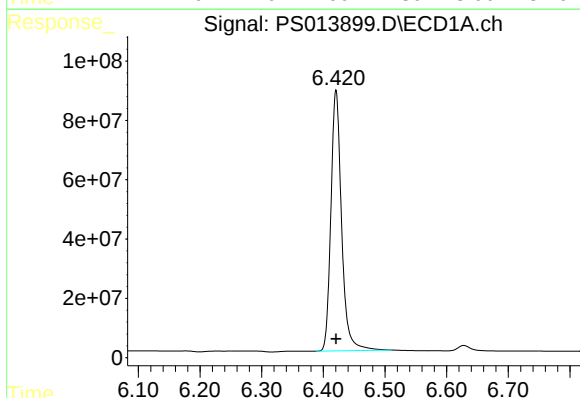


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 1058269085
Conc: 712.14 ng/ml

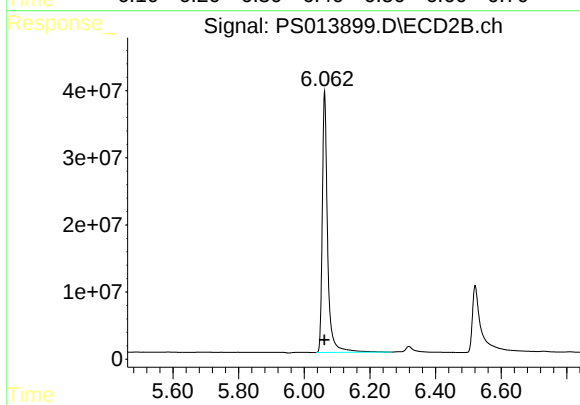

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 436913697
Conc: 719.62 ng/ml

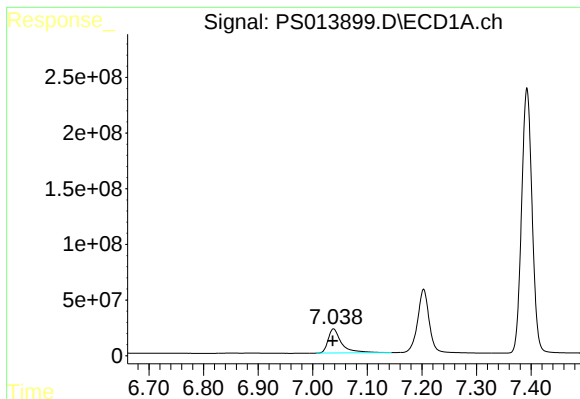

#3 4-Nitrophenol


R.T.: 7.038 min
Delta R.T.: 0.001 min
Response: 372939712
Conc: 686.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

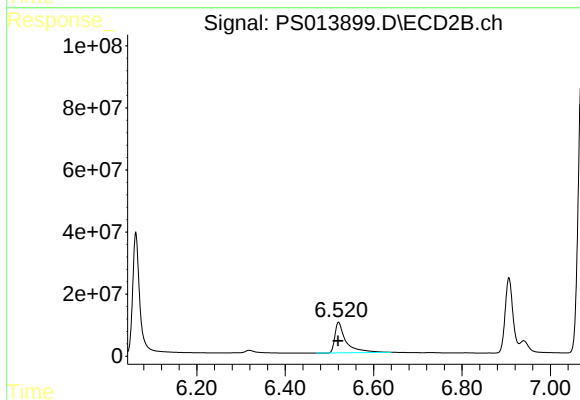


#3 4-Nitrophenol

R.T.: 6.521 min
Delta R.T.: 0.001 min
Response: 172304389
Conc: 685.18 ng/ml

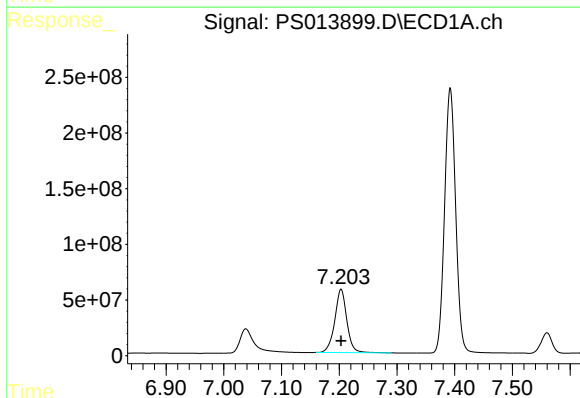


#4 2,4-DCAA

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 828577997
Conc: 770.16 ng/ml

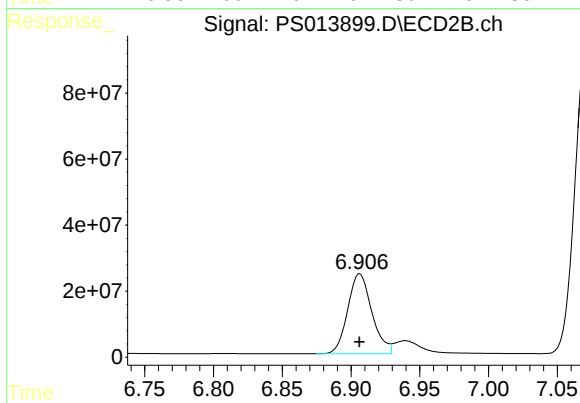

#4 2,4-DCAA


R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 296901973
Conc: 769.67 ng/ml

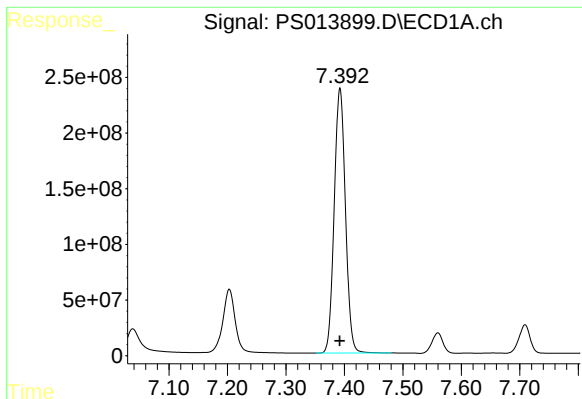

#5 DICAMBA


R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 3173732158
Conc: 738.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

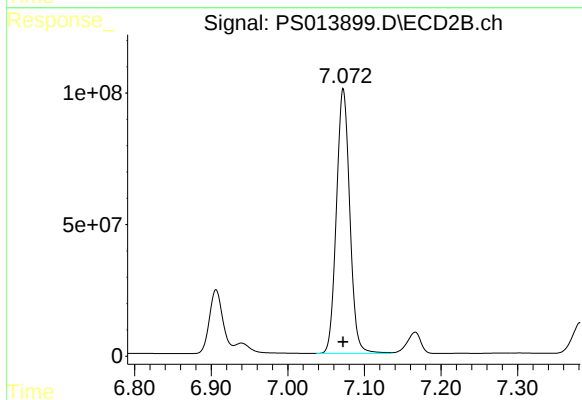


#5 DICAMBA

R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 1218765919
Conc: 739.56 ng/ml

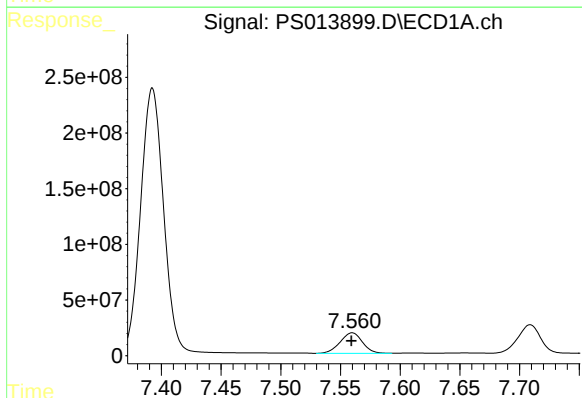


#6 MCP

R.T.: 7.560 min
Delta R.T.: 0.000 min
Response: 239437979
Conc: 75.88 ug/ml

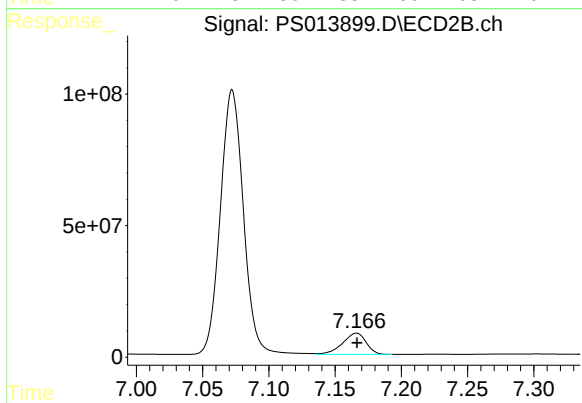

#6 MCP


R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 100433163
Conc: 74.78 ug/ml

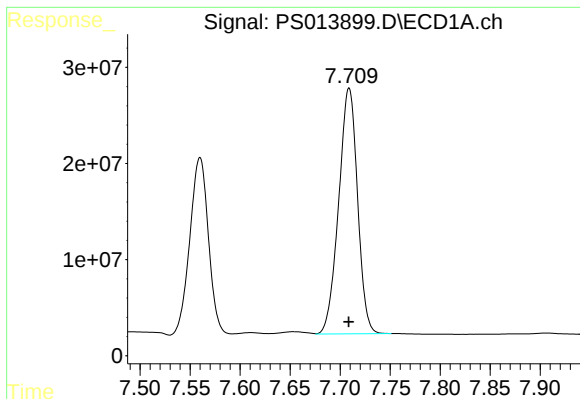

#7 MCPA


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 335352669
Conc: 74.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

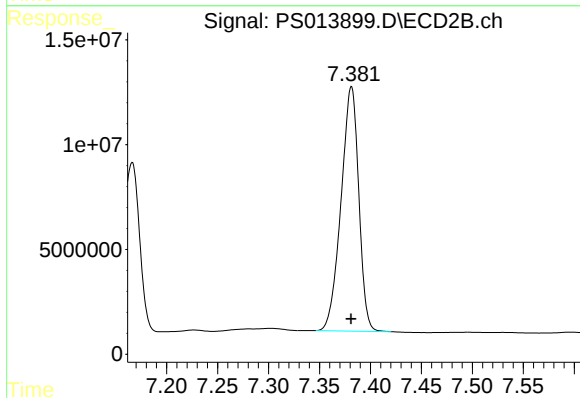


#7 MCPA

R.T.: 7.381 min
Delta R.T.: 0.000 min
Response: 141285412
Conc: 72.88 ug/ml

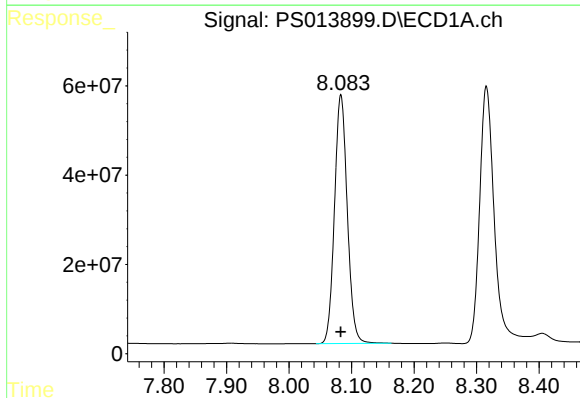


#8 DICHLORPROP

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 791716294
Conc: 728.40 ng/ml

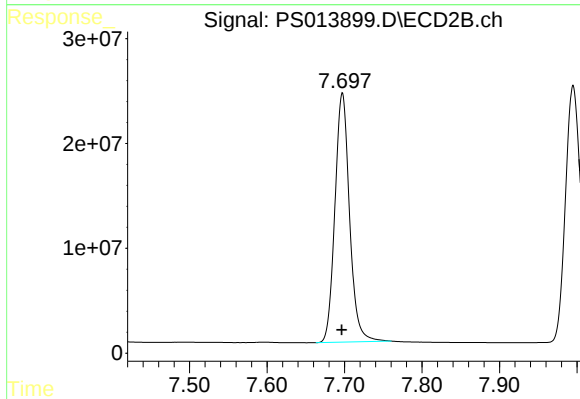

#8 DICHLORPROP


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 311737301
Conc: 732.68 ng/ml

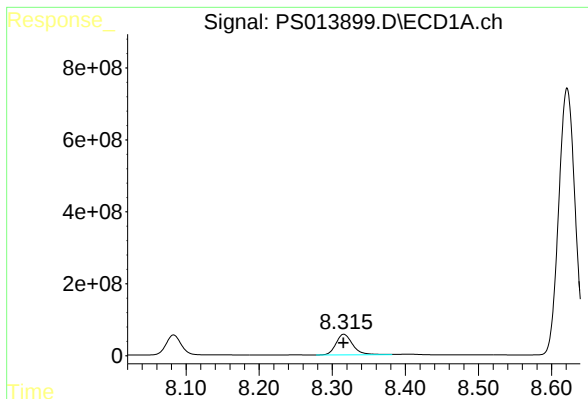

#9 2,4-D


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 908104811
Conc: 739.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

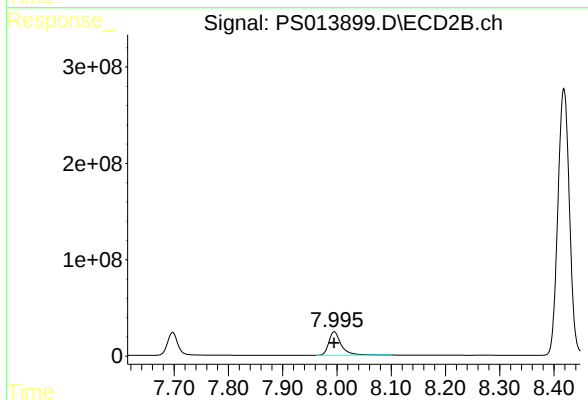


#9 2,4-D

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 386779761
Conc: 725.60 ng/ml

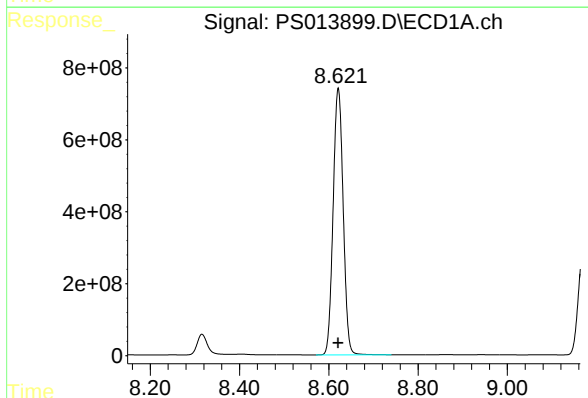


#10 Pentachlorophenol

R.T.: 8.621 min
Delta R.T.: 0.000 min
Response: 11569114948
Conc: 730.54 ng/ml

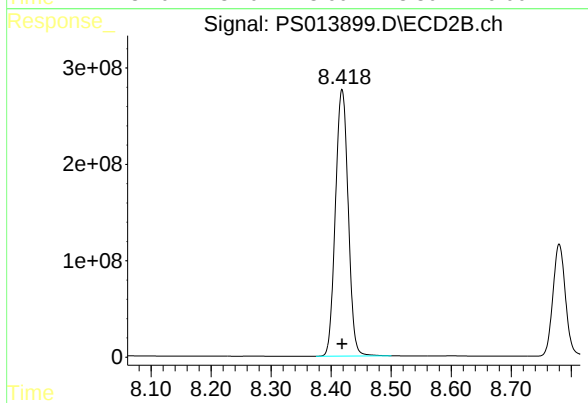

#10 Pentachlorophenol


R.T.: 8.418 min
Delta R.T.: 0.000 min
Response: 4089855113
Conc: 734.17 ng/ml

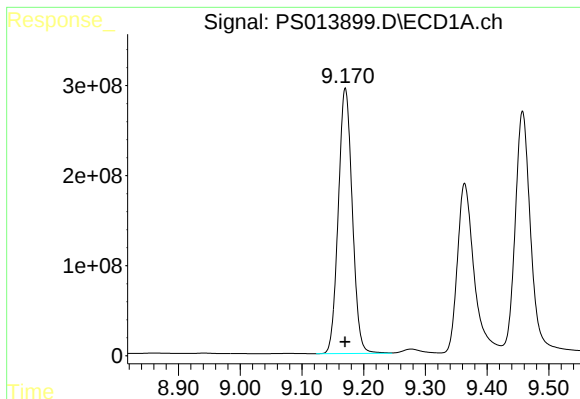

#11 2,4,5-TP (SILVEX)


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 4633324656
Conc: 737.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

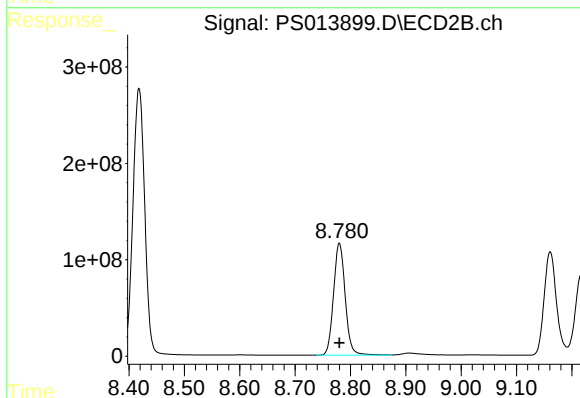


#11 2,4,5-TP (SILVEX)

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 1703935735
Conc: 742.29 ng/ml

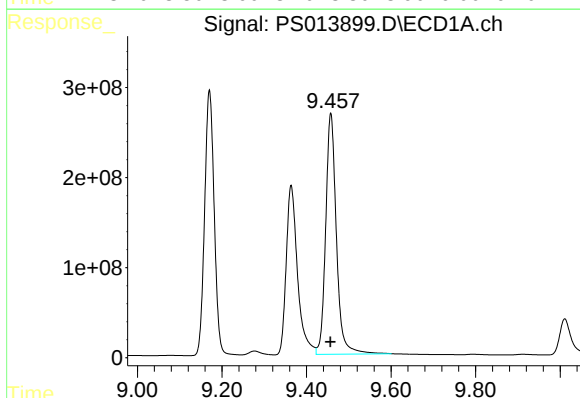


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: 0.000 min
Response: 4710212526
Conc: 731.27 ng/ml

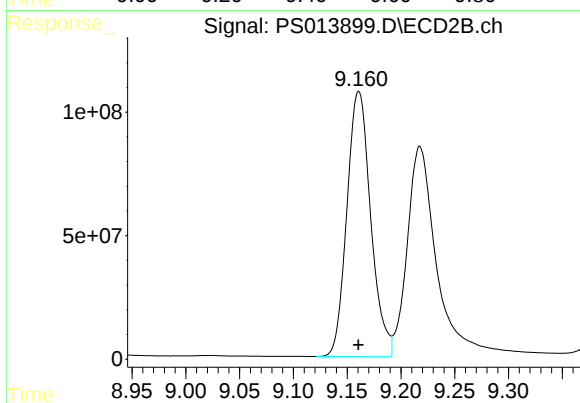

#12 2,4,5-T


R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 1653338221
Conc: 742.49 ng/ml

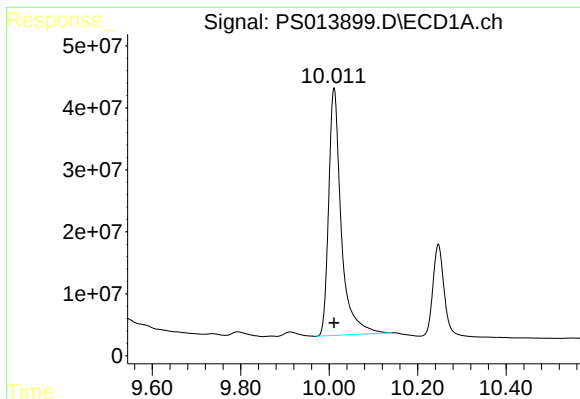

#13 2,4-DB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 787656963
Conc: 713.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

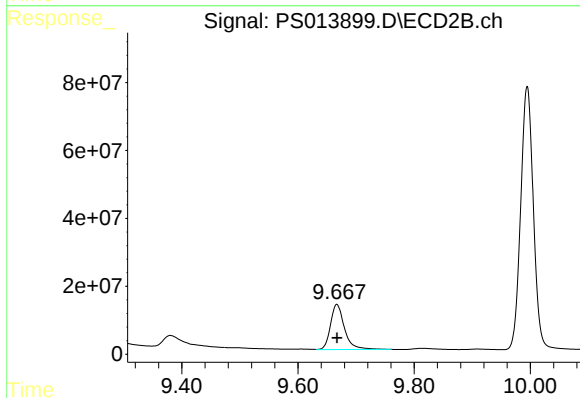


#13 2,4-DB

R.T.: 9.667 min
Delta R.T.: 0.000 min
Response: 222489470
Conc: 744.07 ng/ml

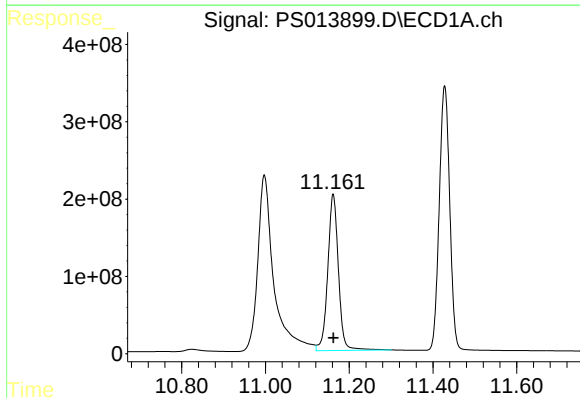


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: 0.000 min
Response: 3574226042
Conc: 705.25 ng/ml

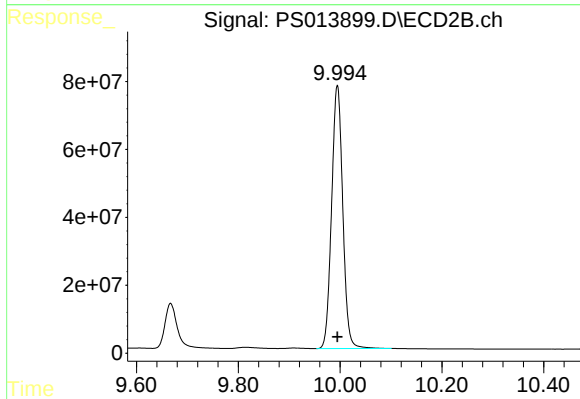

#14 DINOSEB


R.T.: 9.995 min
Delta R.T.: 0.000 min
Response: 1178655545
Conc: 721.46 ng/ml

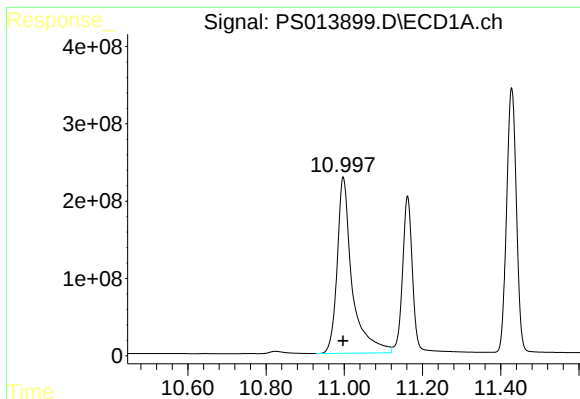

#15 Picloram


R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 6065111171
Conc: 714.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

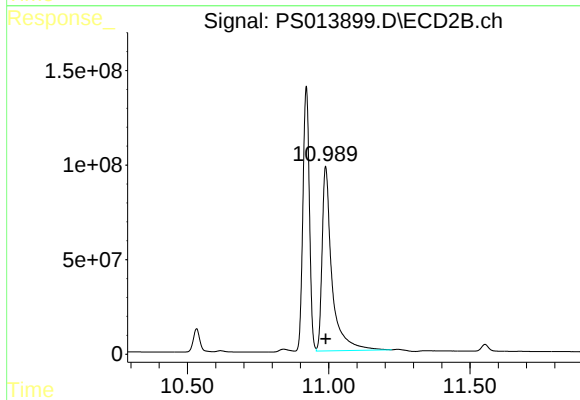


#15 Picloram

R.T.: 10.989 min
Delta R.T.: 0.000 min
Response: 2373751952
Conc: 695.58 ng/ml

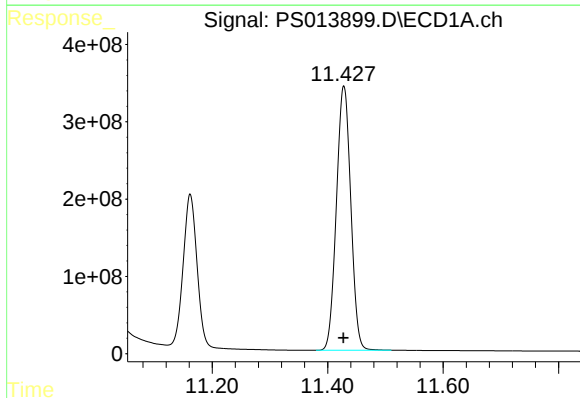

#16 DCPA

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 5920836577
Conc: 732.43 ng/ml

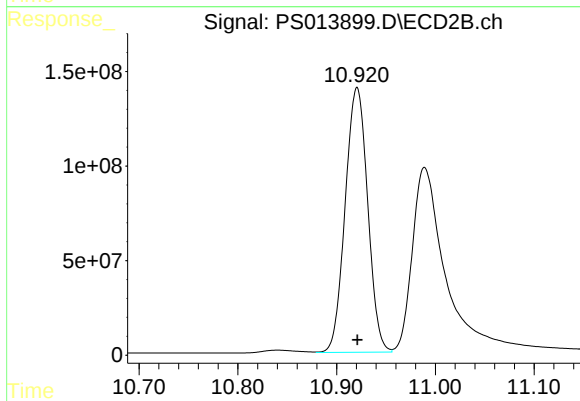

#16 DCPA

R.T.: 10.921 min
Delta R.T.: 0.000 min
Response: 2216860275
Conc: 739.97 ng/ml