

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
 Data File : PS013914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 20:36
 Operator : DD\AJ
 Sample : M1254-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CRT-15

Manual Integrations
 APPROVED

Ankita
 2/2/2021 12:01:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:03:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.201	6.904	373.8E6	112.9E6	347.399m	292.786m
Target Compounds							
10) T	Pentachlo...	8.621	8.417	1265.8E6	496.0E6	79.930	89.032

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012921\
Data File : PS013914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 20:36
Operator : DD\AJ
Sample : M1254-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CRT-15


Manual Integrations
APPROVED

Ankita
2/2/2021 12:01:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:03:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

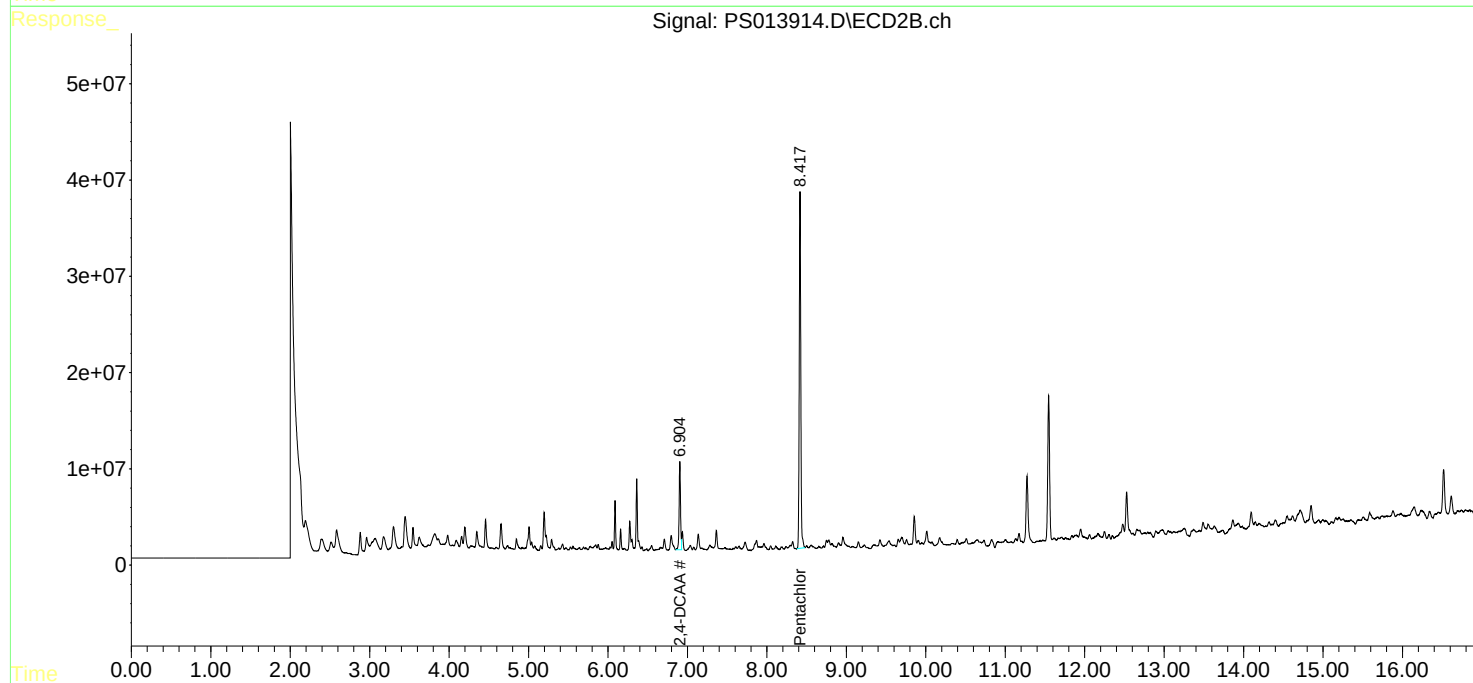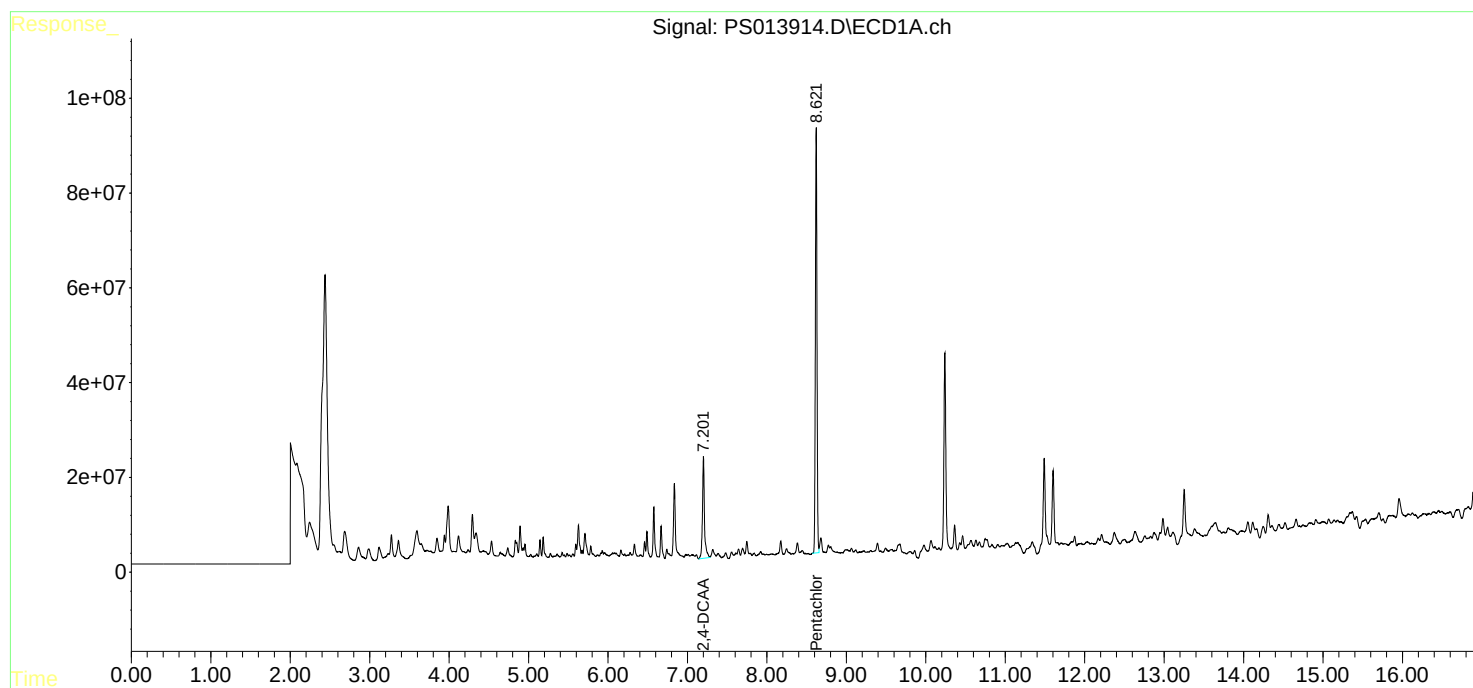

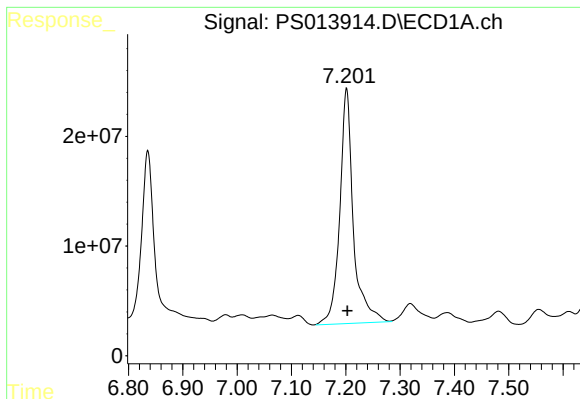


#4 2,4-DCAA

R.T.: 7.201 min
Delta R.T.: -0.002 min
Response: 373750850
Conc: 347.40 ng/ml m

Instrument :
ECD_S
ClientSampleId :
CRT-15


Manual Integrations
APPROVED

Ankita
2/2/2021 12:01:26 PM

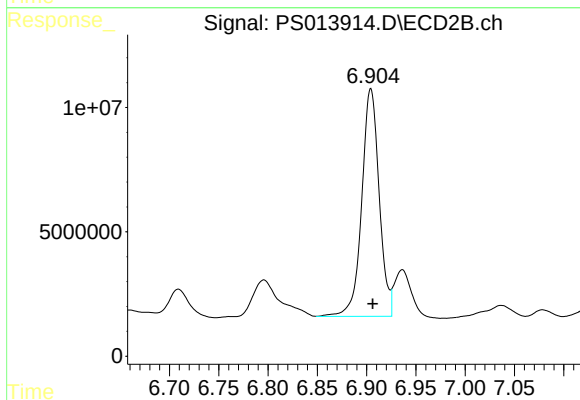


#4 2,4-DCAA

R.T.: 6.904 min
Delta R.T.: -0.002 min
Response: 112943035
Conc: 292.79 ng/ml m

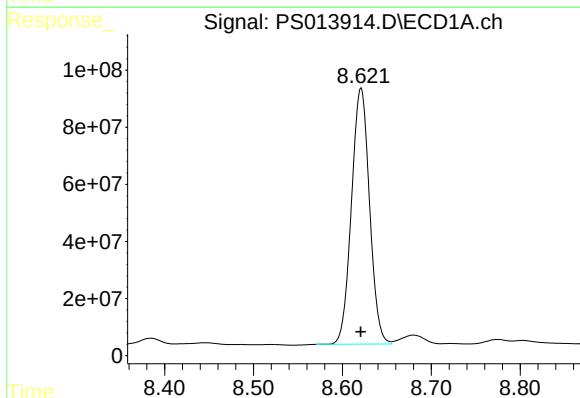

#10 Pentachlorophenol

R.T.: 8.621 min
Delta R.T.: 0.000 min
Response: 1265809383
Conc: 79.93 ng/ml

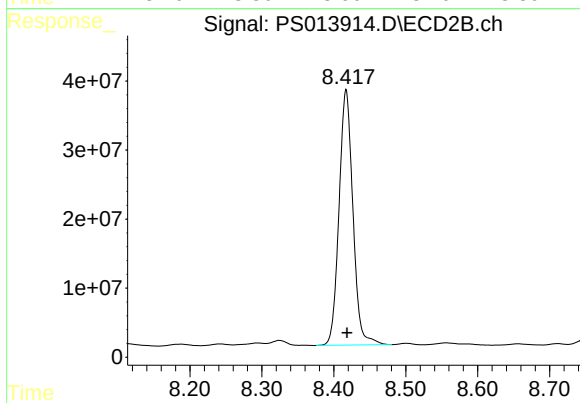

#10 Pentachlorophenol

R.T.: 8.417 min
Delta R.T.: -0.001 min
Response: 495968065
Conc: 89.03 ng/ml