

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
 Data File : PS025657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 09:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 14:35:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.554	0	820560	N.D. <MDL
5) T	DICAMBA	0.000	6.956	0	469.9E6	N.D. 141.205
6) T	MCP	0.000	6.956f	0	469.9E6	N.D. 202.567
7) T	MCPA	0.000	7.159f	0	10448303	N.D. 3.016
8) T	DICHLORPROP	0.000	7.564	0	2963928	N.D. 3.429
9) T	2,4-D	7.240	7.852	1431.4E6	577543	777.356 <MDL #
11) T	2,4,5-TP ...	0.000	8.595	0	505825	N.D. <MDL
14) T	DINOSEB	0.000	9.788	0	2421019	N.D. <MDL
15) T	Picloram	9.651	10.768	113.0E6	13925825	10.927 2.619 #
16) T	DCPA	0.000	10.724	0	7150995	N.D. 1.230



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
Data File : PS025657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 09:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 14:35:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

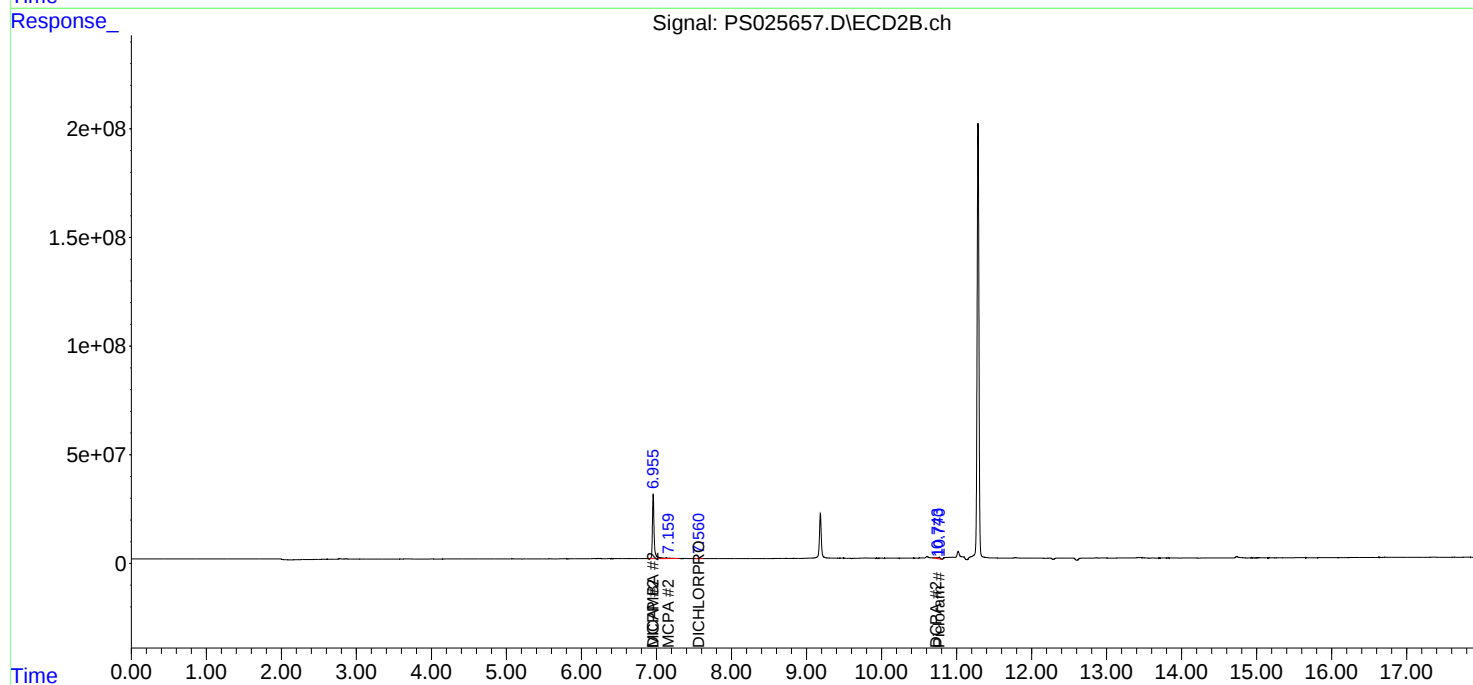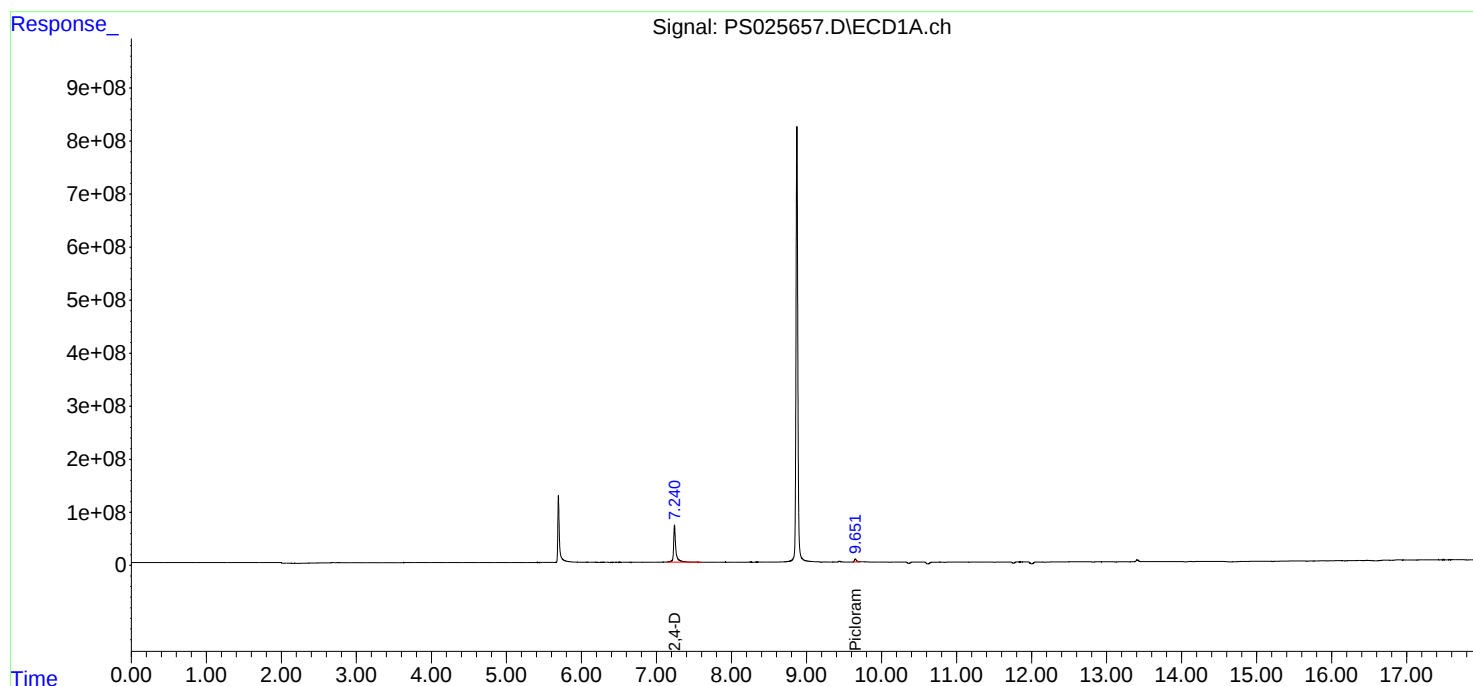


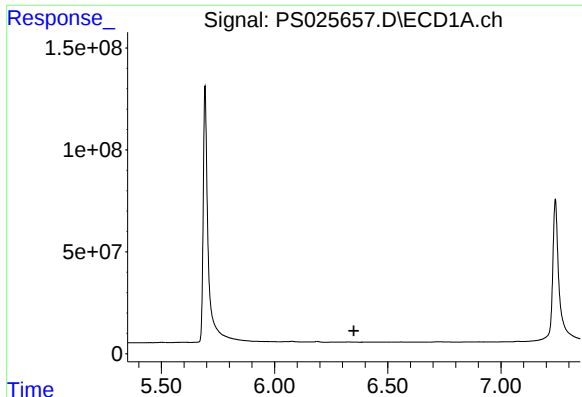

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

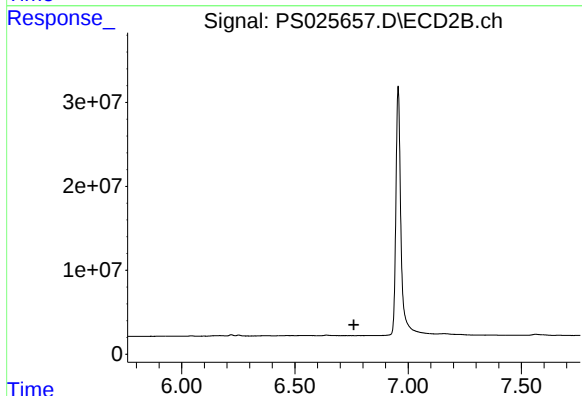


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.761 min
Response: 0
Conc: N.D.

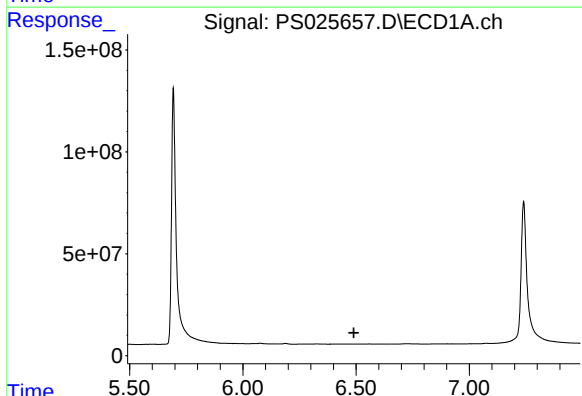


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

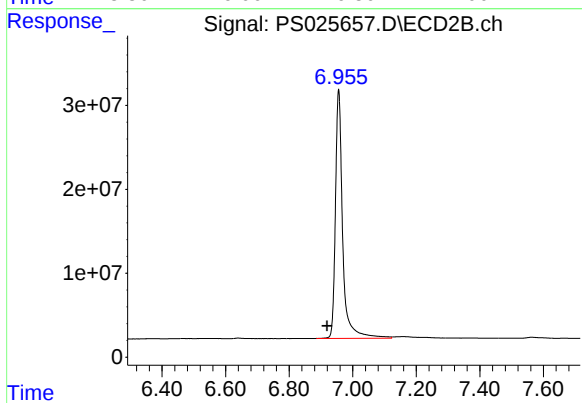

#5 DICAMBA


R.T.: 6.956 min
Delta R.T.: 0.036 min
Response: 469920535
Conc: 141.21 ng/ml

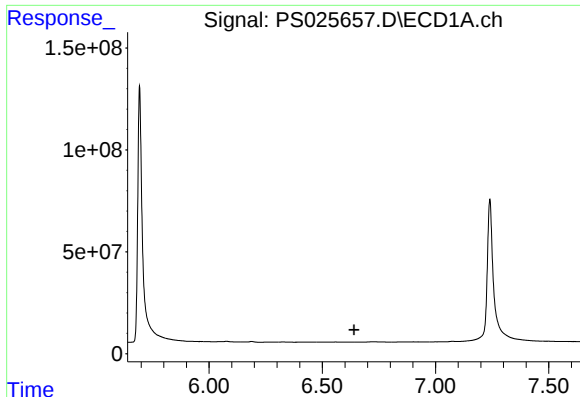

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

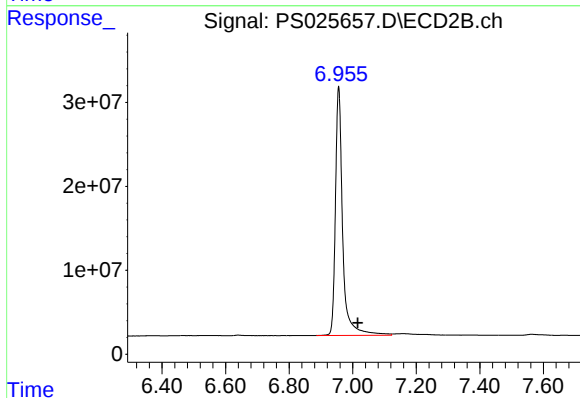


#6 MCPP

R.T.: 6.956 min
Delta R.T.: -0.060 min
Response: 469920535
Conc: 202.57 ug/ml

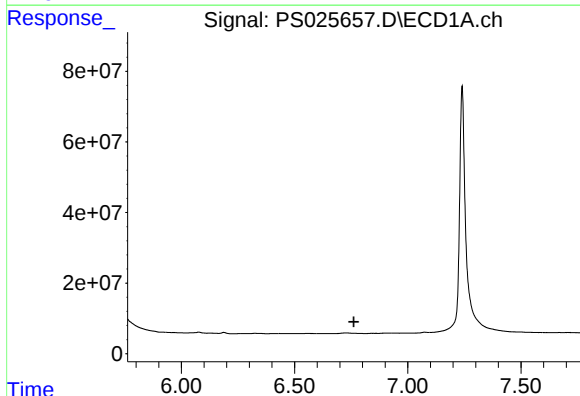


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

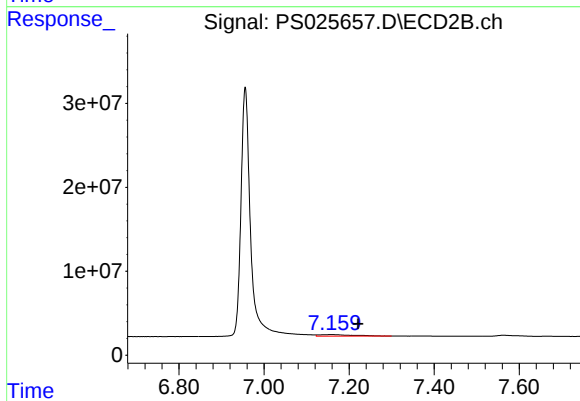

#7 MCPA


R.T.: 7.159 min
Delta R.T.: -0.062 min
Response: 10448303
Conc: 3.02 ug/ml

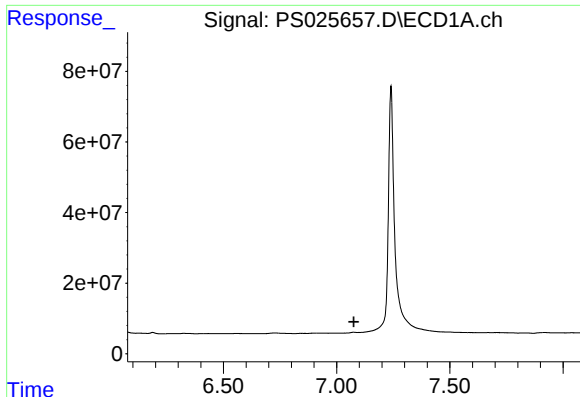

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

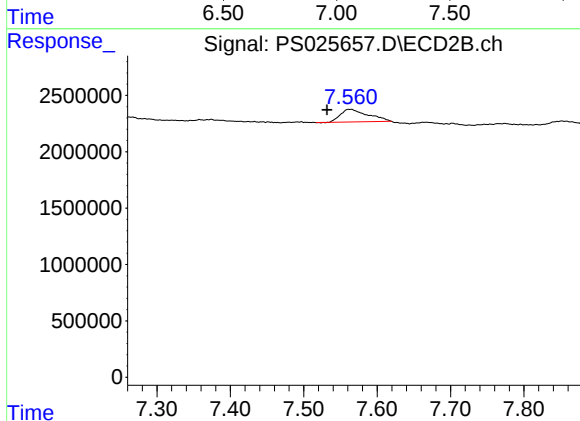


#8 DICHLORPROP

R.T.: 7.564 min
Delta R.T.: 0.033 min
Response: 2963928
Conc: 3.43 ng/ml

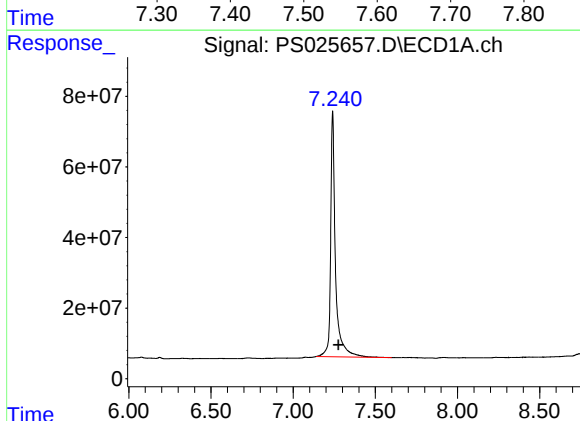


#9 2,4-D

R.T.: 7.240 min
Delta R.T.: -0.036 min
Response: 1431386009
Conc: 777.36 ng/ml

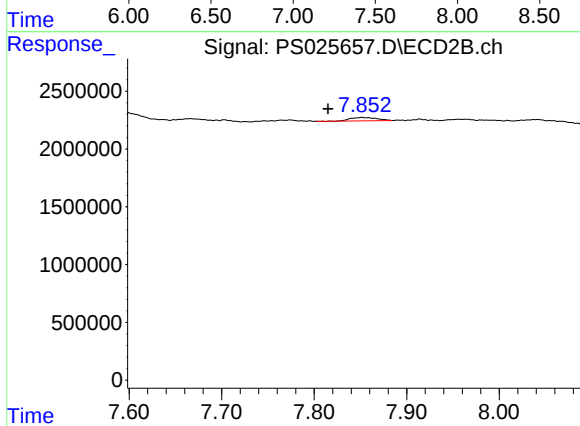

#9 2,4-D


R.T.: 7.852 min
Delta R.T.: 0.037 min
Response: 577543
Conc: N.D.

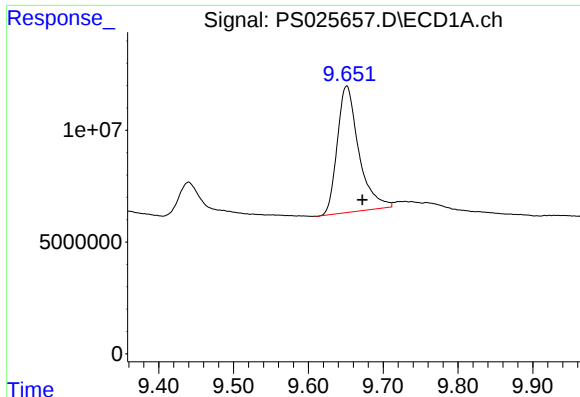

#15 Picloram


R.T.: 9.651 min
Delta R.T.: -0.021 min
Response: 113047020
Conc: 10.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

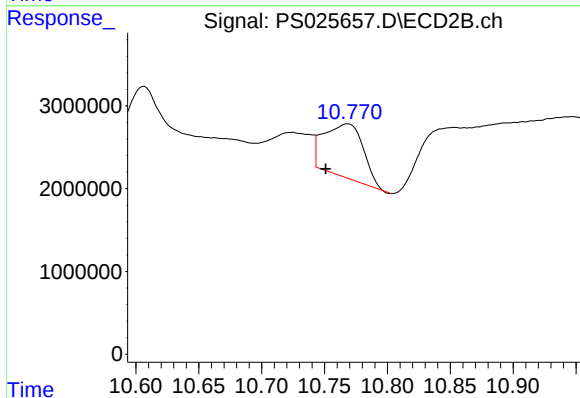


#15 Picloram

R.T.: 10.768 min
Delta R.T.: 0.017 min
Response: 13925825
Conc: 2.62 ng/ml

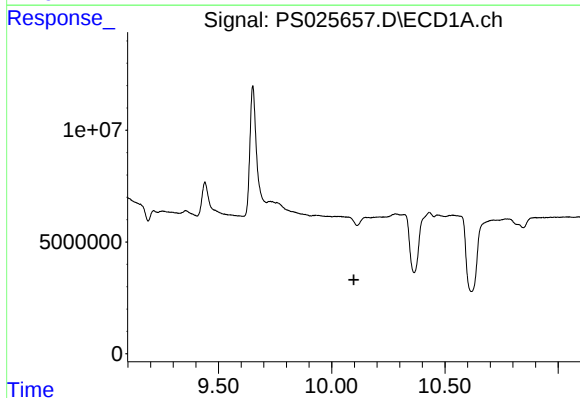

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.098 min
Response: 0
Conc: N.D.

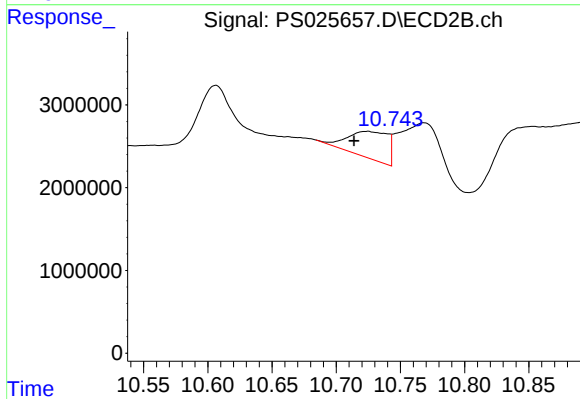

#16 DCPA

R.T.: 10.724 min
Delta R.T.: 0.011 min
Response: 7150995
Conc: 1.23 ng/ml