

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
 Data File : PS025681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 22:02
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:02:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.548	0	291083	N.D.	<MDL
5) T	DICAMBA	0.000	6.956	0	494.4E6	N.D.	148.562
6) T	MCPD	6.701f	6.956f	7346647	494.4E6	1.835	213.121 #
7) T	MCPA	6.701f	7.160f	7346647	19537932	1.298	5.639 #
8) T	DICHLORPROP	7.072	7.552	2203942	8455276	1.337	9.781 #
9) T	2,4-D	7.238	7.843	1207.3E6	2370081	655.642	2.609 #
10) T	Pentachlo...	0.000	8.236	0	866936	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.625	0	1465194	N.D.	<MDL
12) T	2,4,5-T	8.315	8.979	17712772	199906	1.814	<MDL #
13) T	2,4-DB	0.000	9.462	0	950372	N.D.	1.821
14) T	DINOSEB	0.000	9.783	0	927609	N.D.	<MDL
15) T	Picloram	9.644	10.763	155.2E6	14816031	15.001	2.787 #
16) T	DCPA	0.000	10.720	0	9833252	N.D.	1.691



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
Data File : PS025681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 22:02
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:02:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

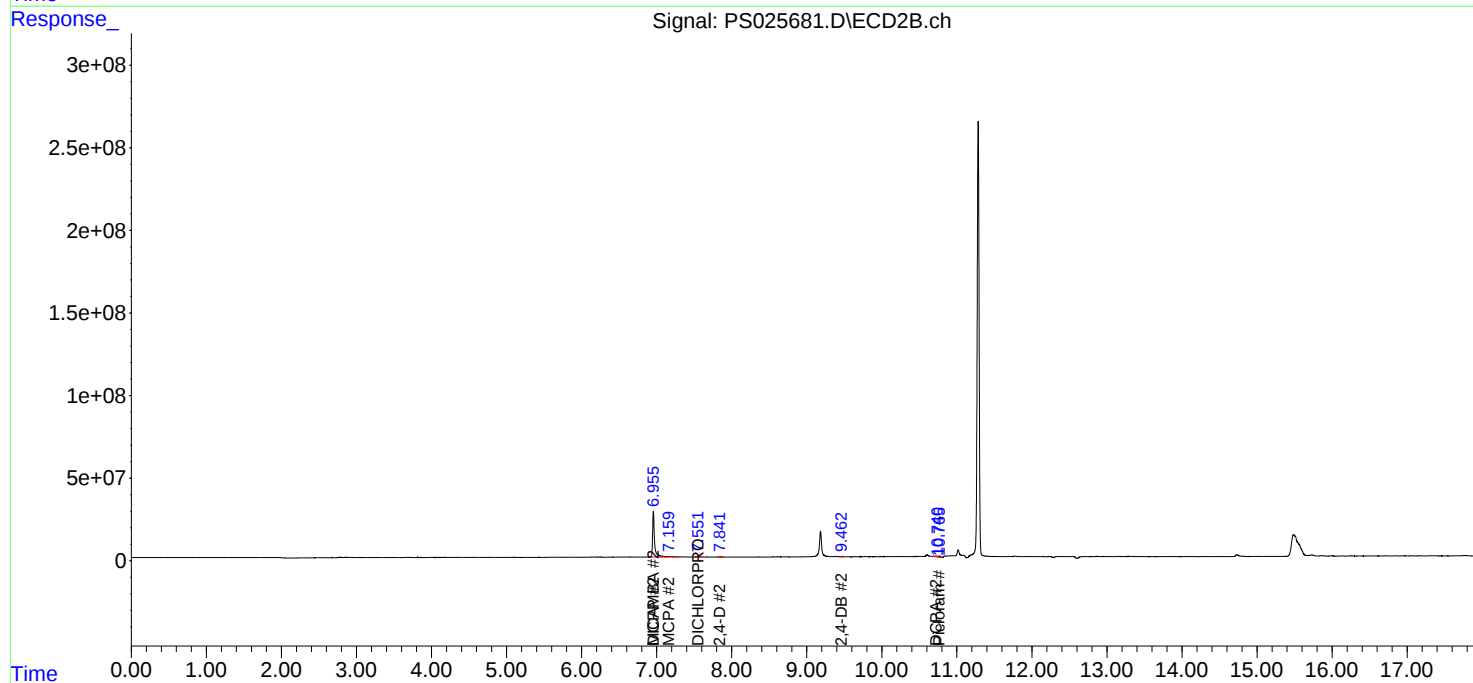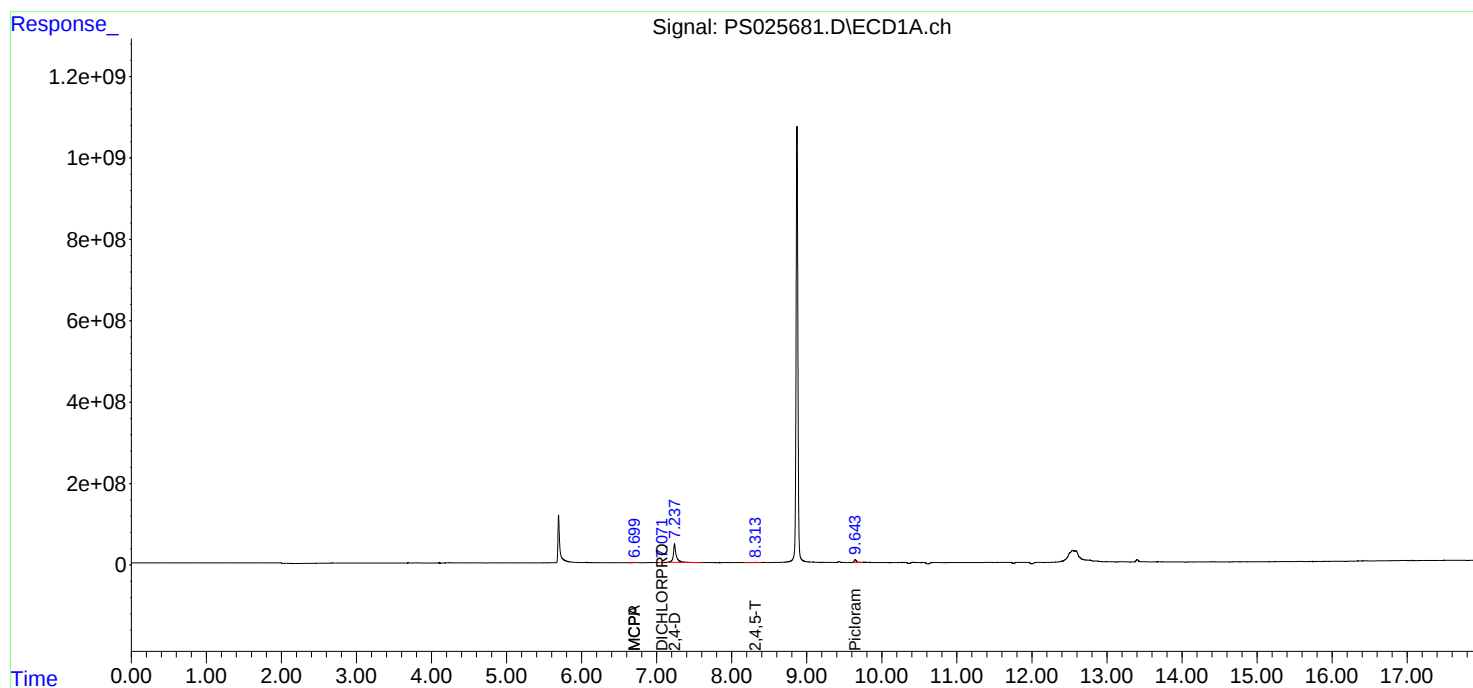


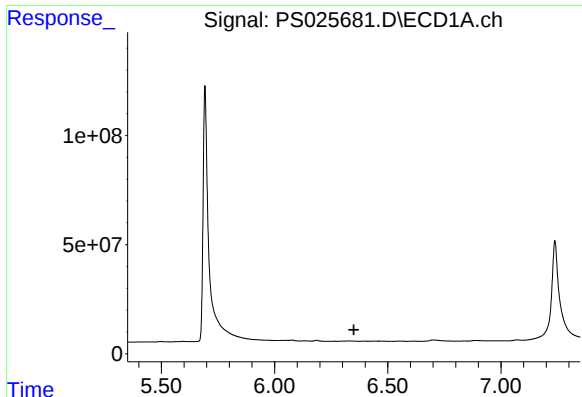

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

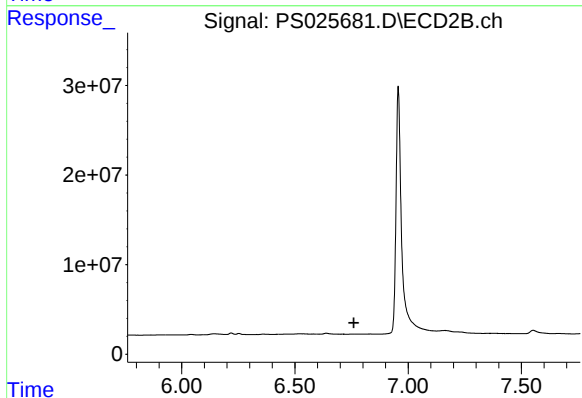


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.761 min
Response: 0
Conc: N.D.

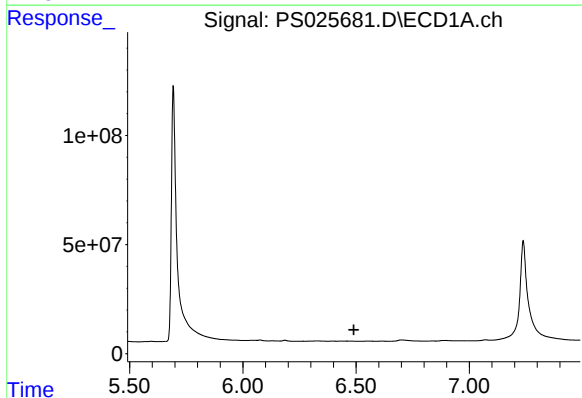


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

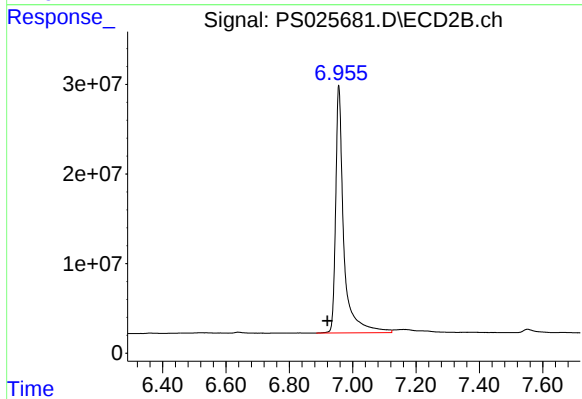

#5 DICAMBA


R.T.: 6.956 min
Delta R.T.: 0.036 min
Response: 494402989
Conc: 148.56 ng/ml

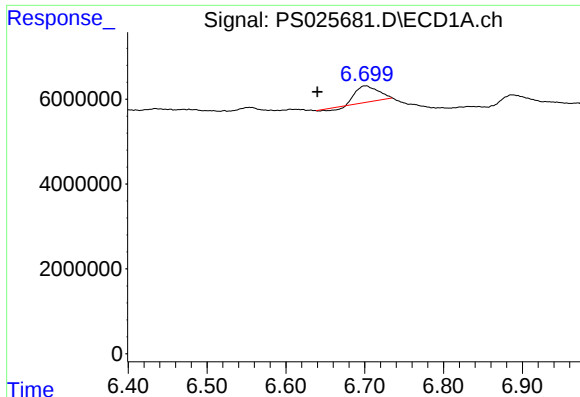

#6 MCPP


R.T.: 6.701 min
Delta R.T.: 0.061 min
Response: 7346647
Conc: 1.83 ug/ml

Instrument :
ECD_S
ClientSampleId :

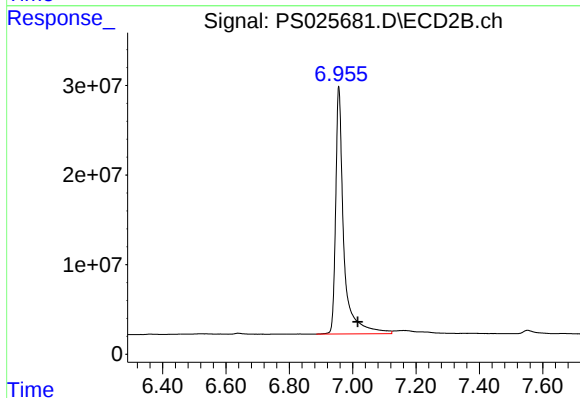


#6 MCPP

R.T.: 6.956 min
Delta R.T.: -0.060 min
Response: 494402989
Conc: 213.12 ug/ml

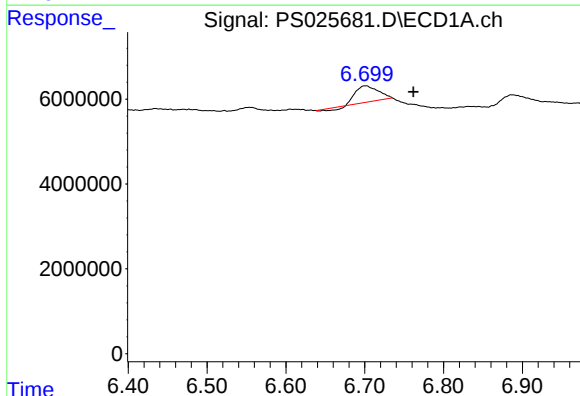


#7 MCPA

R.T.: 6.701 min
Delta R.T.: -0.061 min
Response: 7346647
Conc: 1.30 ug/ml

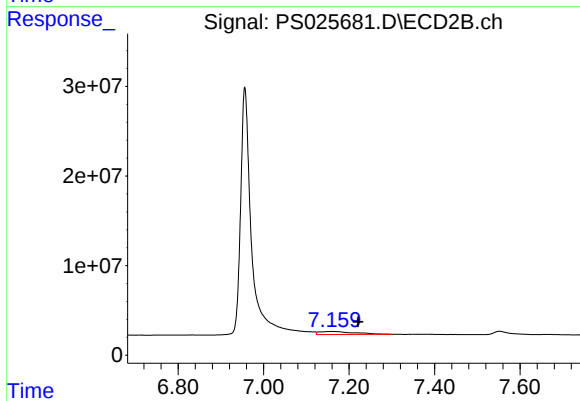

#7 MCPA


R.T.: 7.160 min
Delta R.T.: -0.061 min
Response: 19537932
Conc: 5.64 ug/ml

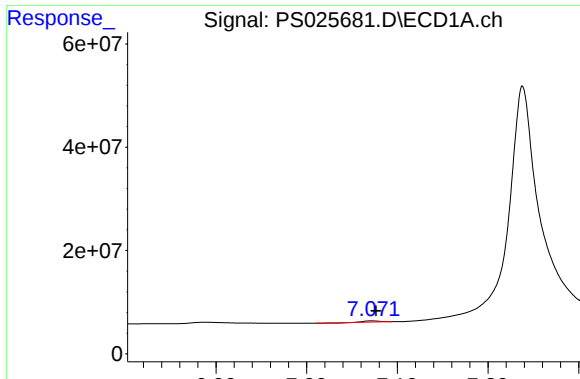

#8 DICHLORPROP


R.T.: 7.072 min
Delta R.T.: -0.005 min
Response: 2203942
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

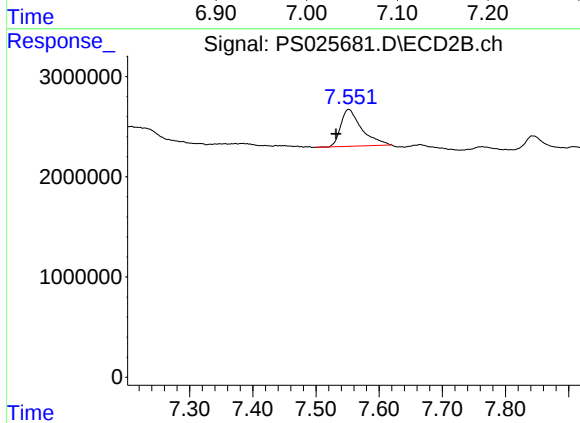


#8 DICHLORPROP

R.T.: 7.552 min
Delta R.T.: 0.020 min
Response: 8455276
Conc: 9.78 ng/ml

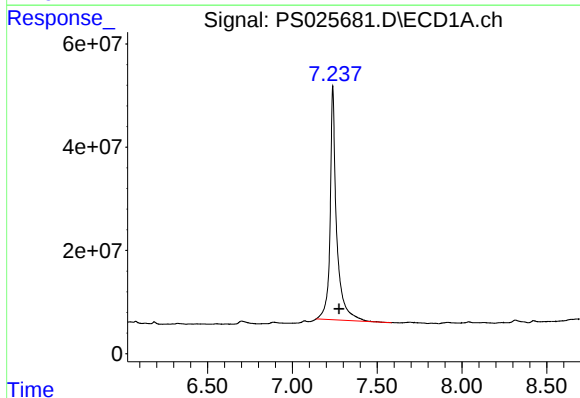


#9 2,4-D

R.T.: 7.238 min
Delta R.T.: -0.037 min
Response: 1207266504
Conc: 655.64 ng/ml

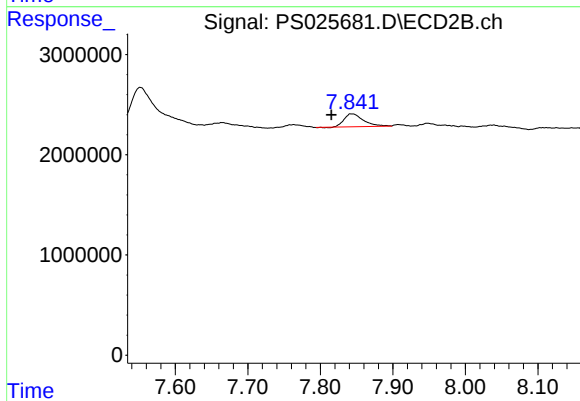

#9 2,4-D


R.T.: 7.843 min
Delta R.T.: 0.028 min
Response: 2370081
Conc: 2.61 ng/ml

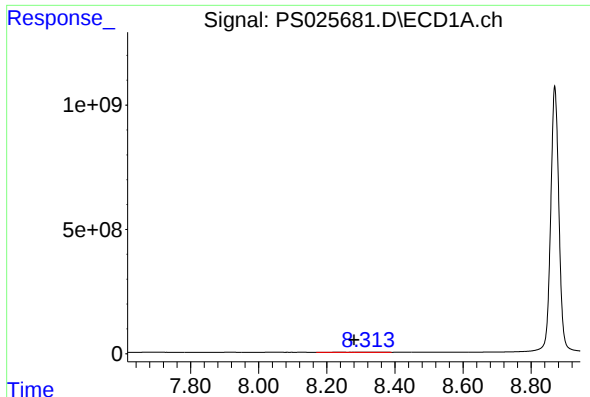

#12 2,4,5-T


R.T.: 8.315 min
Delta R.T.: 0.034 min
Response: 17712772
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

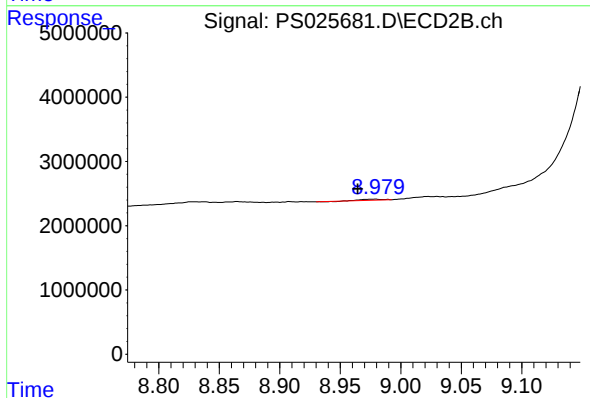


#12 2,4,5-T

R.T.: 8.979 min
Delta R.T.: 0.014 min
Response: 199906
Conc: N.D.

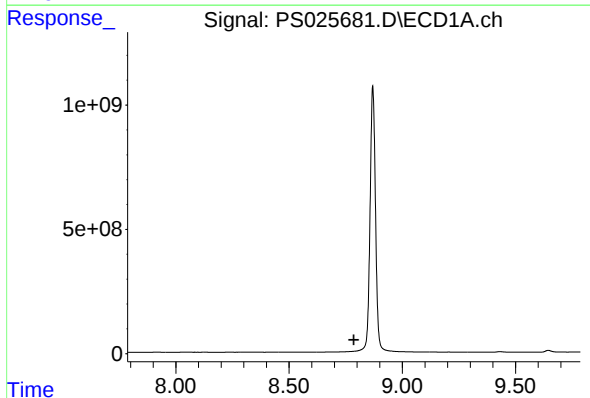


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.786 min
Response: 0
Conc: N.D.

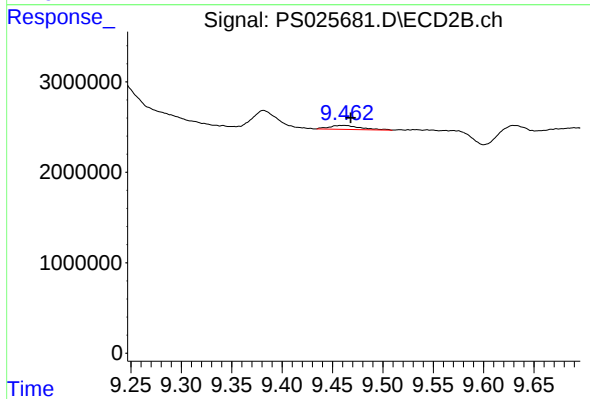

#13 2,4-DB


R.T.: 9.462 min
Delta R.T.: -0.006 min
Response: 950372
Conc: 1.82 ng/ml

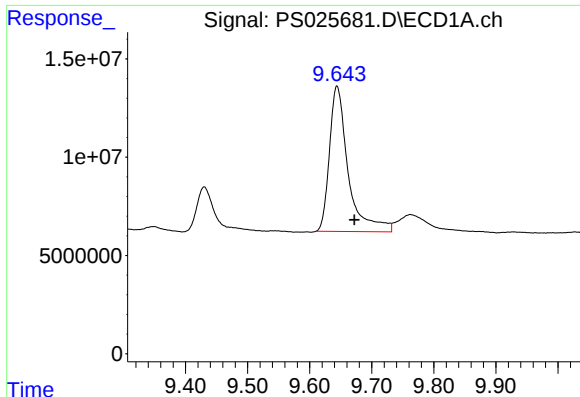

#15 Picloram


R.T.: 9.644 min
Delta R.T.: -0.028 min
Response: 155205809
Conc: 15.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

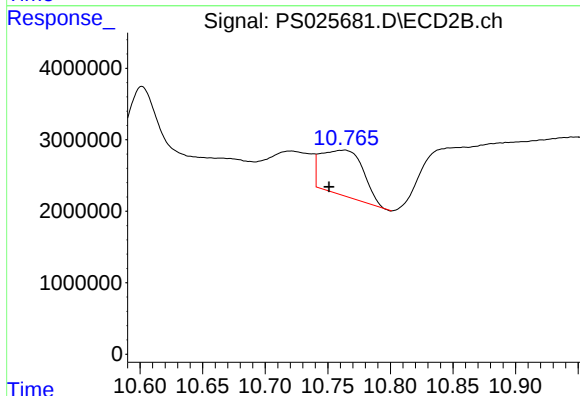


#15 Picloram

R.T.: 10.763 min
Delta R.T.: 0.012 min
Response: 14816031
Conc: 2.79 ng/ml

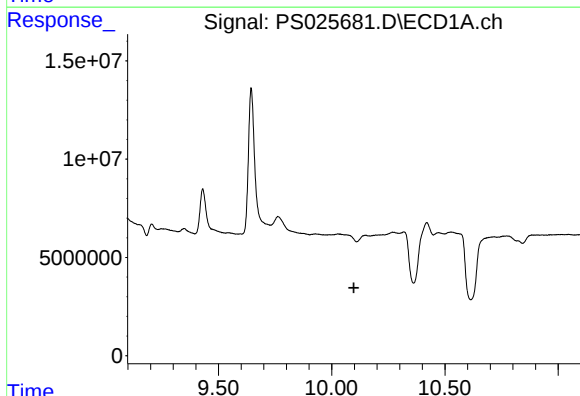

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.098 min
Response: 0
Conc: N.D.

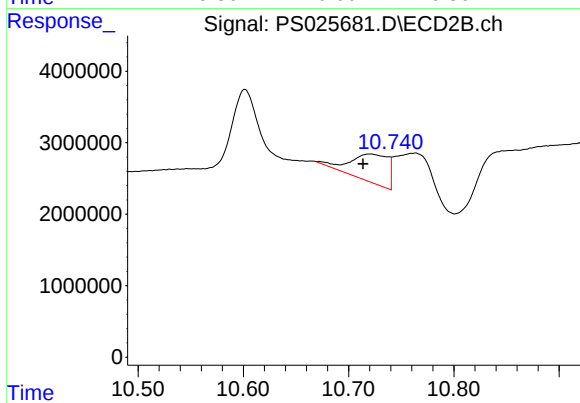

#16 DCPA

R.T.: 10.720 min
Delta R.T.: 0.007 min
Response: 9833252
Conc: 1.69 ng/ml