

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
 Data File : PS025682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 22:26
 Operator : AR\AJ
 Sample : I,BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:03:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.350	6.758	792.0E6	409.5E6	531.767	533.399
Target Compounds							
1) T	Dalapon	0.000	2.548	0	266640	N.D.	<MDL
3) T	4-Nitroph...	6.188	6.364	7189955	1423791	7.957	2.991 #
5) T	DICAMBA	0.000	6.956	0	283704	N.D.	<MDL
6) T	MCP	0.000	6.956f	0	283704	N.D.	<MDL
7) T	MCPA	6.713f	7.151f	9571674	8756816	1.691	2.527 #
8) T	DICHLORPROP	0.000	7.555	0	15478252	N.D.	17.905
9) T	2,4-D	0.000	7.764f	0	567623	N.D.	<MDL
12) T	2,4,5-T	0.000	9.025f	0	881524	N.D.	<MDL
13) T	2,4-DB	0.000	9.470	0	643928	N.D.	1.234
15) T	Picloram	0.000	10.780	0	722790	N.D.	<MDL
16) T	DCPA	0.000	10.711	0	331691	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012924\
Data File : PS025682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 22:26
Operator : AR\AJ
Sample : I,BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:03:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

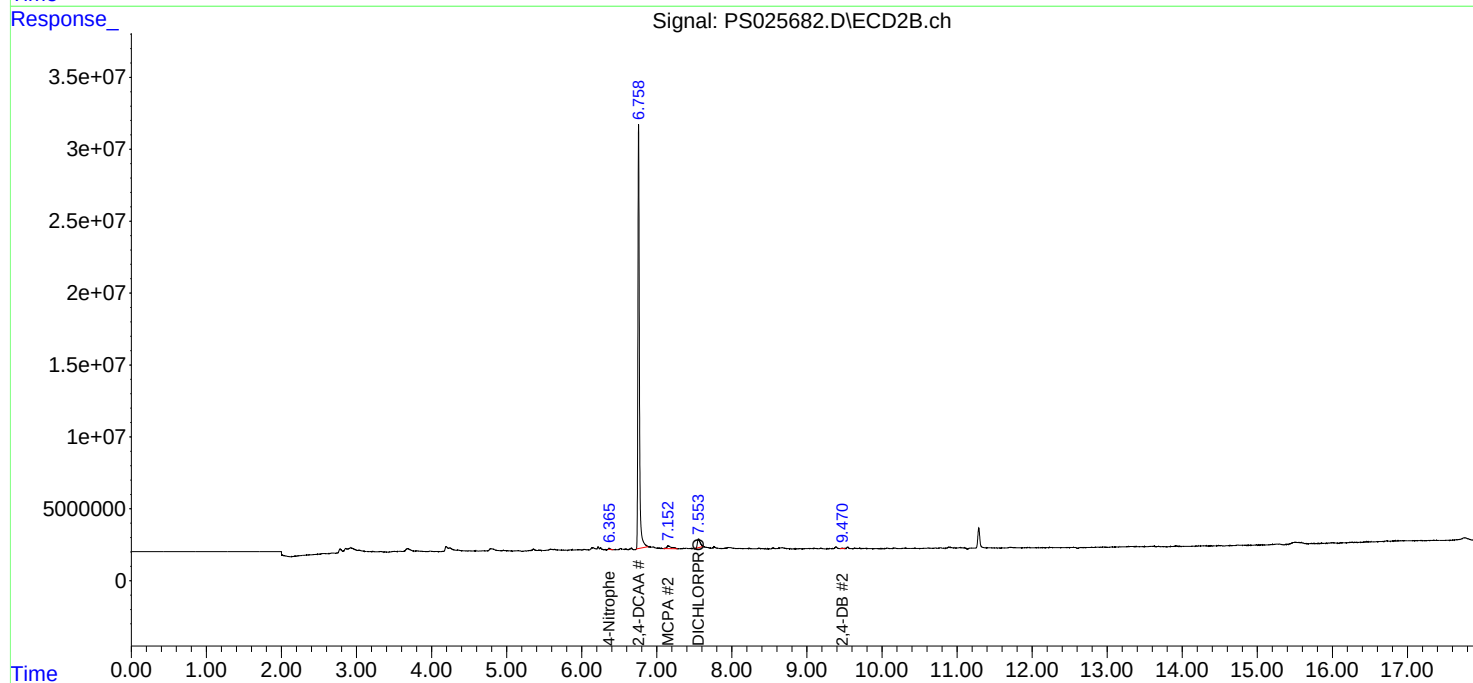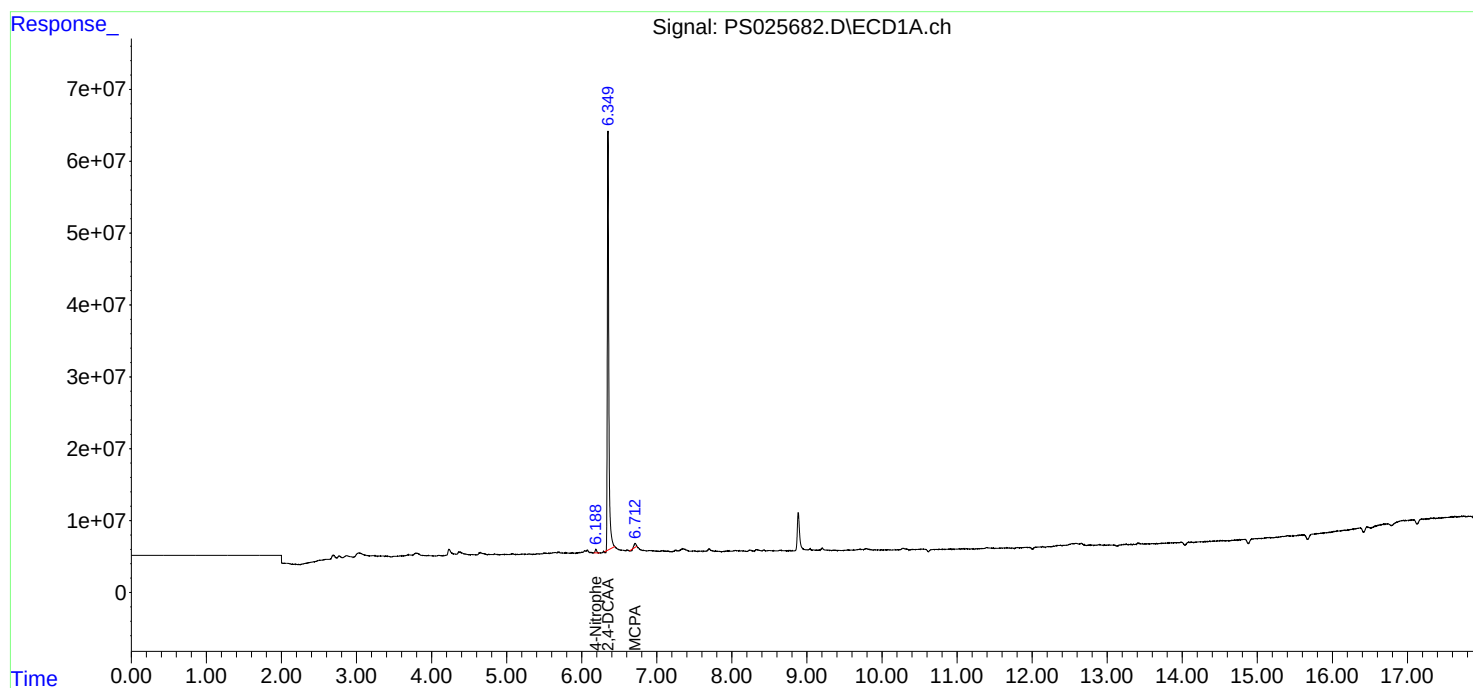


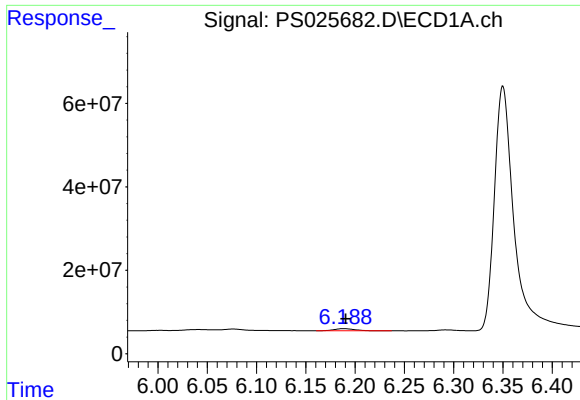

#3 4-Nitrophenol


R.T.: 6.188 min
Delta R.T.: -0.002 min
Response: 7189955
Conc: 7.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

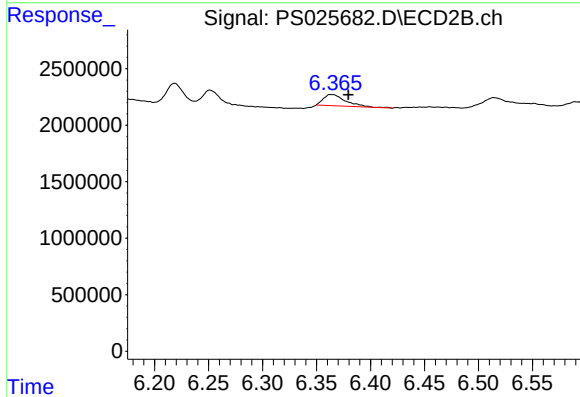


#3 4-Nitrophenol

R.T.: 6.364 min
Delta R.T.: -0.016 min
Response: 1423791
Conc: 2.99 ng/ml

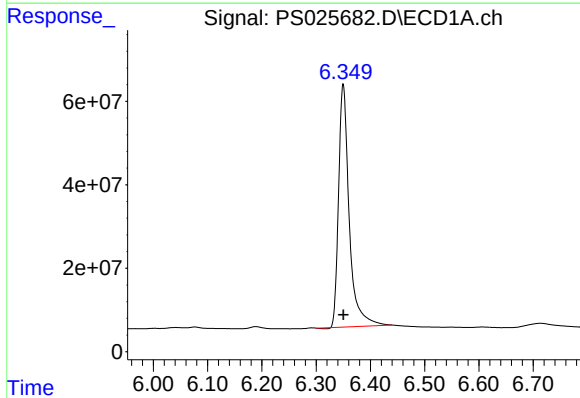


#4 2,4-DCAA

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 792047804
Conc: 531.77 ng/ml

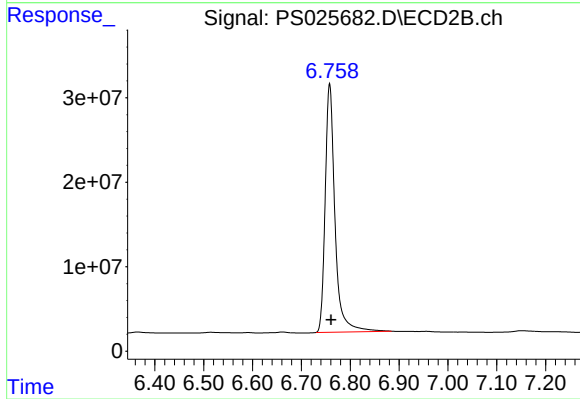

#4 2,4-DCAA


R.T.: 6.758 min
Delta R.T.: -0.003 min
Response: 409543753
Conc: 533.40 ng/ml

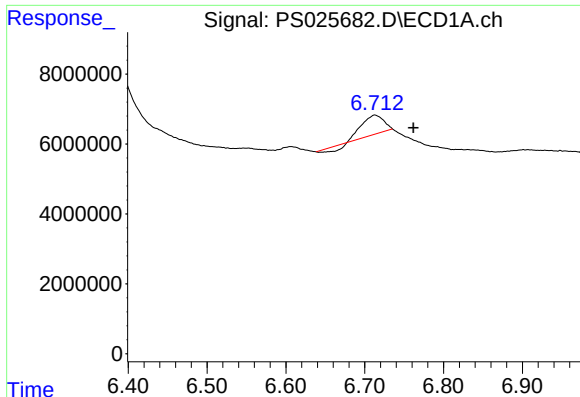

#7 MCPA


R.T.: 6.713 min
Delta R.T.: -0.049 min
Response: 9571674
Conc: 1.69 ug/ml

Instrument :
ECD_S
ClientSampleId :

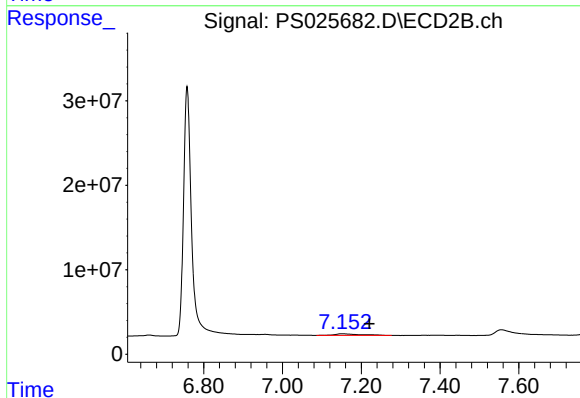


#7 MCPA

R.T.: 7.151 min
Delta R.T.: -0.070 min
Response: 8756816
Conc: 2.53 ug/ml

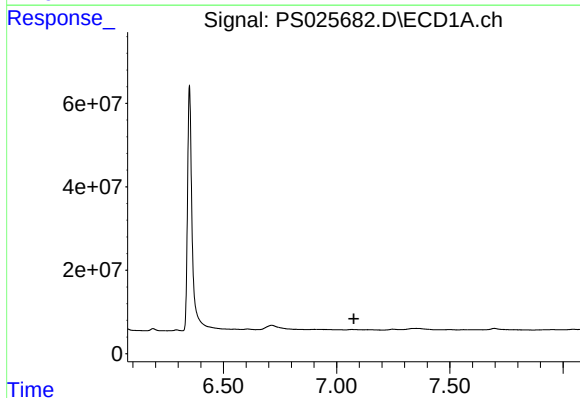


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.077 min
Response: 0
Conc: N.D.

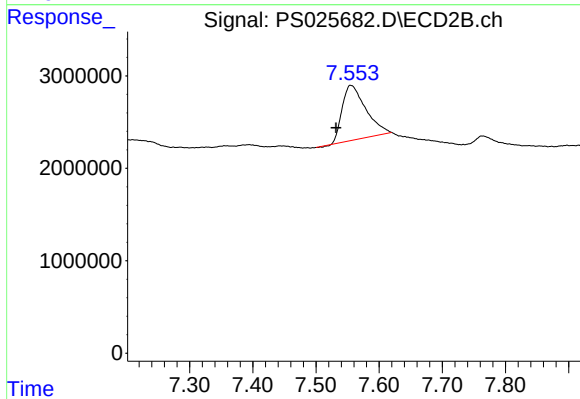

#8 DICHLORPROP


R.T.: 7.555 min
Delta R.T.: 0.023 min
Response: 15478252
Conc: 17.91 ng/ml

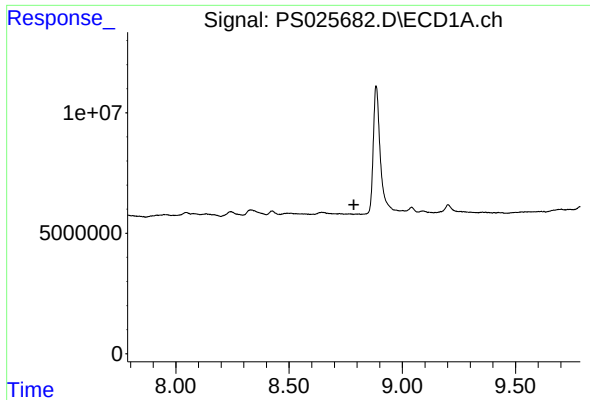

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

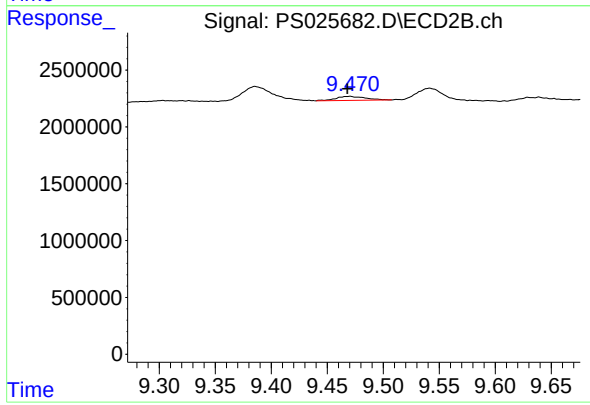

#13 2,4-DB

R.T.: 9.470 min
Delta R.T.: 0.002 min
Response: 643928
Conc: 1.23 ng/ml