

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
 Data File : PS008635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 08:45
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 13:44:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

12) T	2,4,5-T	8.541	8.241	18738216	11878906	2.031	2.246
15) T	Picloram	10.073	10.065	185.2E6	120.5E6	14.834	16.220
16) T	DCPA	10.524	10.015	28792243	17101735	2.426	2.624



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
Data File : PS008635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 08:45
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 13:44:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

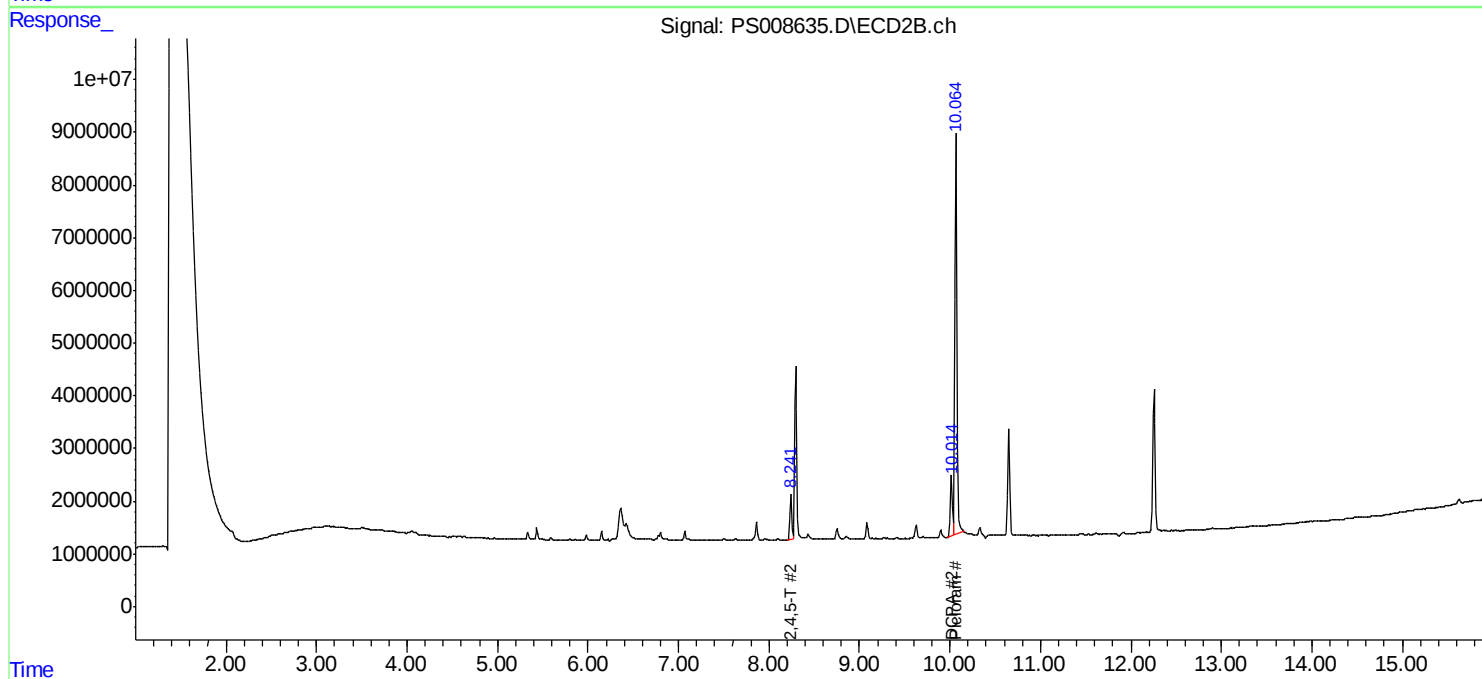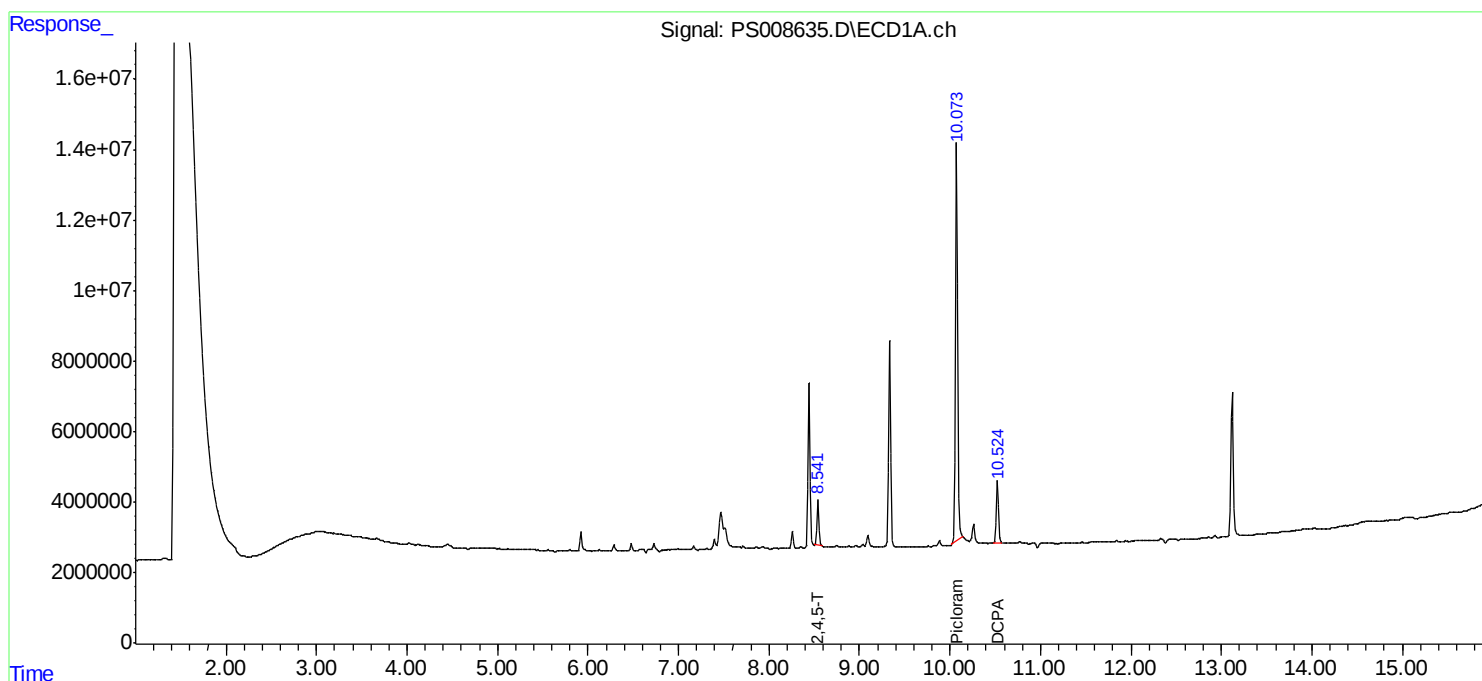


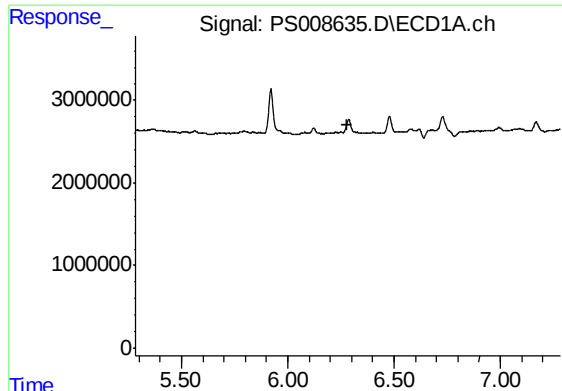

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

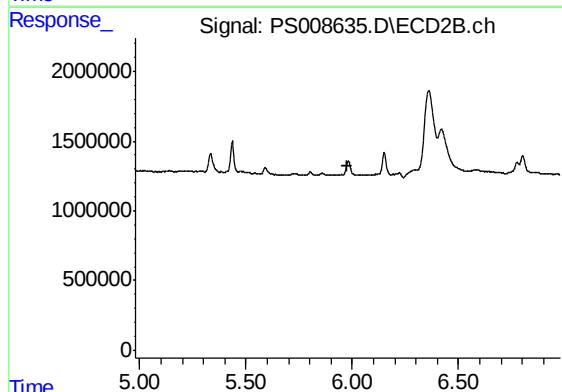


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.979 min
Response: 0
Conc: N.D.

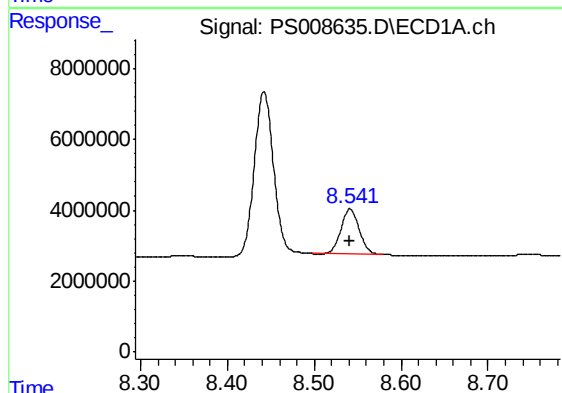


#12 2,4,5-T

R.T.: 8.541 min
Delta R.T.: 0.000 min
Response: 18738216
Conc: 2.03 ng/ml

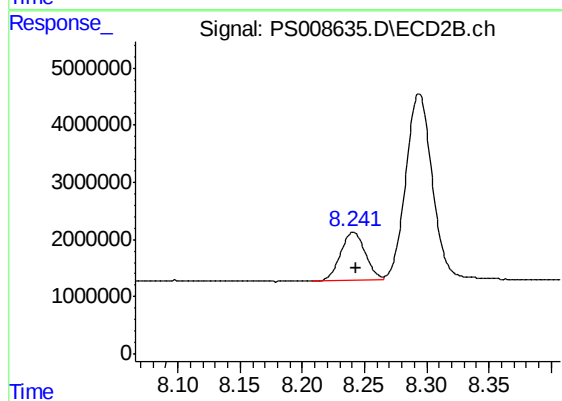

#12 2,4,5-T


R.T.: 8.241 min
Delta R.T.: -0.002 min
Response: 11878906
Conc: 2.25 ng/ml

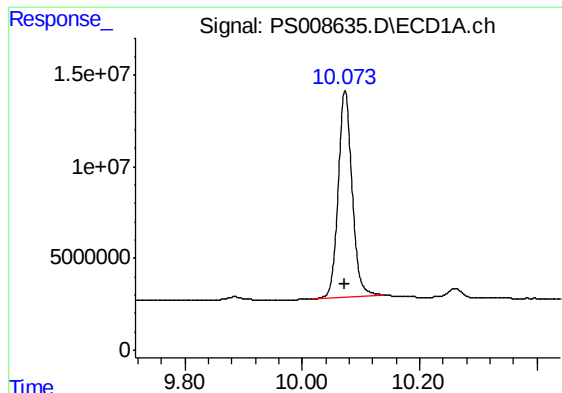

#15 Picloram


R.T.: 10.073 min
Delta R.T.: 0.000 min
Response: 185152620
Conc: 14.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

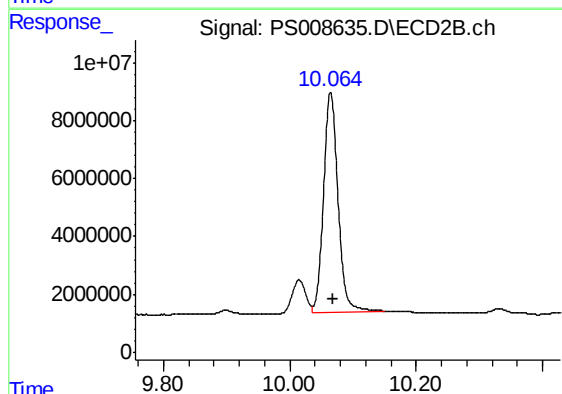


#15 Picloram

R.T.: 10.065 min
Delta R.T.: -0.003 min
Response: 120500949
Conc: 16.22 ng/ml

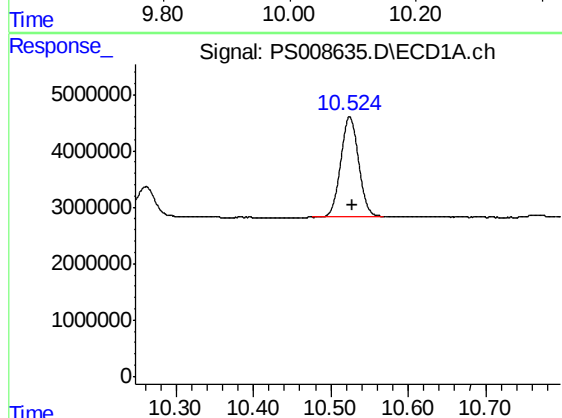

#16 DCPA

R.T.: 10.524 min
Delta R.T.: -0.003 min
Response: 28792243
Conc: 2.43 ng/ml

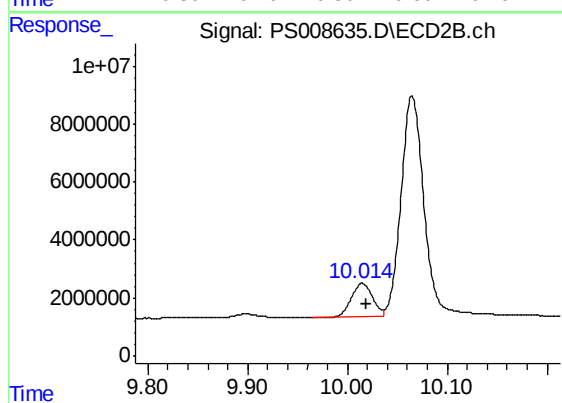

#16 DCPA

R.T.: 10.015 min
Delta R.T.: -0.005 min
Response: 17101735
Conc: 2.62 ng/ml