

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
 Data File : PS008636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 09:07
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 13:44:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.271	5.966	918.5E6	488.1E6	520.172	515.132
Target Compounds							
12) T	2,4,5-T	8.527	8.227	18844137	11605444	2.042	2.195
15) T	Picloram	10.059	10.051	212.6E6	134.1E6	17.030	18.056
16) T	DCPA	10.510	10.001	28994296	16765225	2.443	2.573



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
Data File : PS008636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 09:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 13:44:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

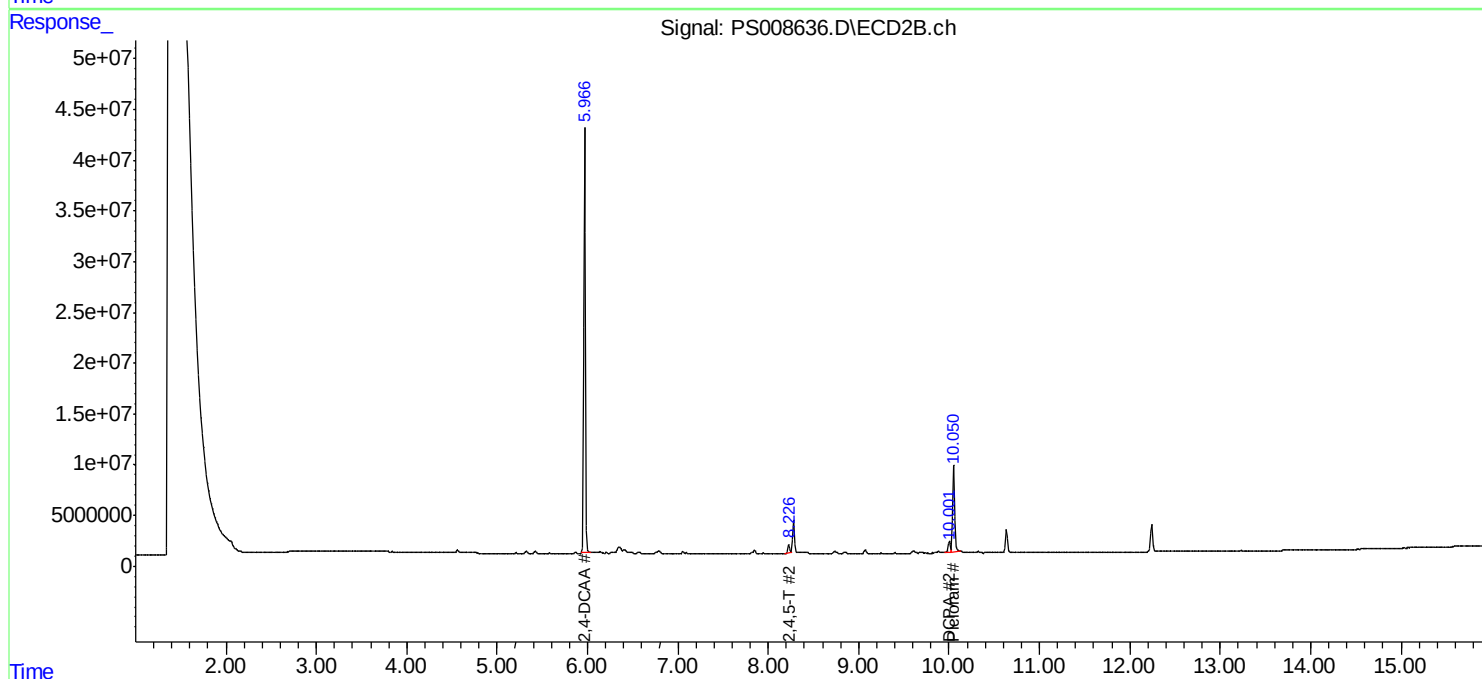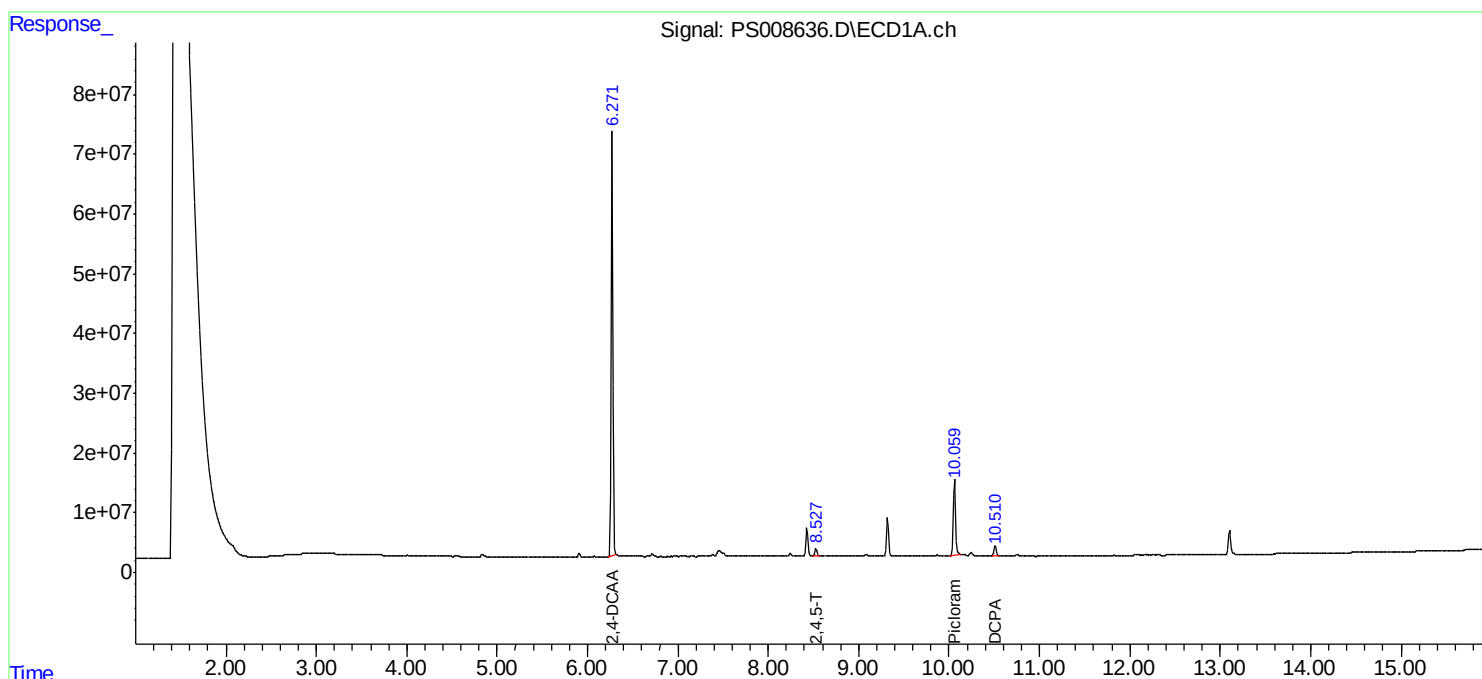


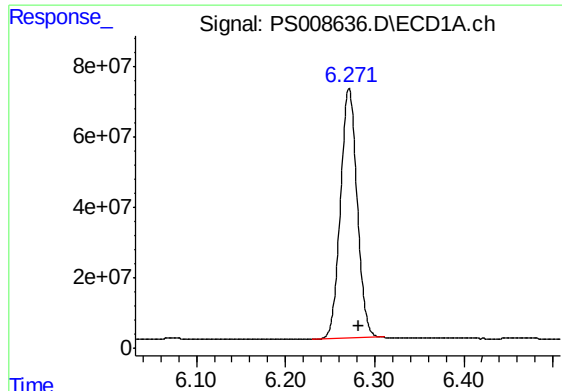

#4 2,4-DCAA


R.T.: 6.271 min
Delta R.T.: -0.011 min
Response: 918468979
Conc: 520.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

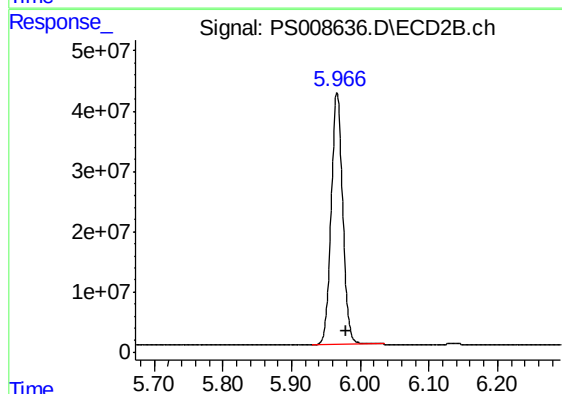


#4 2,4-DCAA

R.T.: 5.966 min
Delta R.T.: -0.013 min
Response: 488068422
Conc: 515.13 ng/ml

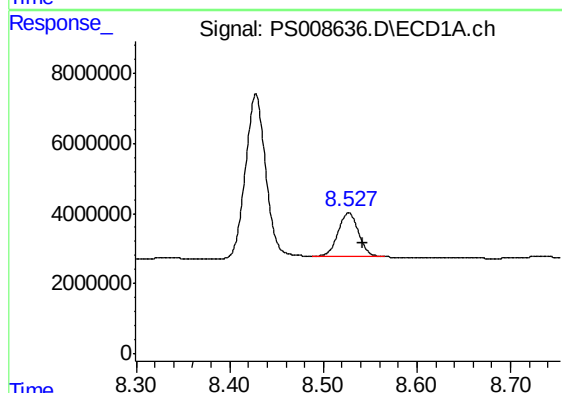


#12 2,4,5-T

R.T.: 8.527 min
Delta R.T.: -0.014 min
Response: 18844137
Conc: 2.04 ng/ml

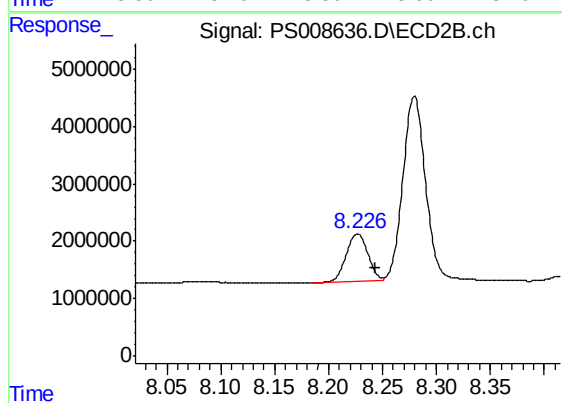

#12 2,4,5-T


R.T.: 8.227 min
Delta R.T.: -0.017 min
Response: 11605444
Conc: 2.19 ng/ml

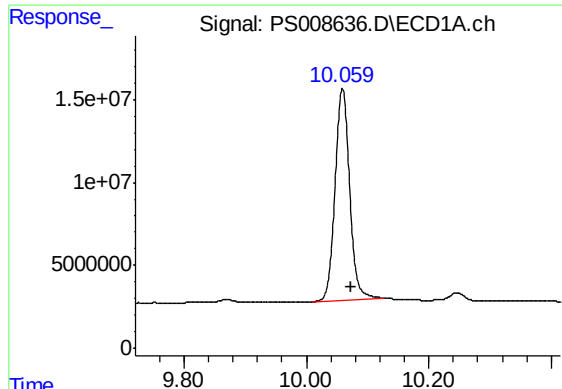

#15 Picloram


R.T.: 10.059 min
Delta R.T.: -0.014 min
Response: 212559779
Conc: 17.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

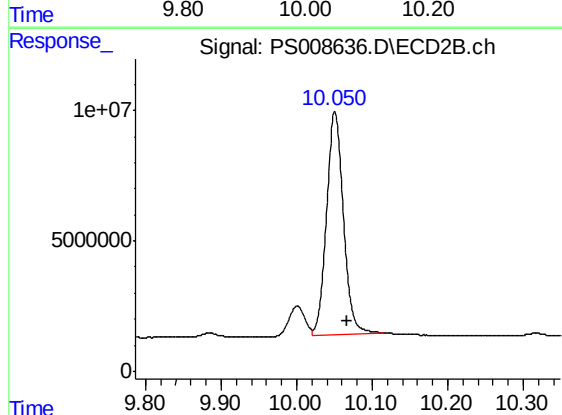


#15 Picloram

R.T.: 10.051 min
Delta R.T.: -0.017 min
Response: 134139270
Conc: 18.06 ng/ml

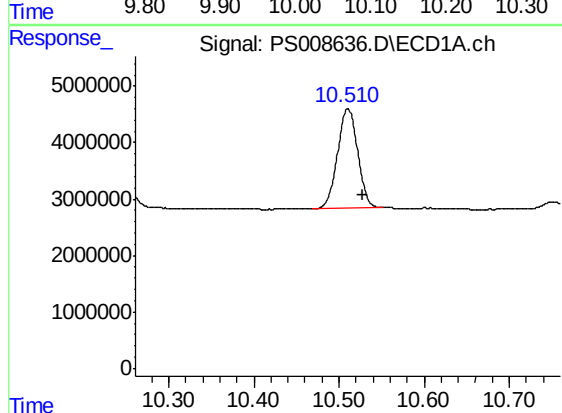

#16 DCPA

R.T.: 10.510 min
Delta R.T.: -0.017 min
Response: 28994296
Conc: 2.44 ng/ml

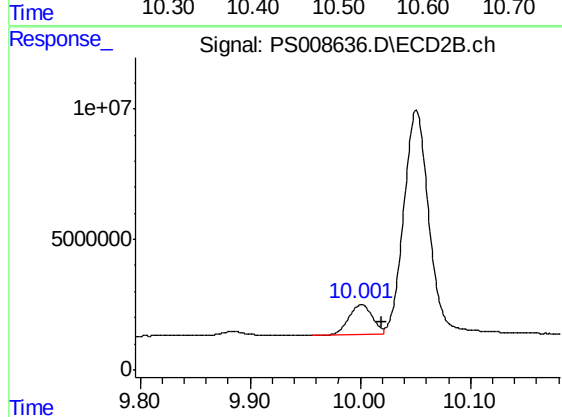

#16 DCPA

R.T.: 10.001 min
Delta R.T.: -0.018 min
Response: 16765225
Conc: 2.57 ng/ml