

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
 Data File : PS008640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 12:10
 Operator : DD\AJ
 Sample : L1287-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AOC-3-EXC-PIT-(0-5)-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 13:45:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.284	5.979	798.3E6	407.6E6	452.126	430.172
Target Compounds							
1) T	Dalapon	2.518	2.205	176.5E6	75767290	68.861	59.766
2) T	3,5-DICHL...	0.000	5.115	0	7484466	N.D.	5.357
5) T	DICAMBA	6.469	0.000	17149187	0	2.495	N.D. #
6) T	MCPD	6.615	6.306	13409001	4394936	2.631	1.445 #
7) T	MCPA	0.000	6.450	0	16652107	N.D.	3.900
8) T	DICHLORPROP	0.000	6.798	0	86081015	N.D.	89.097
9) T	2,4-D	0.000	7.045	0	10684576	N.D.	9.115
10) T	Pentachlo...	7.709	7.500	28531447	23672337	1.174	1.753 #
11) T	2,4,5-TP ...	8.226	7.828	6405681	37186641	<MDL	7.115 #
12) T	2,4,5-T	8.486	8.238	71626520	9817309	7.763	1.856 #
14) T	DINOSEB	10.224	9.129	38973439	104.6E6	5.432	27.683 #
15) T	Picloram	10.060	10.063	79289095	24910968	6.352	3.353 #
16) T	DCPA	0.000	10.063	0	24910968	N.D.	3.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
Data File : PS008640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 12:10
Operator : DD\AJ
Sample : L1287-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 13:45:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

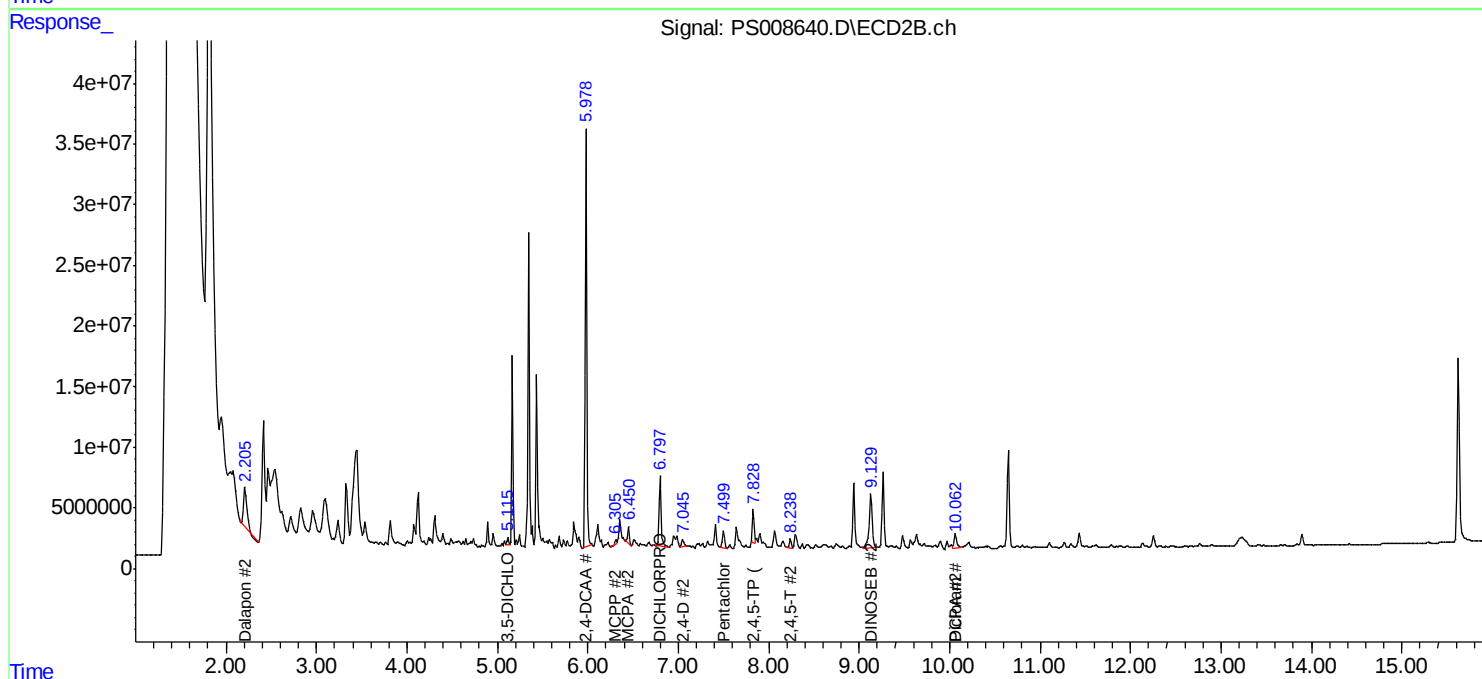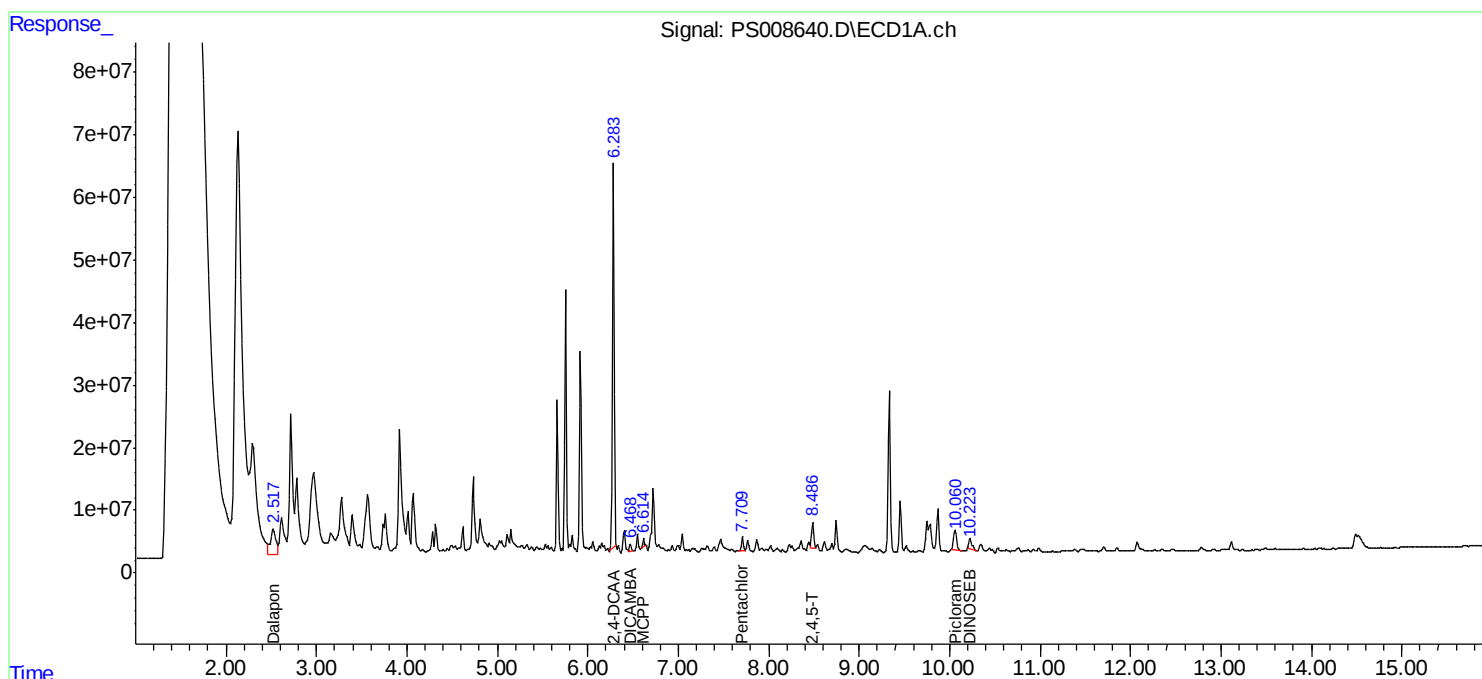


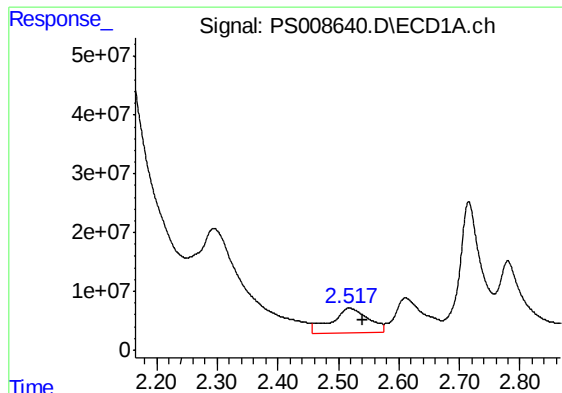

#1 Dalapon


R.T.: 2.518 min
Delta R.T.: -0.022 min
Response: 176548965
Conc: 68.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

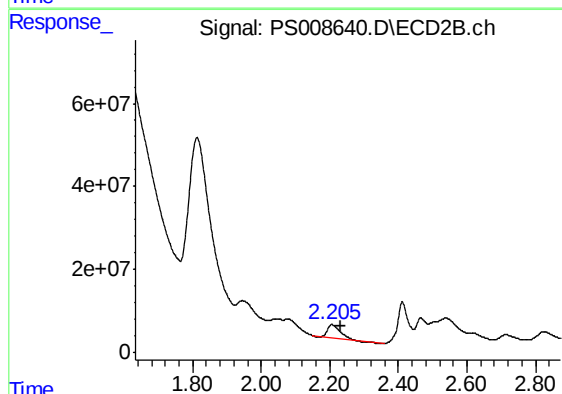


#1 Dalapon

R.T.: 2.205 min
Delta R.T.: -0.026 min
Response: 75767290
Conc: 59.77 ng/ml

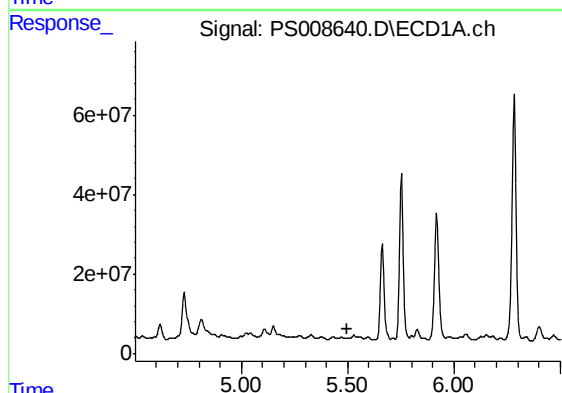


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

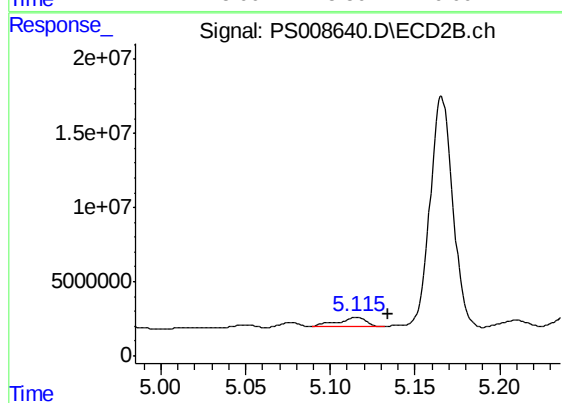

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.115 min
Delta R.T.: -0.019 min
Response: 7484466
Conc: 5.36 ng/ml

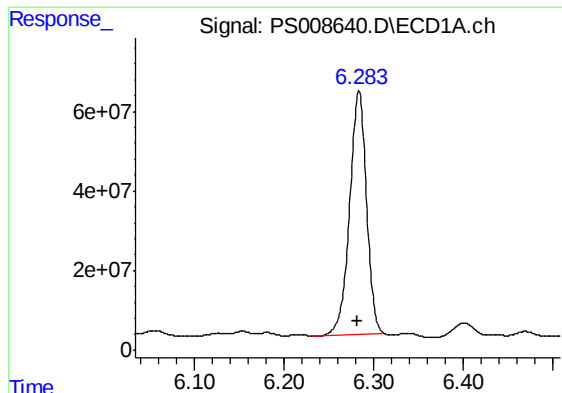

#4 2,4-DCAA


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 798319853
Conc: 452.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

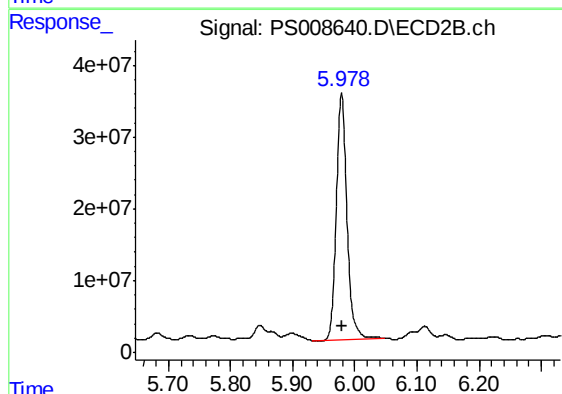


#4 2,4-DCAA

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 407572360
Conc: 430.17 ng/ml

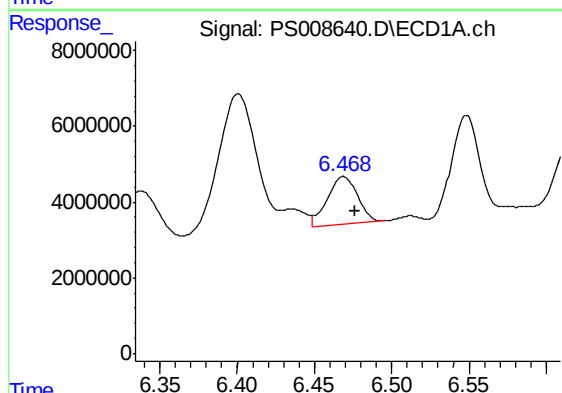


#5 DICAMBA

R.T.: 6.469 min
Delta R.T.: -0.007 min
Response: 17149187
Conc: 2.50 ng/ml

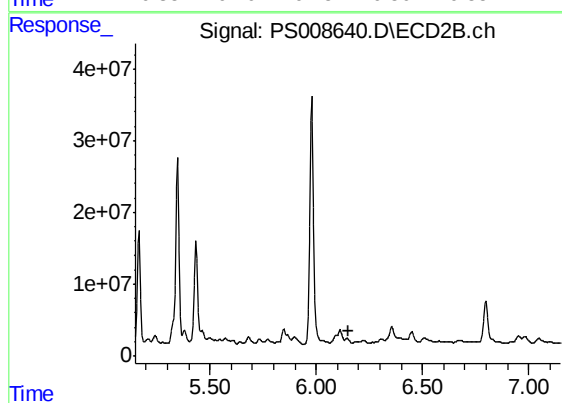

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.150 min
Response: 0
Conc: N.D.

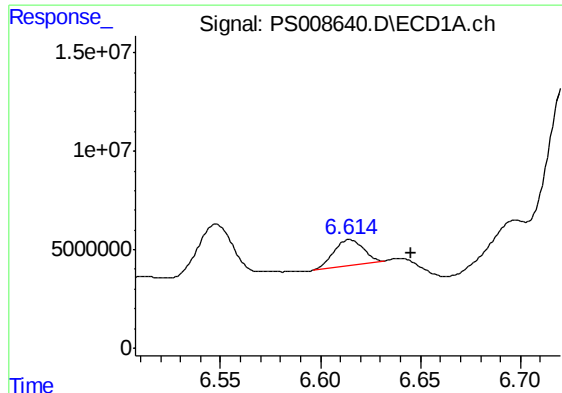

#6 MCPP


R.T.: 6.615 min
Delta R.T.: -0.031 min
Response: 13409001
Conc: 2.63 ug/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

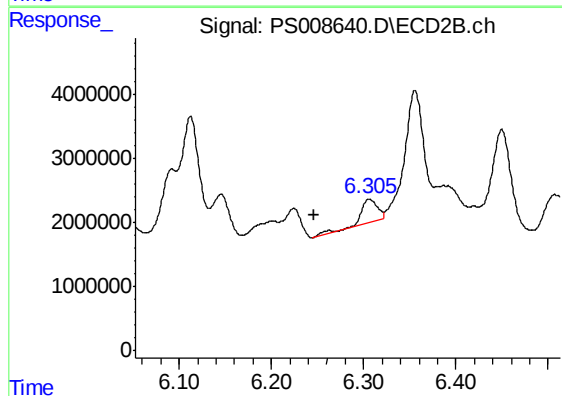


#6 MCPP

R.T.: 6.306 min
Delta R.T.: 0.060 min
Response: 4394936
Conc: 1.45 ug/ml

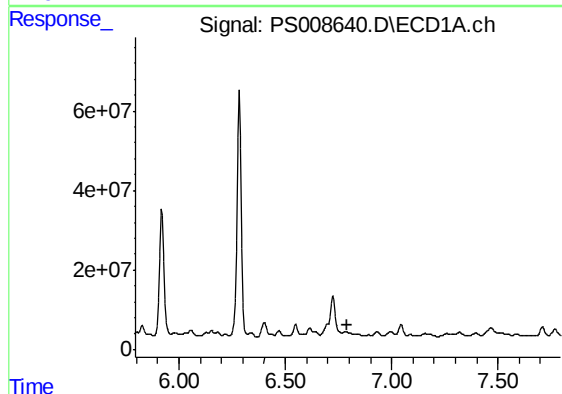


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

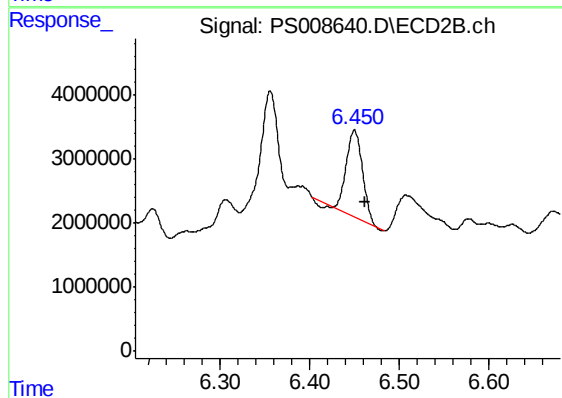

#7 MCPA


R.T.: 6.450 min
Delta R.T.: -0.012 min
Response: 16652107
Conc: 3.90 ug/ml

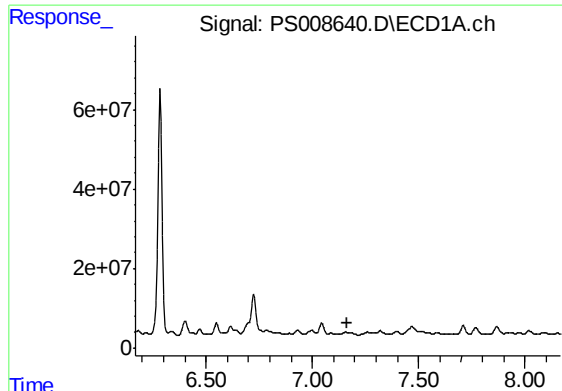

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

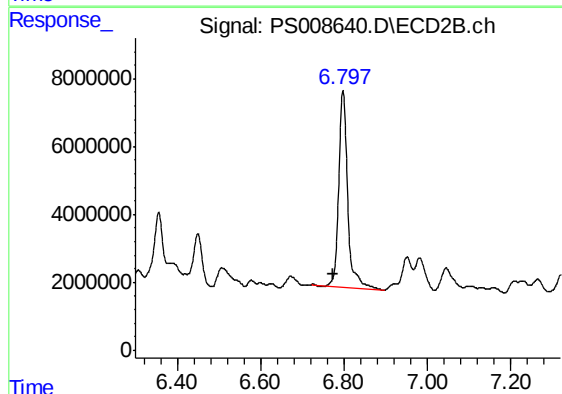


#8 DICHLORPROP

R.T.: 6.798 min
Delta R.T.: 0.023 min
Response: 86081015
Conc: 89.10 ng/ml

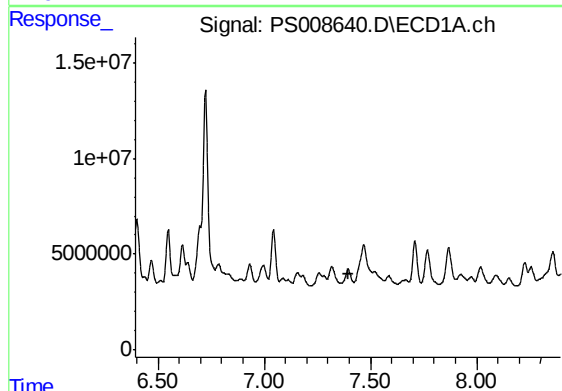


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

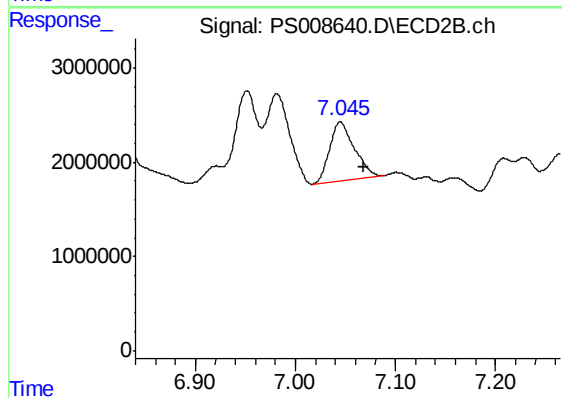

#9 2,4-D


R.T.: 7.045 min
Delta R.T.: -0.024 min
Response: 10684576
Conc: 9.11 ng/ml

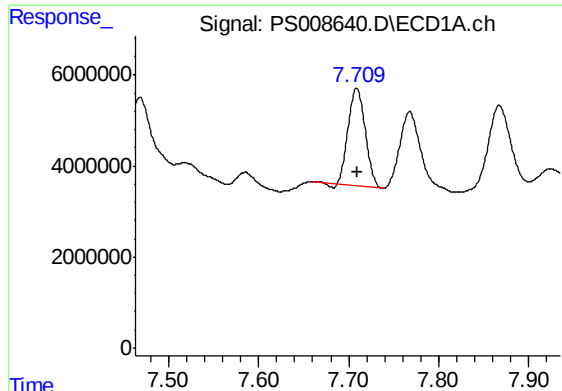

#10 Pentachlorophenol


R.T.: 7.709 min
Delta R.T.: -0.001 min
Response: 28531447
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

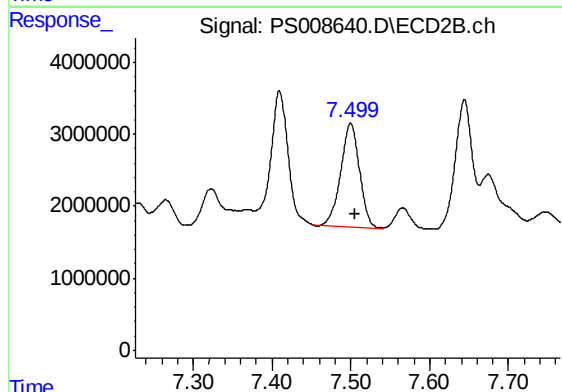


#10 Pentachlorophenol

R.T.: 7.500 min
Delta R.T.: -0.005 min
Response: 23672337
Conc: 1.75 ng/ml

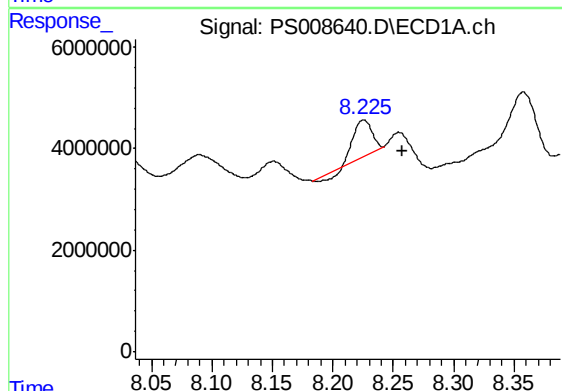


#11 2,4,5-TP (SILVEX)

R.T.: 8.226 min
Delta R.T.: -0.032 min
Response: 6405681
Conc: N.D.

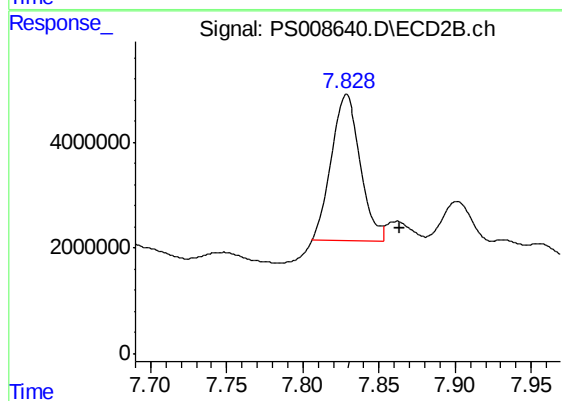

#11 2,4,5-TP (SILVEX)


R.T.: 7.828 min
Delta R.T.: -0.035 min
Response: 37186641
Conc: 7.11 ng/ml

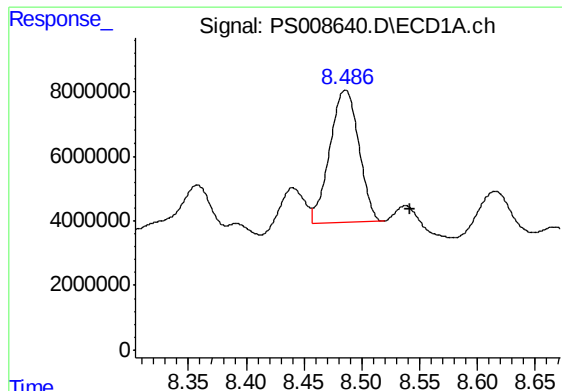

#12 2,4,5-T


R.T.: 8.486 min
Delta R.T.: -0.056 min
Response: 71626520
Conc: 7.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

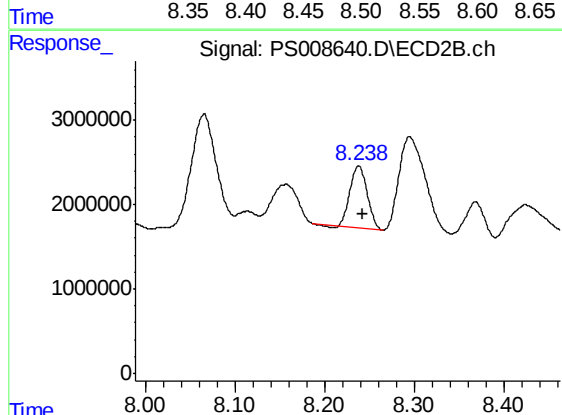


#12 2,4,5-T

R.T.: 8.238 min
Delta R.T.: -0.005 min
Response: 9817309
Conc: 1.86 ng/ml

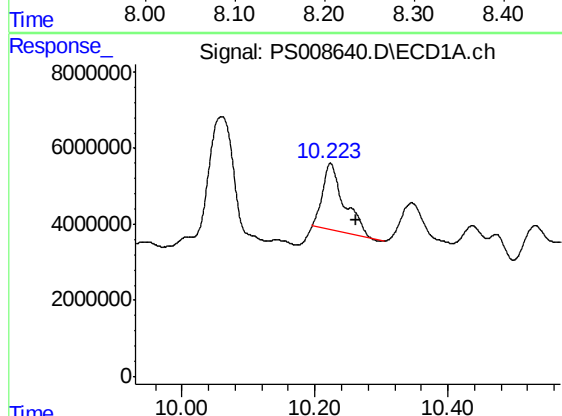


#14 DINOSEB

R.T.: 10.224 min
Delta R.T.: -0.039 min
Response: 38973439
Conc: 5.43 ng/ml

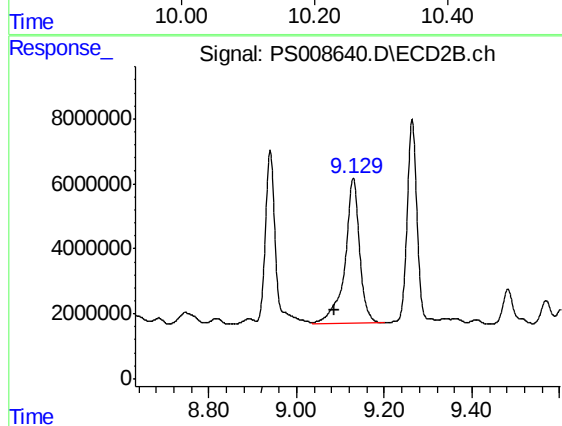

#14 DINOSEB


R.T.: 9.129 min
Delta R.T.: 0.041 min
Response: 104578204
Conc: 27.68 ng/ml

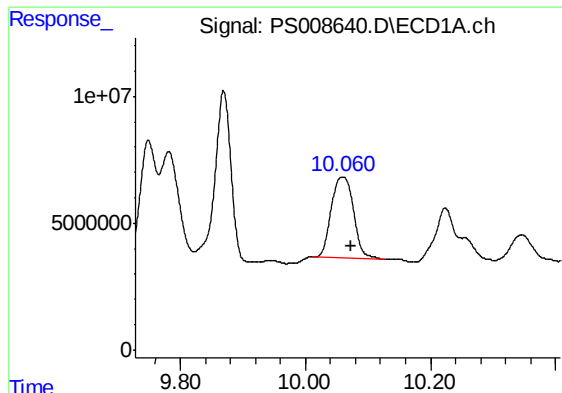

#15 Picloram


R.T.: 10.060 min
Delta R.T.: -0.013 min
Response: 79289095
Conc: 6.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-A

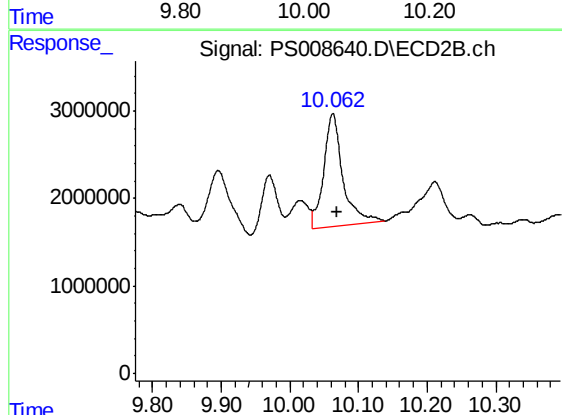


#15 Picloram

R.T.: 10.063 min
Delta R.T.: -0.005 min
Response: 24910968
Conc: 3.35 ng/ml

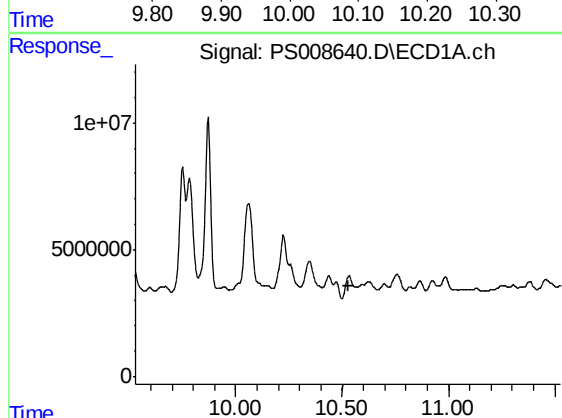

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

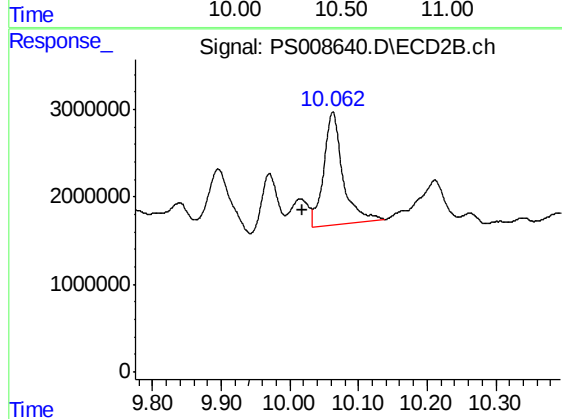

#16 DCPA

R.T.: 10.063 min
Delta R.T.: 0.043 min
Response: 24910968
Conc: 3.82 ng/ml