

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
 Data File : PS008642.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 12:53
 Operator : DD\AJ
 Sample : L1289-38
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 13:46:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.264	5.960	1130.3E6	612.7E6	640.115	646.683
Target Compounds							
1) T	Dalapon	2.498	2.186	210.3E6	121.0E6	82.025	95.442
2) T	3,5-DICHL...	0.000	5.146	0	172.9E6	N.D.	123.750
5) T	DICAMBA	6.448	6.093	13838782	15999987	2.014	4.001 #
6) T	MCPD	6.704	0.000	150.6E6	0	29.557	N.D. #
7) T	MCPA	0.000	6.487	0	9407174	N.D.	2.203
8) T	DICHLORPROP	0.000	6.778	0	62495786	N.D.	64.685
9) T	2,4-D	0.000	7.026	0	12077092	N.D.	10.303
10) T	Pentachlo...	7.747	0.000	36970907	0	1.521	N.D. #
12) T	2,4,5-T	0.000	8.289	0	15802362	N.D.	2.988
14) T	DINOSEB	0.000	9.111	0	108.9E6	N.D.	28.815
15) T	Picloram	10.033	0.000	58135191	0	4.658	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
Data File : PS008642.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 12:53
Operator : DD\AJ
Sample : L1289-38
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 13:46:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

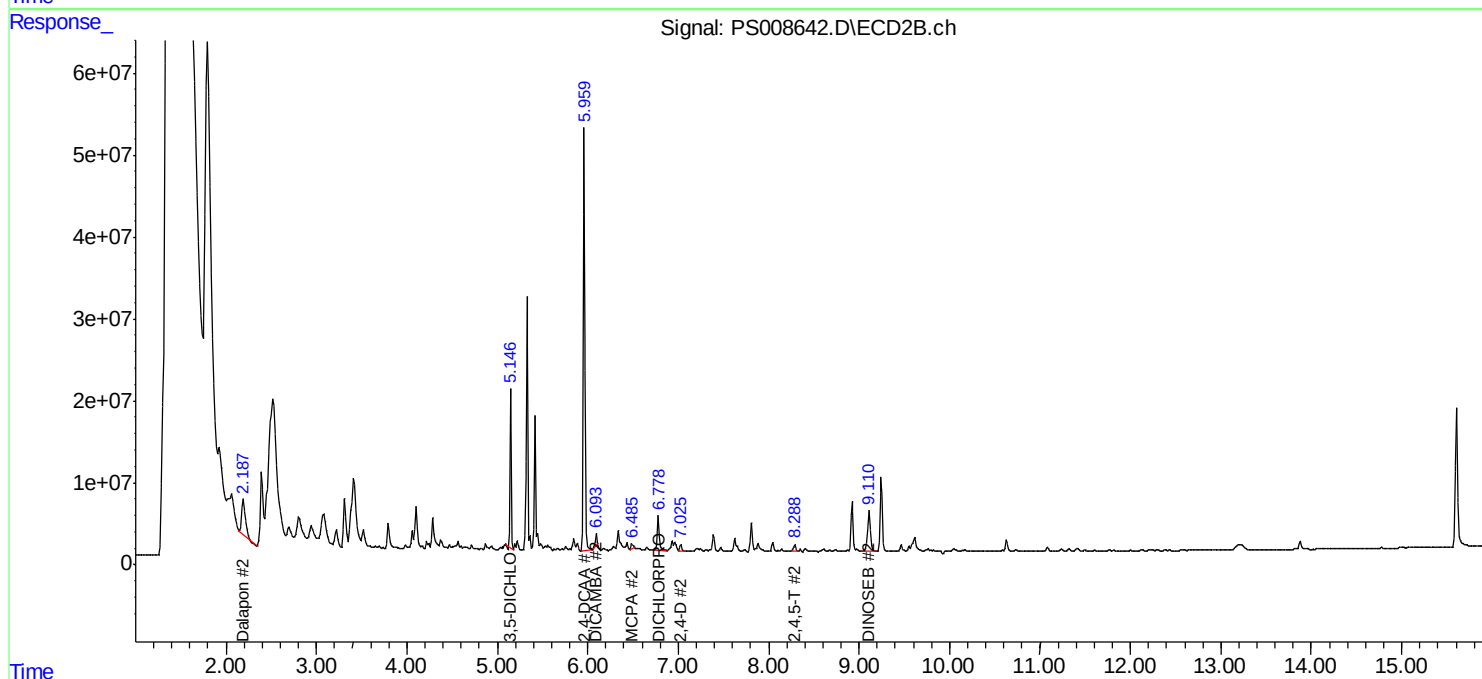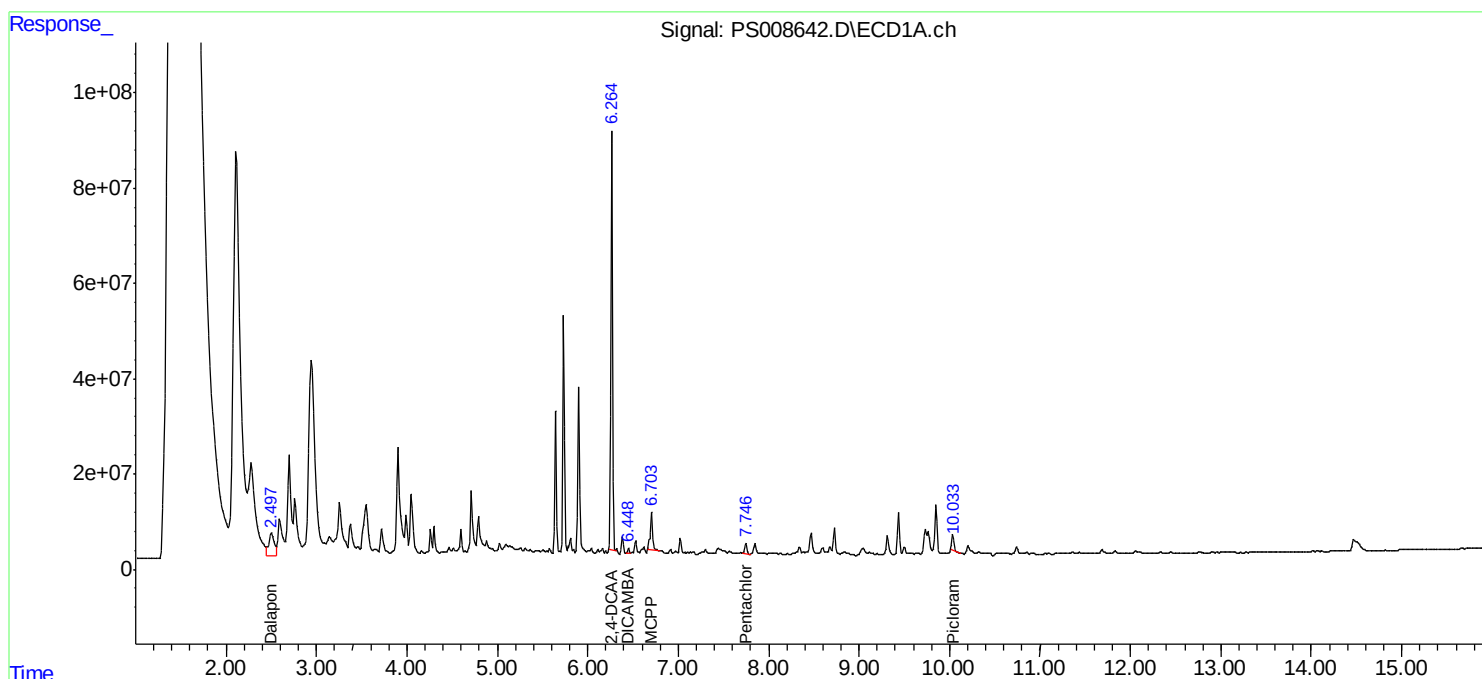


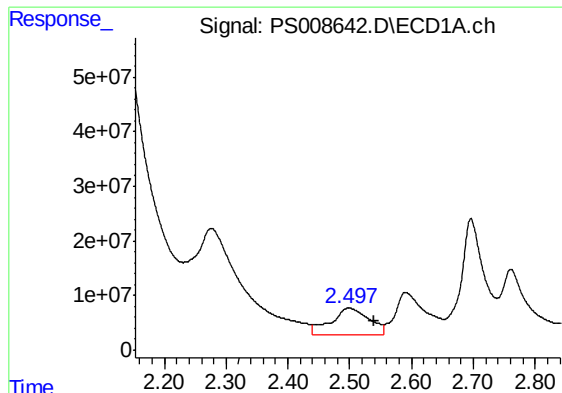

#1 Dalapon


R.T.: 2.498 min
Delta R.T.: -0.042 min
Response: 210299825
Conc: 82.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

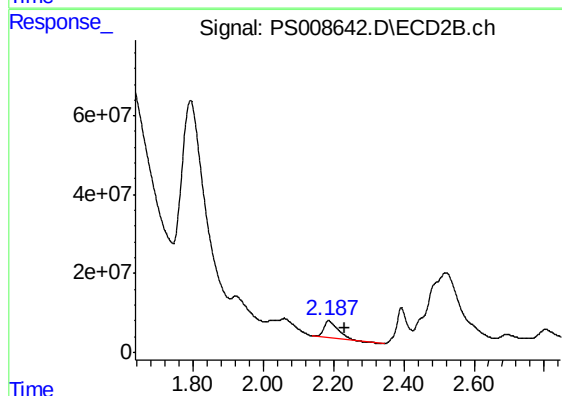


#1 Dalapon

R.T.: 2.186 min
Delta R.T.: -0.045 min
Response: 120996409
Conc: 95.44 ng/ml

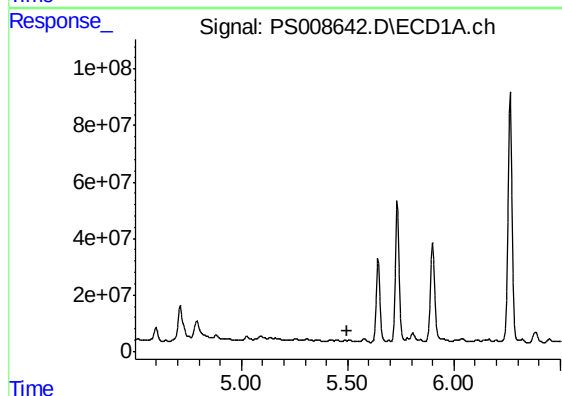


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

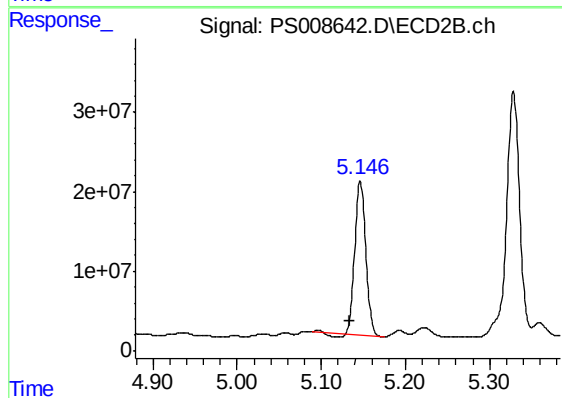

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.012 min
Response: 172900592
Conc: 123.75 ng/ml

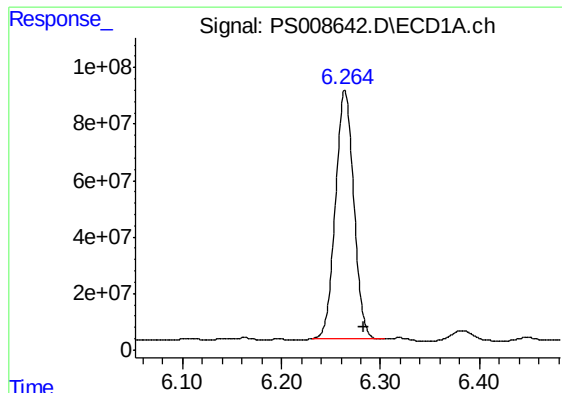

#4 2,4-DCAA


R.T.: 6.264 min
Delta R.T.: -0.019 min
Response: 1130252644
Conc: 640.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

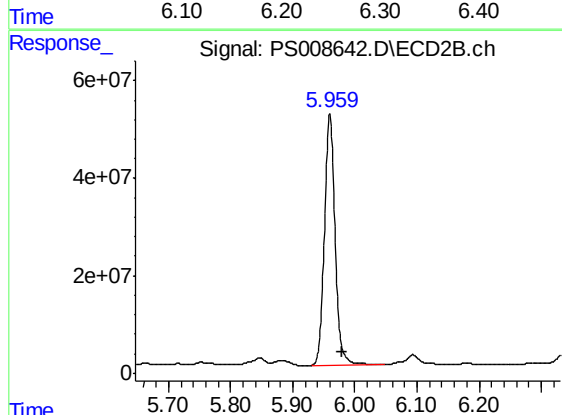


#4 2,4-DCAA

R.T.: 5.960 min
Delta R.T.: -0.020 min
Response: 612707896
Conc: 646.68 ng/ml

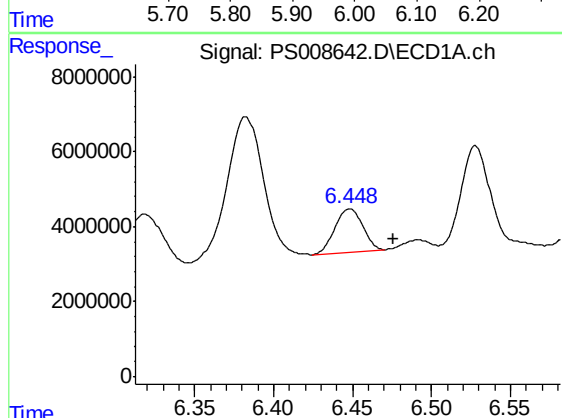


#5 DICAMBA

R.T.: 6.448 min
Delta R.T.: -0.028 min
Response: 13838782
Conc: 2.01 ng/ml

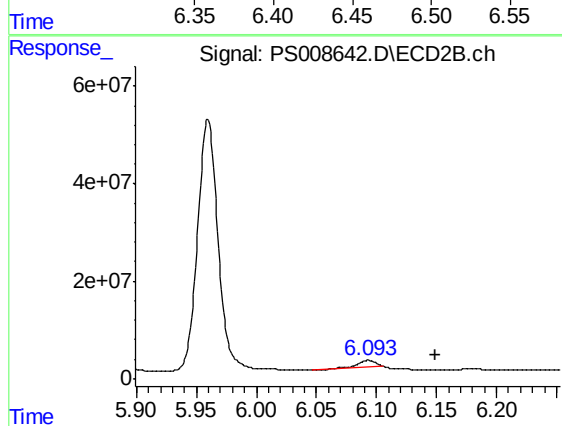

#5 DICAMBA


R.T.: 6.093 min
Delta R.T.: -0.056 min
Response: 15999987
Conc: 4.00 ng/ml

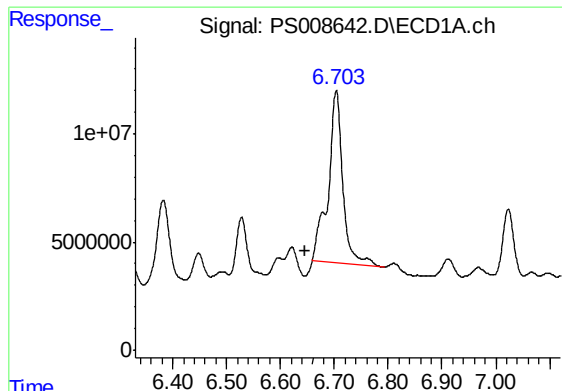

#6 MCPP


R.T.: 6.704 min
Delta R.T.: 0.058 min
Response: 150648313
Conc: 29.56 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

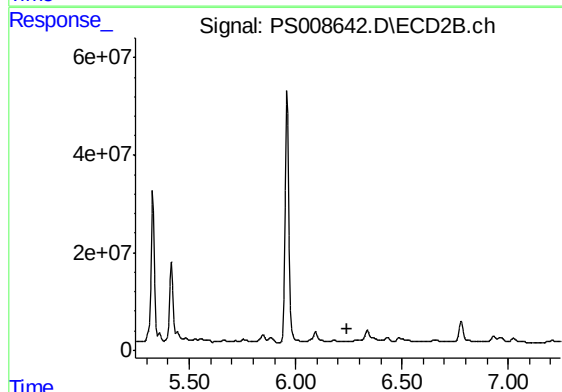


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

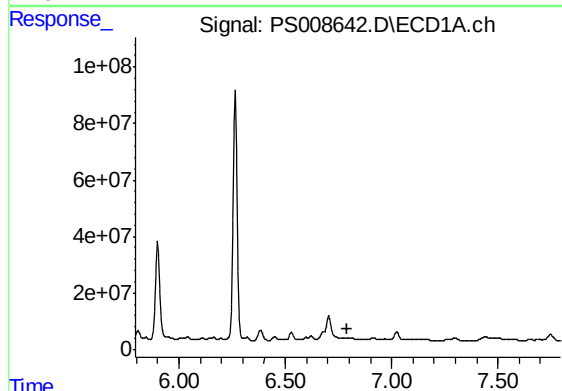


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

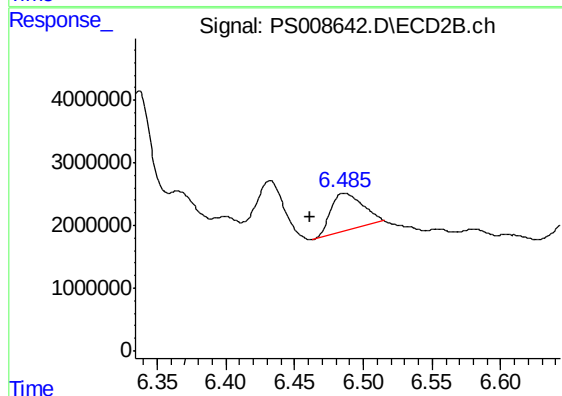

#7 MCPA


R.T.: 6.487 min
Delta R.T.: 0.025 min
Response: 9407174
Conc: 2.20 ug/ml

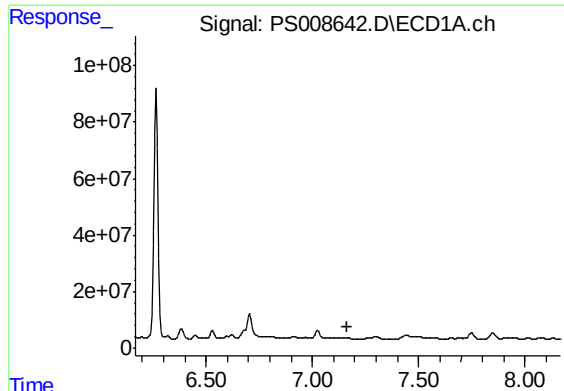

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

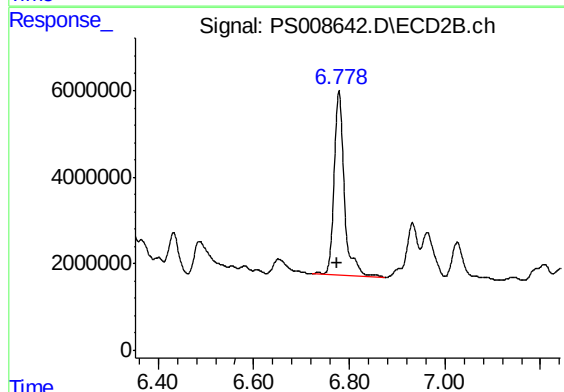


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.004 min
Response: 62495786
Conc: 64.69 ng/ml

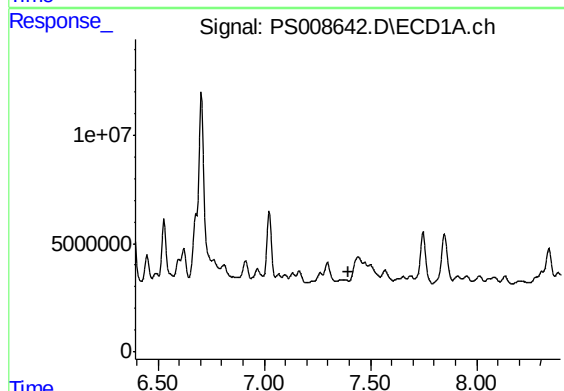


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

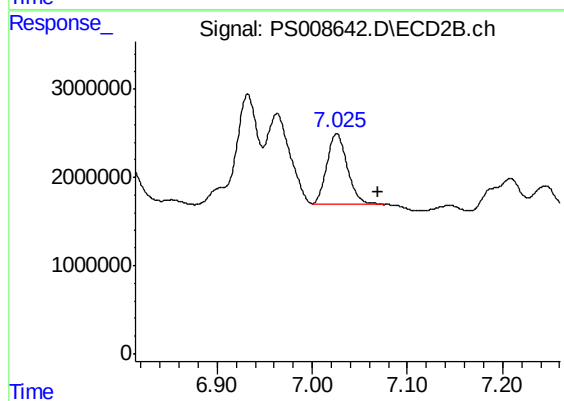

#9 2,4-D


R.T.: 7.026 min
Delta R.T.: -0.043 min
Response: 12077092
Conc: 10.30 ng/ml

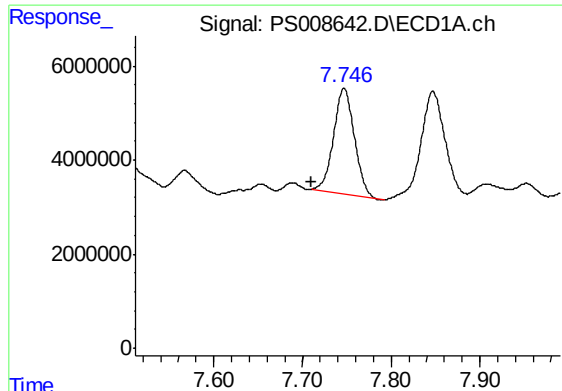

#10 Pentachlorophenol


R.T.: 7.747 min
Delta R.T.: 0.037 min
Response: 36970907
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

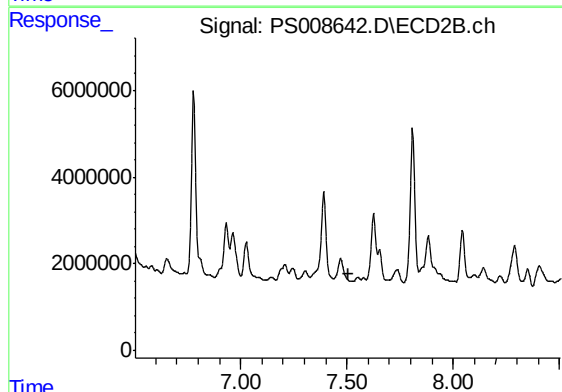


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

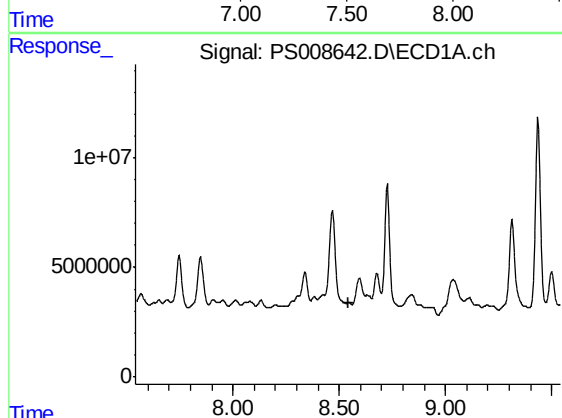


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

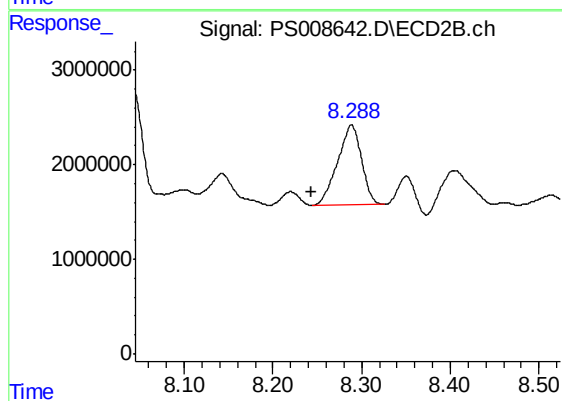

#12 2,4,5-T


R.T.: 8.289 min
Delta R.T.: 0.045 min
Response: 15802362
Conc: 2.99 ng/ml

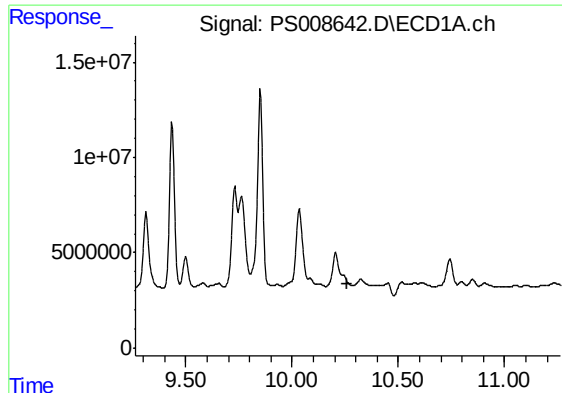

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-COMP

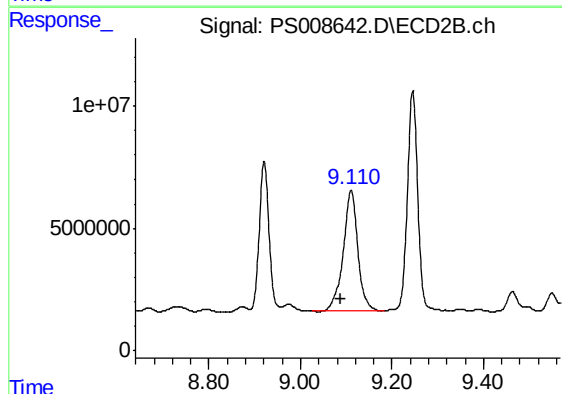


#14 DINOSEB

R.T.: 9.111 min
Delta R.T.: 0.023 min
Response: 108855632
Conc: 28.82 ng/ml

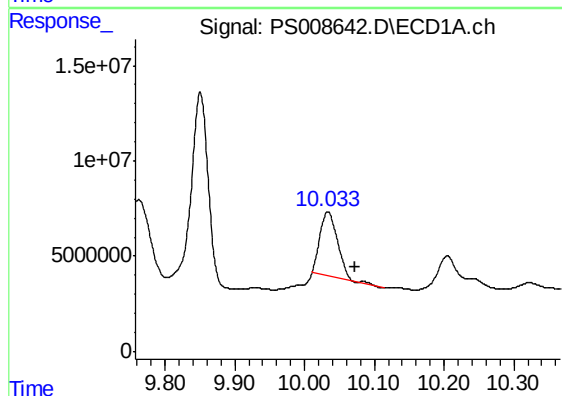

#15 Picloram

R.T.: 10.033 min
Delta R.T.: -0.040 min
Response: 58135191
Conc: 4.66 ng/ml

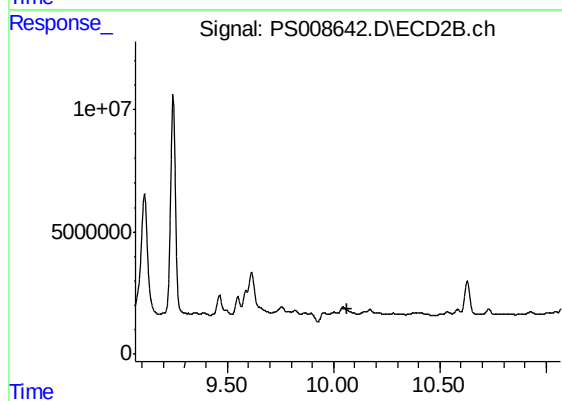

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.