

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
 Data File : PS008648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 18:19
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 00:31:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.284	5.978	923.7E6	494.9E6	523.126	522.377
Target Compounds							
10) T	Pentachlo...	7.710	7.500	27620468	16651035	1.136	1.233
12) T	2,4,5-T	0.000	8.292	0	9260253	N.D.	1.751
15) T	Picloram	0.000	10.063	0	10663430	N.D.	1.435
16) T	DCPA	0.000	10.063	0	10663430	N.D.	1.636



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013020\
Data File : PS008648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 18:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 00:31:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

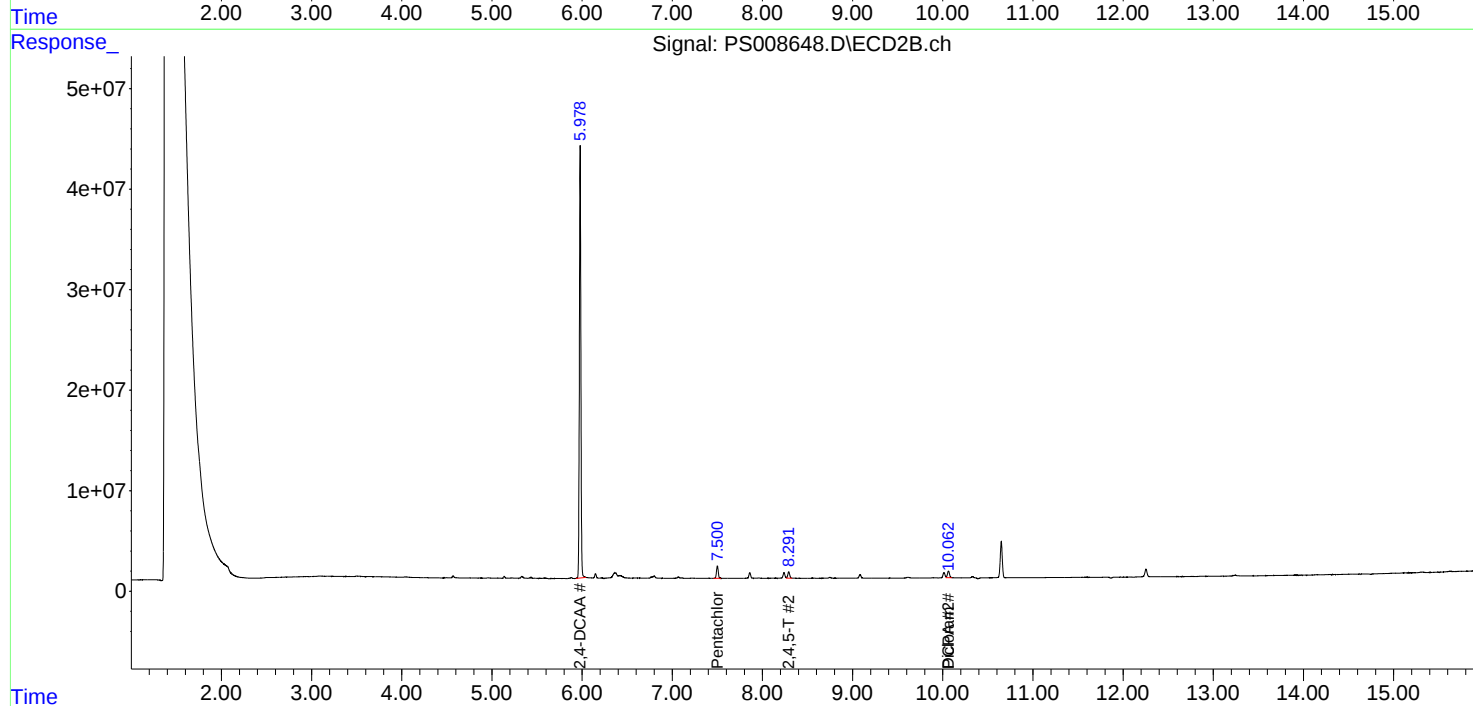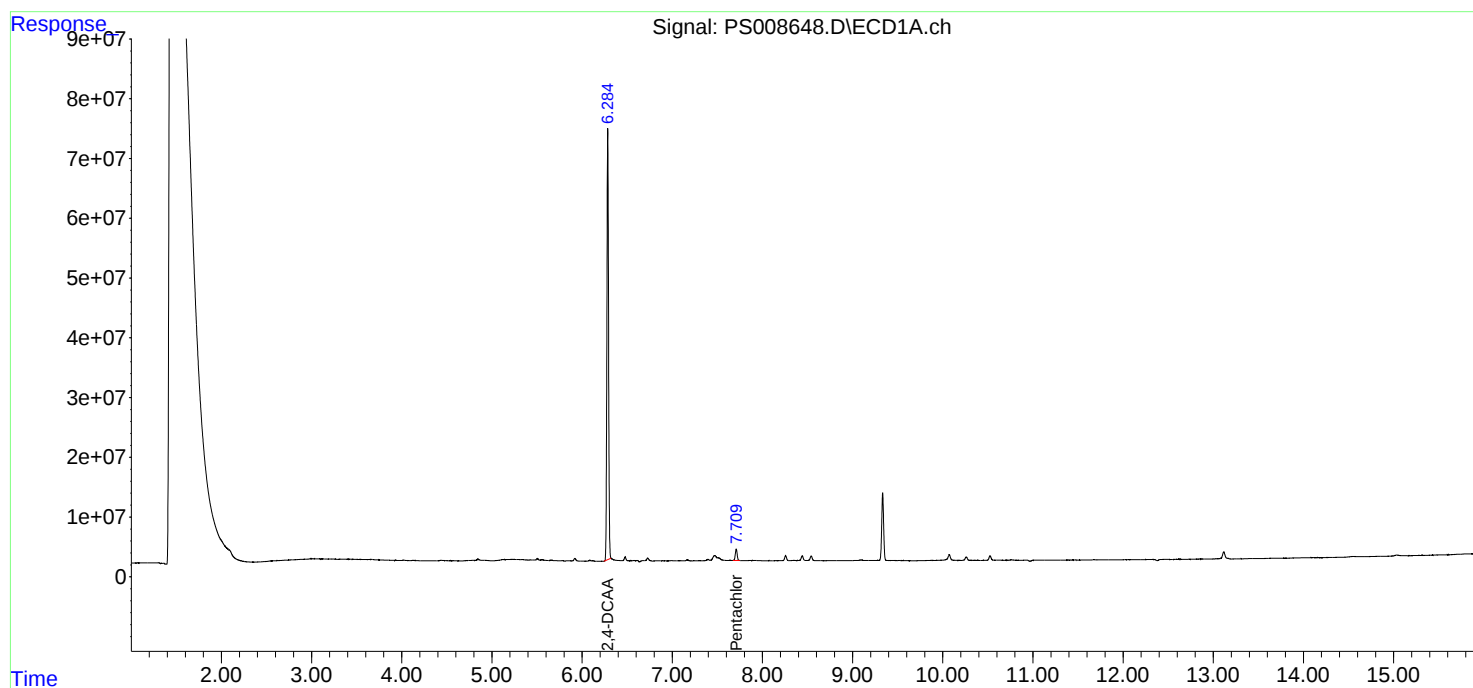


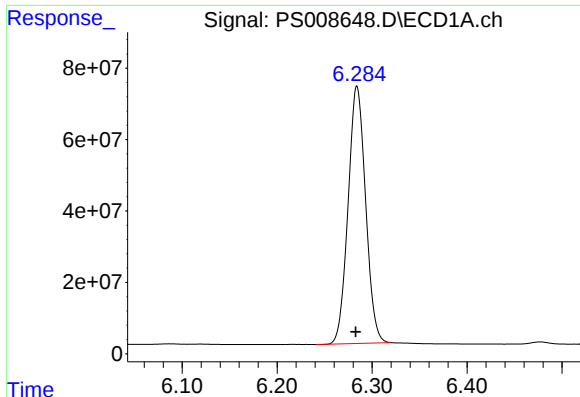

#4 2,4-DCAA


R.T.: 6.284 min
Delta R.T.: 0.001 min
Response: 923686136
Conc: 523.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

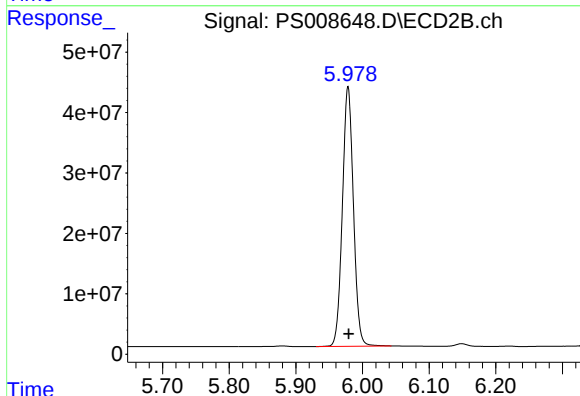


#4 2,4-DCAA

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 494932895
Conc: 522.38 ng/ml

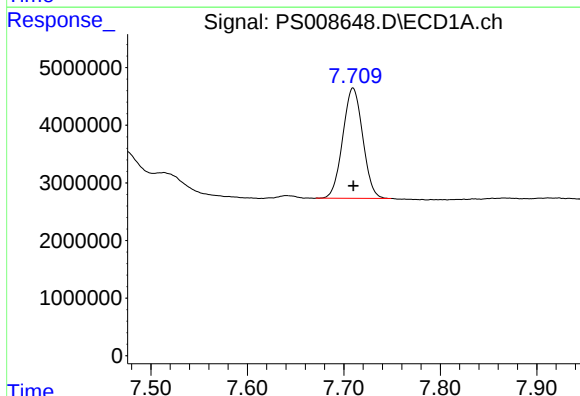


#10 Pentachlorophenol

R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 27620468
Conc: 1.14 ng/ml

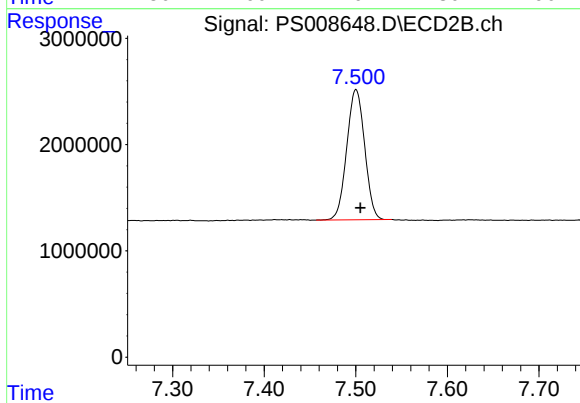

#10 Pentachlorophenol


R.T.: 7.500 min
Delta R.T.: -0.005 min
Response: 16651035
Conc: 1.23 ng/ml

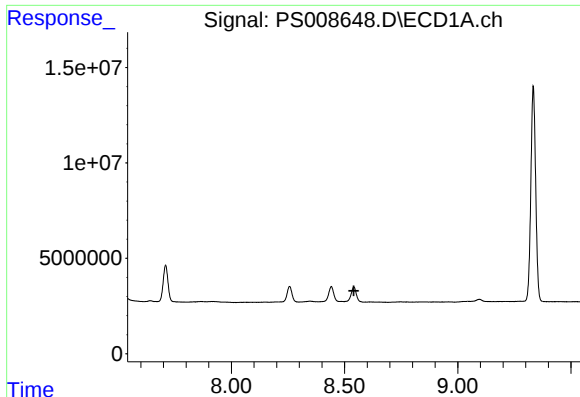

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

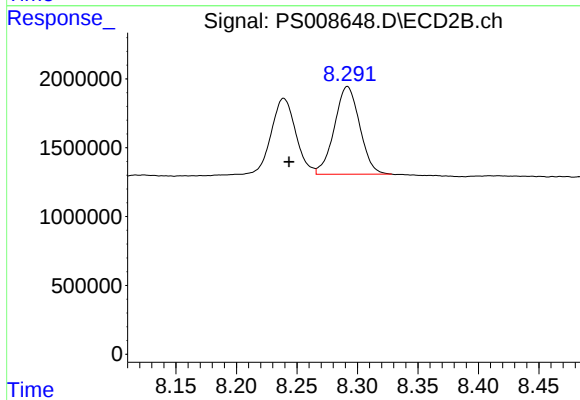


#12 2,4,5-T

R.T.: 8.292 min
Delta R.T.: 0.048 min
Response: 9260253
Conc: 1.75 ng/ml

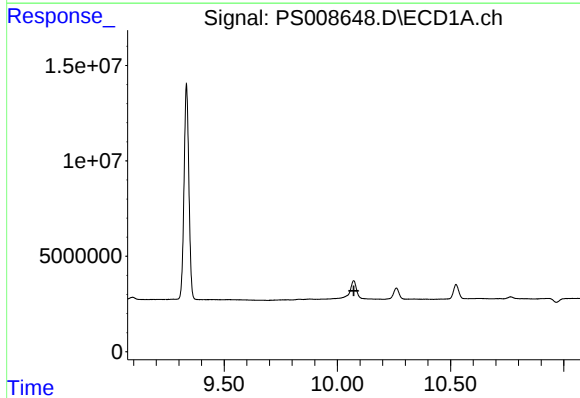


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

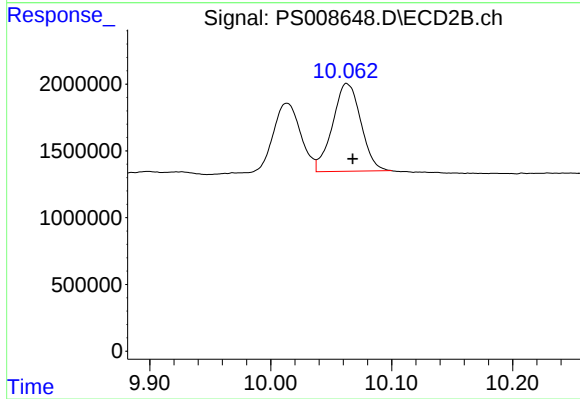

#15 Picloram


R.T.: 10.063 min
Delta R.T.: -0.005 min
Response: 10663430
Conc: 1.44 ng/ml

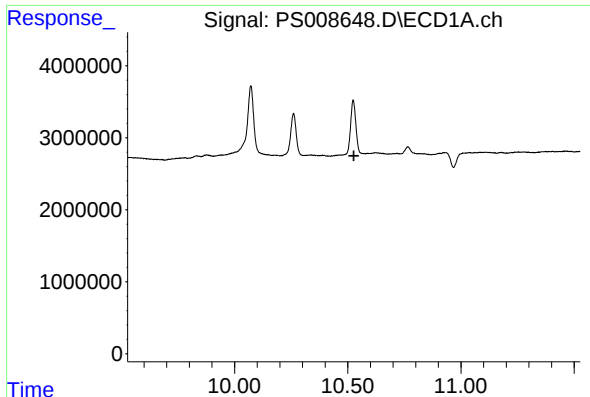

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

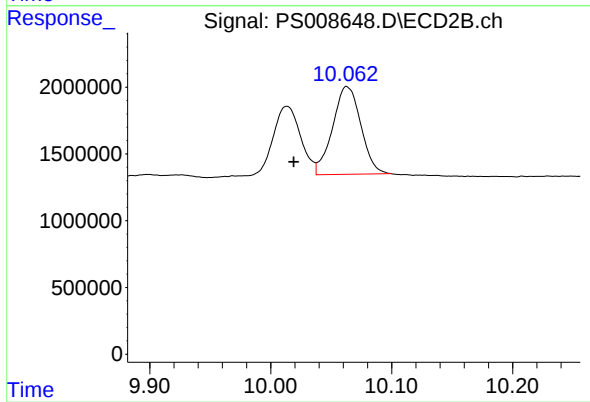

#16 DCPA

R.T.: 10.063 min
Delta R.T.: 0.044 min
Response: 10663430
Conc: 1.64 ng/ml