

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013024\
 Data File : PS025695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2024 21:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-39

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 02:11:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.350	6.757	827.4E6	427.3E6	555.532	556.515
Target Compounds							
1) T	Dalapon	0.000	2.556	0	462467	N.D.	<MDL
3) T	4-Nitroph...	0.000	6.363	0	634777	N.D.	1.333
5) T	DICAMBA	0.000	6.954	0	1065579	N.D.	<MDL
6) T	MCP	0.000	6.954f	0	1065579	N.D.	<MDL
7) T	MCPA	6.712f	0.000	4662599	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.556	0	7814585	N.D.	9.040
9) T	2,4-D	7.248	7.766f	6520916	103226	3.541	<MDL #
11) T	2,4,5-TP ...	0.000	8.631	0	3381245	N.D.	<MDL
12) T	2,4,5-T	0.000	9.029f	0	522344	N.D.	<MDL
15) T	Picloram	0.000	10.772	0	1312354	N.D.	<MDL
16) T	DCPA	0.000	10.709	0	713277	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013024\
Data File : PS025695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2024 21:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-39

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 02:11:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

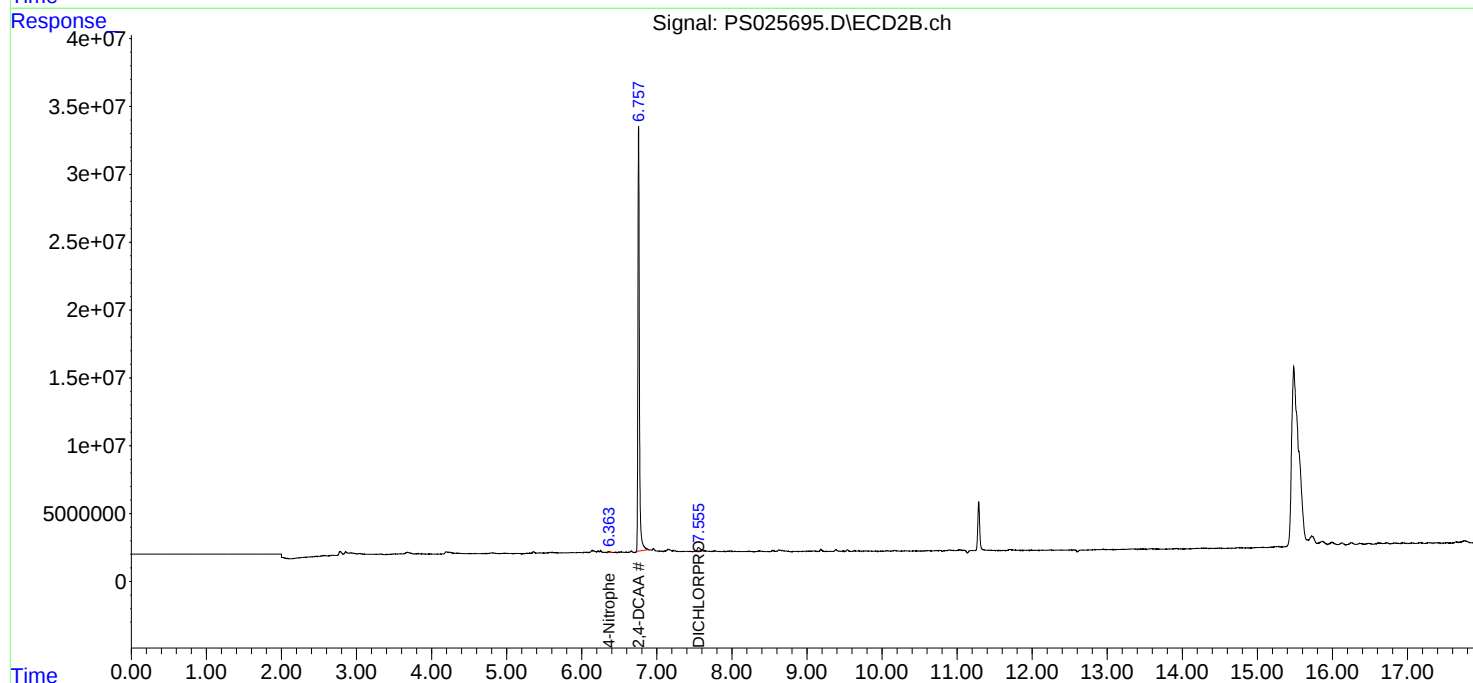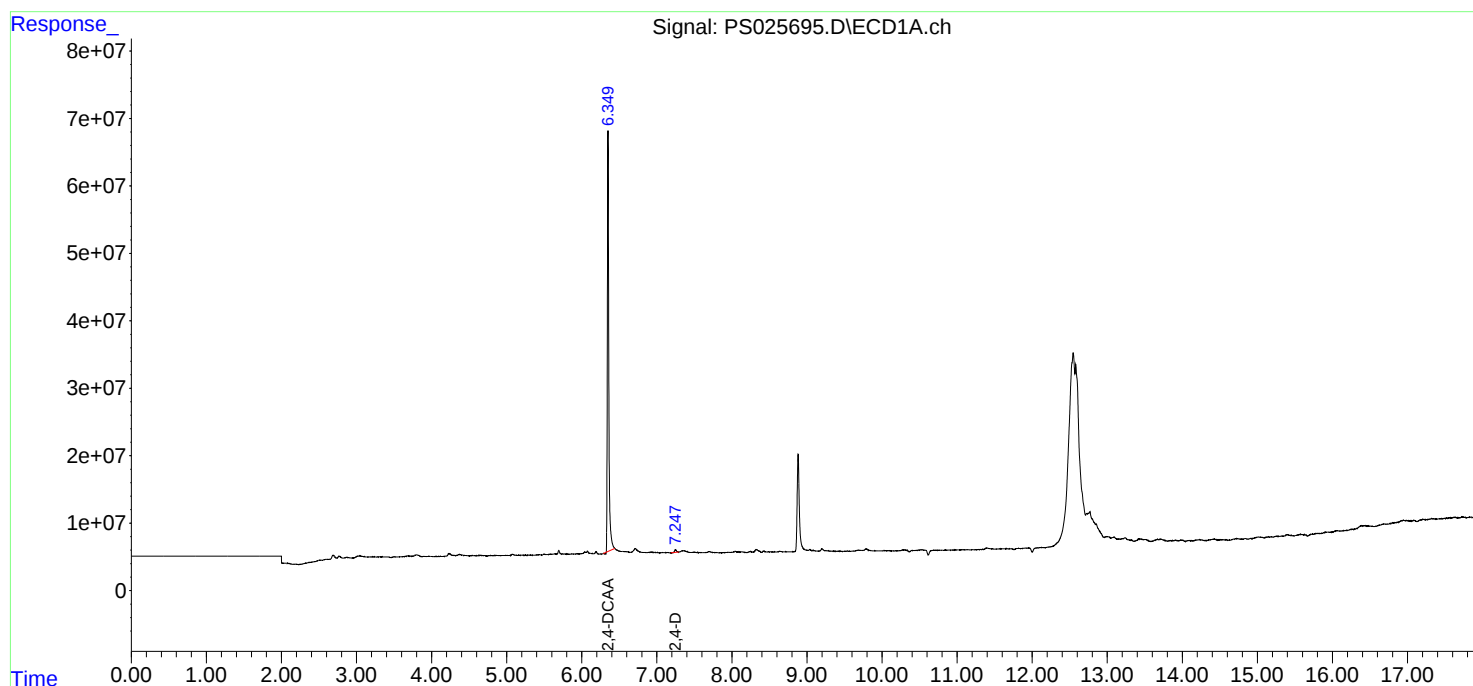


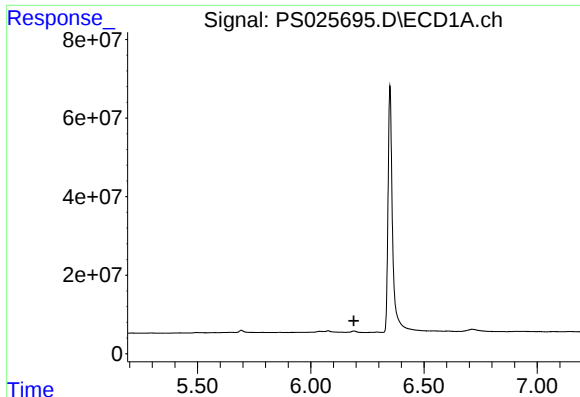

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-39

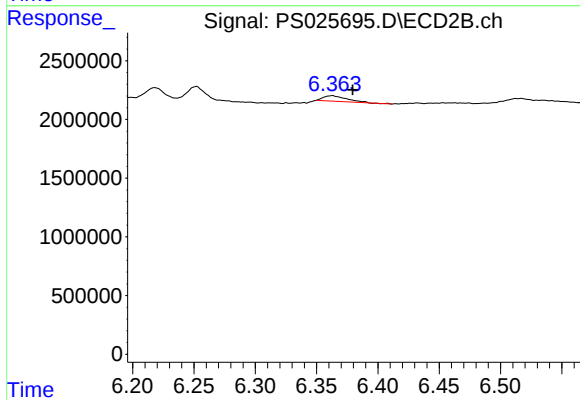


#3 4-Nitrophenol

R.T.: 6.363 min
Delta R.T.: -0.017 min
Response: 634777
Conc: 1.33 ng/ml

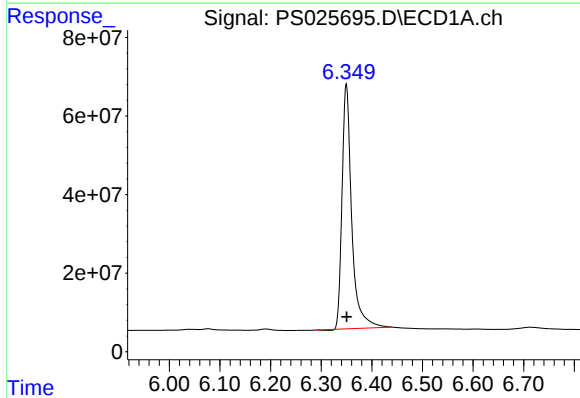


#4 2,4-DCAA

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 827444960
Conc: 555.53 ng/ml

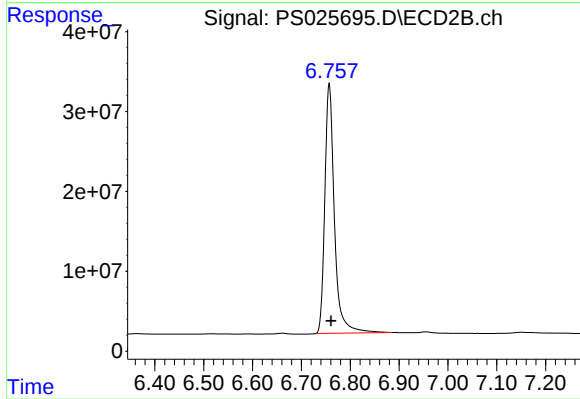

#4 2,4-DCAA


R.T.: 6.757 min
Delta R.T.: -0.004 min
Response: 427292160
Conc: 556.51 ng/ml

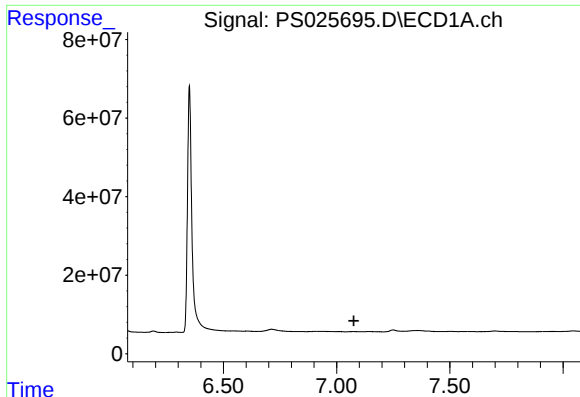

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-39

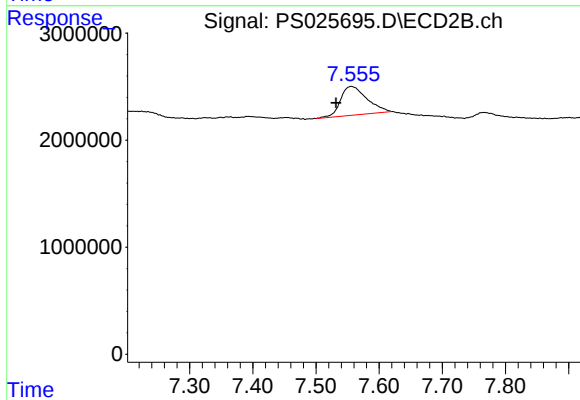


#8 DICHLORPROP

R.T.: 7.556 min
Delta R.T.: 0.024 min
Response: 7814585
Conc: 9.04 ng/ml

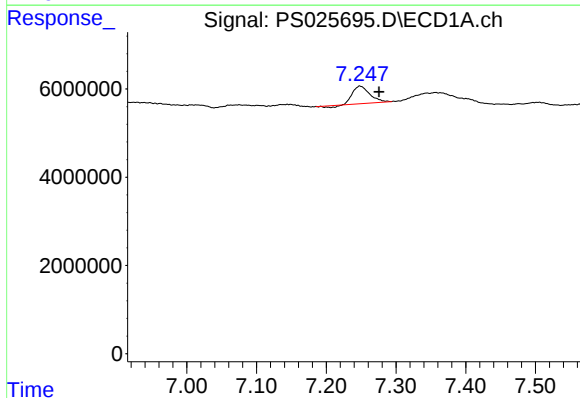

#9 2,4-D

R.T.: 7.248 min
Delta R.T.: -0.027 min
Response: 6520916
Conc: 3.54 ng/ml

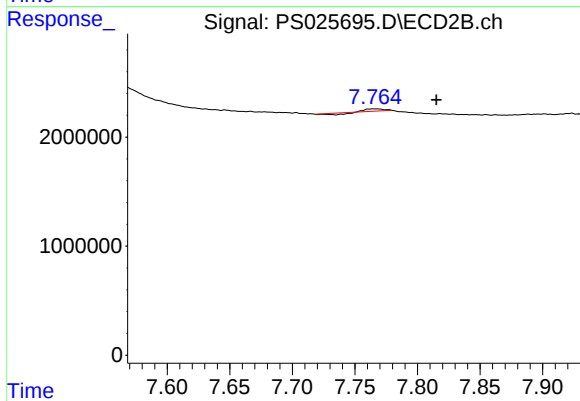

#9 2,4-D

R.T.: 7.766 min
Delta R.T.: -0.049 min
Response: 103226
Conc: N.D.