

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013024\
 Data File : PS025683.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2024 16:08
 Operator : AR\AJ
 Sample : PB158616TB
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB158616TB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/31/2024
 Supervised By : Ankita Jodhani 01/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 02:05:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.755	649.6E6	321.8E6	436.100m	419.096m
Target Compounds							
13) T	2,4-DB	8.793	9.465	558.7E6	329.0E6	519.008	630.230m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013024\
Data File : PS025683.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2024 16:08
Operator : AR\AJ
Sample : PB158616TB
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB158616TB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/31/2024
Supervised By : Ankita Jodhani 01/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 02:05:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

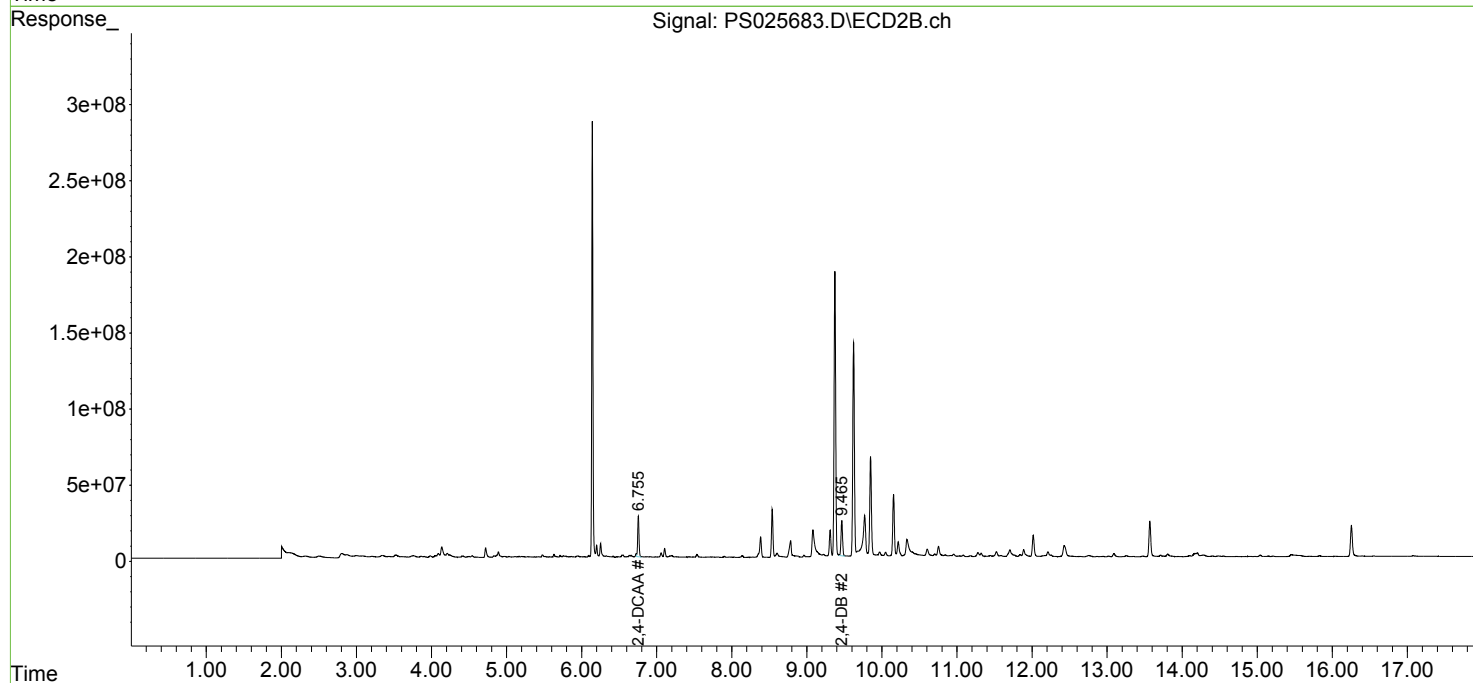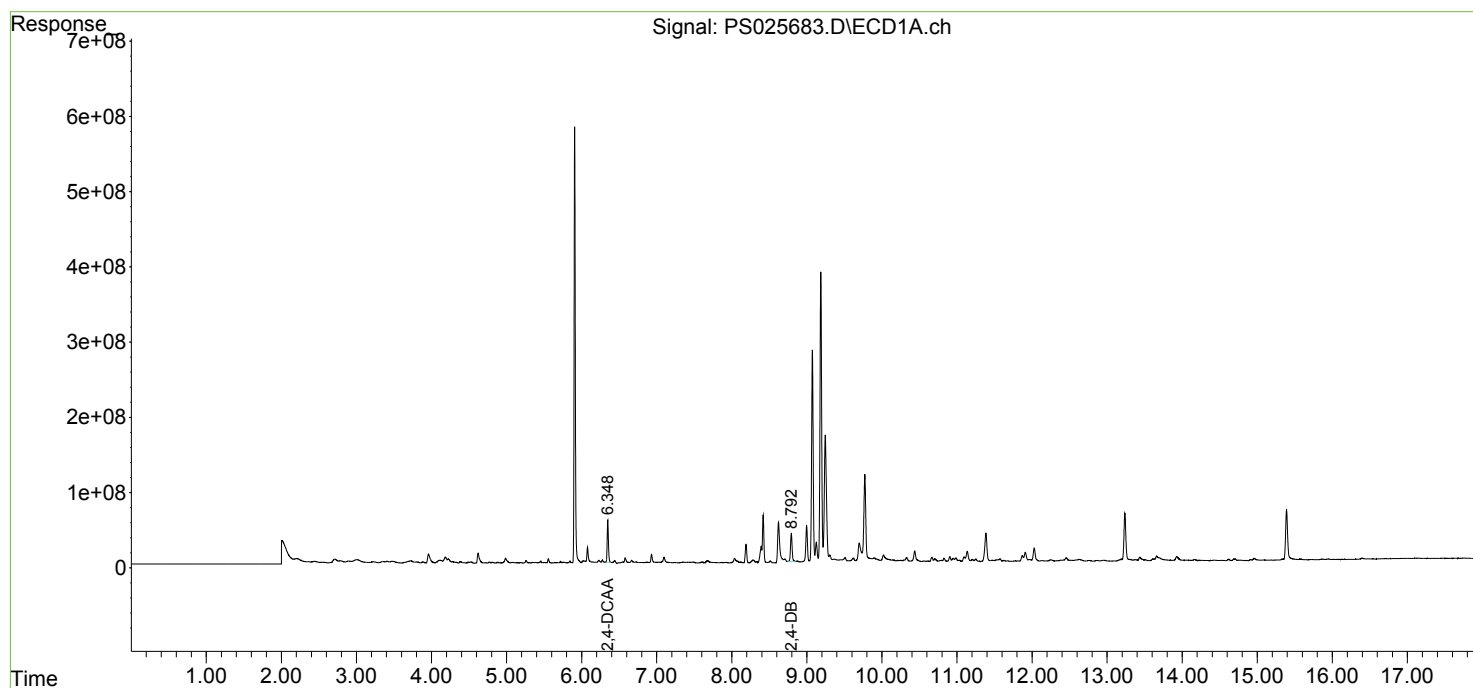

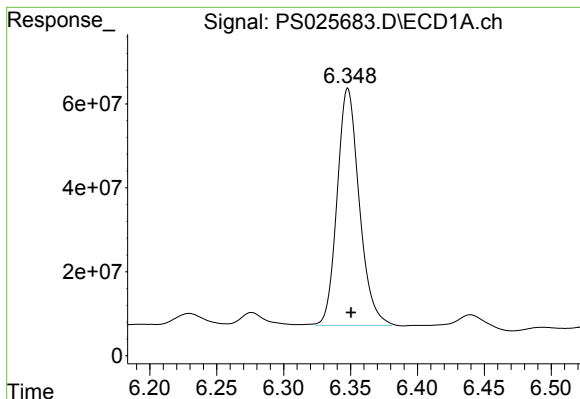


#4 2,4-DCAA

R.T.: 6.348 min
Delta R.T.: -0.003 min
Response: 649555149
Conc: 436.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB158616TB


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2024
Supervised By :Ankita Jodhani 01/31/2024

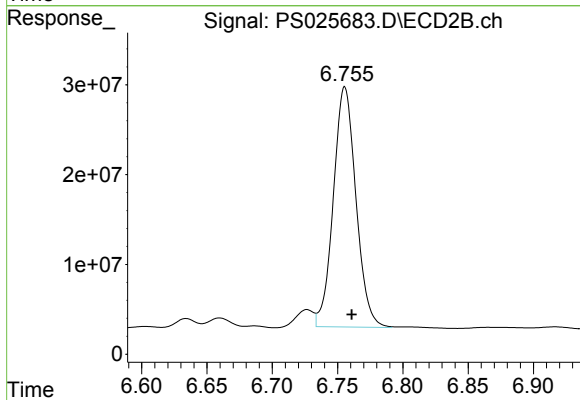


#4 2,4-DCAA

R.T.: 6.755 min
Delta R.T.: -0.006 min
Response: 321782485
Conc: 419.10 ng/ml m

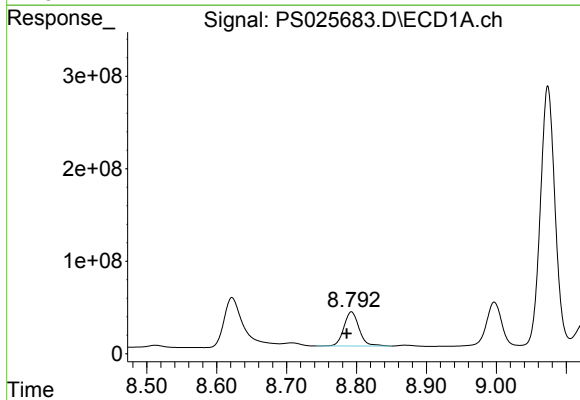

#13 2,4-DB

R.T.: 8.793 min
Delta R.T.: 0.006 min
Response: 558673564
Conc: 519.01 ng/ml

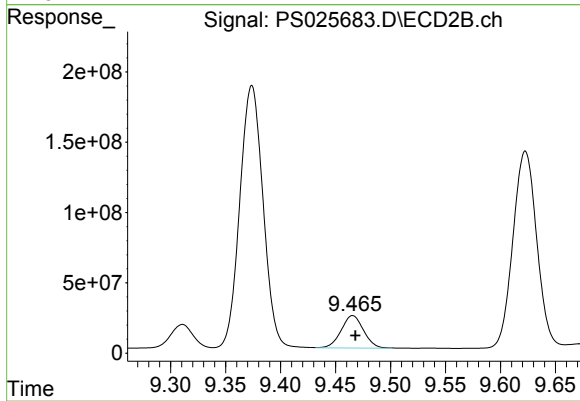

#13 2,4-DB

R.T.: 9.465 min
Delta R.T.: -0.003 min
Response: 328996882
Conc: 630.23 ng/ml m