

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 19:55
 Operator : DD\AJ
 Sample : L1309-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CTY-WC-S-SB-0102

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:29:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.959	782.4E6	412.5E6	443.088	435.359
Target Compounds							
1) T	Dalapon	2.498	2.183	193.6E6	70266478	75.510	55.426 #
2) T	3,5-DICHL...	0.000	5.146	0	146.5E6	N.D.	104.855
5) T	DICAMBA	0.000	6.093	0	12750790	N.D.	3.188
6) T	MCP	6.704	0.000	120.6E6	0	23.668	N.D. #
7) T	MCPA	0.000	6.483	0	26034238	N.D.	6.097
8) T	DICHLORPROP	0.000	6.778	0	36248780	N.D.	37.519
10) T	Pentachlo...	7.746	0.000	29118785	0	1.198	N.D. #
12) T	2,4,5-T	8.595	8.287	12648832	20224701	1.371	3.825 #
14) T	DINOSEB	0.000	9.111	0	74204452	N.D.	19.643
15) T	Picloram	10.032	0.000	37986674	0	3.043	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 19:55
Operator : DD\AJ
Sample : L1309-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:29:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

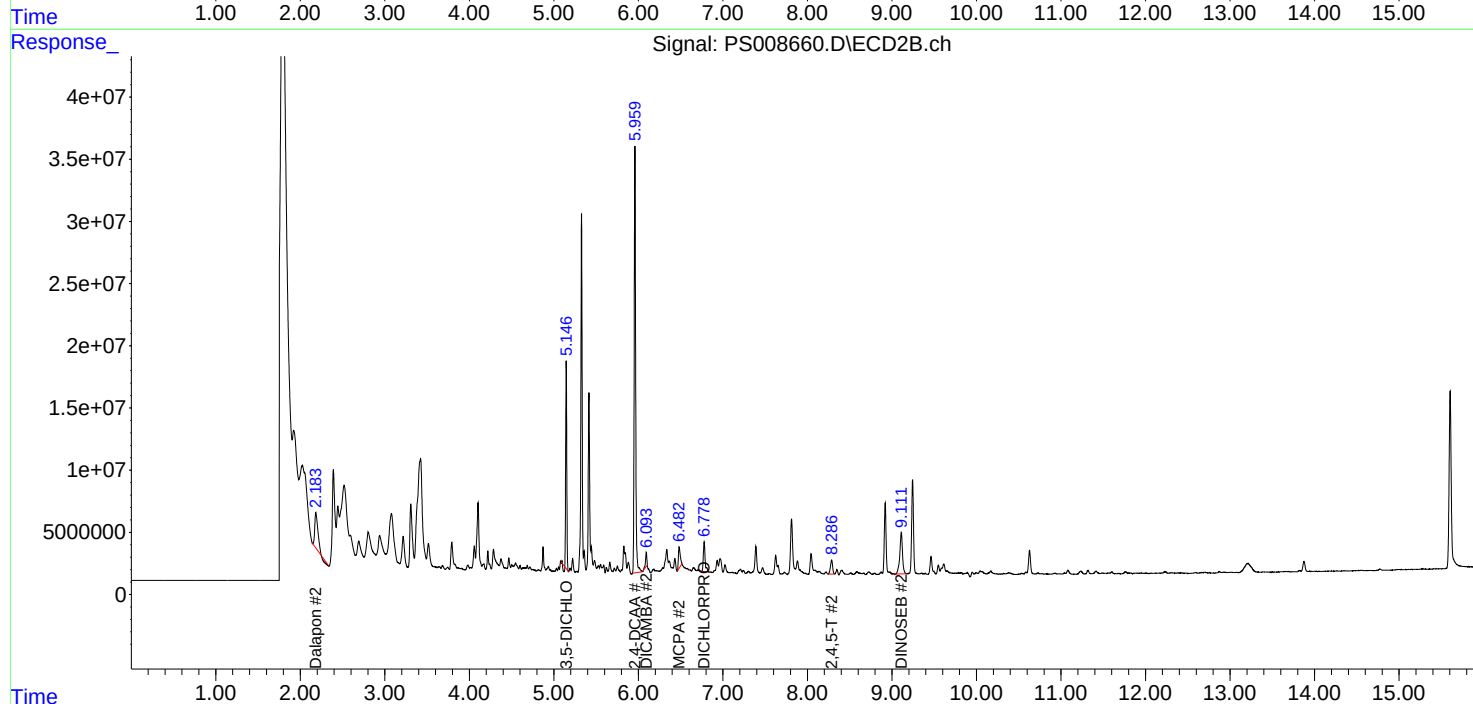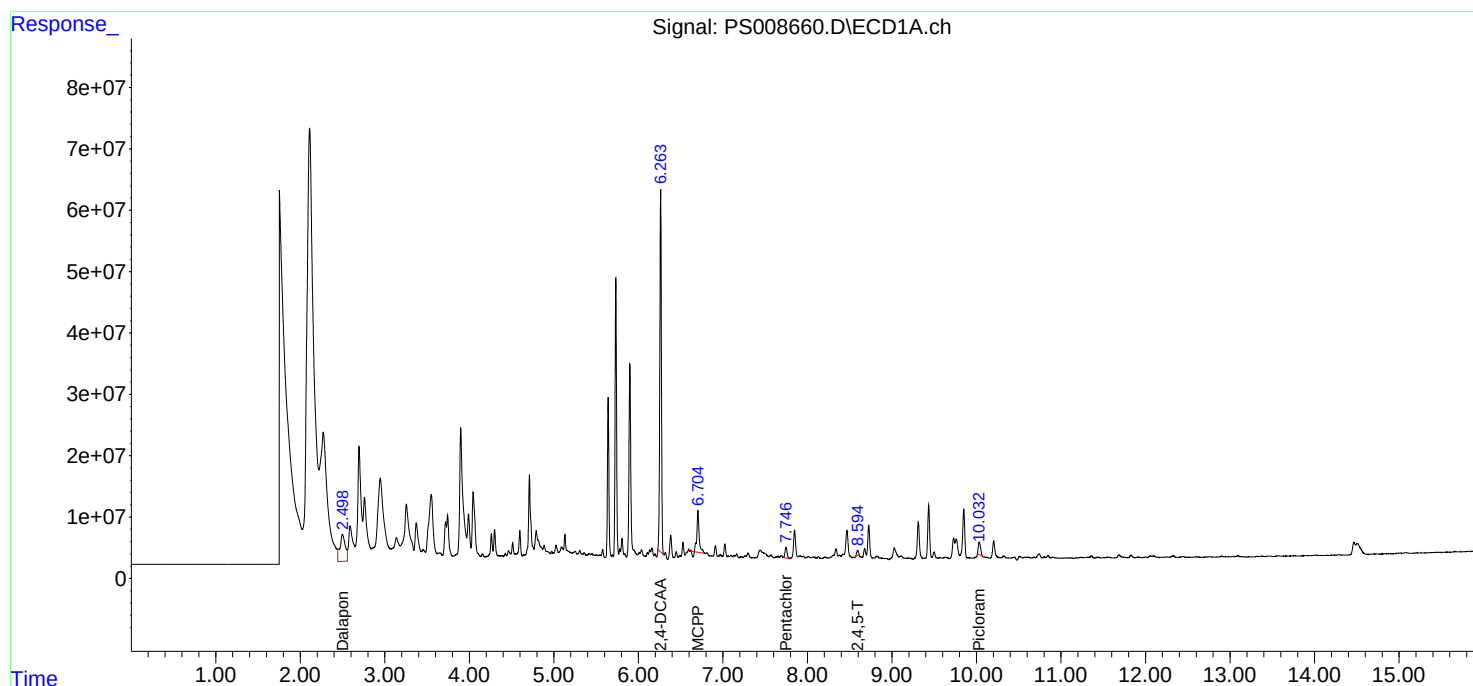


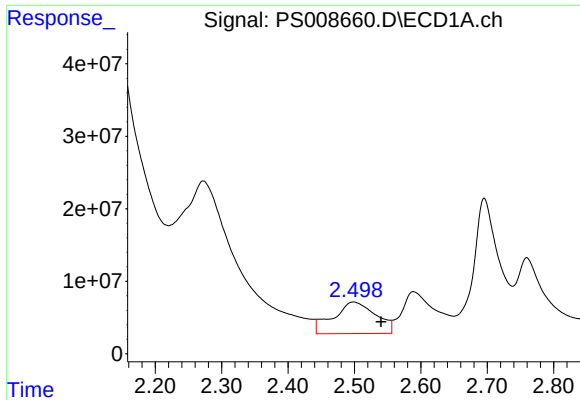

#1 Dalapon


R.T.: 2.498 min
Delta R.T.: -0.042 min
Response: 193595810
Conc: 75.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

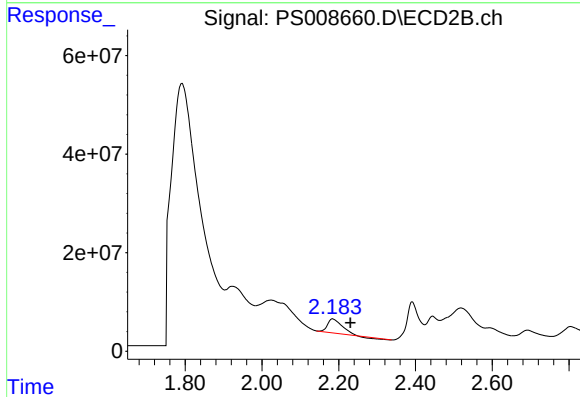


#1 Dalapon

R.T.: 2.183 min
Delta R.T.: -0.048 min
Response: 70266478
Conc: 55.43 ng/ml

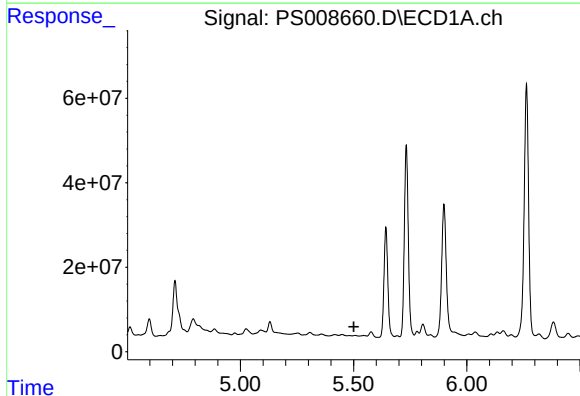


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

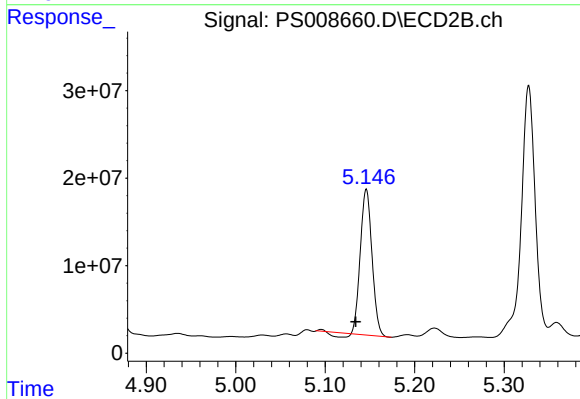

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.012 min
Response: 146500605
Conc: 104.85 ng/ml

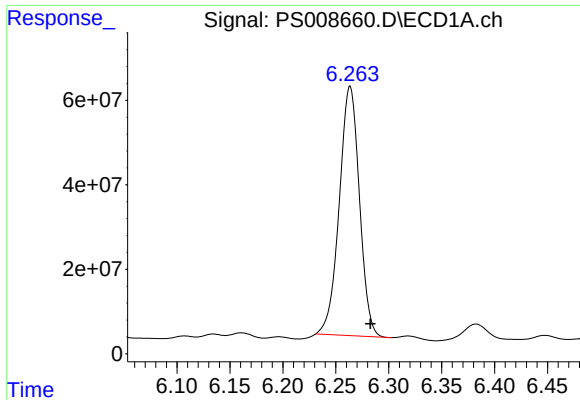

#4 2,4-DCAA


R.T.: 6.263 min
Delta R.T.: -0.019 min
Response: 782362045
Conc: 443.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

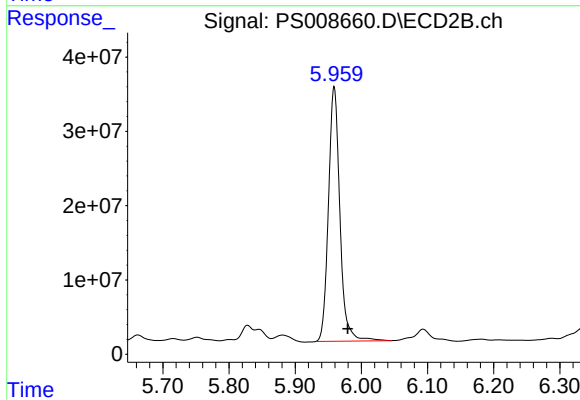


#4 2,4-DCAA

R.T.: 5.959 min
Delta R.T.: -0.020 min
Response: 412486131
Conc: 435.36 ng/ml

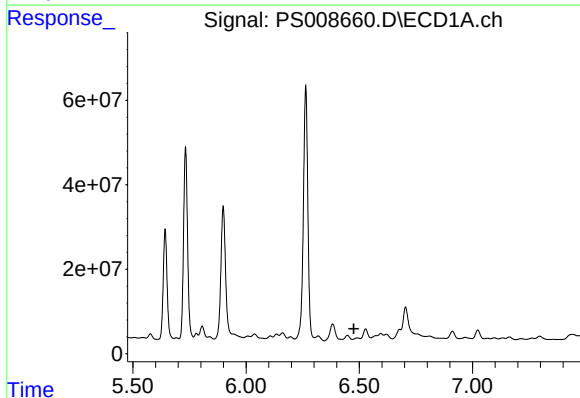


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

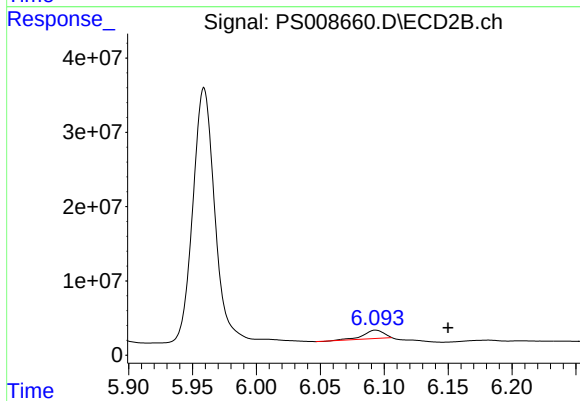

#5 DICAMBA


R.T.: 6.093 min
Delta R.T.: -0.056 min
Response: 12750790
Conc: 3.19 ng/ml

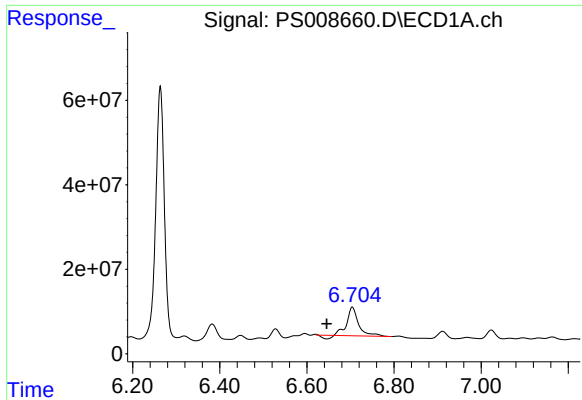

#6 MCPP


R.T.: 6.704 min
Delta R.T.: 0.059 min
Response: 120631563
Conc: 23.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

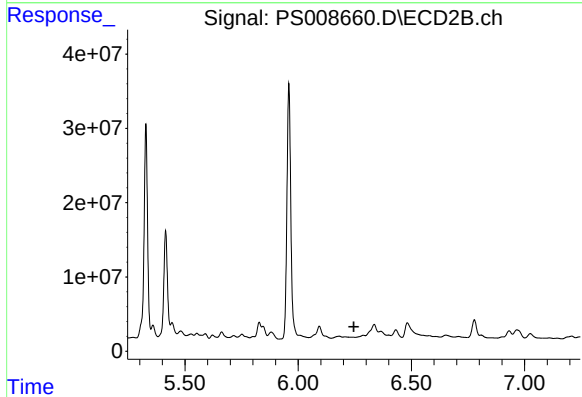


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

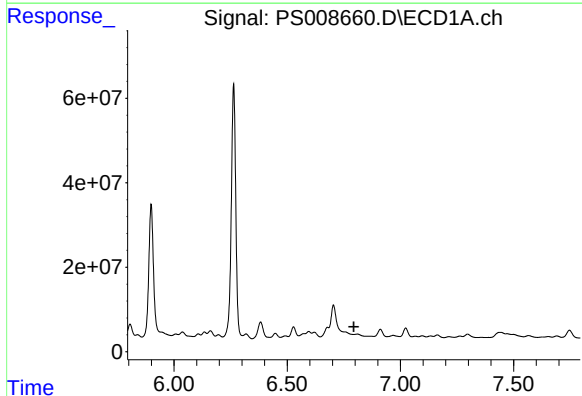


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

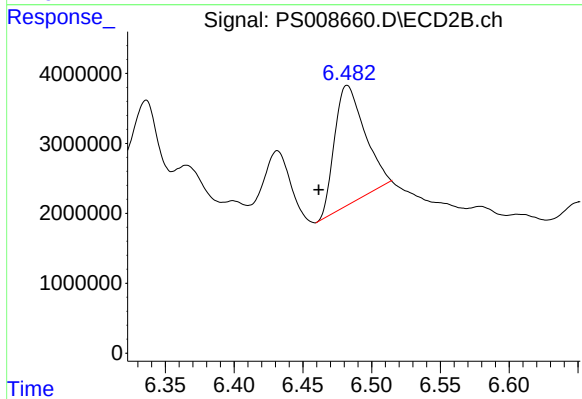

#7 MCPA


R.T.: 6.483 min
Delta R.T.: 0.021 min
Response: 26034238
Conc: 6.10 ug/ml

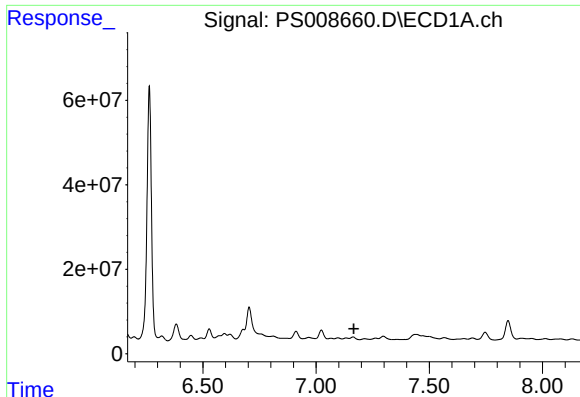

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

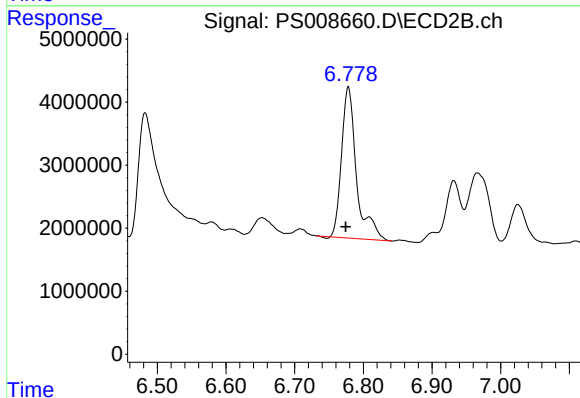


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.003 min
Response: 36248780
Conc: 37.52 ng/ml

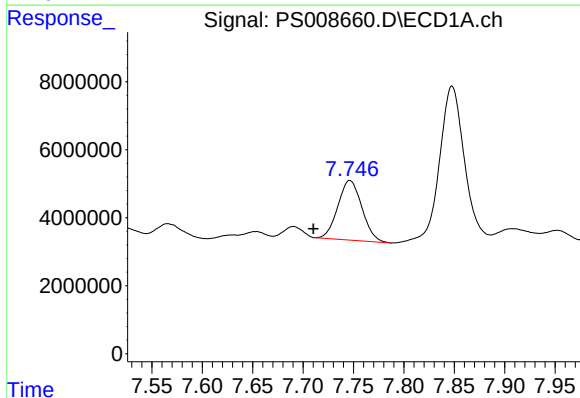


#10 Pentachlorophenol

R.T.: 7.746 min
Delta R.T.: 0.036 min
Response: 29118785
Conc: 1.20 ng/ml

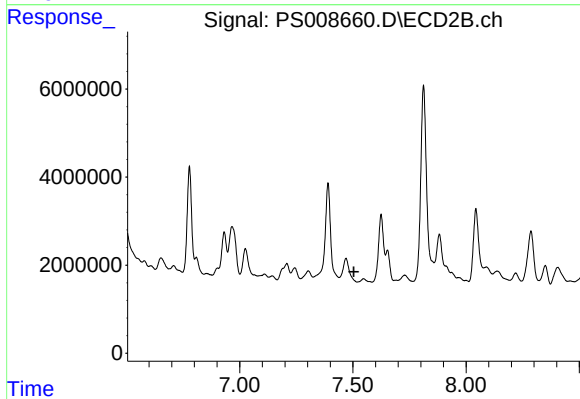

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

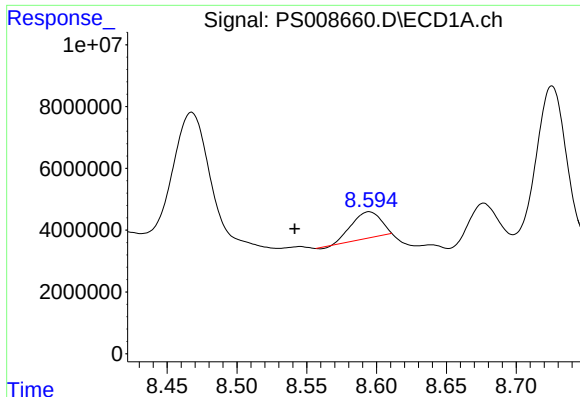

#12 2,4,5-T


R.T.: 8.595 min
Delta R.T.: 0.053 min
Response: 12648832
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

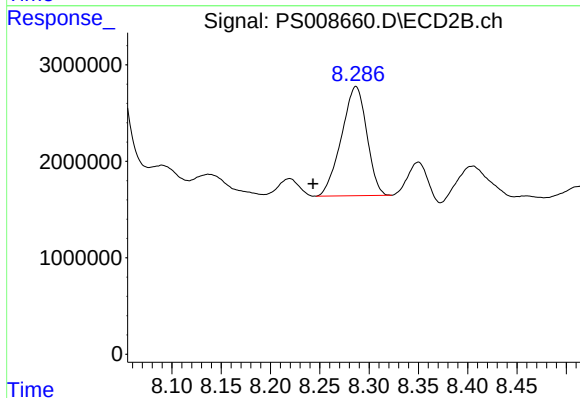


#12 2,4,5-T

R.T.: 8.287 min
Delta R.T.: 0.043 min
Response: 20224701
Conc: 3.82 ng/ml

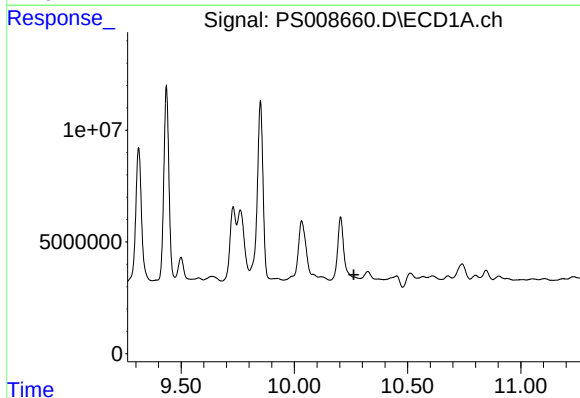


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

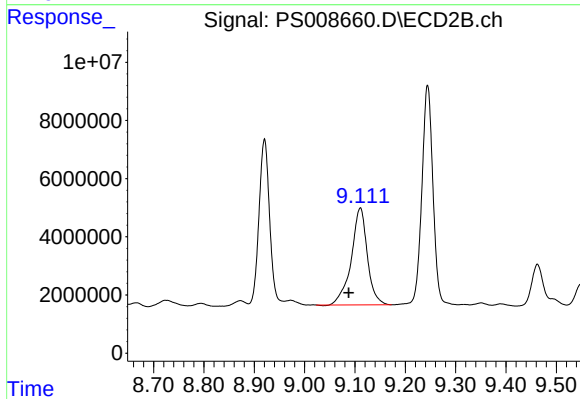

#14 DINOSEB


R.T.: 9.111 min
Delta R.T.: 0.023 min
Response: 74204452
Conc: 19.64 ng/ml

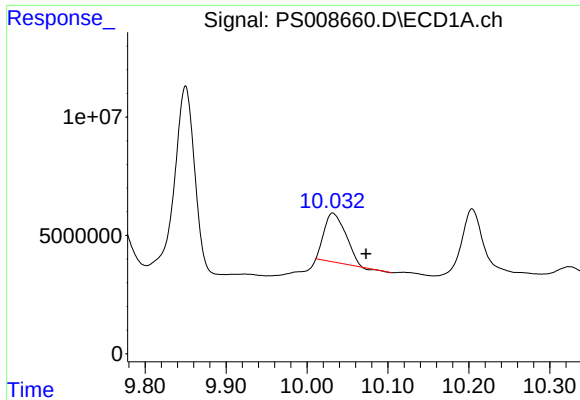

#15 Picloram

R.T.: 10.032 min
Delta R.T.: -0.041 min
Response: 37986674
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-WC-S-SB-0102

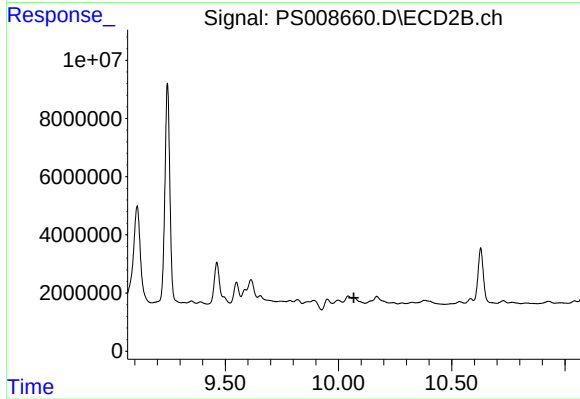

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.