

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 20:17
 Operator : DD\AJ
 Sample : L1325-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 346

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:30:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.959	690.5E6	355.9E6	391.059	375.677
Target Compounds							
1) T	Dalapon	2.498	2.184	167.5E6	61806129	65.313	48.753 #
2) T	3,5-DICHL...	0.000	5.146	0	128.6E6	N.D.	92.057
3) T	4-Nitroph...	6.133	0.000	14423438	0	14.809	N.D. #
5) T	DICAMBA	0.000	6.092	0	15676280	N.D.	3.920
6) T	MCPD	6.677	0.000	29295513	0	5.748	N.D. #
7) T	MCPA	0.000	6.481	0	39764538	N.D.	9.313
8) T	DICHLORPROP	0.000	6.777	0	34047829	N.D.	35.241
9) T	2,4-D	0.000	7.025	0	10449601	N.D.	8.914
10) T	Pentachlo...	7.746	0.000	31903273	0	1.312	N.D. #
12) T	2,4,5-T	8.594	8.287	12753203	18701155	1.382	3.536 #
14) T	DINOSEB	0.000	9.110	0	70631800	N.D.	18.697
15) T	Picloram	10.032	0.000	33589629	0	2.691	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 20:17
Operator : DD\AJ
Sample : L1325-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
346

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:30:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

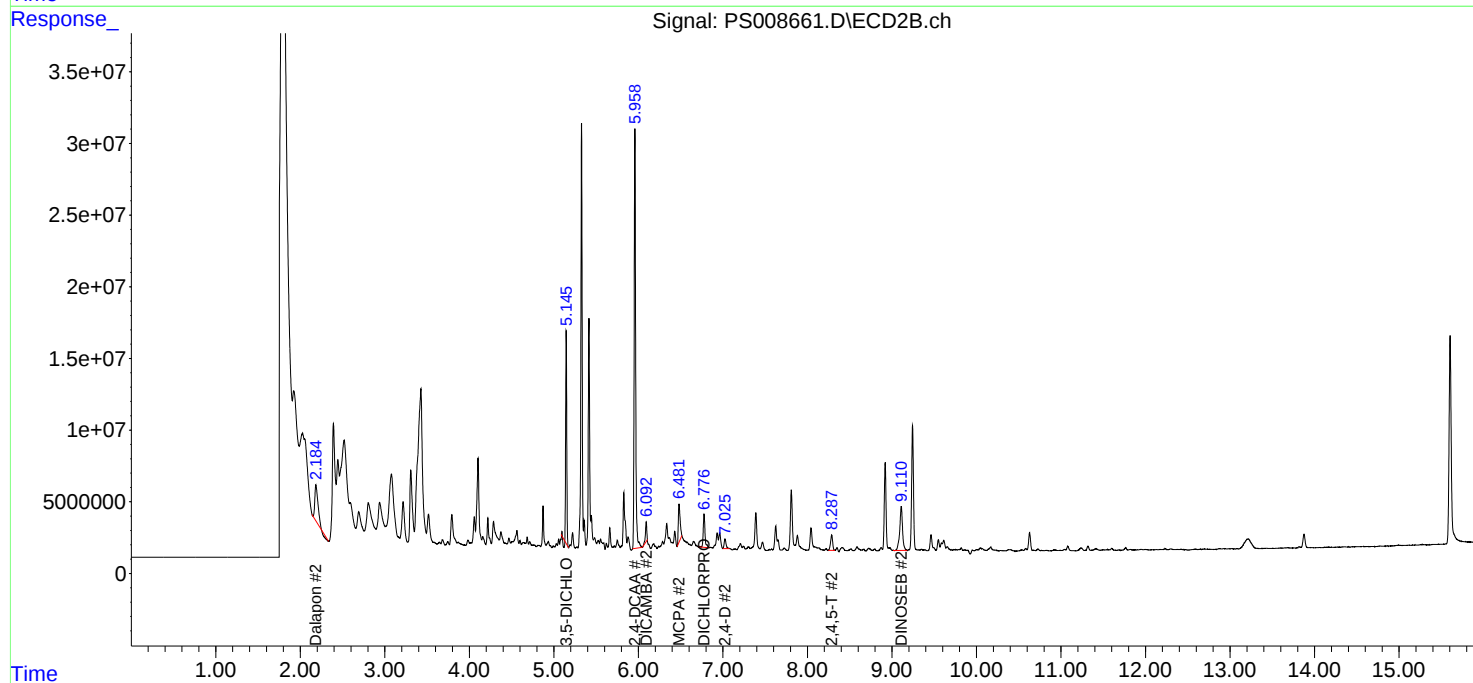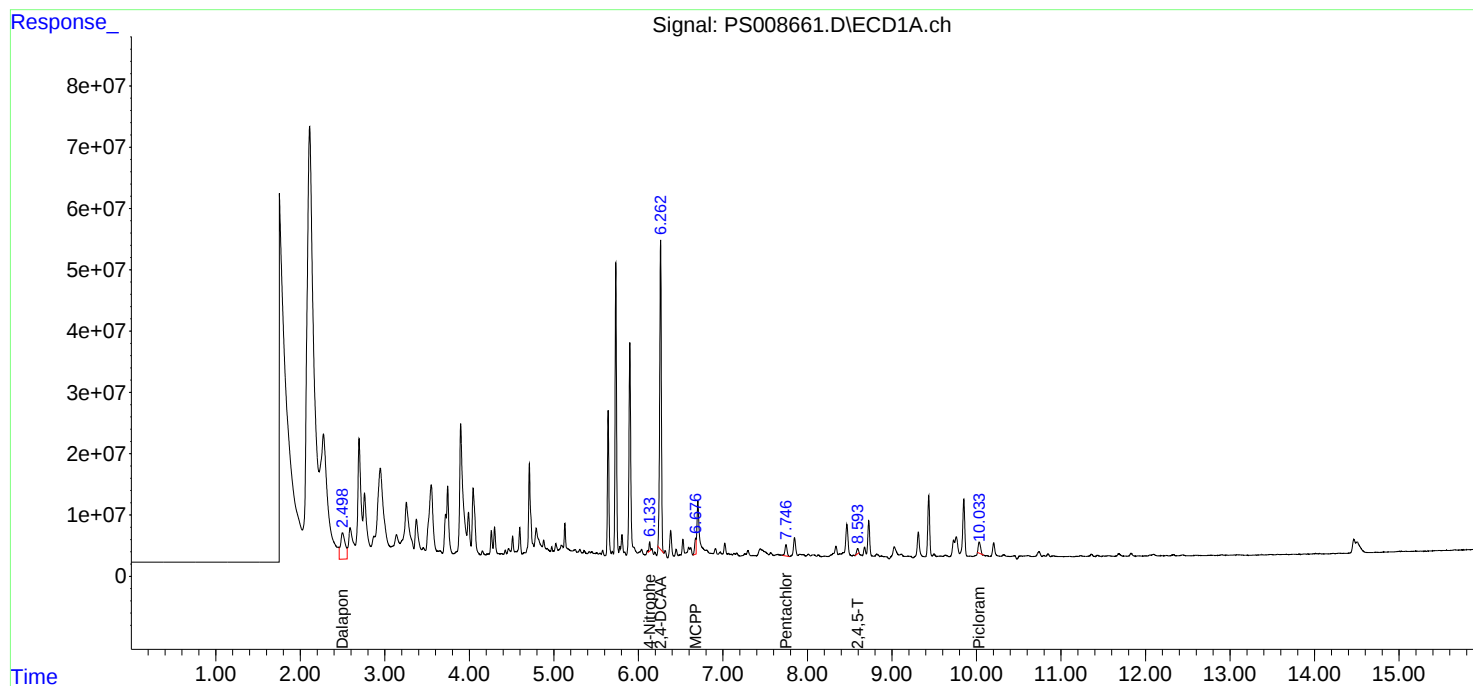


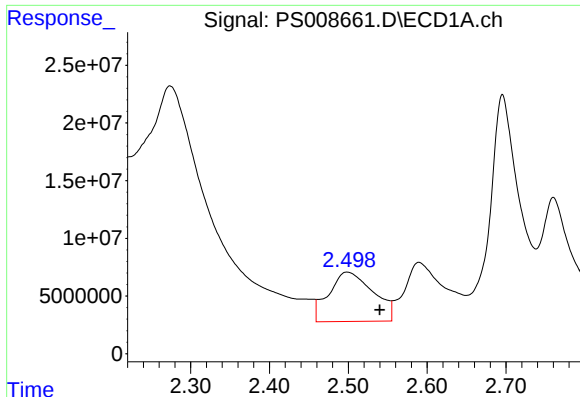

#1 Dalapon


R.T.: 2.498 min
Delta R.T.: -0.042 min
Response: 167452522
Conc: 65.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
346

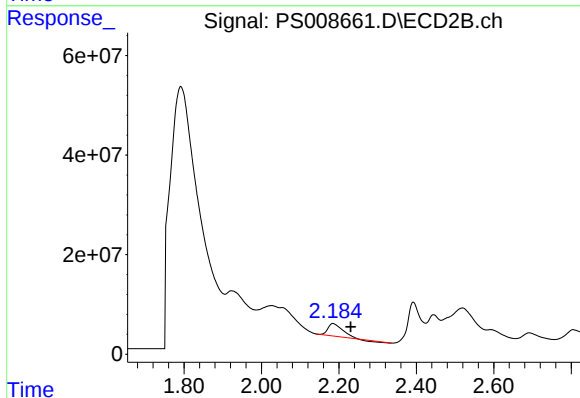


#1 Dalapon

R.T.: 2.184 min
Delta R.T.: -0.047 min
Response: 61806129
Conc: 48.75 ng/ml

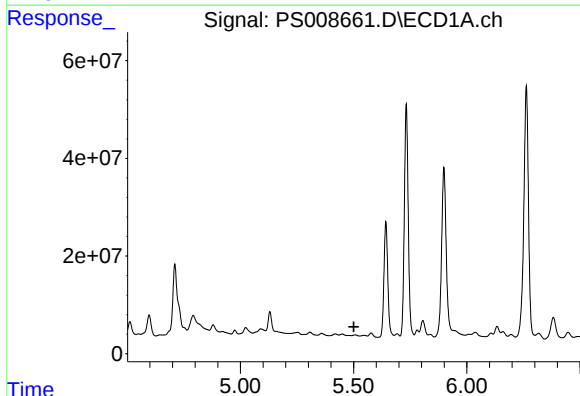


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

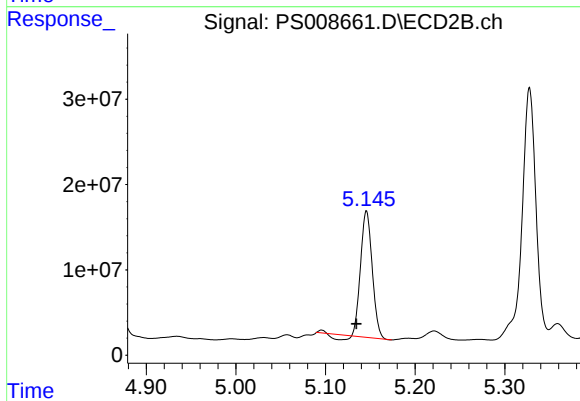

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 128620360
Conc: 92.06 ng/ml

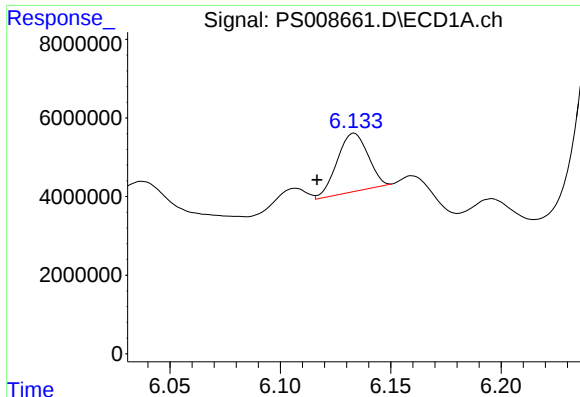

#3 4-Nitrophenol


R.T.: 6.133 min
Delta R.T.: 0.017 min
Response: 14423438
Conc: 14.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
346

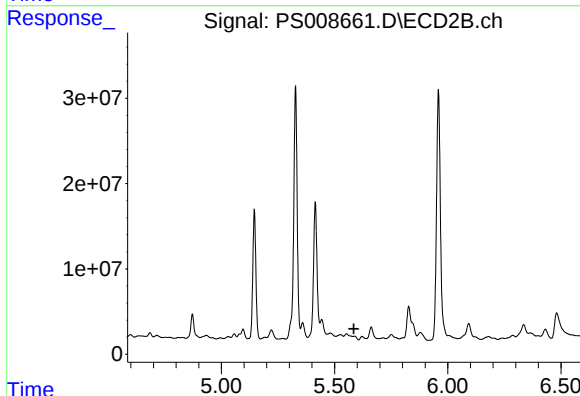


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

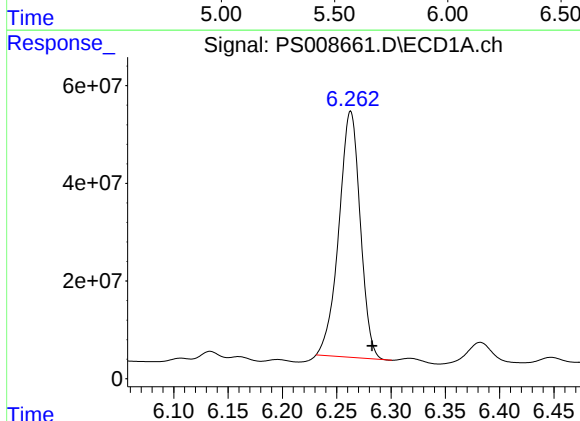


#4 2,4-DCAA

R.T.: 6.263 min
Delta R.T.: -0.020 min
Response: 690494143
Conc: 391.06 ng/ml

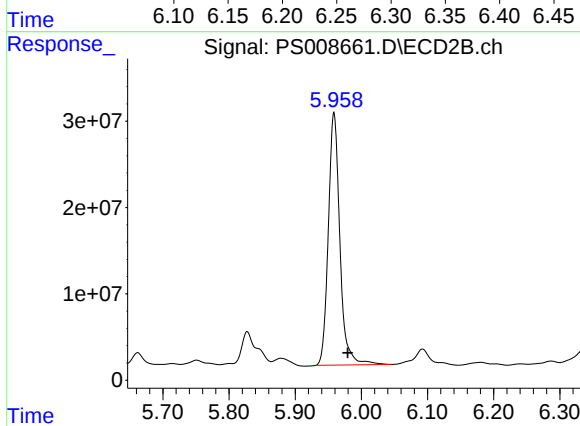

#4 2,4-DCAA


R.T.: 5.959 min
Delta R.T.: -0.020 min
Response: 355940261
Conc: 375.68 ng/ml

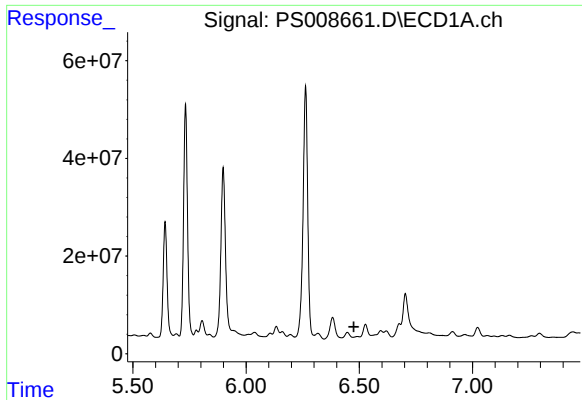

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
346

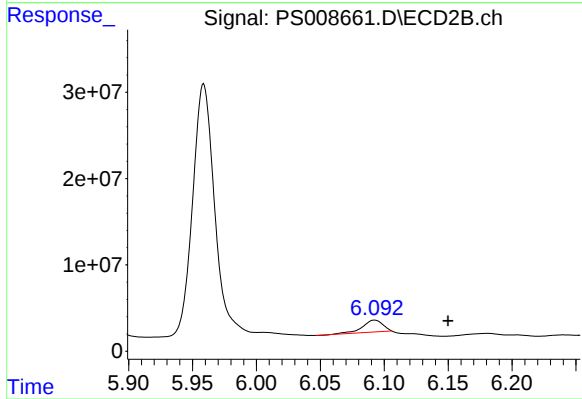


#5 DICAMBA

R.T.: 6.092 min
Delta R.T.: -0.057 min
Response: 15676280
Conc: 3.92 ng/ml

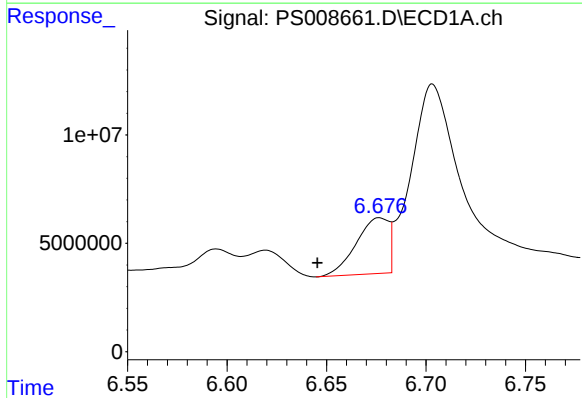


#6 MCP

R.T.: 6.677 min
Delta R.T.: 0.031 min
Response: 29295513
Conc: 5.75 ug/ml

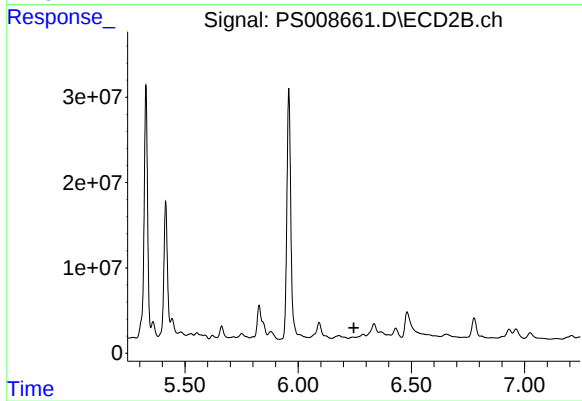

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

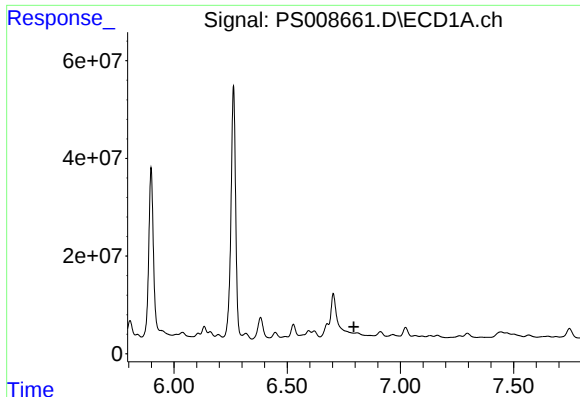

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
346

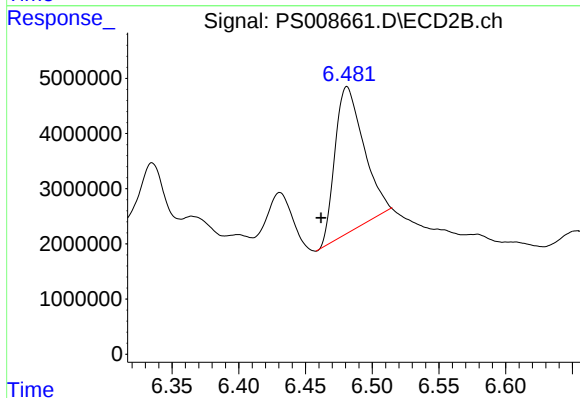


#7 MCPA

R.T.: 6.481 min
Delta R.T.: 0.020 min
Response: 39764538
Conc: 9.31 ug/ml

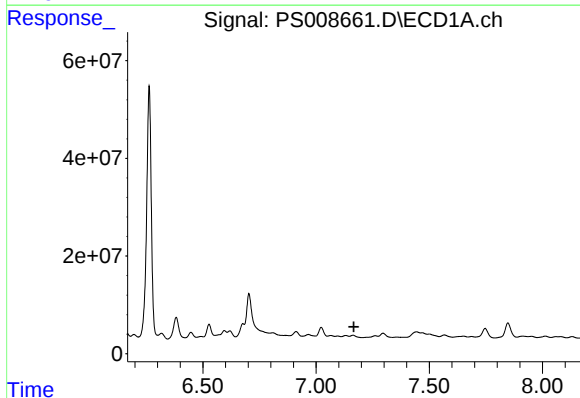


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

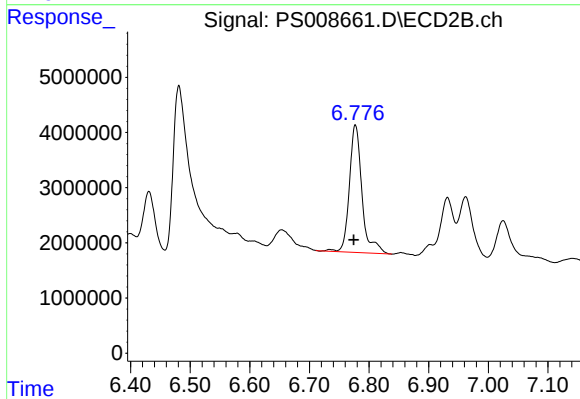

#8 DICHLORPROP


R.T.: 6.777 min
Delta R.T.: 0.003 min
Response: 34047829
Conc: 35.24 ng/ml

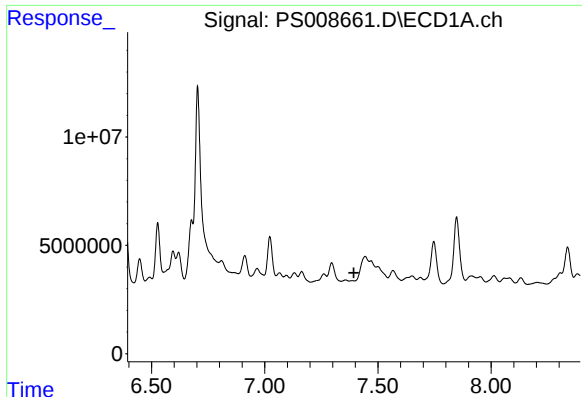

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
346

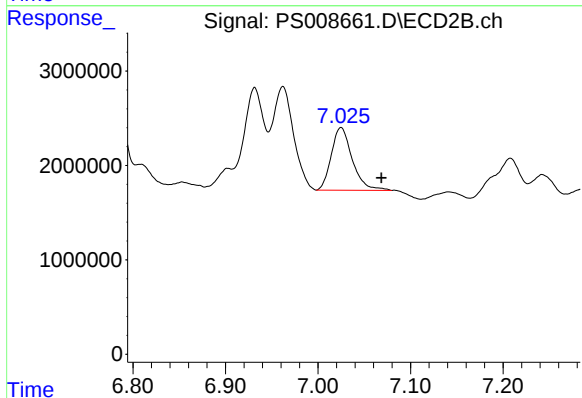


#9 2,4-D

R.T.: 7.025 min
Delta R.T.: -0.044 min
Response: 10449601
Conc: 8.91 ng/ml

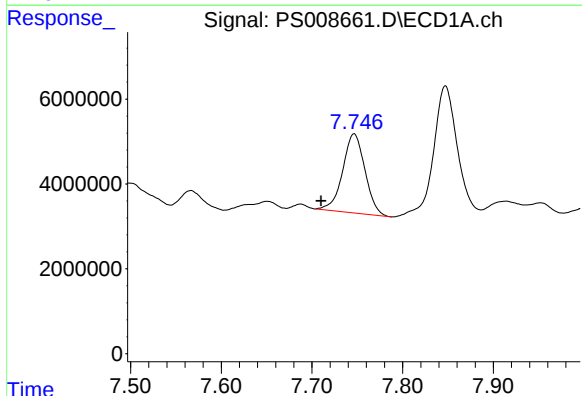


#10 Pentachlorophenol

R.T.: 7.746 min
Delta R.T.: 0.036 min
Response: 31903273
Conc: 1.31 ng/ml

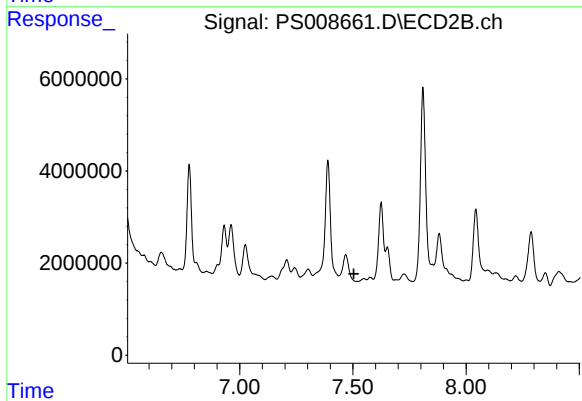

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

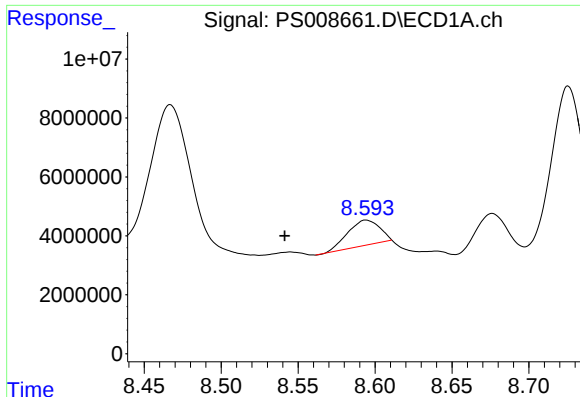

#12 2,4,5-T


R.T.: 8.594 min
Delta R.T.: 0.053 min
Response: 12753203
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
346

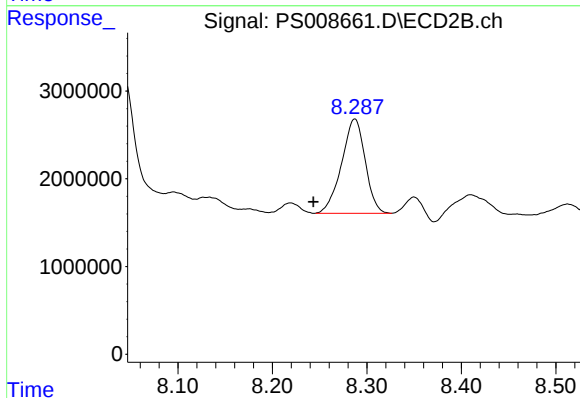


#12 2,4,5-T

R.T.: 8.287 min
Delta R.T.: 0.044 min
Response: 18701155
Conc: 3.54 ng/ml

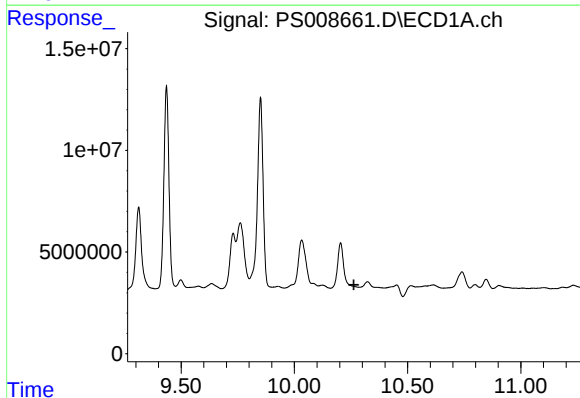


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

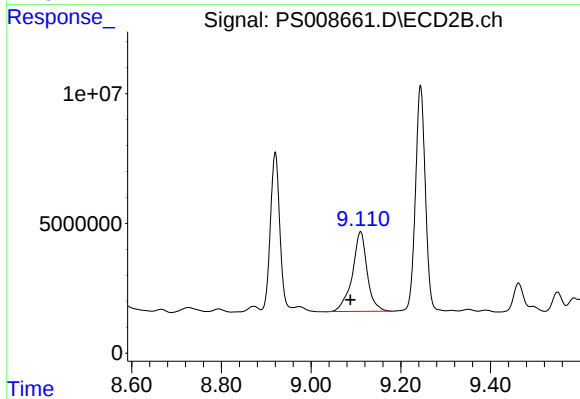

#14 DINOSEB

R.T.: 9.110 min
Delta R.T.: 0.022 min
Response: 70631800
Conc: 18.70 ng/ml

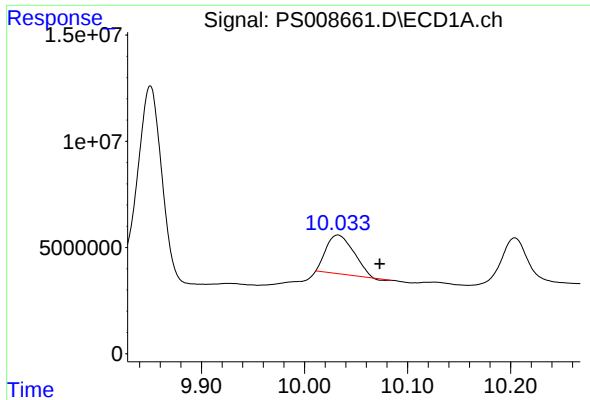

#15 Picloram


R.T.: 10.032 min

Delta R.T.: -0.041 min

Response: 33589629

Conc: 2.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
346

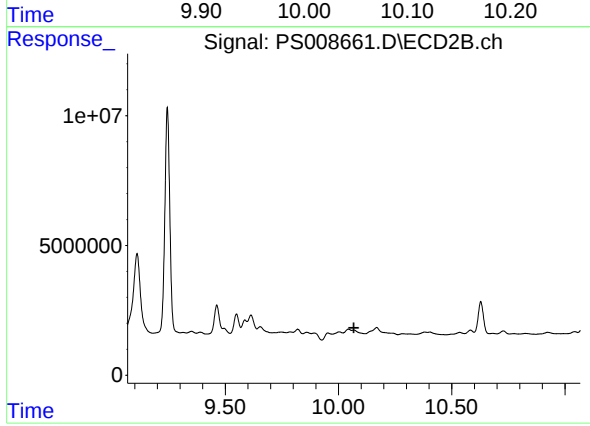

#15 Picloram

R.T.: 0.000 min

Exp R.T. : 10.068 min

Response: 0

Conc: N.D.