

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 20:39
 Operator : DD\AJ
 Sample : L1325-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:30:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.262	5.959	702.3E6	361.4E6	397.731	381.482
Target Compounds							
1) T	Dalapon	2.499	2.184	195.3E6	68449514	76.176	53.993 #
2) T	3,5-DICHL...	0.000	5.146	0	122.3E6	N.D.	87.561
3) T	4-Nitroph...	6.133	0.000	38407377	0	39.434	N.D. #
5) T	DICAMBA	0.000	6.093	0	12626483	N.D.	3.157
6) T	MCPD	6.703	0.000	195.3E6	0	38.316	N.D. #
7) T	MCPA	0.000	6.480	0	53301579	N.D.	12.483
8) T	DICHLORPROP	0.000	6.777	0	34160129	N.D.	35.357
9) T	2,4-D	0.000	7.025	0	10541273	N.D.	8.992
10) T	Pentachlo...	7.746	0.000	33238839	0	1.367	N.D. #
12) T	2,4,5-T	8.594	8.288	11031133	13911921	1.196	2.631 #
14) T	DINOSEB	0.000	9.110	0	69074669	N.D.	18.285
15) T	Picloram	10.030	0.000	28169571	0	2.257	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 20:39
Operator : DD\AJ
Sample : L1325-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:30:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

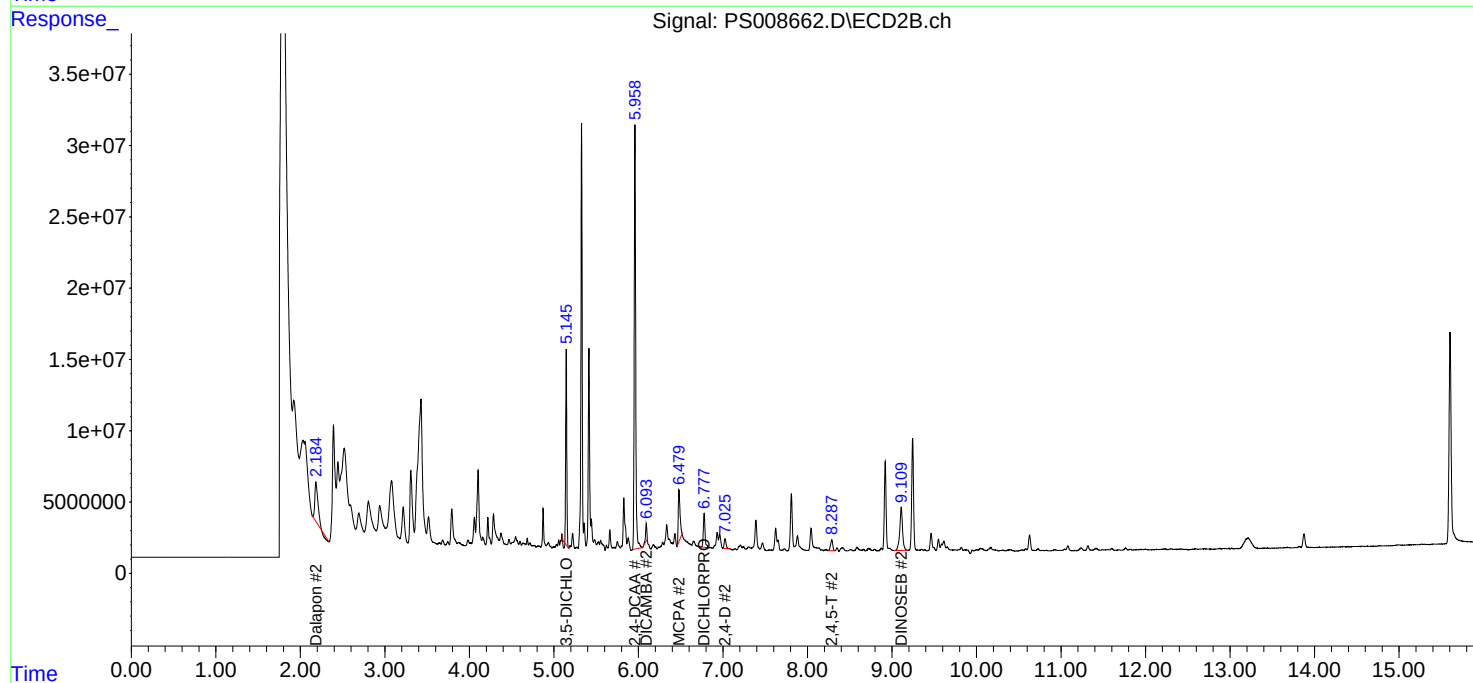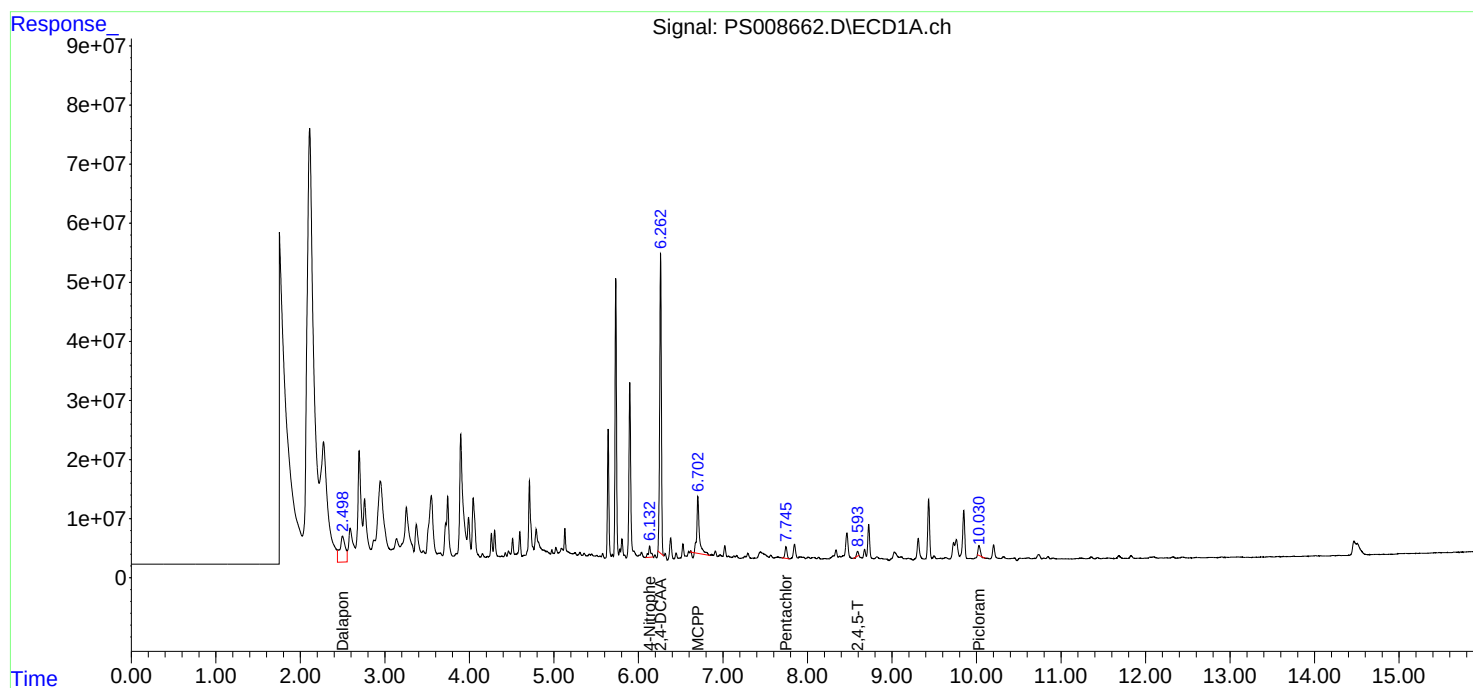


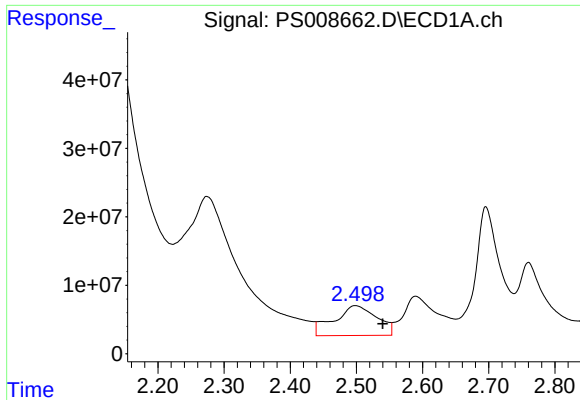

#1 Dalapon


R.T.: 2.499 min
Delta R.T.: -0.041 min
Response: 195304296
Conc: 76.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

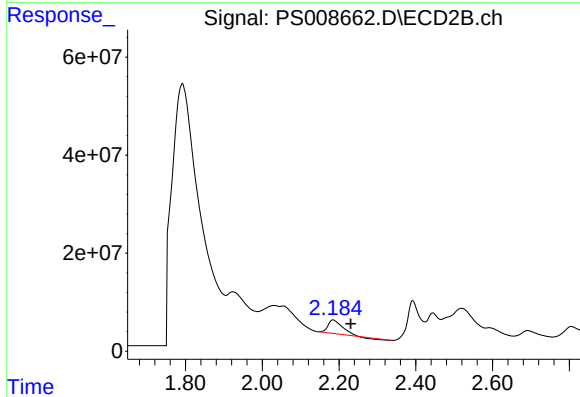


#1 Dalapon

R.T.: 2.184 min
Delta R.T.: -0.047 min
Response: 68449514
Conc: 53.99 ng/ml

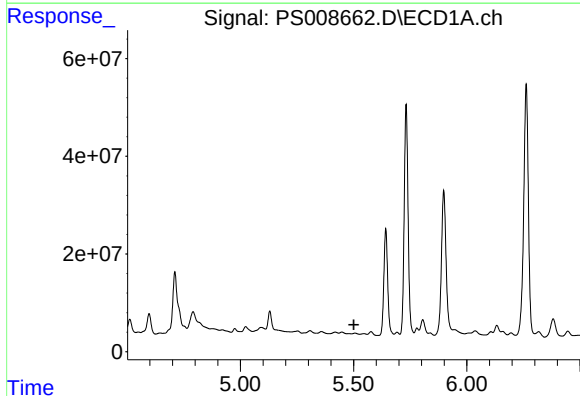


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

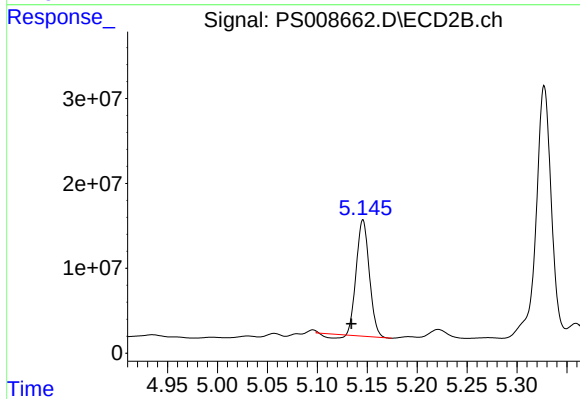

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 122337469
Conc: 87.56 ng/ml

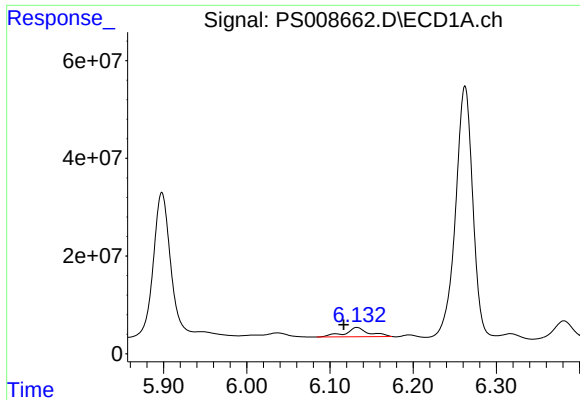

#3 4-Nitrophenol


R.T.: 6.133 min
Delta R.T.: 0.016 min
Response: 38407377
Conc: 39.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

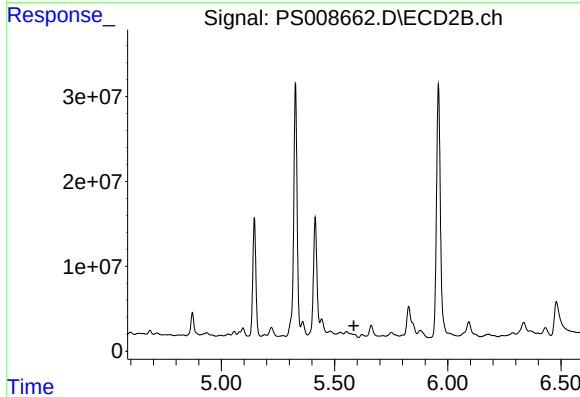


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

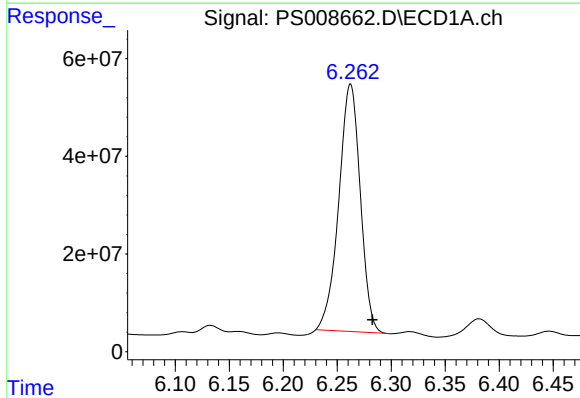


#4 2,4-DCAA

R.T.: 6.262 min
Delta R.T.: -0.020 min
Response: 702274699
Conc: 397.73 ng/ml

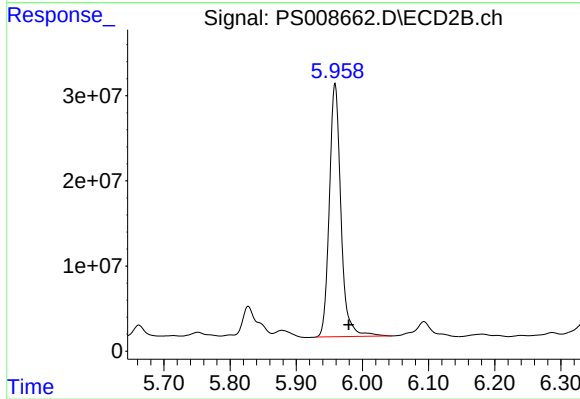

#4 2,4-DCAA


R.T.: 5.959 min
Delta R.T.: -0.021 min
Response: 361440408
Conc: 381.48 ng/ml

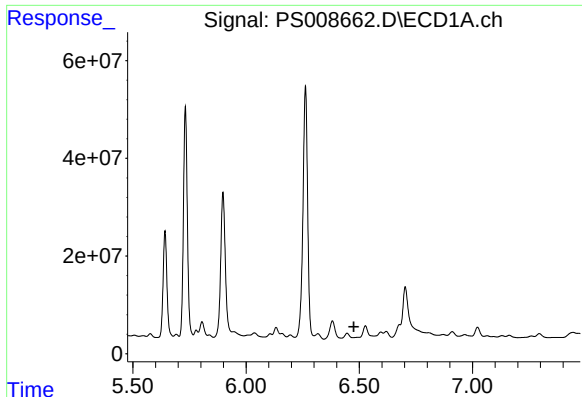

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

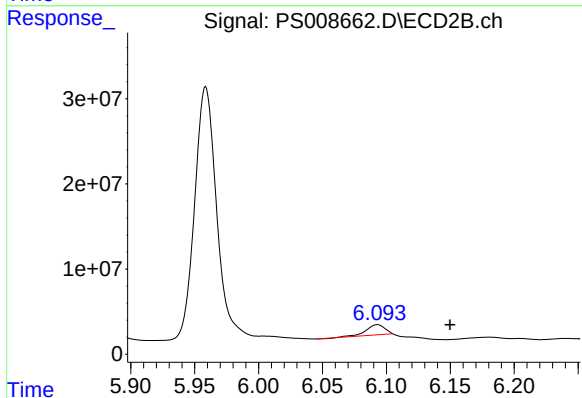


#5 DICAMBA

R.T.: 6.093 min
Delta R.T.: -0.057 min
Response: 12626483
Conc: 3.16 ng/ml

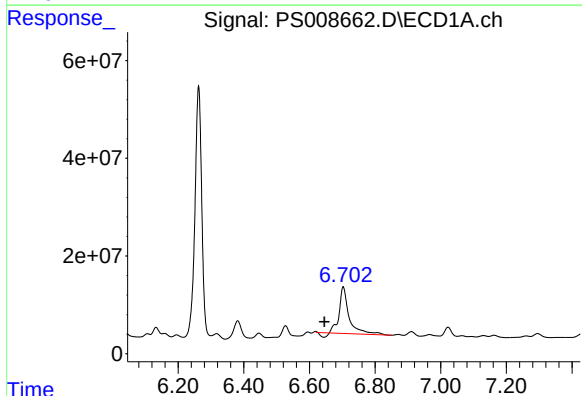


#6 MCP

R.T.: 6.703 min
Delta R.T.: 0.058 min
Response: 195289167
Conc: 38.32 ug/ml

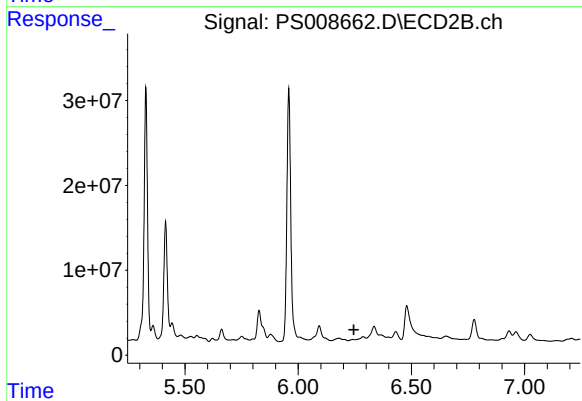

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

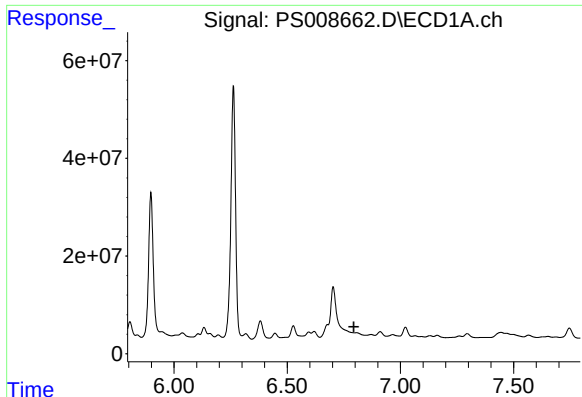

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

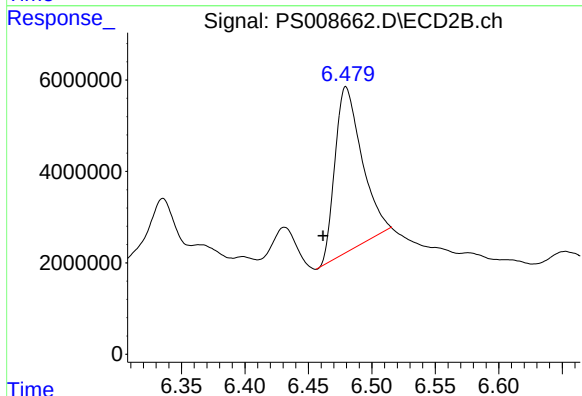


#7 MCPA

R.T.: 6.480 min
Delta R.T.: 0.018 min
Response: 53301579
Conc: 12.48 ug/ml

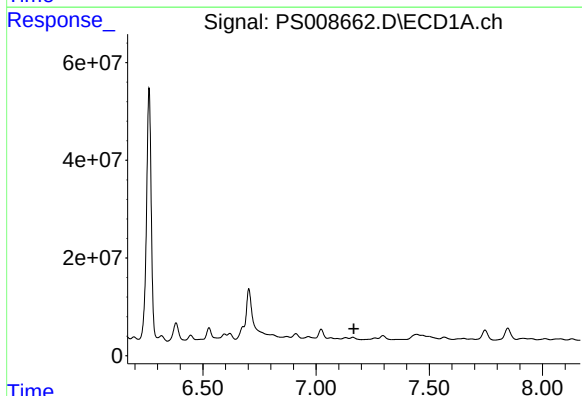


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

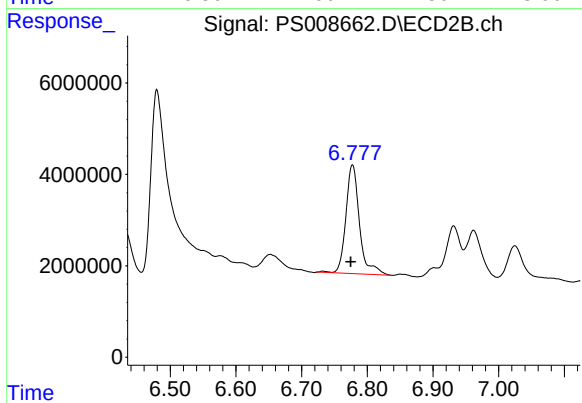

#8 DICHLORPROP


R.T.: 6.777 min
Delta R.T.: 0.003 min
Response: 34160129
Conc: 35.36 ng/ml

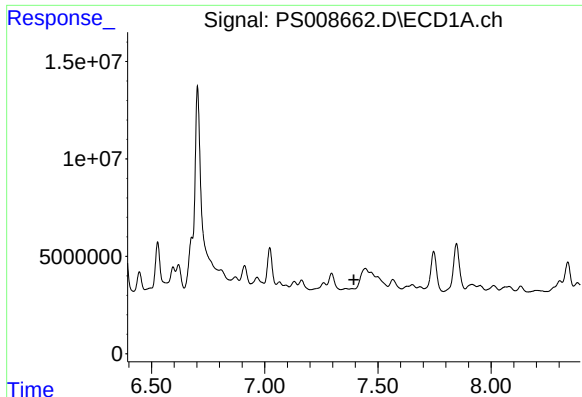

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

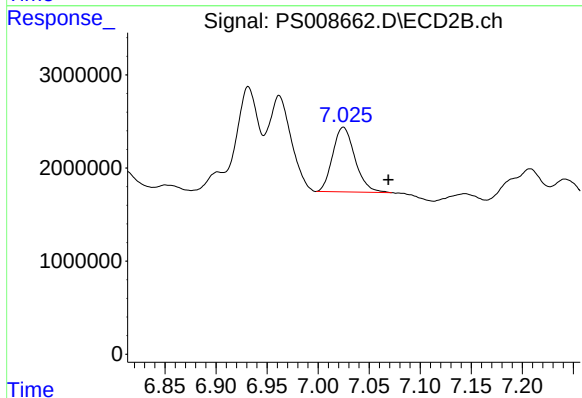


#9 2,4-D

R.T.: 7.025 min
Delta R.T.: -0.044 min
Response: 10541273
Conc: 8.99 ng/ml

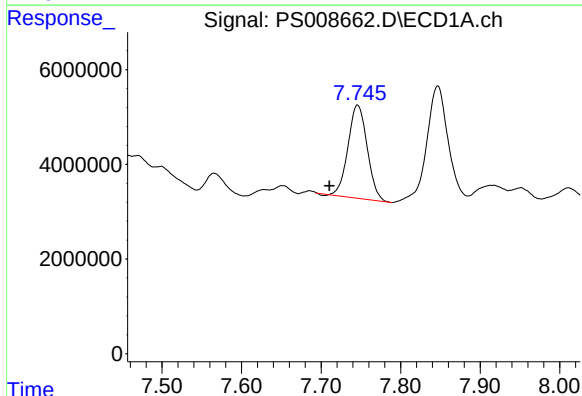


#10 Pentachlorophenol

R.T.: 7.746 min
Delta R.T.: 0.036 min
Response: 33238839
Conc: 1.37 ng/ml

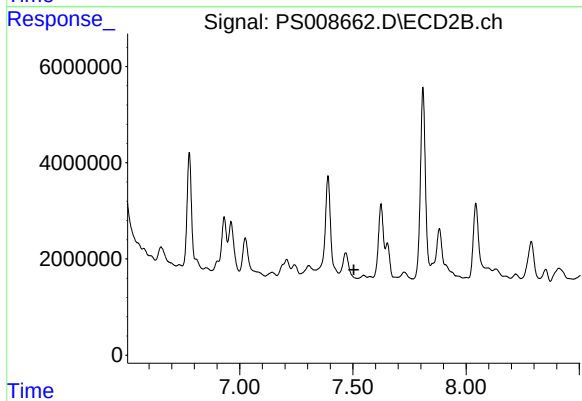

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

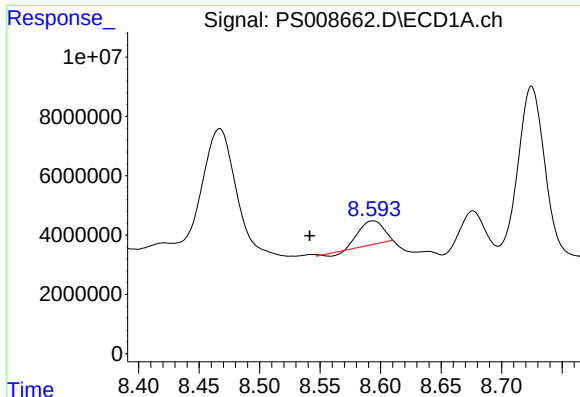

#12 2,4,5-T


R.T.: 8.594 min
Delta R.T.: 0.052 min
Response: 11031133
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

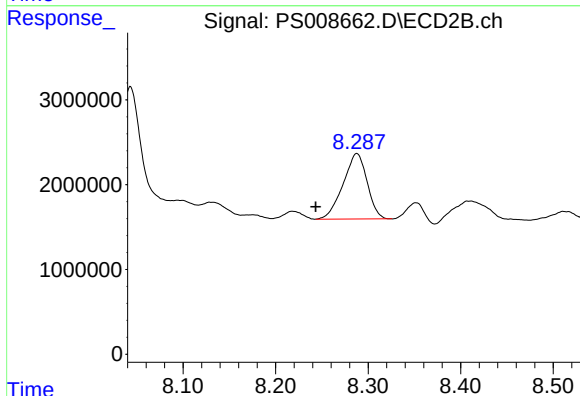


#12 2,4,5-T

R.T.: 8.288 min
Delta R.T.: 0.044 min
Response: 13911921
Conc: 2.63 ng/ml

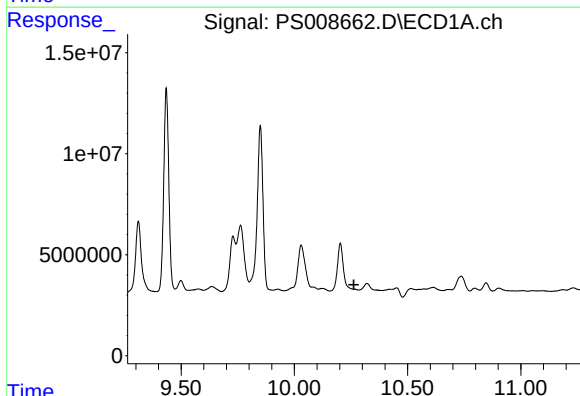


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

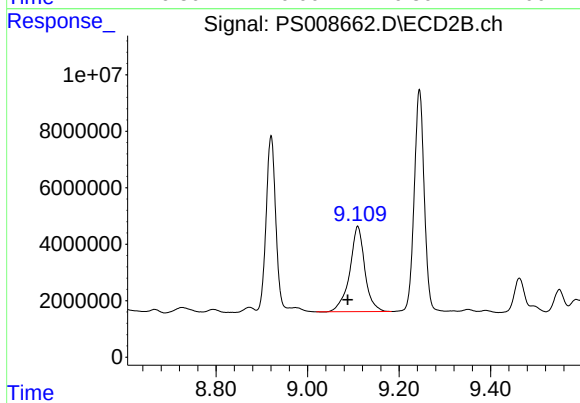

#14 DINOSEB


R.T.: 9.110 min
Delta R.T.: 0.022 min
Response: 69074669
Conc: 18.28 ng/ml

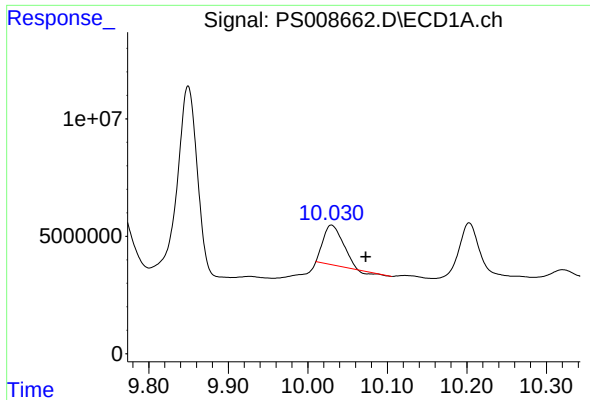

#15 Picloram

R.T.: 10.030 min
Delta R.T.: -0.043 min
Response: 28169571
Conc: 2.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

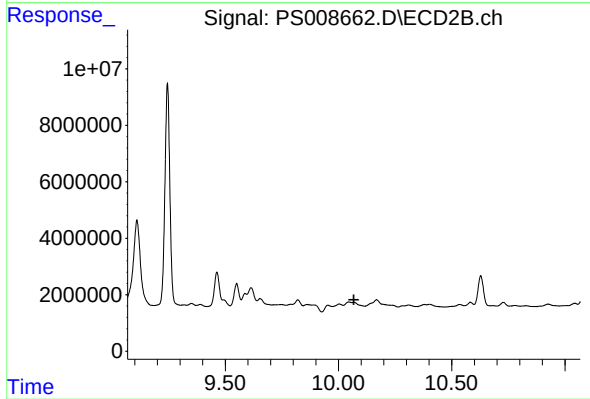

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.