

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 22:50
 Operator : DD\AJ
 Sample : L1333-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1-2-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 02:32:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.262	5.959	668.7E6	342.3E6	378.727	361.236
Target Compounds							
1) T	Dalapon	2.498	2.184	207.6E6	75695308	80.960	59.709 #
2) T	3,5-DICHL...	0.000	5.146	0	133.2E6	N.D.	95.367
3) T	4-Nitroph...	6.133	0.000	19206447	0	19.720	N.D. #
5) T	DICAMBA	0.000	6.093	0	15499782	N.D.	3.876
6) T	MCPD	6.703	0.000	247.8E6	0	48.620	N.D. #
7) T	MCPA	0.000	6.479	0	89939454	N.D.	21.064
8) T	DICHLORPROP	0.000	6.778	0	30928417	N.D.	32.012
9) T	2,4-D	0.000	7.024	0	10193294	N.D.	8.696
10) T	Pentachlo...	7.746	0.000	33121568	0	1.362	N.D. #
12) T	2,4,5-T	8.594	8.286	12782188	15269588	1.385	2.888 #
14) T	DINOSEB	0.000	9.109	0	66139641	N.D.	17.508
15) T	Picloram	10.031	0.000	27080935	0	2.170	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 22:50
Operator : DD\AJ
Sample : L1333-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 02:32:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

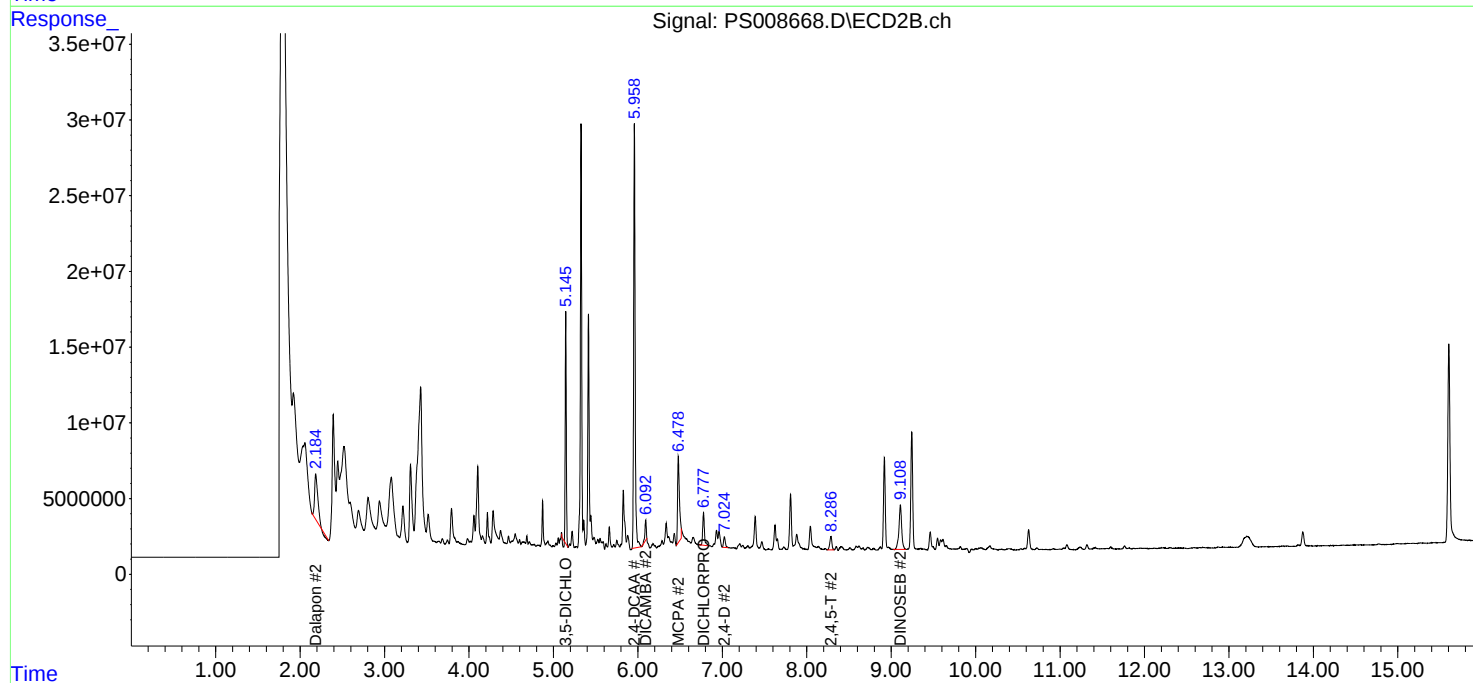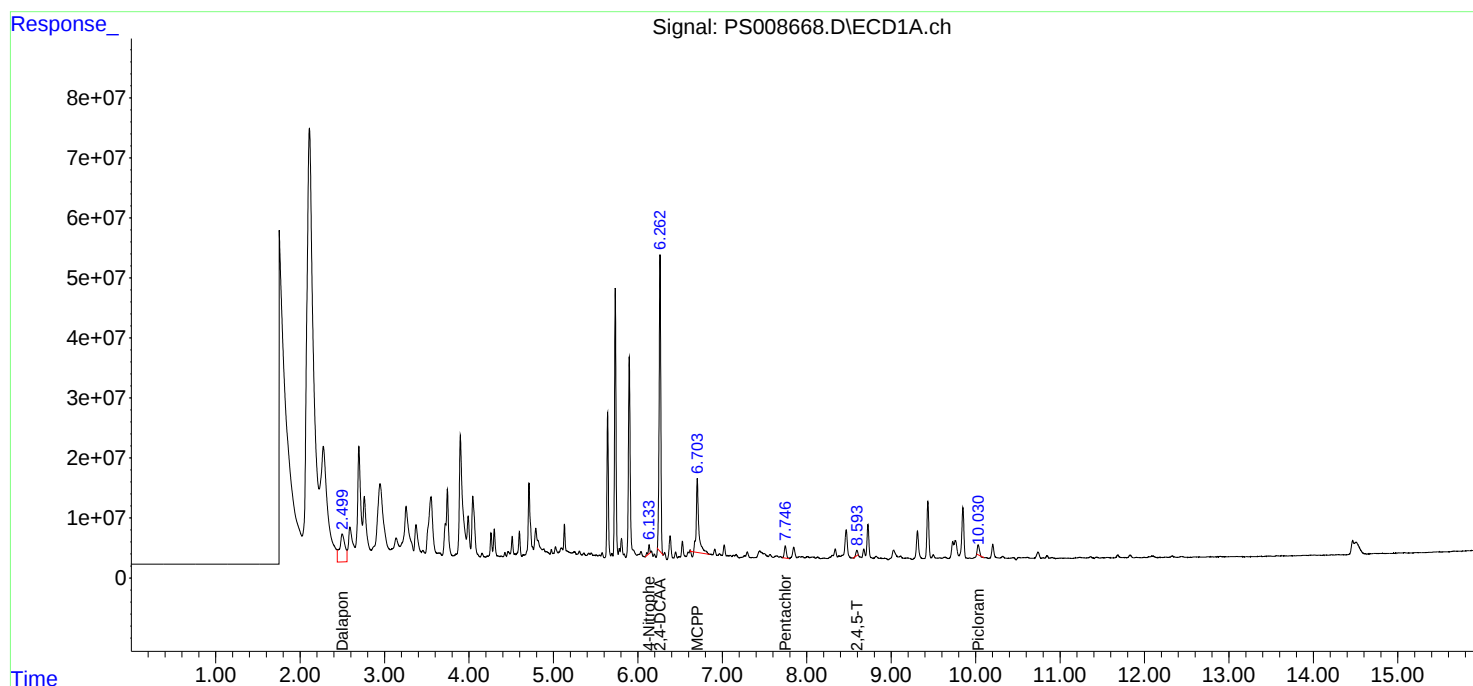


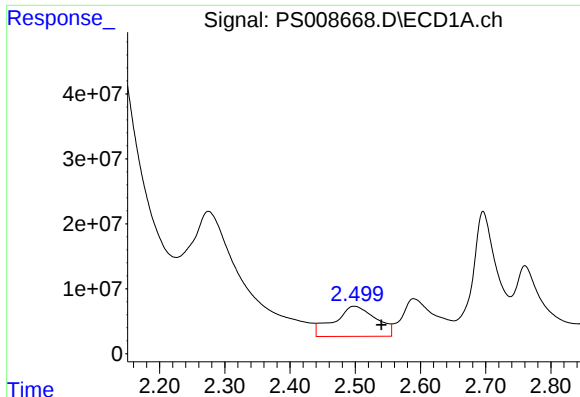

#1 Dalapon


R.T.: 2.498 min
Delta R.T.: -0.042 min
Response: 207568317
Conc: 80.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

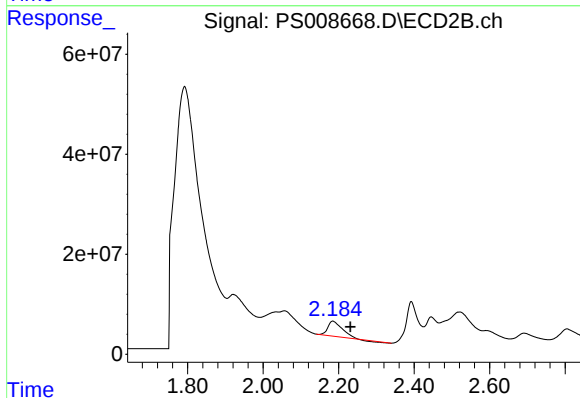


#1 Dalapon

R.T.: 2.184 min
Delta R.T.: -0.047 min
Response: 75695308
Conc: 59.71 ng/ml

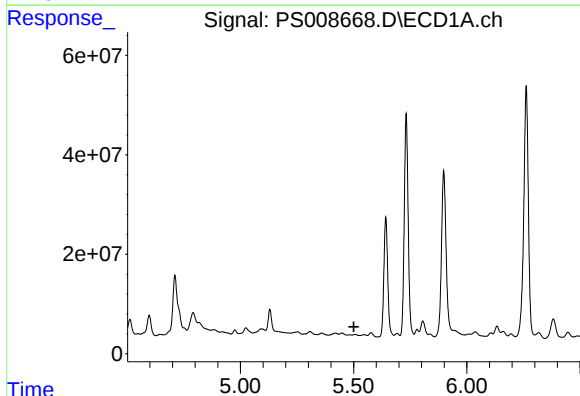


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

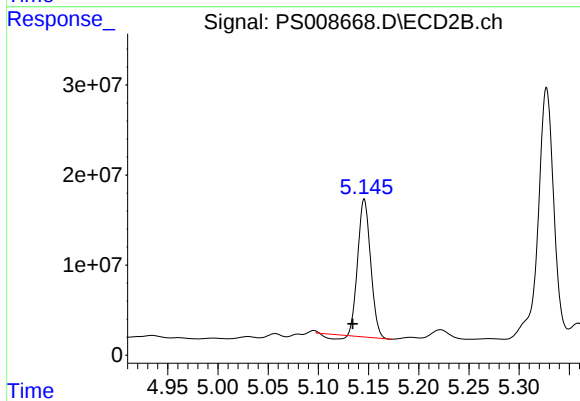

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 133244552
Conc: 95.37 ng/ml

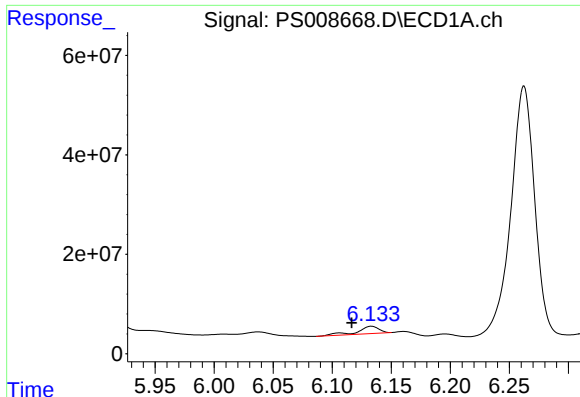

#3 4-Nitrophenol


R.T.: 6.133 min
Delta R.T.: 0.016 min
Response: 19206447
Conc: 19.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

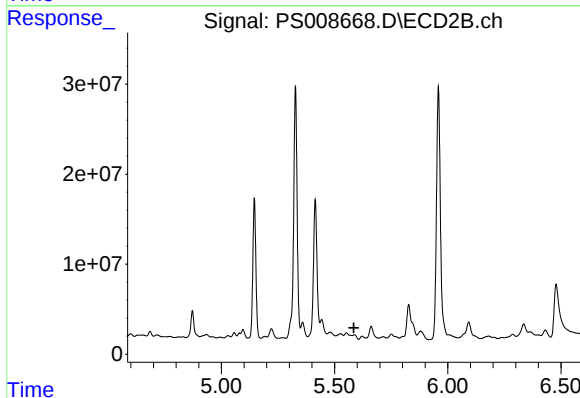


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

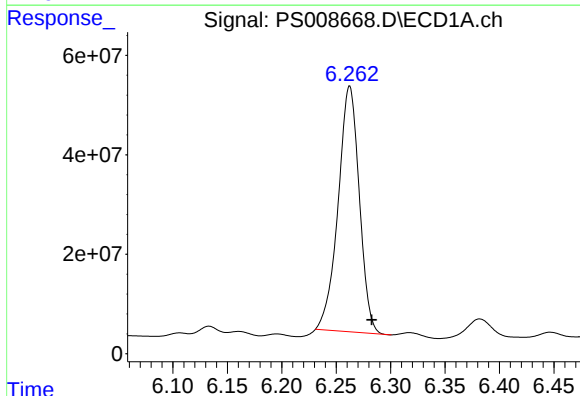


#4 2,4-DCAA

R.T.: 6.262 min
Delta R.T.: -0.020 min
Response: 668719549
Conc: 378.73 ng/ml

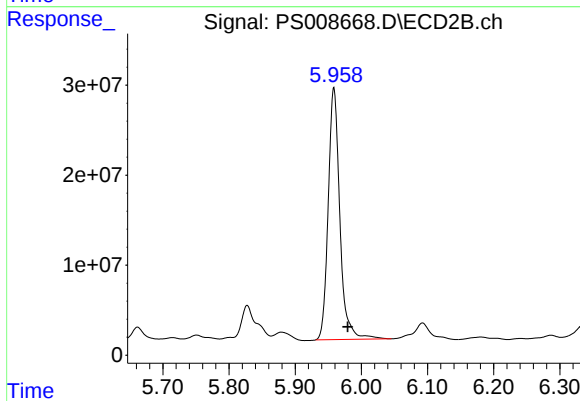

#4 2,4-DCAA


R.T.: 5.959 min
Delta R.T.: -0.021 min
Response: 342257675
Conc: 361.24 ng/ml

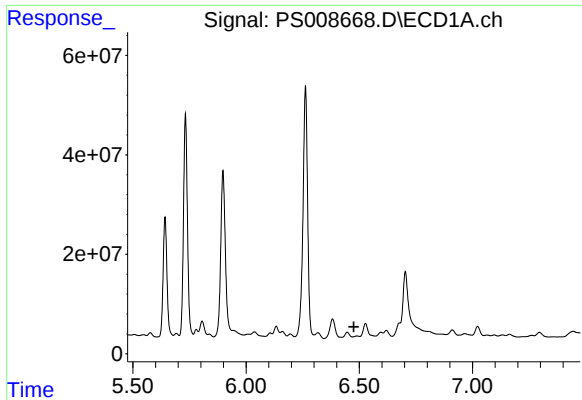

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

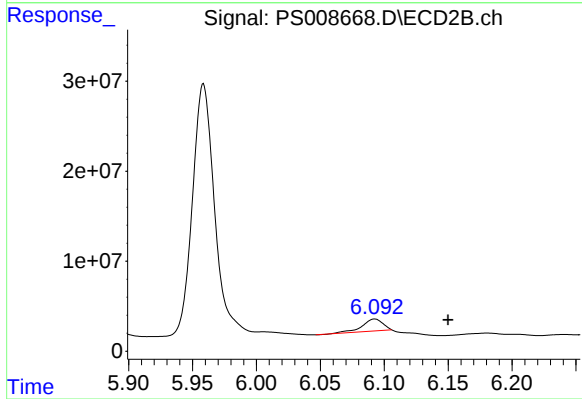


#5 DICAMBA

R.T.: 6.093 min
Delta R.T.: -0.057 min
Response: 15499782
Conc: 3.88 ng/ml

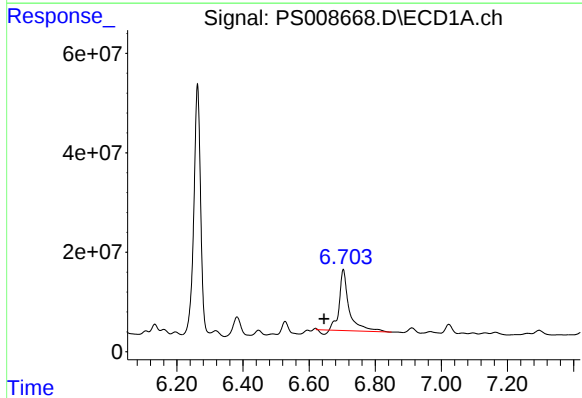


#6 MCP

R.T.: 6.703 min
Delta R.T.: 0.058 min
Response: 247810300
Conc: 48.62 ug/ml

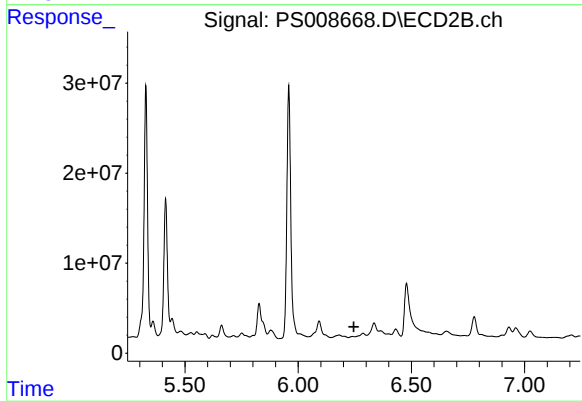

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

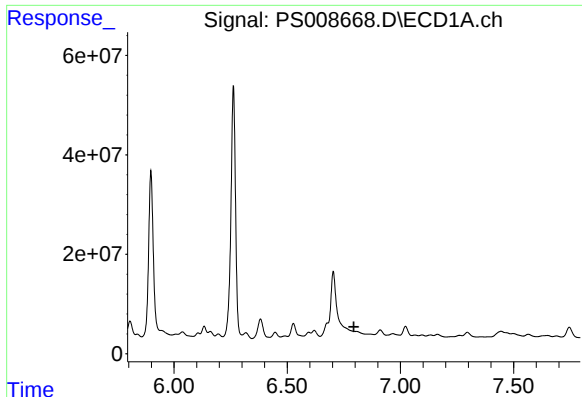

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

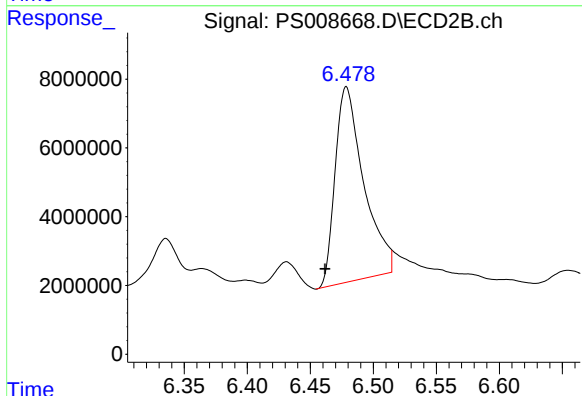


#7 MCPA

R.T.: 6.479 min
Delta R.T.: 0.017 min
Response: 89939454
Conc: 21.06 ug/ml

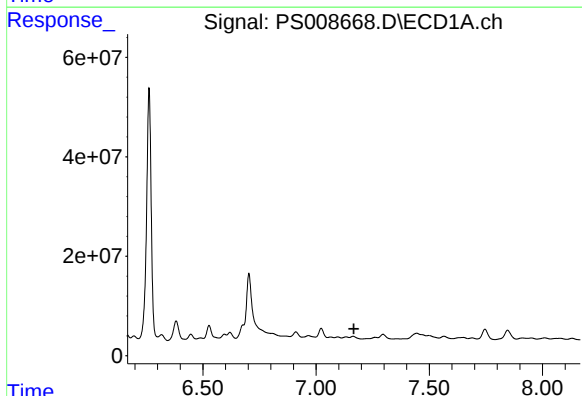


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

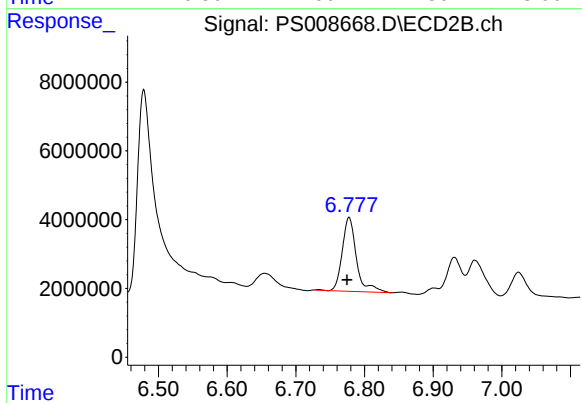

#8 DICHLORPROP


R.T.: 6.778 min
Delta R.T.: 0.003 min
Response: 30928417
Conc: 32.01 ng/ml

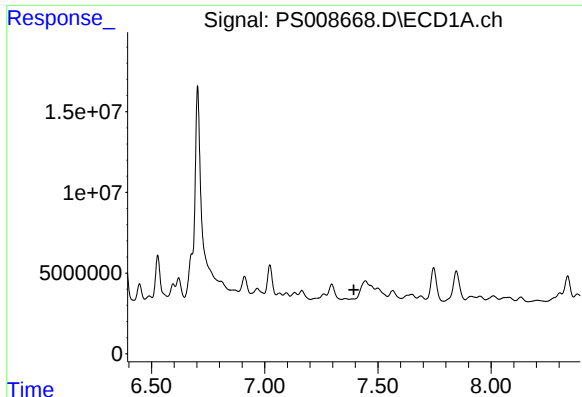

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

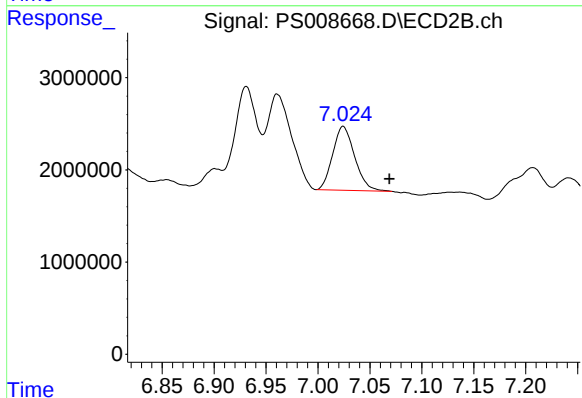


#9 2,4-D

R.T.: 7.024 min
Delta R.T.: -0.044 min
Response: 10193294
Conc: 8.70 ng/ml

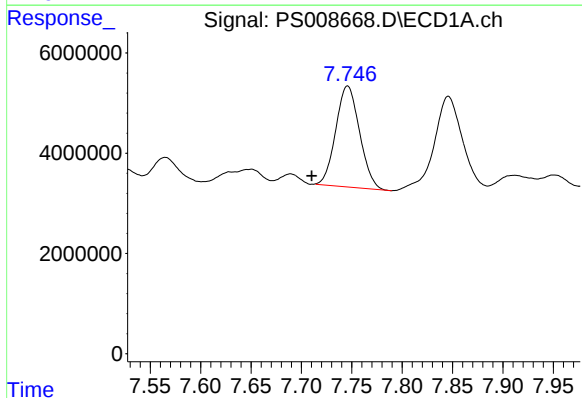


#10 Pentachlorophenol

R.T.: 7.746 min
Delta R.T.: 0.036 min
Response: 33121568
Conc: 1.36 ng/ml

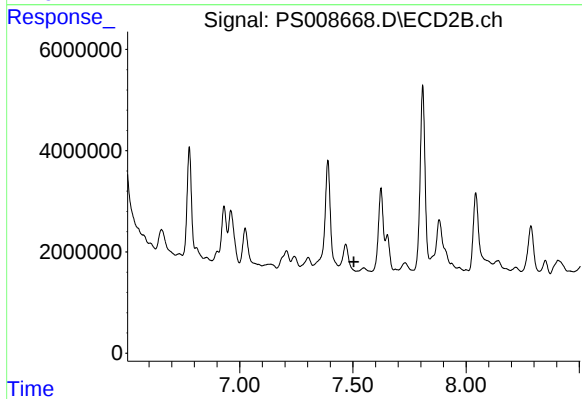

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

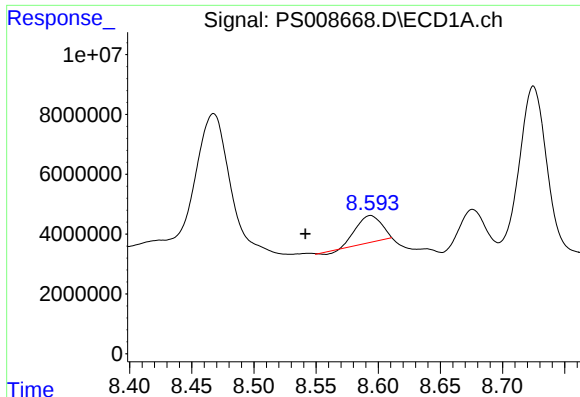

#12 2,4,5-T


R.T.: 8.594 min
Delta R.T.: 0.052 min
Response: 12782188
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

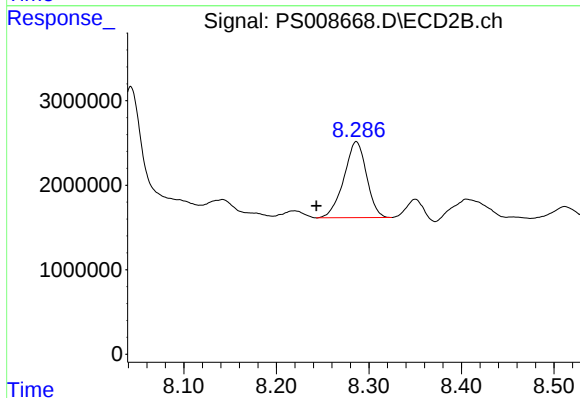


#12 2,4,5-T

R.T.: 8.286 min
Delta R.T.: 0.043 min
Response: 15269588
Conc: 2.89 ng/ml

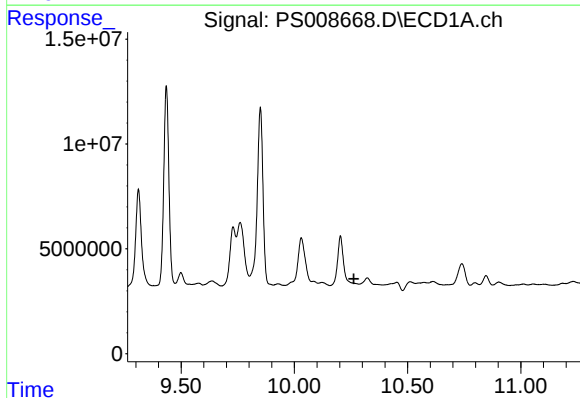


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

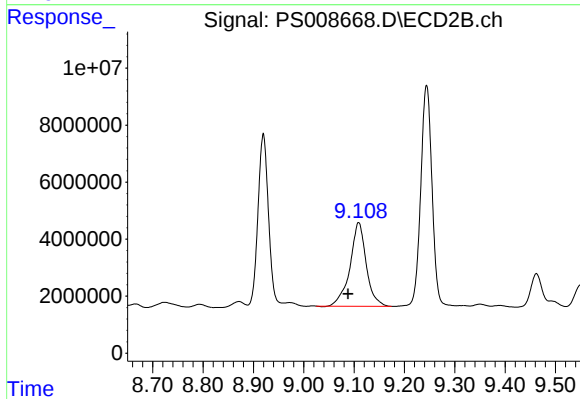

#14 DINOSEB


R.T.: 9.109 min
Delta R.T.: 0.021 min
Response: 66139641
Conc: 17.51 ng/ml

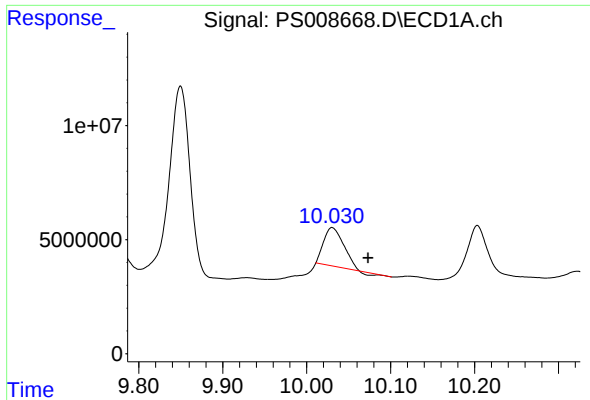

#15 Picloram

R.T.: 10.031 min
Delta R.T.: -0.043 min
Response: 27080935
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1-2-COMP

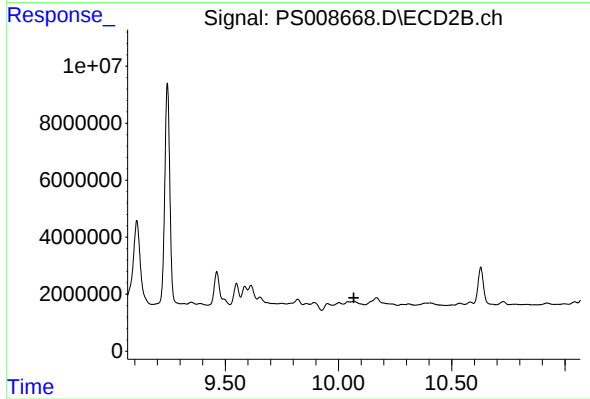

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.