

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 02:28
 Operator : DD\AJ
 Sample : L1310-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CTY-SB-0102-0-80

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:47:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.958	555.5E6	279.1E6	314.607	294.558
Target Compounds							
1) T	Dalapon	2.496	2.180	46075008	-10088463	17.971	N.D. #
2) T	3,5-DICHL...	0.000	5.146	0	35710447	N.D.	25.559
3) T	4-Nitroph...	6.163	5.590	24547664	11851151	25.204	19.960
6) T	MCP	6.700	0.000	15940310	0	3.127	N.D. #
7) T	MCPA	6.811	6.422	57628593	28811235	7.886	6.748
8) T	DICHLORPROP	0.000	6.778	0	24460243	N.D.	25.317
9) T	2,4-D	0.000	7.025	0	12964083	N.D.	11.059
10) T	Pentachlo...	7.747	0.000	38957789	0	1.602	N.D. #
12) T	2,4,5-T	0.000	8.210	0	12262894	N.D.	2.319
13) T	2,4-DB	9.118	8.747	16491397	18367564	11.896	25.947 #
14) T	DINOSEB	0.000	9.077	0	10051234	N.D.	2.661
15) T	Picloram	0.000	10.071	0	31819686	N.D.	4.283
16) T	DCPA	10.519	10.071	9471991	31819686	<MDL	4.883 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 02:28
Operator : DD\AJ
Sample : L1310-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:47:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

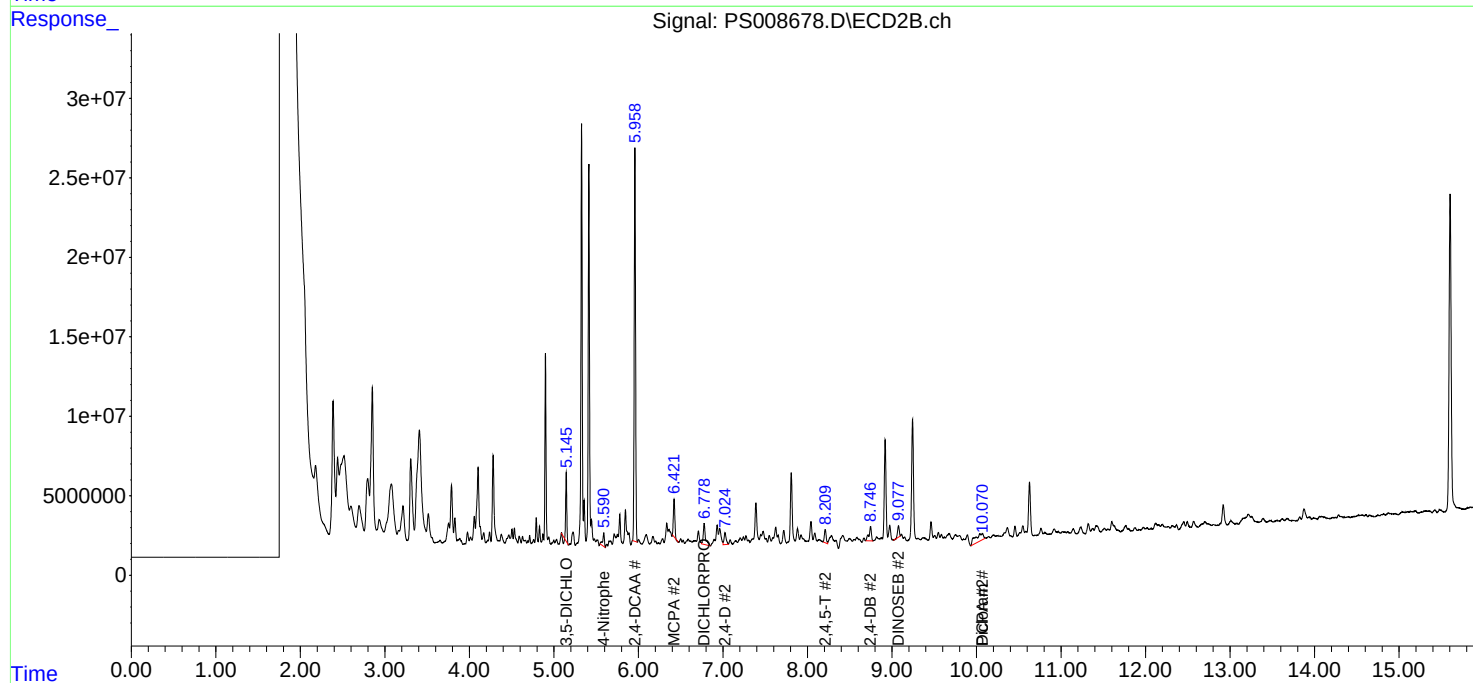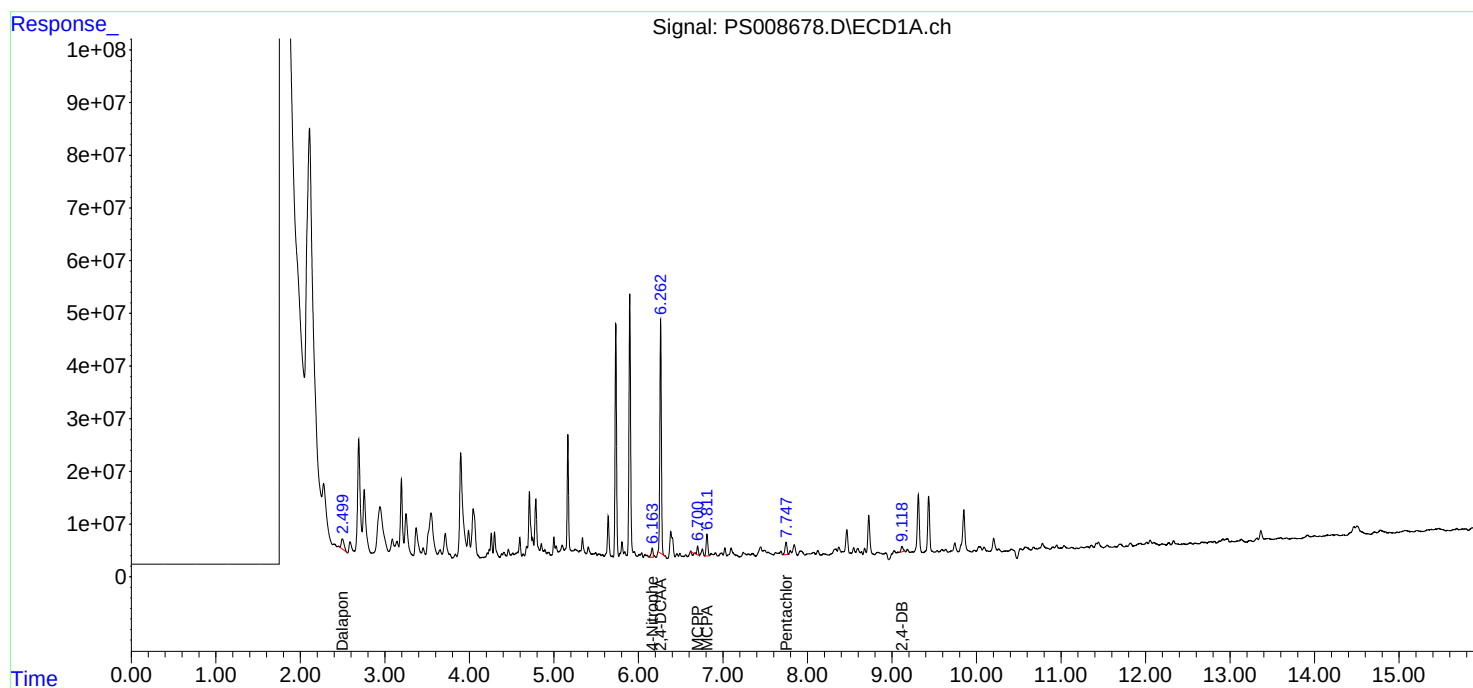


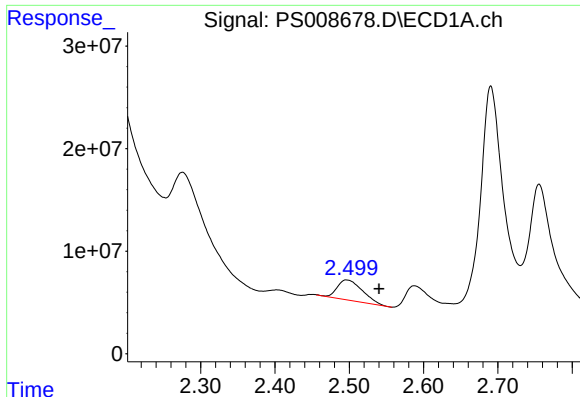

#1 Dalapon


R.T.: 2.496 min
Delta R.T.: -0.044 min
Response: 46075008
Conc: 17.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

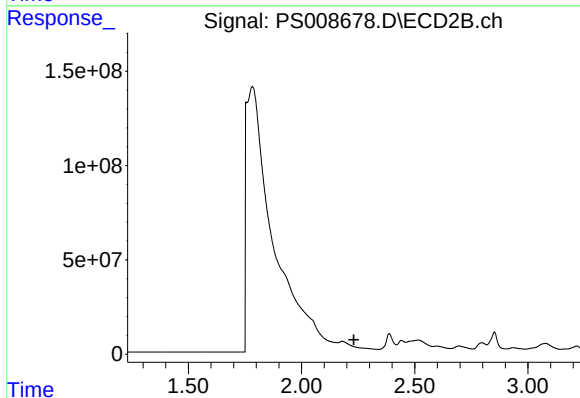


#1 Dalapon

R.T.: 2.180 min
Delta R.T.: -0.051 min
Response: -10088463
Conc: N.D.

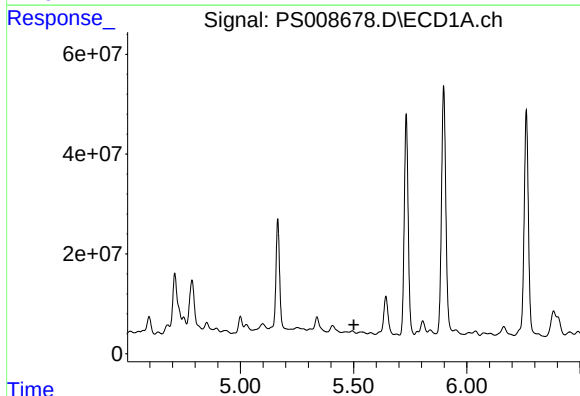


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

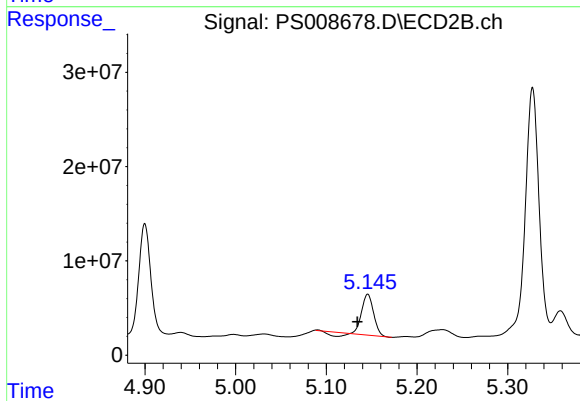

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 35710447
Conc: 25.56 ng/ml

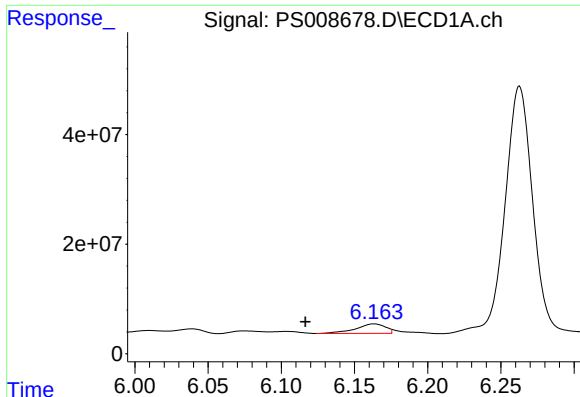

#3 4-Nitrophenol


R.T.: 6.163 min
Delta R.T.: 0.047 min
Response: 24547664
Conc: 25.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

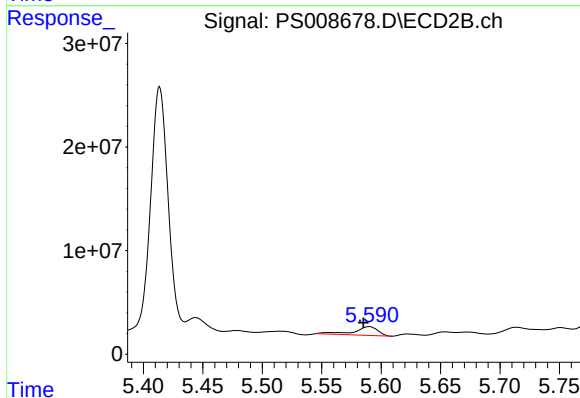


#3 4-Nitrophenol

R.T.: 5.590 min
Delta R.T.: 0.005 min
Response: 11851151
Conc: 19.96 ng/ml

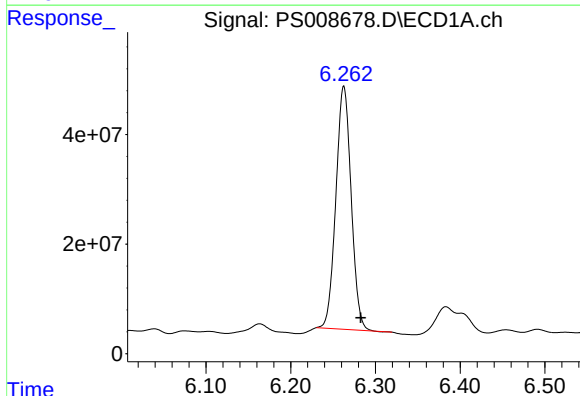


#4 2,4-DCAA

R.T.: 6.263 min
Delta R.T.: -0.020 min
Response: 555502027
Conc: 314.61 ng/ml

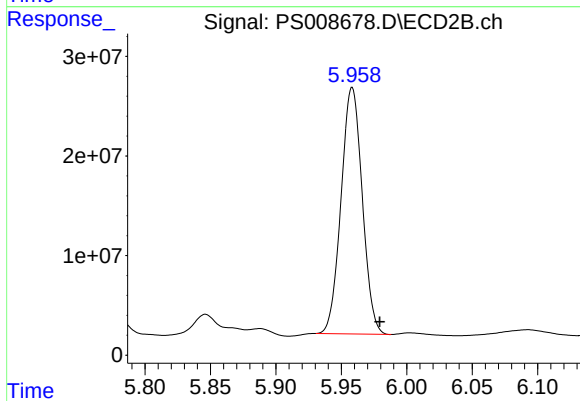

#4 2,4-DCAA


R.T.: 5.958 min
Delta R.T.: -0.021 min
Response: 279083097
Conc: 294.56 ng/ml

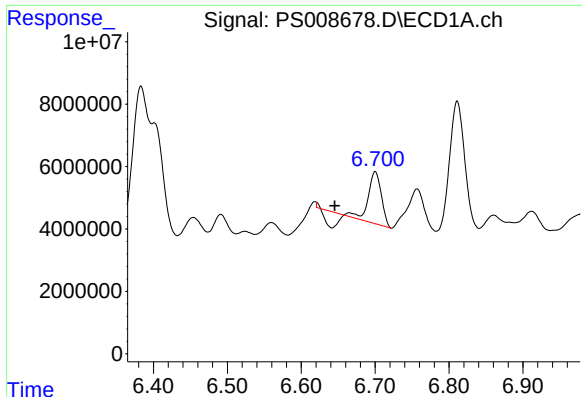

#6 MCPP


R.T.: 6.700 min
Delta R.T.: 0.055 min
Response: 15940310
Conc: 3.13 ug/ml

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

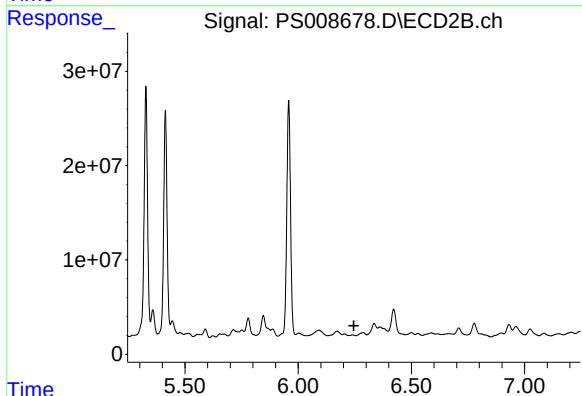


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

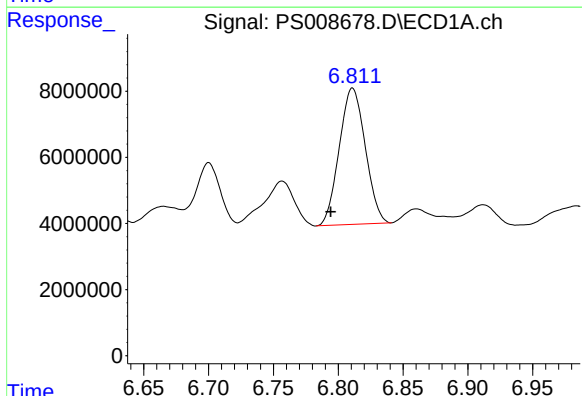


#7 MCPA

R.T.: 6.811 min
Delta R.T.: 0.017 min
Response: 57628593
Conc: 7.89 ug/ml

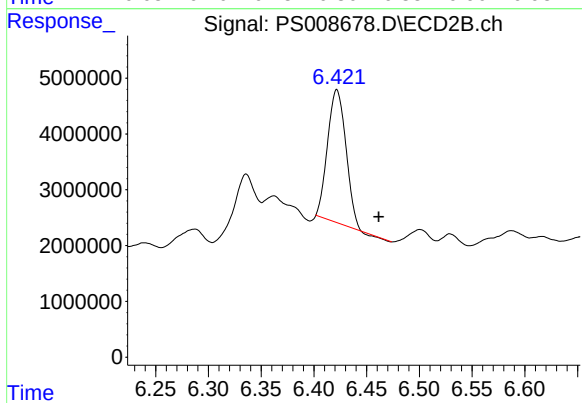

#7 MCPA


R.T.: 6.422 min
Delta R.T.: -0.040 min
Response: 28811235
Conc: 6.75 ug/ml

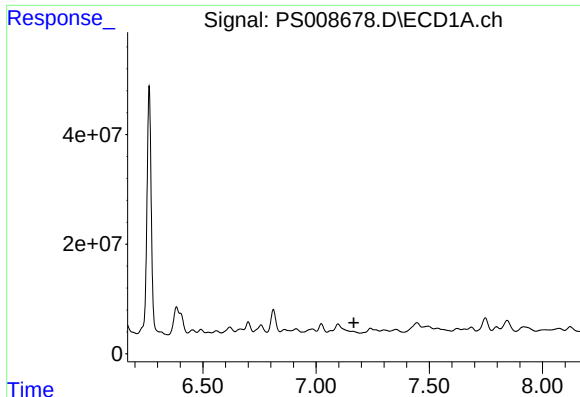

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

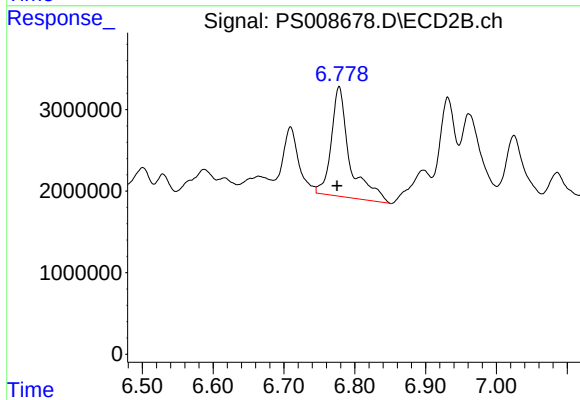


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.003 min
Response: 24460243
Conc: 25.32 ng/ml

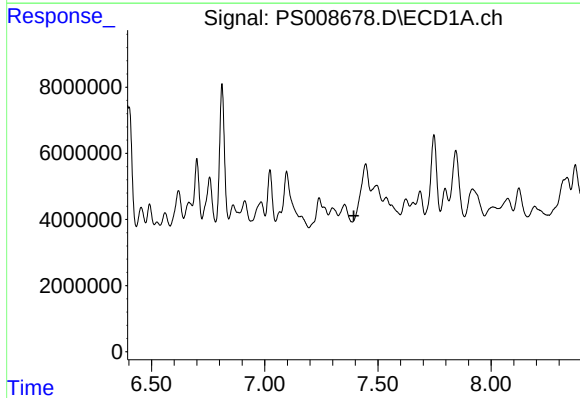


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

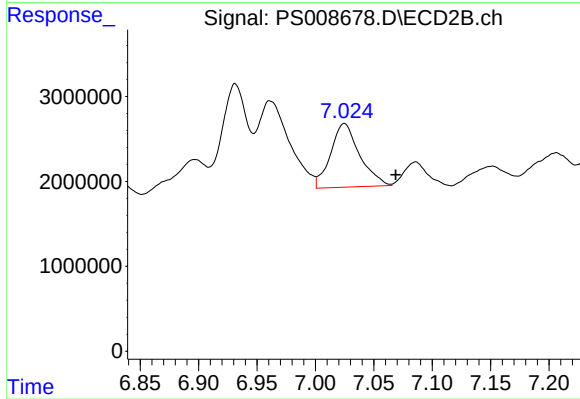

#9 2,4-D


R.T.: 7.025 min
Delta R.T.: -0.044 min
Response: 12964083
Conc: 11.06 ng/ml

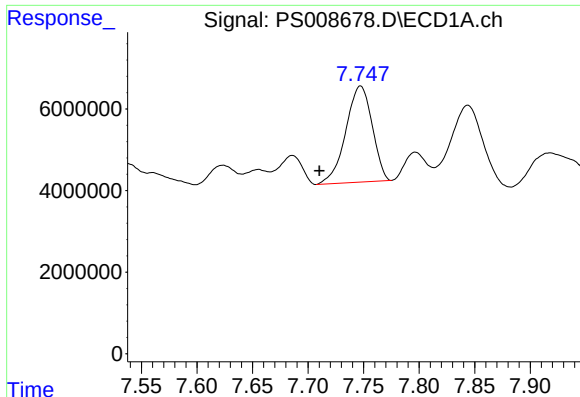

#10 Pentachlorophenol


R.T.: 7.747 min
Delta R.T.: 0.037 min
Response: 38957789
Conc: 1.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

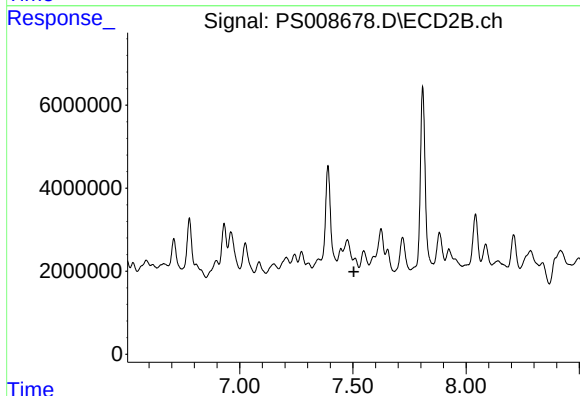


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

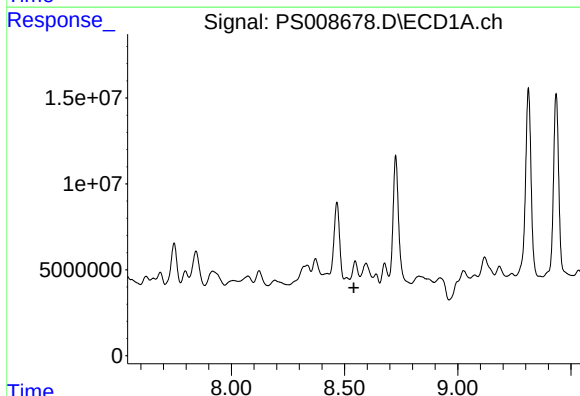


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

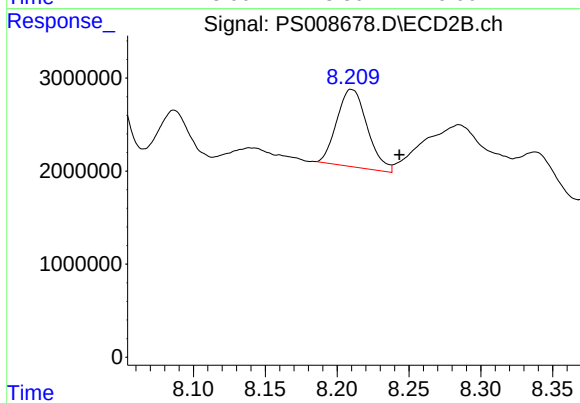

#12 2,4,5-T


R.T.: 8.210 min
Delta R.T.: -0.033 min
Response: 12262894
Conc: 2.32 ng/ml

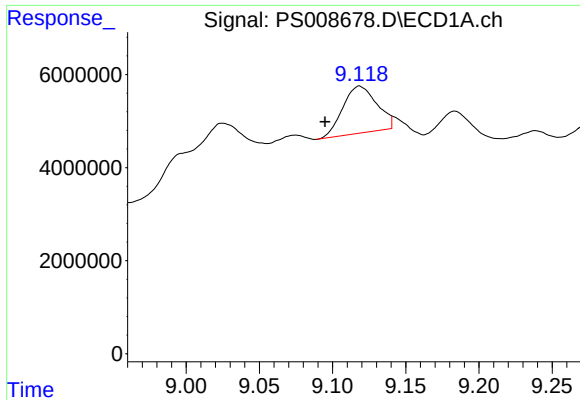

#13 2,4-DB


R.T.: 9.118 min
Delta R.T.: 0.024 min
Response: 16491397
Conc: 11.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

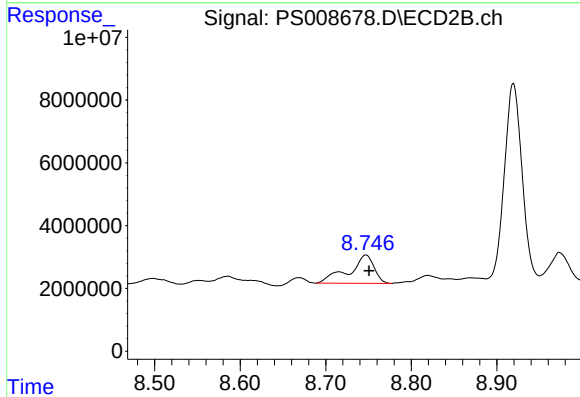


#13 2,4-DB

R.T.: 8.747 min
Delta R.T.: -0.004 min
Response: 18367564
Conc: 25.95 ng/ml

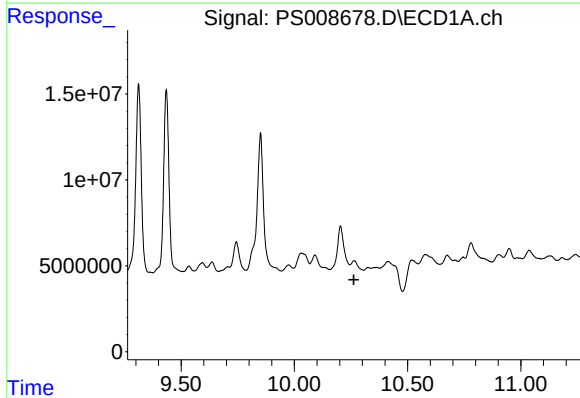


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

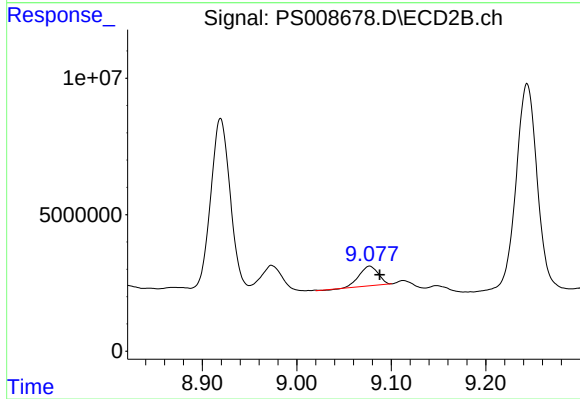

#14 DINOSEB


R.T.: 9.077 min
Delta R.T.: -0.011 min
Response: 10051234
Conc: 2.66 ng/ml

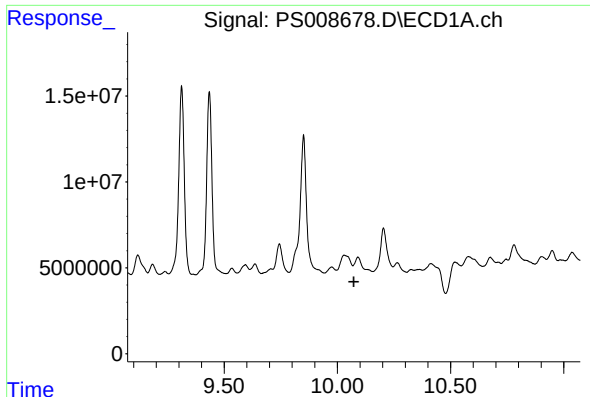

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CTY-SB-0102-0-80

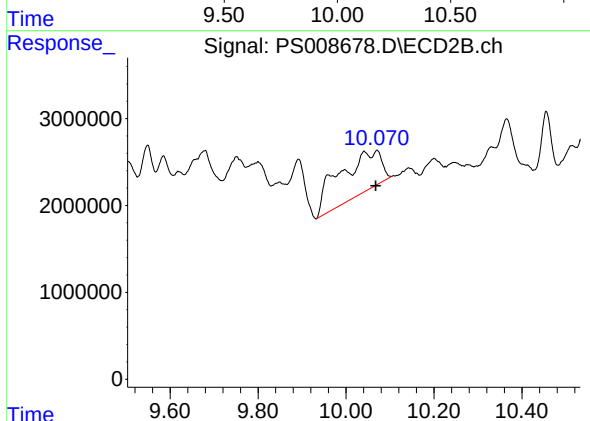


#15 Picloram

R.T.: 10.071 min
Delta R.T.: 0.003 min
Response: 31819686
Conc: 4.28 ng/ml

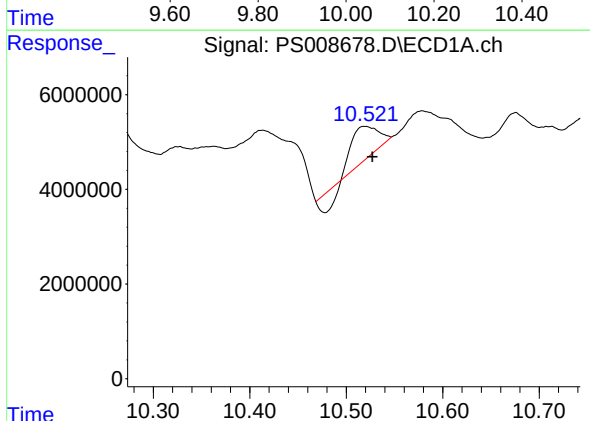

#16 DCPA

R.T.: 10.519 min
Delta R.T.: -0.008 min
Response: 9471991
Conc: N.D.

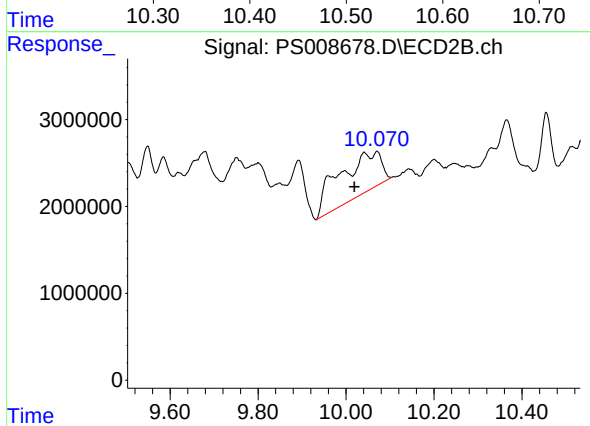

#16 DCPA

R.T.: 10.071 min
Delta R.T.: 0.052 min
Response: 31819686
Conc: 4.88 ng/ml