

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 03:33
 Operator : DD\AJ
 Sample : L1313-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 124018-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:48:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.958	560.4E6	276.6E6	317.396	291.969
Target Compounds							
1) T	Dalapon	2.497	2.180	46667538	-10139187	18.202	N.D. #
2) T	3,5-DICHL...	0.000	5.145	0	73280545	N.D.	52.449
5) T	DICAMBA	0.000	6.092	0	7752621	N.D.	1.939
6) T	MCP	6.703	0.000	19279867	0	3.783	N.D. #
7) T	MCPA	6.812	6.420	55708613	26915582	7.624	6.304
8) T	DICHLORPROP	0.000	6.777	0	25819611	N.D.	26.724
9) T	2,4-D	0.000	7.024	0	12076423	N.D.	10.302
10) T	Pentachlo...	7.747	7.476	36778824	12550694	1.513	<MDL #
14) T	DINOSEB	0.000	9.076	0	16278129	N.D.	4.309
15) T	Picloram	0.000	10.041	0	14287280	N.D.	1.923
16) T	DCPA	10.521	10.041	4297580	14287280	<MDL	2.192 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 03:33
Operator : DD\AJ
Sample : L1313-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
124018-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:48:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

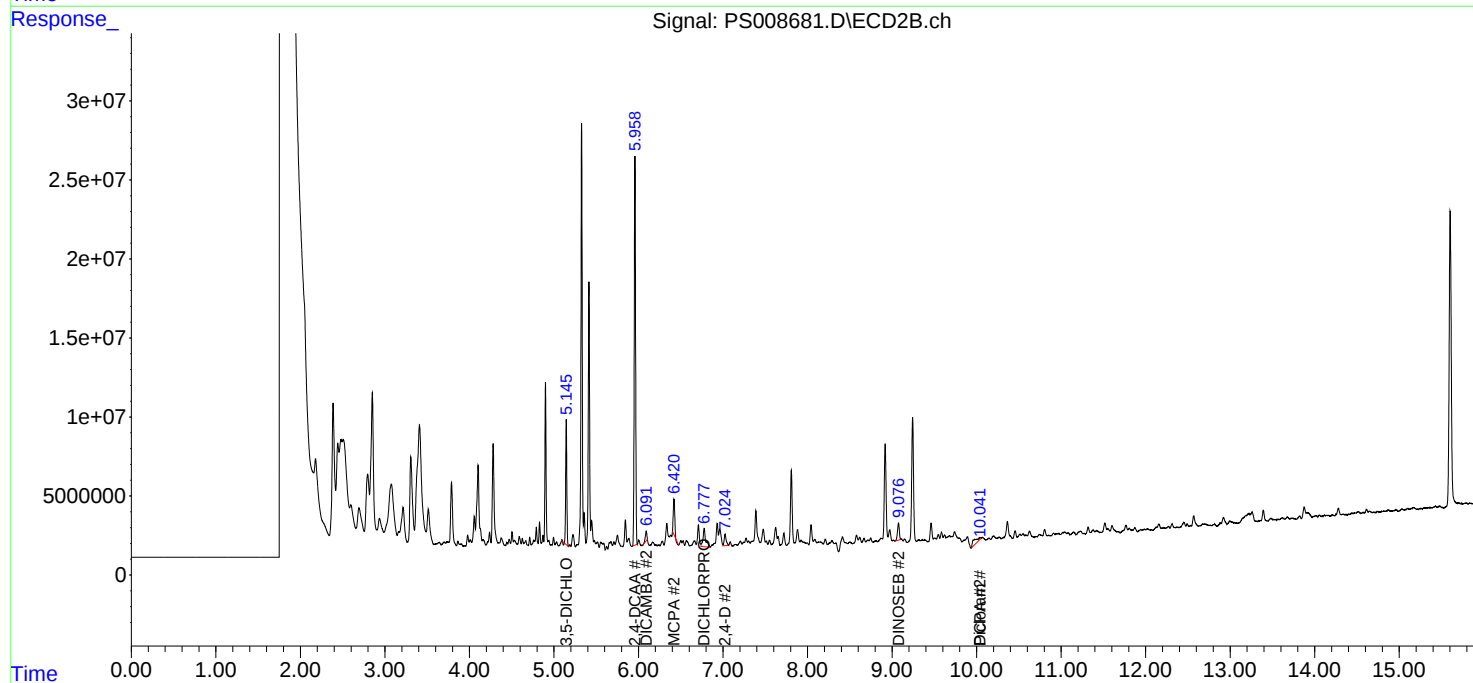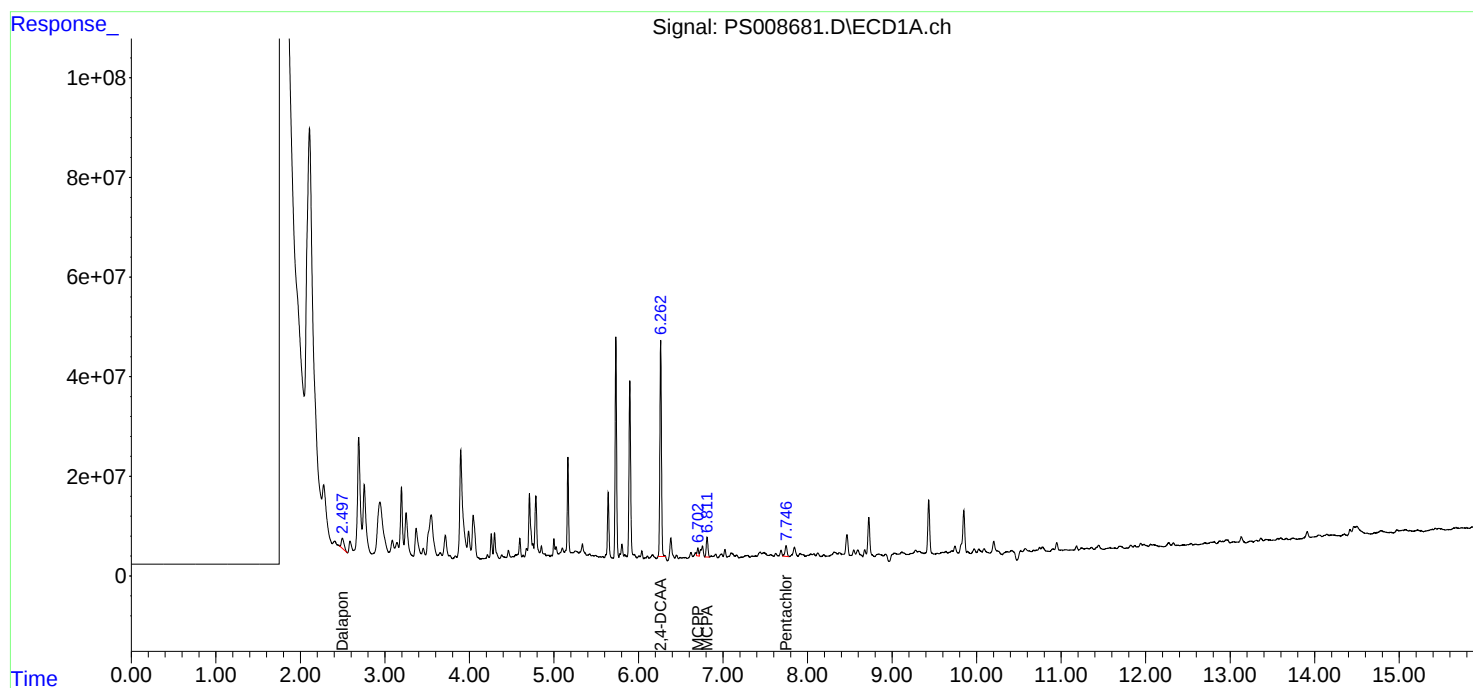


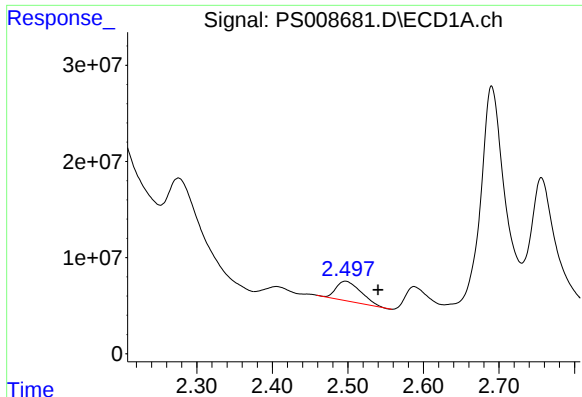

#1 Dalapon


R.T.: 2.497 min
Delta R.T.: -0.043 min
Response: 46667538
Conc: 18.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
124018-A

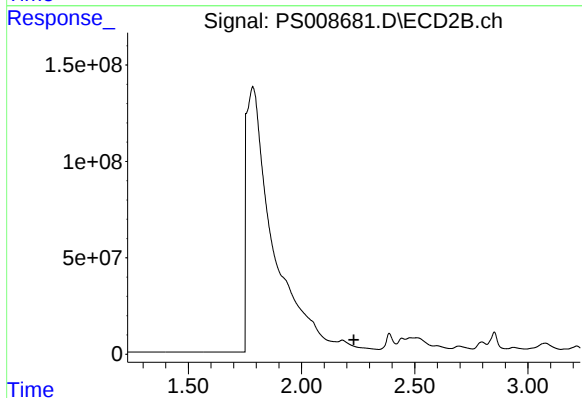


#1 Dalapon

R.T.: 2.180 min
Delta R.T.: -0.051 min
Response: -10139187
Conc: N.D.

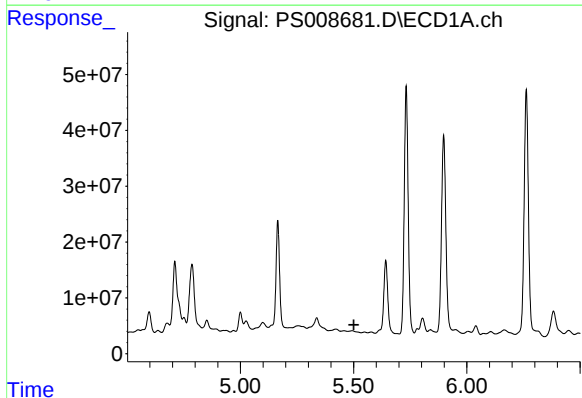


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

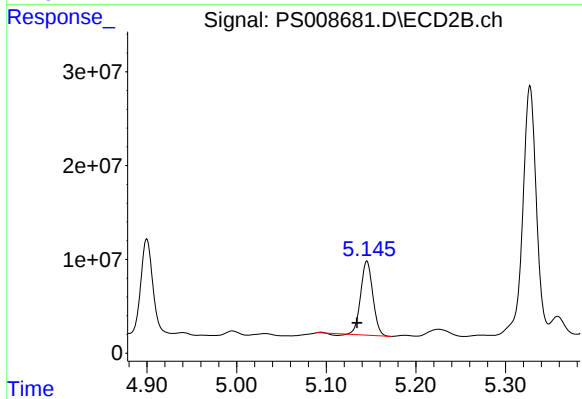

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.145 min
Delta R.T.: 0.011 min
Response: 73280545
Conc: 52.45 ng/ml

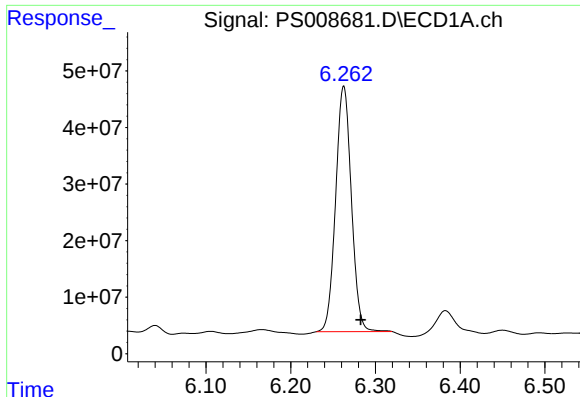

#4 2,4-DCAA


R.T.: 6.263 min
Delta R.T.: -0.020 min
Response: 560427798
Conc: 317.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
124018-A

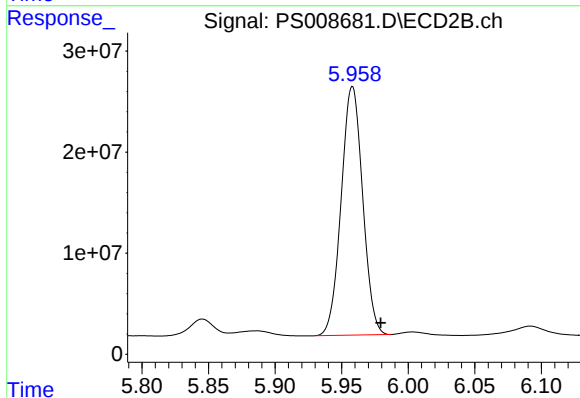


#4 2,4-DCAA

R.T.: 5.958 min
Delta R.T.: -0.021 min
Response: 276629820
Conc: 291.97 ng/ml

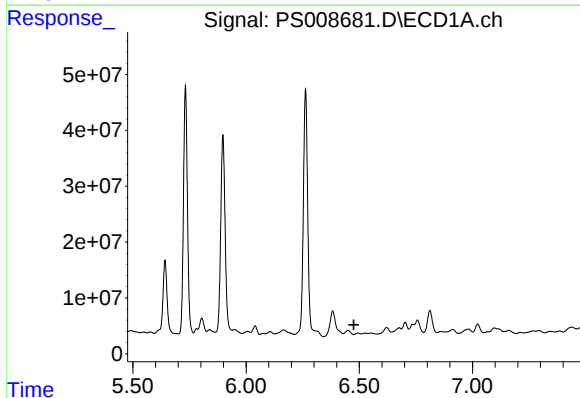


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

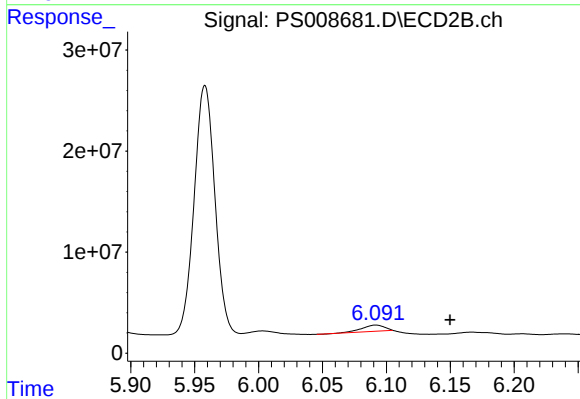

#5 DICAMBA


R.T.: 6.092 min
Delta R.T.: -0.058 min
Response: 7752621
Conc: 1.94 ng/ml

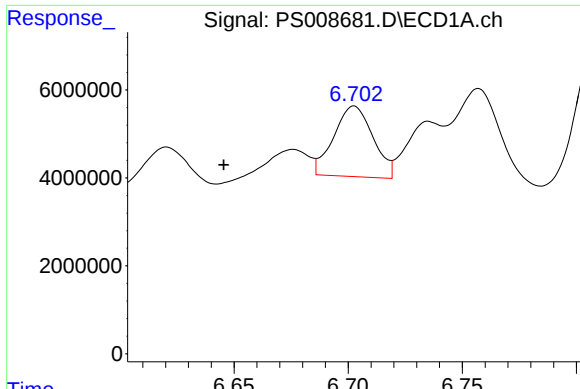

#6 MCP


R.T.: 6.703 min
Delta R.T.: 0.057 min
Response: 19279867
Conc: 3.78 ug/ml

Instrument :
ECD_S
ClientSampleId :
124018-A

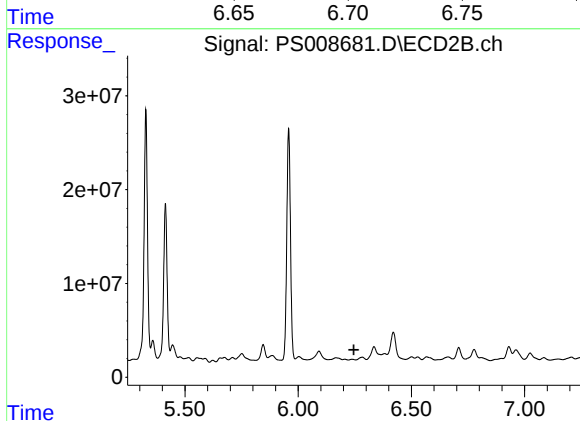


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

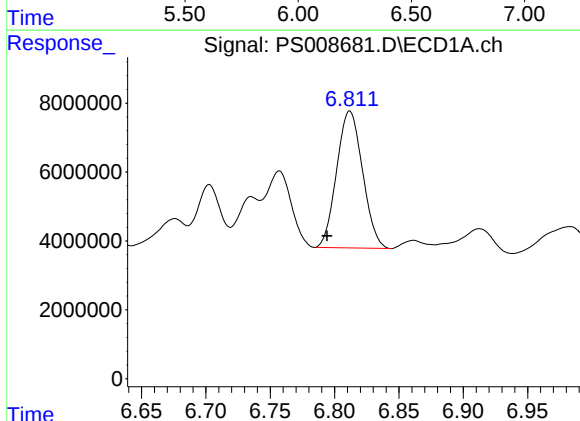


#7 MCP

R.T.: 6.812 min
Delta R.T.: 0.018 min
Response: 55708613
Conc: 7.62 ug/ml

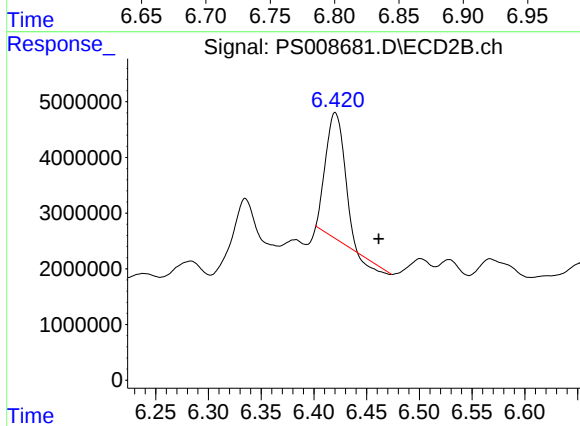

#7 MCP


R.T.: 6.420 min
Delta R.T.: -0.041 min
Response: 26915582
Conc: 6.30 ug/ml

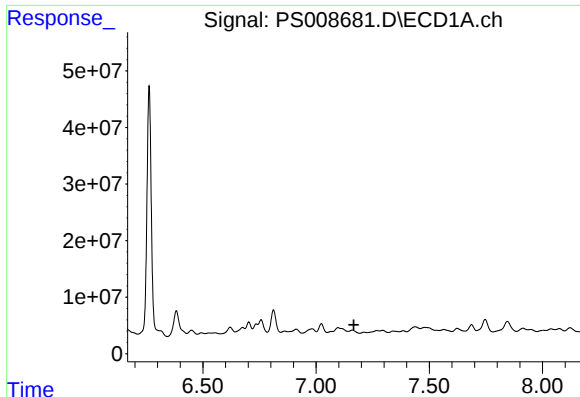

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
124018-A

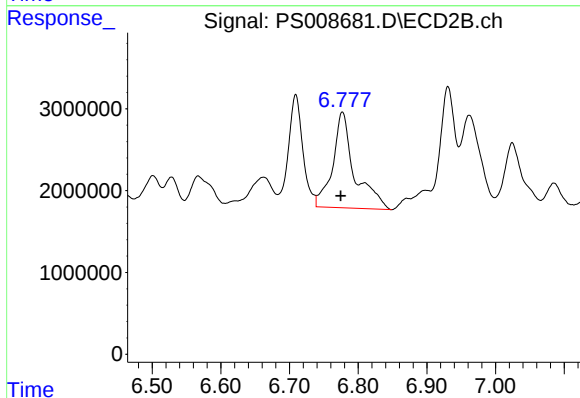


#8 DICHLORPROP

R.T.: 6.777 min
Delta R.T.: 0.002 min
Response: 25819611
Conc: 26.72 ng/ml

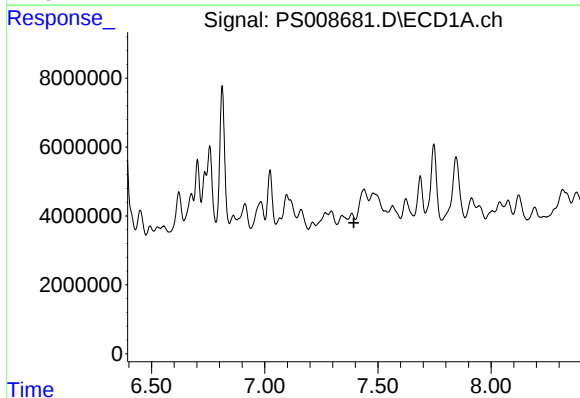


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

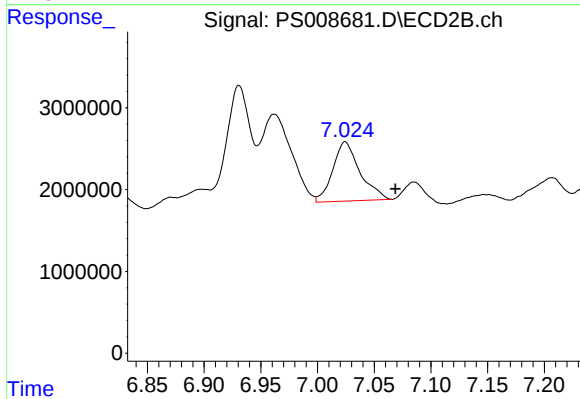

#9 2,4-D


R.T.: 7.024 min
Delta R.T.: -0.044 min
Response: 12076423
Conc: 10.30 ng/ml

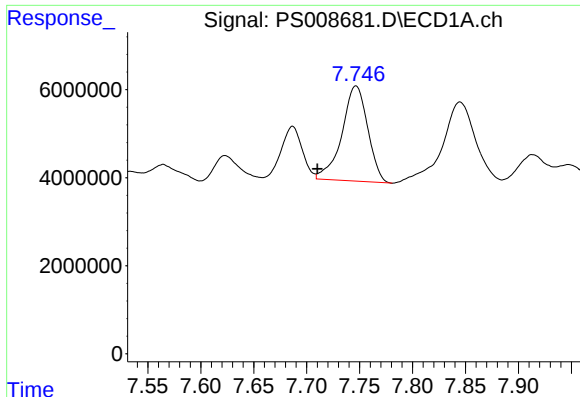

#10 Pentachlorophenol


R.T.: 7.747 min
Delta R.T.: 0.036 min
Response: 36778824
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
124018-A

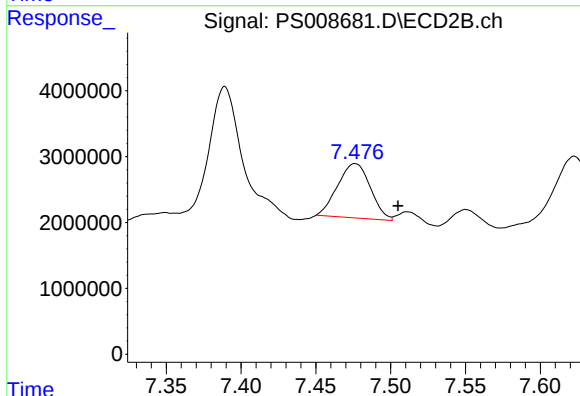


#10 Pentachlorophenol

R.T.: 7.476 min
Delta R.T.: -0.029 min
Response: 12550694
Conc: N.D.

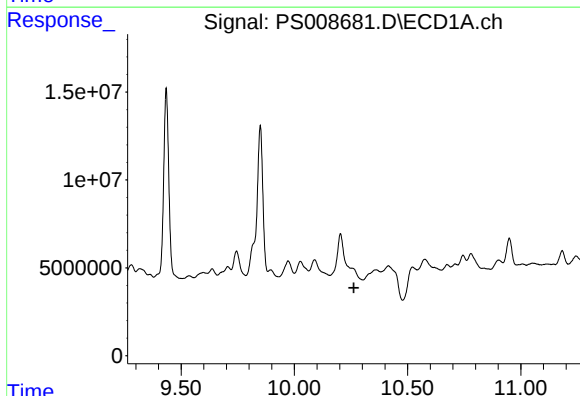


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

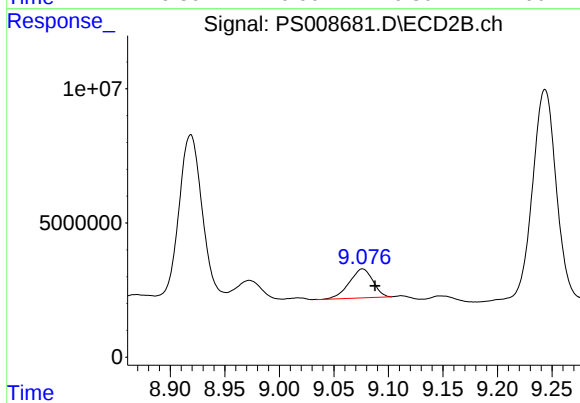

#14 DINOSEB


R.T.: 9.076 min
Delta R.T.: -0.011 min
Response: 16278129
Conc: 4.31 ng/ml

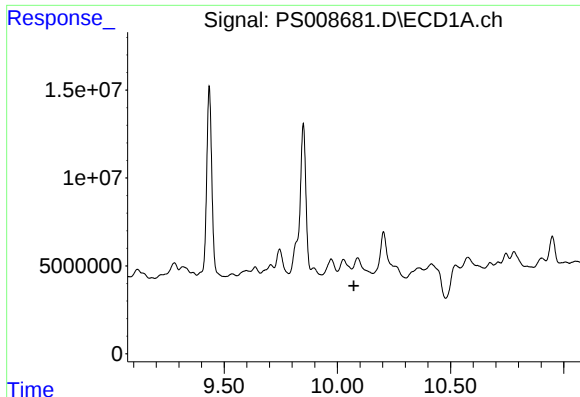

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
124018-A

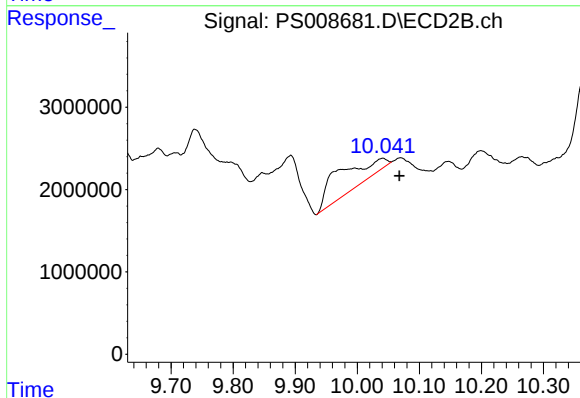


#15 Picloram

R.T.: 10.041 min
Delta R.T.: -0.026 min
Response: 14287280
Conc: 1.92 ng/ml

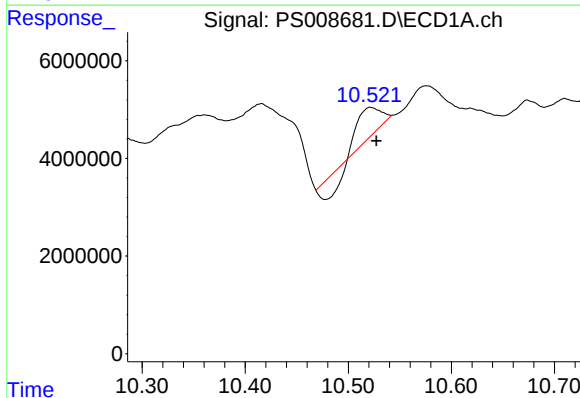

#16 DCPA

R.T.: 10.521 min
Delta R.T.: -0.006 min
Response: 4297580
Conc: N.D.

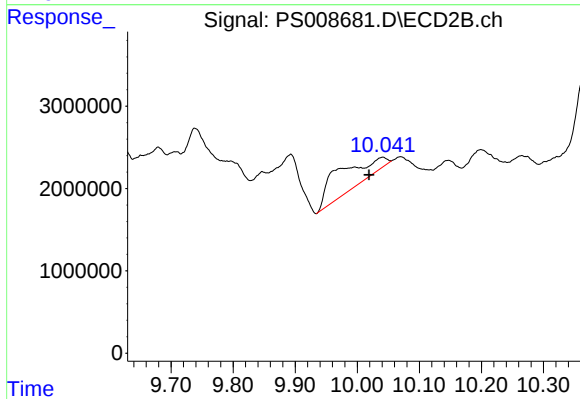

#16 DCPA

R.T.: 10.041 min
Delta R.T.: 0.022 min
Response: 14287280
Conc: 2.19 ng/ml