

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 03:55
 Operator : DD\AJ
 Sample : L1313-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:49:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.294	5.959	113.0E6	303.8E6	63.972	320.681 #
Target Compounds							
1) T	Dalapon	2.585	0.000	196.1E6	0	76.467	N.D. #
2) T	3,5-DICHL...	0.000	5.146	0	93623229	N.D.	67.009
5) T	DICAMBA	0.000	6.092	0	12469742	N.D.	3.118
6) T	MCP	6.703	0.000	29943153	0	5.875	N.D. #
7) T	MCPA	6.811	6.448	95094937	23665840	13.014	5.543 #
8) T	DICHLORPROP	0.000	6.776	0	27000803	N.D.	27.947
9) T	2,4-D	7.385	7.088	51567546	9942965	28.348	8.482 #
10) T	Pentachlo...	7.686	7.480	1356.1E6	420.0E6	55.781	31.099 #
11) T	2,4,5-TP ...	8.195	7.883	6064540	16247415	<MDL	3.109 #
12) T	2,4,5-T	0.000	8.248	0	19179645	N.D.	3.627
13) T	2,4-DB	9.026	8.739	31065241	47845382	22.410	67.588 #
15) T	Picloram	0.000	10.052	0	21202774	N.D.	2.854
16) T	DCPA	10.523	10.052	21340382	21202774	1.798	3.254 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 03:55
Operator : DD\AJ
Sample : L1313-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:49:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

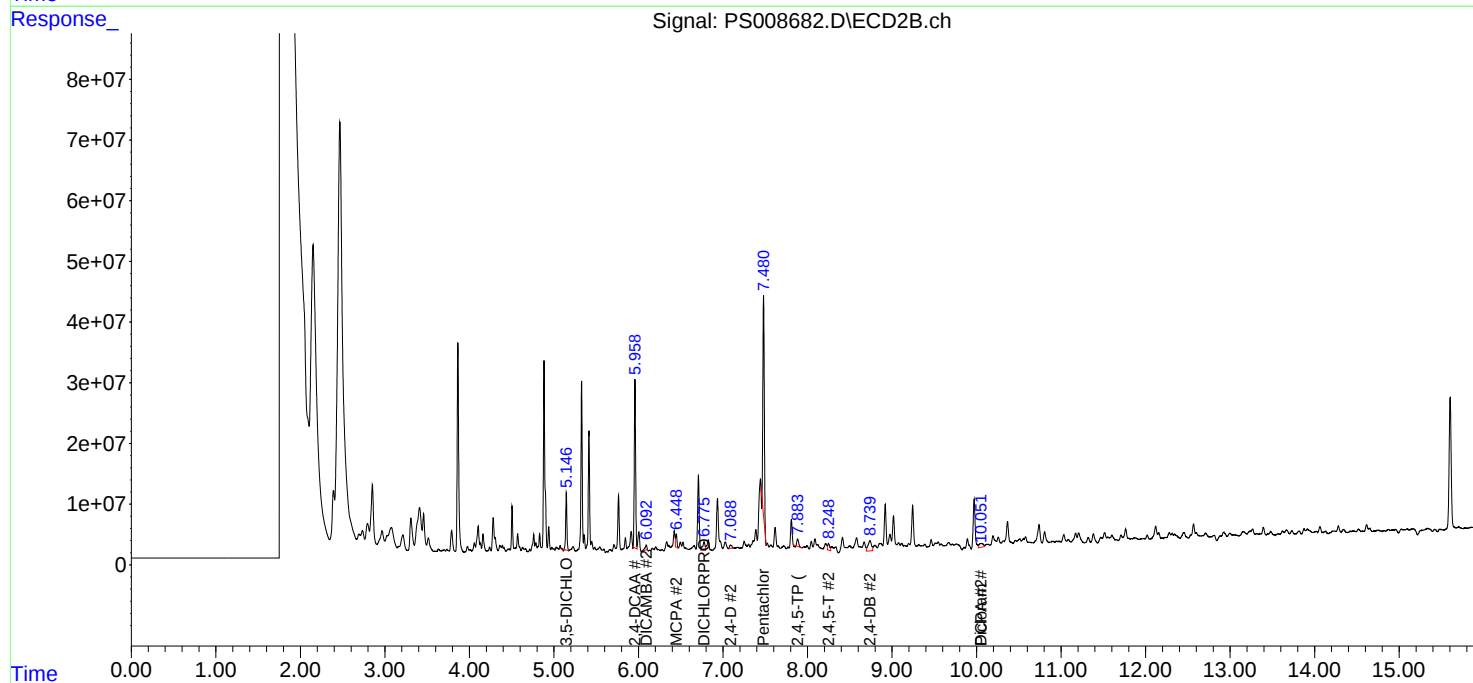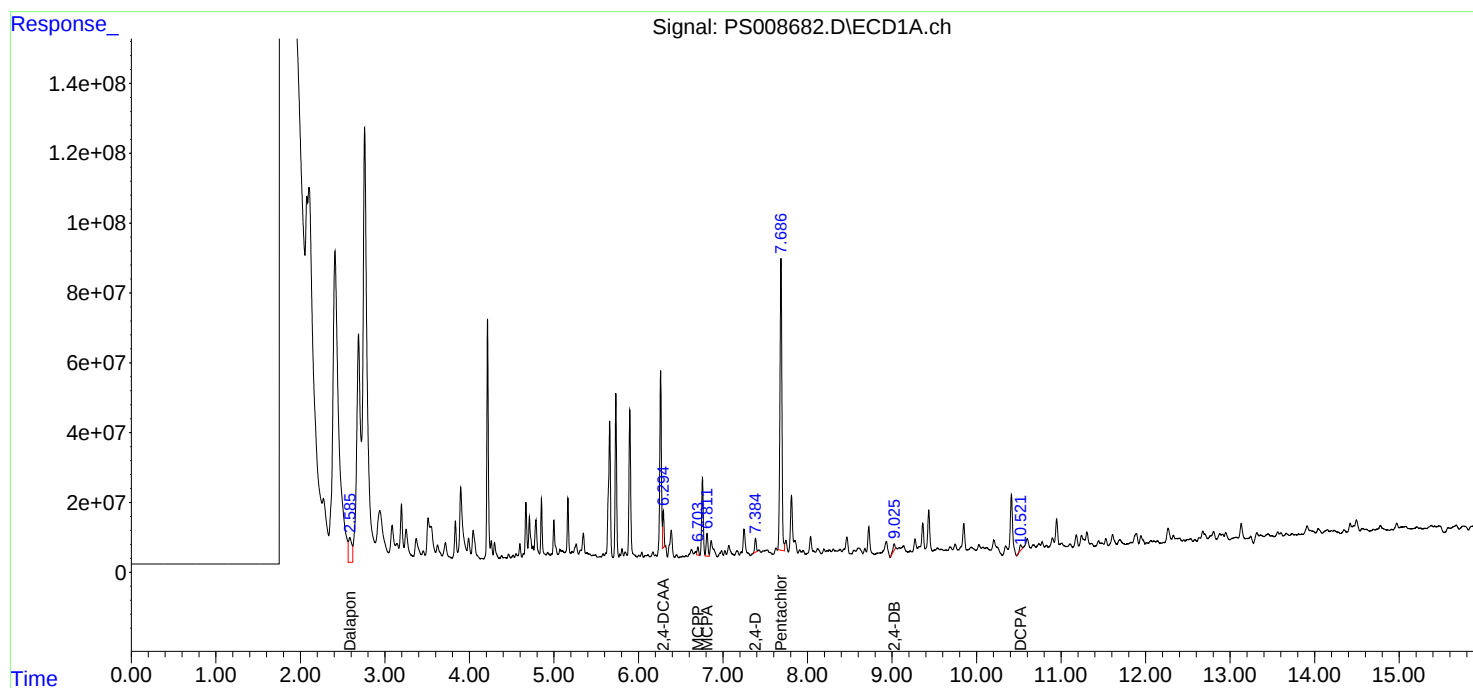


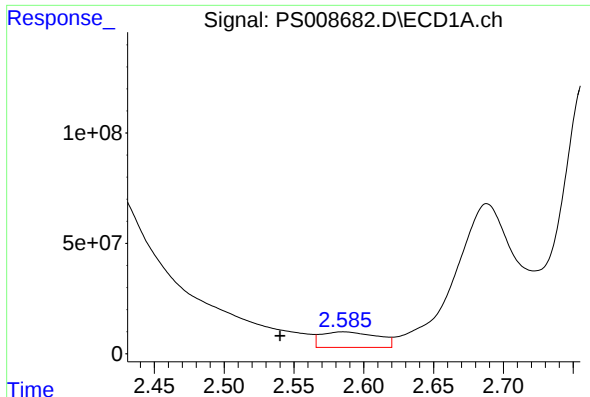

#1 Dalapon


R.T.: 2.585 min
Delta R.T.: 0.045 min
Response: 196050745
Conc: 76.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

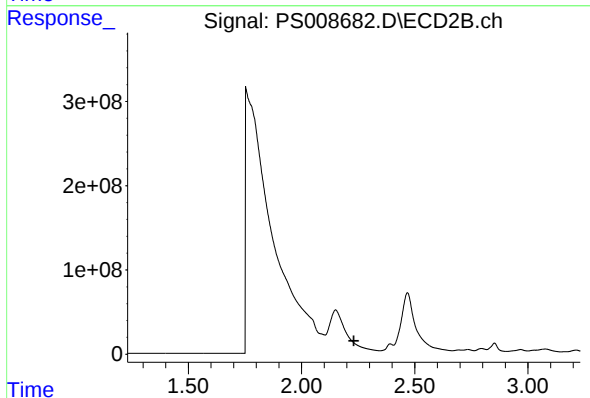


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.231 min
Response: 0
Conc: N.D.

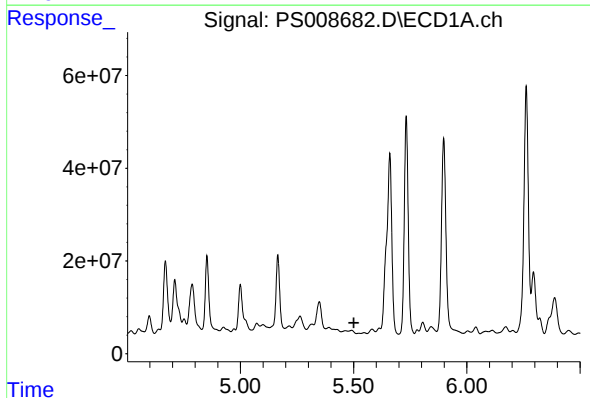


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

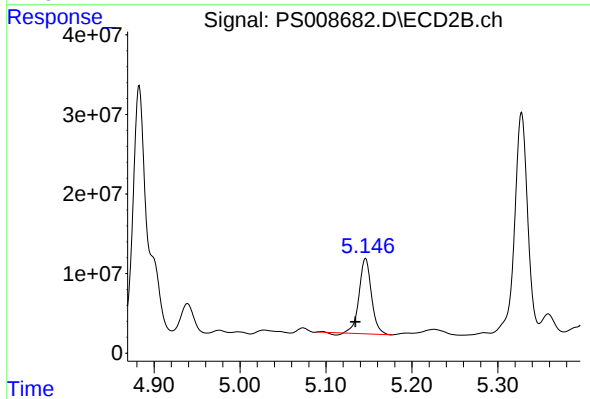

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.012 min
Response: 93623229
Conc: 67.01 ng/ml

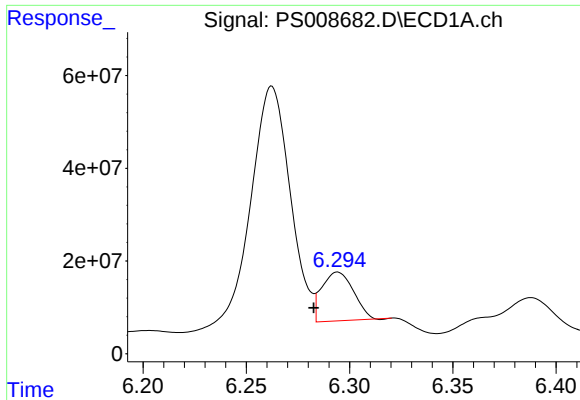

#4 2,4-DCAA


R.T.: 6.294 min
Delta R.T.: 0.012 min
Response: 112955318
Conc: 63.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

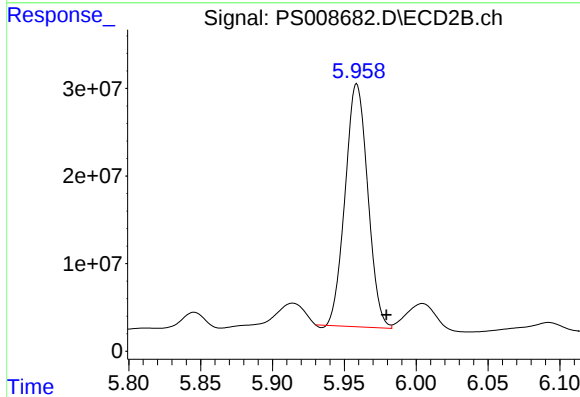


#4 2,4-DCAA

R.T.: 5.959 min
Delta R.T.: -0.021 min
Response: 303833380
Conc: 320.68 ng/ml

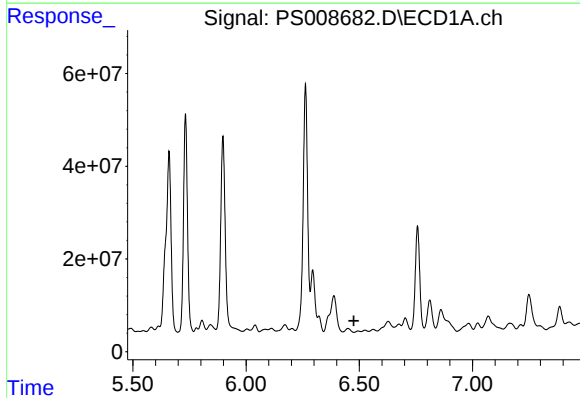


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

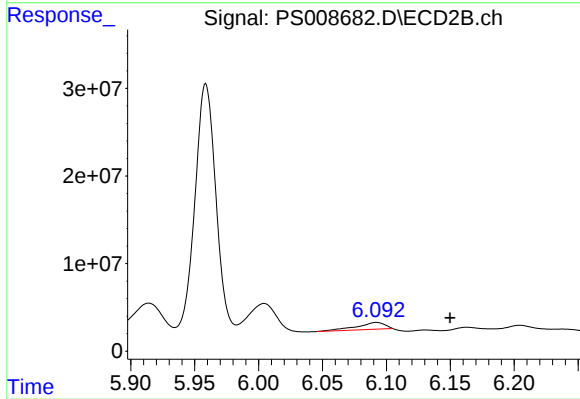

#5 DICAMBA


R.T.: 6.092 min
Delta R.T.: -0.058 min
Response: 12469742
Conc: 3.12 ng/ml

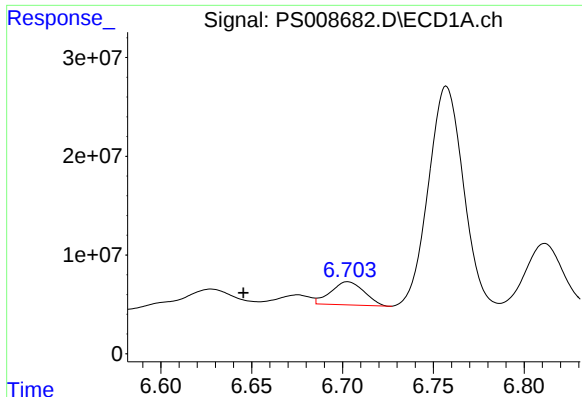

#6 MCPP


R.T.: 6.703 min
Delta R.T.: 0.058 min
Response: 29943153
Conc: 5.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

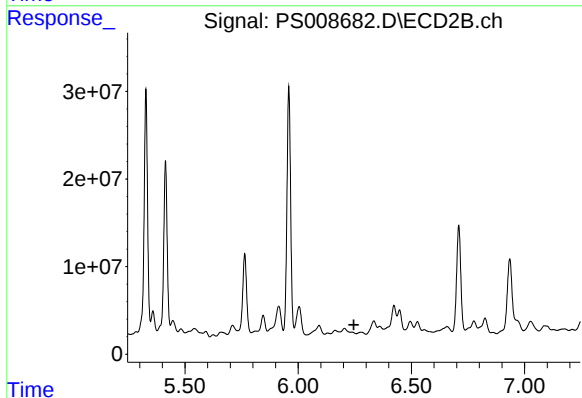


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

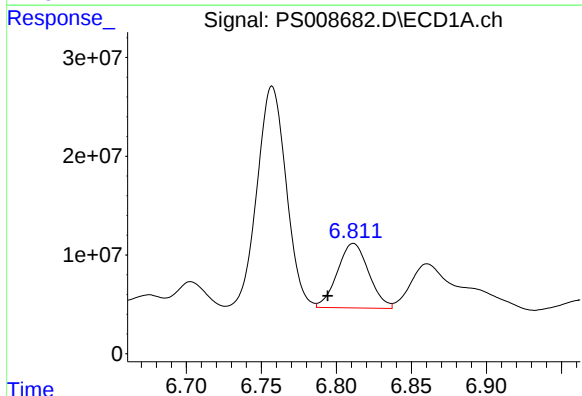


#7 MCPA

R.T.: 6.811 min
Delta R.T.: 0.017 min
Response: 95094937
Conc: 13.01 ug/ml

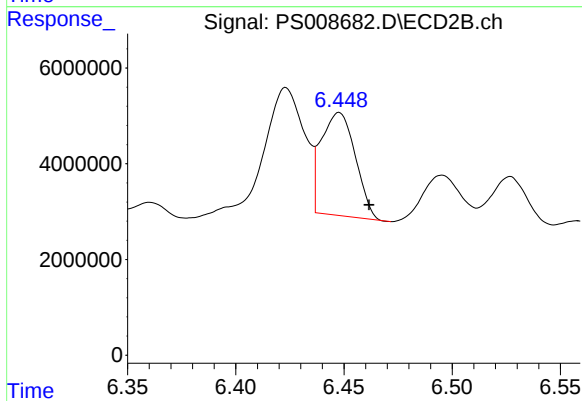

#7 MCPA


R.T.: 6.448 min
Delta R.T.: -0.014 min
Response: 23665840
Conc: 5.54 ug/ml

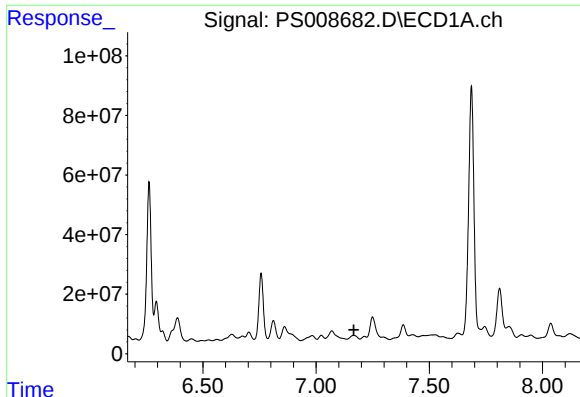

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

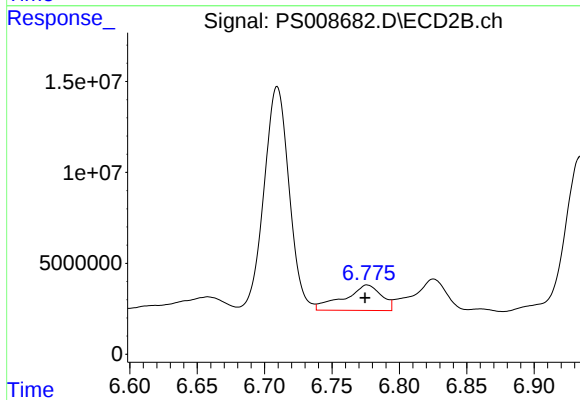


#8 DICHLORPROP

R.T.: 6.776 min
Delta R.T.: 0.001 min
Response: 27000803
Conc: 27.95 ng/ml

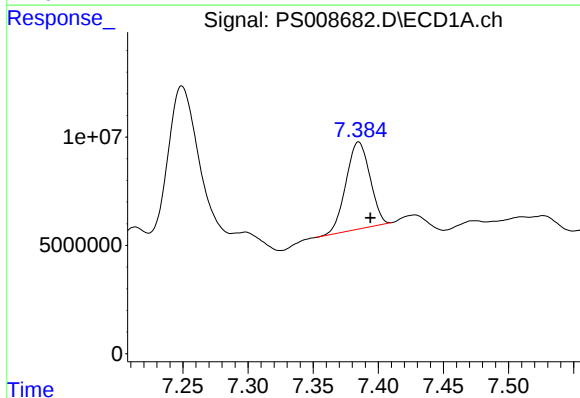


#9 2,4-D

R.T.: 7.385 min
Delta R.T.: -0.009 min
Response: 51567546
Conc: 28.35 ng/ml

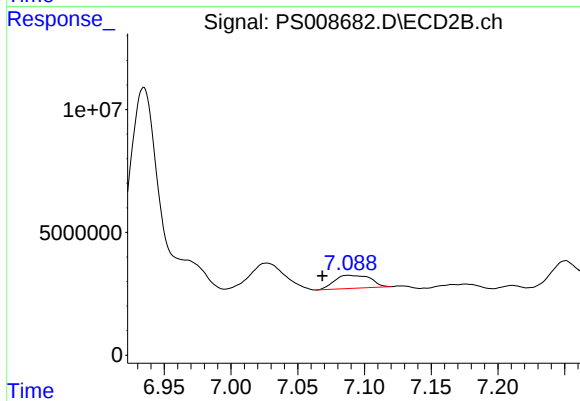

#9 2,4-D


R.T.: 7.088 min
Delta R.T.: 0.019 min
Response: 9942965
Conc: 8.48 ng/ml

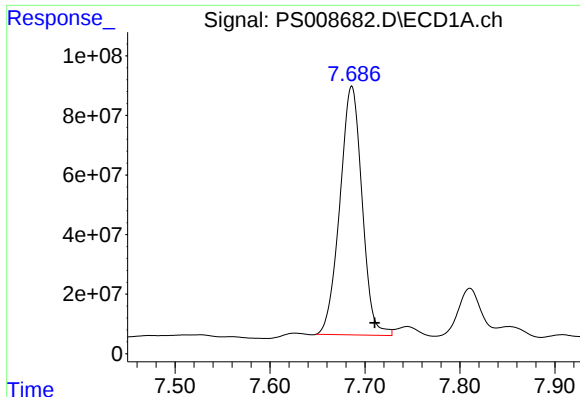

#10 Pentachlorophenol


R.T.: 7.686 min
Delta R.T.: -0.024 min
Response: 1356074262
Conc: 55.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

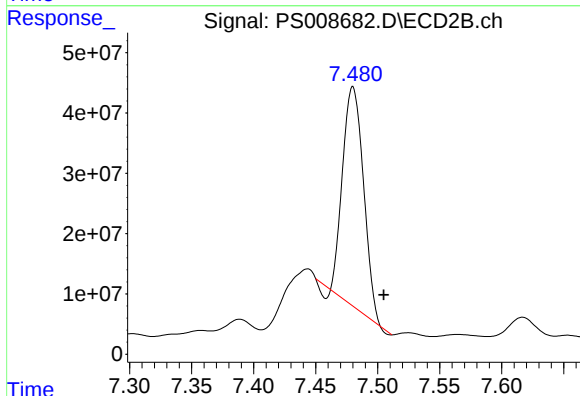


#10 Pentachlorophenol

R.T.: 7.480 min
Delta R.T.: -0.025 min
Response: 419996397
Conc: 31.10 ng/ml

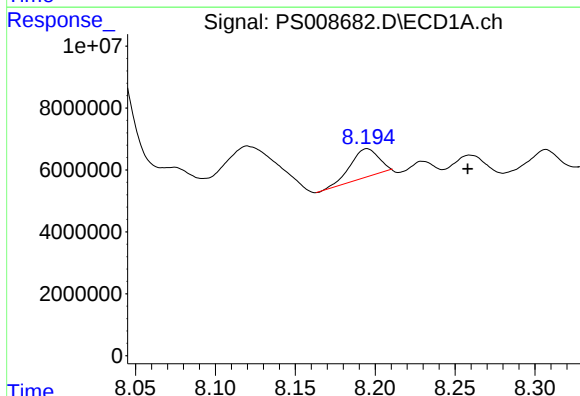


#11 2,4,5-TP (SILVEX)

R.T.: 8.195 min
Delta R.T.: -0.063 min
Response: 6064540
Conc: N.D.

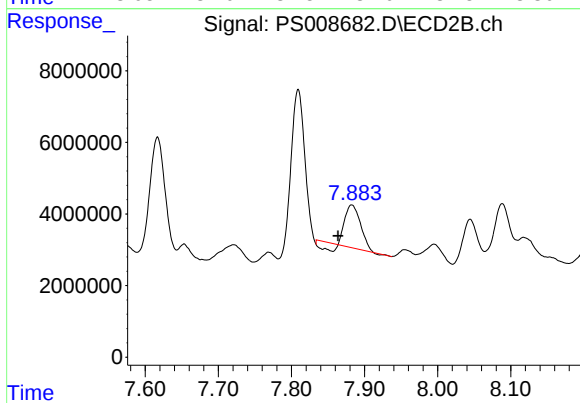

#11 2,4,5-TP (SILVEX)


R.T.: 7.883 min
Delta R.T.: 0.019 min
Response: 16247415
Conc: 3.11 ng/ml

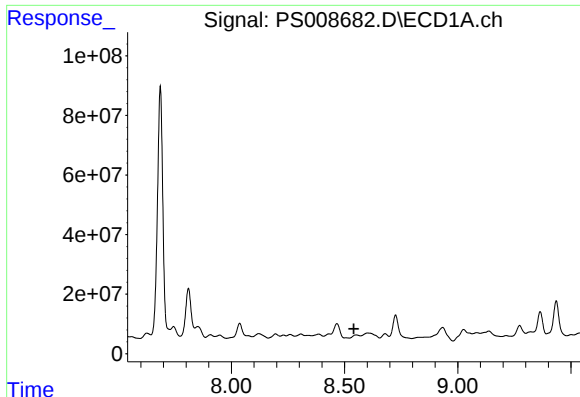

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

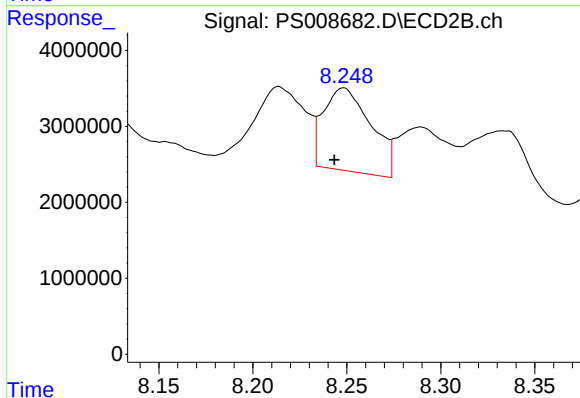


#12 2,4,5-T

R.T.: 8.248 min
Delta R.T.: 0.005 min
Response: 19179645
Conc: 3.63 ng/ml

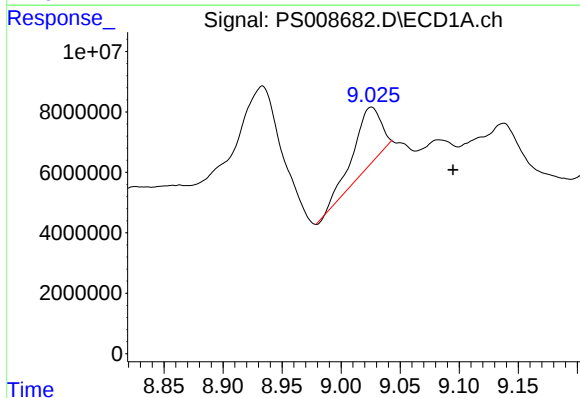


#13 2,4-DB

R.T.: 9.026 min
Delta R.T.: -0.069 min
Response: 31065241
Conc: 22.41 ng/ml

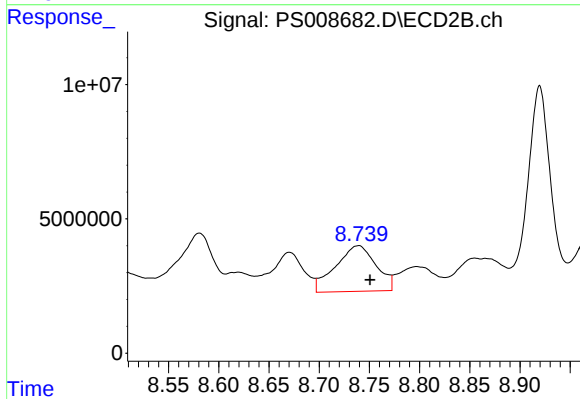

#13 2,4-DB


R.T.: 8.739 min
Delta R.T.: -0.011 min
Response: 47845382
Conc: 67.59 ng/ml

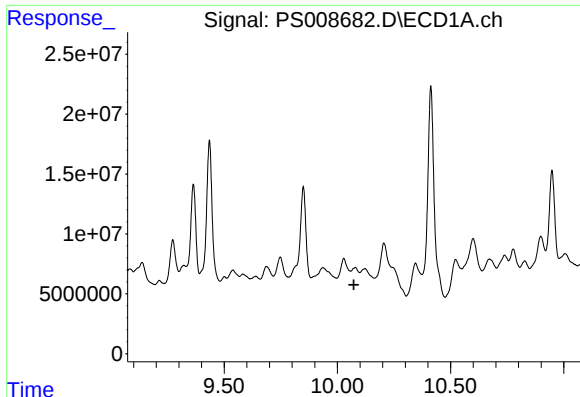

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

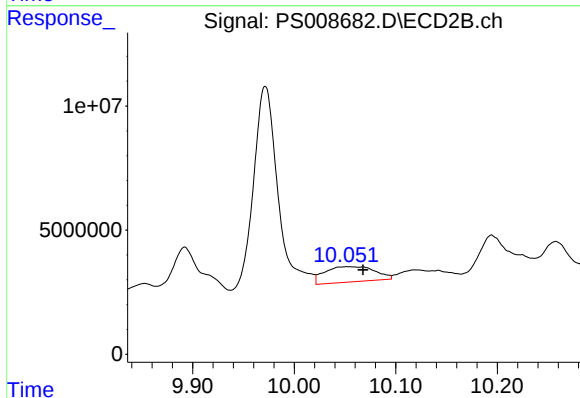


#15 Picloram

R.T.: 10.052 min
Delta R.T.: -0.016 min
Response: 21202774
Conc: 2.85 ng/ml

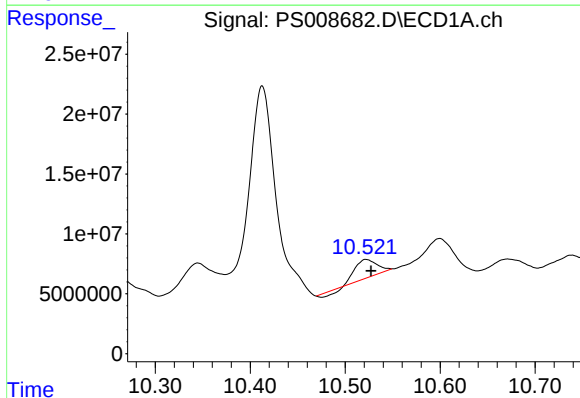

#16 DCPA

R.T.: 10.523 min
Delta R.T.: -0.005 min
Response: 21340382
Conc: 1.80 ng/ml

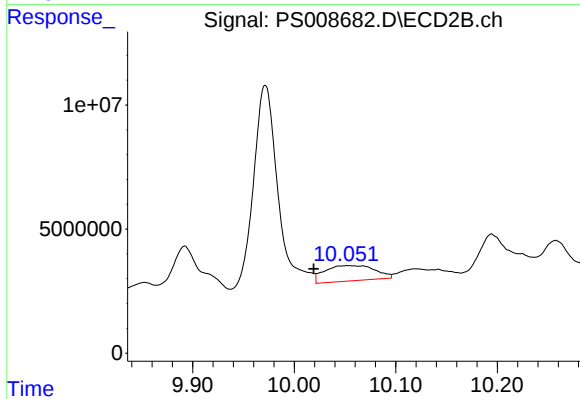

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.033 min
Response: 21202774
Conc: 3.25 ng/ml