

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 07:34
 Operator : DD\AJ
 Sample : PB126523BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126523BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 00:25:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.959	1053.3E6	526.2E6	596.543	555.333
Target Compounds							
1) T	Dalapon	2.497	2.183	76648258	99064480	29.896	78.142 #
2) T	3,5-DICHL...	0.000	5.146	0	99758934	N.D.	71.400
5) T	DICAMBA	0.000	6.093	0	8026754	N.D.	2.007
6) T	MCP	6.677	0.000	20578568	0	4.038	N.D. #
7) T	MCPA	6.811	6.423	79376256	39061768	10.863	9.148
8) T	DICHLORPROP	0.000	6.778	0	17373781	N.D.	17.983
9) T	2,4-D	0.000	7.026	0	10909262	N.D.	9.306
10) T	Pentachlo...	7.746	0.000	41454211	0	1.705	N.D. #
14) T	DINOSEB	0.000	9.077	0	7745249	N.D.	2.050
15) T	Picloram	0.000	10.038	0	34061673	N.D.	4.585
16) T	DCPA	0.000	10.038	0	34061673	N.D.	5.227



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 07:34
Operator : DD\AJ
Sample : PB126523BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB126523BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 00:25:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

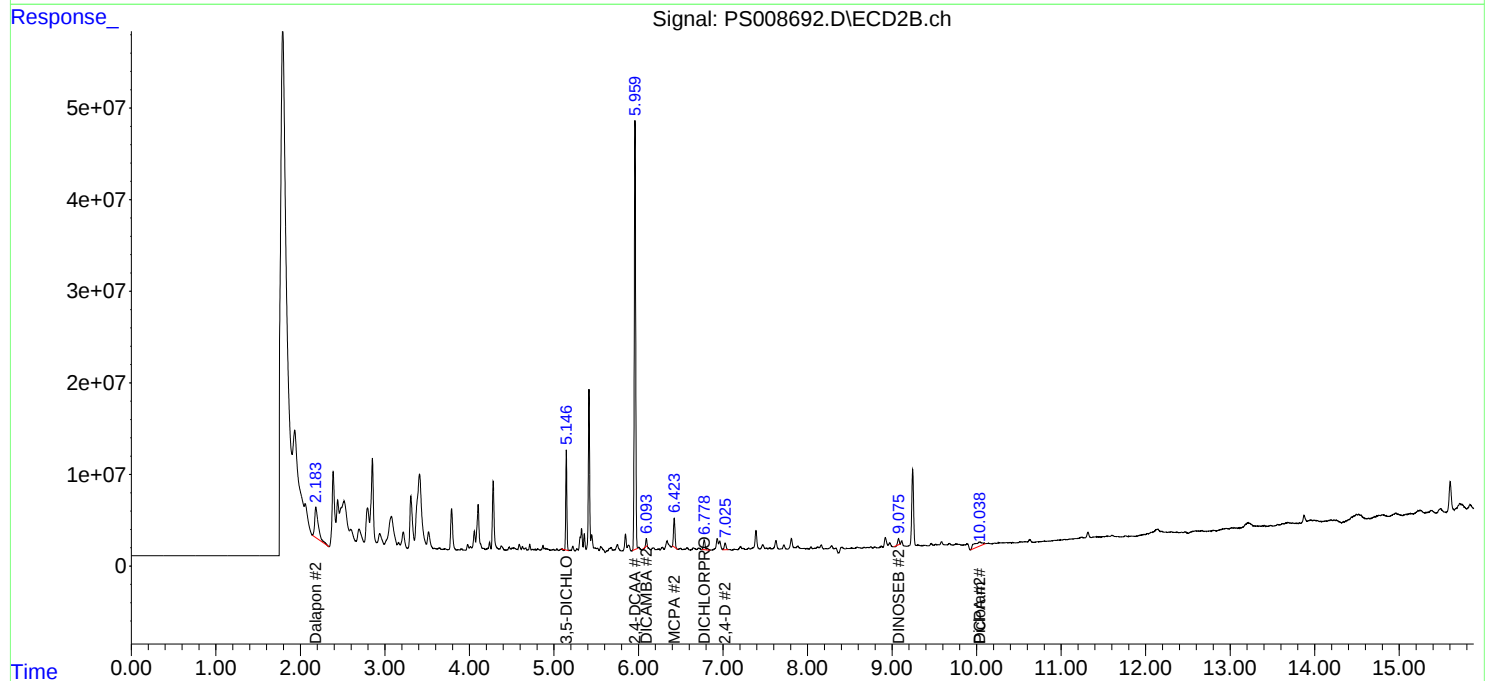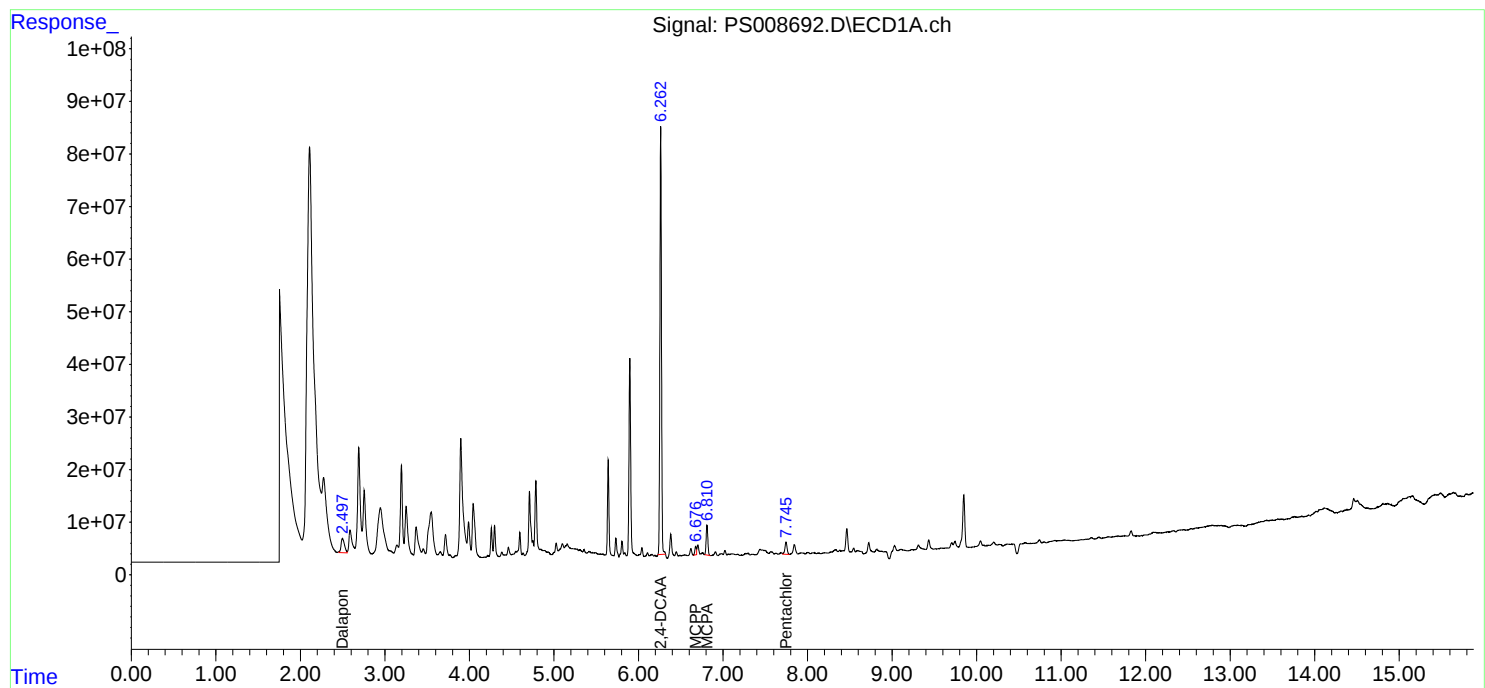


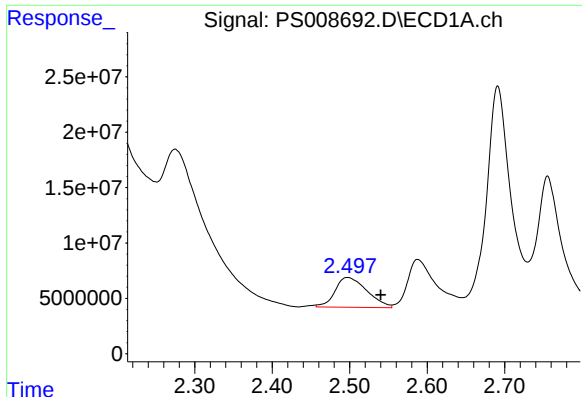

#1 Dalapon


R.T.: 2.497 min
Delta R.T.: -0.043 min
Response: 76648258
Conc: 29.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126523BL

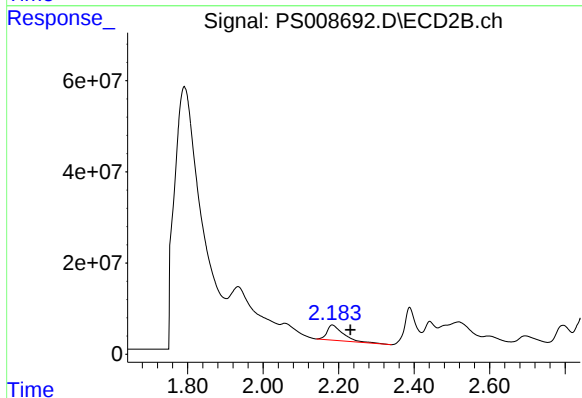


#1 Dalapon

R.T.: 2.183 min
Delta R.T.: -0.048 min
Response: 99064480
Conc: 78.14 ng/ml

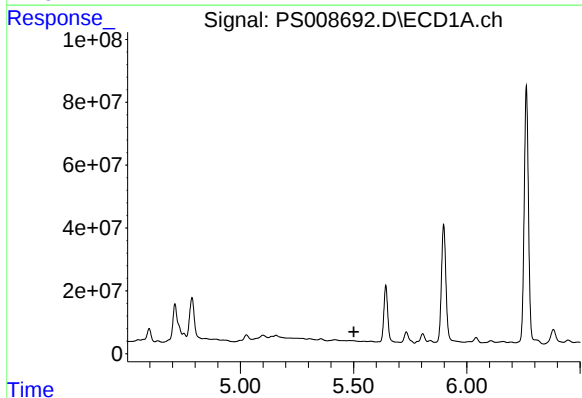


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

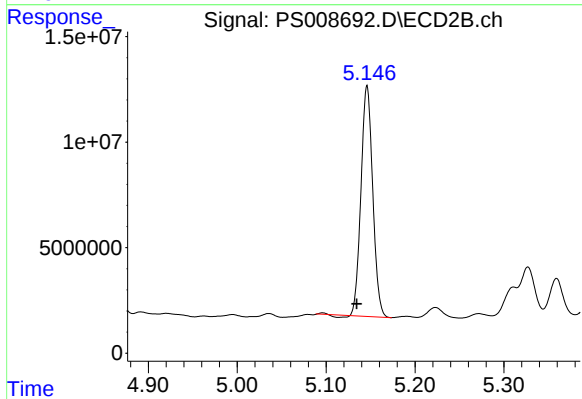

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.012 min
Response: 99758934
Conc: 71.40 ng/ml

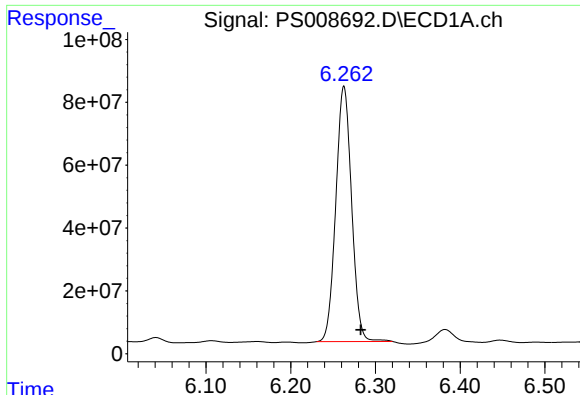

#4 2,4-DCAA


R.T.: 6.263 min
Delta R.T.: -0.020 min
Response: 1053318523
Conc: 596.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126523BL

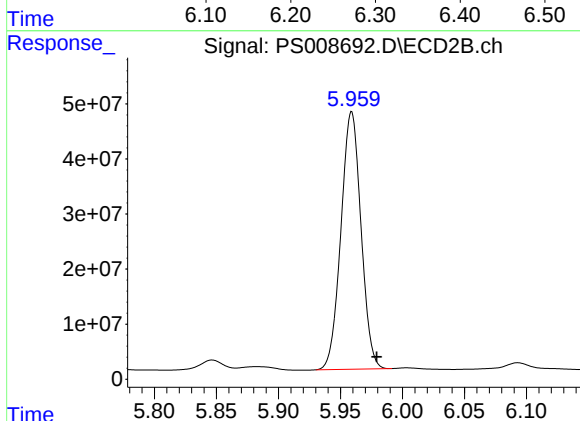


#4 2,4-DCAA

R.T.: 5.959 min
Delta R.T.: -0.020 min
Response: 526157438
Conc: 555.33 ng/ml

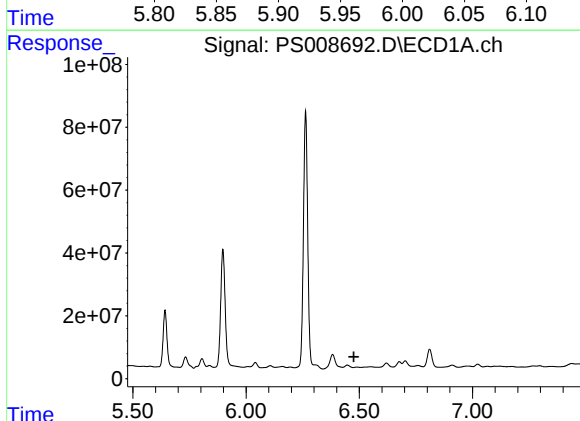


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

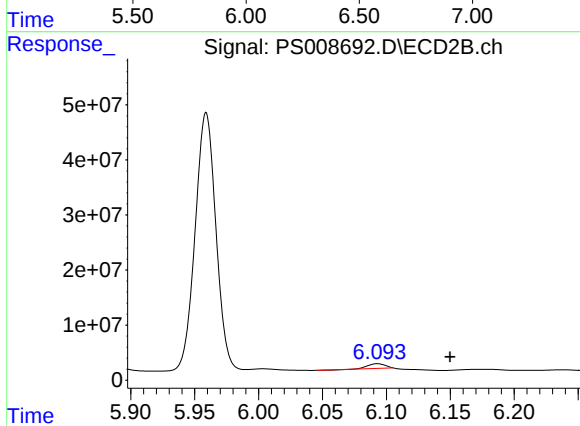

#5 DICAMBA


R.T.: 6.093 min
Delta R.T.: -0.057 min
Response: 8026754
Conc: 2.01 ng/ml

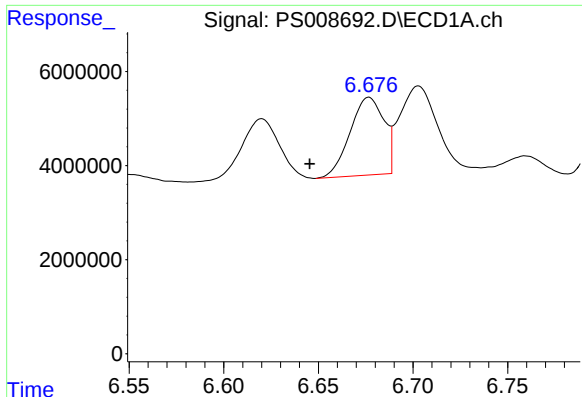

#6 MCPP


R.T.: 6.677 min
Delta R.T.: 0.031 min
Response: 20578568
Conc: 4.04 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB126523BL

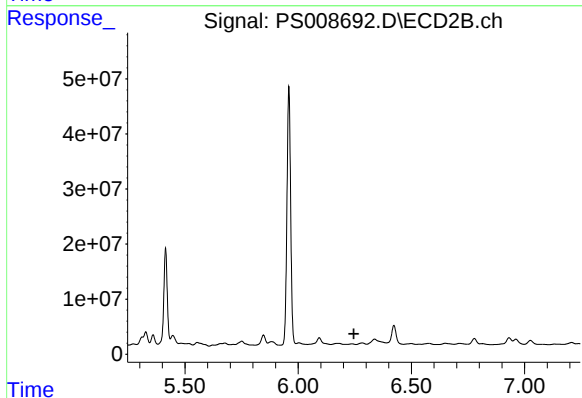


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

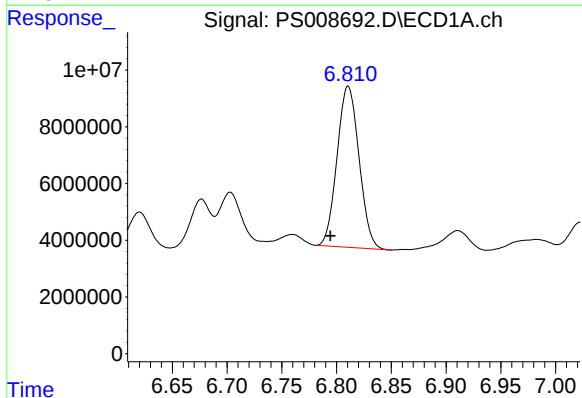


#7 MCPA

R.T.: 6.811 min
Delta R.T.: 0.016 min
Response: 79376256
Conc: 10.86 ug/ml

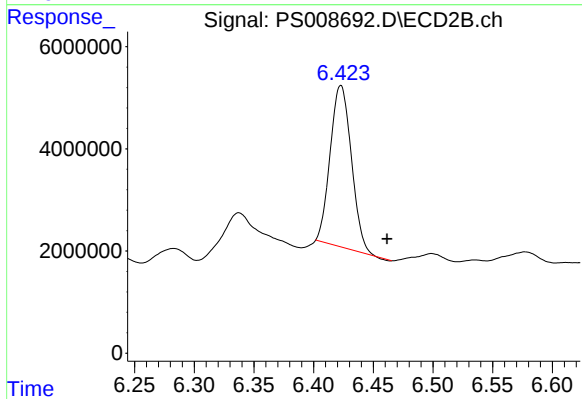

#7 MCPA


R.T.: 6.423 min
Delta R.T.: -0.039 min
Response: 39061768
Conc: 9.15 ug/ml

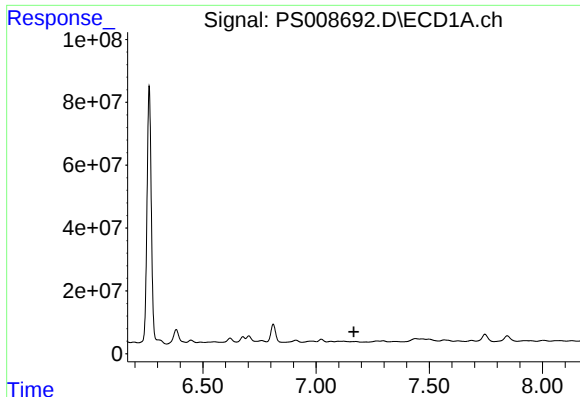

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126523BL

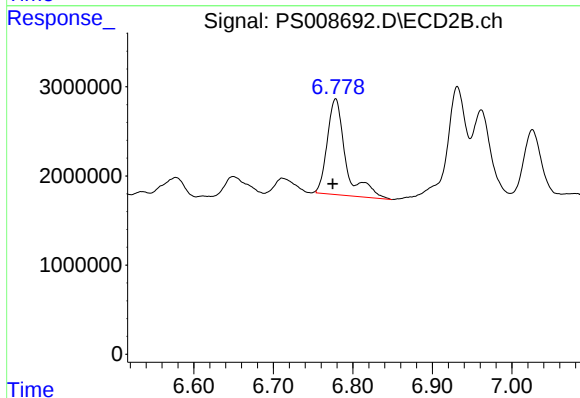


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.003 min
Response: 17373781
Conc: 17.98 ng/ml

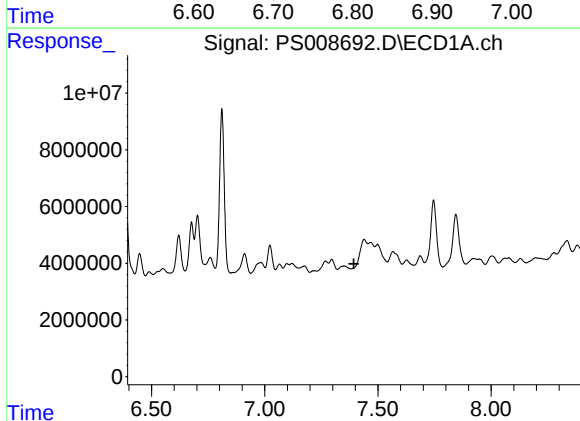


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

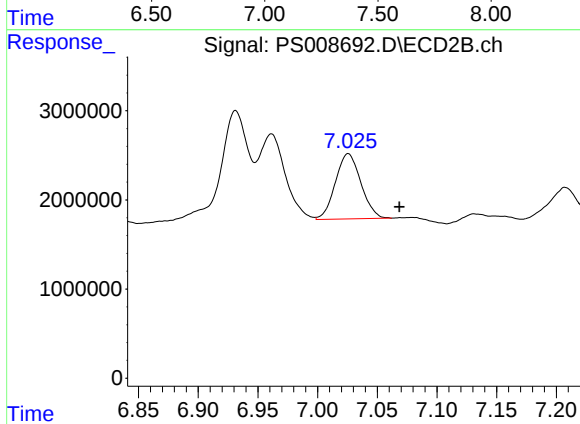

#9 2,4-D


R.T.: 7.026 min
Delta R.T.: -0.043 min
Response: 10909262
Conc: 9.31 ng/ml

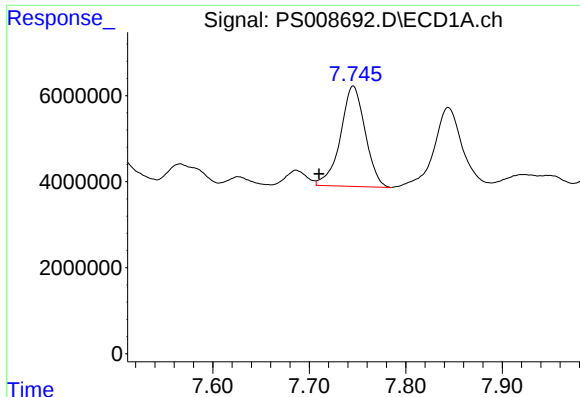

#10 Pentachlorophenol


R.T.: 7.746 min
Delta R.T.: 0.035 min
Response: 41454211
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126523BL

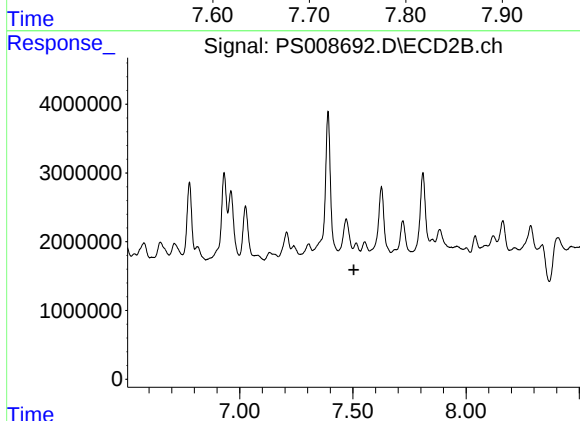


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

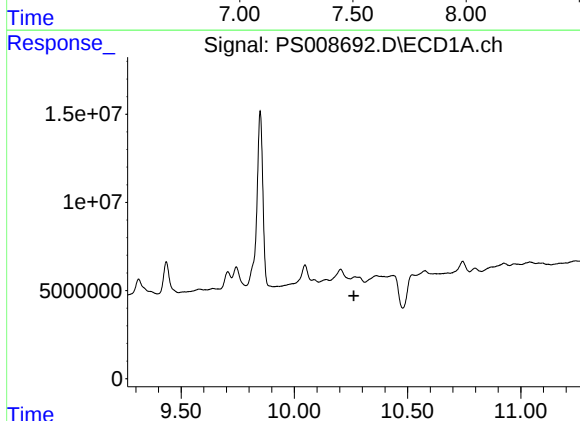


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

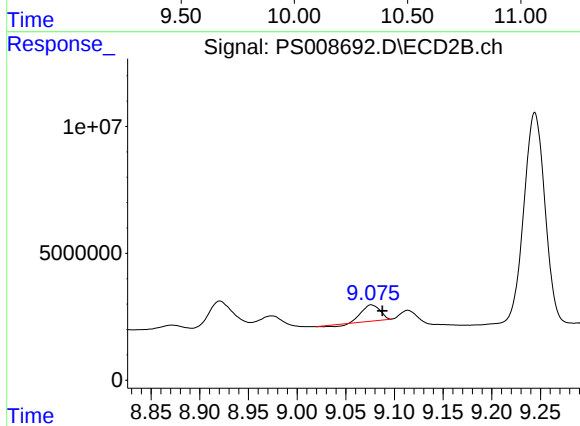

#14 DINOSEB


R.T.: 9.077 min
Delta R.T.: -0.011 min
Response: 7745249
Conc: 2.05 ng/ml

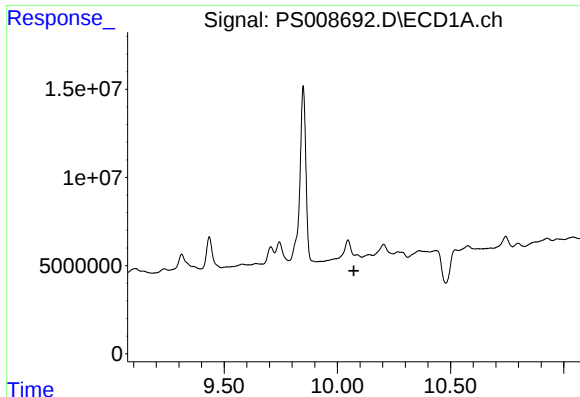

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126523BL

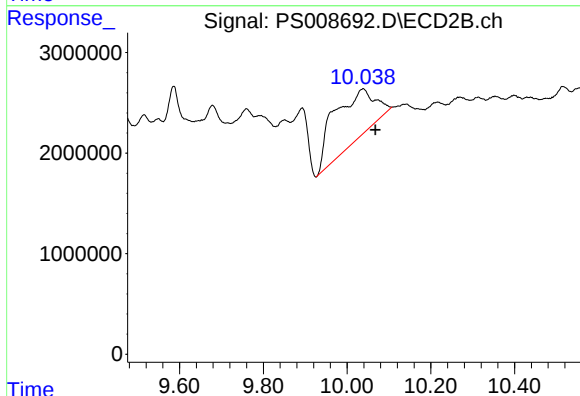


#15 Picloram

R.T.: 10.038 min
Delta R.T.: -0.030 min
Response: 34061673
Conc: 4.58 ng/ml

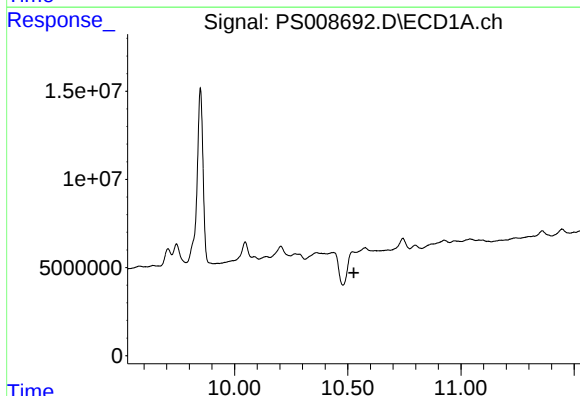

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

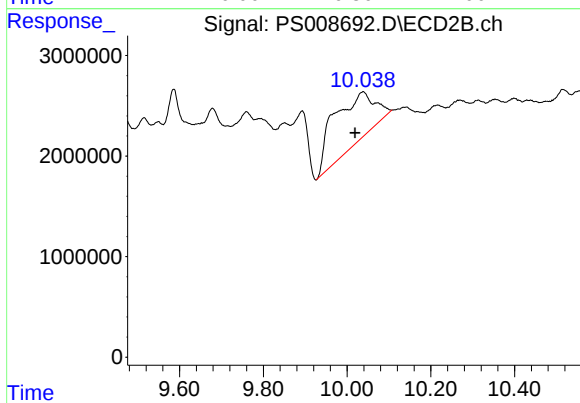

#16 DCPA

R.T.: 10.038 min
Delta R.T.: 0.019 min
Response: 34061673
Conc: 5.23 ng/ml