

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 08:39
 Operator : DD\AJ
 Sample : L1332-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 KIT-SINK-1ST-DRAW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 00:26:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.263	5.958	982.1E6	490.1E6	556.200	517.297
Target Compounds							
1) T	Dalapon	2.495	2.180	222.0E6	16798632	86.575	13.251 #
2) T	3,5-DICHL...	0.000	5.146	0	66440876	N.D.	47.554
5) T	DICAMBA	0.000	6.092	0	5524834	N.D.	1.382
6) T	MCP	6.703	0.000	23431687	0	4.597	N.D. #
7) T	MCPA	6.811	6.423	73333726	36257857	10.036	8.492
8) T	DICHLORPROP	0.000	6.778	0	18645784	N.D.	19.299
9) T	2,4-D	0.000	7.025	0	15154526	N.D.	12.928
10) T	Pentachlo...	7.688	7.479	29118744	17781048	1.198	1.317
12) T	2,4,5-T	0.000	8.272	0	11916273	N.D.	2.253
15) T	Picloram	10.115	10.043	31304656	23081912	2.508	3.107
16) T	DCPA	10.504	10.043	641.5E6	23081912	54.050	3.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 08:39
Operator : DD\AJ
Sample : L1332-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 00:26:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

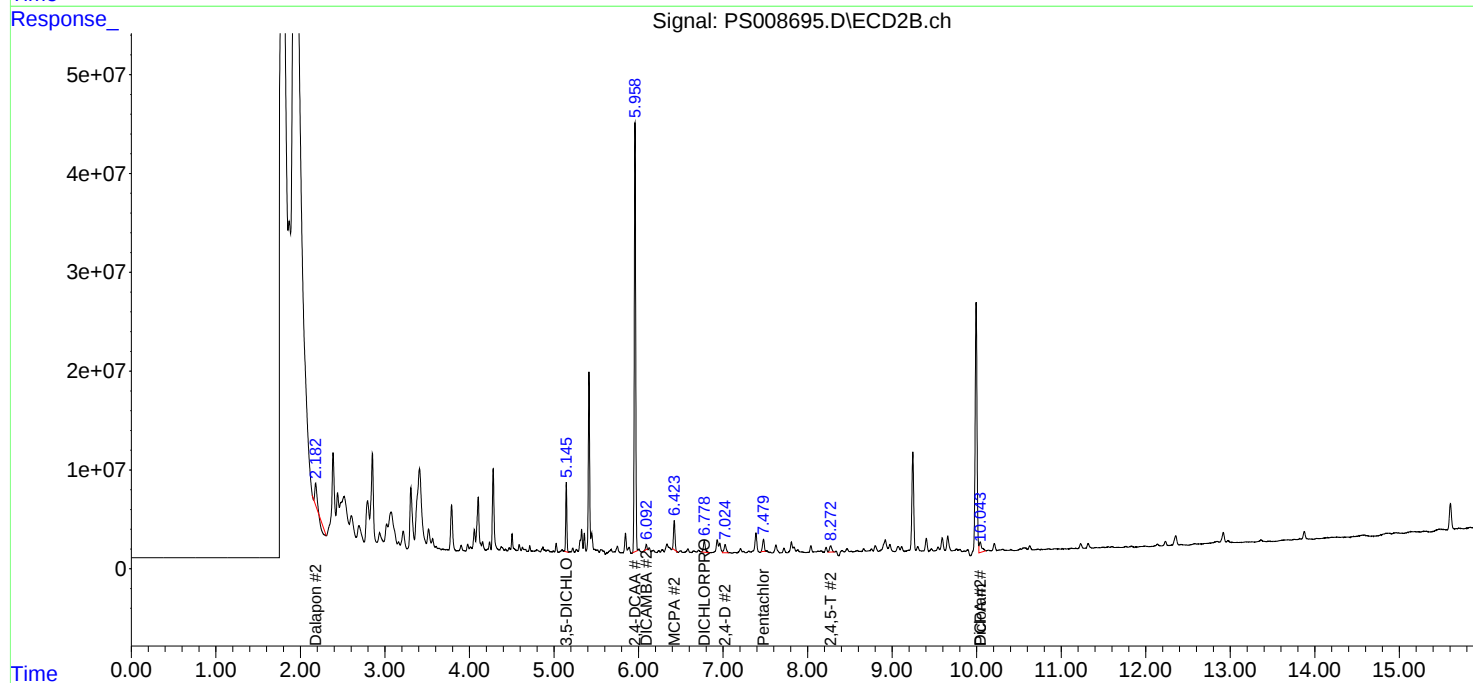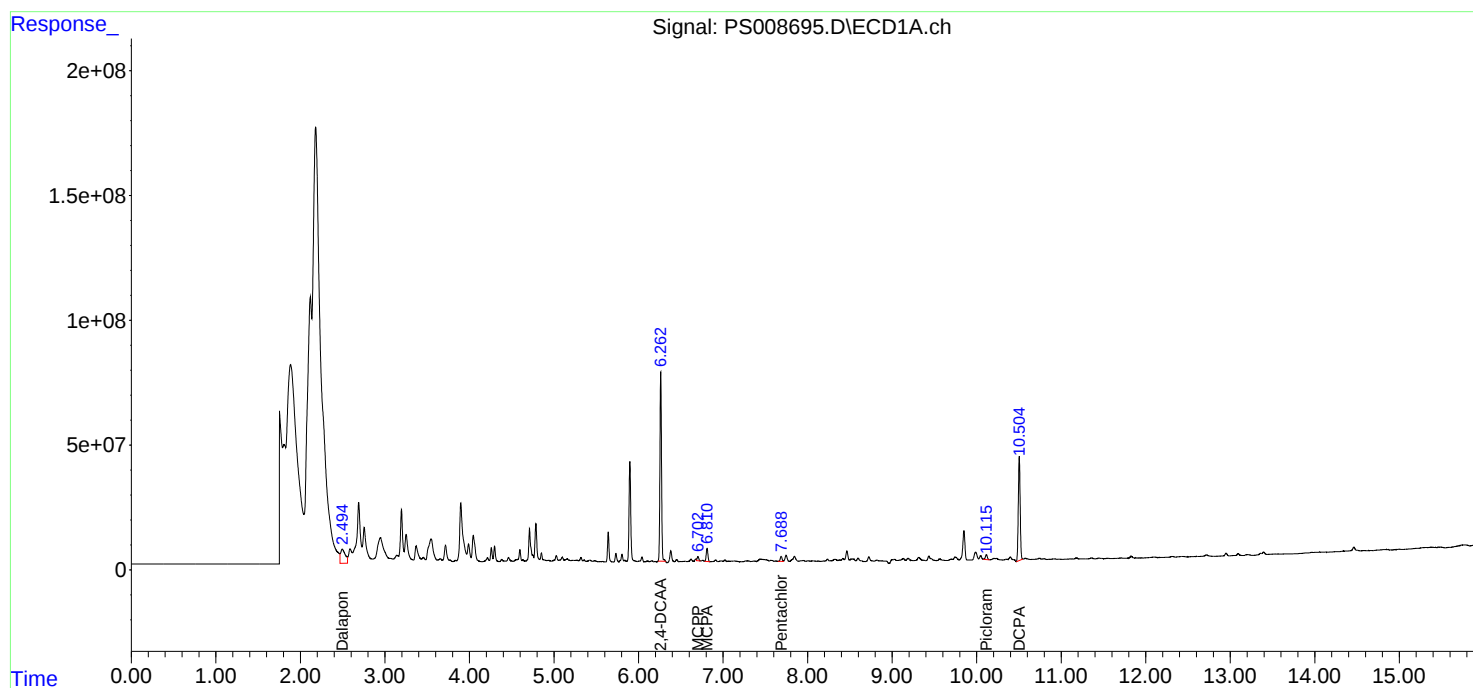


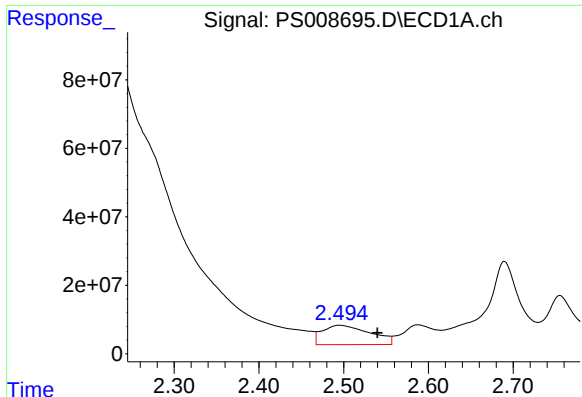

#1 Dalapon


R.T.: 2.495 min
Delta R.T.: -0.045 min
Response: 221964587
Conc: 86.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

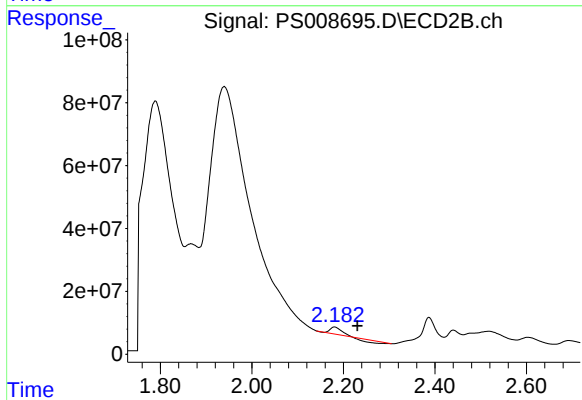


#1 Dalapon

R.T.: 2.180 min
Delta R.T.: -0.051 min
Response: 16798632
Conc: 13.25 ng/ml

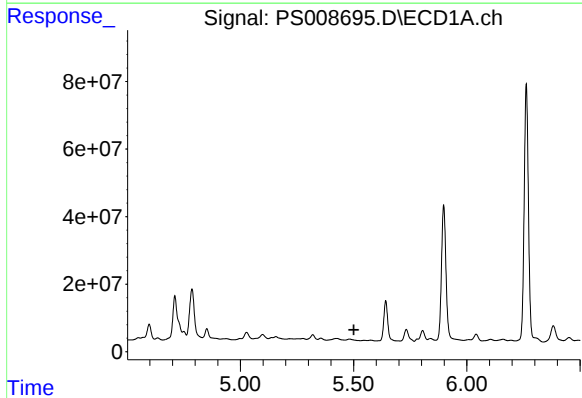


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

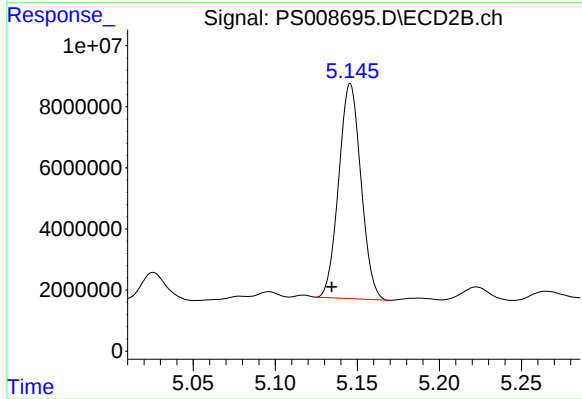

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.146 min
Delta R.T.: 0.011 min
Response: 66440876
Conc: 47.55 ng/ml

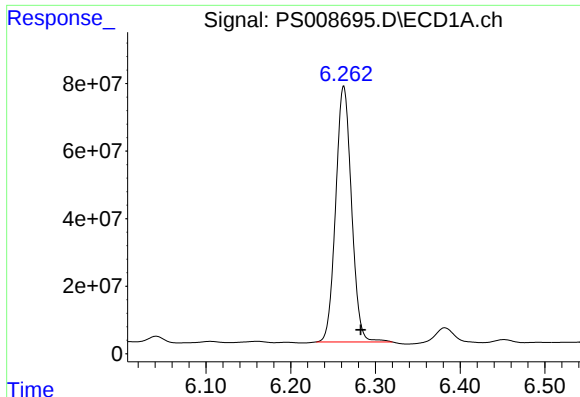

#4 2,4-DCAA


R.T.: 6.263 min
Delta R.T.: -0.020 min
Response: 982083731
Conc: 556.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

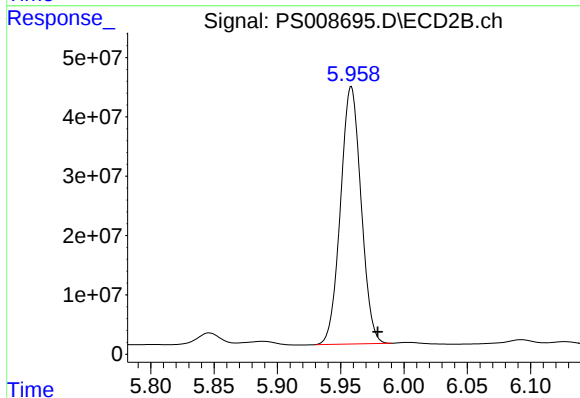


#4 2,4-DCAA

R.T.: 5.958 min
Delta R.T.: -0.021 min
Response: 490119842
Conc: 517.30 ng/ml

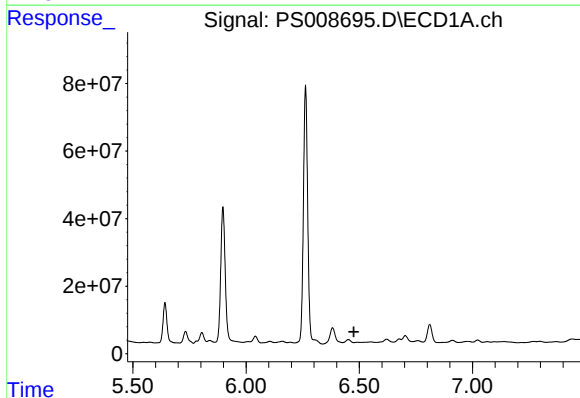


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

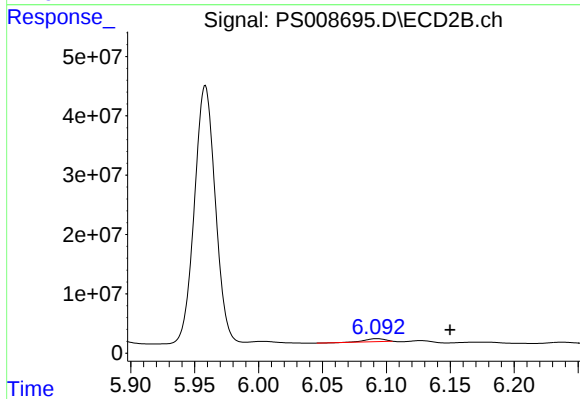

#5 DICAMBA


R.T.: 6.092 min
Delta R.T.: -0.057 min
Response: 5524834
Conc: 1.38 ng/ml

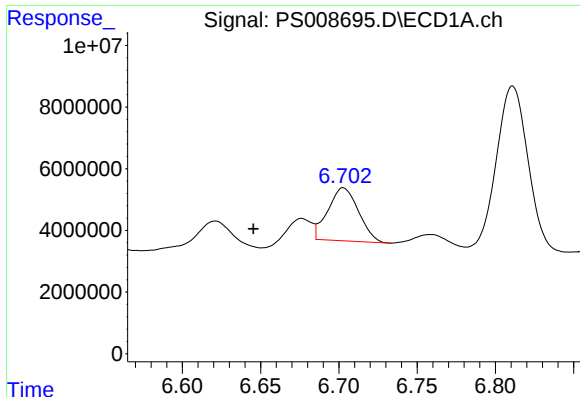

#6 MCP


R.T.: 6.703 min
Delta R.T.: 0.057 min
Response: 23431687
Conc: 4.60 ug/ml

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

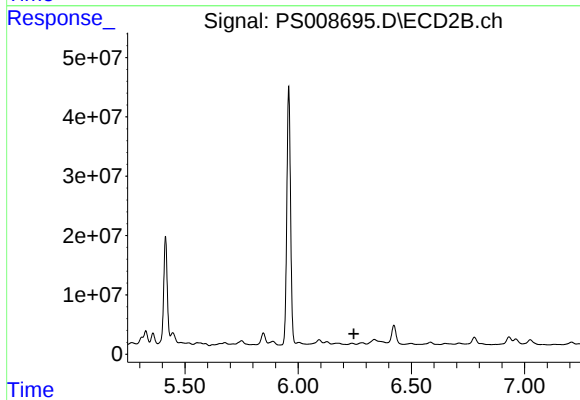


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

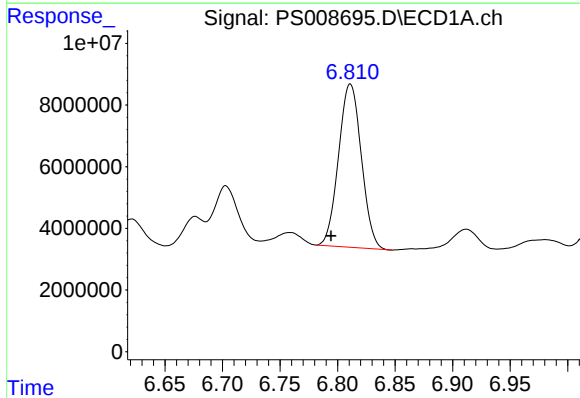


#7 MCP

R.T.: 6.811 min
Delta R.T.: 0.017 min
Response: 73333726
Conc: 10.04 ug/ml

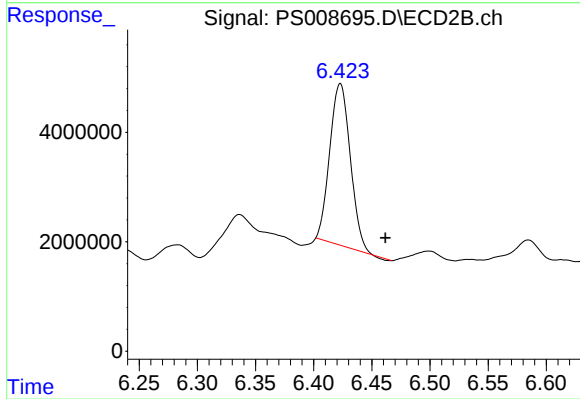

#7 MCP


R.T.: 6.423 min
Delta R.T.: -0.039 min
Response: 36257857
Conc: 8.49 ug/ml

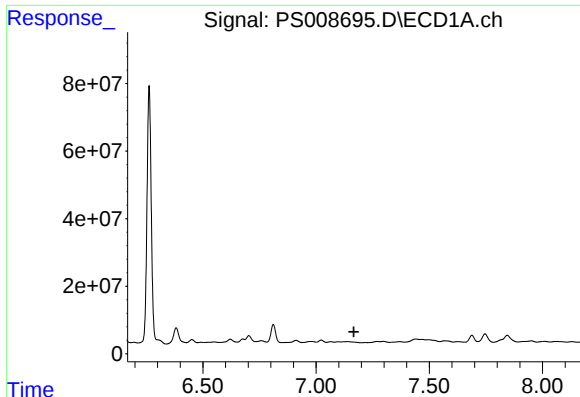

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

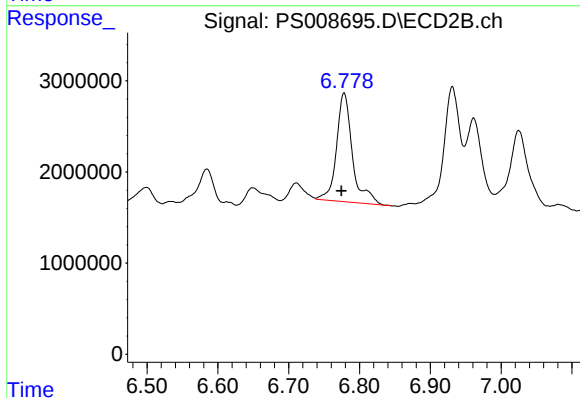


#8 DICHLORPROP

R.T.: 6.778 min
Delta R.T.: 0.004 min
Response: 18645784
Conc: 19.30 ng/ml

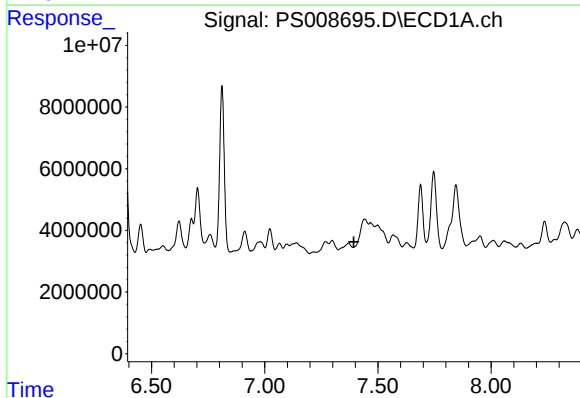


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

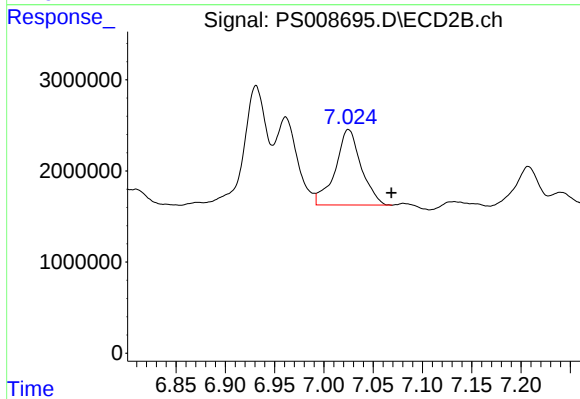

#9 2,4-D


R.T.: 7.025 min
Delta R.T.: -0.044 min
Response: 15154526
Conc: 12.93 ng/ml

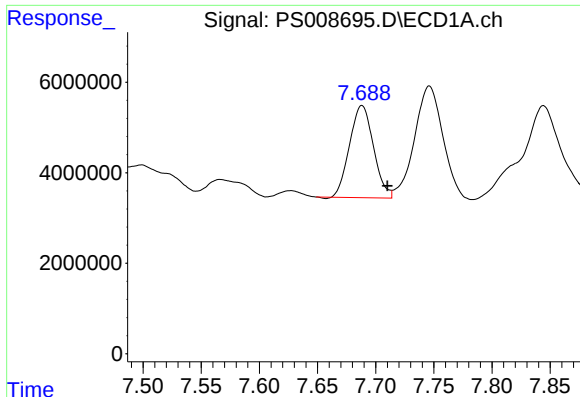

#10 Pentachlorophenol


R.T.: 7.688 min
Delta R.T.: -0.022 min
Response: 29118744
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

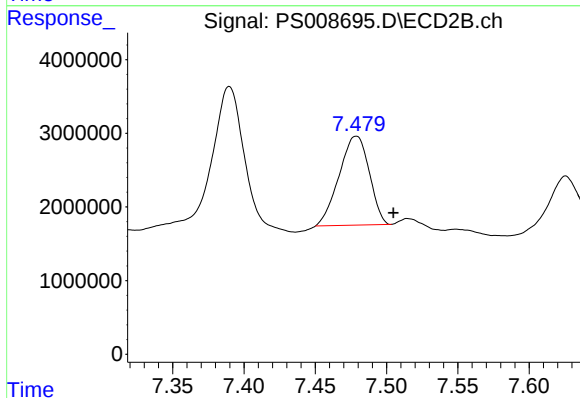


#10 Pentachlorophenol

R.T.: 7.479 min
Delta R.T.: -0.026 min
Response: 17781048
Conc: 1.32 ng/ml

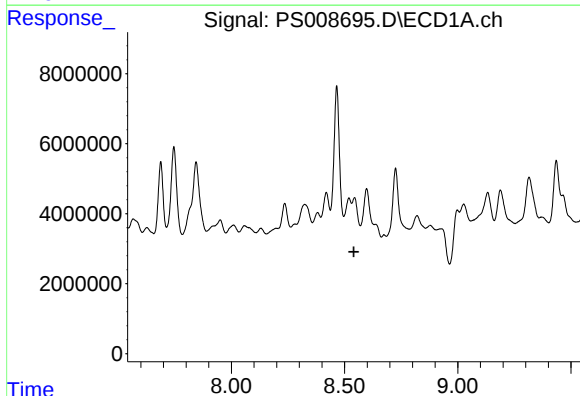


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.541 min
Response: 0
Conc: N.D.

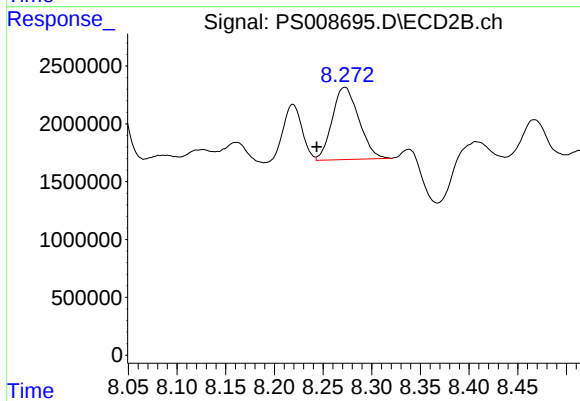

#12 2,4,5-T


R.T.: 8.272 min
Delta R.T.: 0.029 min
Response: 11916273
Conc: 2.25 ng/ml

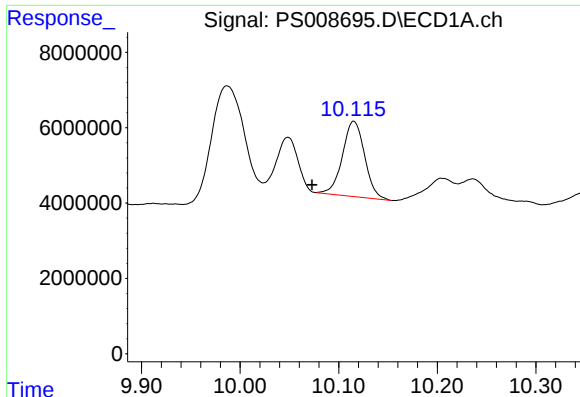

#15 Picloram


R.T.: 10.115 min
Delta R.T.: 0.042 min
Response: 31304656
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
KIT-SINK-1ST-DRAW

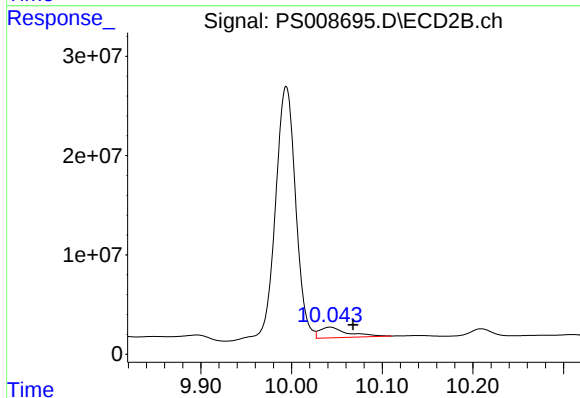


#15 Picloram

R.T.: 10.043 min
Delta R.T.: -0.025 min
Response: 23081912
Conc: 3.11 ng/ml

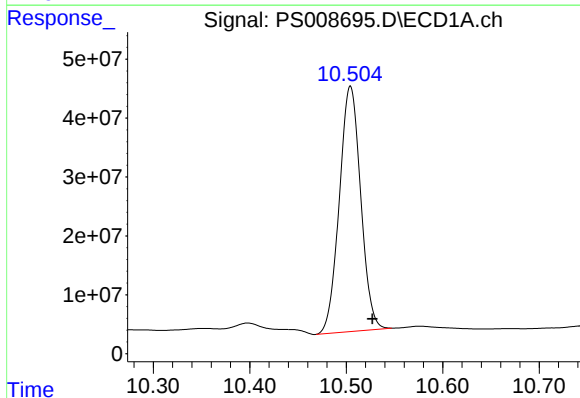

#16 DCPA

R.T.: 10.504 min
Delta R.T.: -0.023 min
Response: 641452736
Conc: 54.05 ng/ml

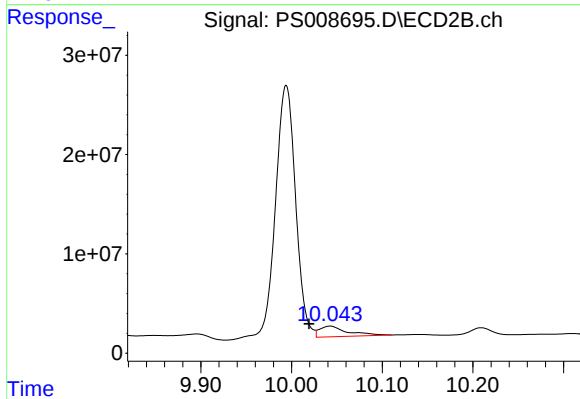

#16 DCPA

R.T.: 10.043 min
Delta R.T.: 0.024 min
Response: 23081912
Conc: 3.54 ng/ml