

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
 Data File : PS008689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 06:28
 Operator : DD\AJ
 Sample : L1319-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RAINEY-PARK-BH-02-A

Manual Integrations
 APPROVED

mohammad
 2/4/2020 12:34:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 00:24:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.262	5.958	739.6E6	323.1E6	418.859m	341.007m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013120\
Data File : PS008689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 06:28
Operator : DD\AJ
Sample : L1319-11
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
RAINEY-PARK-BH-02-A


Manual Integrations
APPROVED

mohammad
2/4/2020 12:34:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 00:24:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

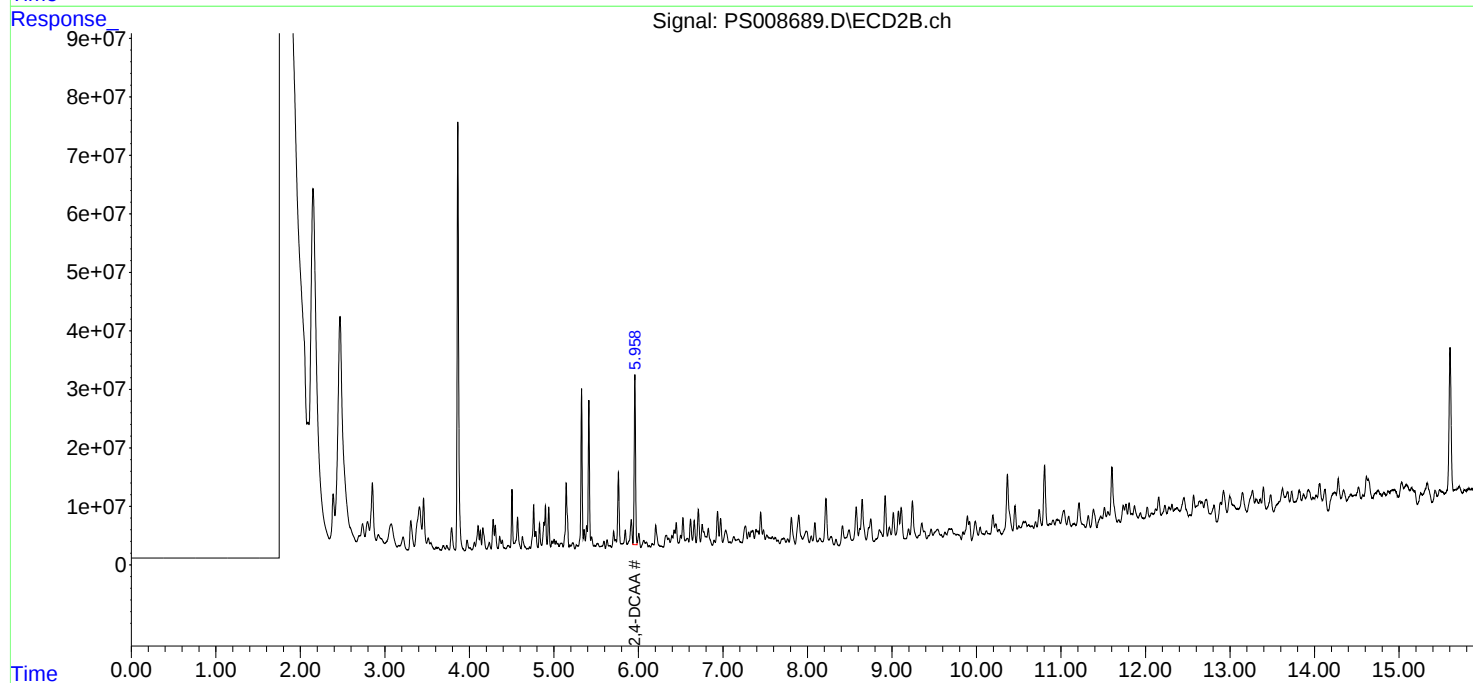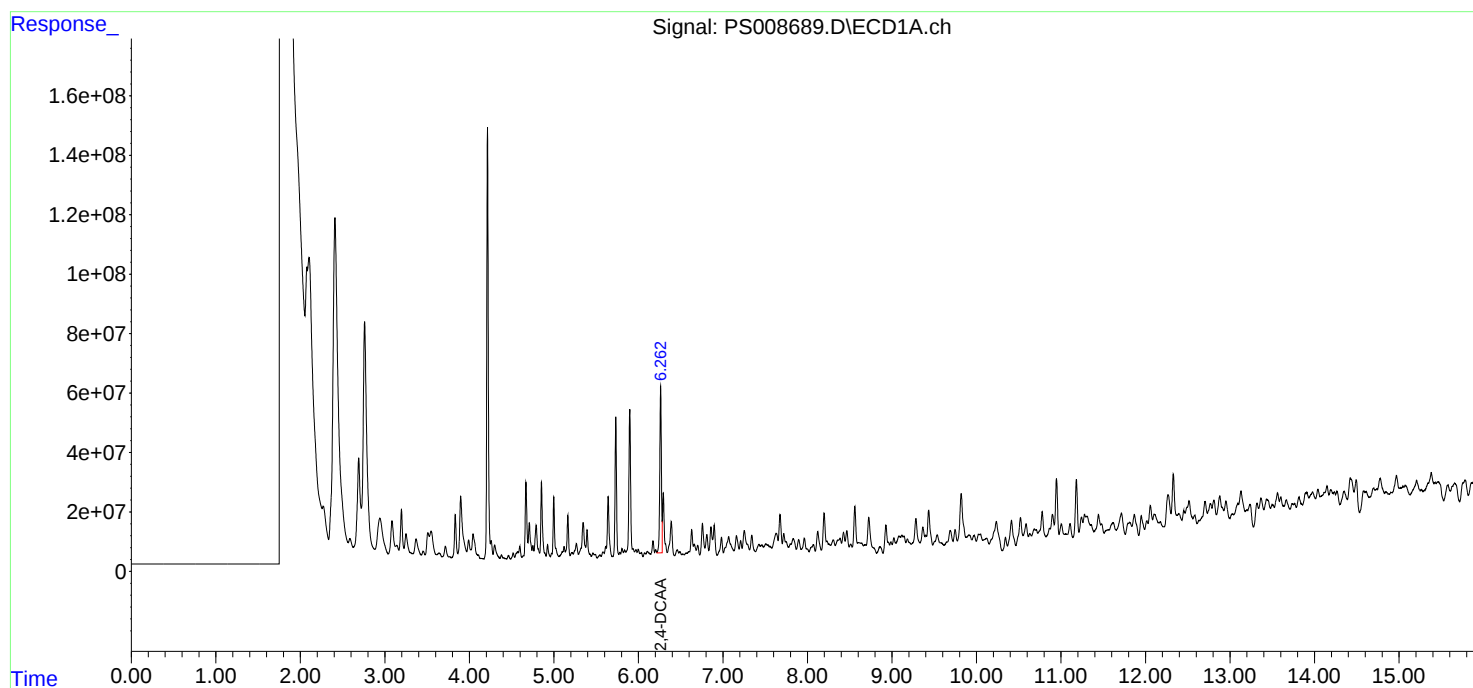

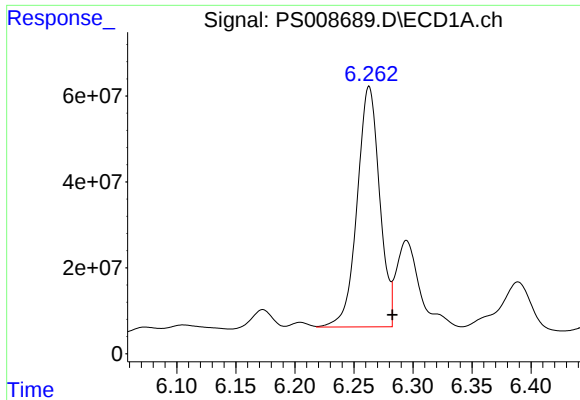


#4 2,4-DCAA

R.T.: 6.262 min
Delta R.T.: -0.020 min
Response: 739580570
Conc: 418.86 ng/ml m

Instrument :
ECD_S
ClientSampleId :
RAINEY-PARK-BH-02-A

Manual Integrations
APPROVED

mohammad
2/4/2020 12:34:26 PM

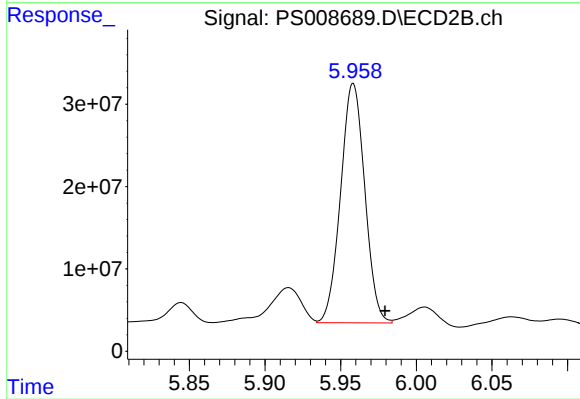

#4 2,4-DCAA

R.T.: 5.958 min
Delta R.T.: -0.021 min
Response: 323091751
Conc: 341.01 ng/ml m