

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013122\
 Data File : PS018166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2022 09:41
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:28:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) T	2,4-D	8.197f	0.000	7007801	0	3.848	N.D. #
11) T	2,4,5-TP ...	0.000	8.435f	0	17630155	N.D.	4.946
12) T	2,4,5-T	9.280	8.912f	17317467	7677345	1.954	2.347
13) T	2,4-DB	9.816	0.000	11897448	0	7.197	N.D. #
14) T	DINOSEB	11.027f	0.000	16651526	0	2.536	N.D. #
15) T	Picloram	10.800	10.670	97769478	59872013	8.191	12.804 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013122\
Data File : PS018166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2022 09:41
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:28:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

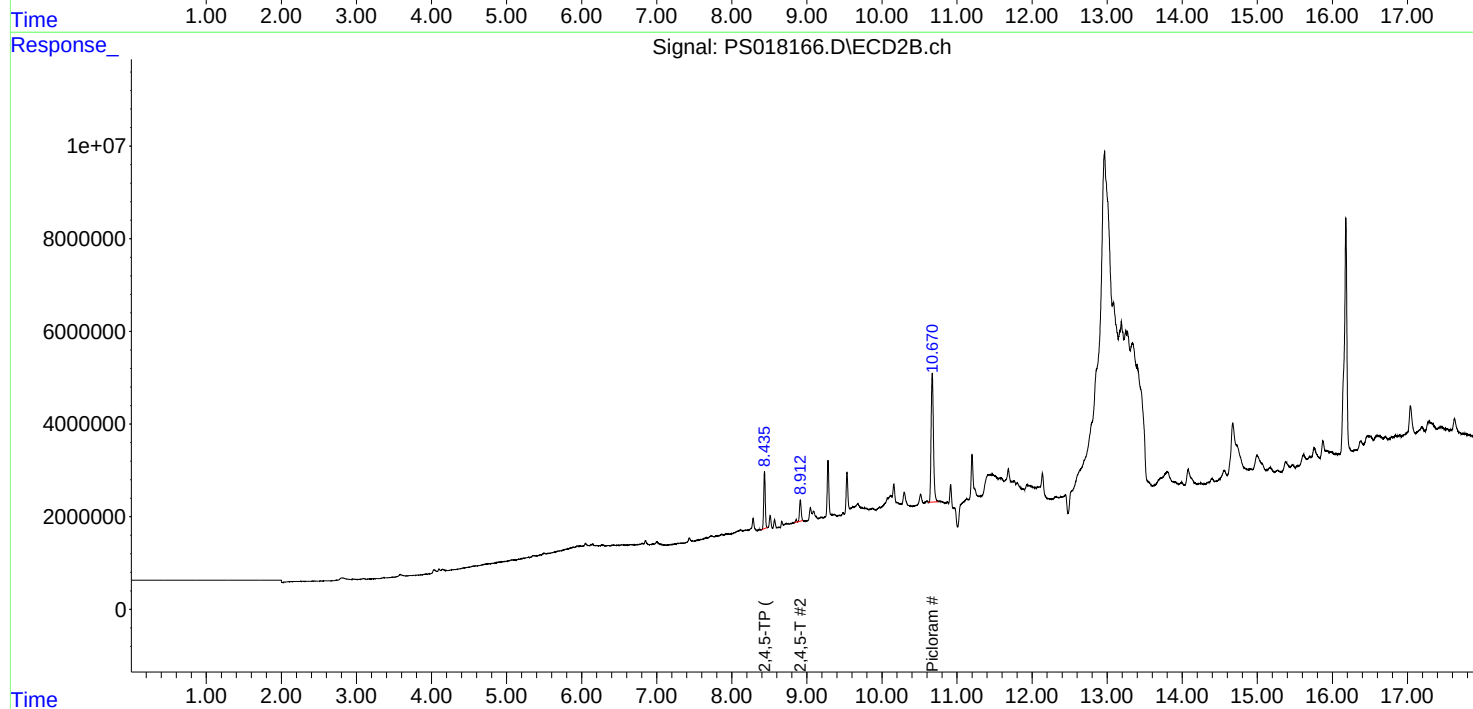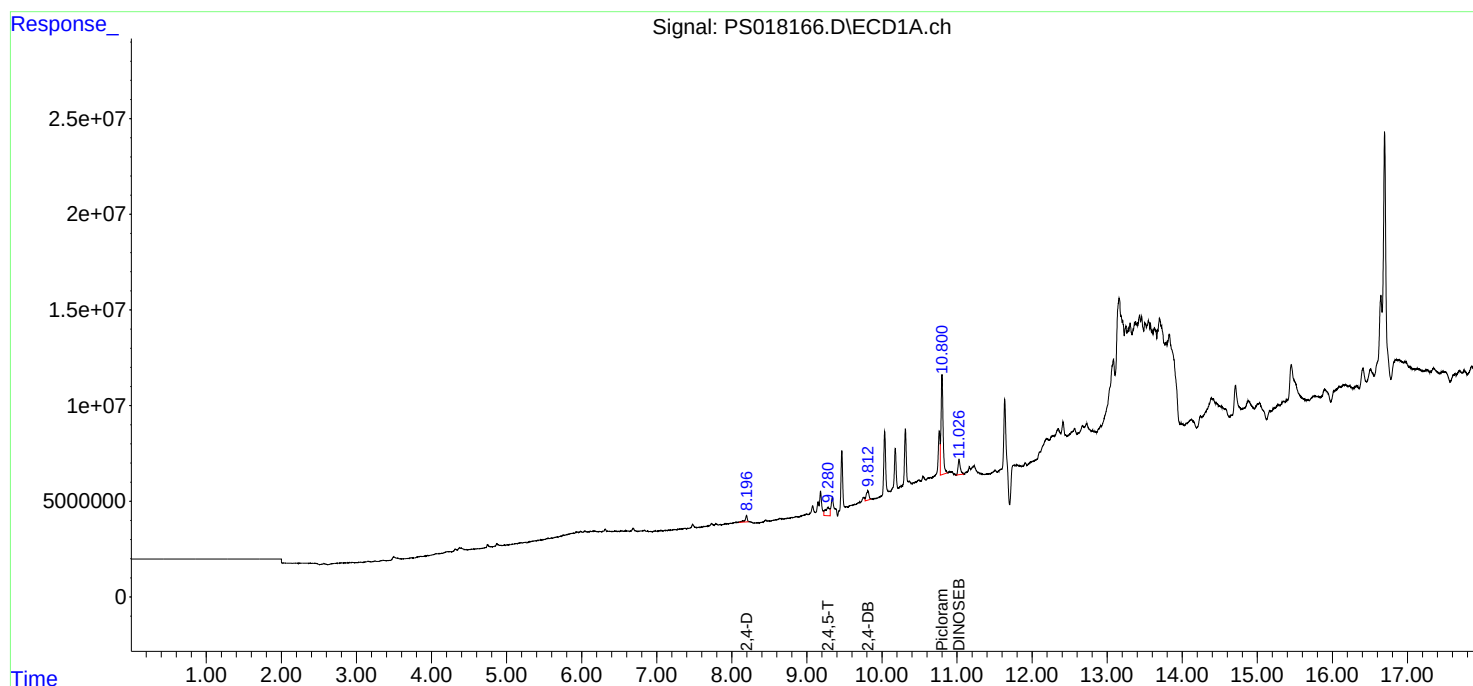


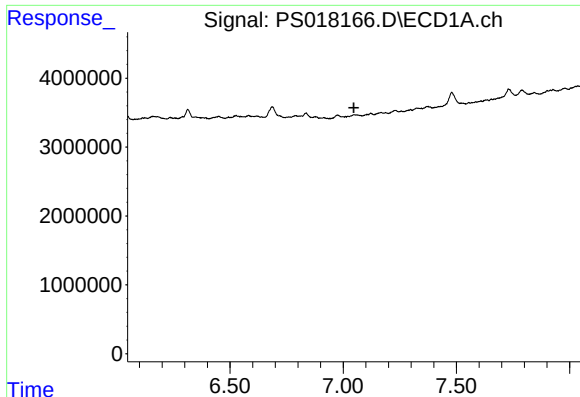

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

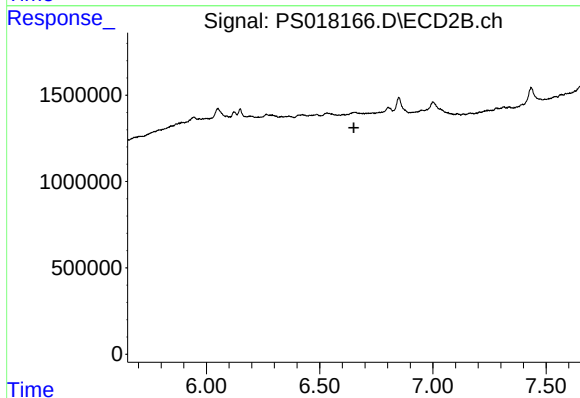


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

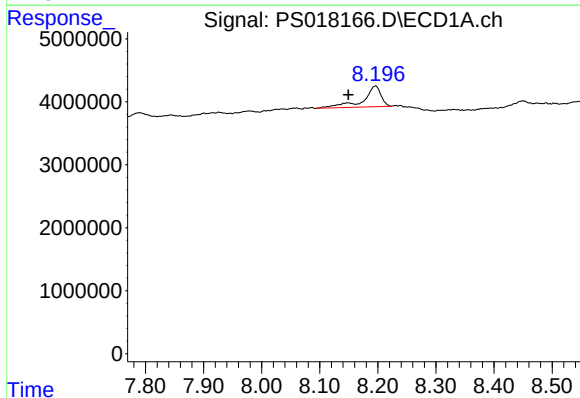


#9 2,4-D

R.T.: 8.197 min
Delta R.T.: 0.047 min
Response: 7007801
Conc: 3.85 ng/ml

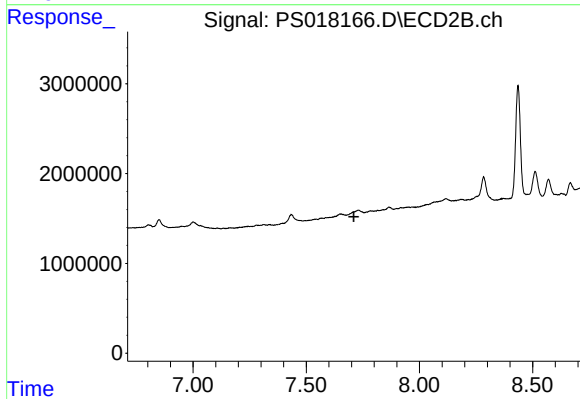

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.710 min
Response: 0
Conc: N.D.

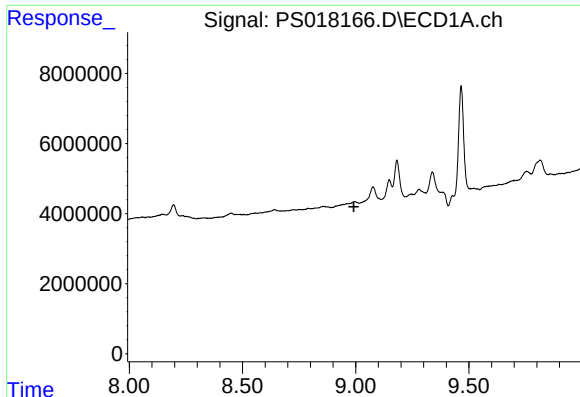

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

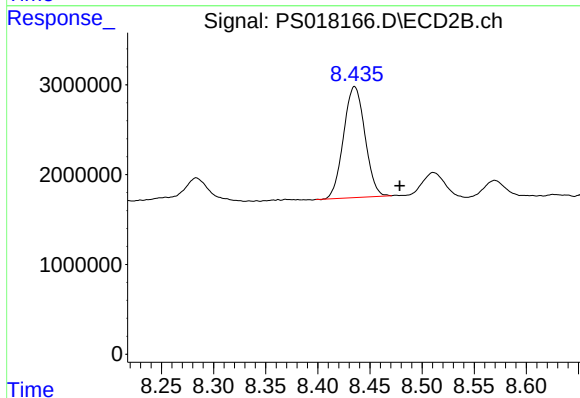


#11 2,4,5-TP (SILVEX)

R.T.: 8.435 min
Delta R.T.: -0.043 min
Response: 17630155
Conc: 4.95 ng/ml

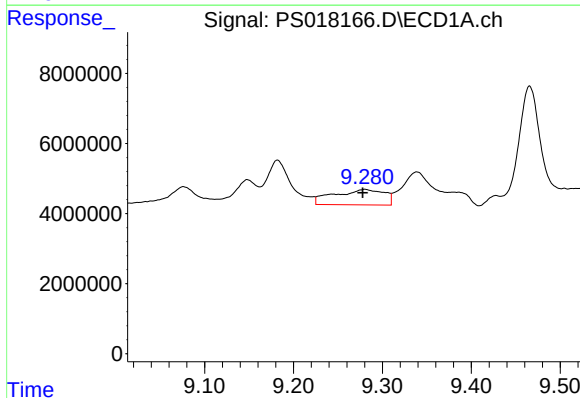


#12 2,4,5-T

R.T.: 9.280 min
Delta R.T.: 0.002 min
Response: 17317467
Conc: 1.95 ng/ml

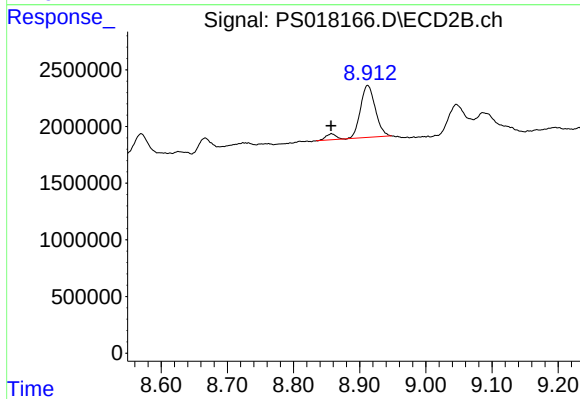

#12 2,4,5-T


R.T.: 8.912 min
Delta R.T.: 0.055 min
Response: 7677345
Conc: 2.35 ng/ml

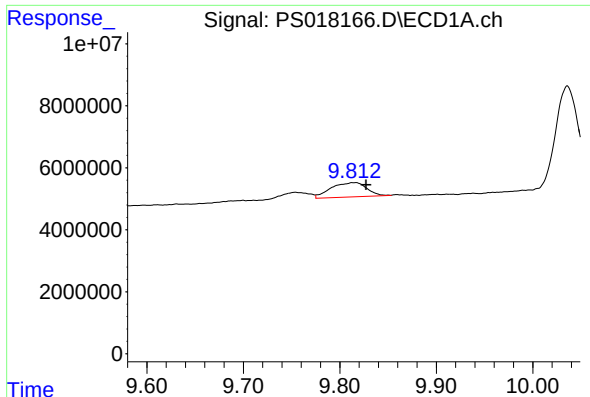

#13 2,4-DB


R.T.: 9.816 min
Delta R.T.: -0.011 min
Response: 11897448
Conc: 7.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

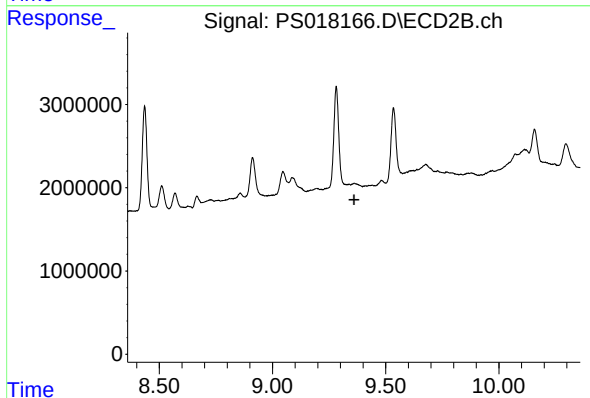


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

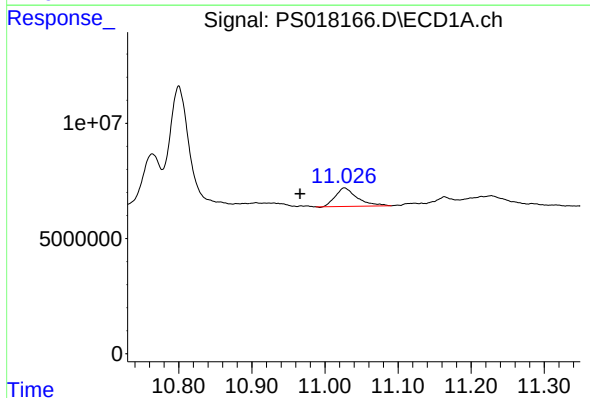


#14 DINOSEB

R.T.: 11.027 min
Delta R.T.: 0.061 min
Response: 16651526
Conc: 2.54 ng/ml

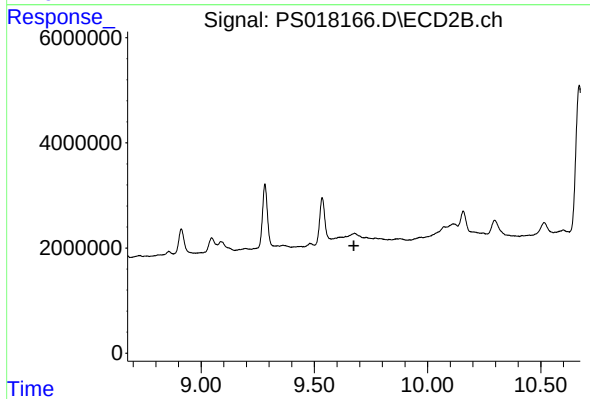

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

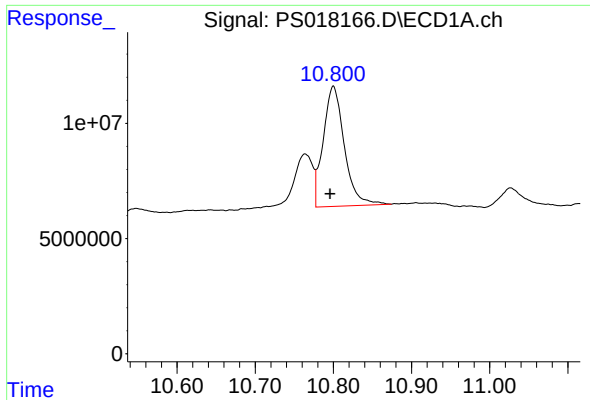

#15 Picloram

R.T.: 10.800 min
Delta R.T.: 0.004 min
Response: 97769478
Conc: 8.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

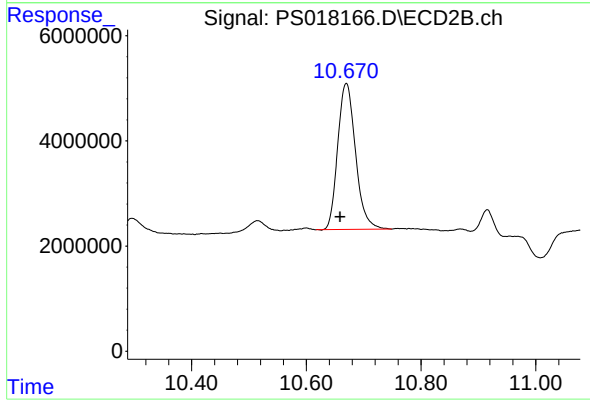

#15 Picloram

R.T.: 10.670 min
Delta R.T.: 0.011 min
Response: 59872013
Conc: 12.80 ng/ml