

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013122\
 Data File : PS018167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2022 10:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:29:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.045	6.651	622.3E6	304.8E6	430.485	525.295
Target Compounds							
9) T	2,4-D	8.212f	0.000	2599358	0	1.427	N.D. #
11) T	2,4,5-TP ...	0.000	8.450	0	8317657	N.D.	2.333
12) T	2,4,5-T	9.209f	0.000	7144041	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.292f	0	8304781	N.D.	18.770
15) T	Picloram	10.775	10.719f	8971338	19641834	<MDL	4.200 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013122\
Data File : PS018167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2022 10:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:29:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

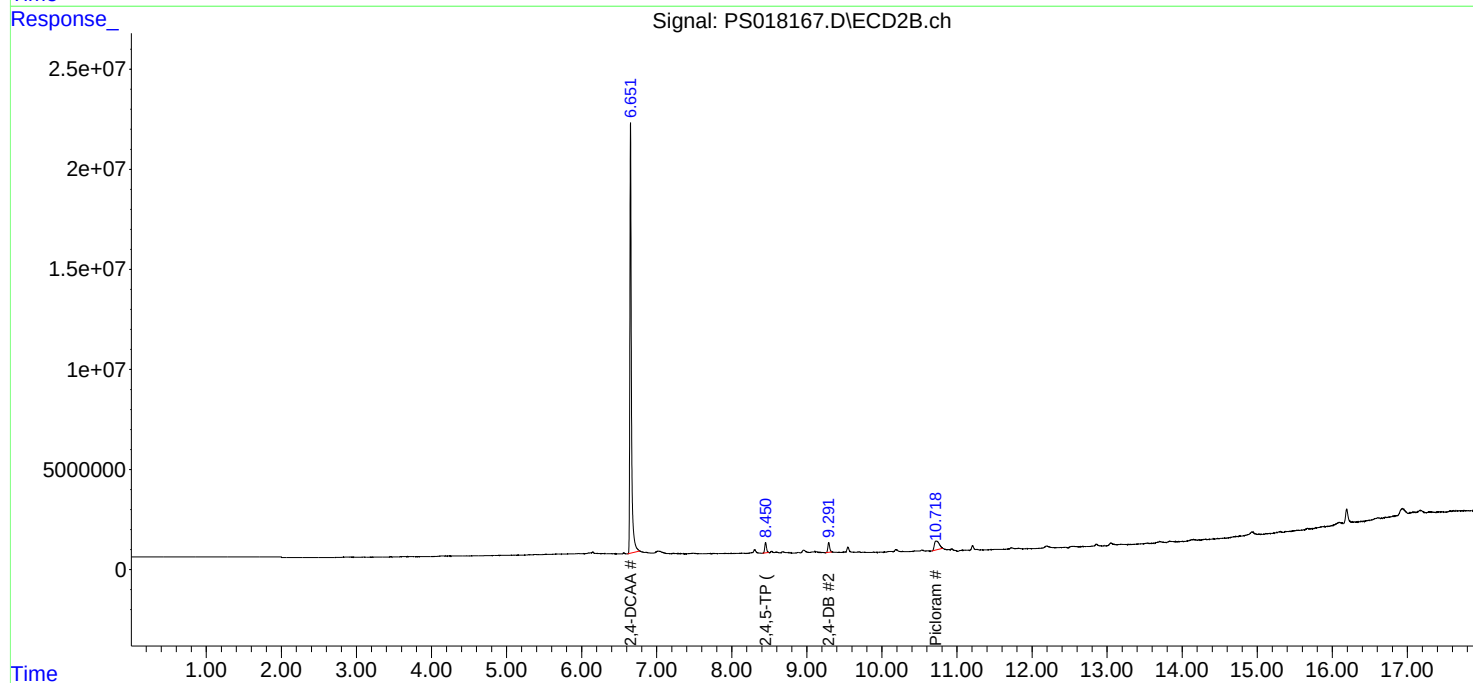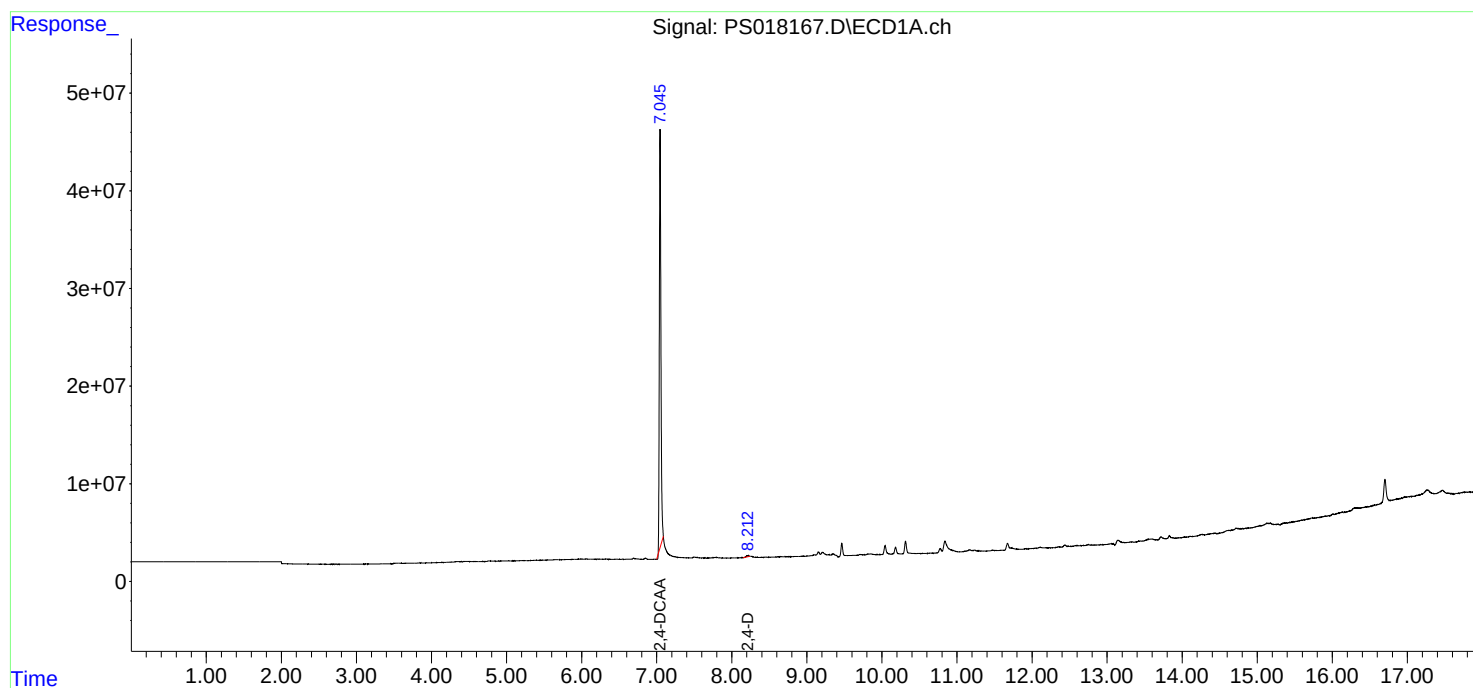


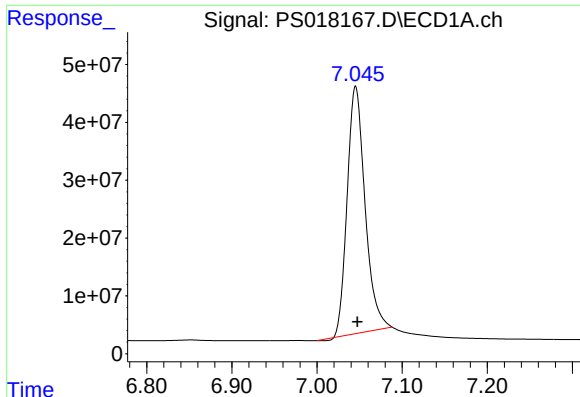

#4 2,4-DCAA


R.T.: 7.045 min
Delta R.T.: -0.002 min
Response: 622261502
Conc: 430.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

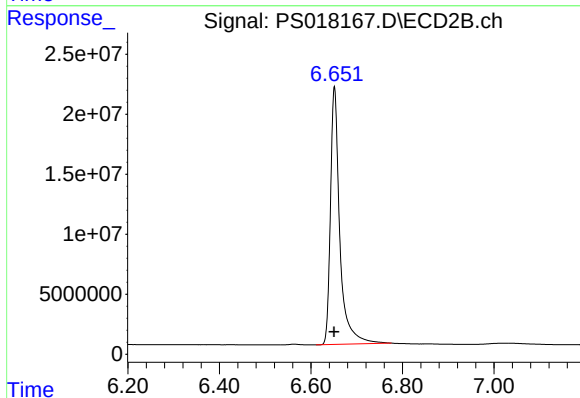


#4 2,4-DCAA

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 304801752
Conc: 525.29 ng/ml

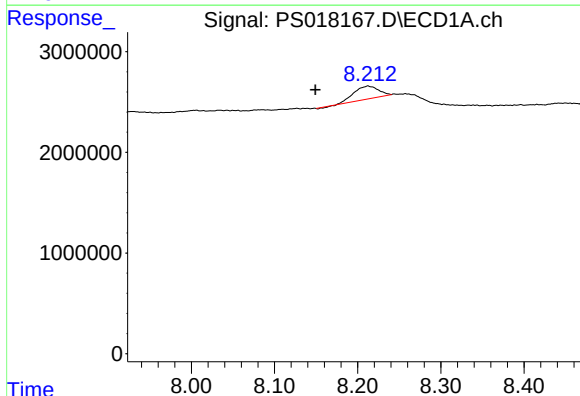


#9 2,4-D

R.T.: 8.212 min
Delta R.T.: 0.063 min
Response: 2599358
Conc: 1.43 ng/ml

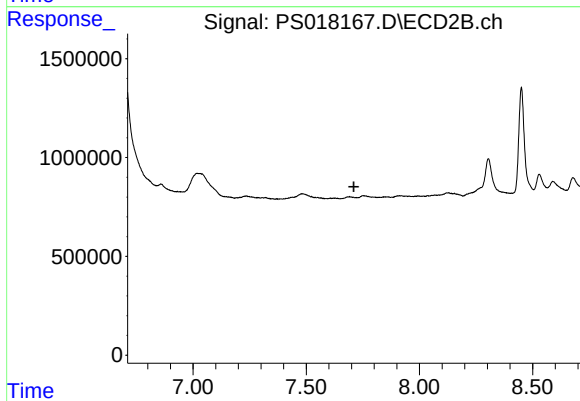

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

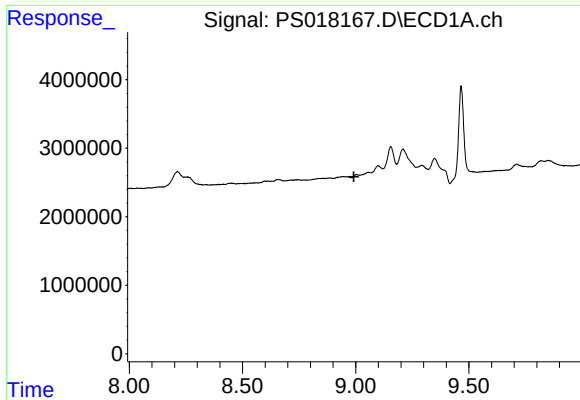

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

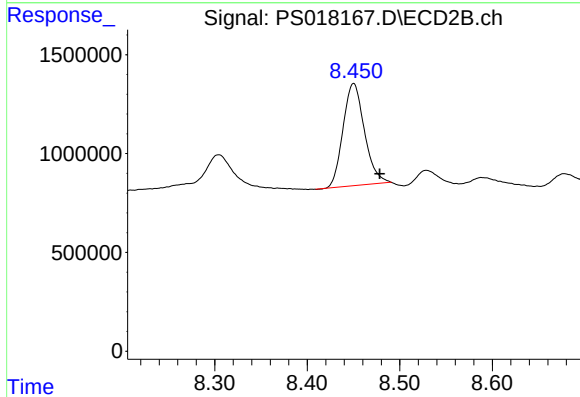


#11 2,4,5-TP (SILVEX)

R.T.: 8.450 min
Delta R.T.: -0.028 min
Response: 8317657
Conc: 2.33 ng/ml

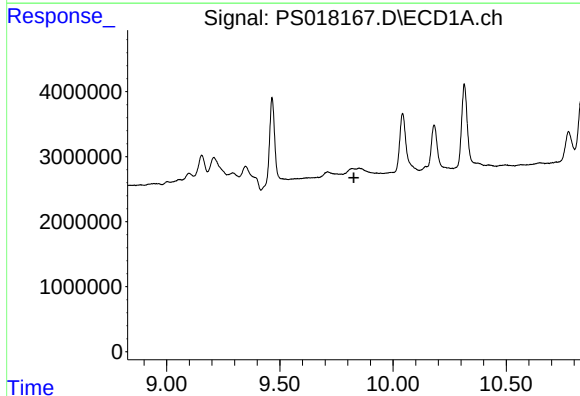


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.827 min
Response: 0
Conc: N.D.

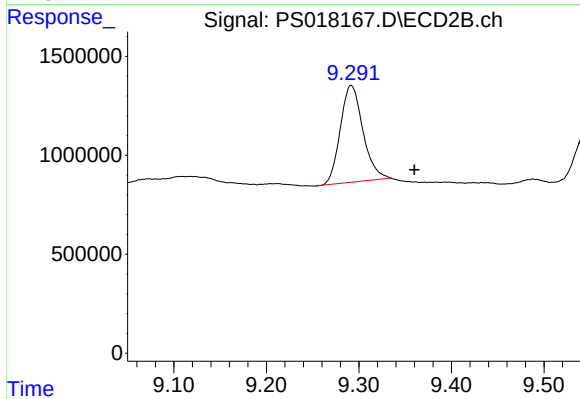

#13 2,4-DB


R.T.: 9.292 min
Delta R.T.: -0.068 min
Response: 8304781
Conc: 18.77 ng/ml

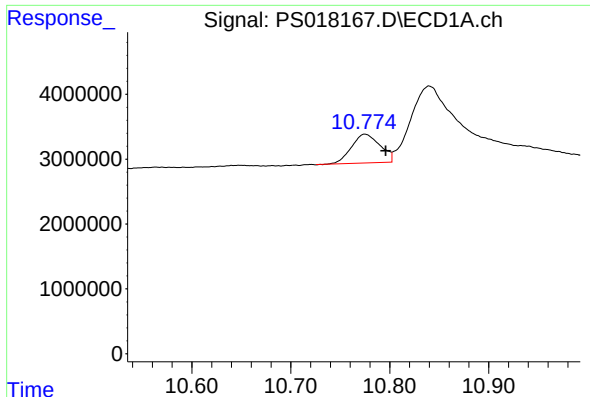

#15 Picloram

R.T.: 10.775 min
Delta R.T.: -0.021 min
Response: 8971338
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

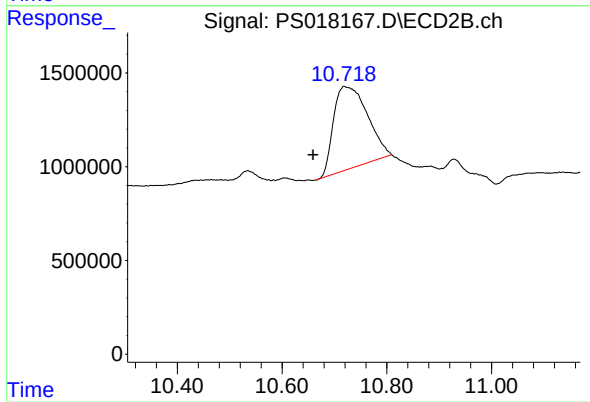

#15 Picloram

R.T.: 10.719 min
Delta R.T.: 0.060 min
Response: 19641834
Conc: 4.20 ng/ml