

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013123\
 Data File : PS021946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2023 16:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 20:37:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.386	6.817	1255.3E6	1172.0E6	450.969	652.326 #
Target Compounds							
1) T	Dalapon	2.516	0.000	517420	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.755	0.000	2288538	0	<MDL	N.D. #
3) T	4-Nitroph...	6.245	0.000	7499494	0	5.145	N.D. #
7) T	MCPA	0.000	7.250	0	16046437	N.D.	1.769
9) T	2,4-D	7.387f	0.000	39607967	0	10.198	N.D. #
11) T	2,4,5-TP ...	8.066	0.000	621531	0	<MDL	N.D. #
12) T	2,4,5-T	8.316	0.000	882181	0	<MDL	N.D. #
14) T	DINOSEB	9.922	0.000	1974369	0	<MDL	N.D. #
15) T	Picloram	9.779f	10.827	1188300	5082351	<MDL	<MDL #
16) T	DCPA	10.178	10.827	1345258	5082351	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013123\
Data File : PS021946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2023 16:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 20:37:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

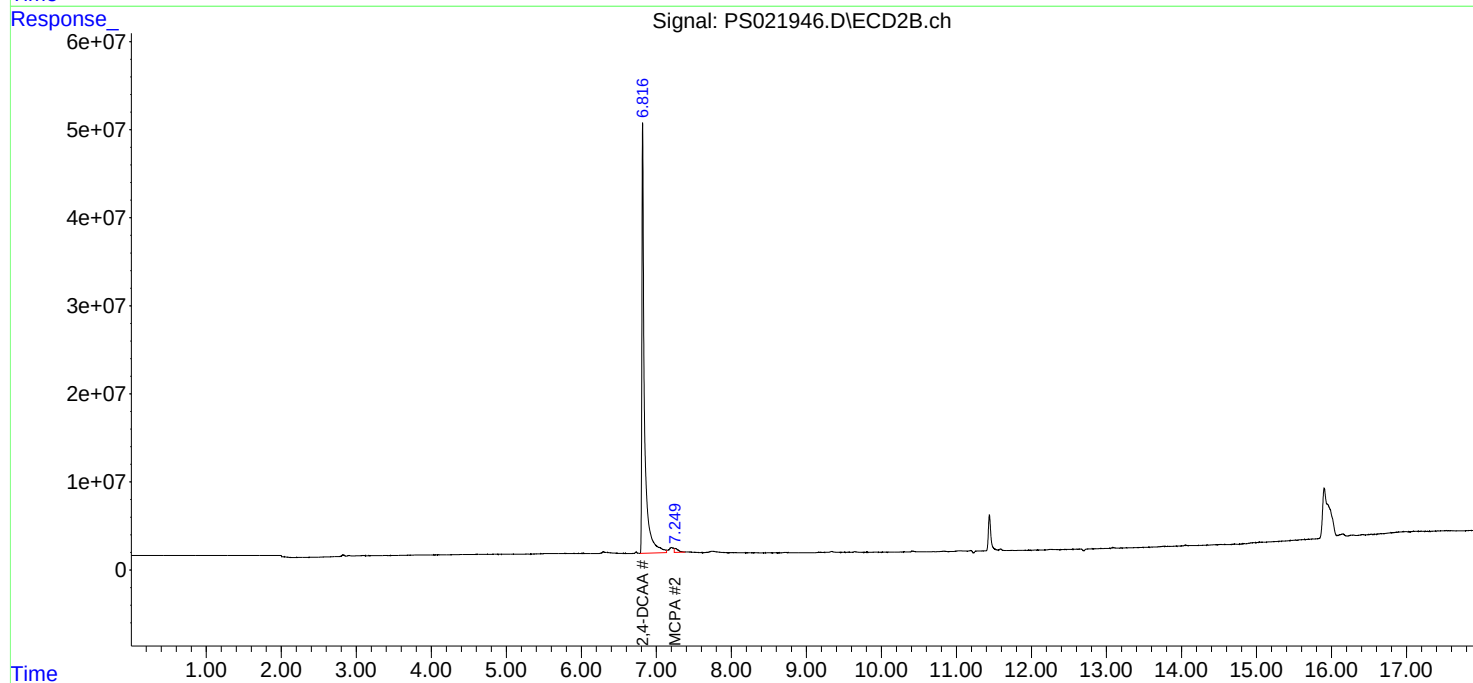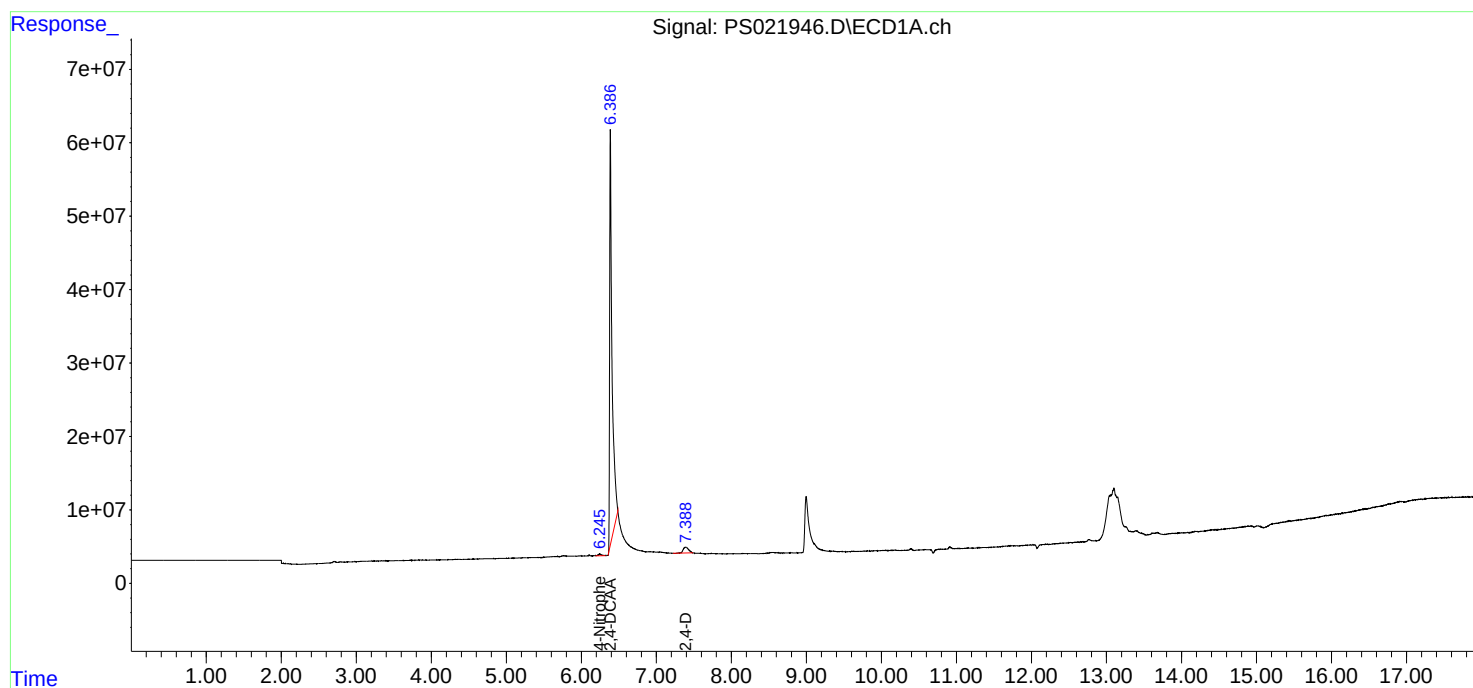


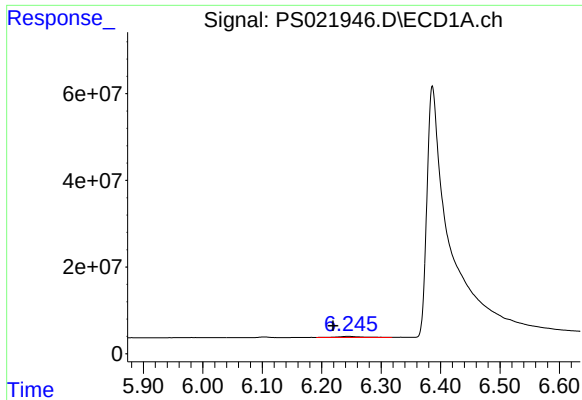

#3 4-Nitrophenol


R.T.: 6.245 min
Delta R.T.: 0.025 min
Response: 7499494
Conc: 5.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

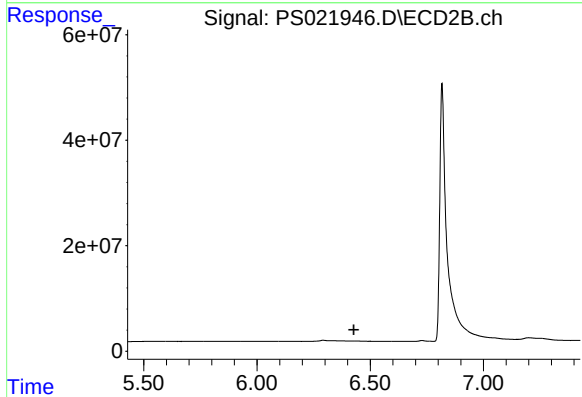


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

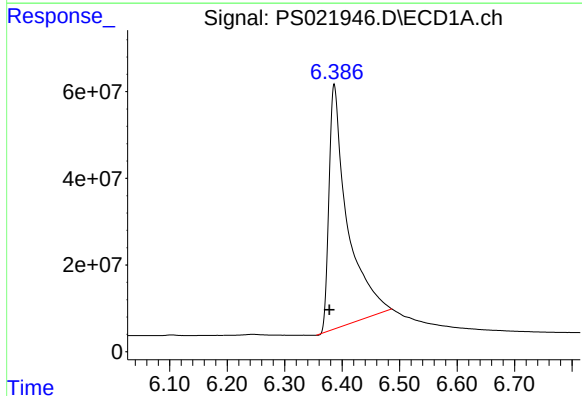


#4 2,4-DCAA

R.T.: 6.386 min
Delta R.T.: 0.009 min
Response: 1255302336
Conc: 450.97 ng/ml

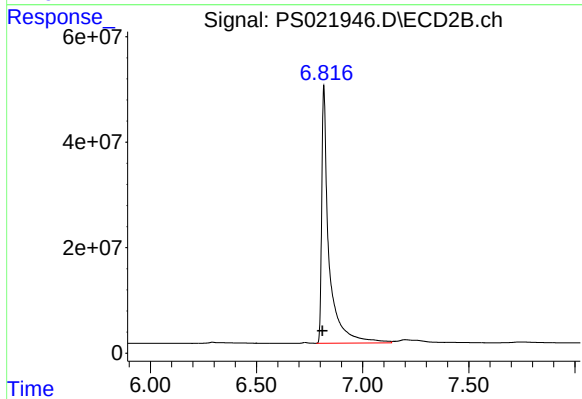

#4 2,4-DCAA


R.T.: 6.817 min
Delta R.T.: 0.006 min
Response: 1172027039
Conc: 652.33 ng/ml

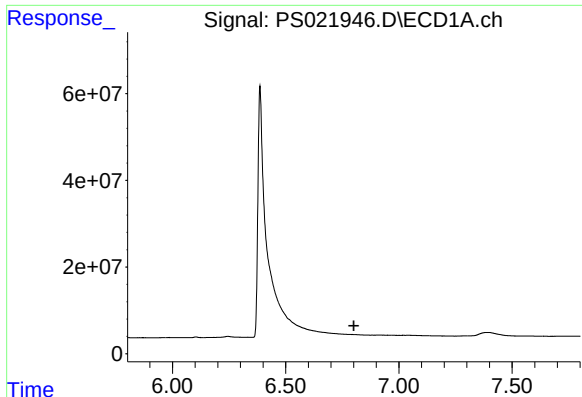

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

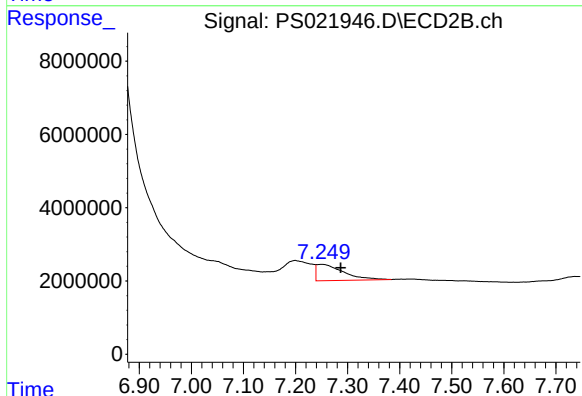


#7 MCPA

R.T.: 7.250 min
Delta R.T.: -0.037 min
Response: 16046437
Conc: 1.77 ug/ml

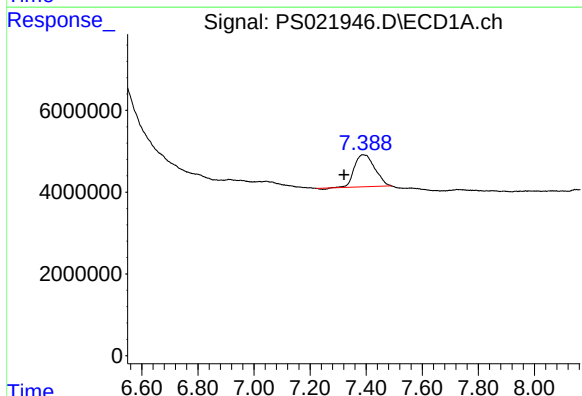

#9 2,4-D

R.T.: 7.387 min
Delta R.T.: 0.066 min
Response: 39607967
Conc: 10.20 ng/ml

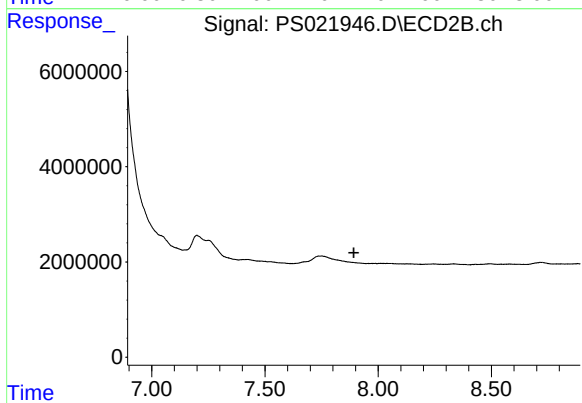

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.893 min
Response: 0
Conc: N.D.