

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013124\
 Data File : PS025687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2024 09:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 21:36:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.558	0	635083	<MDL
5) T	DICAMBA	0.000	6.955	0	594.2E6	178.558
6) T	MCP	0.000	6.955f	0	594.2E6	256.151
7) T	MCPA	0.000	7.155f	0	9846766	2.842
8) T	DICHLORPROP	7.075	7.557	-1806643	6407927	7.413
9) T	2,4-D	7.238	7.846	1352.7E6	1802626	1.984 #
10) T	Pentachlo...	0.000	8.236	0	87963	<MDL
11) T	2,4,5-TP ...	0.000	8.548f	0	391373	<MDL
14) T	DINOSEB	0.000	9.768	0	1664768	<MDL
15) T	Picloram	9.646	10.765	155.8E6	20103912	3.781 #
16) T	DCPA	0.000	10.721	0	6461289	1.111



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013124\
Data File : PS025687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2024 09:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 21:36:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

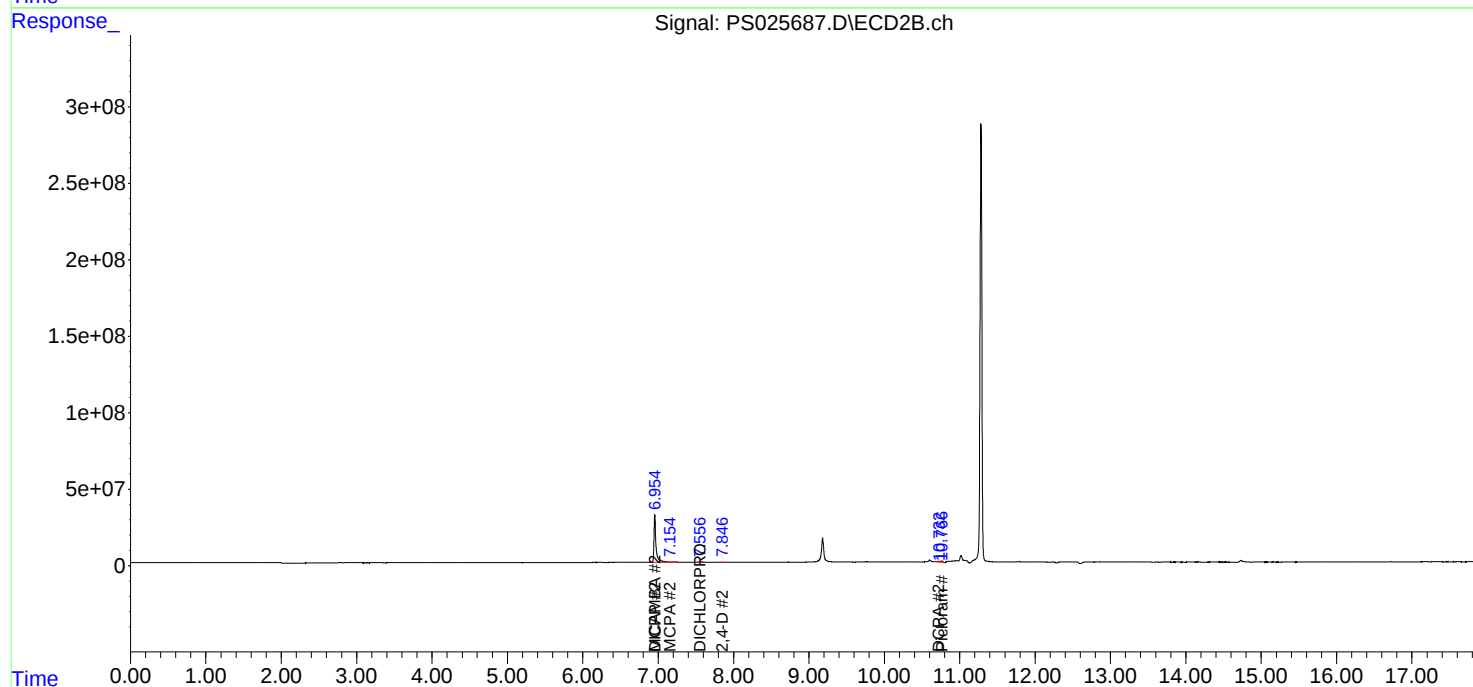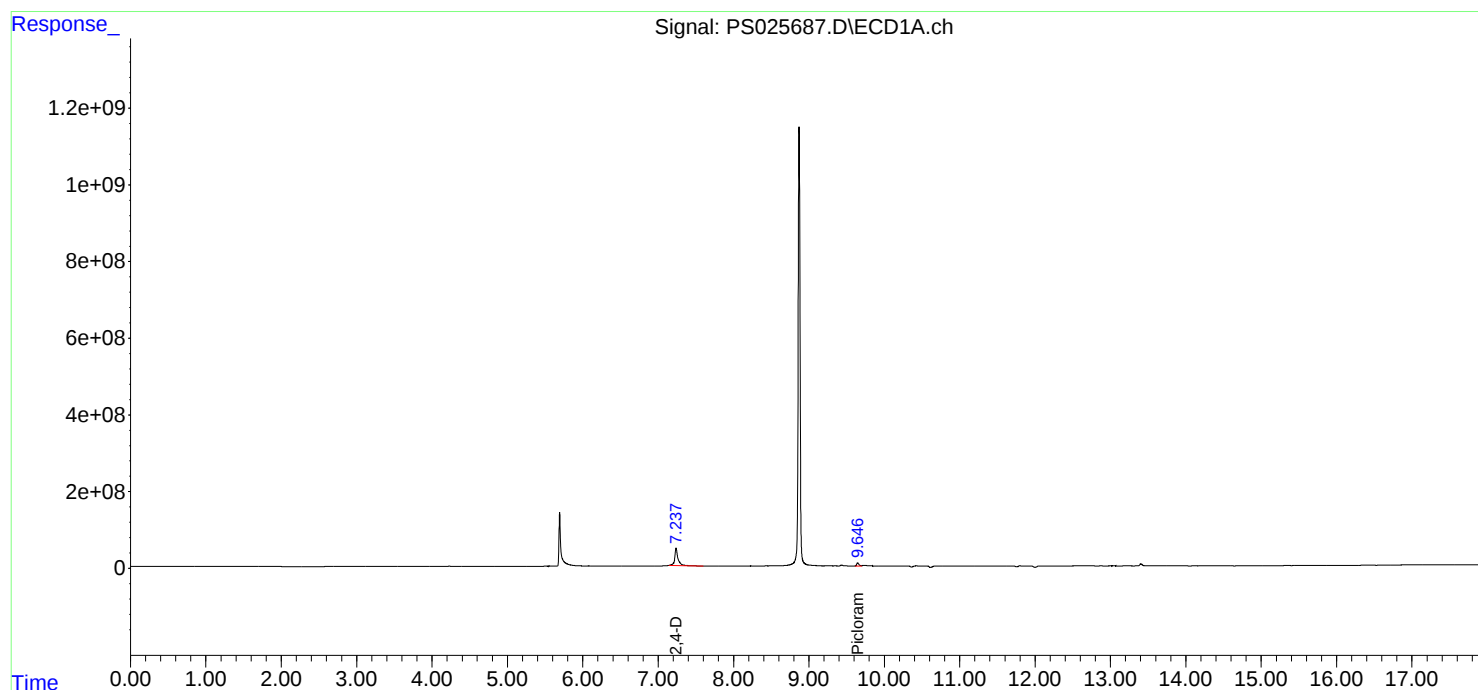


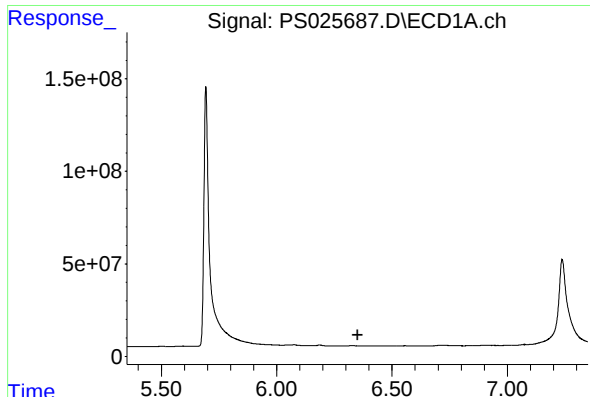

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

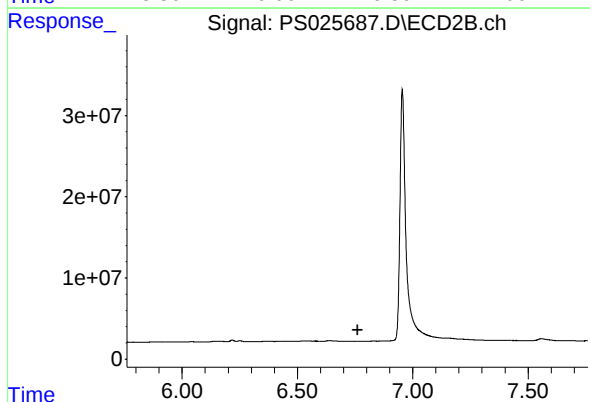


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.761 min
Response: 0
Conc: N.D.

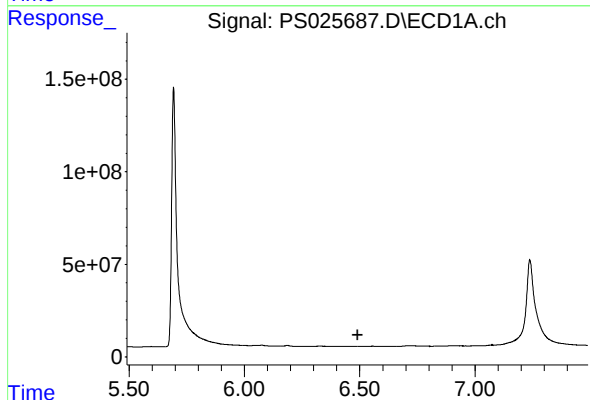


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

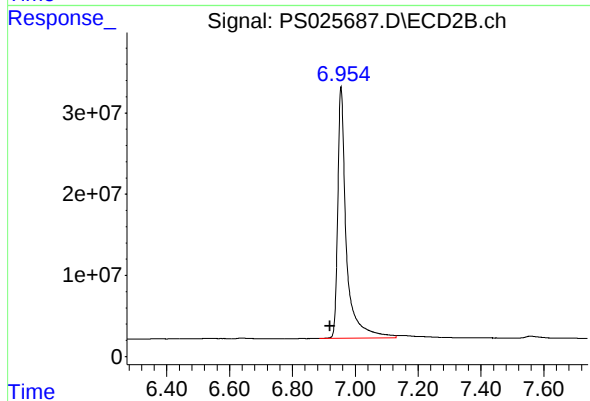

#5 DICAMBA


R.T.: 6.955 min
Delta R.T.: 0.035 min
Response: 594225237
Conc: 178.56 ng/ml

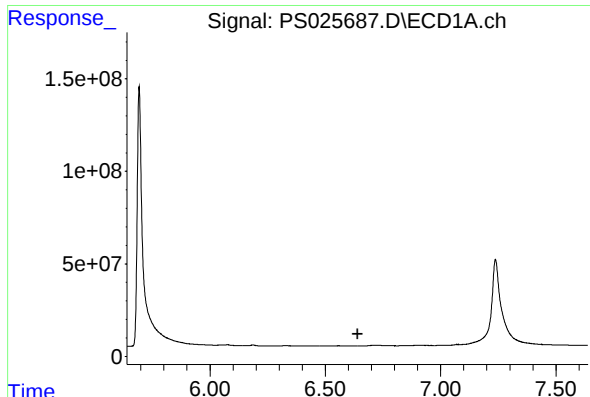

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

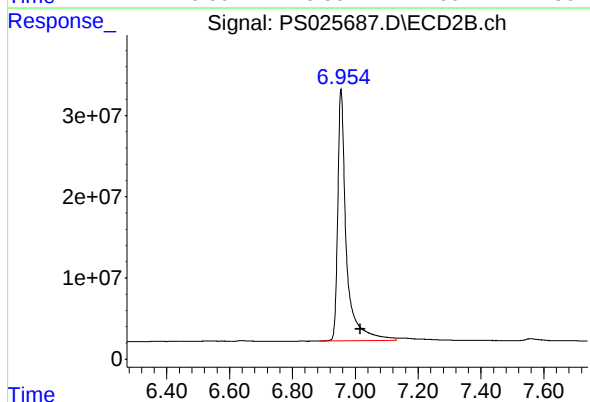


#6 MCPP

R.T.: 6.955 min
Delta R.T.: -0.062 min
Response: 594225237
Conc: 256.15 ug/ml

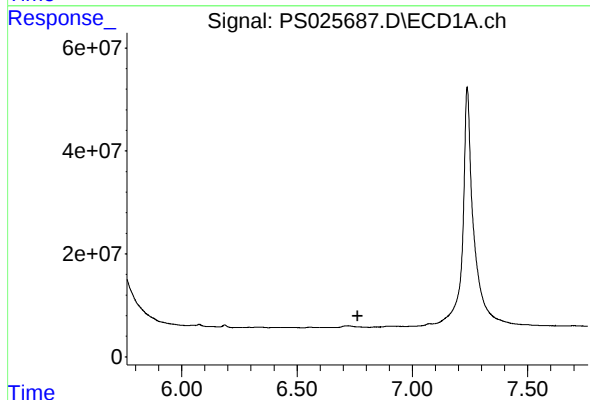


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

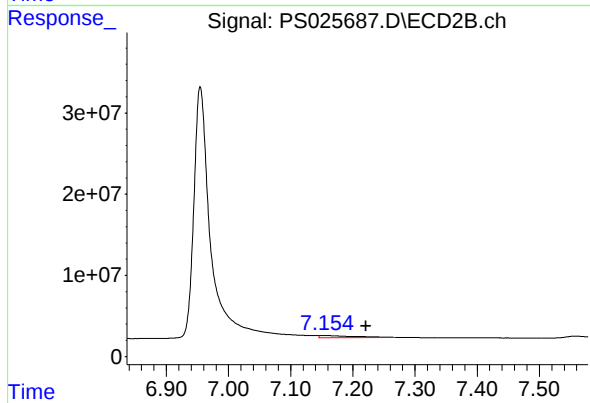

#7 MCPA


R.T.: 7.155 min
Delta R.T.: -0.066 min
Response: 9846766
Conc: 2.84 ug/ml

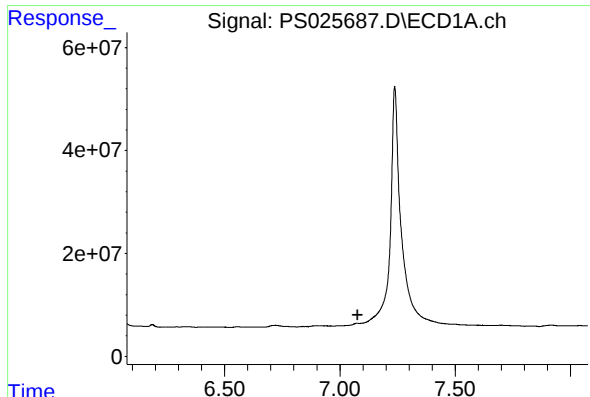

#8 DICHLORPROP


R.T.: 7.075 min
Delta R.T.: -0.001 min
Response: -1806643
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

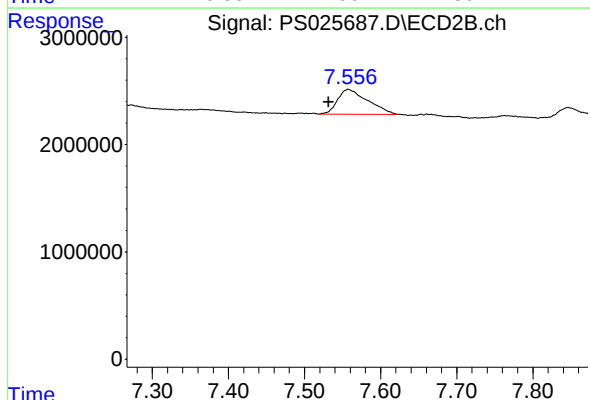


#8 DICHLORPROP

R.T.: 7.557 min
Delta R.T.: 0.025 min
Response: 6407927
Conc: 7.41 ng/ml

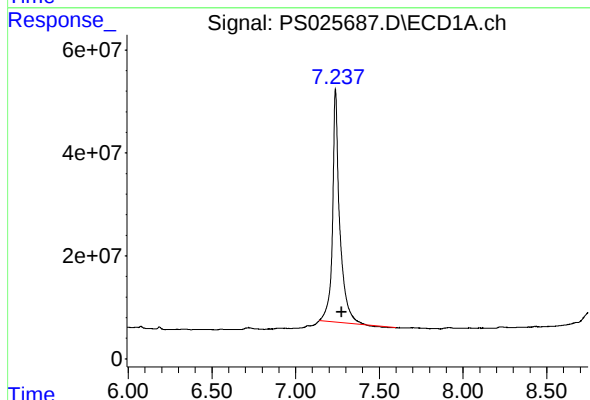


#9 2,4-D

R.T.: 7.238 min
Delta R.T.: -0.038 min
Response: 1352651179
Conc: 734.60 ng/ml

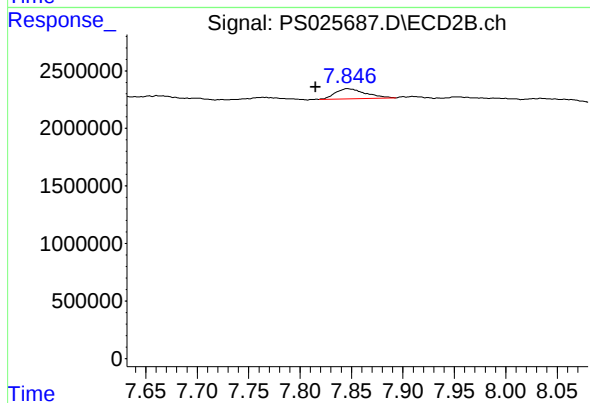

#9 2,4-D


R.T.: 7.846 min
Delta R.T.: 0.031 min
Response: 1802626
Conc: 1.98 ng/ml

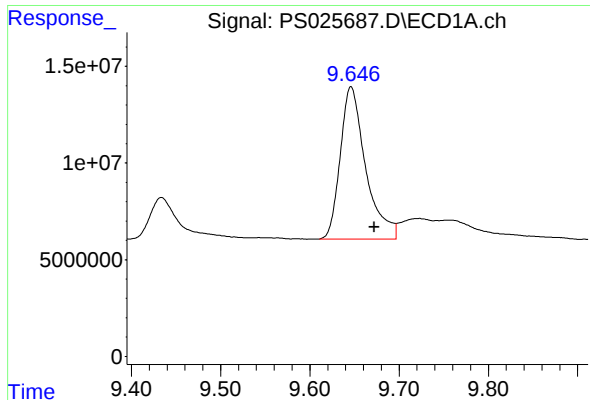

#15 Picloram


R.T.: 9.646 min
Delta R.T.: -0.026 min
Response: 155811242
Conc: 15.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

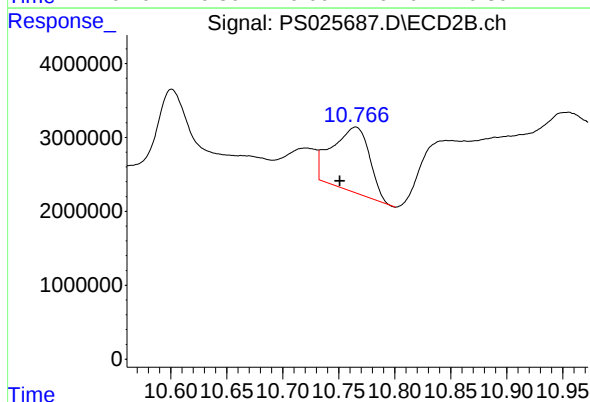


#15 Picloram

R.T.: 10.765 min
Delta R.T.: 0.014 min
Response: 20103912
Conc: 3.78 ng/ml

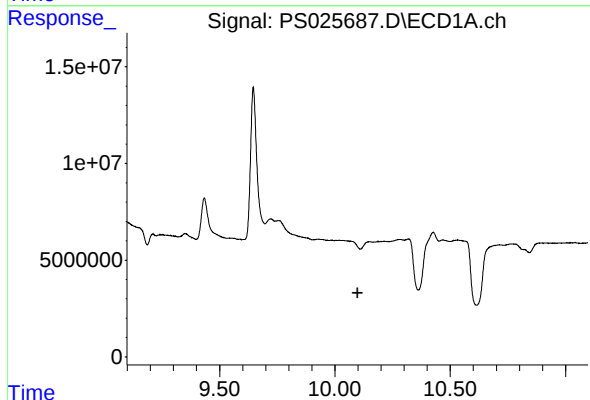

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.098 min
Response: 0
Conc: N.D.

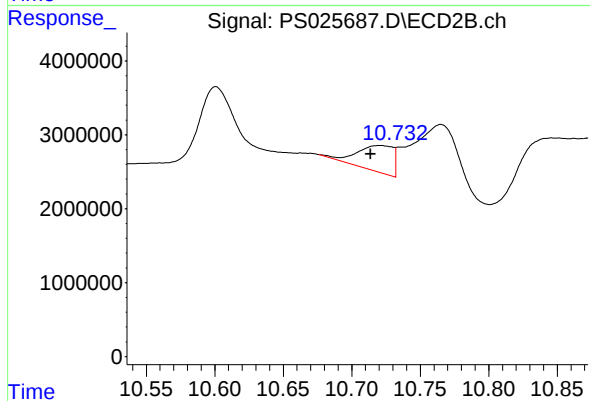

#16 DCPA

R.T.: 10.721 min
Delta R.T.: 0.007 min
Response: 6461289
Conc: 1.11 ng/ml