

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013125\
 Data File : PS029006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2025 10:23
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:25:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 14 12:25:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	0.000	279204	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.617	0.000	674200	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.356	0.000	16617528	0	4.158	N.D. #
3) T	4-Nitroph...	6.980	0.000	10818002	0	6.105	N.D. #
5) T	DICAMBA	7.404	7.874	217385	4091357	<MDL	<MDL #
6) T	MCPD	7.559	7.962	-272273	9907180	N.D.	3.294
7) T	MCPA	7.721	0.000	197550	0	<MDL	N.D. #
8) T	DICHLORPROP	8.114f	8.627f	1164651	8075155	<MDL	5.745 #
9) T	2,4-D	8.332	0.000	27964282	0	8.275	N.D. #
10) T	Pentachlo...	8.610	0.000	234003	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.165	0.000	1232994	0	<MDL	N.D. #
12) T	2,4,5-T	9.485	10.224	-367332	3226989	N.D.	<MDL
13) T	2,4-DB	10.070	0.000	1248319	0	<MDL	N.D. #
14) T	DINOSEB	11.228f	0.000	5579219	0	<MDL	N.D. #
15) T	Picloram	11.077	12.255	96881268	30160951	3.071	2.248 #
16) T	DCPA	11.534	12.255f	5802912	30160951	<MDL	2.657 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013125\
Data File : PS029006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2025 10:23
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:25:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
Quant Title : 8080.M
QLast Update : Tue Jan 14 12:25:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

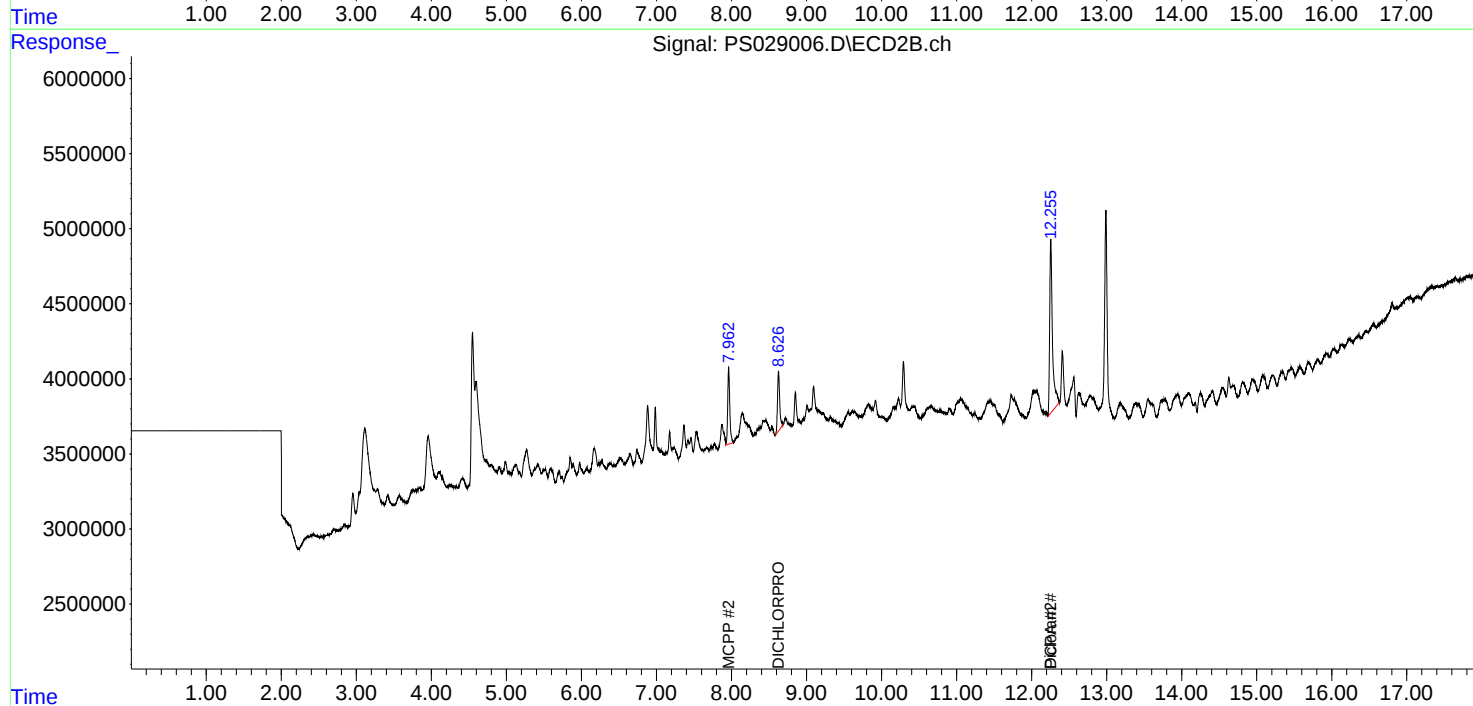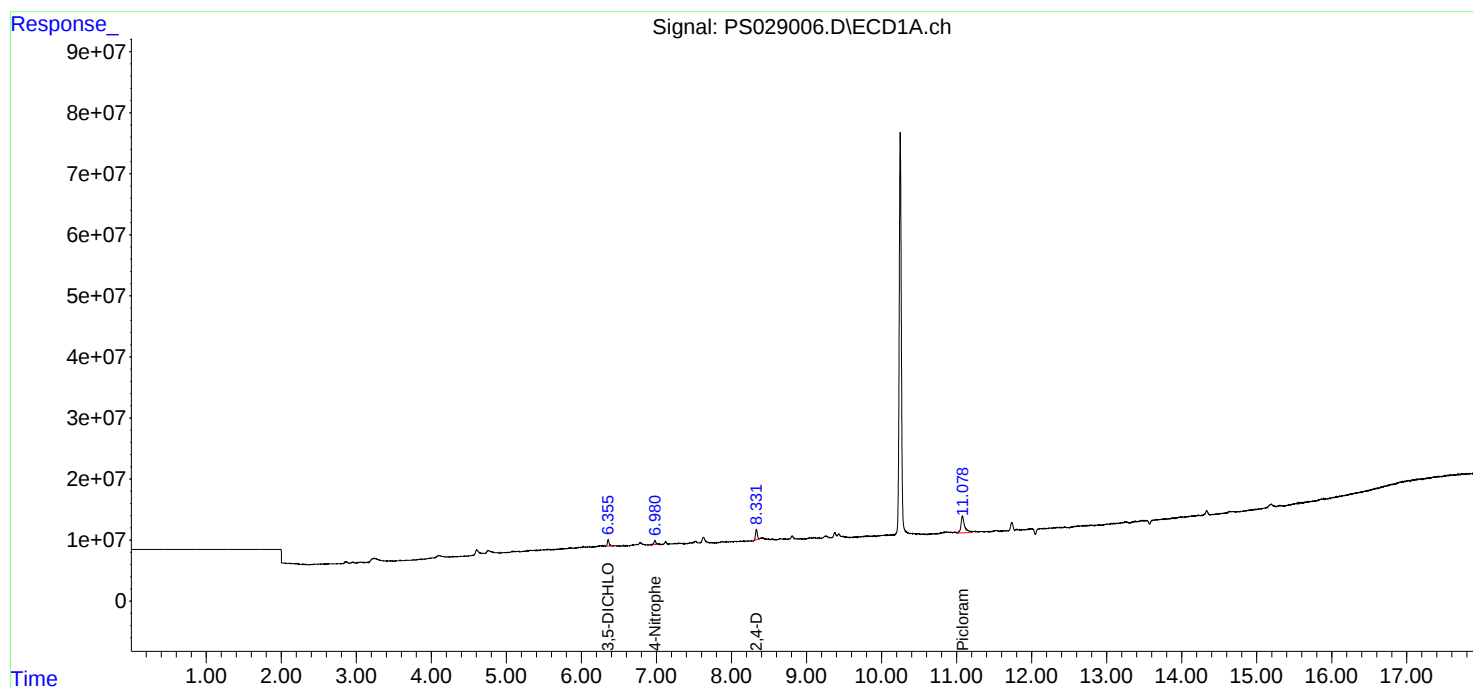


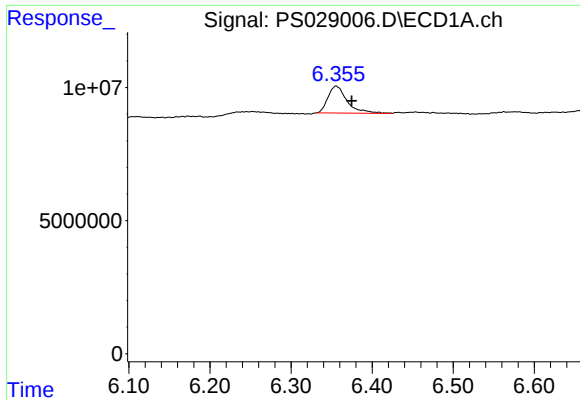

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.356 min
Delta R.T.: -0.019 min
Response: 16617528
Conc: 4.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

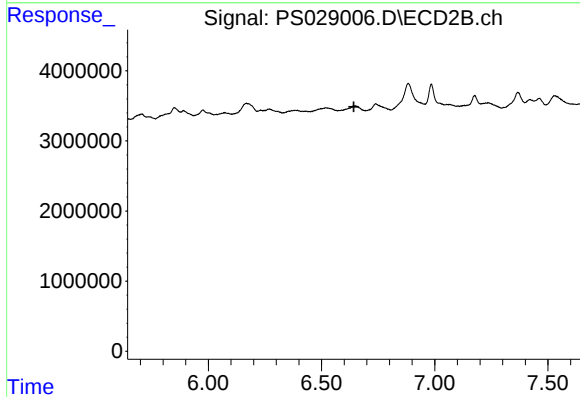


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

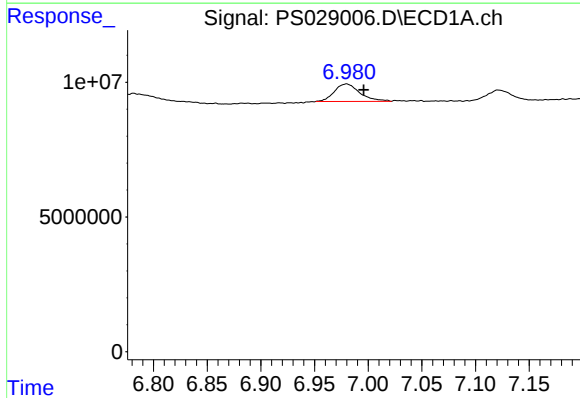


#3 4-Nitrophenol

R.T.: 6.980 min
Delta R.T.: -0.016 min
Response: 10818002
Conc: 6.10 ng/ml

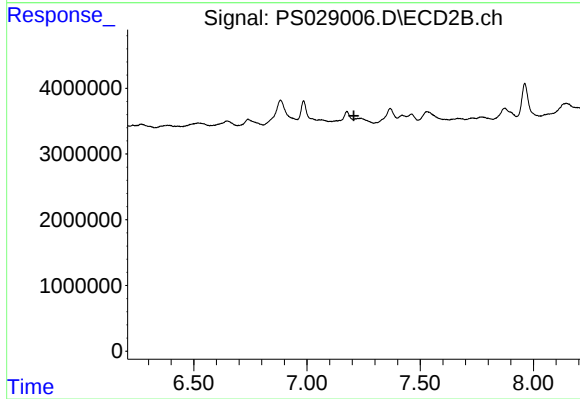

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

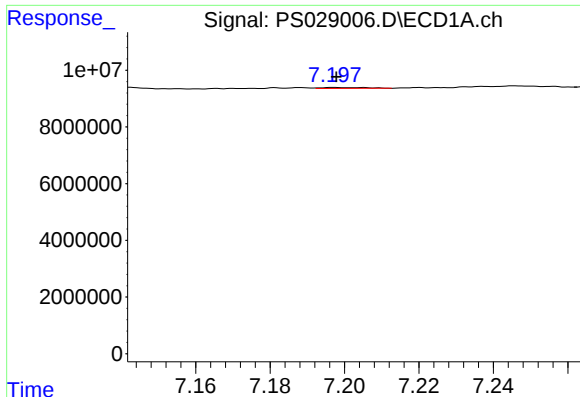

#4 2,4-DCAA


R.T.: 7.198 min
Delta R.T.: 0.000 min
Response: 279204
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

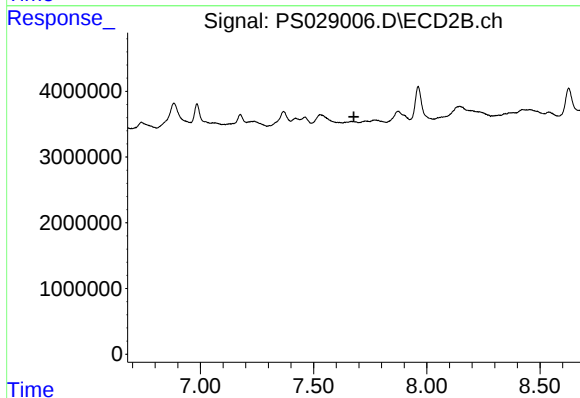


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.678 min
Response: 0
Conc: N.D.

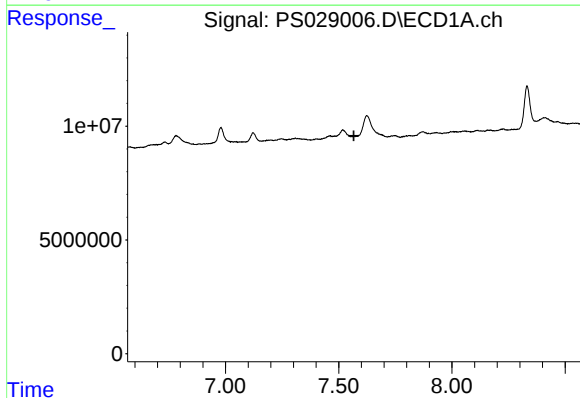


#6 MCPP

R.T.: 7.559 min
Delta R.T.: -0.008 min
Response: -272273
Conc: N.D.

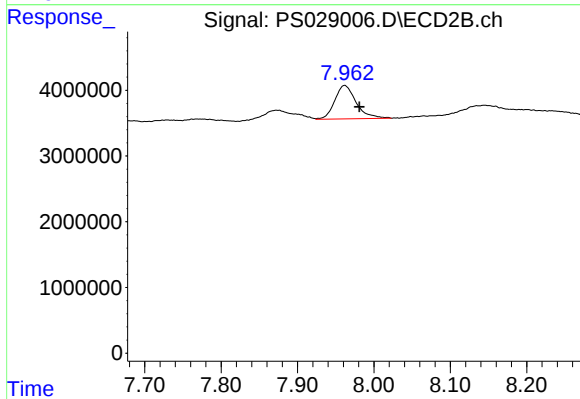

#6 MCPP


R.T.: 7.962 min
Delta R.T.: -0.019 min
Response: 9907180
Conc: 3.29 ug/ml

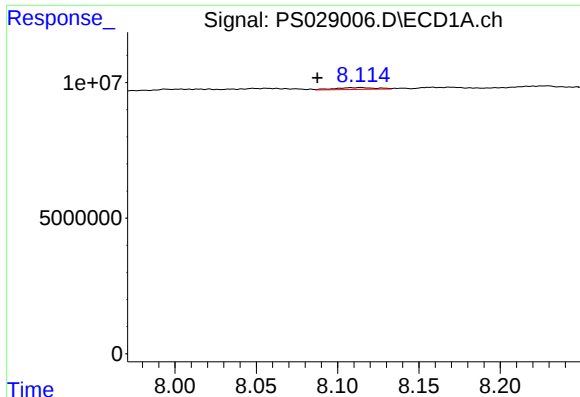

#8 DICHLORPROP


R.T.: 8.114 min
Delta R.T.: 0.027 min
Response: 1164651
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

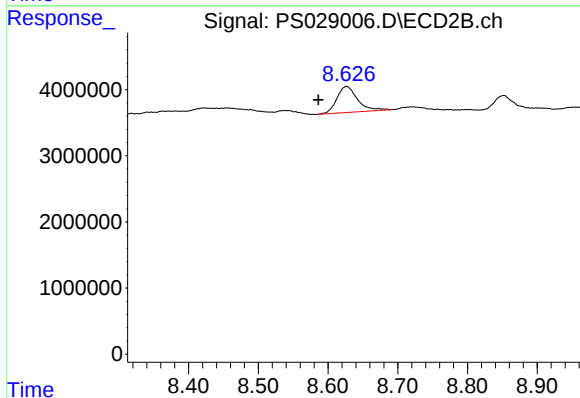


#8 DICHLORPROP

R.T.: 8.627 min
Delta R.T.: 0.040 min
Response: 8075155
Conc: 5.74 ng/ml

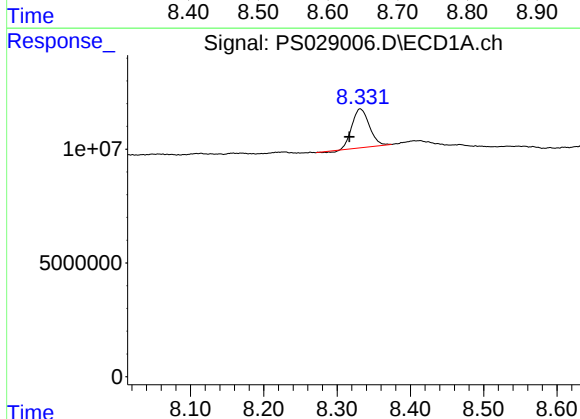


#9 2,4-D

R.T.: 8.332 min
Delta R.T.: 0.015 min
Response: 27964282
Conc: 8.27 ng/ml

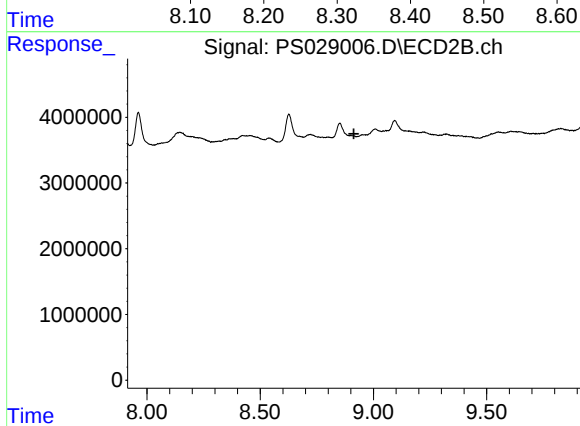

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.914 min
Response: 0
Conc: N.D.

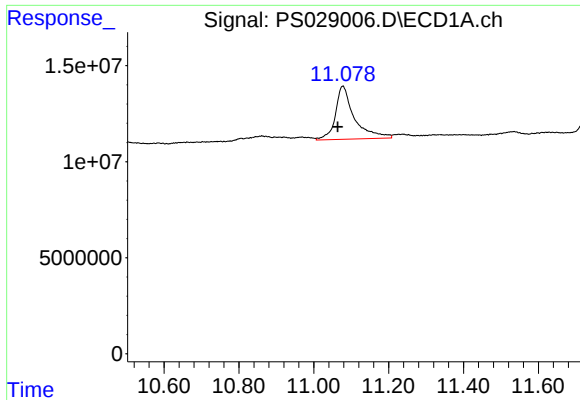

#15 Picloram


R.T.: 11.077 min
Delta R.T.: 0.013 min
Response: 96881268
Conc: 3.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

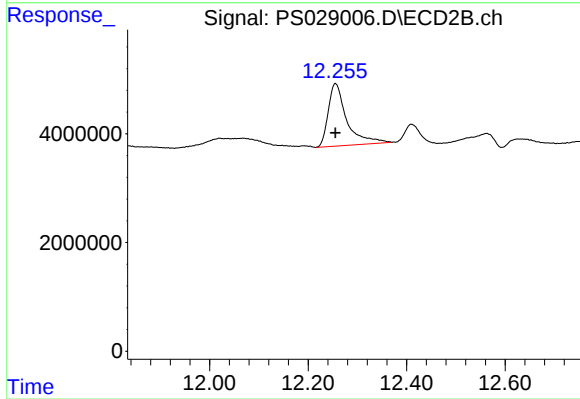


#15 Picloram

R.T.: 12.255 min
Delta R.T.: 0.000 min
Response: 30160951
Conc: 2.25 ng/ml

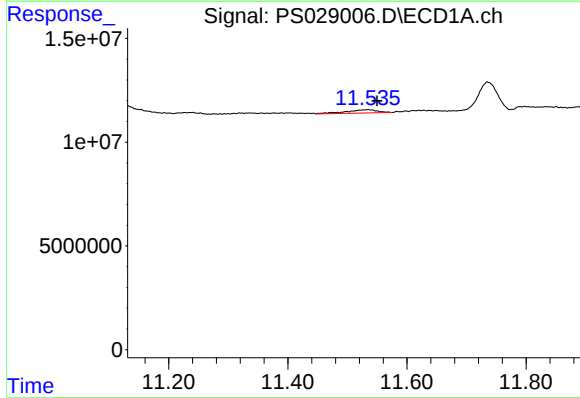

#16 DCPA

R.T.: 11.534 min
Delta R.T.: -0.016 min
Response: 5802912
Conc: N.D.

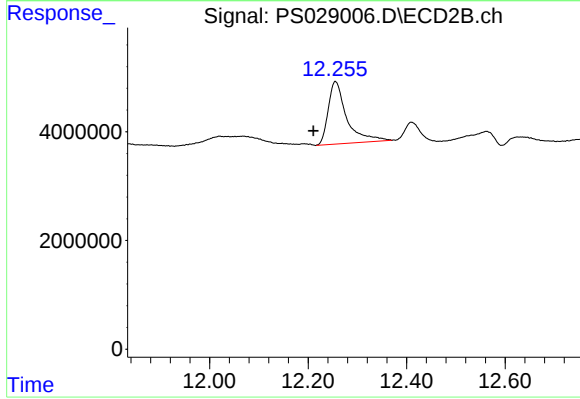

#16 DCPA

R.T.: 12.255 min
Delta R.T.: 0.044 min
Response: 30160951
Conc: 2.66 ng/ml