

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013125\
 Data File : PS029019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2025 20:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 00:28:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 14 12:25:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.195	7.672	1617.7E6	614.5E6	581.074	550.702
Target Compounds							
1) T	Dalapon	2.595	2.711f	979377	3381718	<MDL	1.658 #
2) T	3,5-DICHL...	6.352	0.000	1717925	0	<MDL	N.D. #
3) T	4-Nitroph...	6.982	0.000	10856527	0	6.126	N.D. #
5) T	DICAMBA	7.379	7.866	294915	8367567	<MDL	1.503 #
6) T	MCPD	0.000	7.971	0	2636626	N.D.	<MDL
7) T	MCPA	7.747f	8.195f	1083255	7227237	<MDL	1.702 #
8) T	DICHLORPROP	8.054f	8.627f	3499812	13293030	1.105	9.457 #
10) T	Pentachlo...	8.609	9.428	4011060	18894412	<MDL	<MDL #
11) T	2,4,5-TP ...	9.170	9.816	8702958	6200969	<MDL	<MDL #
12) T	2,4,5-T	9.487	10.224	3111405	15784199	<MDL	1.752 #
13) T	2,4-DB	10.087f	0.000	18234994	0	5.140	N.D. #
14) T	DINOSEB	11.253	0.000	9027213	0	<MDL	N.D. #
15) T	Picloram	11.067	12.257	53639596	5229388	1.700	<MDL #
16) T	DCPA	11.533	12.204	19294466	1719624	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS013125\
Data File : PS029019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2025 20:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 00:28:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
Quant Title : 8080.M
QLast Update : Tue Jan 14 12:25:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

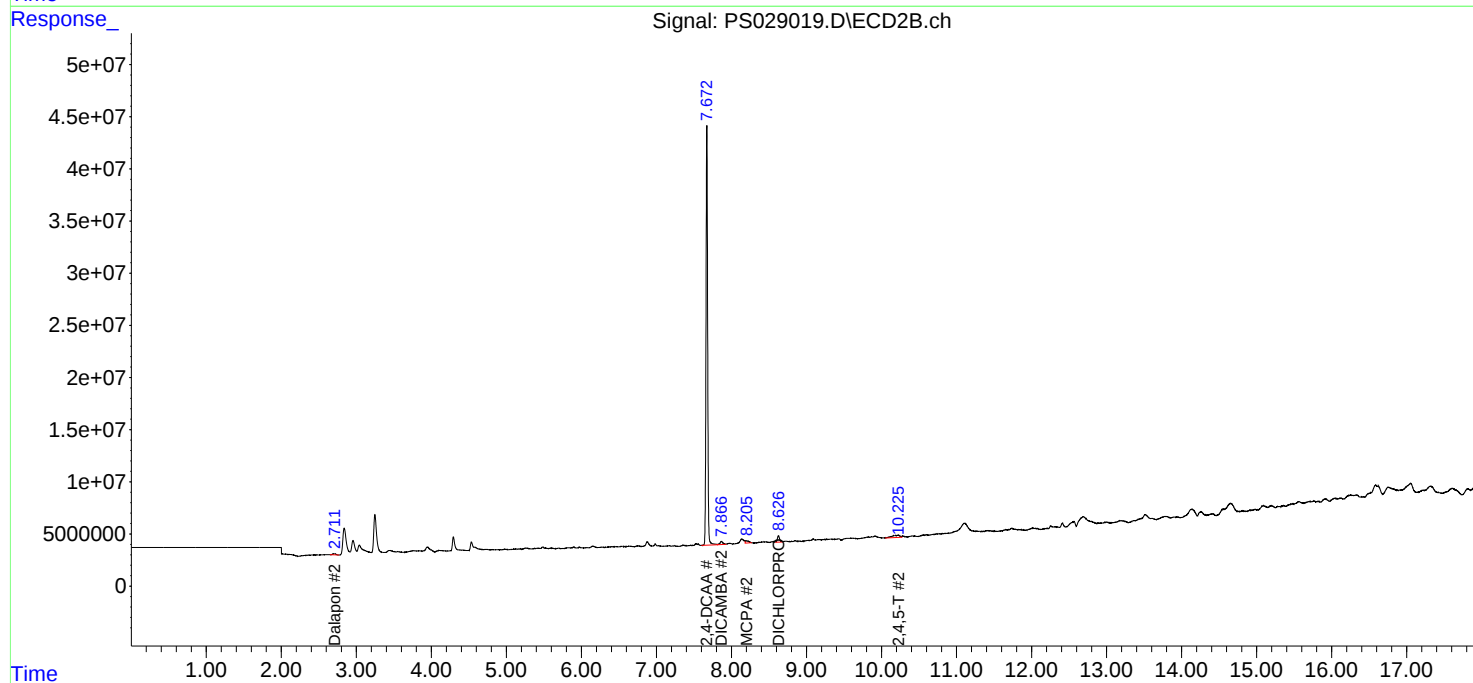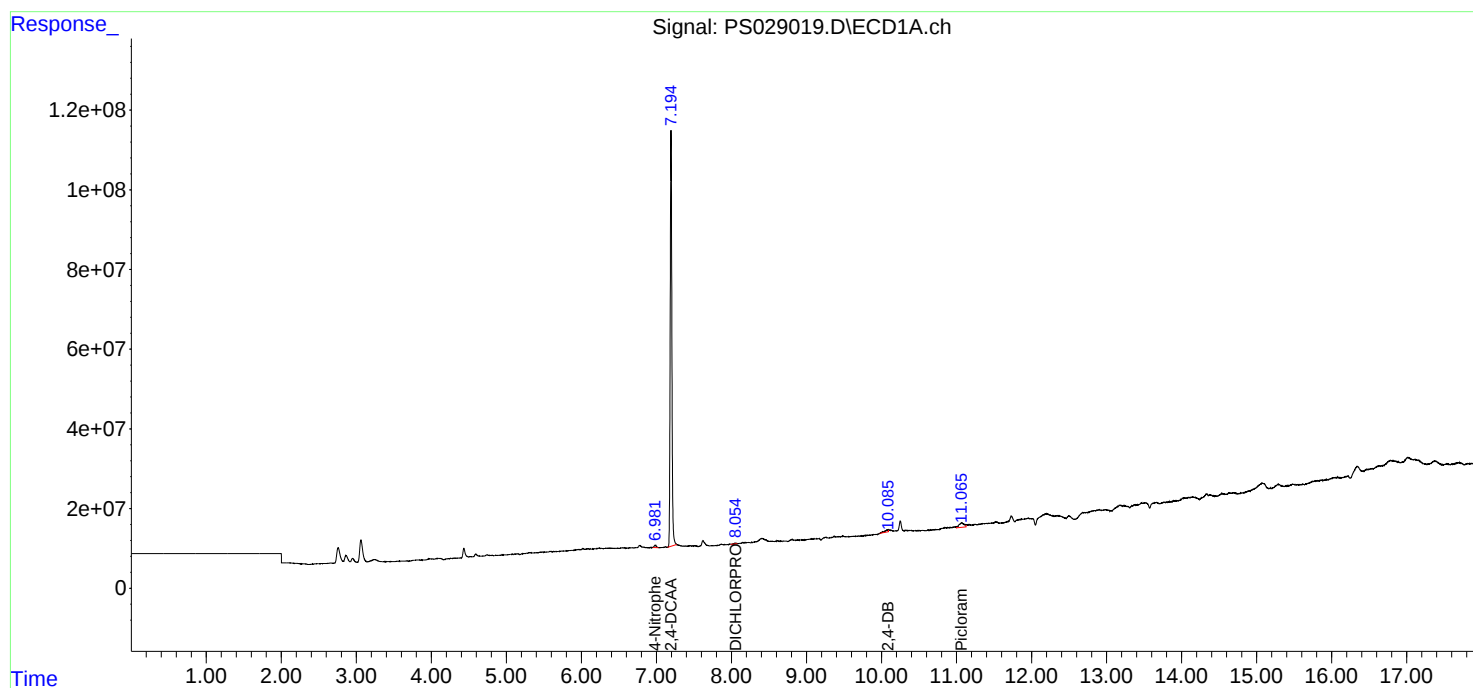


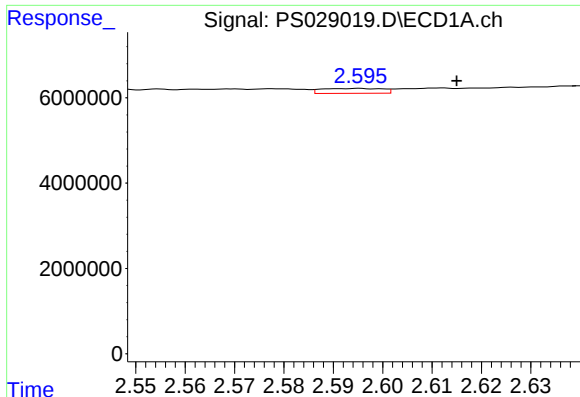

#1 Dalapon


R.T.: 2.595 min
Delta R.T.: -0.020 min
Response: 979377
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

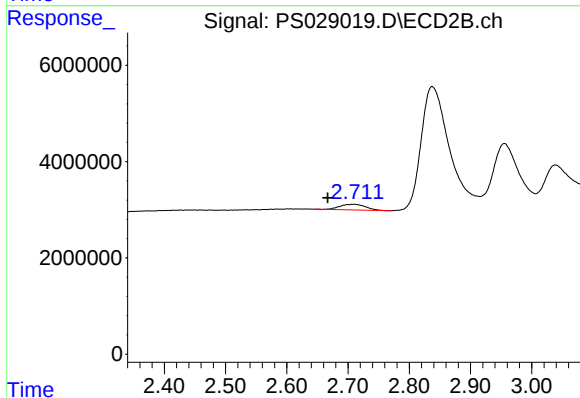


#1 Dalapon

R.T.: 2.711 min
Delta R.T.: 0.044 min
Response: 3381718
Conc: 1.66 ng/ml

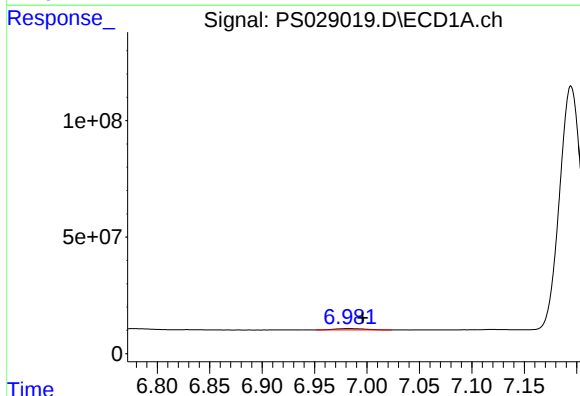


#3 4-Nitrophenol

R.T.: 6.982 min
Delta R.T.: -0.014 min
Response: 10856527
Conc: 6.13 ng/ml

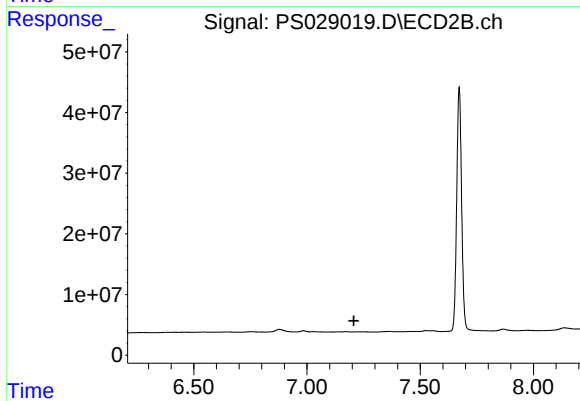

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.207 min
Response: 0
Conc: N.D.

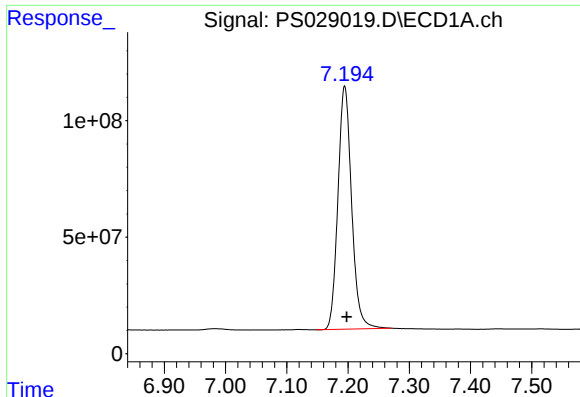

#4 2,4-DCAA


R.T.: 7.195 min
Delta R.T.: -0.003 min
Response: 1617716853
Conc: 581.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

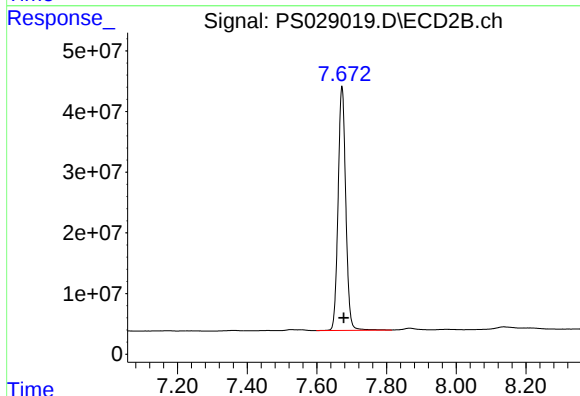


#4 2,4-DCAA

R.T.: 7.672 min
Delta R.T.: -0.006 min
Response: 614480244
Conc: 550.70 ng/ml

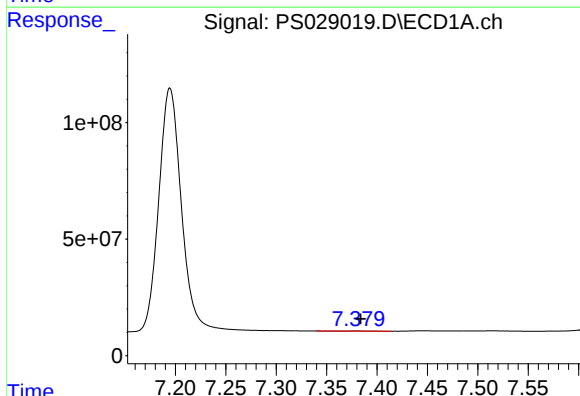


#5 DICAMBA

R.T.: 7.379 min
Delta R.T.: -0.005 min
Response: 294915
Conc: N.D.

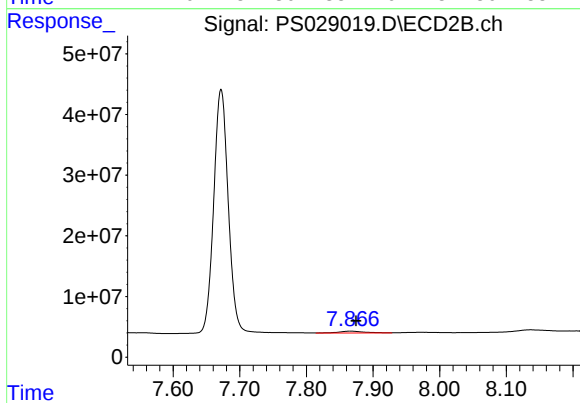

#5 DICAMBA


R.T.: 7.866 min
Delta R.T.: -0.008 min
Response: 8367567
Conc: 1.50 ng/ml

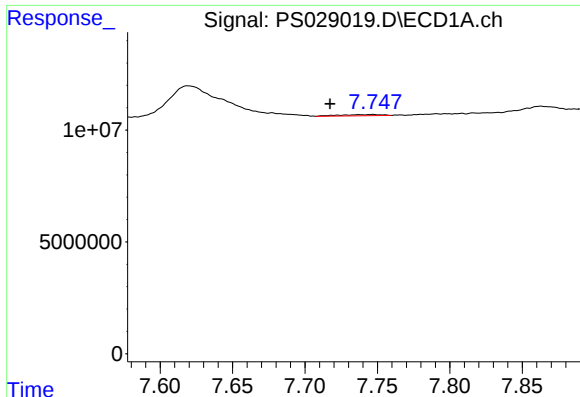

#7 MCPA


R.T.: 7.747 min
Delta R.T.: 0.029 min
Response: 1083255
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

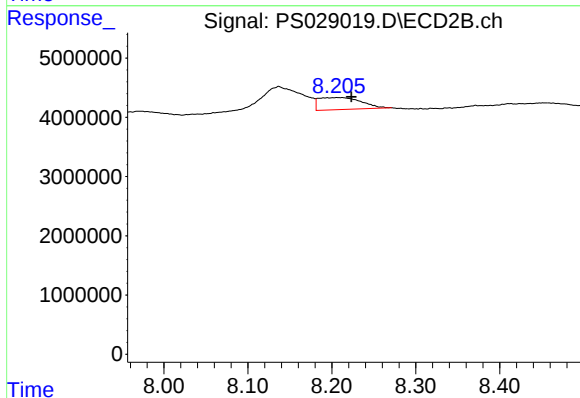


#7 MCPA

R.T.: 8.195 min
Delta R.T.: -0.028 min
Response: 7227237
Conc: 1.70 ug/ml

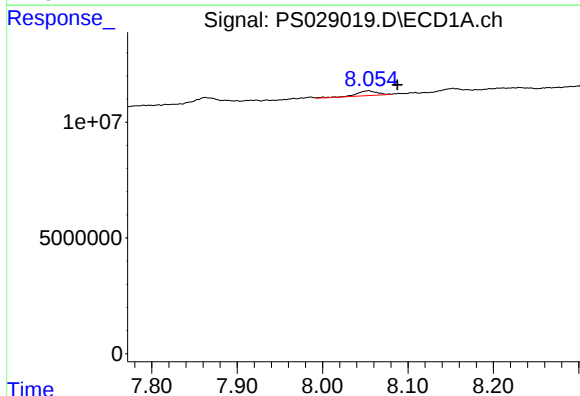


#8 DICHLORPROP

R.T.: 8.054 min
Delta R.T.: -0.034 min
Response: 3499812
Conc: 1.10 ng/ml

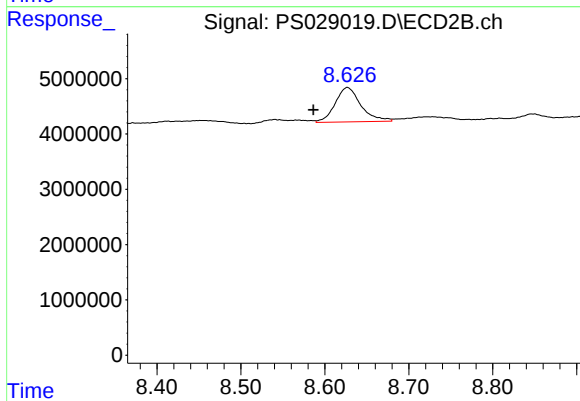

#8 DICHLORPROP


R.T.: 8.627 min
Delta R.T.: 0.041 min
Response: 13293030
Conc: 9.46 ng/ml

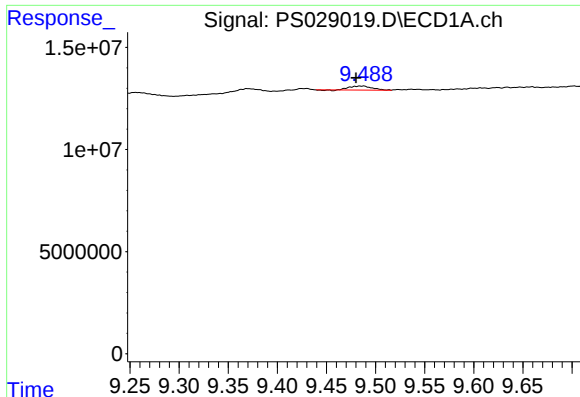

#12 2,4,5-T


R.T.: 9.487 min
Delta R.T.: 0.007 min
Response: 3111405
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

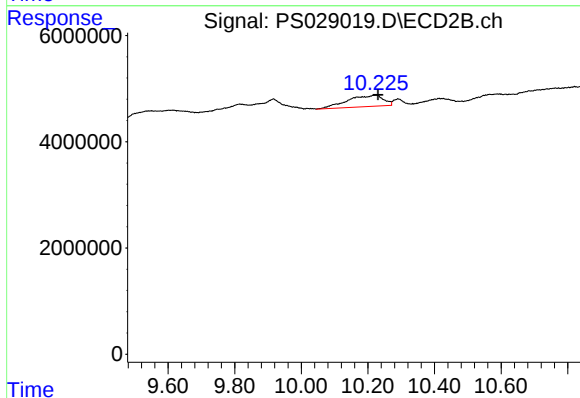


#12 2,4,5-T

R.T.: 10.224 min
Delta R.T.: -0.007 min
Response: 15784199
Conc: 1.75 ng/ml

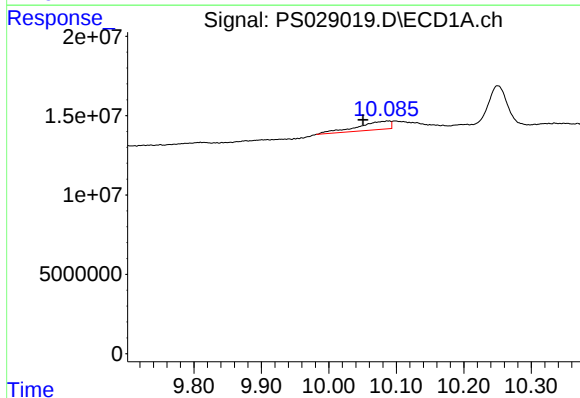


#13 2,4-DB

R.T.: 10.087 min
Delta R.T.: 0.036 min
Response: 18234994
Conc: 5.14 ng/ml

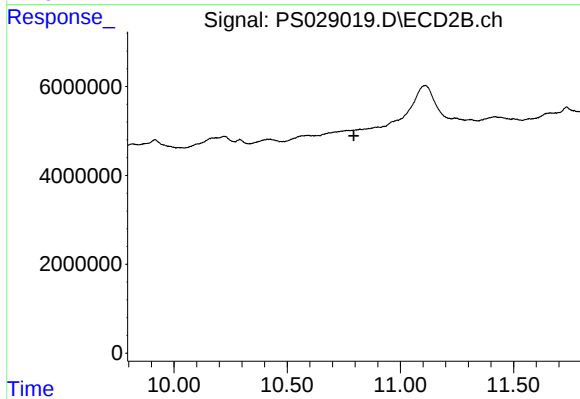

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.795 min
Response: 0
Conc: N.D.

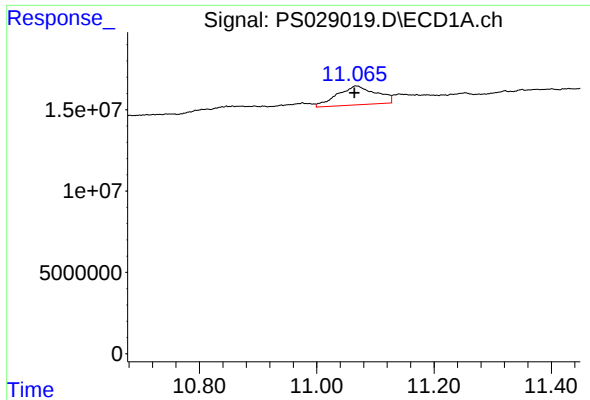

#15 Picloram

R.T.: 11.067 min
Delta R.T.: 0.002 min
Response: 53639596
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

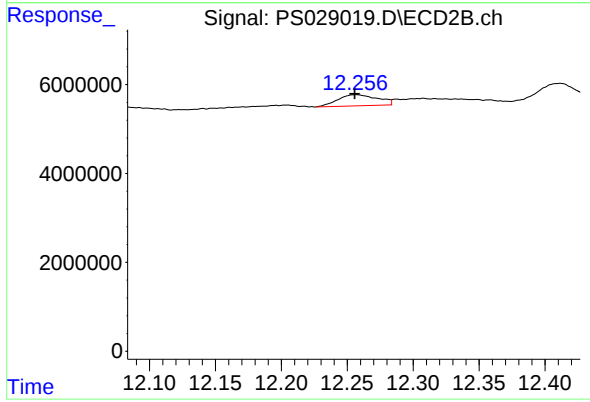

#15 Picloram

R.T.: 12.257 min
Delta R.T.: 0.000 min
Response: 5229388
Conc: N.D.